

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL120320\
 Data File : VL036056.D
 Acq On : 3 Dec 2020 18:29
 Operator : SY/AP
 Sample : OC120120 CAN 10258
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC120120 CAN 10258

Quant Time: Dec 04 10:17:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL120320AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Dec 04 03:52:25 2020
 QLast Update : Fri Dec 04 03:52:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.65	49	1061389	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.16	114	3713886	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.07	117	3381374	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.40	95	2506131	9.74	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.40%


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
20) Methylene Chloride	4.33	84	55778	0.589	ppbv	97
26) Hexane	5.67	57	15111	0.125	ppbv #	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL120320\
Data File : VL036056.D
Acq On : 3 Dec 2020 18:29
Operator : SY/AP
Sample : OC120120 CAN 10258
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC120120 CAN 10258

Quant Time: Dec 04 10:17:31 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL120320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Dec 04 03:52:25 2020
QLast Update : Fri Dec 04 03:52:25 2020
Response via : Initial Calibration

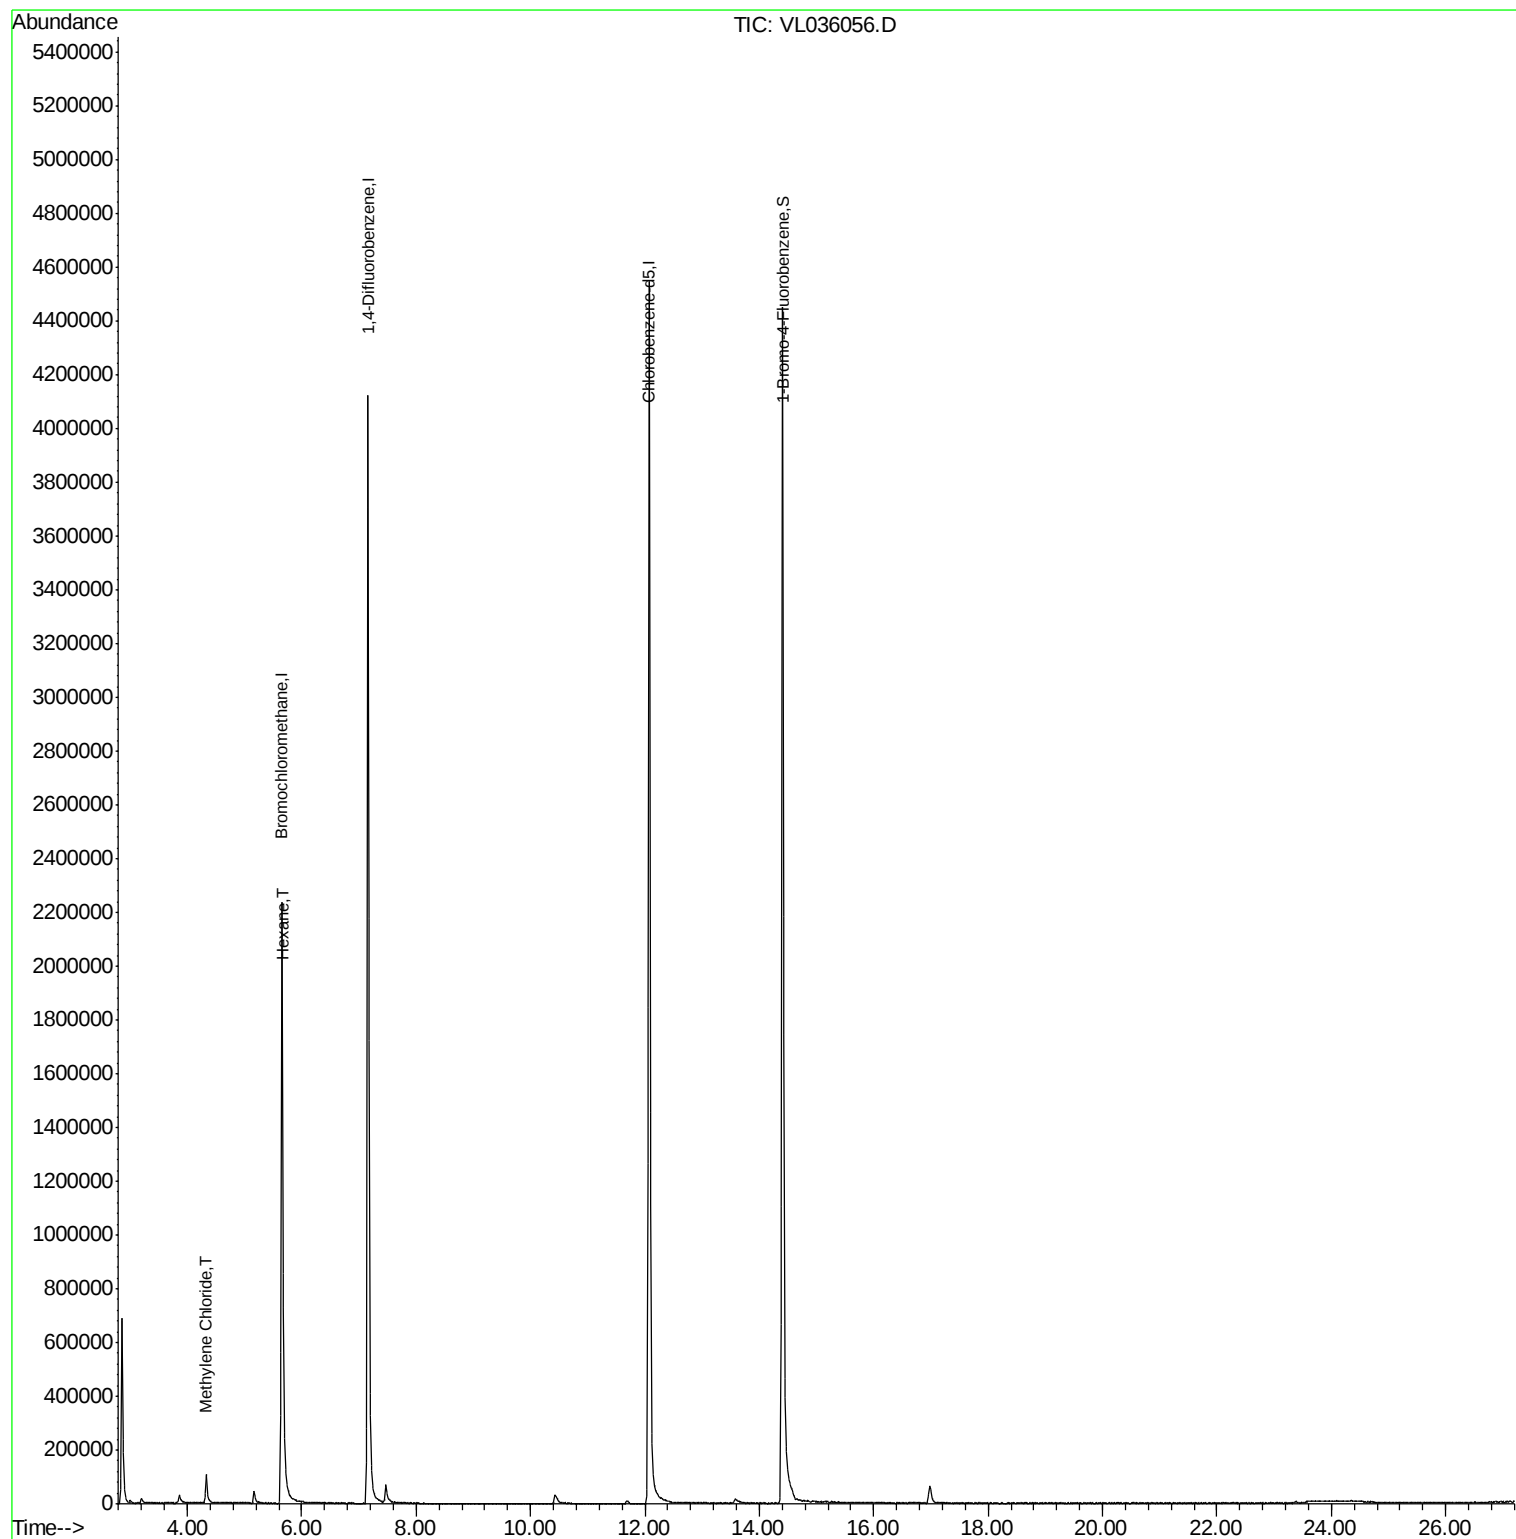

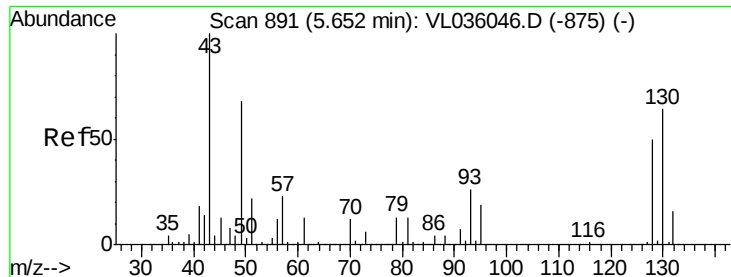

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.65 min Scan# 891

Delta R.T. -0.00 min

Lab File: VL036056.D

Acq: 3 Dec 2020 18:29

Instrument :

MSVOA_L

ClientSampleId :

QC120120 CAN 10258


Tot Ion: 49 Resp: 1061389

Ion Ratio Lower Upper

49 100

128 75.2 38.3 114.8




130 96.8 49.1 147.4

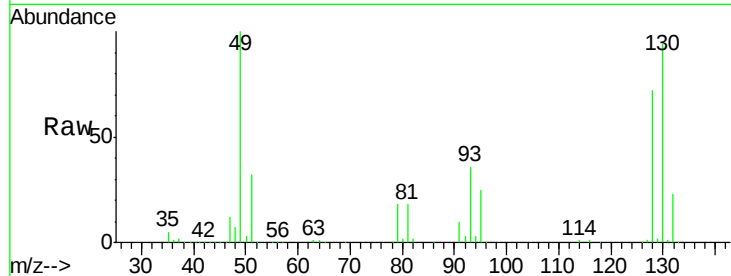

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

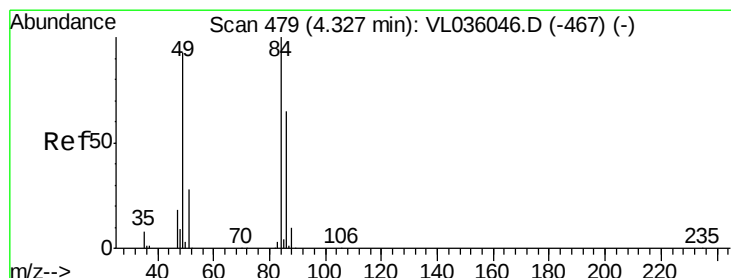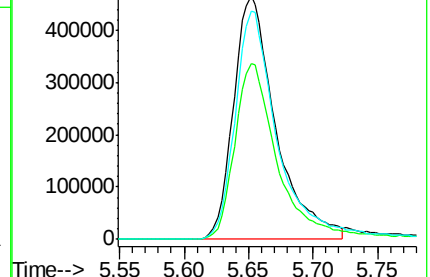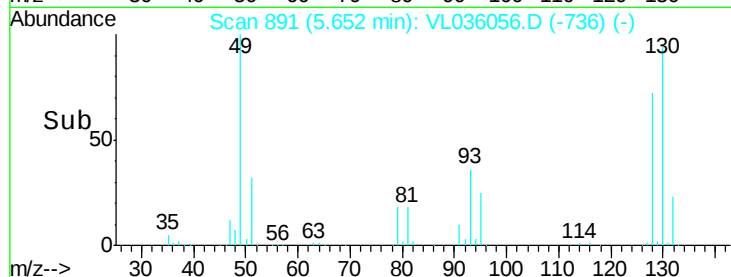

#20

Methylene Chloride

Concen: 0.589 ppbv

RT: 4.33 min Scan# 481

Delta R.T. 0.01 min

Lab File: VL036056.D

Acq: 3 Dec 2020 18:29

Tgt Ion: 84 Resp: 55778


Ion Ratio Lower Upper

84 100

49 96.0 74.4 111.6

51 28.6 22.5 33.7

86 61.6 52.2 78.2


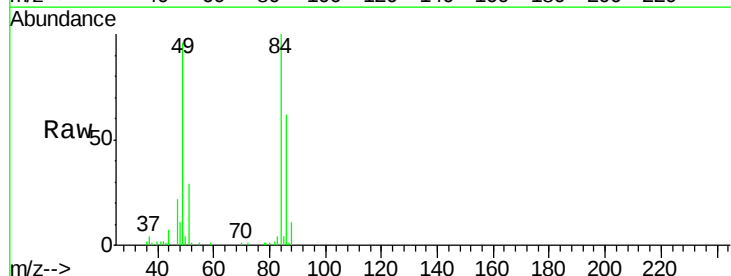



Abundance Ion 84.00 (83.70 to 84.70): VL0

Ion 49.10 (48.80 to 49.80): VL0

Ion 51.10 (50.80 to 51.80): VL0

Ion 86.00 (85.70 to 86.70): VL0

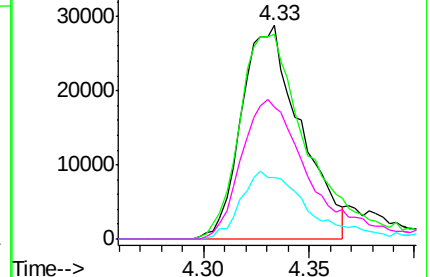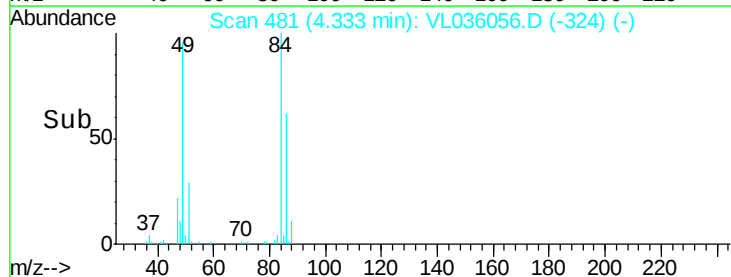

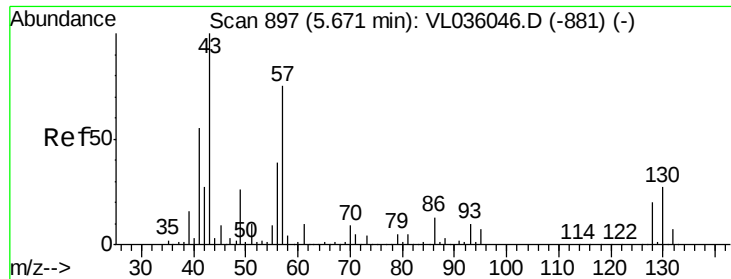

#26

Hexane

Concen: 0.125 ppbv

RT: 5.67 min Scan# 897

Delta R.T. -0.00 min

Lab File: VL036056.D

Acq: 3 Dec 2020 18:29

Instrument :

MSVOA_L

ClientSampleId :

QC120120 CAN 10258

Tot Ion: 57 Resp: 15111


Ion Ratio Lower Upper

57 100

41 98.0 61.6 92.4#

43 73.2 152.9 229.3#

56 64.5 43.0 64.6



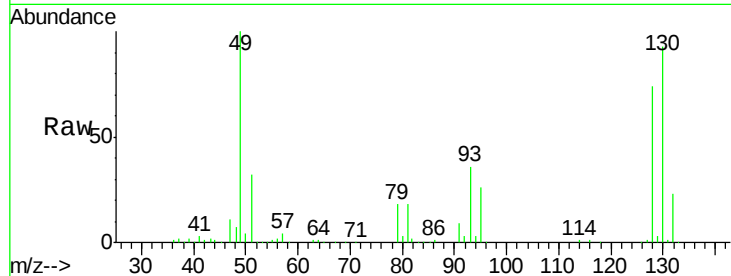


Abundance Ion 57.10 (56.80 to 57.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 43.10 (42.80 to 43.80): VL0

Ion 56.10 (55.80 to 56.80): VL0

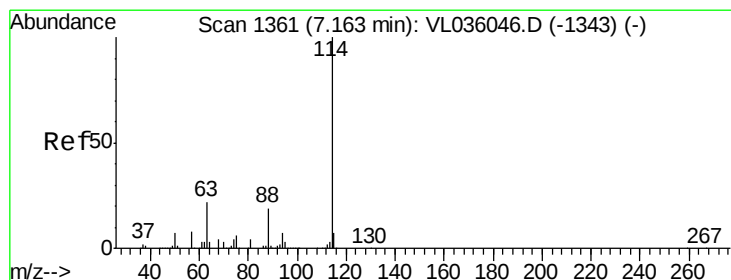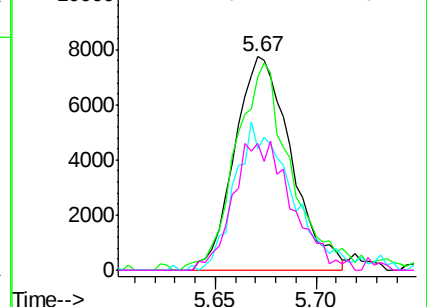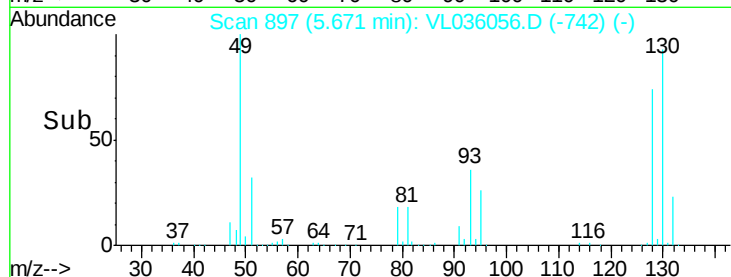

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.16 min Scan# 1360

Delta R.T. -0.00 min

Lab File: VL036056.D

Acq: 3 Dec 2020 18:29


Tgt Ion:114 Resp: 3713886

Ion Ratio Lower Upper

114 100

63 21.2 17.2 25.8



88 17.4 14.0 21.0

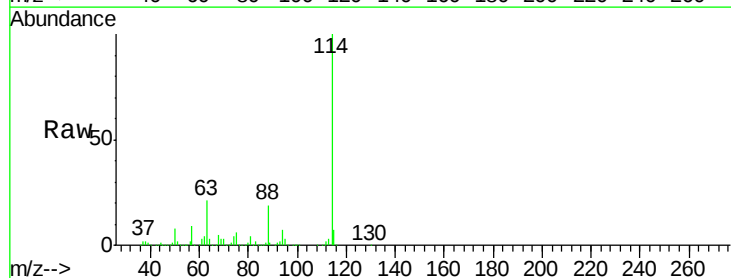


Abundance Ion 114.10 (113.80 to 114.80): V

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

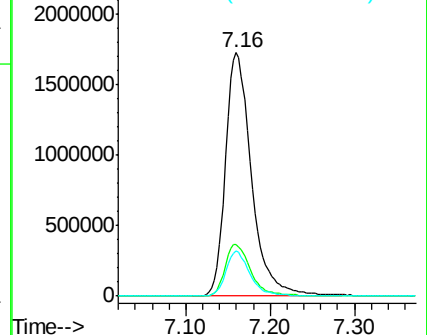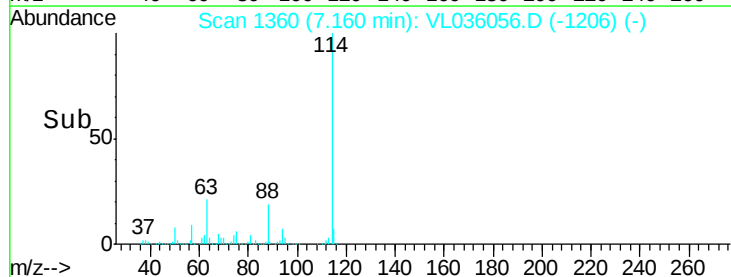

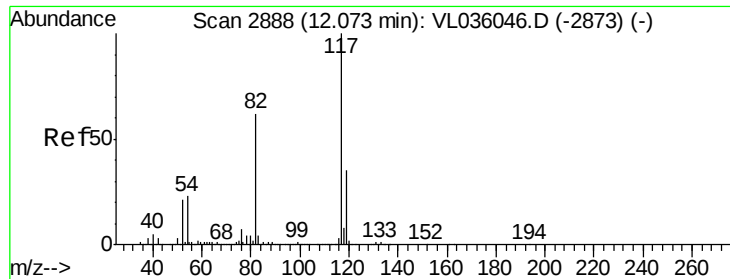

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.07 min Scan# 2888

Delta R.T. -0.00 min

Lab File: VL036056.D

Acq: 3 Dec 2020 18:29

Instrument :

MSVOA_L

ClientSampleId :

QC120120 CAN 10258


Tot Ion:117 Resp: 3381374

Ion Ratio Lower Upper

117 100

82 61.9 49.9 74.9




119 34.2 28.7 43.1

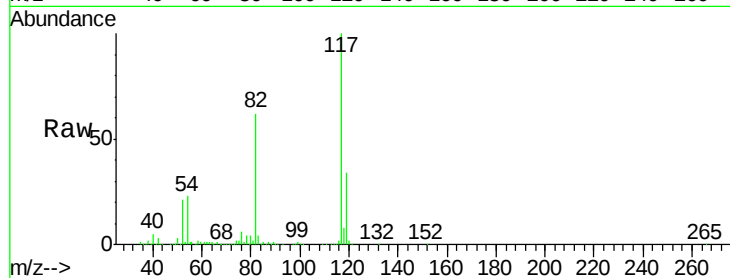

Abundance Ion 117.10 (116.80 to 117.80): V

Ion 82.10 (81.80 to 82.80): VL0

Ion 119.10 (118.80 to 119.80): V

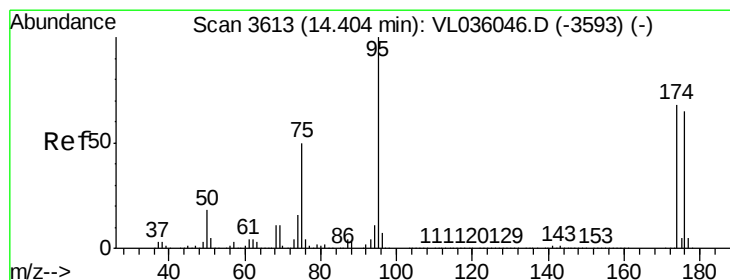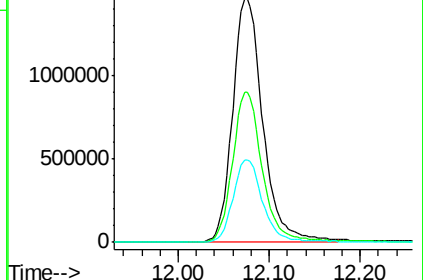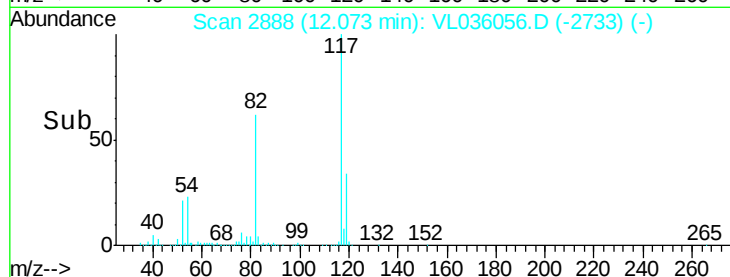

#68

1-Bromo-4-Fluorobenzene

Concen: 9.740 ppbv

RT: 14.40 min Scan# 3613

Delta R.T. -0.00 min

Lab File: VL036056.D

Acq: 3 Dec 2020 18:29


Tgt Ion: 95 Resp: 2506131

Ion Ratio Lower Upper

95 100

174 69.8 54.2 81.2

175 4.8 3.8 5.8

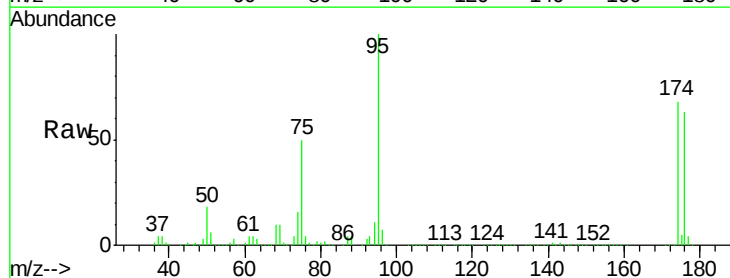

Abundance Ion 95.10 (94.80 to 95.80): VL0

Ion 174.00 (173.70 to 174.70): V

Ion 175.00 (174.70 to 175.70): V

