


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL120320\
 Data File : VL036045.D
 Acq On : 3 Dec 2020 9:10
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120320AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Nov 04 02:40:06 2020
 Last Update : Wed Nov 04 02:40:06 2020

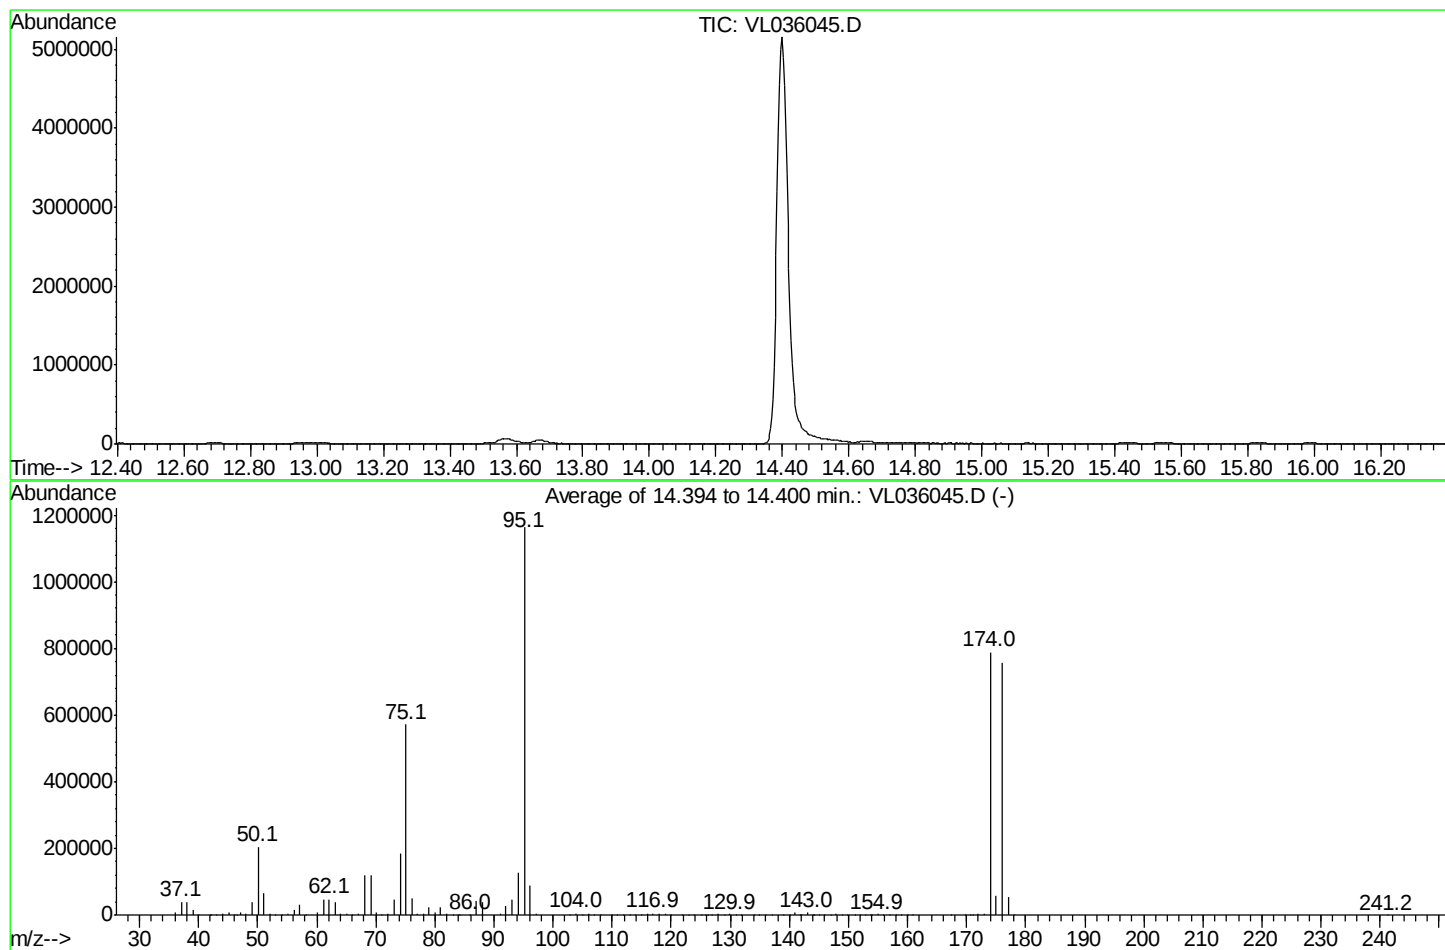

AutoFind: Scans 3610, 3611, 3612; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	17.7	205354	PASS
75	95	30	66	49.1	570986	PASS
95	95	100	100	100.0	1163093	PASS
96	95	5	9	7.5	87696	PASS
173	174	0.00	2	0.6	4904	PASS
174	95	50	120	67.8	788565	PASS
175	174	4	9	7.2	56802	PASS
176	174	93	101	96.0	757013	PASS
177	176	5	9	7.0	52840	PASS