


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL120718\
 Data File : VL032919.D
 Acq On : 7 Dec 2018 3:00
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120718AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Dec 07 09:35:17 2018
 Last Update : Fri Dec 07 09:35:17 2018

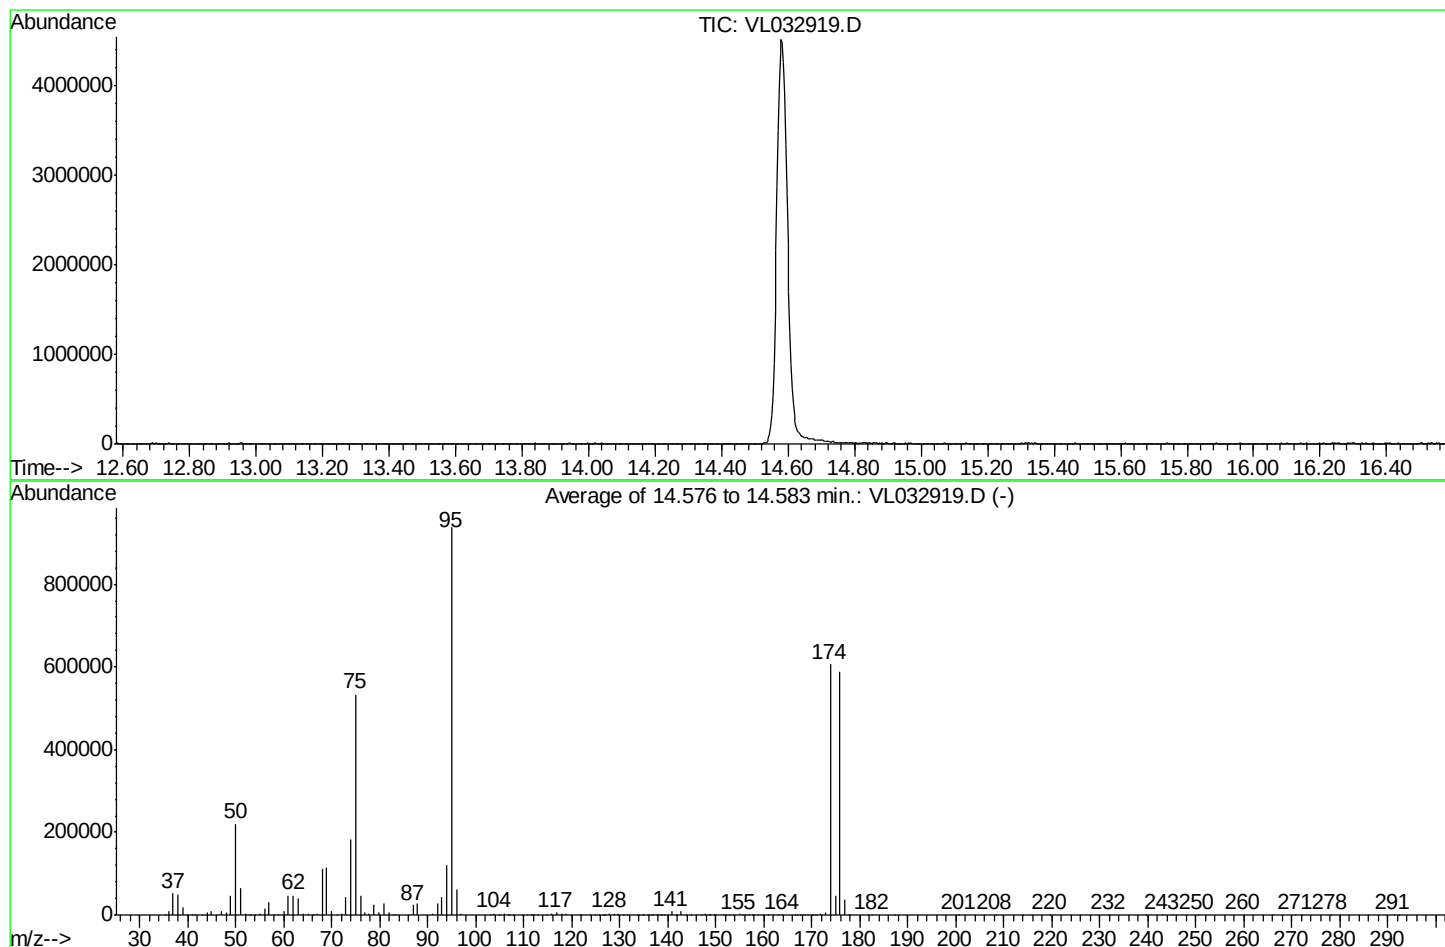

AutoFind: Scans 3620, 3621, 3622; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	221226	PASS
75	95	30	66	57.0	533952	PASS
95	95	100	100	100.0	937557	PASS
96	95	5	9	6.7	63272	PASS
173	174	0.00	2	1.2	7421	PASS
174	95	50	120	64.6	605655	PASS
175	174	4	9	7.8	47309	PASS
176	174	93	101	97.1	588330	PASS
177	176	5	9	6.5	38154	PASS