


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL120720\
 Data File : VL036063.D
 Acq On : 7 Dec 2020 11:50
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120720AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Dec 04 03:46:13 2020
 Last Update : Fri Dec 04 03:46:13 2020

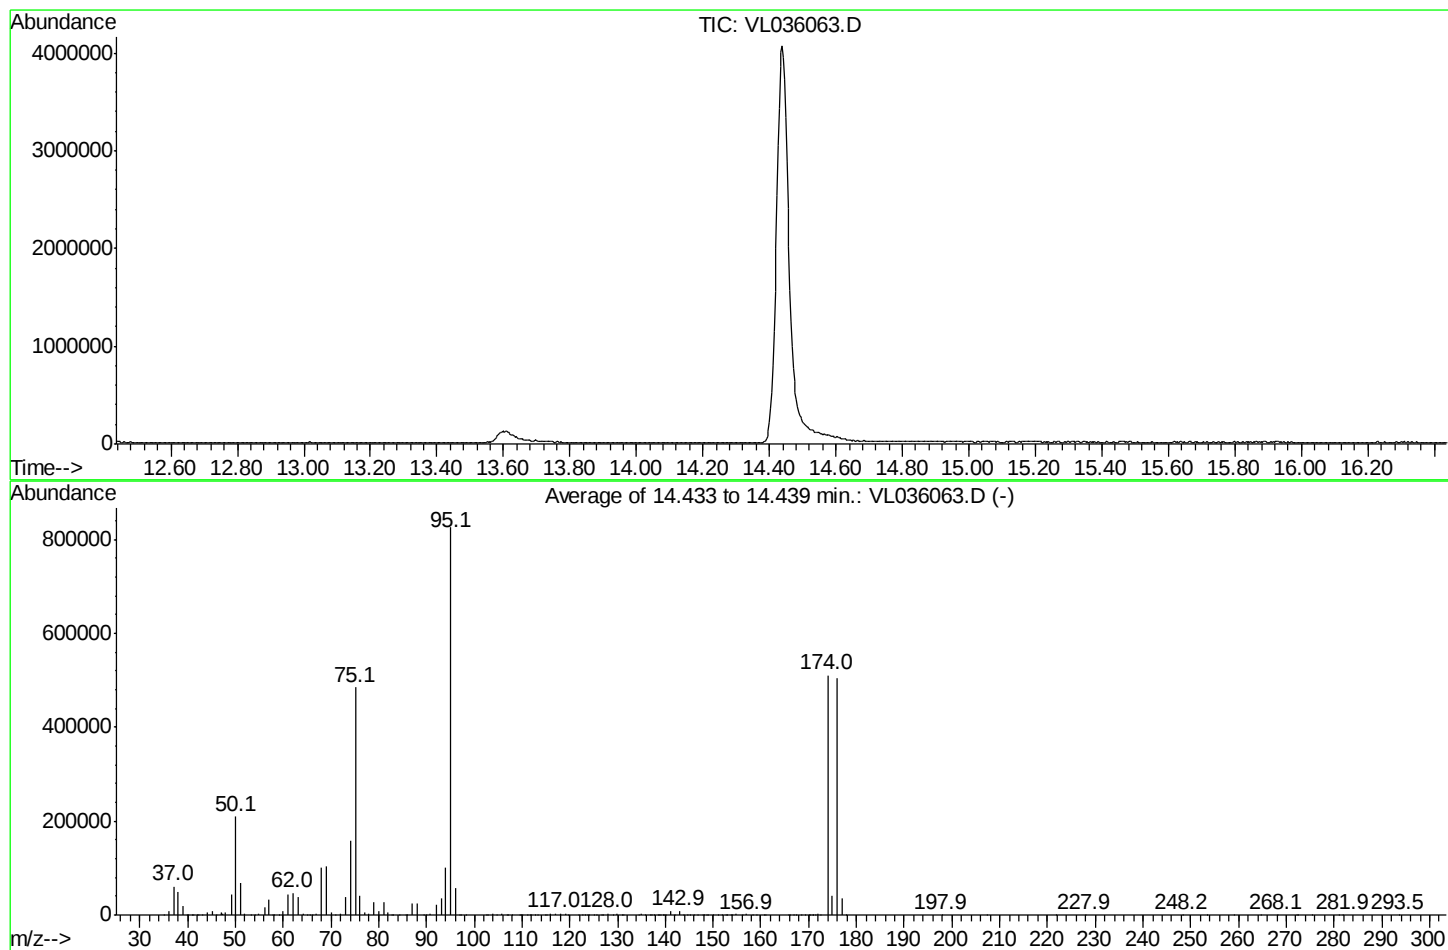

AutoFind: Scans 3622, 3623, 3624; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.3	209380	PASS
75	95	30	66	58.6	484394	PASS
95	95	100	100	100.0	826325	PASS
96	95	5	9	6.9	57104	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	61.8	510762	PASS
175	174	4	9	7.8	39909	PASS
176	174	93	101	98.6	503722	PASS
177	176	5	9	7.0	35138	PASS