


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121620\
 Data File : VL036162.D
 Acq On : 16 Dec 2020 8:51
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120720AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Dec 07 16:56:49 2020
 Last Update : Mon Dec 07 16:56:49 2020

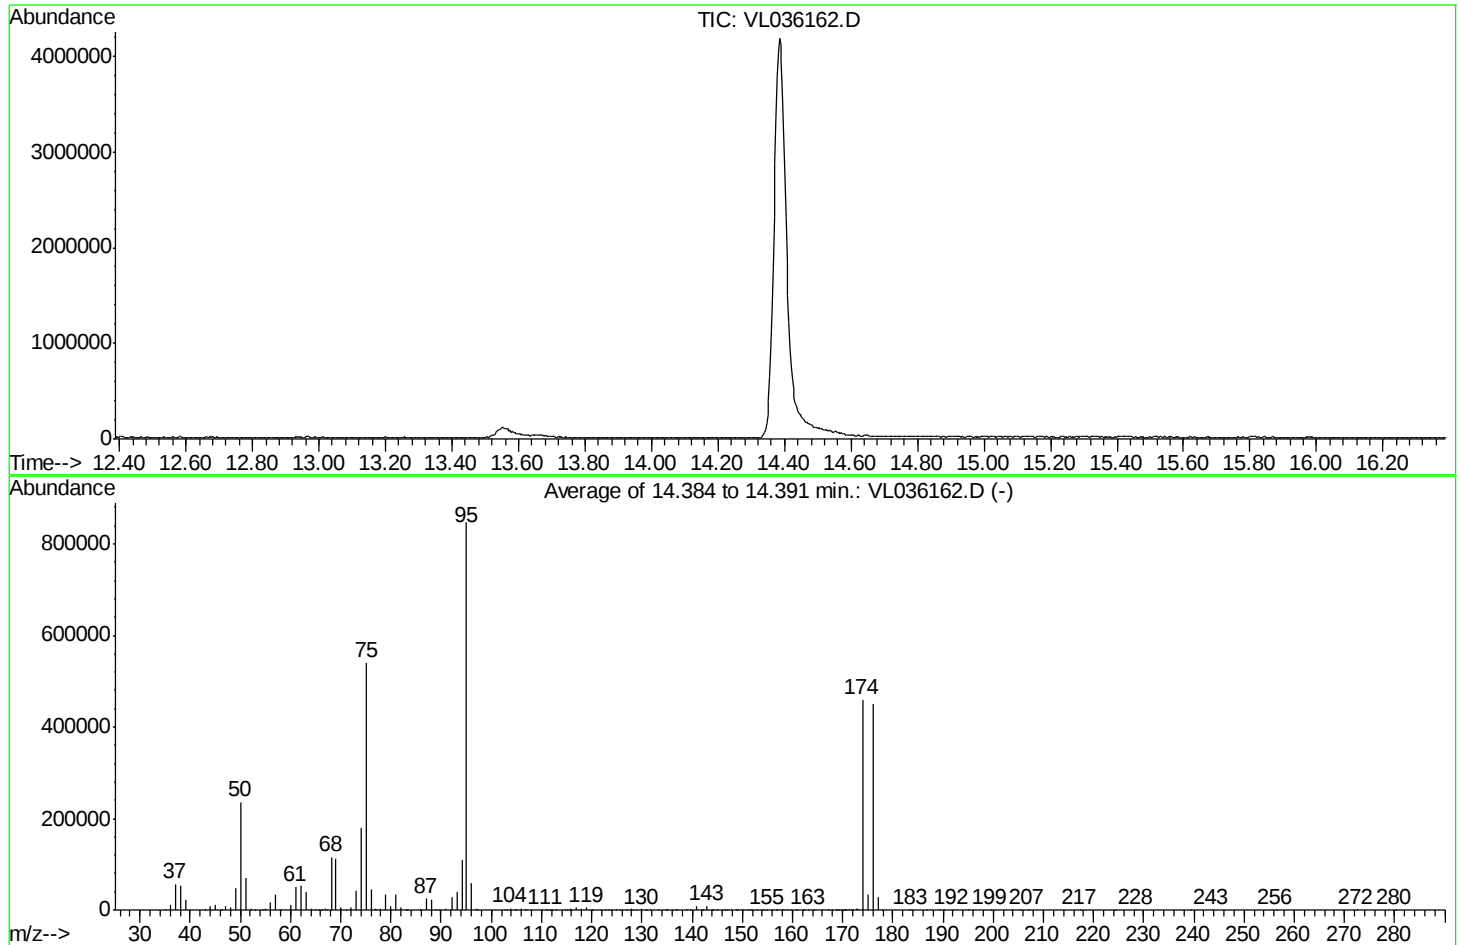

AutoFind: Scans 3607, 3608, 3609; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.9	236342	PASS
75	95	30	66	63.9	541215	PASS
95	95	100	100	100.0	847146	PASS
96	95	5	9	7.0	59664	PASS
173	174	0.00	2	0.7	3052	PASS
174	95	50	120	54.3	460053	PASS
175	174	4	9	7.2	33074	PASS
176	174	93	101	97.9	450496	PASS
177	176	5	9	6.3	28514	PASS