

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_L\Data\VL121824\  
 Data File : VL041807.D  
 Acq On : 18 Dec 2024 22:37  
 Operator : SY/MD  
 Sample : P5295-01 4X  
 Misc : 400mL/MSVOA\_L  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :

Quant Time: Dec 19 08:00:48 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_L\methods\VL121624AIR.M  
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Fri Aug 26 06:05:16 2022  
 QLast Update : Thu Dec 19 07:32:09 2024  
 Response via : Initial Calibration


| Compound                     | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|------------------------------|--------|-------|----------|----------|--------|----------|
| -----                        |        |       |          |          |        |          |
| Internal Standards           |        |       |          |          |        |          |
| 1) Bromochloromethane        | 2.797  | 49    | 73010    | 10.000   | ppbv   | 0.01     |
| 33) 1,4-Difluorobenzene      | 3.972  | 114   | 173625   | 10.000   | ppbv   | 0.02     |
| 55) Chlorobenzene-d5         | 8.895  | 117   | 170332   | 10.000   | ppbv   | 0.02     |
| System Monitoring Compounds  |        |       |          |          |        |          |
| 68) 1-Bromo-4-Fluorobenzene  | 10.387 | 95    | 135837   | 9.570    | ppbv   | 0.01     |
| Spiked Amount                | 10.000 | Range | 65 - 135 | Recovery | =      | 95.700%  |
| Target Compounds             |        |       |          |          |        |          |
|                              |        |       |          |          | Qvalue |          |
| 2) Dichlorodifluoromethane   | 1.499  | 85    | 1539     | 0.118    | ppbv   | 91       |
| 3) Chlorodifluoromethane     | 1.466  | 51    | 2506     | 0.210    | ppbv # | 65       |
| 4) Chloromethane             | 1.531  | 50    | 431      | 0.085    | ppbv # | 77       |
| 8) Dichlorotetrafluoroethane | 1.499  | 85    | 1539     | 0.132    | ppbv # | 18       |
| 9) Propene                   | 1.622  | 41    | 1914     | 0.371    | ppbv   | 97       |
| 10) Heptane                  | 5.004  | 43    | 452      | 0.034    | ppbv   | 98       |
| 11) Trichlorofluoromethane   | 1.884  | 101   | 724      | 0.052    | ppbv # | 79       |
| 13) Ethanol                  | 1.725  | 45    | 11589    | 27.120   | ppbv # | 34       |
| 15) Acetone                  | 1.842  | 43    | 9724     | 0.685    | ppbv   | 94       |
| 16) 1,3-Butadiene            | 1.609  | 39    | 643      | 0.115    | ppbv # | 13       |
| 17) tert-Butyl alcohol       | 2.049  | 59    | 1952     | 0.139    | ppbv # | 78       |
| 19) Isopropyl Alcohol        | 1.894  | 45    | 7976     | 0.936    | ppbv # | 39       |
| 20) Methylene Chloride       | 2.068  | 84    | 1631     | 0.403    | ppbv   | 92       |
| 22) trans-1,2-Dichloroethene | 2.797  | 96    | 174      | 0.035    | ppbv # | 1        |
| 23) Vinyl Acetate            | 2.470  | 43    | 551      | 0.084    | ppbv # | 1        |
| 25) Ethyl Acetate            | 2.849  | 43    | 3744     | 0.142    | ppbv # | 87       |
| 26) Hexane                   | 2.842  | 57    | 1571     | 0.157    | ppbv # | 88       |
| 29) Chloroform               | 2.861  | 83    | 1319     | 0.086    | ppbv   | 98       |
| 30) Cyclohexane              | 3.871  | 84    | 314      | 0.037    | ppbv # | 31       |
| 34) 2-Butanone               | 2.570  | 43    | 2830     | 0.203    | ppbv   | 96       |
| 36) Benzene                  | 3.674  | 78    | 945      | 0.053    | ppbv # | 81       |
| 38) Trichloroethene          | 4.564  | 130   | 929      | 0.122    | ppbv # | 38       |
| 39) 1,2-Dichloropropane      | 3.972  | 63    | 48675    | 7.494    | ppbv # | 18       |
| 41) Tetrahydrofuran          | 3.078  | 42    | 1030     | 0.132    | ppbv   | 93       |
| 52) Tetrachloroethene        | 8.241  | 164   | 184475   | 27.596   | ppbv   | 93       |
| 53) Toluene                  | 6.949  | 91    | 17152    | 0.842    | ppbv   | 100      |
| 57) Chlorobenzene            | 8.937  | 112   | 734      | 0.042    | ppbv # | 58       |
| 58) Ethyl Benzene            | 9.364  | 91    | 3771     | 0.123    | ppbv   | 91       |
| 59) m/p-Xylene               | 9.548  | 91    | 1601     | 0.065    | ppbv # | 100      |
| 60) o-Xylene                 | 9.972  | 91    | 3367     | 0.136    | ppbv   | 100      |
| 61) Styrene                  | 9.885  | 104   | 1059     | 0.099    | ppbv   | 91       |
| -----                        |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_L\Data\VL121824\  
Data File : VL041807.D  
Acq On : 18 Dec 2024 22:37  
Operator : SY/MD  
Sample : P5295-01 4X  
Misc : 400mL/MSVOA\_L  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :

Quant Time: Dec 19 08:00:48 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_L\methods\VL121624AIR.M  
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Fri Aug 26 06:05:16 2022  
QLast Update : Thu Dec 19 07:32:09 2024  
Response via : Initial Calibration




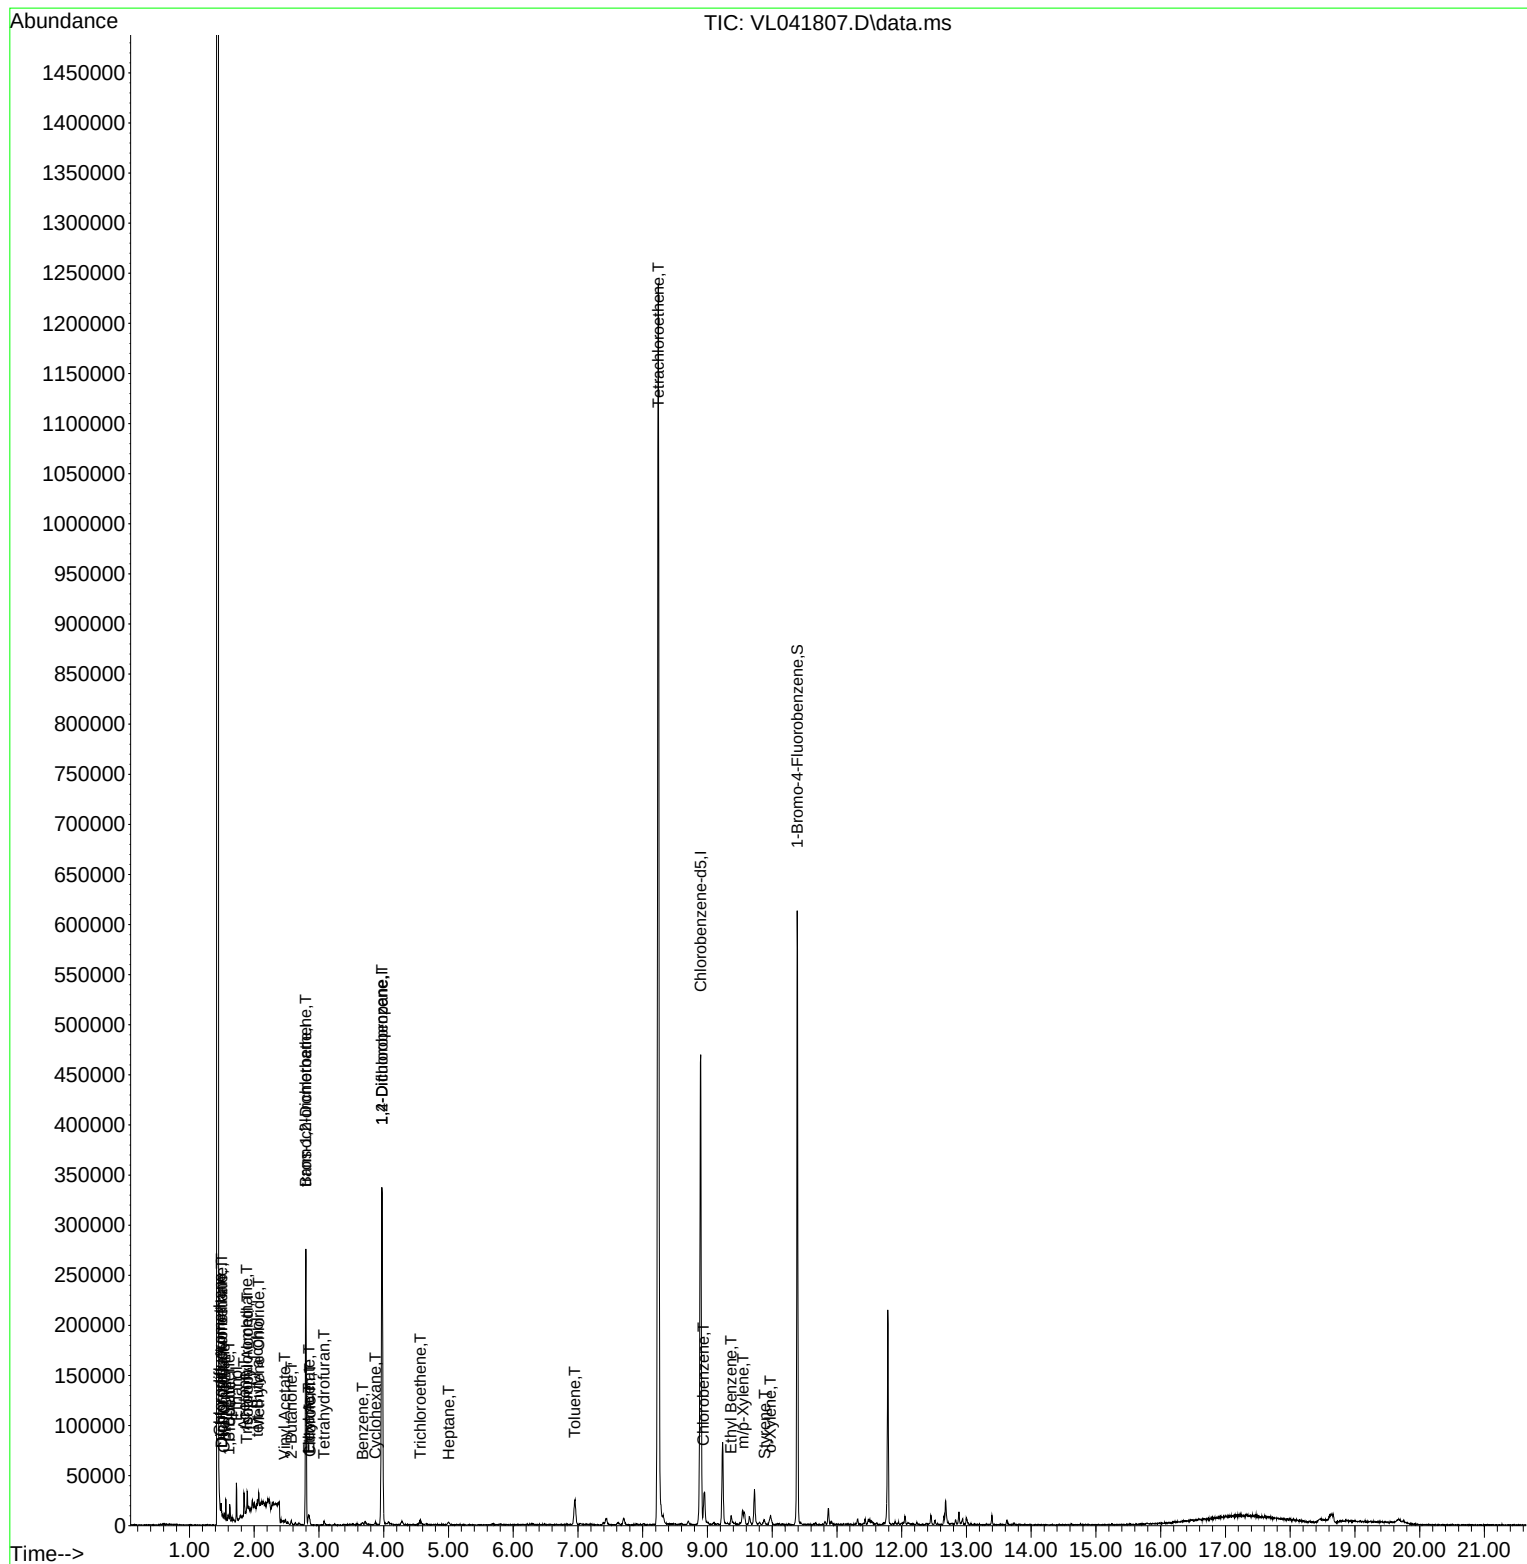




#1  
Bromochloromethane  
Concen: 10.000 ppbv  
RT: 2.797 min Scan# 81  
Delta R.T. 0.013 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37




Instrument :  
MSVOA\_L  
ClientSampleId :


Tgt Ion: 49 Resp: 73010  
Ion Ratio Lower Upper  
49 100  
128 41.4 21.6 64.6  
130 53.9 28.3 85.0



#2  
Dichlorodifluoromethane  
Concen: 0.118 ppbv  
RT: 1.499 min Scan# 436  
Delta R.T. 0.003 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37


Tgt Ion: 85 Resp: 1539  
Ion Ratio Lower Upper  
85 100  
87 25.5 24.5 36.7

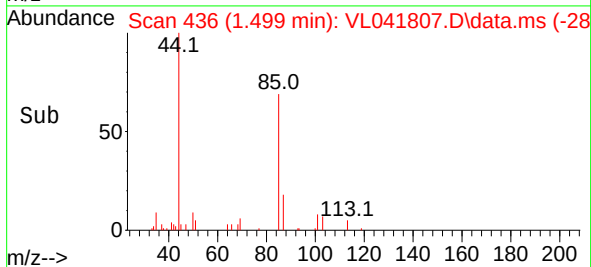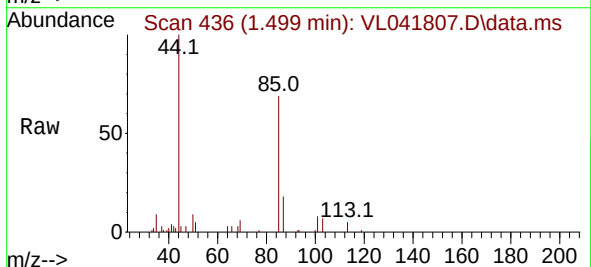






#3  
Chlorodifluoromethane  
Concen: 0.210 ppbv  
RT: 1.466 min Scan# 41  
Delta R.T. -0.007 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37

Instrument :  
MSVOA\_L  
ClientSampleId :



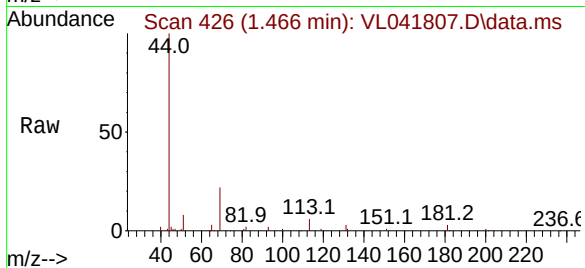



Tgt Ion: 51 Resp: 2506  
Ion Ratio Lower Upper  
51 100  
67 3.1 15.0 22.4#

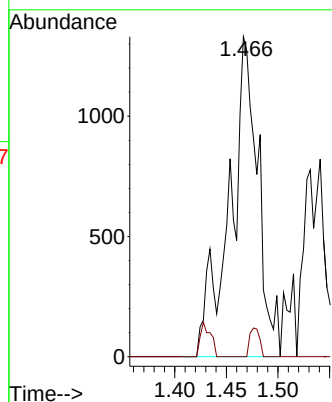

#4  
Chloromethane  
Concen: 0.085 ppbv  
RT: 1.531 min Scan# 446  
Delta R.T. -0.000 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37

Tgt Ion: 50 Resp: 431  
Ion Ratio Lower Upper  
50 100  
52 45.4 26.2 39.2#


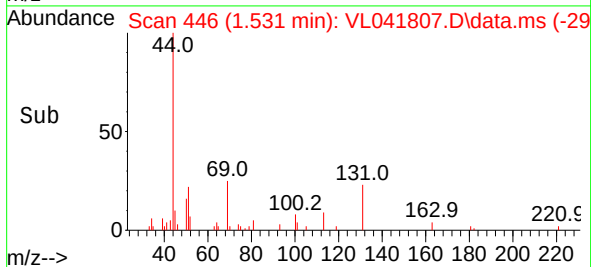
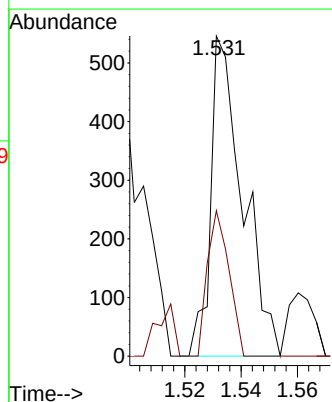
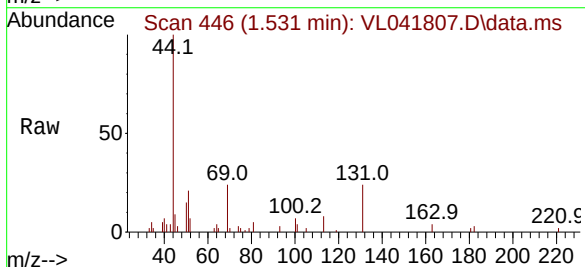




#8  
Dichlorotetrafluoroethane  
Concen: 0.132 ppbv  
RT: 1.499 min Scan# 411  
Delta R.T. -0.055 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37




Instrument :  
MSVOA\_1  
ClientSampleId :


Tgt Ion: 85 Resp: 1539  
Ion Ratio Lower Upper  
85 100  
135 0.0 51.9 77.9#

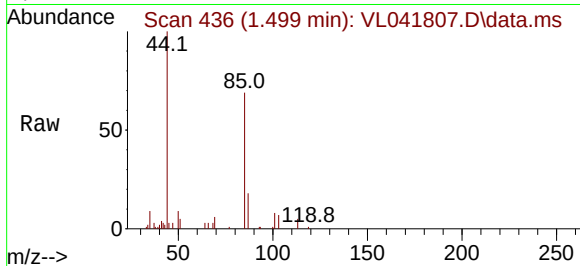

#9  
Propene  
Concen: 0.371 ppbv  
RT: 1.622 min Scan# 474  
Delta R.T. 0.139 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37

Tgt Ion: 41 Resp: 1914  
Ion Ratio Lower Upper  
41 100  
42 68.0 52.4 78.6

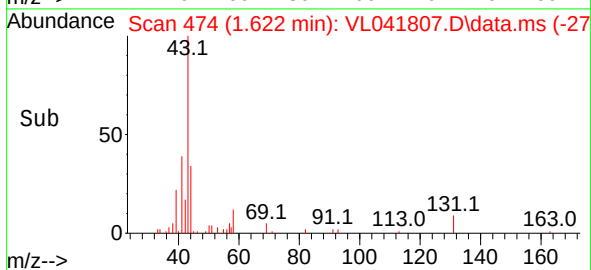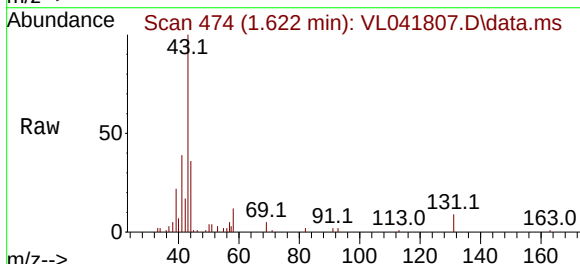



#10

Heptane

Concen: 0.034 ppbv

RT: 5.004 min Scan# 1

Delta R.T. 0.026 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_L





ClientSampleId :

Tgt Ion: 43 Resp: 452

Ion Ratio Lower Upper

43 100

57 49.6 38.5 57.7

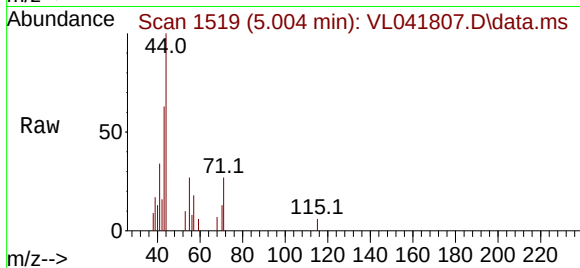

#11

Trichlorofluoromethane

Concen: 0.052 ppbv

RT: 1.884 min Scan# 555

Delta R.T. 0.009 min

Lab File: VL041807.D




Acq: 18 Dec 2024 22:37


Tgt Ion:101 Resp: 724

Ion Ratio Lower Upper

101 100

103 48.6 51.8 77.8#

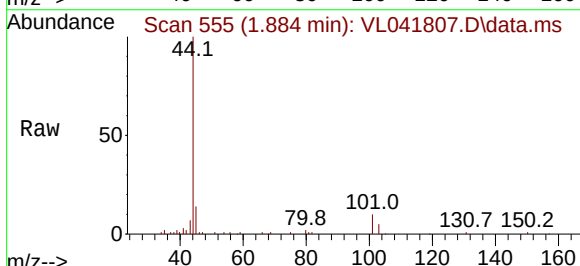



#13

Ethanol

Concen: 27.120 ppbv

RT: 1.725 min Scan# 506

Delta R.T. 0.006 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_1





ClientSampleId :

Tgt Ion: 45 Resp: 11589

Ion Ratio Lower Upper

45 100

46 0.0 16.4 65.8#

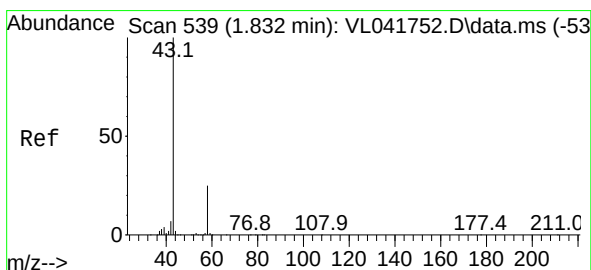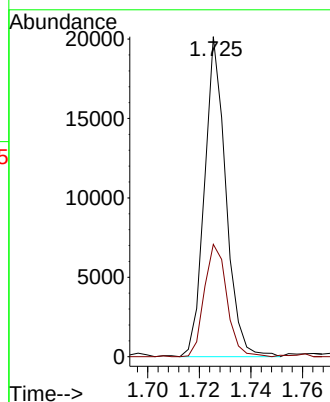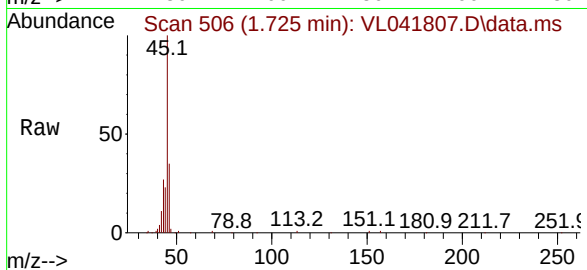

#15

Acetone

Concen: 0.685 ppbv

RT: 1.842 min Scan# 542

Delta R.T. 0.009 min

Lab File: VL041807.D




Acq: 18 Dec 2024 22:37


Tgt Ion: 43 Resp: 9724

Ion Ratio Lower Upper

43 100

58 27.5 19.7 29.5

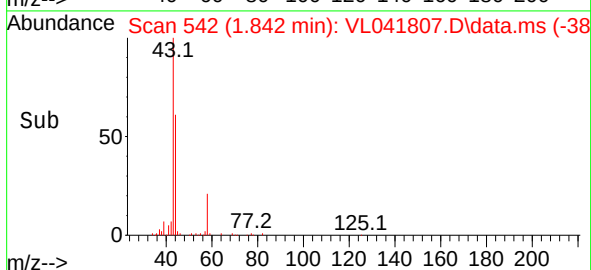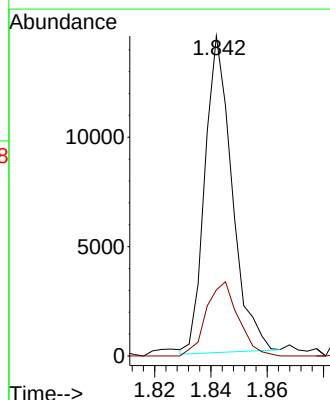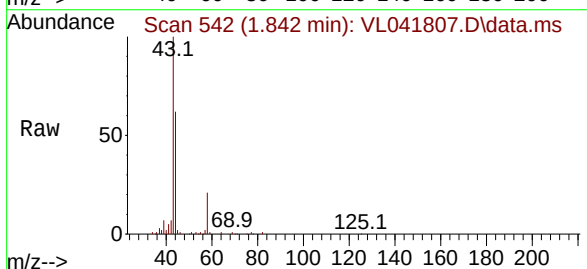



#16

1,3-Butadiene

Concen: 0.115 ppbv

RT: 1.609 min Scan# 41

Delta R.T. 0.003 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_L





ClientSampleId :

Tgt Ion: 39 Resp: 643

Ion Ratio Lower Upper

39 100

54 0.0 58.4 87.6#

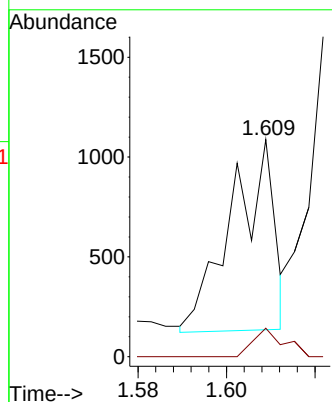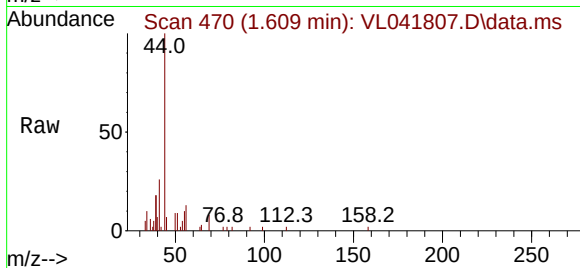

#17

tert-Butyl alcohol

Concen: 0.139 ppbv

RT: 2.049 min Scan# 606

Delta R.T. 0.013 min

Lab File: VL041807.D




Acq: 18 Dec 2024 22:37

Tgt Ion: 59 Resp: 1952


Ion Ratio Lower Upper

59 100

57 19.0 8.6 13.0#

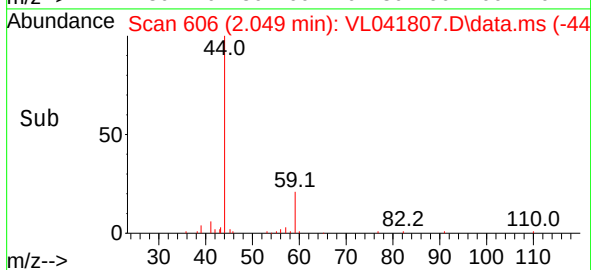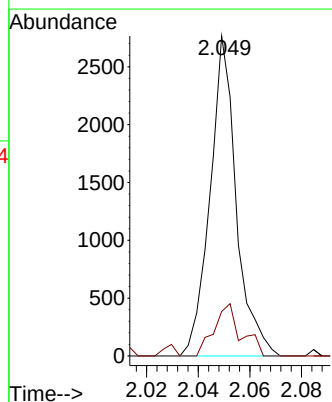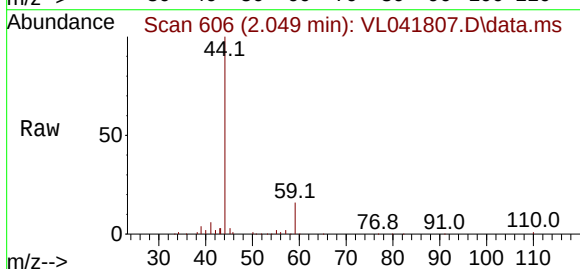









#19  
Isopropyl Alcohol  
Concen: 0.936 ppbv  
RT: 1.894 min Scan# 51  
Delta R.T. 0.009 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37




Instrument :  
MSVOA\_L  
ClientSampleId :


Tgt Ion: 45 Resp: 7976  
Ion Ratio Lower Upper  
45 100  
58 2.9 33.3 49.9#

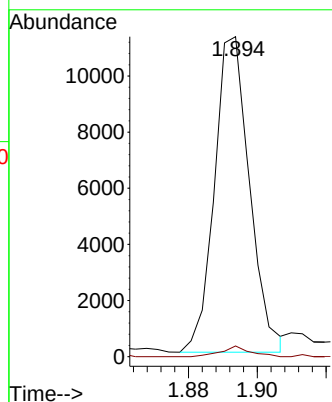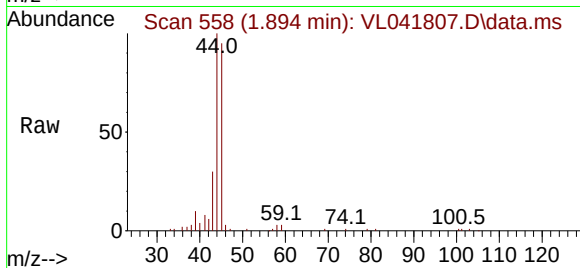

#20  
Methylene Chloride  
Concen: 0.403 ppbv  
RT: 2.068 min Scan# 612  
Delta R.T. 0.009 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37

Tgt Ion: 84 Resp: 1631  
Ion Ratio Lower Upper  
84 100  
49 150.4 132.6 198.8  
51 49.4 37.6 56.4  
86 65.6 51.4 77.0

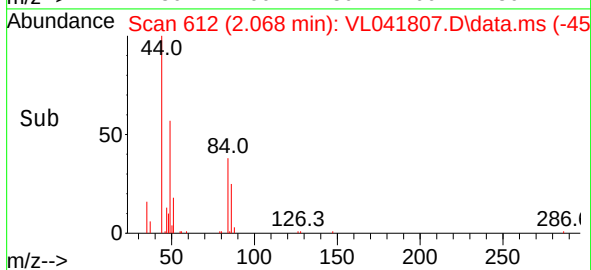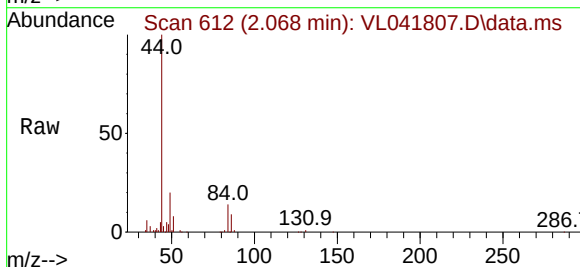



#22

trans-1,2-Dichloroethene

Concen: 0.035 ppbv

RT: 2.797 min Scan# 81

Delta R.T. 0.459 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_L

ClientSampleId :





Tgt Ion: 96 Resp: 174

Ion Ratio Lower Upper

96 100

61 0.0 146.3 219.5#

98 0.0 50.8 76.2#

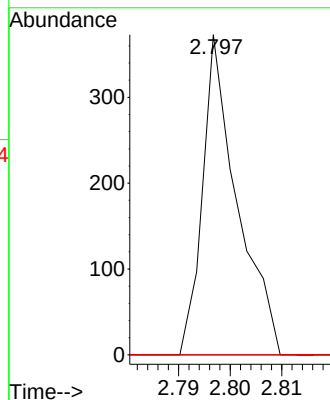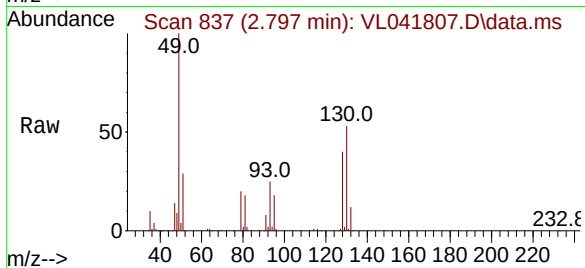

#23

Vinyl Acetate

Concen: 0.084 ppbv

RT: 2.470 min Scan# 736

Delta R.T. 0.013 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Tgt Ion: 43 Resp: 551



Ion Ratio Lower Upper


43 100

86 74.1 6.6 10.0#

42 0.0 8.2 12.2#

44 171.9 5.0 7.4#

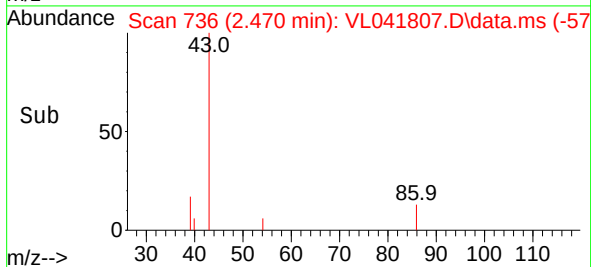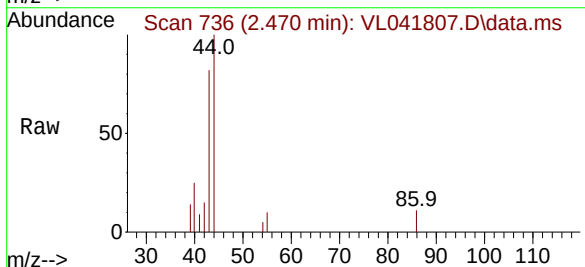



#25

Ethyl Acetate

Concen: 0.142 ppbv

RT: 2.849 min Scan# 849

Delta R.T. 0.016 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_L

ClientSampleId :

Tgt Ion: 43 Resp: 3744





Ion Ratio Lower Upper

43 100

45 20.1 8.1 12.1#

61 11.6 7.0 10.6#

70 8.0 6.5 9.7

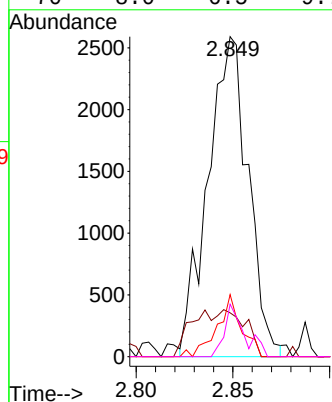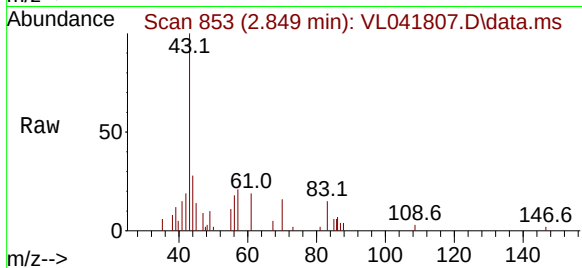

#26

Hexane

Concen: 0.157 ppbv

RT: 2.842 min Scan# 851

Delta R.T. 0.019 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Tgt Ion: 57 Resp: 1571




Ion Ratio Lower Upper


57 100

41 121.2 79.6 119.4#

43 253.7 211.0 316.6

56 73.6 42.6 63.8#

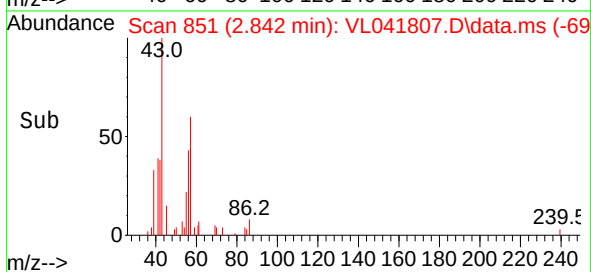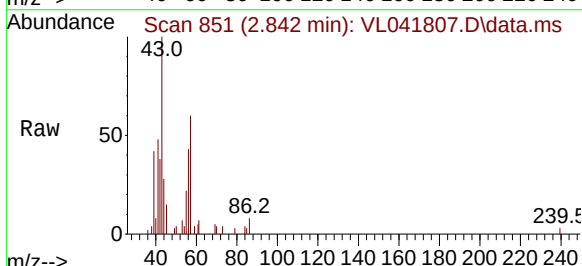



#29

Chloroform

Concen: 0.086 ppbv

RT: 2.861 min Scan# 85

Delta R.T. 0.016 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_L





ClientSampleId :

Tgt Ion: 83 Resp: 1319

Ion Ratio Lower Upper

83 100

85 66.2 51.8 77.6

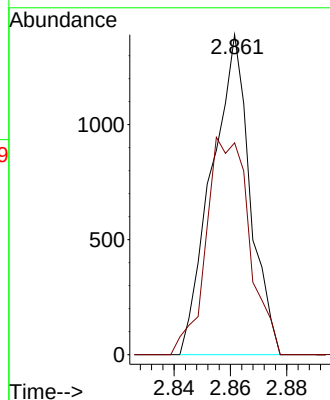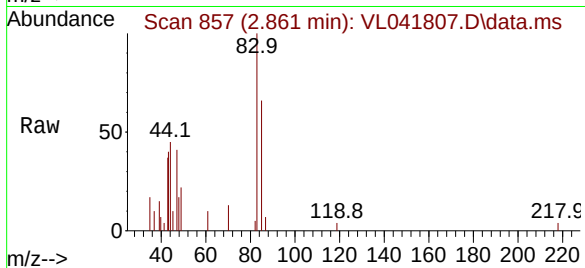

#30

Cyclohexane

Concen: 0.037 ppbv

RT: 3.871 min Scan# 1169

Delta R.T. 0.016 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37




Tgt Ion: 84 Resp: 314


Ion Ratio Lower Upper

84 100

56 170.4 102.3 153.5#

41 201.9 74.0 111.0#

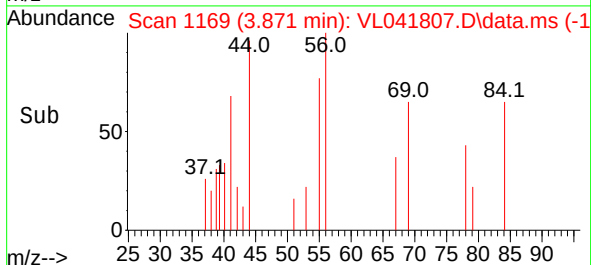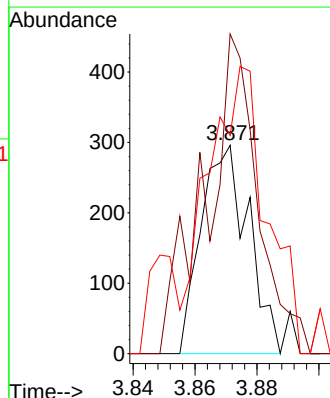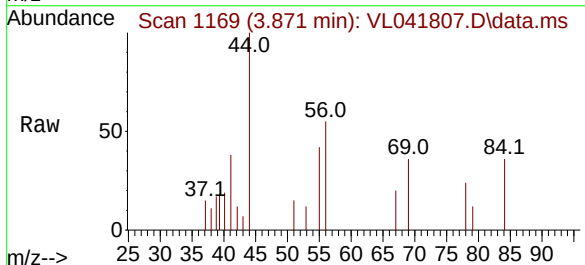



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 3.972 min Scan# 1195

Delta R.T. 0.016 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_L

ClientSampleId :





Tgt Ion:114 Resp: 173625

Ion Ratio Lower Upper

114 100

63 28.1 21.8 32.8

88 18.5 14.8 22.2

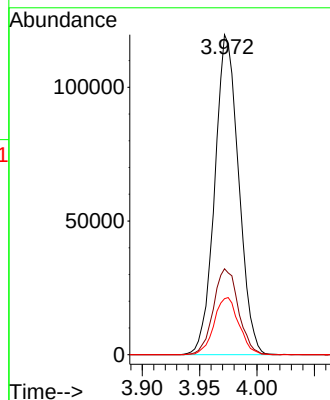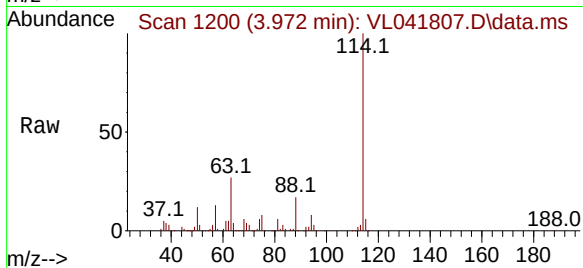

#34

2-Butanone

Concen: 0.203 ppbv

RT: 2.570 min Scan# 767

Delta R.T. 0.016 min

Lab File: VL041807.D




Acq: 18 Dec 2024 22:37


Tgt Ion: 43 Resp: 2830

Ion Ratio Lower Upper

43 100

72 19.3 16.8 25.2

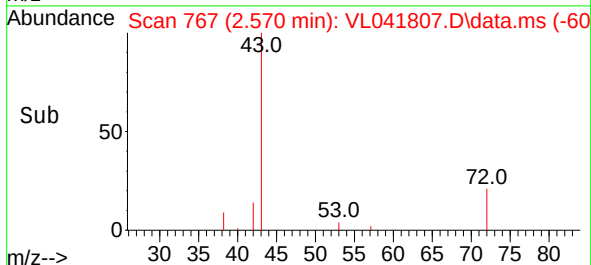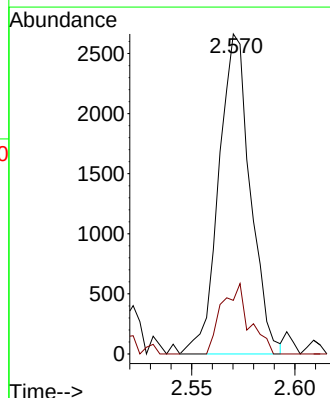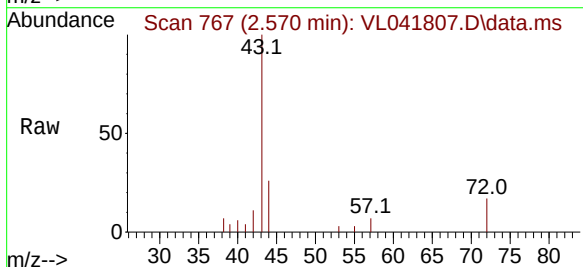



#36

Benzene

Concen: 0.053 ppbv

RT: 3.674 min Scan# 1108

Delta R.T. 0.019 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_L

ClientSampleId :





Tgt Ion: 78 Resp: 945

Ion Ratio Lower Upper

78 100

77 31.7 17.8 26.6#

50 12.7 17.2 25.8#

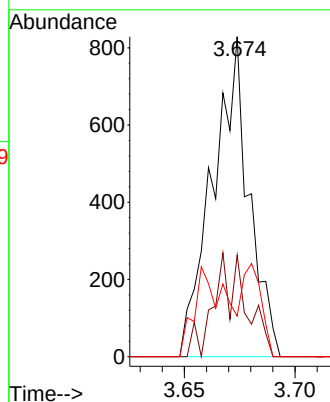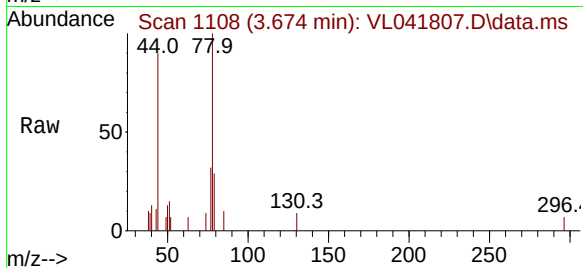

#38

Trichloroethene

Concen: 0.122 ppbv

RT: 4.564 min Scan# 1383

Delta R.T. 0.019 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Tgt Ion:130 Resp: 929




Ion Ratio Lower Upper


130 100

95 37.6 87.0 130.6#

132 31.3 75.0 112.6#

97 30.0 57.2 85.8#

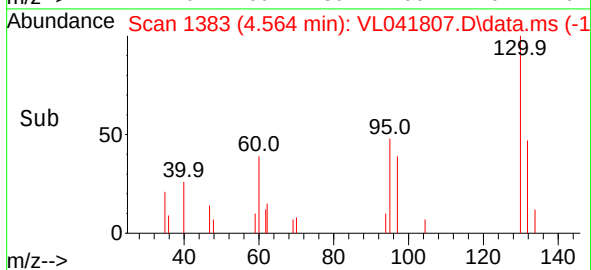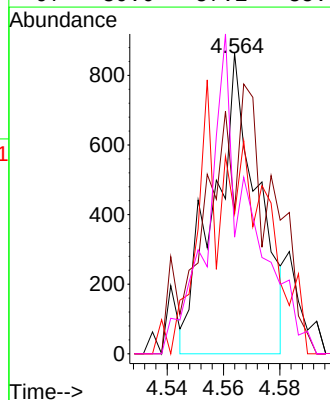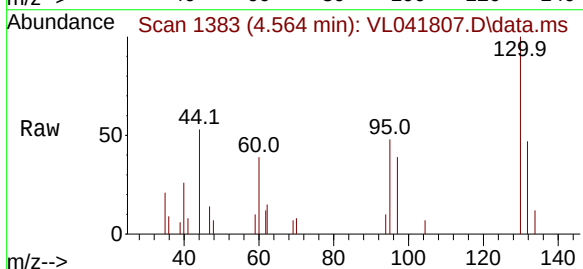



#39

1,2-Dichloropropane

Concen: 7.494 ppbv

RT: 3.972 min Scan# 11

Delta R.T. -0.337 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_L

ClientSampleId :





Tgt Ion: 63 Resp: 48675

Ion Ratio Lower Upper

63 100

41 0.6 75.3 112.9#

62 20.3 57.3 85.9#

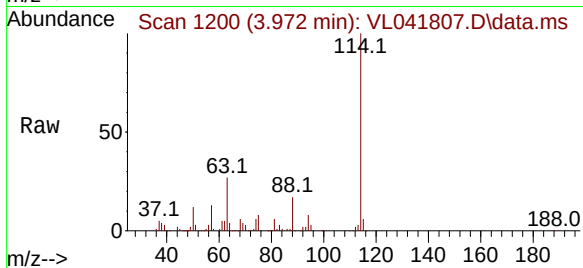

#41

Tetrahydrofuran

Concen: 0.132 ppbv

RT: 3.078 min Scan# 924

Delta R.T. 0.029 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37




Tgt Ion: 42 Resp: 1030


Ion Ratio Lower Upper

42 100

72 41.8 29.1 43.7


71 32.8 28.4 42.6

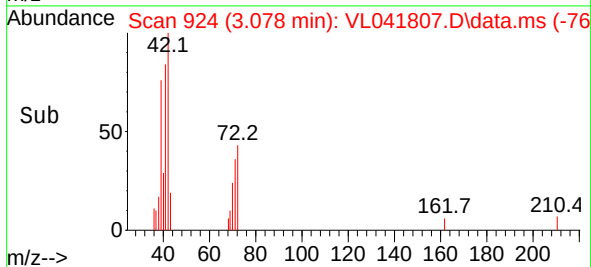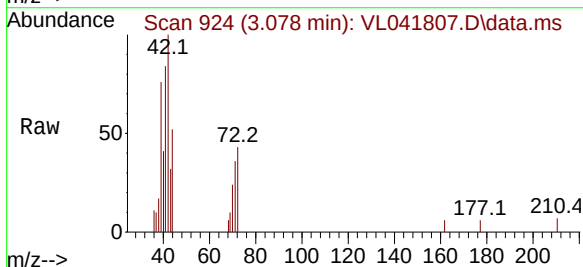






#52  
Tetrachloroethene  
Concen: 27.596 ppbv  
RT: 8.241 min Scan# 2120  
Delta R.T. 0.019 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37

Instrument :  
MSVOA\_L  
ClientSampleId :






Tgt Ion:164 Resp: 184475  
Ion Ratio Lower Upper  
164 100  
166 129.1 99.8 149.6  
129 109.7 79.6 119.4  
131 106.7 78.6 117.8

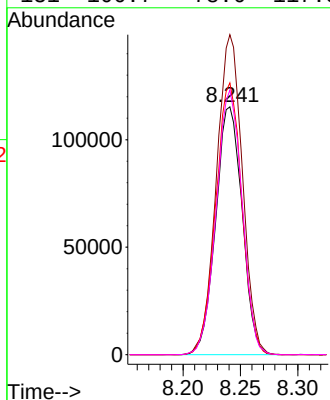


#53  
Toluene  
Concen: 0.842 ppbv  
RT: 6.949 min Scan# 2120  
Delta R.T. 0.019 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37

Tgt Ion: 91 Resp: 17152  
Ion Ratio Lower Upper  
91 100  
92 59.6 47.9 71.9

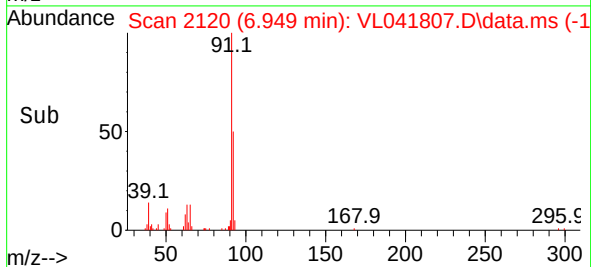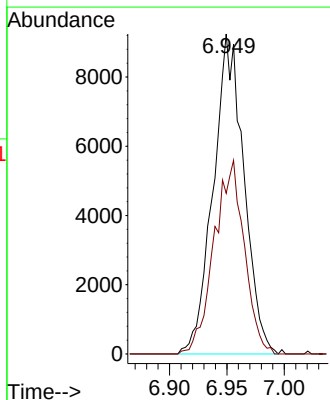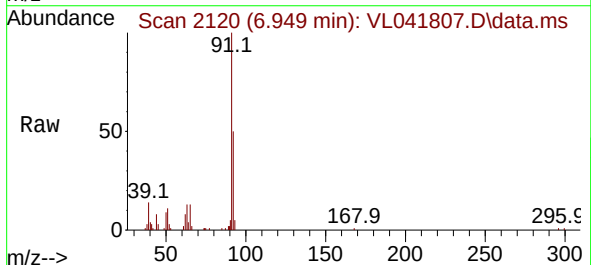









#55  
Chlorobenzene-d5  
Concen: 10.000 ppbv  
RT: 8.895 min Scan# 21  
Delta R.T. 0.016 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37




Instrument :  
MSVOA\_L  
ClientSampleId :


Tgt Ion:117 Resp: 170332  
Ion Ratio Lower Upper  
117 100  
82 68.1 53.8 80.8  
119 32.1 26.7 40.1

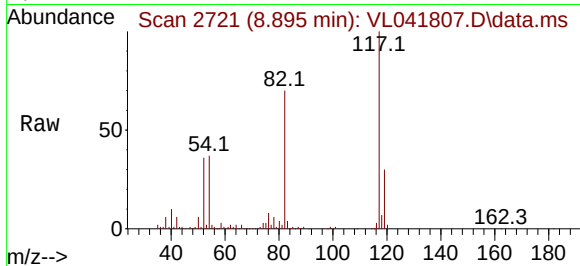

#57  
Chlorobenzene  
Concen: 0.042 ppbv  
RT: 8.937 min Scan# 2734  
Delta R.T. 0.016 min  
Lab File: VL041807.D  
Acq: 18 Dec 2024 22:37

Tgt Ion:112 Resp: 734  
Ion Ratio Lower Upper  
112 100  
77 32.3 57.4 86.0#  
114 46.1 27.4 33.4#

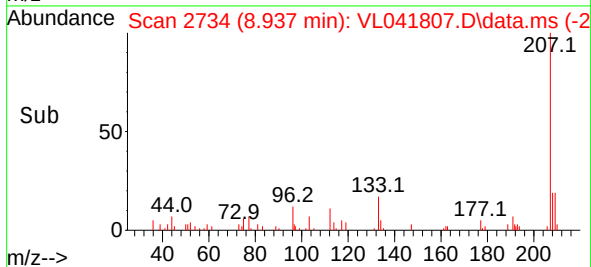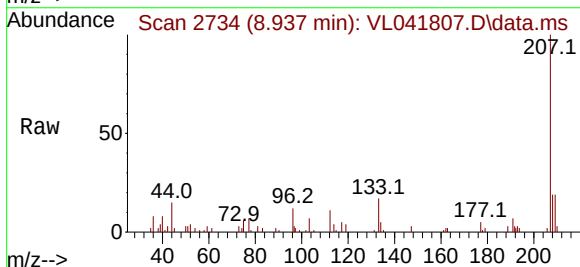



#58

Ethyl Benzene

Concen: 0.123 ppbv

RT: 9.364 min Scan# 2866

Delta R.T. 0.009 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_1





ClientSampleId :

Tgt Ion: 91 Resp: 3771

Ion Ratio Lower Upper

91 100

106 24.6 23.5 35.3

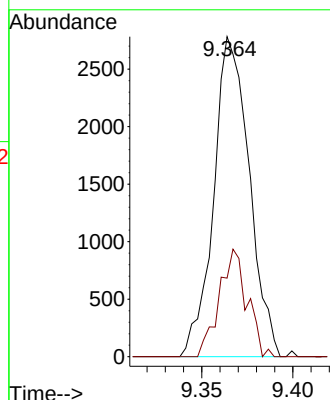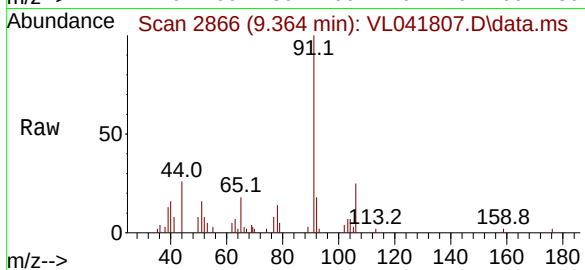

#59

m/p-Xylene

Concen: 0.065 ppbv

RT: 9.548 min Scan# 2923

Delta R.T. -0.000 min

Lab File: VL041807.D




Acq: 18 Dec 2024 22:37


Tgt Ion: 91 Resp: 1601

Ion Ratio Lower Upper

91 100

106 262.5 0.0 0.0#

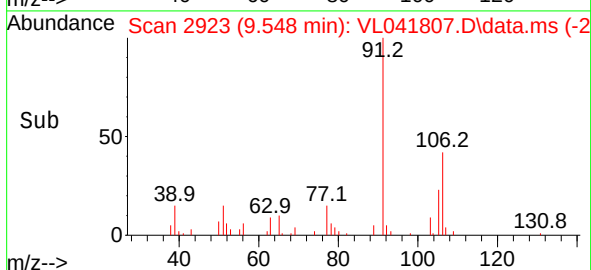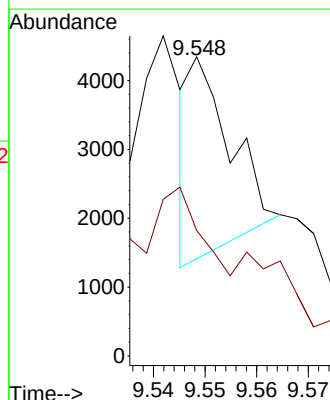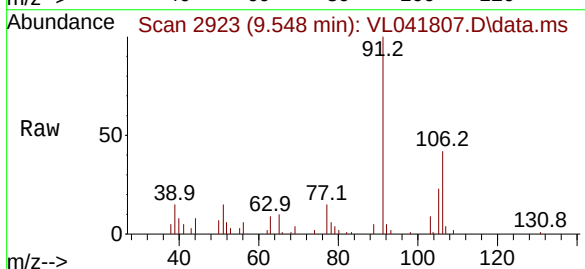



#60

o-Xylene

Concen: 0.136 ppbv

RT: 9.972 min Scan# 3051

Delta R.T. 0.009 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37

Instrument :

MSVOA\_L





ClientSampleId :

Tgt Ion: 91 Resp: 3367

Ion Ratio Lower Upper

91 100

106 42.3 21.1 63.4



#61

Styrene

Concen: 0.099 ppbv

RT: 9.885 min Scan# 3027

Delta R.T. 0.016 min

Lab File: VL041807.D

Acq: 18 Dec 2024 22:37




Tgt Ion: 104 Resp: 1059


Ion Ratio Lower Upper

104 100

78 49.2 43.8 65.6


103 40.2 37.8 56.6

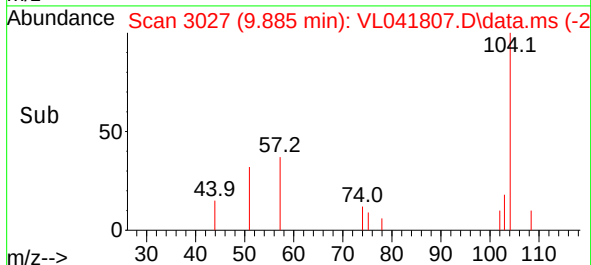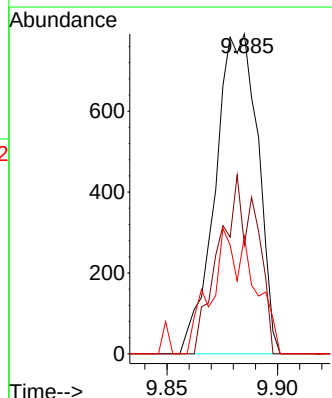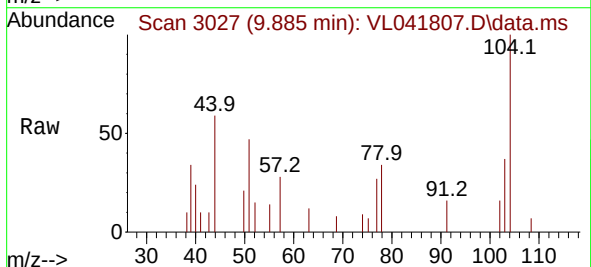

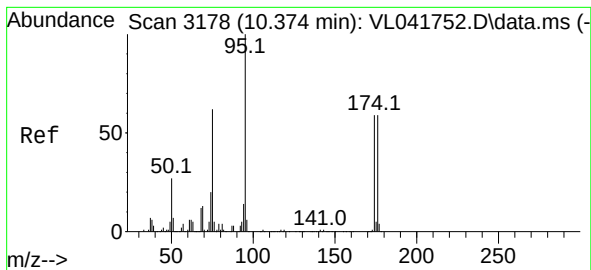

#68  
 1-Bromo-4-Fluorobenzene  
 Concen: 9.570 ppbv  
 RT: 10.387 min Scan# 3178  
 Delta R.T. 0.013 min  
 Lab File: VL041807.D  
 Acq: 18 Dec 2024 22:37

Instrument :  
 MSVOA\_L  
 ClientSampleId :

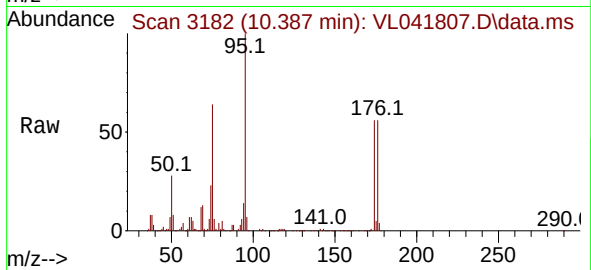

Tgt Ion: 95 Resp: 135837  
 Ion Ratio Lower Upper  
 95 100  
 174 57.3 47.6 71.4  
 175 4.6 3.7 5.5

