

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
 Data File : VL041800.D
 Acq On : 18 Dec 2024 18:50
 Operator : SY/MD
 Sample : P5293-03
 Misc : 400mL/MSVOA_L
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 C0AC1

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 12/19/2024
 Supervised By : Mahesh Dadoda 12/19/2024

Quant Time: Dec 19 07:57:35 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Thu Dec 19 07:32:09 2024

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.797	49	75472	10.000	ppbv	0.01
33) 1,4-Difluorobenzene	3.971	114	186655	10.000	ppbv	0.02
55) Chlorobenzene-d5	8.894	117	166096	10.000	ppbv	0.02
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.390	95	150452	10.870	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	= 108.700%	
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.502	85	5105	0.380	ppbv	91
3) Chlorodifluoromethane	1.479	51	3096m	0.252	ppbv	
4) Chloromethane	1.537	50	10014	1.906	ppbv	92
9) Propene	1.486	41	31355	5.878	ppbv	88
10) Heptane	4.994	43	4991m	0.364	ppbv	
11) Trichlorofluoromethane	1.884	101	2747	0.193	ppbv #	82
13) Ethanol	1.732	45	2100930	4756.166	ppbv	99
15) Acetone	1.838	43	315433	21.480	ppbv	98
17) tert-Butyl alcohol	2.052	59	15513	1.065	ppbv	100
19) Isopropyl Alcohol	1.894	45	43147	4.897	ppbv #	1
20) Methylene Chloride	2.068	84	6983	1.668	ppbv	88
25) Ethyl Acetate	2.848	43	30957	1.133	ppbv #	90
29) Chloroform	2.858	83	23212	1.469	ppbv	95
34) 2-Butanone	2.567	43	72623	4.836	ppbv	99
35) Carbon Tetrachloride	3.777	117	981m	0.074	ppbv	
36) Benzene	3.667	78	15442	0.800	ppbv	97
42) Bromodichloromethane	4.499	83	3849m	0.278	ppbv	
50) 4-Methyl-2-Pentanone	5.800	43	5944m	0.291	ppbv	
53) Toluene	6.949	91	27768	1.269	ppbv	96
58) Ethyl Benzene	9.364	91	10320m	0.345	ppbv	
59) m/p-Xylene	9.545	91	39541	1.645	ppbv #	100
60) o-Xylene	9.975	91	15281	0.634	ppbv	97
61) Styrene	9.885	104	4539	0.435	ppbv	98
64) n-propylbenzene	10.995	120	2431m	0.265	ppbv	
69) p-Isopropyltoluene	11.937	119	6800	0.182	ppbv #	85
72) 4-Ethyltoluene	11.137	105	15210	0.534	ppbv #	55
73) 1,3,5-Trimethylbenzene	11.215	105	15880	0.673	ppbv	89
74) 1,2,4-Trimethylbenzene	11.548	105	73547	2.896	ppbv #	58
79) Naphthalene	13.526	128	3853m	0.218	ppbv	
80) Naphthalene,2-methyl-	14.471	142	645	0.118	ppbv #	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
Data File : VL041800.D
Acq On : 18 Dec 2024 18:50
Operator : SY/MD
Sample : P5293-03
Misc : 400mL/MSVOA_L
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
C0AC1

Quant Time: Dec 19 07:57:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Thu Dec 19 07:32:09 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 12/19/2024
Supervised By : Mahesh Dadoda 12/19/2024

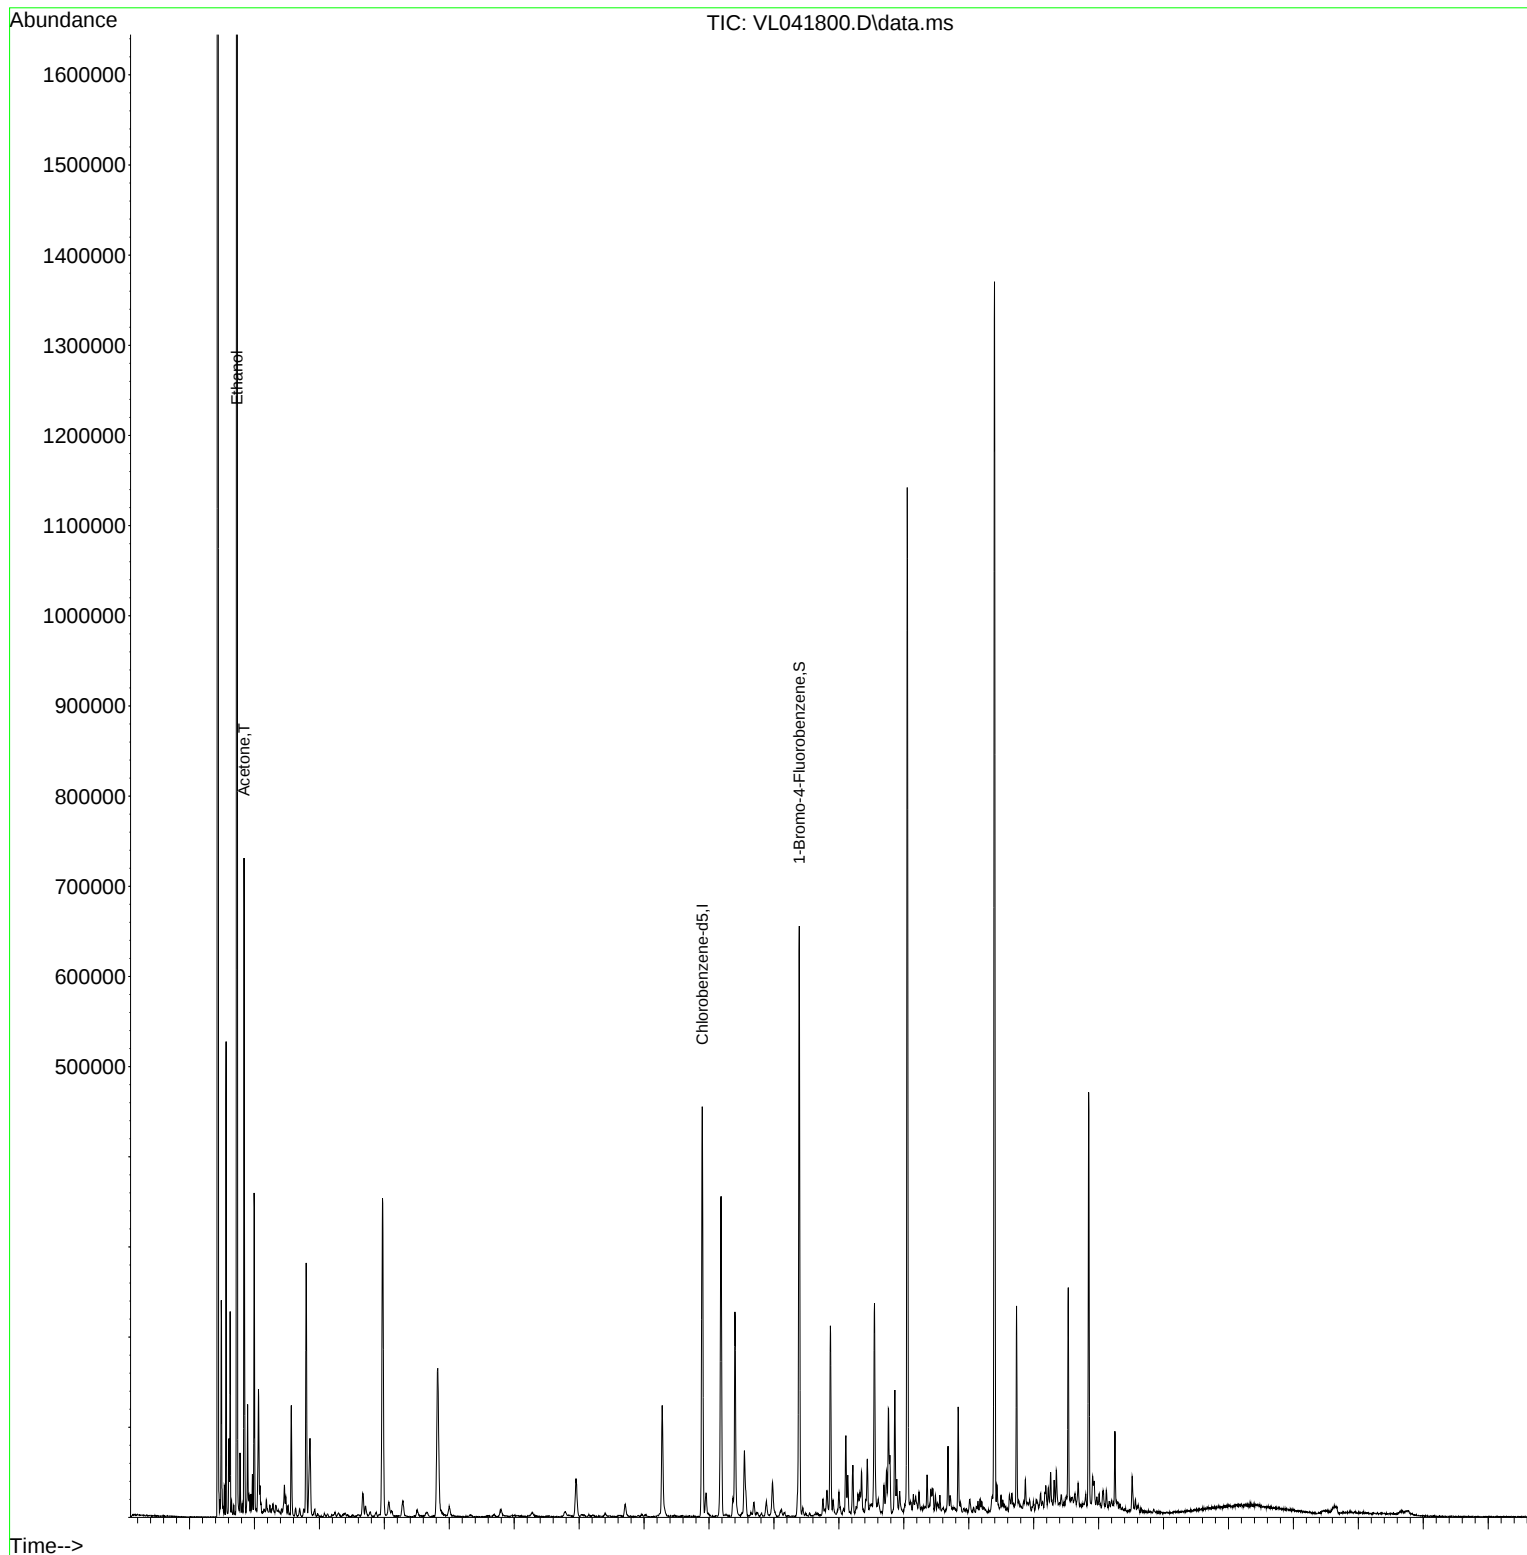



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.797 min Scan# 833
Delta R.T. 0.013 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1

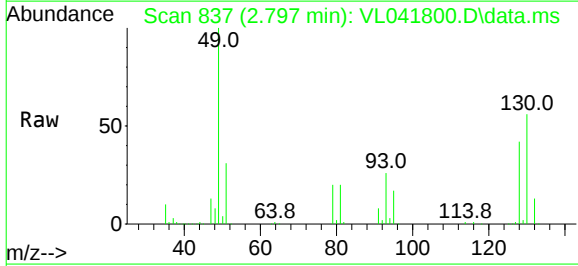

Tgt Ion: 49 Resp: 75472
Ion Ratio Lower Upper
49 100
128 41.8 21.6 64.6
130 53.9 28.3 85.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

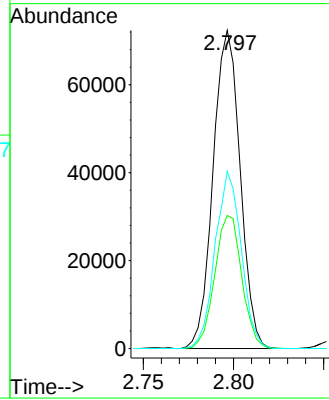

#2
Dichlorodifluoromethane
Concen: 0.380 ppbv
RT: 1.502 min Scan# 437
Delta R.T. 0.006 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50


Tgt Ion: 85 Resp: 5105
Ion Ratio Lower Upper
85 100
87 35.6 24.5 36.7

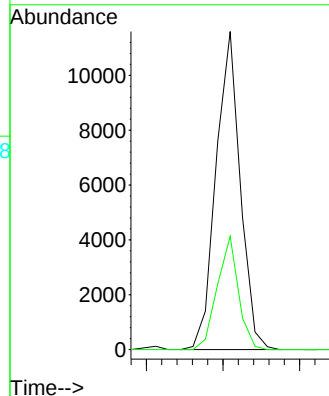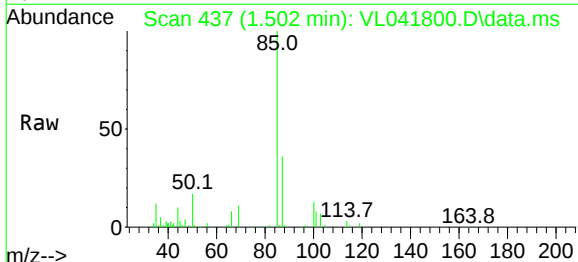



#3
Chlorodifluoromethane
Concen: 0.252 ppbv
RT: 1.479 min Scan# 431
Delta R.T. 0.006 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1



Tgt Ion: 51 Resp: 3096
Ion Ratio Lower Upper
51 100
67 3.0 15.0 22.4#




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

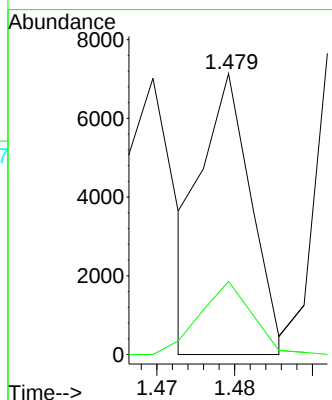

#4
Chloromethane
Concen: 1.906 ppbv
RT: 1.537 min Scan# 448
Delta R.T. 0.006 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

Tgt Ion: 50 Resp: 10014
Ion Ratio Lower Upper
50 100
52 28.1 26.2 39.2

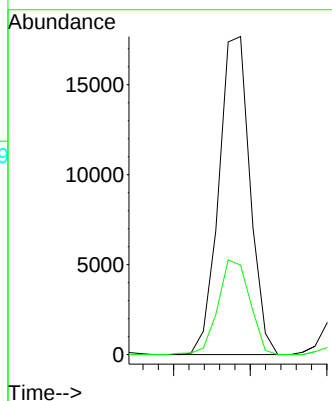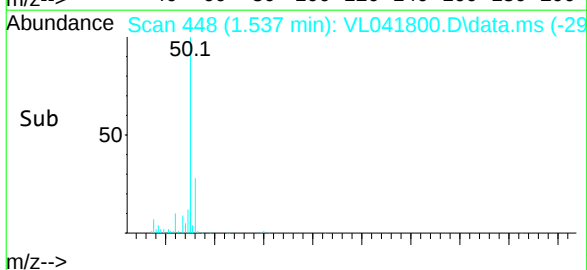



#9

Propene

Concen: 5.878 ppbv

RT: 1.486 min Scan# 431

Delta R.T. 0.003 min

Lab File: VL041800.D

Acq: 18 Dec 2024 18:50

Instrument :

MSVOA_L

ClientSampleId :

C0AC1

Tgt Ion: 41 Resp: 31355

Ion Ratio Lower Upper

41 100





42 55.6 52.4 78.6

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 12/19/2024

Supervised By :Mahesh Dadoda 12/19/2024

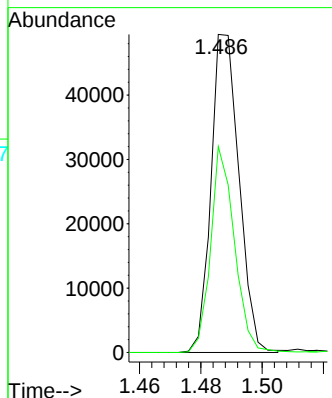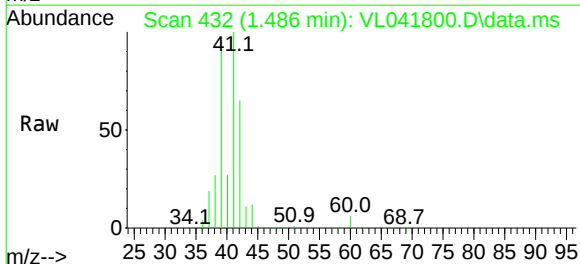

#10

Heptane

Concen: 0.364 ppbv m

RT: 4.994 min Scan# 1516

Delta R.T. 0.016 min

Lab File: VL041800.D




Acq: 18 Dec 2024 18:50


Tgt Ion: 43 Resp: 4991

Ion Ratio Lower Upper

43 100

57 37.8 38.5 57.7#

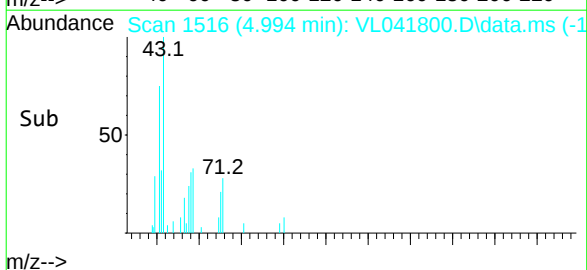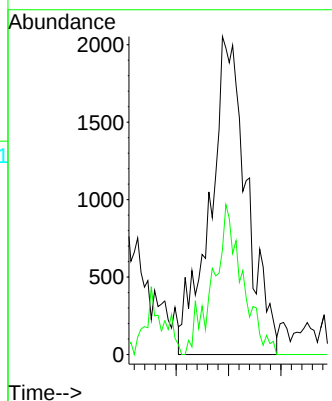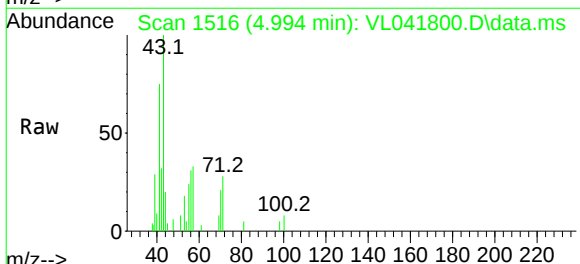







#11
Trichlorofluoromethane
Concen: 0.193 ppbv
RT: 1.884 min Scan# 552
Delta R.T. 0.009 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

Instrument :
MSVOA_L
ClientSampleId :
C0AC1

Tgt Ion:101 Resp: 2747
Ion Ratio Lower Upper
101 100
103 50.7 51.8 77.8#




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

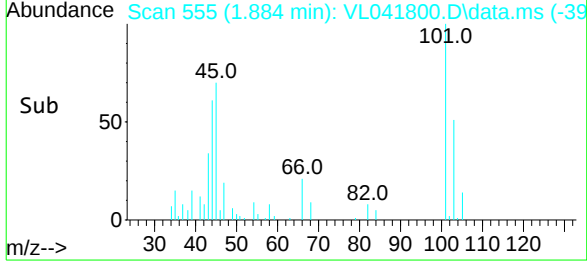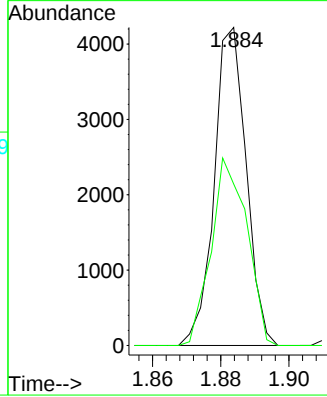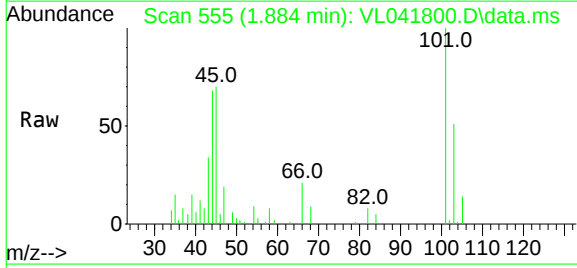

#13
Ethanol
Concen: 4756.166 ppbv
RT: 1.732 min Scan# 508
Delta R.T. 0.012 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50


Tgt Ion: 45 Resp: 2100930
Ion Ratio Lower Upper
45 100
46 40.2 16.4 65.8

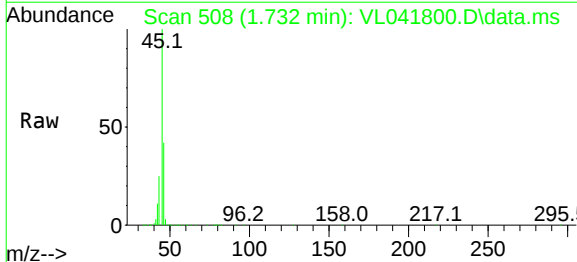



#15
Acetone
Concen: 21.480 ppbv
RT: 1.838 min Scan# 541
Delta R.T. 0.006 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1

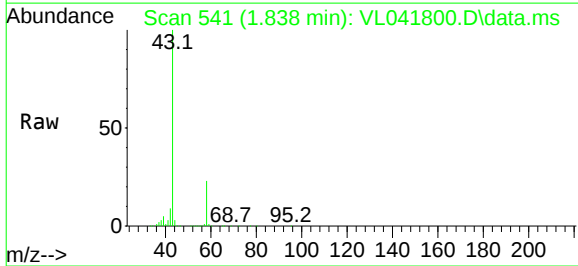

Tgt Ion: 43 Resp: 315433
Ion Ratio Lower Upper
43 100
58 23.8 19.7 29.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

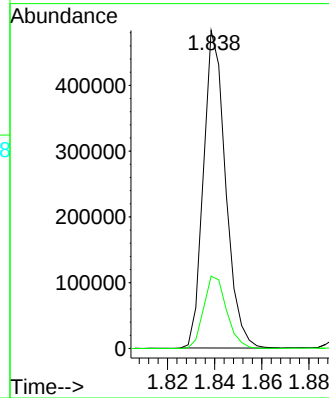

#17
tert-Butyl alcohol
Concen: 1.065 ppbv
RT: 2.052 min Scan# 607
Delta R.T. 0.016 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50


Tgt Ion: 59 Resp: 15513
Ion Ratio Lower Upper
59 100
57 10.7 8.6 13.0

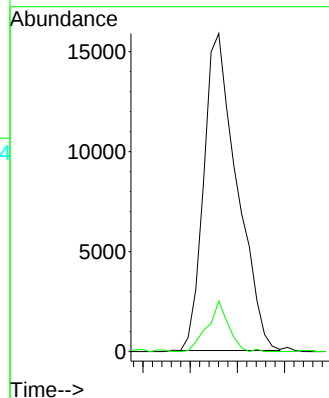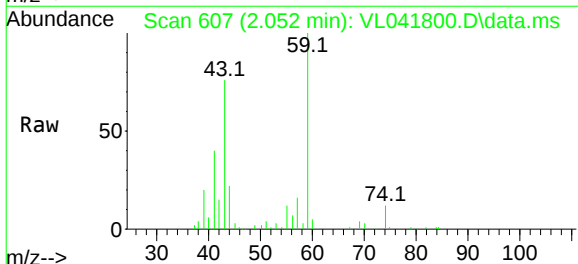



#19
Isopropyl Alcohol
Concen: 4.897 ppbv
RT: 1.894 min Scan# 555
Delta R.T. 0.009 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1




Tgt Ion: 45 Resp: 43147
Ion Ratio Lower Upper
45 100
58 172.8 33.3 49.9#

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

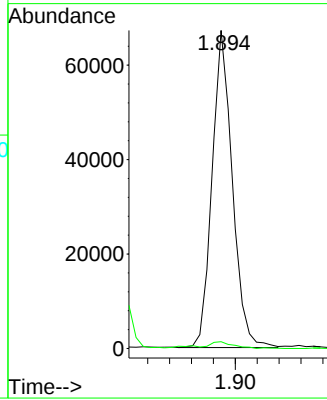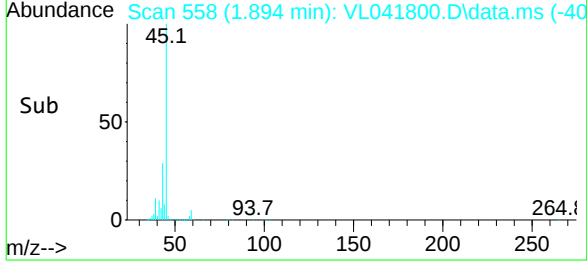


#20
Methylene Chloride
Concen: 1.668 ppbv
RT: 2.068 min Scan# 612
Delta R.T. 0.009 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

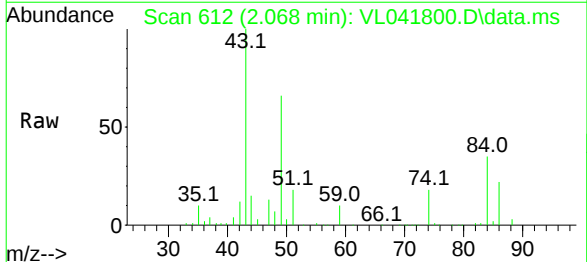


Tgt Ion: 84 Resp: 6983
Ion Ratio Lower Upper
84 100
49 191.7 132.6 198.8
51 47.4 37.6 56.4
86 65.1 51.4 77.0

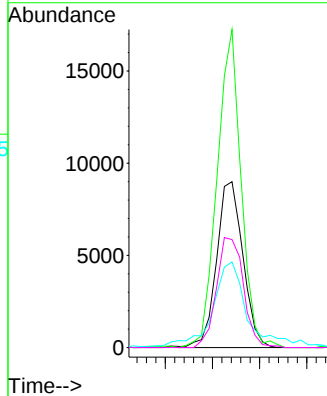



#25
Ethyl Acetate
Concen: 1.133 ppbv
RT: 2.848 min Scan# 855
Delta R.T. 0.016 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1

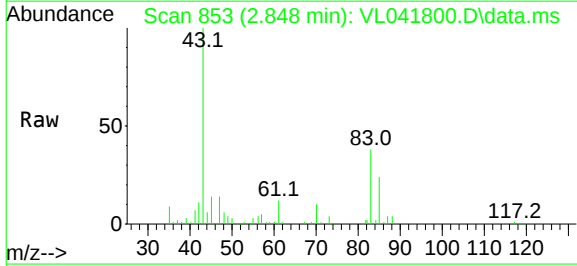

Tgt Ion	Ratio	Lower	Upper
43	100		
45	17.4	8.1	12.1
61	10.3	7.0	10.6
70	9.6	6.5	9.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

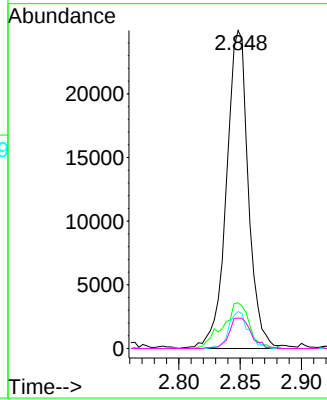

#29
Chloroform
Concen: 1.469 ppbv
RT: 2.858 min Scan# 856
Delta R.T. 0.012 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50


Tgt Ion	Ratio	Lower	Upper
83	100		
85	60.8	51.8	77.6

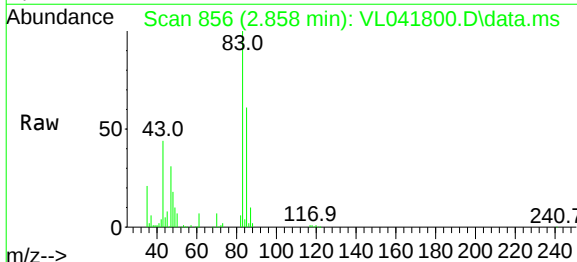

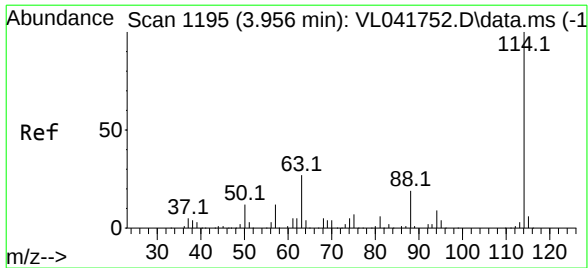

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.971 min Scan# 12
Delta R.T. 0.016 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1

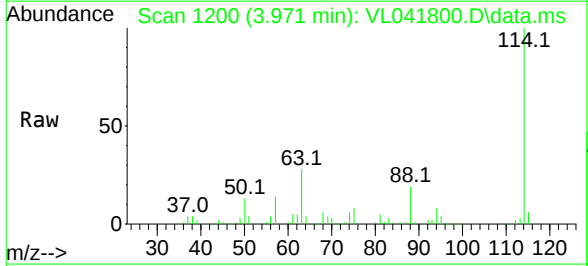

Tgt Ion: 114 Resp: 186655
Ion Ratio Lower Upper
114 100
63 27.7 21.8 32.8
88 18.3 14.8 22.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

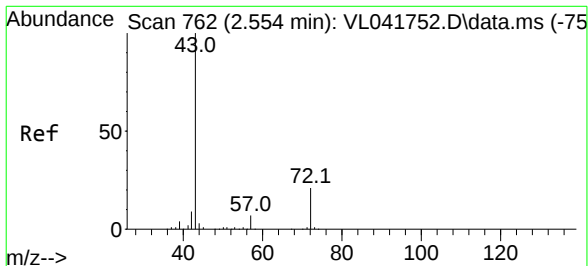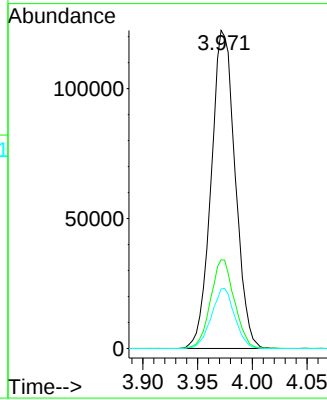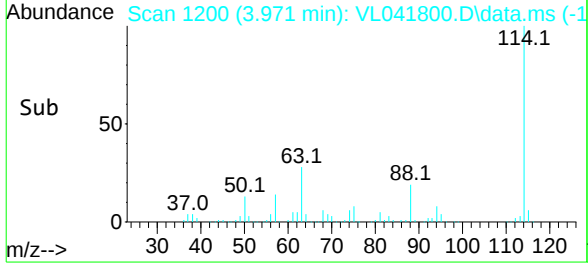

#34
2-Butanone
Concen: 4.836 ppbv
RT: 2.567 min Scan# 766
Delta R.T. 0.012 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50


Tgt Ion: 43 Resp: 72623
Ion Ratio Lower Upper
43 100
72 20.6 16.8 25.2

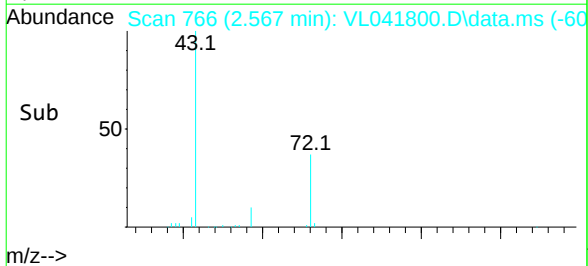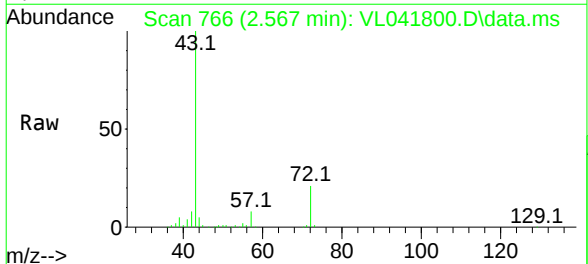



#35
Carbon Tetrachloride
Concen: 0.074 ppbv m
RT: 3.777 min Scan# 11
Delta R.T. 0.019 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1

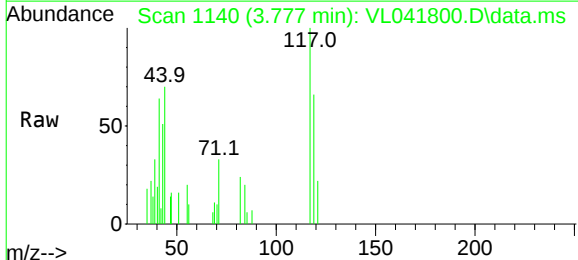

Tgt Ion: 117 Resp: 981
Ion Ratio Lower Upper
117 100
119 66.1 73.7 110.5#
121 22.4 23.0 34.4#




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024



#36
Benzene
Concen: 0.800 ppbv
RT: 3.667 min Scan# 1106
Delta R.T. 0.012 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50


Tgt Ion: 78 Resp: 15442
Ion Ratio Lower Upper
78 100
77 22.4 17.8 26.6
50 18.4 17.2 25.8

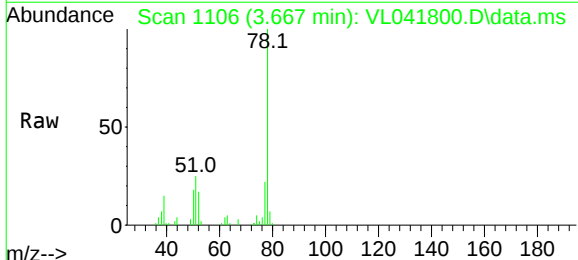



#42
Bromodichloromethane
Concen: 0.278 ppbv m
RT: 4.499 min Scan# 1358
Delta R.T. 0.016 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1




Tgt Ion: 83 Resp: 3849
Ion Ratio Lower Upper
83 100
85 57.4 48.0 72.0
127 8.1 5.8 8.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024




#50
4-Methyl-2-Pentanone
Concen: 0.291 ppbv m
RT: 5.800 min Scan# 1765
Delta R.T. 0.051 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

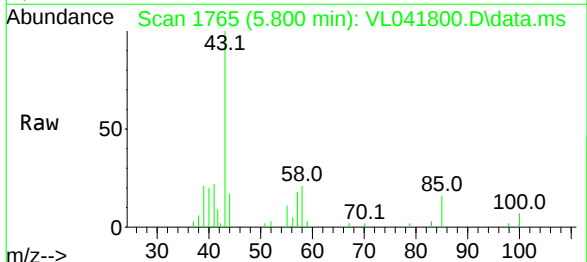

Tgt Ion: 43 Resp: 5944
Ion Ratio Lower Upper
43 100
58 0.0 26.8 40.2#





#53

Toluene

Concen: 1.269 ppbv

RT: 6.949 min Scan# 2114

Delta R.T. 0.019 min

Lab File: VL041800.D

Acq: 18 Dec 2024 18:50

Instrument :

MSVOA_L

ClientSampleId :

C0AC1

Tgt Ion: 91 Resp: 27768

Ion Ratio Lower Upper

91 100





92 57.1 47.9 71.9

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 12/19/2024

Supervised By :Mahesh Dadoda 12/19/2024

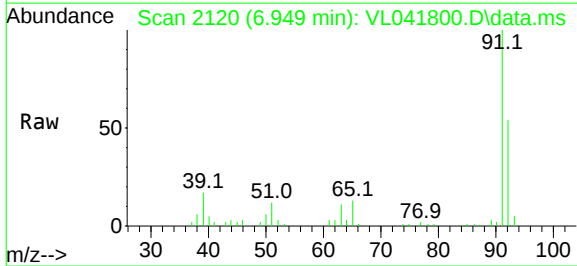

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 8.894 min Scan# 2721

Delta R.T. 0.016 min

Lab File: VL041800.D

Acq: 18 Dec 2024 18:50




Tgt Ion:117 Resp: 166096


Ion Ratio Lower Upper

117 100

82 67.9 53.8 80.8

119 31.7 26.7 40.1





#58

Ethyl Benzene

Concen: 0.345 ppbv m

RT: 9.364 min Scan# 2863

Delta R.T. 0.009 min

Lab File: VL041800.D

Acq: 18 Dec 2024 18:50

Instrument :

MSVOA_L

ClientSampleId :

C0AC1

Tgt Ion: 91 Resp: 10320

Ion Ratio Lower Upper

91 100





106 24.4 23.5 35.3

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 12/19/2024

Supervised By :Mahesh Dadoda 12/19/2024

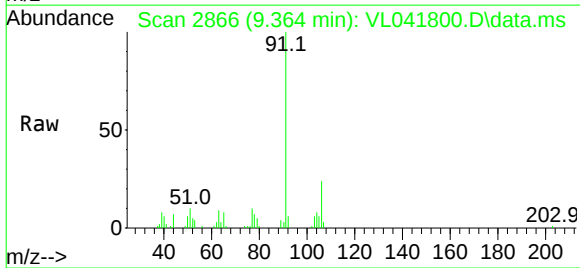

#59

m/p-Xylene

Concen: 1.645 ppbv

RT: 9.545 min Scan# 2922

Delta R.T. -0.004 min

Lab File: VL041800.D




Acq: 18 Dec 2024 18:50


Tgt Ion: 91 Resp: 39541

Ion Ratio Lower Upper

91 100


106 46.9 0.0 0.0#

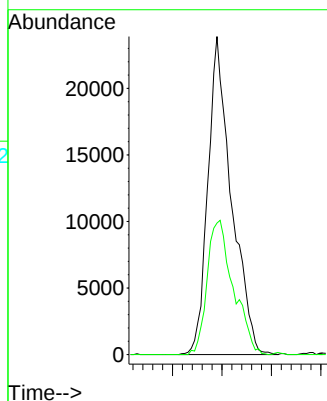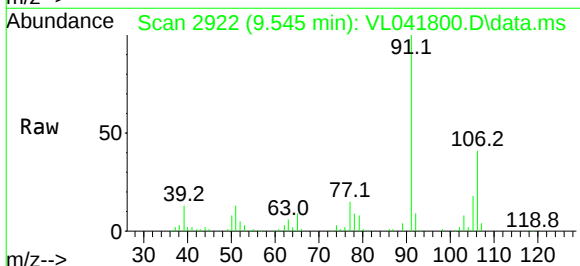

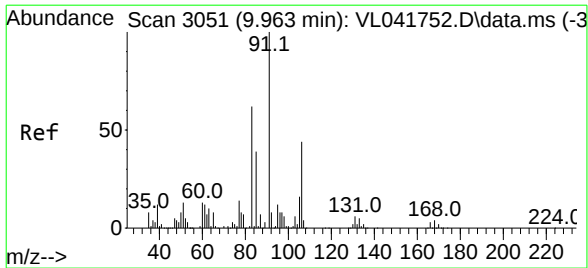

#60
o-Xylene
Concen: 0.634 ppbv
RT: 9.975 min Scan# 3055
Delta R.T. 0.012 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1

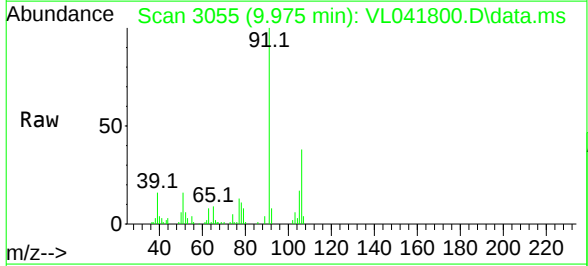

Tgt Ion: 91 Resp: 15281
Ion Ratio Lower Upper
91 100
106 44.0 21.1 63.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

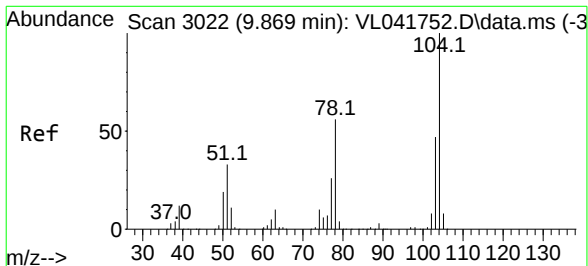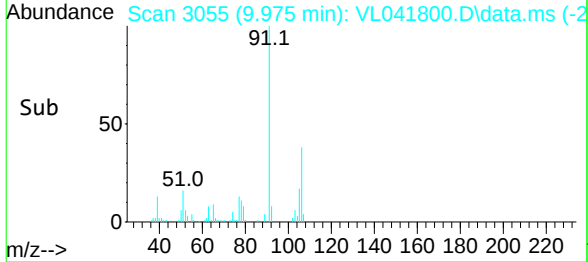

#61
Styrene
Concen: 0.435 ppbv
RT: 9.885 min Scan# 3027
Delta R.T. 0.016 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

Tgt Ion:104 Resp: 4539
Ion Ratio Lower Upper
104 100
78 54.2 43.8 65.6
103 45.3 37.8 56.6

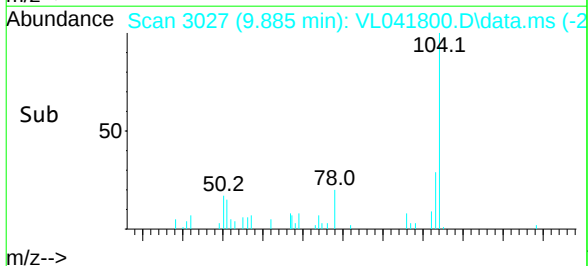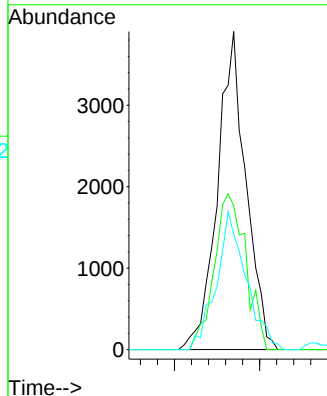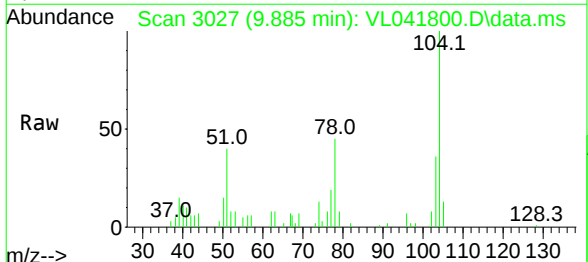

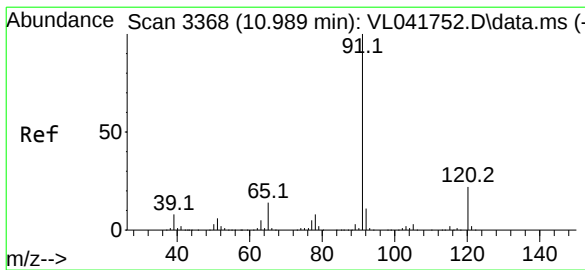





#64
n-propylbenzene
Concen: 0.265 ppbv m
RT: 10.995 min Scan# 3368
Delta R.T. 0.006 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

Instrument :
MSVOA_L
ClientSampleId :
C0AC1

Tgt Ion: 120 Resp: 2431
Ion Ratio Lower Upper
120 100
91 452.3 387.3 580.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

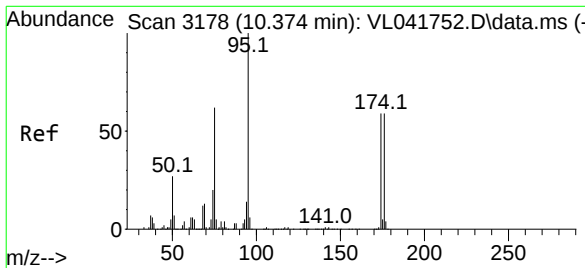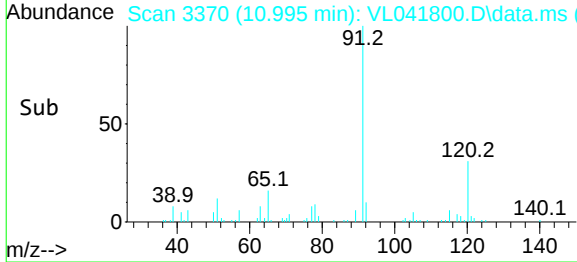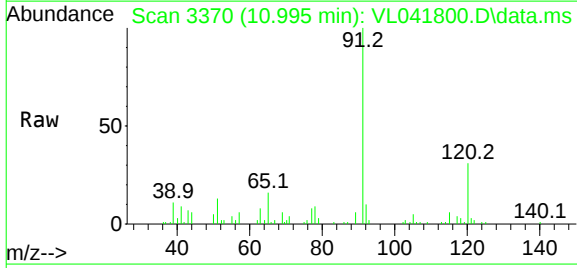

#68
1-Bromo-4-Fluorobenzene
Concen: 10.870 ppbv
RT: 10.390 min Scan# 3183
Delta R.T. 0.016 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

Tgt Ion: 95 Resp: 150452
Ion Ratio Lower Upper
95 100
174 58.0 47.6 71.4
175 4.8 3.7 5.5

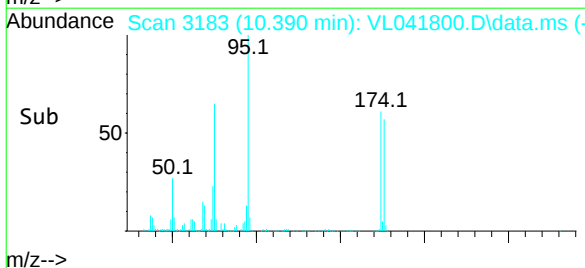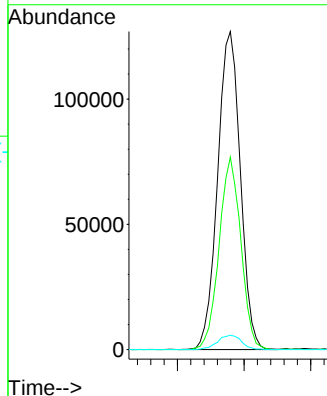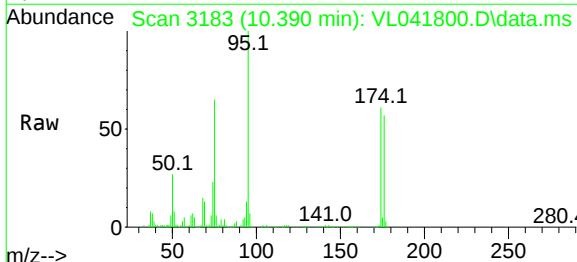



#69

p-Isopropyltoluene

Concen: 0.182 ppbv

RT: 11.937 min Scan# 3657

Delta R.T. 0.012 min

Lab File: VL041800.D

Acq: 18 Dec 2024 18:50

Instrument :

MSVOA_L

ClientSampleId :





C0AC1

Tgt Ion:	119	Resp:	6800
Ion Ratio	Lower	Upper	
119	100		
134	30.8	19.6	29.4#
91	39.3	24.4	36.6#

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

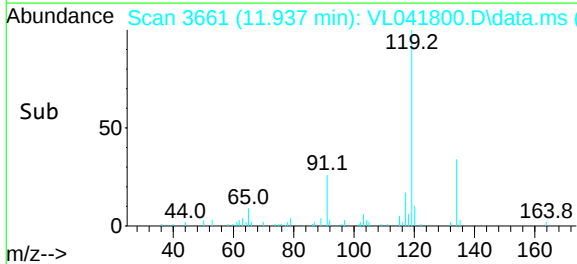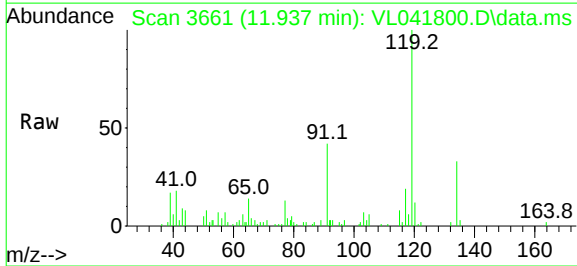

#72

4-Ethyltoluene

Concen: 0.534 ppbv




RT: 11.137 min Scan# 3414


Delta R.T. 0.012 min

Lab File: VL041800.D

Acq: 18 Dec 2024 18:50


Tgt Ion:	105	Resp:	15210
Ion Ratio	Lower	Upper	
105	100		
120	0.0	23.3	34.9#
91	0.0	10.9	16.3#
77	0.0	11.6	17.4#

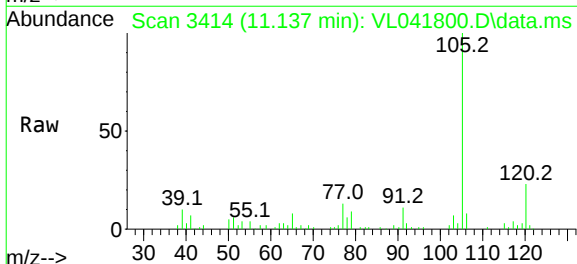

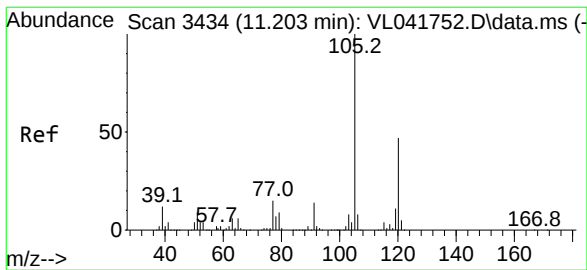

#73
1,3,5-Trimethylbenzene
Concen: 0.673 ppbv
RT: 11.215 min Scan# 341
Delta R.T. 0.012 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50




Instrument :
MSVOA_L
ClientSampleId :
C0AC1

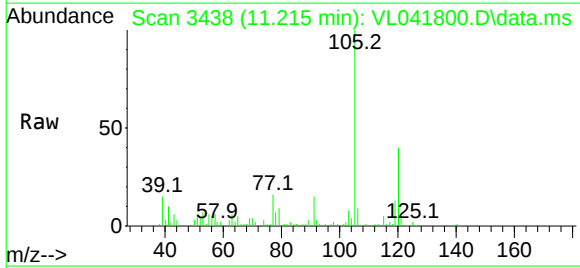

Tgt Ion:105 Resp: 15880
Ion Ratio Lower Upper
105 100
120 39.6 37.4 56.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

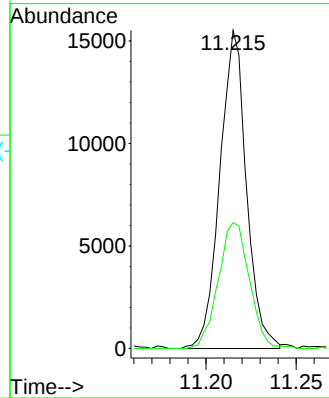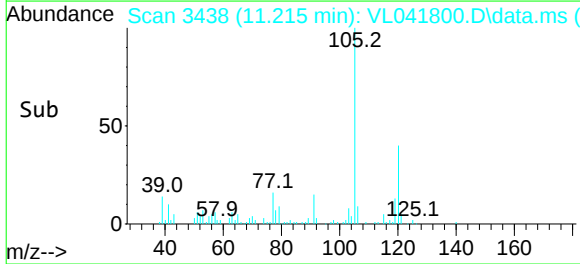

#74
1,2,4-Trimethylbenzene
Concen: 2.896 ppbv
RT: 11.548 min Scan# 3541
Delta R.T. 0.012 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

Tgt Ion:105 Resp: 73547
Ion Ratio Lower Upper
105 100
120 41.5 39.0 58.4
91 13.2 58.1 87.1#
77 15.1 21.8 32.8#

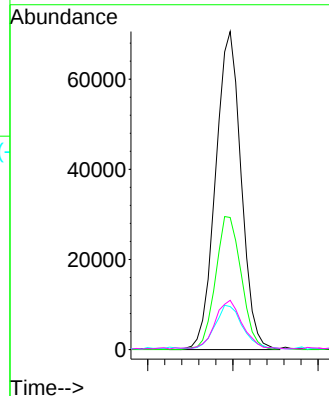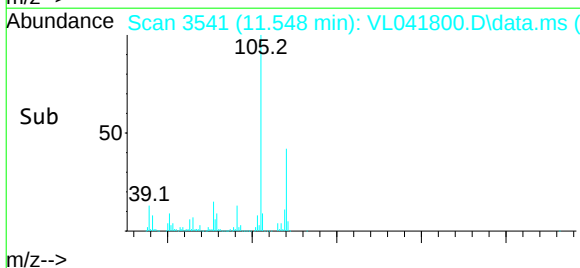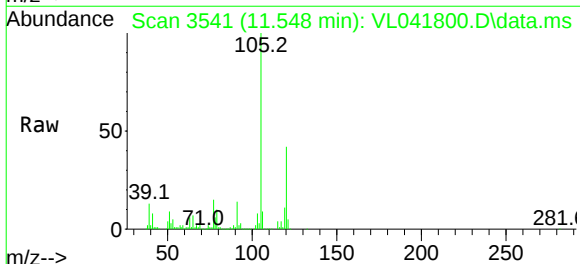

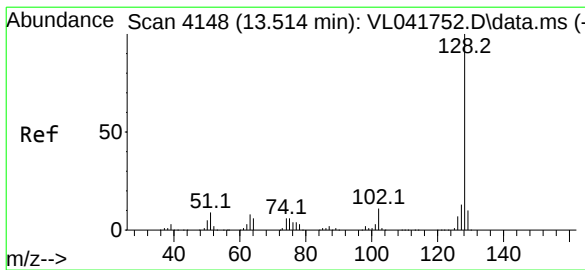





#79
Naphthalene
Concen: 0.218 ppbv m
RT: 13.526 min Scan# 4148
Delta R.T. 0.012 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

Instrument :
MSVOA_L
ClientSampleId :
C0AC1

Tgt Ion:	128	Resp:	3853
Ion Ratio	Lower	Upper	
128	100		
127	17.9	10.7	16.1#
129	16.6	8.2	12.4#

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 12/19/2024
Supervised By :Mahesh Dadoda 12/19/2024

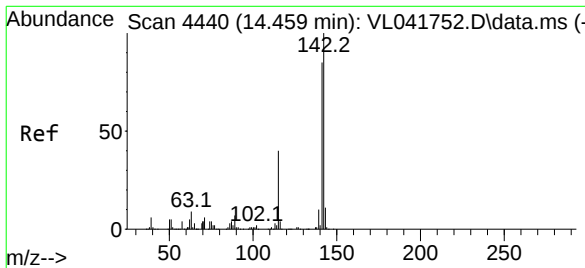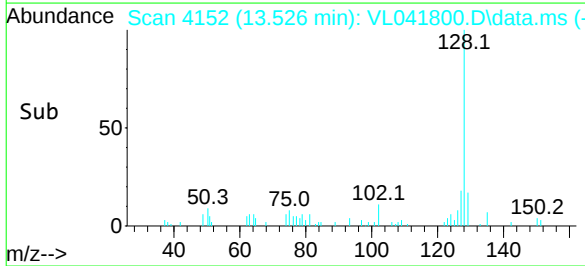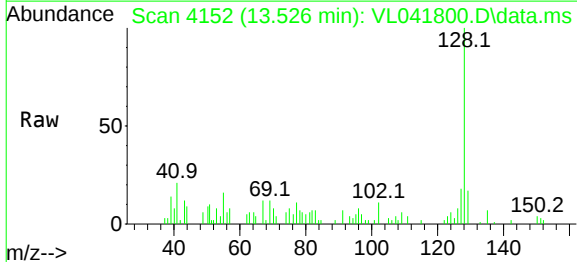

#80
Naphthalene, 2-methyl-
Concen: 0.118 ppbv
RT: 14.471 min Scan# 4444
Delta R.T. 0.012 min
Lab File: VL041800.D
Acq: 18 Dec 2024 18:50

Tgt Ion:	142	Resp:	645
Ion Ratio	Lower	Upper	
142	100		
141	94.1	68.4	102.6
115	81.9	32.5	48.7#

