
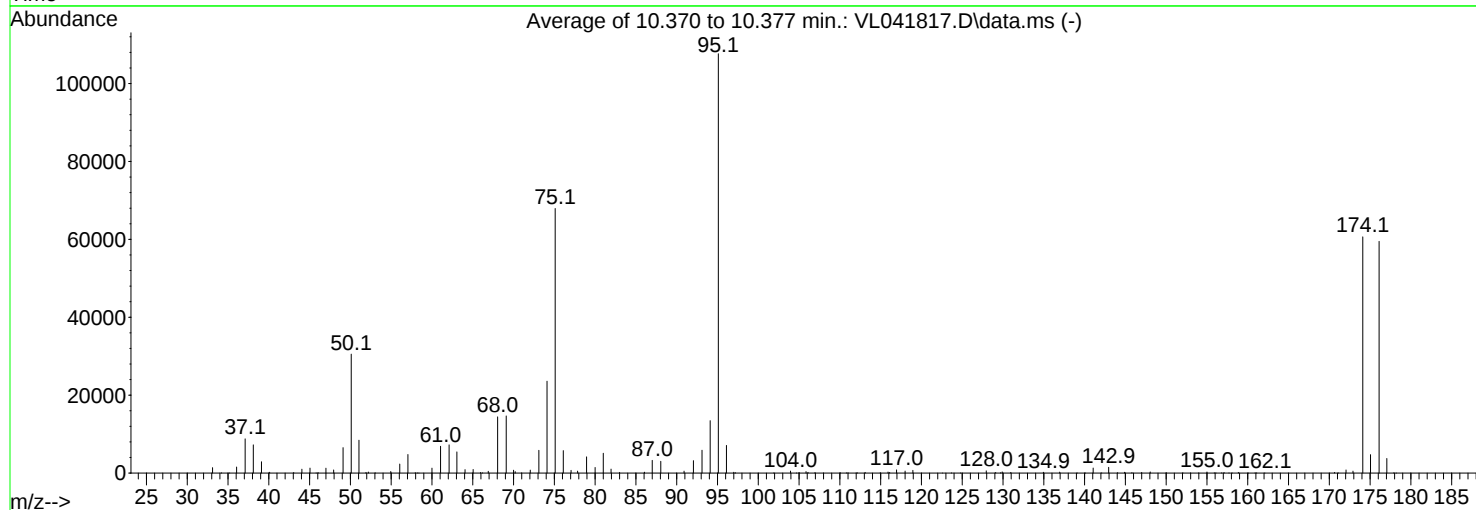


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121924\
Data File : VL041817.D
Acq On : 19 Dec 2024 11:34
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Dec 19 07:32:09 2024

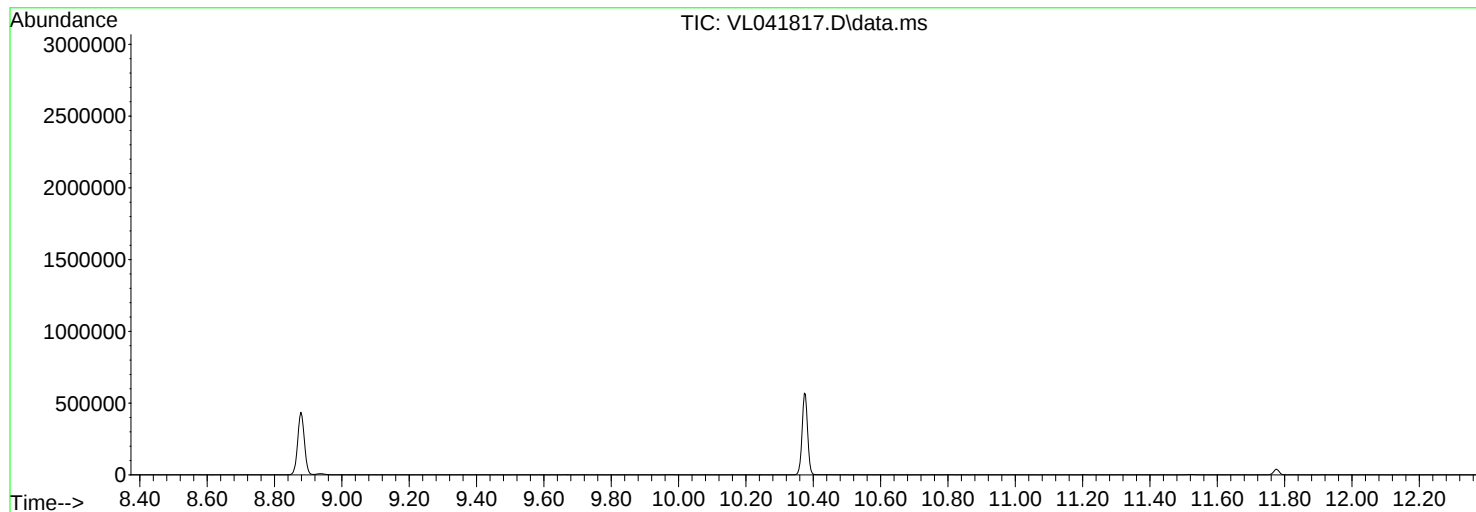

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	28.4	30533	PASS
75	95	30	66	63.1	67925	PASS
95	95	100	100	100.0	107659	PASS
96	95	5	9	6.6	7104	PASS
173	174	0.00	2	0.8	504	PASS
174	95	50	120	56.3	60651	PASS
175	174	4	9	7.8	4737	PASS
176	174	93	101	98.1	59491	PASS
177	176	5	9	6.3	3750	PASS

Average of 10.370 to 10.377 min.: VL041817.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1389	45.80	35	56.05	2313	65.95	134
34.20	57	46.05	119	57.05	4767	66.20	68
35.20	26	47.00	1260	57.95	74	66.90	455
36.05	1548	47.95	797	58.20	45	68.05	1443
37.10	8786	49.10	6533	58.40	19	69.10	14670
38.10	7246	50.10	30533	60.00	1264	70.00	741
39.10	2908	51.05	8445	61.05	6875	70.20	377
40.10	209	51.90	141	62.10	7254	71.00	25
43.05	142	52.20	276	63.05	5437	72.05	770
44.05	1007	53.05	48	64.05	886	73.10	5843
45.05	1276	54.95	406	65.05	928	74.10	23592

Average of 10.370 to 10.377 min.: VL041817.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	67925	88.05	3020	104.70	31	113.10	176
76.10	5772	90.90	508	105.00	132	114.95	66
77.05	707	92.05	3189	105.85	384	115.90	274
77.85	503	93.10	5868	106.10	185	116.10	167
78.95	4171	94.10	13455	106.95	113	116.95	827
80.00	1450	95.10	107659	108.00	17	118.00	520
81.00	5092	96.10	7104	110.05	90	118.95	711
81.95	1021	97.00	211	110.80	66	122.60	18
83.00	147	97.20	88	111.00	69	123.70	54
86.05	234	101.90	30	112.00	27	124.80	32
87.00	3264	103.95	515	112.15	59	127.95	585

Average of 10.370 to 10.377 min.: VL041817.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.10	157	144.05	107	156.10	37	171.10	53
129.70	93	144.90	208	156.80	56	172.05	807
129.90	314	145.80	124	157.10	129	172.90	504
130.95	167	147.00	145	157.70	36	174.10	60651
134.95	206	148.05	294	158.10	26	175.05	4737
136.95	245	150.00	104	158.85	175	176.10	59491
139.10	31	152.05	62	160.10	17	177.05	3750
140.10	21	153.00	28	160.90	55	177.90	52
141.05	1292	154.00	37	161.10	53	178.20	20
142.10	48	155.00	282	162.10	17		
142.95	1481	155.90	67	170.65	170		