


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL122018\
 Data File : VL033023.D
 Acq On : 20 Dec 2018 12:20
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL120718AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Dec 07 09:35:17 2018
 Last Update : Fri Dec 07 09:35:17 2018

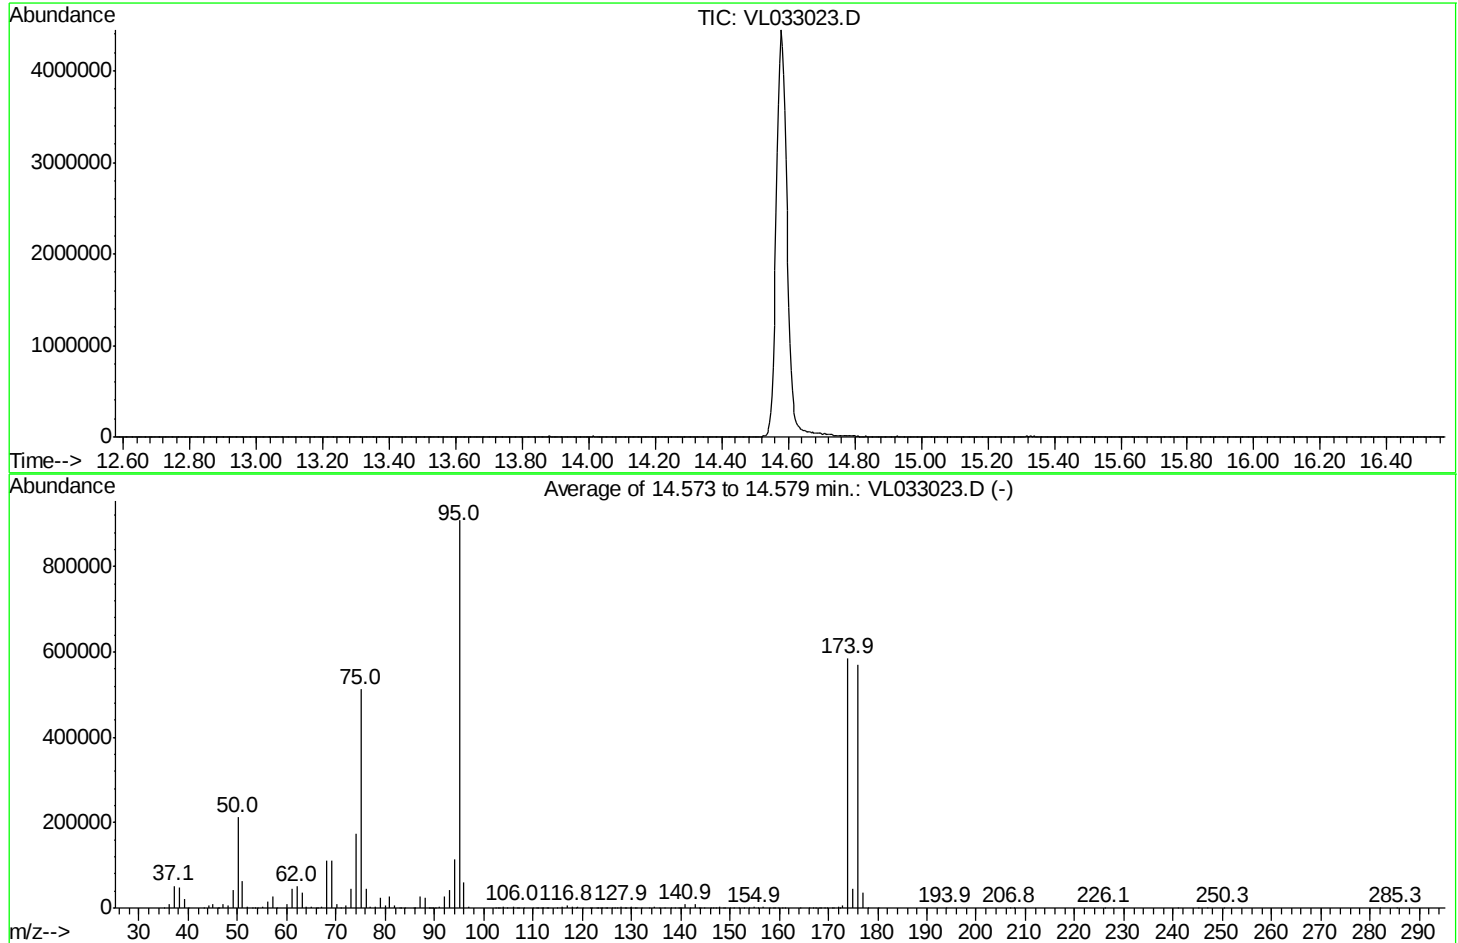

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	212330	PASS
75	95	30	66	56.4	512512	PASS
95	95	100	100	100.0	908138	PASS
96	95	5	9	6.5	58842	PASS
173	174	0.00	2	1.0	5876	PASS
174	95	50	120	64.3	584384	PASS
175	174	4	9	7.6	44392	PASS
176	174	93	101	97.6	570282	PASS
177	176	5	9	6.6	37570	PASS