


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL122123\
Data File : VL040922.D
Acq On : 21 Dec 2023 8:22
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL122023AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Dec 22 23:57:16 2023

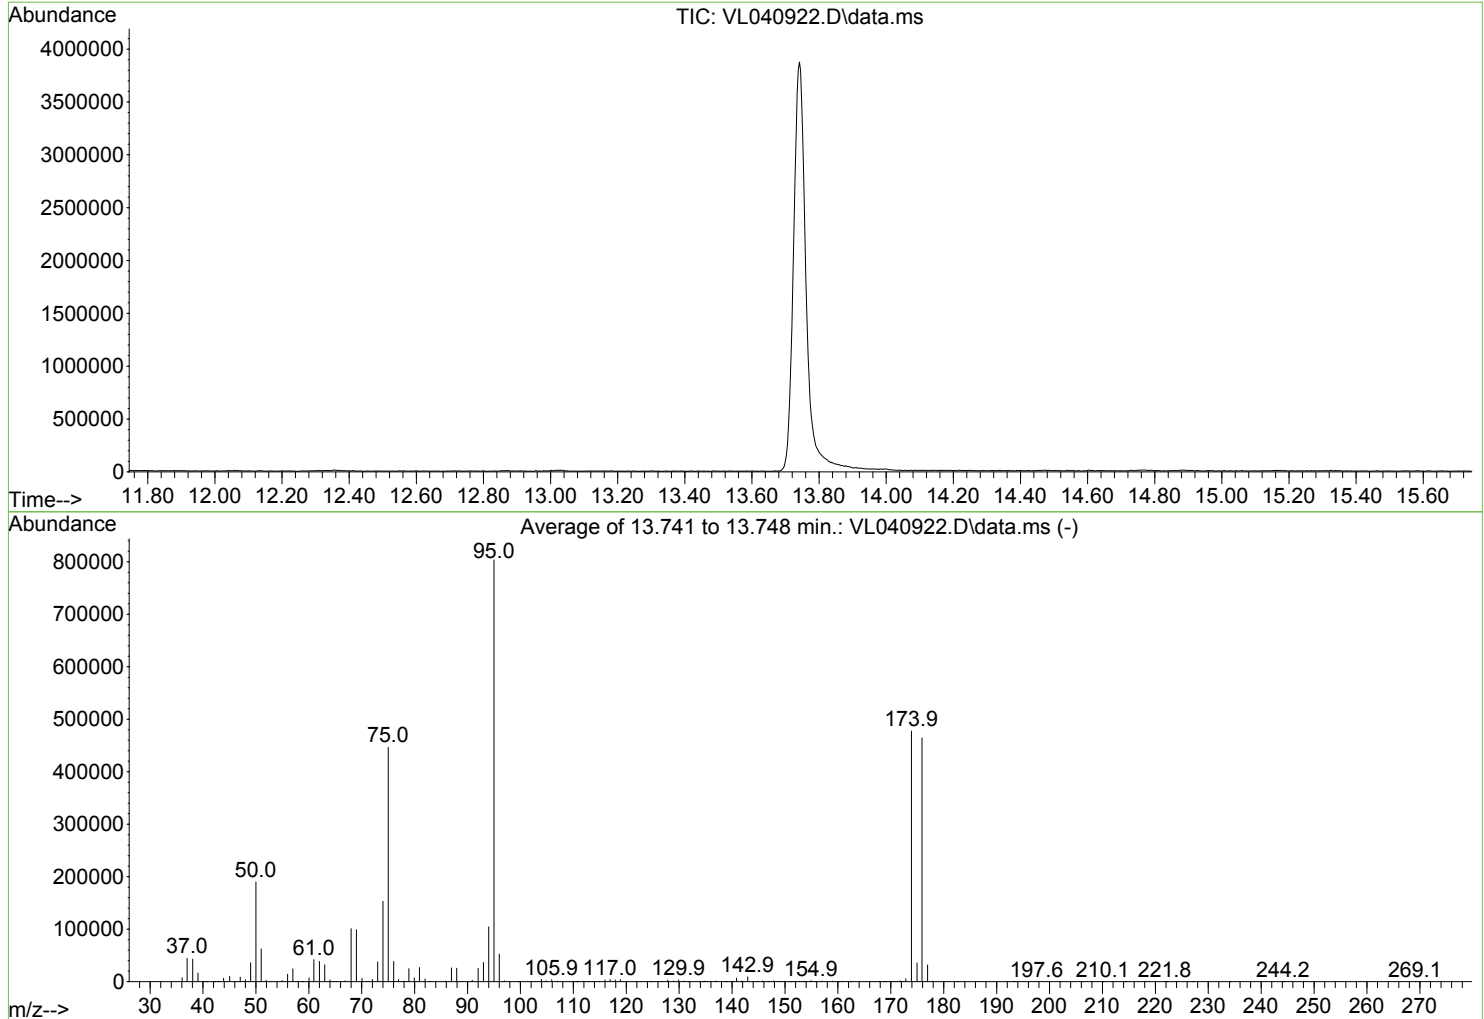

AutoFind: Scans 3464, 3465, 3466; Background Corrected with Scan 3435

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.6	189931	PASS
75	95	30	66	55.5	446357	PASS
95	95	100	100	100.0	803712	PASS
96	95	5	9	6.5	52552	PASS
173	174	0.00	2	1.2	5954	PASS
174	95	50	120	59.4	477355	PASS
175	174	4	9	7.5	35813	PASS
176	174	93	101	97.3	464320	PASS
177	176	5	9	6.8	31723	PASS

Average of 13.741 to 13.748 min.: VL040922.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7381	45.05	9936	57.00	24560	65.25	291
37.00	44579	46.00	517	57.80	412	66.05	241
38.05	42918	47.05	8667	58.00	643	66.85	166
39.05	16539	48.00	3832	58.70	88	68.00	10106
39.90	12	49.00	36016	59.00	206	69.00	98867
40.20	793	50.00	189931	60.05	7063	70.05	5985
40.70	57	51.00	62352	60.95	41912	70.95	303
42.20	53	51.95	2489	62.00	38555	72.00	4431
42.85	366	52.80	208	63.00	32181	73.00	37469
43.20	300	54.95	2239	64.00	3095	74.00	152939
43.90	6447	56.00	13924	64.70	273	75.00	446357

Average of 13.741 to 13.748 min.: VL040922.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	38493	85.85	853	102.75	425	113.00	433
76.95	3973	86.95	26395	103.95	4243	113.90	51
77.60	616	87.95	25680	104.85	1466	114.90	591
77.90	550	90.90	2891	105.90	3782	115.95	3039
78.10	1040	92.00	25221	106.90	898	116.95	4068
78.90	24816	93.00	36701	109.85	616	117.95	3016
79.95	7063	94.00	104149	110.10	124	118.90	3967
80.90	26776	95.00	803712	110.60	167	121.95	234
81.95	5192	96.00	52552	111.00	698	122.80	278
82.80	399	97.00	1614	111.75	651	123.95	438
83.05	656	99.50	53	112.75	470	124.60	132

Average of 13.741 to 13.748 min.: VL040922.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.10	222	135.05	958	144.00	326	152.75	750
125.60	255	135.85	234	144.90	741	153.10	261
126.85	424	136.95	1214	145.75	1234	153.50	107
127.85	2807	138.65	407	146.70	313	153.80	134
128.95	1304	138.90	65	146.90	92	154.05	502
129.90	2971	139.65	479	147.90	1474	154.95	1864
130.95	1358	140.20	539	149.00	486	155.80	206
131.65	125	140.85	6620	149.85	709	156.95	974
133.90	106	141.85	1147	151.00	73	158.95	931
134.50	86	142.95	9058	151.50	302	160.10	79
134.80	743	143.80	208	151.80	146	160.85	995

Average of 13.741 to 13.748 min.: VL040922.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
162.40	58	171.20	437	197.60	212		
166.10	255	171.75	1675	210.10	111		
166.80	253	172.30	547	214.30	136		
167.80	98	172.85	5954	221.80	259		
168.30	339	173.90	477355	222.20	59		
168.70	175	174.95	35813	227.10	56		
169.00	82	175.90	464320	234.20	53		
169.65	482	176.95	31723	244.20	90		
170.00	141	177.95	892	269.10	85		
170.55	557	182.60	75	269.80	58		
170.90	371	193.25	134				