
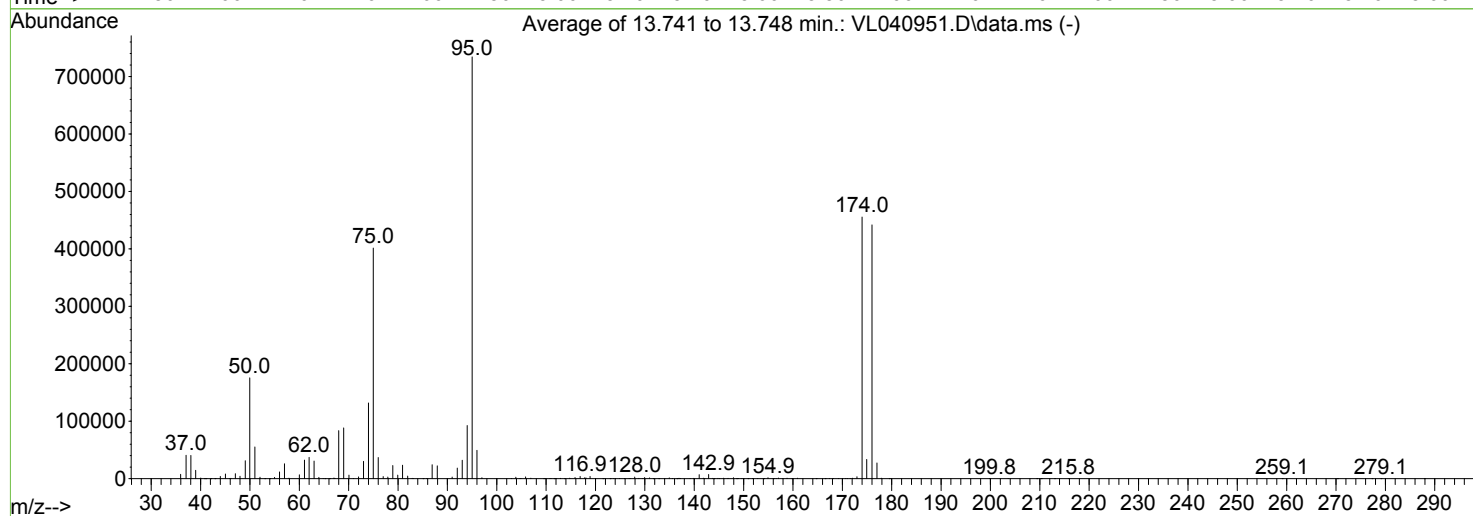


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL122223\
 Data File : VL040951.D
 Acq On : 22 Dec 2023 8:48
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL122023AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Fri Dec 22 23:57:16 2023

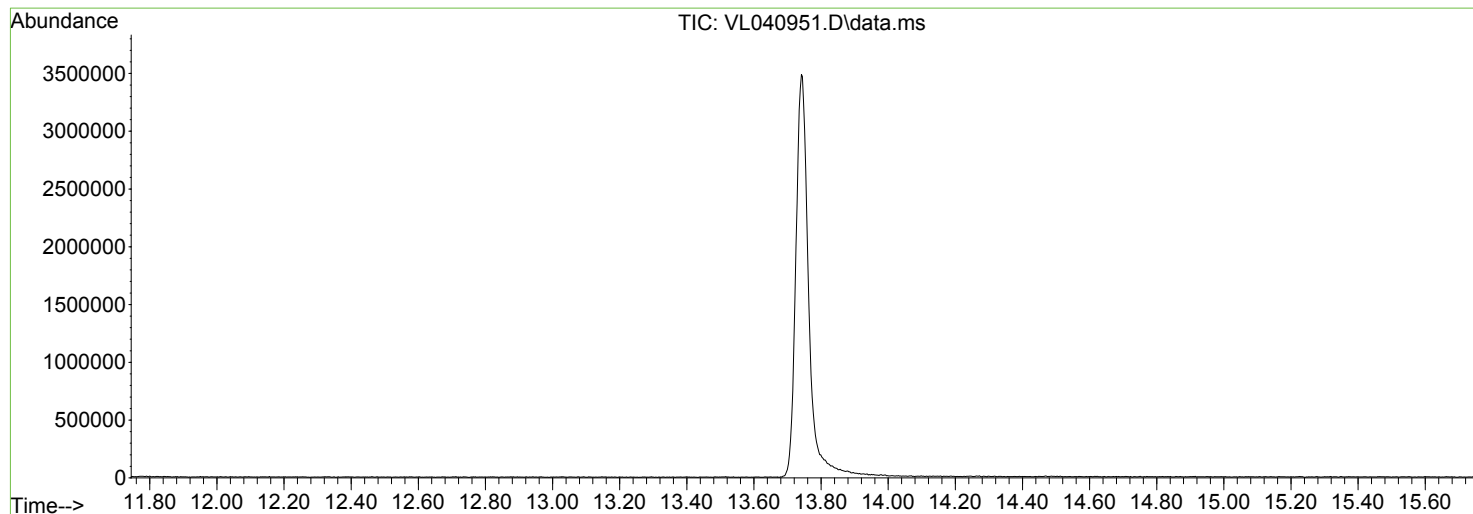

AutoFind: Scans 3464, 3465, 3466; Background Corrected with Scan 3441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	175449	PASS
75	95	30	66	54.7	401344	PASS
95	95	100	100	100.0	734272	PASS
96	95	5	9	6.7	49304	PASS
173	174	0.00	2	0.8	3485	PASS
174	95	50	120	62.0	455381	PASS
175	174	4	9	7.4	33496	PASS
176	174	93	101	97.0	441664	PASS
177	176	5	9	6.2	27205	PASS

Average of 13.741 to 13.748 min.: VL040951.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	7537	45.05	8048	55.00	2352	66.10	9126
37.05	40763	45.90	227	56.00	11785	67.00	126
38.05	40397	46.15	486	57.00	25999	67.20	71
39.00	14378	47.05	8772	57.90	943	68.00	8352
40.05	1057	48.00	4115	60.00	6564	69.00	88216
40.80	66	49.05	31125	61.05	32317	70.05	6134
41.10	124	49.95	175449	62.00	37171	70.95	397
42.10	67	51.00	55283	63.00	30632	72.00	3058
42.90	159	52.05	2555	63.95	2370	73.00	29960
43.10	168	53.00	107	64.85	243	74.00	131859
44.00	4034	54.00	57	65.20	120	75.00	401344

Average of 13.741 to 13.748 min.: VL040951.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.00	36912	86.00	286	103.85	2599	112.10	219
77.00	3720	86.90	24197	104.70	359	112.90	506
77.95	2714	87.95	22424	104.90	319	113.70	50
78.95	22907	90.95	2693	105.85	3190	114.80	772
79.95	6242	92.00	18291	106.90	818	115.85	1889
80.90	23448	93.00	32131	109.50	82	116.90	3947
81.95	4553	94.00	92499	109.90	424	117.75	1513
82.85	542	95.00	734272	110.75	335	118.05	1377
83.10	197	96.00	49304	111.00	308	118.90	3797
85.05	157	97.00	1692	111.60	155	121.50	70
85.80	235	103.00	358	111.90	328	121.90	349

Average of 13.741 to 13.748 min.: VL040951.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.95	140	130.95	1329	139.90	550	147.95	1753
123.70	198	131.70	145	141.00	6863	148.60	78
124.05	263	132.80	74	141.85	836	148.95	286
124.85	402	134.05	212	142.10	392	149.65	337
125.90	338	134.95	1391	142.90	7335	150.05	239
126.80	356	135.60	244	143.75	474	150.90	57
127.00	215	136.50	83	144.00	98	151.80	347
127.95	2736	136.75	725	144.80	455	152.00	192
128.80	678	137.00	500	145.10	386	152.85	261
129.60	352	137.20	198	145.95	854	154.05	153
129.95	1830	139.15	292	146.85	448	154.95	1810

Average of 13.741 to 13.748 min.: VL040951.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.00	124	169.25	431	177.90	819	279.10	149
156.60	166	170.05	308	179.50	81	287.90	64
157.05	1082	170.70	441	199.80	172		
157.95	298	171.00	167	203.60	165		
158.80	795	171.60	217	209.40	66		
159.80	76	172.05	864	210.30	148		
160.90	967	172.95	3485	213.00	68		
164.70	91	174.00	455381	215.85	109		
166.50	56	174.95	33496	259.10	100		
167.40	165	176.00	441664	270.30	62		
168.15	260	177.00	27205	277.30	73		