

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
 Data File : VX044579.D
 Acq On : 31 Dec 2024 14:48
 Operator : JC/MD
 Sample : VX0101WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK750

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	5645	6004	0.64%	0.089%
2	1.368	42	46	58	rBV	102355	118713	12.71%	1.762%
3	1.642	88	91	101	rVB	86897	124287	13.31%	1.844%
4	2.294	192	198	210	rBV	219551	344173	36.86%	5.107%
5	2.502	228	232	235	rVV3	1242	2059	0.22%	0.031%
6	2.642	252	255	258	rVB2	859	1094	0.12%	0.016%
7	2.782	273	278	284	rBV6	2278	3966	0.42%	0.059%
8	2.941	295	304	315	rBV2	6120	16399	1.76%	0.243%
9	3.087	323	328	329	rBV3	1738	2733	0.29%	0.041%
10	3.373	372	375	376	rVB2	484	436	0.05%	0.006%
11	3.428	379	384	390	rBV5	1957	5111	0.55%	0.076%
12	3.654	418	421	423	rBV3	493	546	0.06%	0.008%
13	3.764	437	439	442	rBV3	517	656	0.07%	0.010%
14	3.818	447	448	452	rVB2	805	735	0.08%	0.011%
15	3.861	452	455	456	rBV2	715	743	0.08%	0.011%
16	3.922	462	465	469	rBV4	383	516	0.06%	0.008%
17	4.001	475	478	480	rBV2	533	692	0.07%	0.010%
18	4.282	522	524	526	rBV2	513	417	0.04%	0.006%
19	4.373	538	539	544	rVB3	490	435	0.05%	0.006%
20	4.459	544	553	570	rBV	67388	208420	22.32%	3.093%
21	4.885	619	623	624	rBV2	702	760	0.08%	0.011%
22	4.934	629	631	633	rVB2	604	586	0.06%	0.009%
23	5.050	638	650	667	rBV	129701	405443	43.42%	6.016%
24	5.275	685	687	692	rVB2	601	745	0.08%	0.011%
25	5.349	695	699	700	rBV2	542	518	0.06%	0.008%
26	5.440	711	714	715	rBV2	972	941	0.10%	0.014%
27	5.550	727	732	733	rBV3	580	964	0.10%	0.014%
28	5.660	747	750	751	rBV3	875	769	0.08%	0.011%
29	5.873	784	785	788	rBV	414	469	0.05%	0.007%
30	5.958	788	799	817	rBV2	313801	933682	100.00%	13.855%
31	6.196	835	838	839	rBV3	683	641	0.07%	0.010%
32	6.495	884	887	888	rVB3	621	599	0.06%	0.009%
33	6.757	920	930	942	rBV	185652	462437	49.53%	6.862%
34	7.123	983	990	1000	rVB	3966	11145	1.19%	0.165%
35	7.214	1003	1005	1006	rBV2	498	522	0.06%	0.008%
36	7.306	1011	1020	1038	rBV	190752	439863	47.11%	6.527%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
 Data File : VX044579.D
 Acq On : 31 Dec 2024 14:48
 Operator : JC/MD
 Sample : VX0101WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK750

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.830	1102	1106	1111	rVV5	1009	1509	0.16%	0.022%
38	8.013	1131	1136	1137	rBV3	462	532	0.06%	0.008%
39	8.110	1150	1152	1155	rVB2	515	430	0.05%	0.006%
40	8.147	1155	1158	1159	rBV2	664	462	0.05%	0.007%
41	8.263	1174	1177	1180	rVV3	658	886	0.09%	0.013%
42	8.324	1181	1187	1208	rVV	117370	206397	22.11%	3.063%
43	8.464	1208	1210	1213	rVB2	676	584	0.06%	0.009%
44	8.586	1226	1230	1233	rBV3	1406	1934	0.21%	0.029%
45	8.647	1233	1240	1250	rBV	425503	685243	73.39%	10.168%
46	8.946	1284	1289	1304	rBV	80078	132804	14.22%	1.971%
47	9.159	1318	1324	1331	rBV7	2128	3510	0.38%	0.052%
48	9.275	1339	1343	1347	rBV4	2316	3384	0.36%	0.050%
49	9.330	1350	1352	1354	rBV3	669	643	0.07%	0.010%
50	9.384	1356	1361	1380	rBV	273931	427224	45.76%	6.339%
51	9.671	1407	1408	1410	rBV2	598	580	0.06%	0.009%
52	9.695	1410	1412	1417	rVB4	1038	1420	0.15%	0.021%
53	9.805	1429	1430	1435	rBV3	591	595	0.06%	0.009%
54	9.982	1457	1459	1461	rBV2	568	493	0.05%	0.007%
55	10.049	1465	1470	1487	rVV	380718	543990	58.26%	8.072%
56	10.195	1490	1494	1498	rBV3	3608	4561	0.49%	0.068%
57	10.281	1506	1508	1509	rBV2	579	406	0.04%	0.006%
58	10.305	1509	1512	1518	rVB3	3722	5202	0.56%	0.077%
59	10.604	1558	1561	1564	rBV4	506	609	0.07%	0.009%
60	10.640	1564	1567	1578	rVV6	3932	9442	1.01%	0.140%
61	10.805	1591	1594	1597	rBV4	803	932	0.10%	0.014%
62	10.878	1604	1606	1609	rVB4	615	638	0.07%	0.009%
63	10.963	1616	1620	1629	rVB4	3423	5830	0.62%	0.087%
64	11.098	1636	1642	1648	rBV4	896	2306	0.25%	0.034%
65	11.189	1652	1657	1669	rVB	371366	473720	50.74%	7.029%
66	11.305	1674	1676	1680	rVB4	786	1177	0.13%	0.017%
67	11.396	1690	1691	1694	rVB2	675	615	0.07%	0.009%
68	11.421	1694	1695	1697	rBV2	433	408	0.04%	0.006%
69	11.451	1697	1700	1705	rVV3	3286	4808	0.51%	0.071%
70	11.549	1714	1716	1718	rBV2	461	454	0.05%	0.007%
71	11.713	1742	1743	1746	rVB2	618	443	0.05%	0.007%
72	11.756	1746	1750	1756	rVB	3932	5134	0.55%	0.076%
73	11.969	1782	1785	1788	rBV3	4036	4872	0.52%	0.072%
74	12.018	1788	1793	1807	rVB	360542	466966	50.01%	6.929%
75	12.317	1837	1842	1860	rVV	466350	597929	64.04%	8.873%
76	12.762	1912	1915	1918	rBV3	2488	2850	0.31%	0.042%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
 Data File : VX044579.D
 Acq On : 31 Dec 2024 14:48
 Operator : JC/MD
 Sample : VX0101WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK750

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.859	1929	1931	1933	rVB2	572	455	0.05%	0.007%
78	13.122	1969	1974	1979	rVV6	2336	3315	0.36%	0.049%
79	13.262	1995	1997	1999	rBV	476	392	0.04%	0.006%
80	13.390	2015	2018	2022	rBV3	497	760	0.08%	0.011%
81	13.518	2037	2039	2041	rBV3	484	531	0.06%	0.008%
82	13.597	2048	2052	2055	rBV5	3558	4305	0.46%	0.064%
83	13.780	2078	2082	2086	rBV2	5800	7300	0.78%	0.108%
84	13.963	2108	2112	2119	rBV3	3782	6186	0.66%	0.092%
85	14.042	2122	2125	2127	rBV2	514	553	0.06%	0.008%
86	14.103	2132	2135	2136	rBV2	813	610	0.07%	0.009%
87	14.128	2136	2139	2143	rBV2	3680	4122	0.44%	0.061%
88	14.207	2149	2152	2154	rBV3	384	547	0.06%	0.008%
89	14.323	2170	2171	2174	rBV2	579	464	0.05%	0.007%
90	14.585	2213	2214	2218	rBV3	610	689	0.07%	0.010%
91	14.823	2251	2253	2256	rVB3	429	448	0.05%	0.007%
92	14.932	2267	2271	2272	rBV2	625	792	0.08%	0.012%
93	14.981	2278	2279	2282	rVB3	528	393	0.04%	0.006%
94	15.103	2297	2299	2300	rBV2	671	431	0.05%	0.006%
95	15.121	2300	2302	2304	rBV3	430	460	0.05%	0.007%
96	15.390	2342	2346	2353	rVB4	1690	3352	0.36%	0.050%
97	15.560	2373	2374	2377	rVB2	695	443	0.05%	0.007%
98	15.774	2407	2409	2411	rBV2	619	692	0.07%	0.010%
99	15.999	2444	2446	2450	rBV3	727	865	0.09%	0.013%
100	16.676	2553	2557	2558	rBV2	591	857	0.09%	0.013%

Sum of corrected areas: 6739103




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
Data File : VX044579.D
Acq On : 31 Dec 2024 14:48
Operator : JC/MD
Sample : VX0101WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK750

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

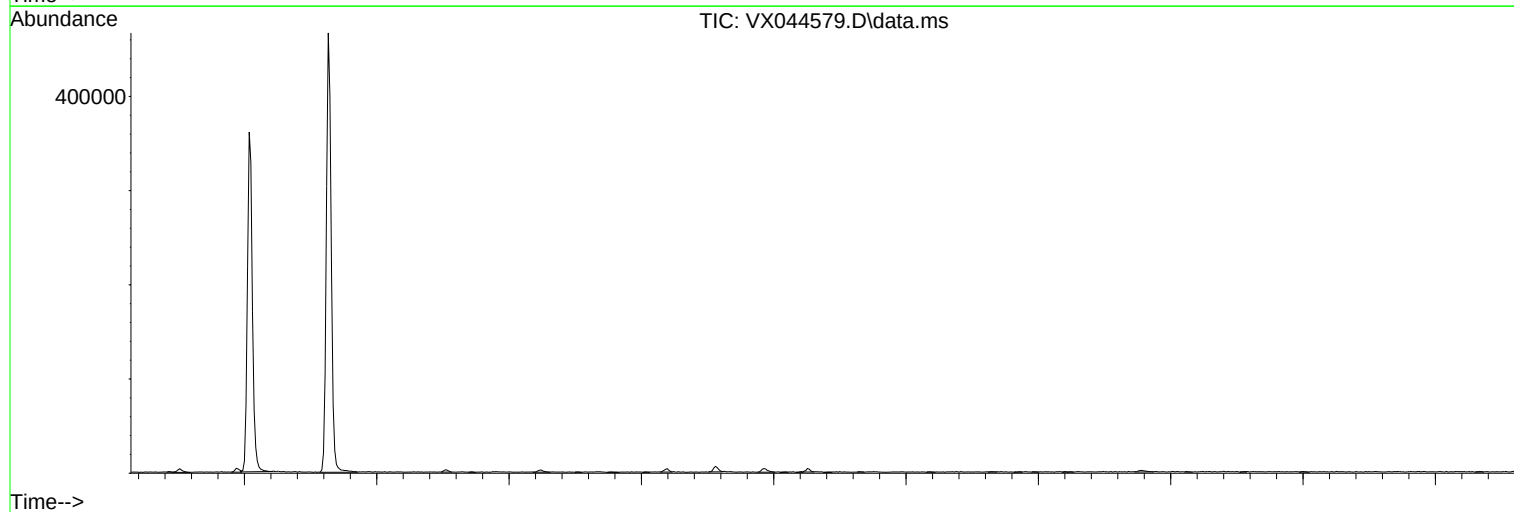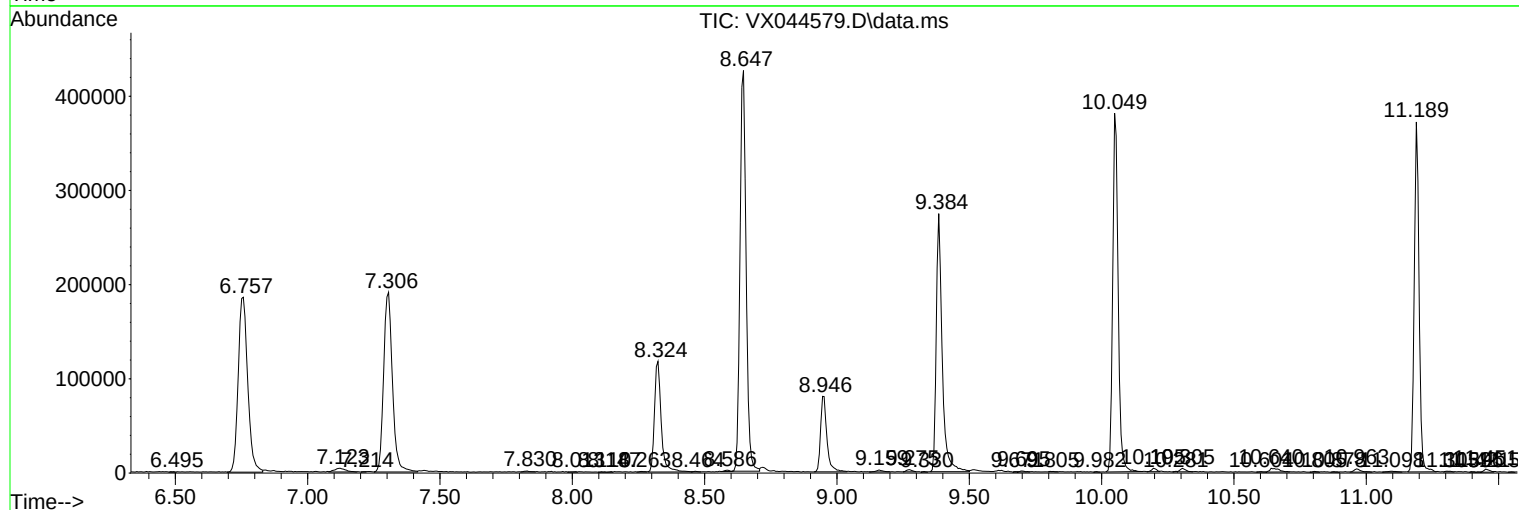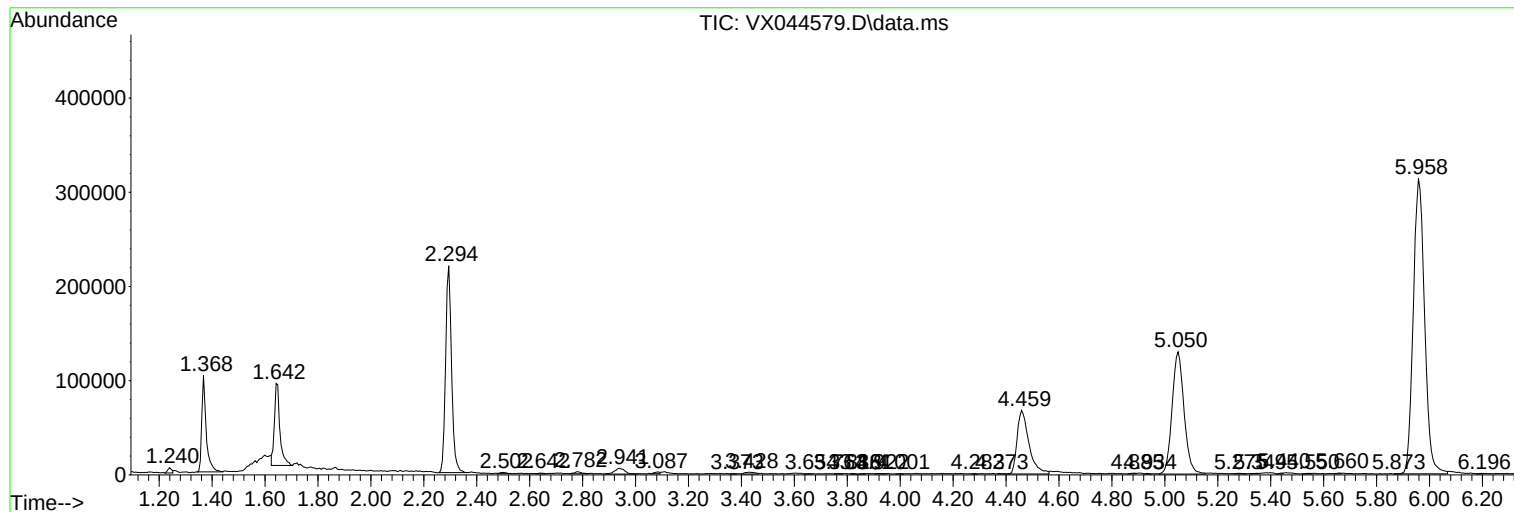

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
Data File : VX044579.D
Acq On : 31 Dec 2024 14:48
Operator : JC/MD
Sample : VX0101WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK750

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
Data File : VX044579.D
Acq On : 31 Dec 2024 14:48
Operator : JC/MD
Sample : VX0101WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK750

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc