

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
 Data File : VX044580.D
 Acq On : 31 Dec 2024 15:16
 Operator : JC/MD
 Sample : P5344-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	4424	4964	0.57%	0.079%
2	1.368	42	46	57	rVB	93134	109930	12.65%	1.740%
3	1.648	88	92	100	rVB	80028	111651	12.85%	1.767%
4	2.294	192	198	209	rVB	183527	291301	33.52%	4.610%
5	2.374	209	211	212	rBV2	946	629	0.07%	0.010%
6	2.502	229	232	235	rBV	1145	1123	0.13%	0.018%
7	2.697	262	264	266	rBV2	561	525	0.06%	0.008%
8	2.782	275	278	283	rVB4	1696	2633	0.30%	0.042%
9	2.941	298	304	314	rVB2	6984	16668	1.92%	0.264%
10	3.099	324	330	331	rBV3	1470	2616	0.30%	0.041%
11	3.337	368	369	374	rVB3	560	730	0.08%	0.012%
12	3.386	374	377	380	rBV3	363	589	0.07%	0.009%
13	3.422	380	383	385	rBV2	1108	1509	0.17%	0.024%
14	3.508	395	397	401	rBV2	616	854	0.10%	0.014%
15	3.703	427	429	432	rVB2	488	492	0.06%	0.008%
16	3.758	434	438	439	rBV3	607	523	0.06%	0.008%
17	3.892	457	460	464	rVB3	631	978	0.11%	0.015%
18	4.050	484	486	488	rVV2	460	501	0.06%	0.008%
19	4.099	491	494	497	rBV2	459	807	0.09%	0.013%
20	4.221	512	514	518	rBV3	572	852	0.10%	0.013%
21	4.318	528	530	532	rBV	438	489	0.06%	0.008%
22	4.459	546	553	571	rBV	60734	188287	21.67%	2.980%
23	5.050	637	650	668	rBV	119861	376509	43.33%	5.958%
24	5.958	789	799	819	rBV2	286940	868958	100.00%	13.752%
25	6.220	840	842	846	rBV2	624	678	0.08%	0.011%
26	6.544	893	895	898	rVB3	432	550	0.06%	0.009%
27	6.757	920	930	946	rVV	195253	479494	55.18%	7.588%
28	6.928	956	958	960	rBV2	563	534	0.06%	0.008%
29	7.104	982	987	988	rBV4	2564	2509	0.29%	0.040%
30	7.239	1007	1009	1011	rBV2	439	425	0.05%	0.007%
31	7.306	1011	1020	1037	rBV	172811	404652	46.57%	6.404%
32	7.635	1072	1074	1076	rVV	587	498	0.06%	0.008%
33	7.818	1102	1104	1105	rBV2	483	475	0.05%	0.008%
34	7.964	1126	1128	1132	rVB4	630	836	0.10%	0.013%
35	7.995	1132	1133	1136	rBV	774	531	0.06%	0.008%
36	8.245	1172	1174	1176	rVB3	698	601	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
 Data File : VX044580.D
 Acq On : 31 Dec 2024 15:16
 Operator : JC/MD
 Sample : P5344-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	8.324	1180	1187	1201	rBV	110501	191282	22.01%	3.027%
38	8.421	1201	1203	1207	rVB3	810	837	0.10%	0.013%
39	8.586	1226	1230	1231	rBV4	1832	2087	0.24%	0.033%
40	8.647	1234	1240	1248	rBV	393340	625934	72.03%	9.906%
41	8.952	1284	1290	1301	rBV	74598	121351	13.97%	1.920%
42	9.153	1320	1323	1327	rBV4	1837	2629	0.30%	0.042%
43	9.275	1340	1343	1347	rVB4	3195	4068	0.47%	0.064%
44	9.385	1356	1361	1379	rBV	243385	395337	45.50%	6.256%
45	9.702	1410	1413	1415	rVV2	914	1111	0.13%	0.018%
46	9.756	1420	1422	1424	rBV3	401	435	0.05%	0.007%
47	9.964	1453	1456	1461	rBV4	523	925	0.11%	0.015%
48	10.049	1465	1470	1481	rBV	390986	564719	64.99%	8.937%
49	10.195	1492	1494	1498	rVB2	2361	2717	0.31%	0.043%
50	10.305	1509	1512	1518	rVB4	2835	4046	0.47%	0.064%
51	10.640	1564	1567	1578	rVB5	2611	6569	0.76%	0.104%
52	10.799	1591	1593	1600	rVB5	762	1375	0.16%	0.022%
53	10.970	1615	1621	1624	rBV5	2723	4316	0.50%	0.068%
54	11.085	1638	1640	1641	rBV	477	446	0.05%	0.007%
55	11.104	1641	1643	1647	rVV3	749	717	0.08%	0.011%
56	11.189	1652	1657	1668	rVV	348686	443538	51.04%	7.019%
57	11.311	1673	1677	1678	rVV3	811	1282	0.15%	0.020%
58	11.451	1697	1700	1703	rBV3	2449	3350	0.39%	0.053%
59	11.543	1710	1715	1717	rBV3	641	820	0.09%	0.013%
60	11.604	1722	1725	1728	rBV4	559	842	0.10%	0.013%
61	11.756	1747	1750	1755	rVB2	2931	3541	0.41%	0.056%
62	11.909	1773	1775	1778	rVB2	607	705	0.08%	0.011%
63	11.976	1782	1786	1788	rBV2	3043	3899	0.45%	0.062%
64	12.018	1788	1793	1801	rBV	368168	469949	54.08%	7.437%
65	12.226	1824	1827	1828	rBV3	677	653	0.08%	0.010%
66	12.317	1837	1842	1858	rBV	427070	544868	62.70%	8.623%
67	12.573	1882	1884	1887	rVB3	603	623	0.07%	0.010%
68	12.664	1897	1899	1903	rVV3	517	705	0.08%	0.011%
69	12.762	1911	1915	1917	rBV3	2363	3093	0.36%	0.049%
70	12.914	1938	1940	1943	rBV	465	575	0.07%	0.009%
71	12.951	1944	1946	1948	rVB	1166	800	0.09%	0.013%
72	12.981	1948	1951	1953	rBV2	563	635	0.07%	0.010%
73	13.079	1964	1967	1968	rBV2	570	501	0.06%	0.008%
74	13.116	1971	1973	1977	rVB4	1505	1745	0.20%	0.028%
75	13.268	1996	1998	1999	rBV2	506	450	0.05%	0.007%
76	13.286	1999	2001	2002	rVV	646	531	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
 Data File : VX044580.D
 Acq On : 31 Dec 2024 15:16
 Operator : JC/MD
 Sample : P5344-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.317	2004	2006	2008	rVV2	590	521	0.06%	0.008%
78	13.341	2008	2010	2012	rVB2	613	501	0.06%	0.008%
79	13.366	2012	2014	2016	rBV2	382	514	0.06%	0.008%
80	13.390	2016	2018	2020	rVV2	662	472	0.05%	0.007%
81	13.555	2044	2045	2048	rVB2	725	507	0.06%	0.008%
82	13.597	2048	2052	2057	rBV4	1672	2718	0.31%	0.043%
83	13.634	2057	2058	2062	rVV2	653	599	0.07%	0.009%
84	13.725	2072	2073	2076	rVB2	680	484	0.06%	0.008%
85	13.780	2078	2082	2084	rBV3	2308	3043	0.35%	0.048%
86	13.969	2108	2113	2120	rVB4	2015	3533	0.41%	0.056%
87	14.024	2120	2122	2125	rBV2	576	596	0.07%	0.009%
88	14.128	2134	2139	2145	rBV	3804	5839	0.67%	0.092%
89	14.231	2152	2156	2157	rBV3	508	641	0.07%	0.010%
90	14.250	2157	2159	2161	rBV3	402	457	0.05%	0.007%
91	14.560	2208	2210	2214	rBV4	534	655	0.08%	0.010%
92	14.835	2253	2255	2257	rBV2	505	438	0.05%	0.007%
93	15.091	2294	2297	2299	rBV3	539	483	0.06%	0.008%
94	15.390	2341	2346	2351	rVB4	1925	3004	0.35%	0.048%
95	15.792	2409	2412	2415	rBV2	838	905	0.10%	0.014%
96	16.127	2465	2467	2471	rVB3	683	493	0.06%	0.008%
97	16.176	2473	2475	2478	rBV2	493	527	0.06%	0.008%
98	16.322	2496	2499	2500	rBV3	936	888	0.10%	0.014%
99	16.438	2516	2518	2522	rVB3	616	618	0.07%	0.010%
100	16.493	2526	2527	2529	rBV2	765	519	0.06%	0.008%

Sum of corrected areas: 6318862




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
Data File : VX044580.D
Acq On : 31 Dec 2024 15:16
Operator : JC/MD
Sample : P5344-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

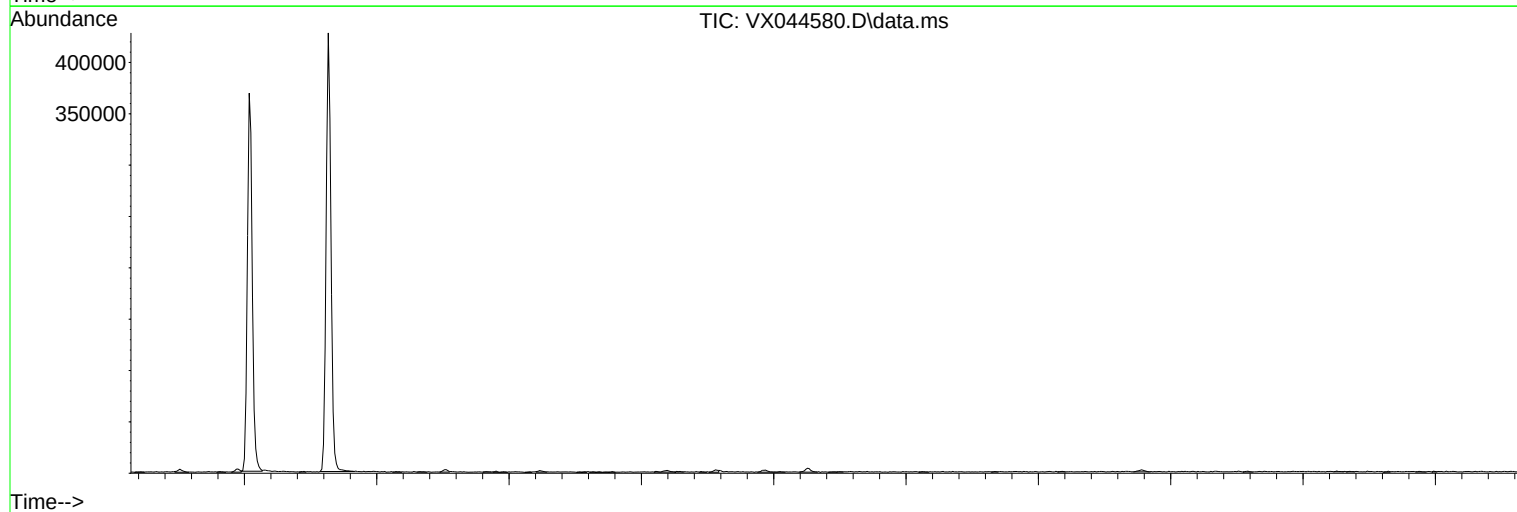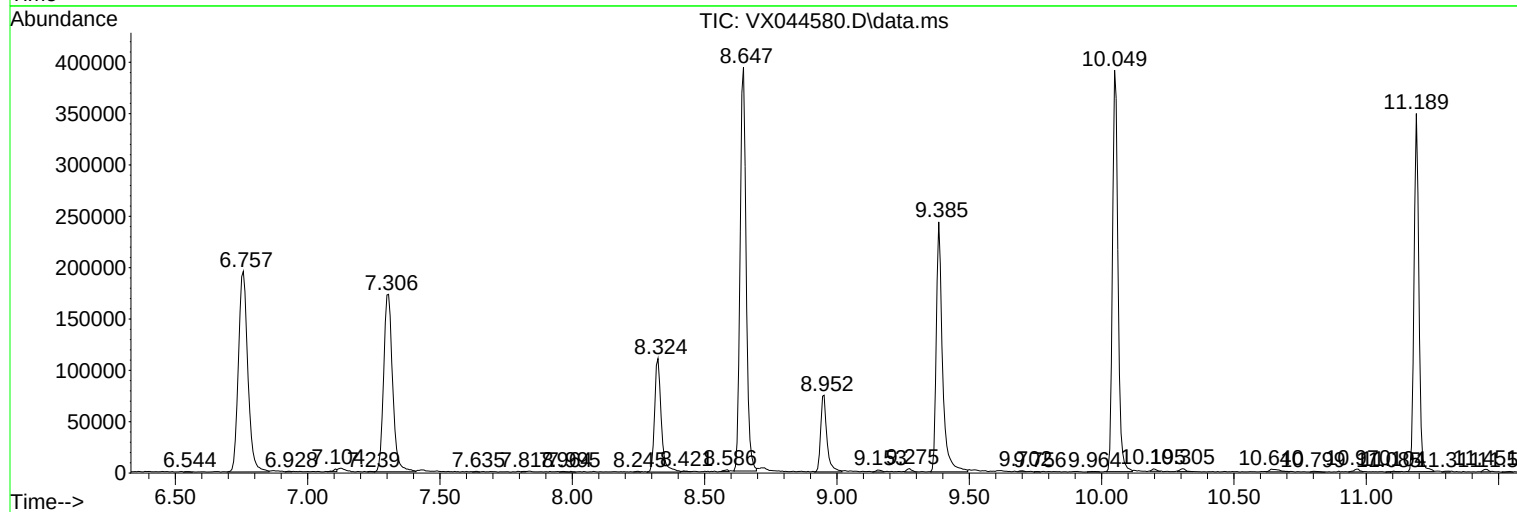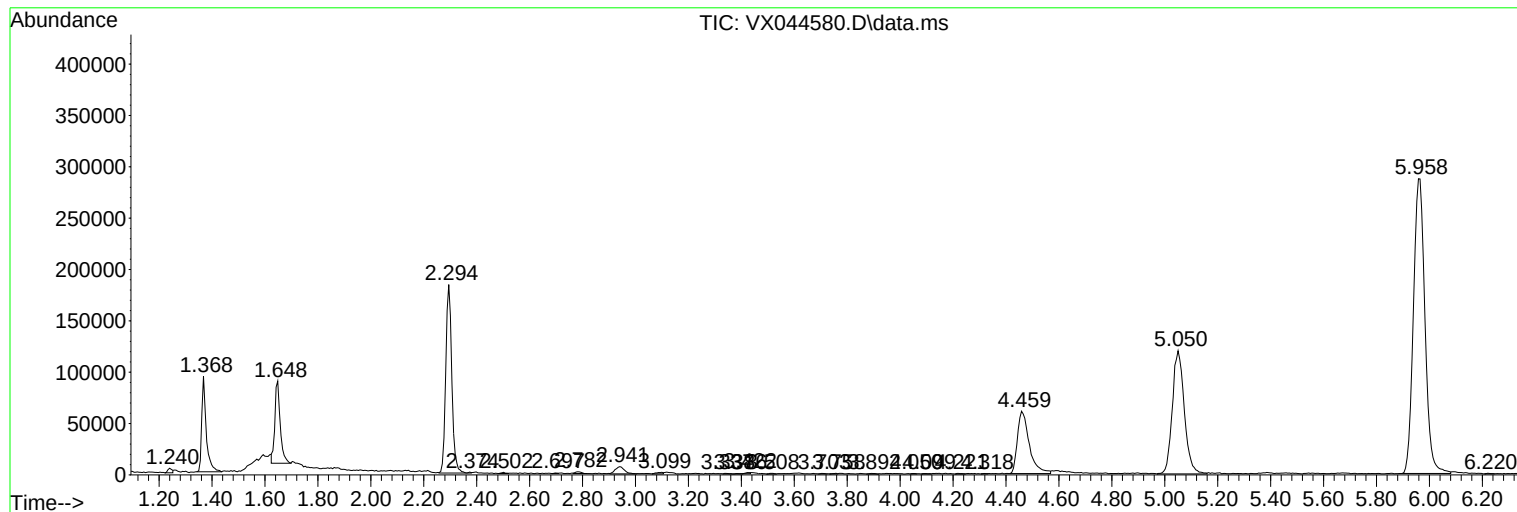

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
Data File : VX044580.D
Acq On : 31 Dec 2024 15:16
Operator : JC/MD
Sample : P5344-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
Data File : VX044580.D
Acq On : 31 Dec 2024 15:16
Operator : JC/MD
Sample : P5344-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
