
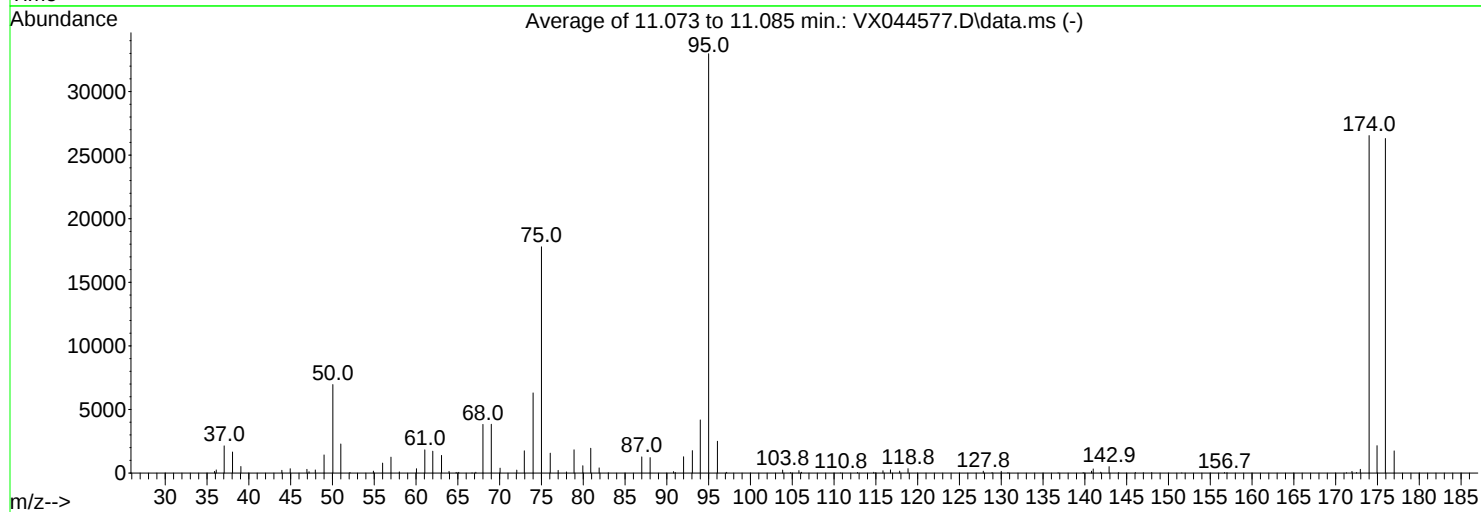


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010125\
Data File : VX044577.D
Acq On : 31 Dec 2024 13:51
Operator : JC/MD
Sample : BFB711
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB711

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Title : VOC Analysis
Last Update : Tue Dec 31 01:02:15 2024

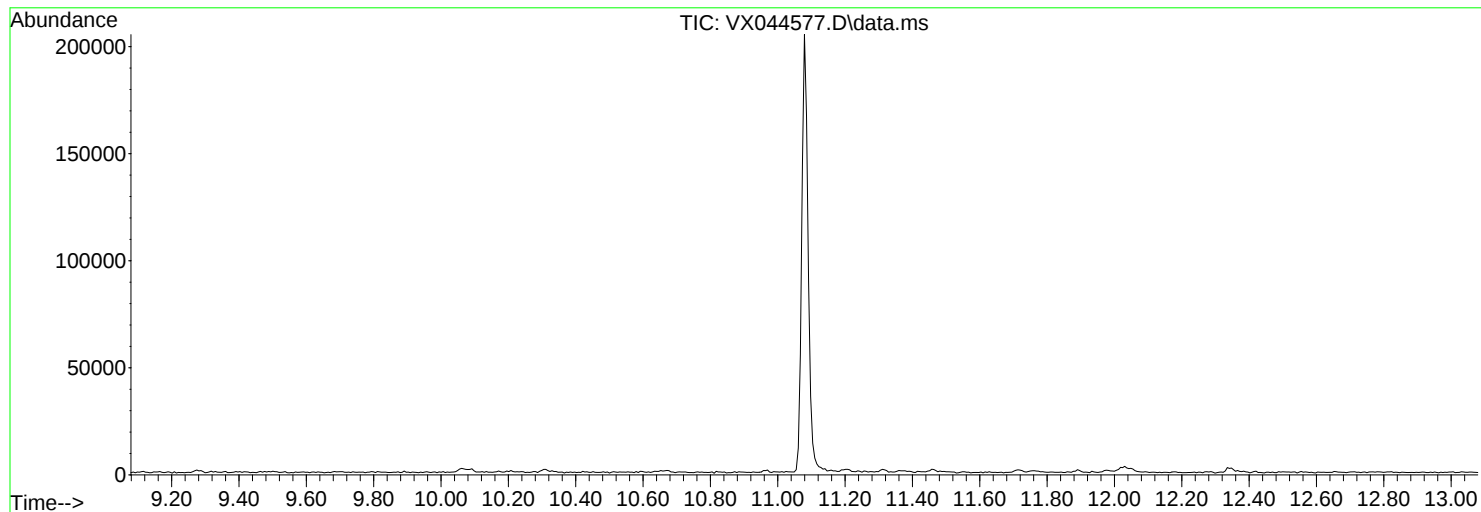

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	6960	PASS
75	95	30	80	54.0	17793	PASS
95	95	100	100	100.0	32973	PASS
96	95	5	9	7.6	2504	PASS
173	174	0.00	2	1.1	297	PASS
174	95	50	120	80.5	26536	PASS
175	174	5	9	8.1	2154	PASS
176	174	95	101	99.1	26307	PASS
177	176	5	9	6.6	1743	PASS

m/z	Abundance
38.10	117.0
39.10	590.0
40.00	433.0
43.90	239.0

Instrument :
MSVOA_X
ClientSampleId :
BFB711

m/z	Abundance
35.90	395.0
37.10	2142.0
38.10	1566.0
39.10	1059.0
40.10	349.0
44.00	447.0
44.90	387.0
46.90	325.0
47.90	297.0
49.00	1410.0
50.00	6200.0
51.00	2231.0
52.10	74.0
54.90	175.0
56.00	512.0
57.00	1322.0
58.00	58.0
60.00	413.0
61.10	1586.0
62.00	1368.0
63.00	1115.0
64.00	96.0
64.80	160.0
66.70	55.0
68.00	3220.0
69.00	3340.0
70.00	464.0
72.10	199.0
73.00	1665.0
74.00	5945.0
75.00	15685.0
76.10	1203.0
77.00	231.0
78.00	135.0
78.90	1596.0
80.00	432.0
80.90	1519.0
81.90	399.0
87.00	1182.0
88.00	996.0
90.80	96.0
92.00	878.0
93.00	1645.0
94.00	3579.0
95.00	28856.0
96.10	2137.0
103.90	253.0
104.80	126.0
105.80	185.0
114.80	69.0
115.90	179.0
116.80	289.0
117.80	165.0
118.80	364.0
127.90	126.0
128.90	61.0
130.10	141.0
140.80	459.0
141.90	58.0
142.80	440.0
146.10	66.0
148.00	52.0
156.70	67.0
171.30	89.0
171.90	63.0
172.50	139.0
173.00	181.0
174.00	20104.0
175.00	1642.0
175.90	19192.0
177.00	1184.0

Instrument :
MSVOA_X
ClientSampleId :
BFB711

m/z	Abundance
36.10	386.0
37.00	2578.0
38.00	2039.0
39.00	1306.0
40.00	397.0
43.90	593.0
45.00	434.0
47.00	558.0
48.00	282.0
49.00	1693.0
50.00	8299.0
51.00	2580.0
52.10	63.0
54.90	202.0
56.00	1000.0
57.00	1439.0
58.00	104.0
60.10	258.0
61.10	2106.0
62.00	2243.0
63.00	1676.0
64.00	189.0
65.10	119.0
67.10	88.0
68.00	4865.0
69.00	4428.0
70.10	337.0
71.90	260.0
73.00	2034.0
74.00	7460.0
75.00	21984.0
76.00	2282.0
77.00	126.0
78.00	138.0
78.90	2177.0
80.00	744.0
80.90	2425.0
81.90	541.0
83.00	58.0
87.00	1447.0
88.00	1302.0
90.80	252.0
92.10	1861.0
93.10	1893.0
94.00	5047.0
95.00	39144.0
96.10	2783.0
97.20	88.0
103.80	252.0
105.90	232.0
112.80	73.0
114.70	130.0
115.80	183.0
116.70	219.0
117.90	158.0
118.90	327.0
127.80	225.0
128.90	63.0
130.00	136.0
130.80	121.0
136.80	79.0
139.80	65.0
141.00	491.0
141.90	87.0
142.90	554.0
144.00	64.0
146.00	57.0
147.00	65.0
156.70	60.0
172.00	170.0
173.00	382.0
174.00	31584.0
175.00	2792.0
176.00	30456.0
177.00	2276.0

Instrument :
MSVOA_X
ClientSampleId :
BFB711

m/z	Abundance
36.10	366.0
37.00	1709.0
38.10	1721.0
39.10	952.0
40.00	496.0
44.10	332.0
45.00	210.0
47.20	315.0
47.90	156.0
49.00	1180.0
50.10	6381.0
51.00	2046.0
55.00	87.0
56.00	844.0
57.00	1003.0
58.00	126.0
60.00	365.0
61.00	1795.0
62.00	1551.0
63.10	1378.0
63.90	110.0
65.10	63.0
67.20	103.0
68.00	3396.0
69.00	3748.0
70.00	363.0
72.10	248.0
72.90	1553.0
74.00	5500.0
75.00	15711.0
76.00	1214.0
77.00	277.0
78.90	1726.0
79.80	556.0
80.90	1916.0
81.80	283.0
87.00	1187.0
88.00	1350.0
91.00	137.0
91.90	1109.0
93.00	1762.0
94.00	3908.0
95.00	30920.0
96.00	2592.0
97.10	94.0
103.80	210.0
105.70	189.0
106.10	201.0
110.80	57.0
112.80	81.0
115.00	59.0
115.80	193.0
116.70	256.0
117.80	141.0
118.80	346.0
127.80	98.0
129.90	146.0
139.80	57.0
141.00	483.0
141.90	75.0
143.00	525.0
144.10	60.0
148.00	58.0
151.60	54.0
157.00	77.0
172.00	163.0
172.90	328.0
174.00	27920.0
174.90	2027.0
175.90	29272.0
177.00	1769.0

Instrument :
MSVOA_X
ClientSampleId :
BFB711