


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX010219\
Data File : VX006870.D
Acq On : 02 Jan 2019 09:43
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
Title : SW846 8260
Last Update : Wed Dec 19 15:20:58 2018

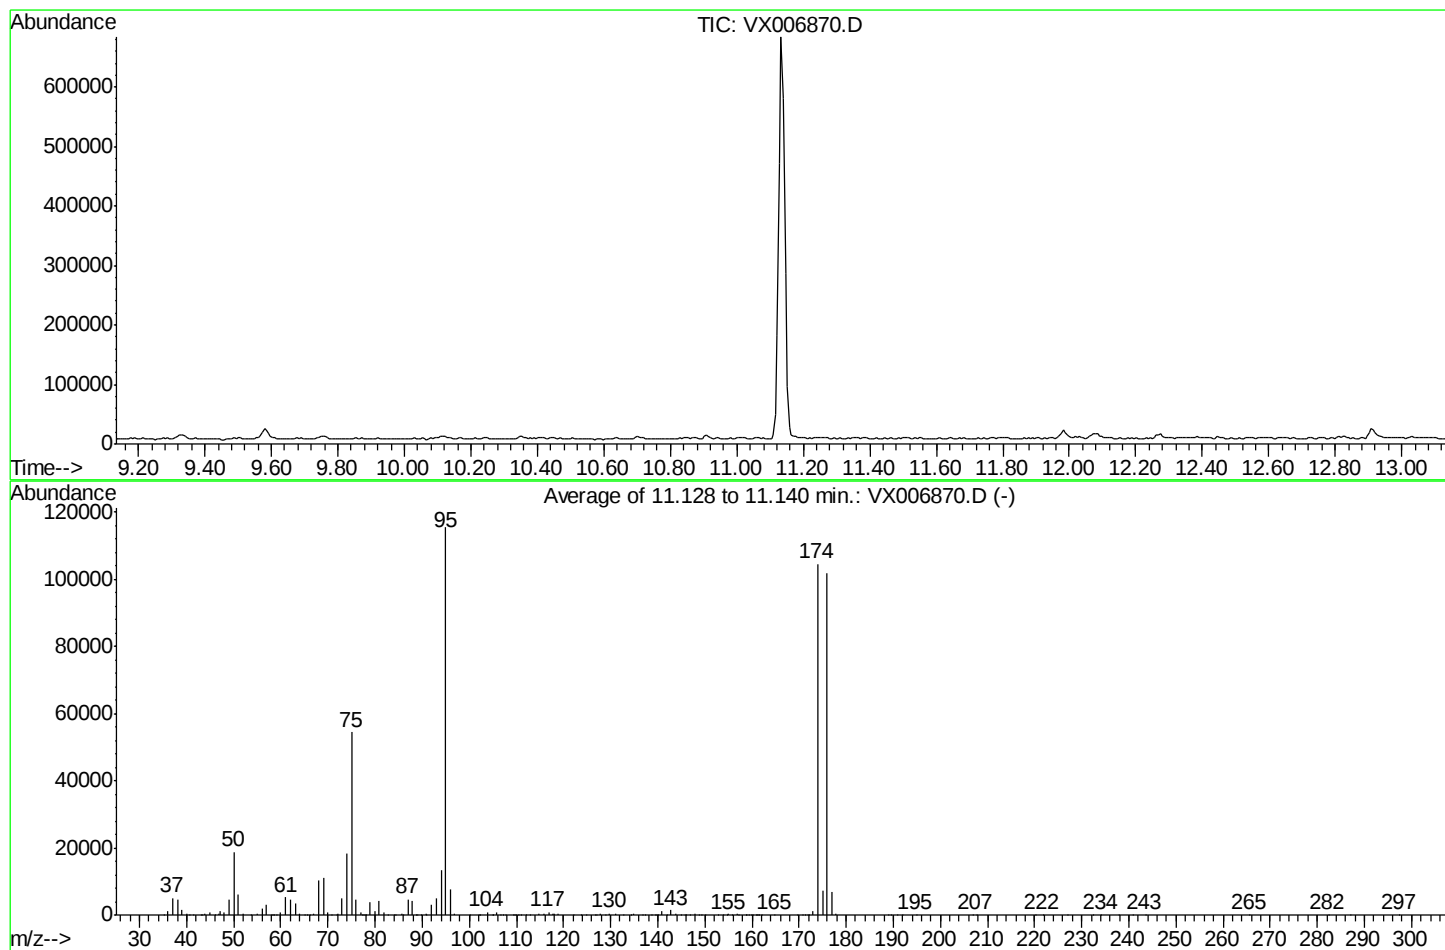

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	18744	PASS
75	95	30	60	47.2	54533	PASS
95	95	100	100	100.0	115504	PASS
96	95	5	9	6.7	7764	PASS
173	174	0.00	2	1.2	1231	PASS
174	95	50	100	90.5	104570	PASS
175	174	5	9	6.8	7141	PASS
176	174	95	101	97.4	101824	PASS
177	176	5	9	6.7	6867	PASS