

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010224\
 Data File : VX039575.D
 Acq On : 02 Jan 2024 16:31
 Operator : JC/MD
 Sample : P1002-10 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1218

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M

Title : SW846 8260

Signal : TIC: VX039575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	24	28	41	rBV	393736	401556	63.08%	10.005%
2	1.618	69	87	88	rBV5	7914	32641	5.13%	0.813%
3	2.093	157	165	172	rBV	8527	17447	2.74%	0.435%
4	2.386	206	213	225	rVB	11204	19850	3.12%	0.495%
5	2.941	296	304	312	rBV	7563	18294	2.87%	0.456%
6	4.239	510	517	526	rBV4	2319	7100	1.12%	0.177%
7	4.593	565	575	589	rBV5	2311	9306	1.46%	0.232%
8	5.385	693	705	719	rBV	66387	198751	31.22%	4.952%
9	5.544	721	731	745	rVV	98896	283766	44.58%	7.070%
10	5.952	788	798	812	rBV	79269	213317	33.51%	5.315%
11	6.757	921	930	944	rBV	188666	455637	71.58%	11.353%
12	8.647	1233	1240	1250	rBV	407146	636550	100.00%	15.860%
13	10.049	1465	1470	1485	rBV	438624	623373	97.93%	15.532%
14	10.299	1506	1511	1520	rVB2	3869	6604	1.04%	0.165%
15	10.683	1571	1574	1583	rVB	5810	9282	1.46%	0.231%
16	11.079	1634	1639	1646	rBV	366992	472572	74.24%	11.775%
17	11.134	1646	1648	1655	rVB4	4811	6869	1.08%	0.171%
18	11.683	1734	1738	1745	rBV2	5744	7370	1.16%	0.184%
19	12.018	1788	1793	1802	rBV	416314	557772	87.62%	13.897%
20	12.219	1821	1826	1836	rBV2	20936	35454	5.57%	0.883%




Sum of corrected areas: 4013511

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010224\
Data File : VX039575.D
Acq On : 02 Jan 2024 16:31
Operator : JC/MD
Sample : P1002-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

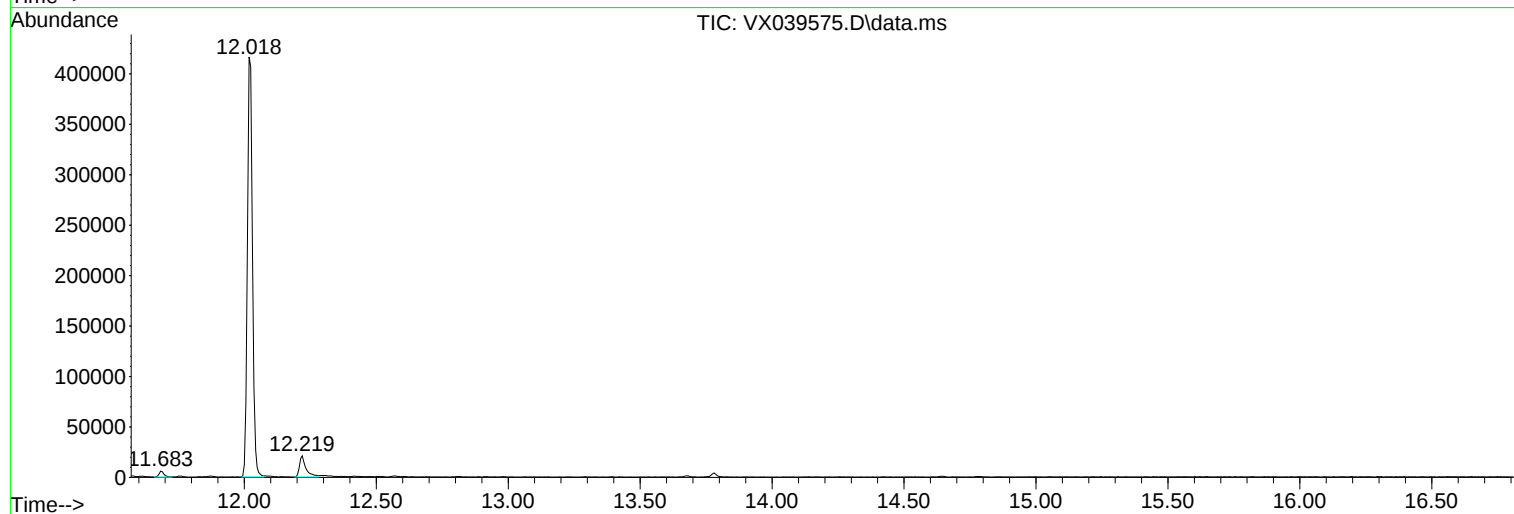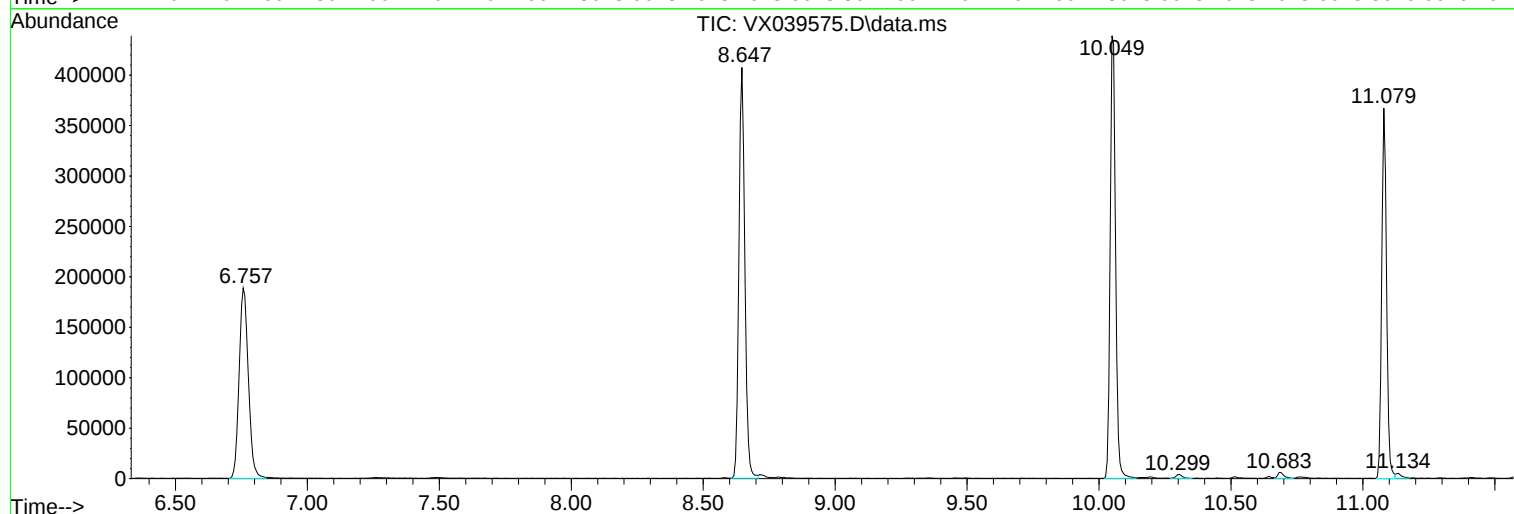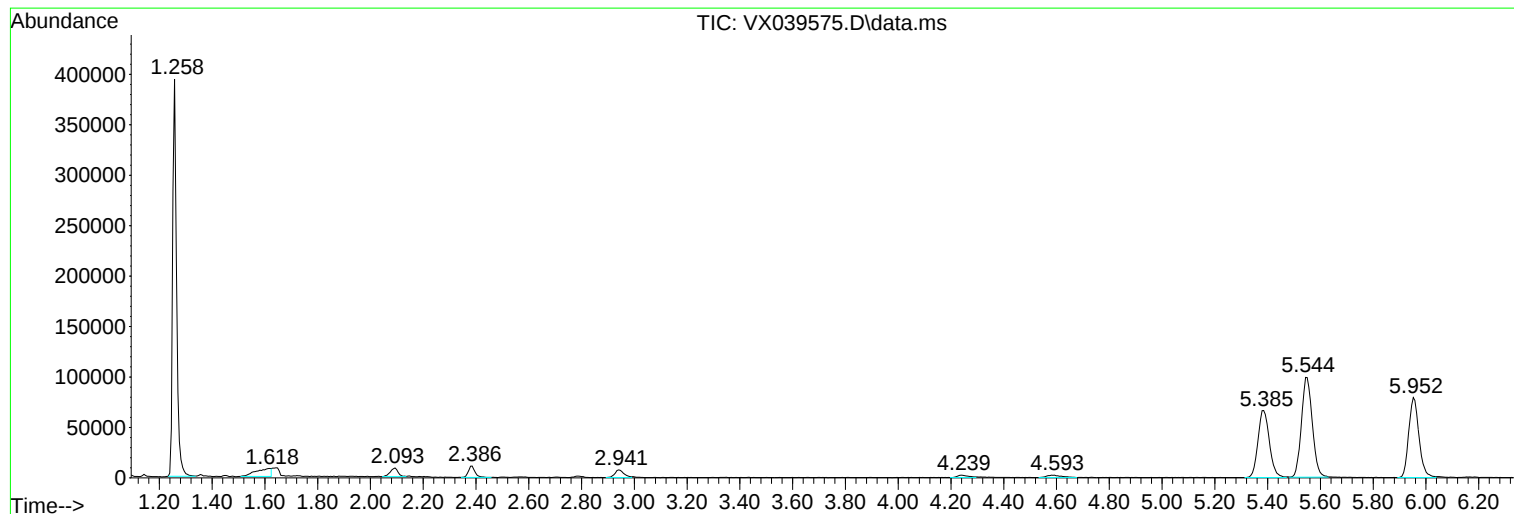

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010224\
Data File : VX039575.D
Acq On : 02 Jan 2024 16:31
Operator : JC/MD
Sample : P1002-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1218










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dimethyl ether Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.258	70.75 ug/l	401556	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dimethyl ether	46	C2H6O	000115-10-6	90
2			Ethanol	46	C2H6O	000064-17-5	7
3			Formic acid	46	CH2O2	000064-18-6	7
4			Hydrazine, methyl-	46	CH6N2	000060-34-4	4
5			Ethene, fluoro-	46	C2H3F	000075-02-5	4

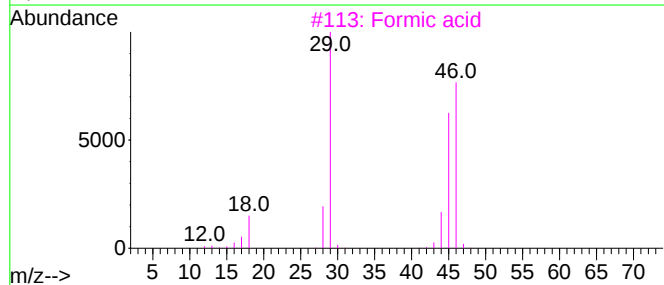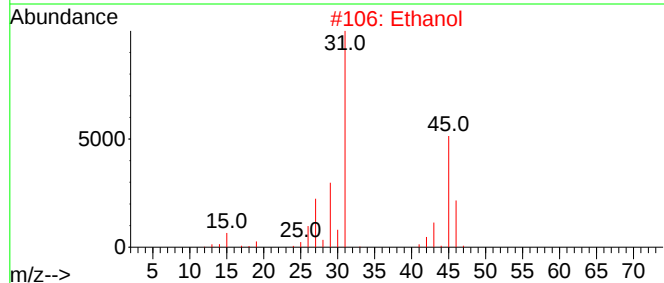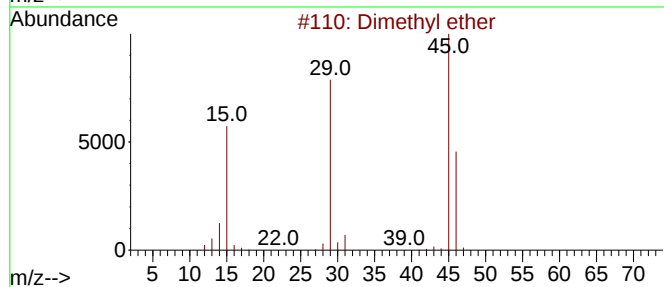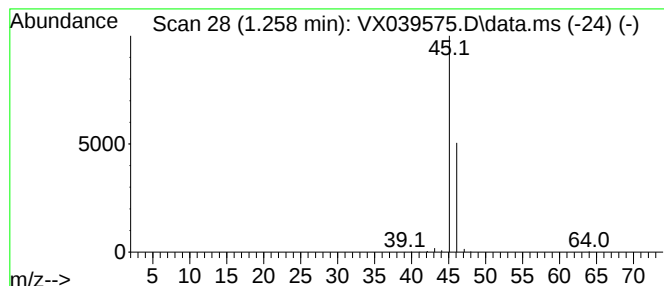

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010224\
Data File : VX039575.D
Acq On : 02 Jan 2024 16:31
Operator : JC/MD
Sample : P1002-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dimethyl ether	1.258	70.8	ug/l	401556	1	5.550	283766	50.0