

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
 Data File : VX026218.D
 Acq On : 03 Jan 2022 14:28
 Operator : JC/MD
 Sample : M5257-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 04 03:50:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	168100	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	289994	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	262134	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	130742	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	129689	53.328	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	106.660%
35) Dibromofluoromethane	5.391	113	95529	50.669	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.340%
50) Toluene-d8	8.653	98	347458	49.546	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.100%
62) 4-Bromofluorobenzene	11.085	95	129849	52.013	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	104.020%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.953	59	2064	4.249	ug/l #	73
13) Acrolein	2.245	56	113	0.651	ug/l #	71
16) Acetone	2.379	43	24424	18.536	ug/l	97
18) Methyl Acetate	2.709	43	2375	0.556	ug/l #	85
20) Methylene Chloride	2.794	84	7504	2.667	ug/l #	92
25) 2-Butanone	4.568	43	6082	3.314	ug/l #	89
29) Tetrahydrofuran	5.019	42	245	0.212	ug/l #	60
31) Cyclohexane	5.556	56	4514	1.303	ug/l #	49
36) 1,1-Dichloropropene	5.562	75	14800	4.867	ug/l #	50
38) Carbon Tetrachloride	5.556	117	17497	5.173	ug/l #	16
40) Benzene	6.043	78	3405	0.392	ug/l	93
41) Methacrylonitrile	5.031	41	403	0.202	ug/l #	45
43) Isopropyl Acetate	6.342	43	17987	3.130	ug/l	96
48) Methyl methacrylate	7.598	41	7417	2.691	ug/l #	12
49) 1,4-Dioxane	7.793	88	199	3.918	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	61604	17.227	ug/l #	50
52) Toluene	8.720	92	19595	3.668	ug/l	99
53) t-1,3-Dichloropropene	8.714	75	286	1.970	ug/l #	1
54) cis-1,3-Dichloropropene	8.549	75	24354	6.878	ug/l #	69
57) 1,3-Dichloropropane	9.482	76	13397	3.562	ug/l #	43
59) 2-Hexanone	9.378	43	7581	2.799	ug/l #	25
67) Ethyl Benzene	10.195	91	146849	14.262	ug/l	99
68) m/p-Xylenes	10.305	106	305204	79.387	ug/l	93
69) o-Xylene	10.646	106	686778	182.576	ug/l	94
70) Styrene	10.646	104	48574	7.877	ug/l #	1
73) Isopropylbenzene	10.963	105	31517	3.101	ug/l	97
74) N-amyl acetate	10.860	43	1195	0.256	ug/l #	1
76) 1,2,3-Trichloropropane	11.378	75	8330	2.640	ug/l #	1
78) n-propylbenzene	11.305	91	43326	3.708	ug/l #	51
79) 2-Chlorotoluene	11.378	91	113555	15.788	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	1212980	143.827	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	70988	65.077	ug/l #	10
82) 4-Chlorotoluene	11.451	91	142595	17.554	ug/l #	44
83) tert-Butylbenzene	11.756	119	188327	23.006	ug/l #	44
84) 1,2,4-Trimethylbenzene	11.756	105	1579017	187.379	ug/l	99
85) sec-Butylbenzene	11.756	105	1579017	154.572	ug/l #	56

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
 Data File : VX026218.D
 Acq On : 03 Jan 2022 14:28
 Operator : JC/MD
 Sample : M5257-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 04 03:50:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
86) p-Isopropyltoluene	12.012	119	55066	6.466	ug/l	97
89) n-Butylbenzene	12.323	91	55800	7.373	ug/l #	1
90) Hexachloroethane	12.554	117	26119	15.356	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	12.969	75	20246	22.883	ug/l #	1
95) Naphthalene	13.780	128	5079868	502.726	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
Data File : VX026218.D
Acq On : 03 Jan 2022 14:28
Operator : JC/MD
Sample : M5257-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jan 04 03:50:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration




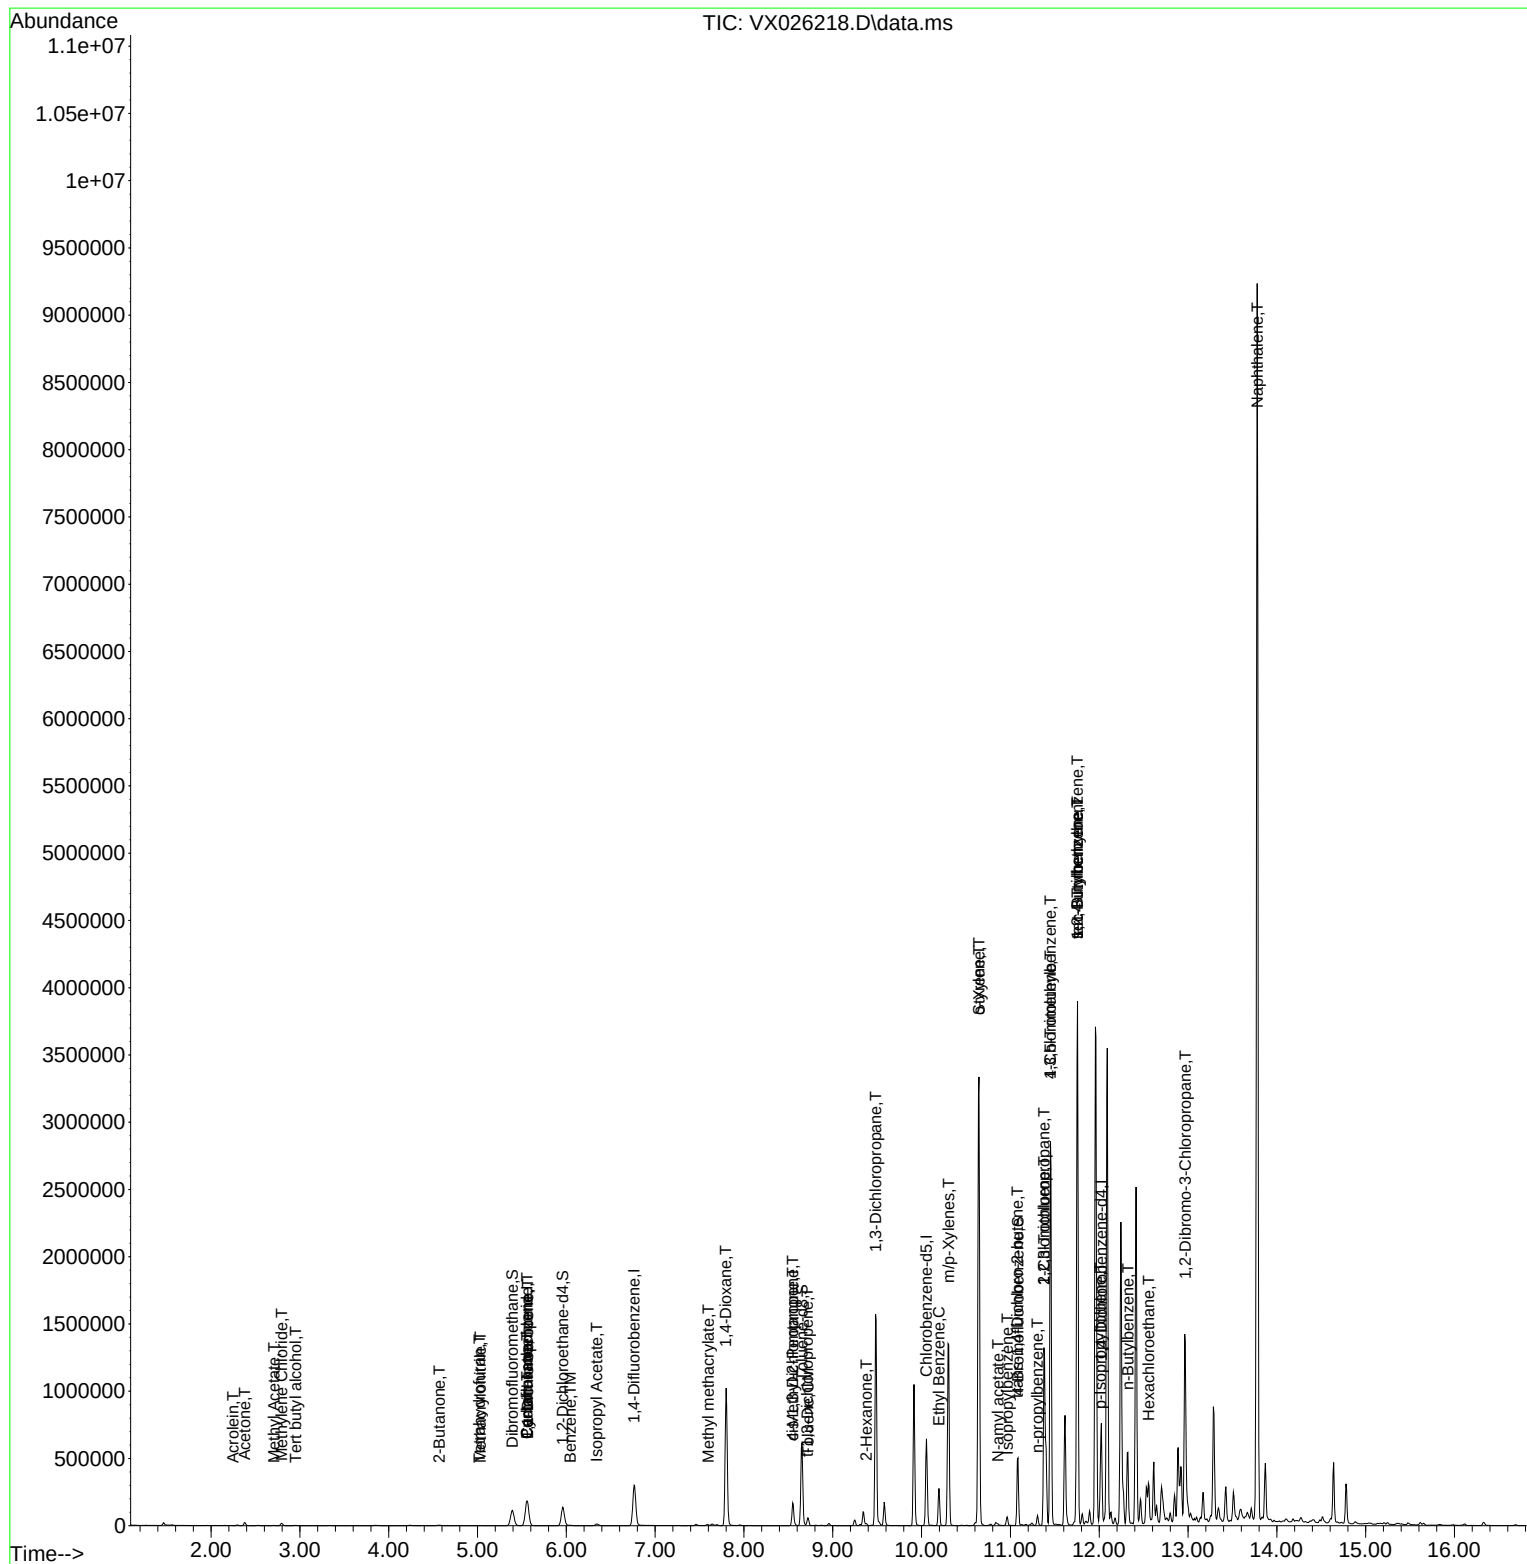


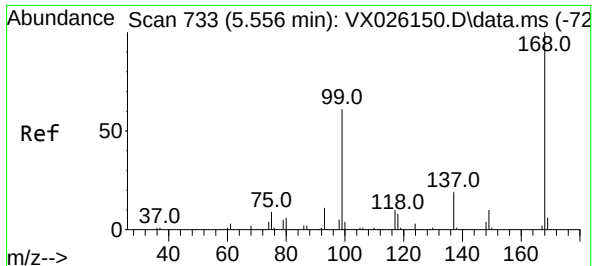

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 168100
Ion Ratio Lower Upper
168 100
99 61.1 45.8 68.8

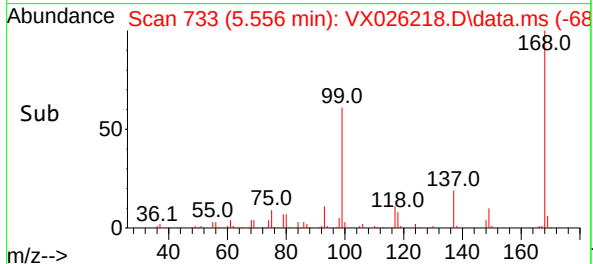

#11
Tert butyl alcohol
Concen: 4.249 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.030 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28


Tgt Ion: 59 Resp: 2064
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

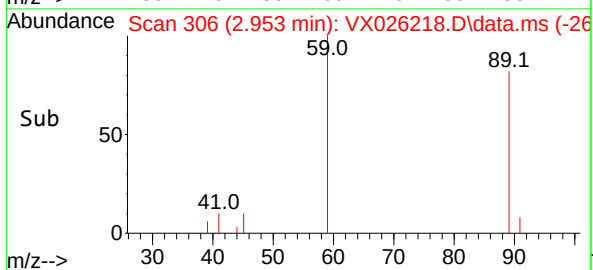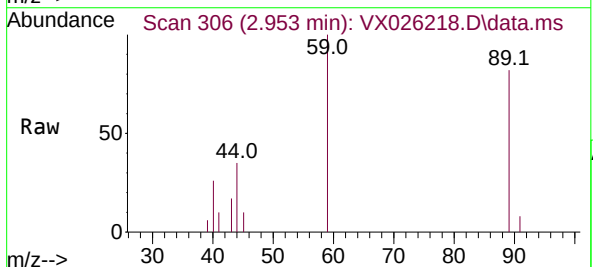



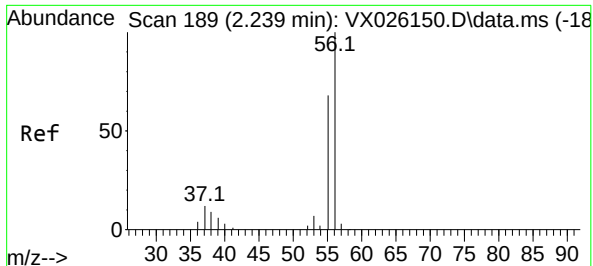


#13
Acrolein
Concen: 0.651 ug/l
RT: 2.245 min Scan# 19
Delta R.T. 0.006 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 113
Ion Ratio Lower Upper
56 100
55 47.8 57.4 86.2#

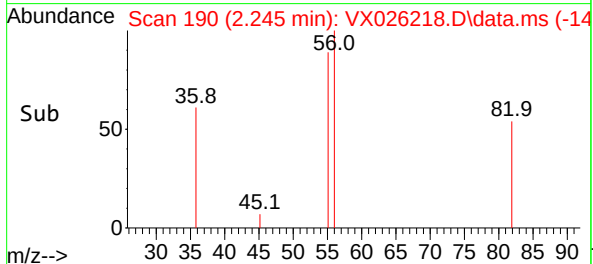

#16
Acetone
Concen: 18.536 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.007 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 43 Resp: 24424
Ion Ratio Lower Upper
43 100
58 29.2 24.8 37.2


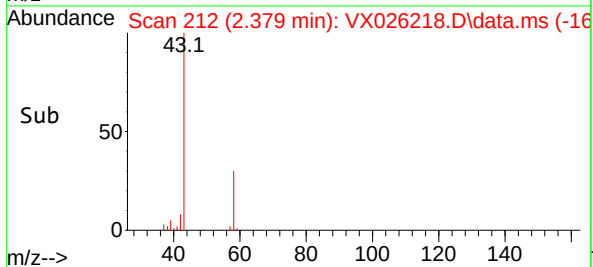

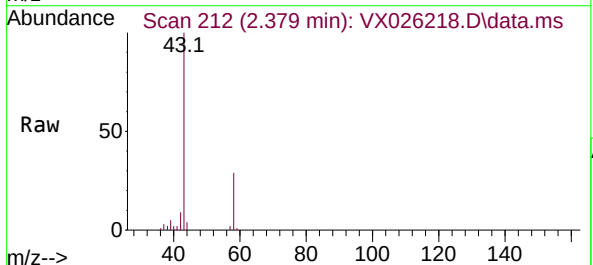




#18
Methyl Acetate
Concen: 0.556 ug/l
RT: 2.709 min Scan# 20
Delta R.T. -0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2375
Ion Ratio Lower Upper
43 100
74 16.5 19.1 28.7#

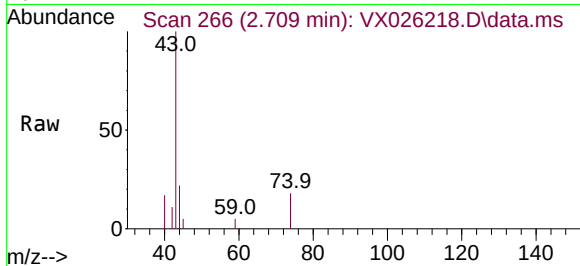

#20
Methylene Chloride
Concen: 2.667 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 84 Resp: 7504
Ion Ratio Lower Upper
84 100
49 131.7 97.1 145.7
51 44.8 29.3 43.9#
86 64.5 50.8 76.2

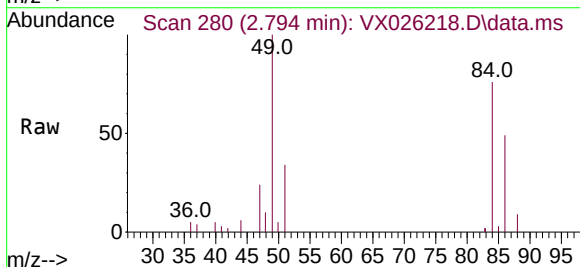

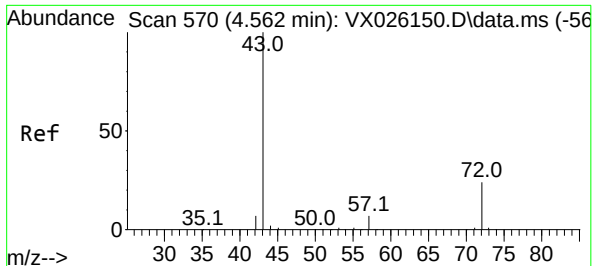

#25

2-Butanone

Concen: 3.314 ug/l

RT: 4.568 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 6082

Ion Ratio Lower Upper

43 100

72 20.6 21.0 31.4#

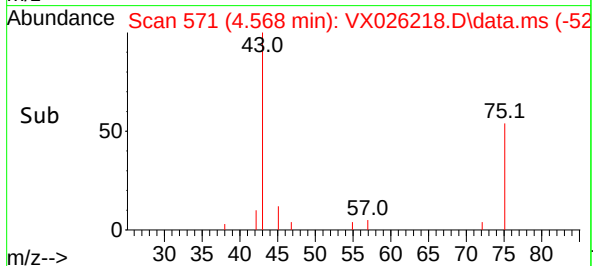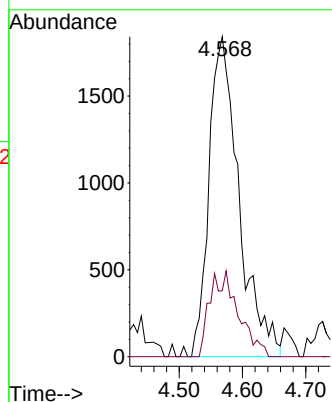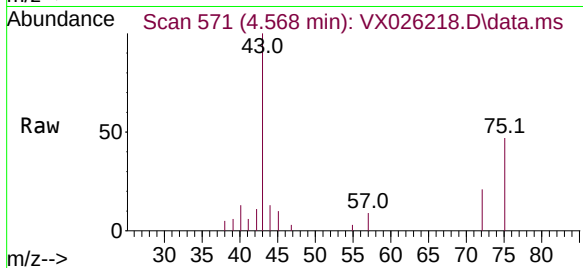

#29

Tetrahydrofuran

Concen: 0.212 ug/l

RT: 5.019 min Scan# 645

Delta R.T. 0.006 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28



Tgt Ion: 42 Resp: 245


Ion Ratio Lower Upper

42 100

72 38.0 37.0 55.6


71 86.9 34.1 51.1#

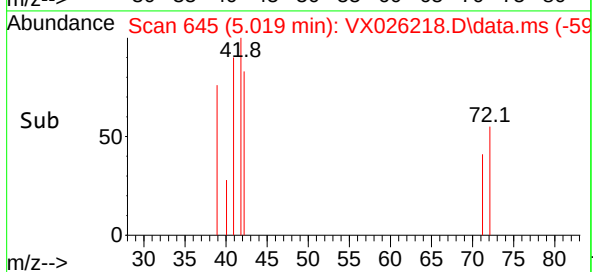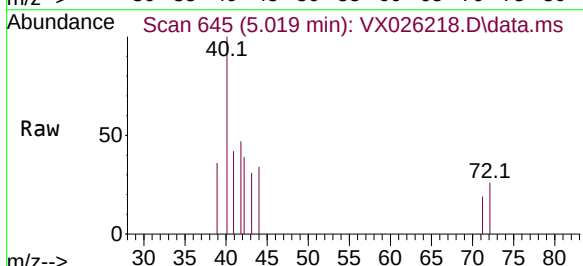



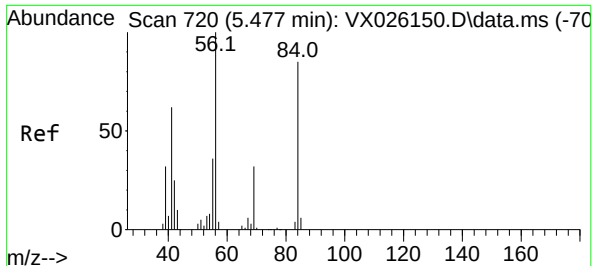


#31
Cyclohexane
Concen: 1.303 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.079 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 4514
Ion Ratio Lower Upper
56 100
69 128.6 23.9 35.9#
84 83.4 73.2 109.8

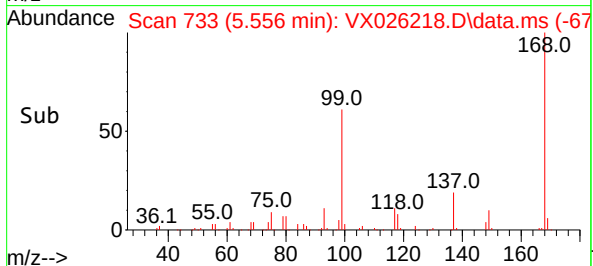

#33
1,2-Dichloroethane-d4
Concen: 53.328 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 65 Resp: 129689
Ion Ratio Lower Upper
65 100
67 50.4 0.0 103.4


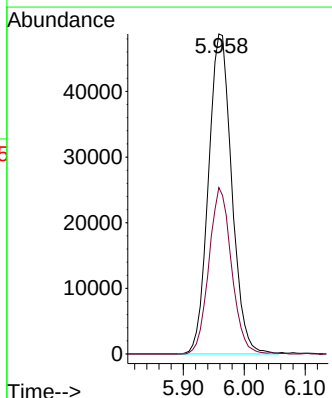

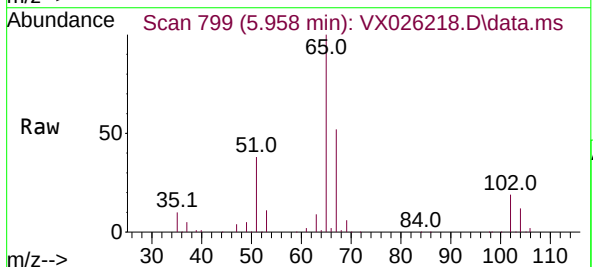




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 289994
Ion Ratio Lower Upper
114 100
63 21.2 0.0 40.0
88 16.2 0.0 30.6



#35
Dibromofluoromethane
Concen: 50.669 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion:113 Resp: 95529
Ion Ratio Lower Upper
113 100
111 103.8 81.8 122.8
192 19.1 15.0 22.4









#36
1,1-Dichloropropene
Concen: 4.867 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 14800
Ion Ratio Lower Upper
75 100
110 9.9 18.2 54.6#
77 0.0 24.7 37.1#



#38
Carbon Tetrachloride
Concen: 5.173 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 117 Resp: 17497
Ion Ratio Lower Upper
117 100
119 6.0 77.2 115.8#
121 0.0 23.8 35.8#



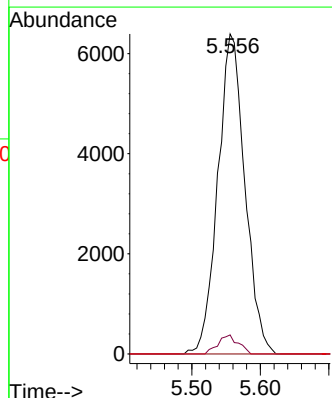



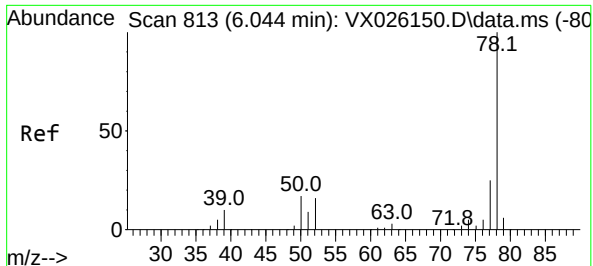

#40
Benzene
Concen: 0.392 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.001 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 78 Resp: 3405
Ion Ratio Lower Upper
78 100
77 19.7 18.6 27.8

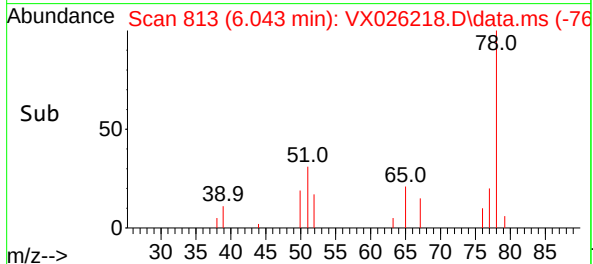

#41
Methacrylonitrile
Concen: 0.202 ug/l
RT: 5.031 min Scan# 647
Delta R.T. 0.103 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28


Tgt Ion: 41 Resp: 403
Ion Ratio Lower Upper
41 100
39 62.5 44.2 66.2
67 0.0 59.7 89.5#
52 0.0 24.2 36.2#

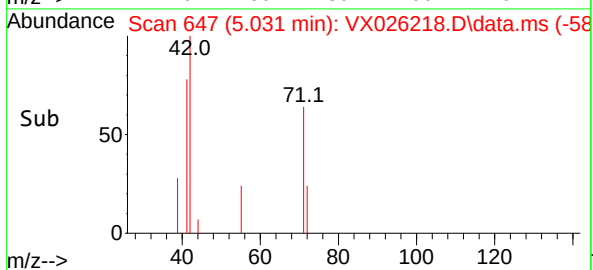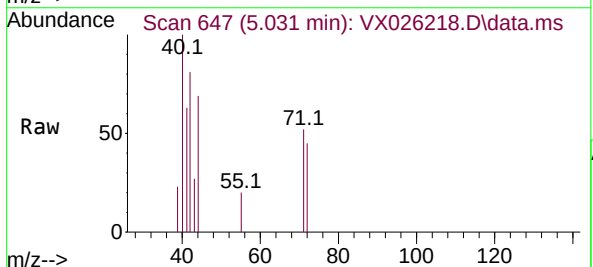






#43
Isopropyl Acetate
Concen: 3.130 ug/l
RT: 6.342 min Scan# 81
Delta R.T. -0.006 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion: 43 Resp: 17987




Ion	Ratio	Lower	Upper
43	100		
61	18.3	15.7	23.5
87	11.6	11.2	16.8




#48
Methyl methacrylate
Concen: 2.691 ug/l
RT: 7.598 min Scan# 1068
Delta R.T. -0.098 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 41 Resp: 7417

Ion	Ratio	Lower	Upper
41	100		
69	0.0	67.3	100.9#
39	0.0	50.2	75.2#

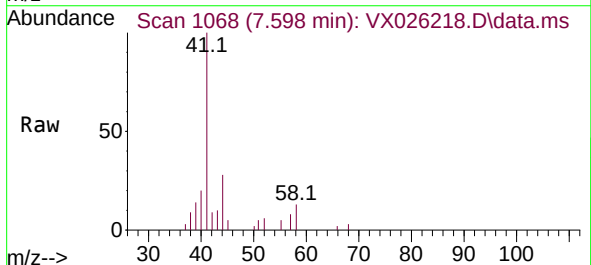



#49

1,4-Dioxane

Concen: 3.918 ug/l

RT: 7.793 min Scan# 1100

Delta R.T. 0.109 min


Lab File: VX026218.D

Acq: 03 Jan 2022 14:28

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 88 Resp: 199

Ion Ratio Lower Upper

88 100

43 466396.5 25.3 37.9#

58 1980.9 51.8 77.6#

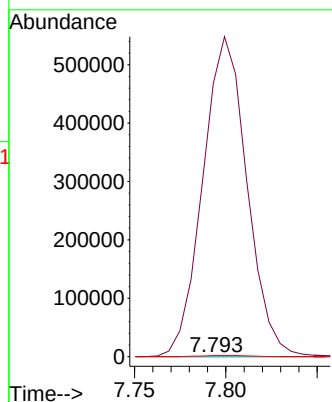

#50

Toluene-d8

Concen: 49.546 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX026218.D




Acq: 03 Jan 2022 14:28


Tgt Ion: 98 Resp: 347458

Ion Ratio Lower Upper

98 100

100 65.2 52.6 78.8







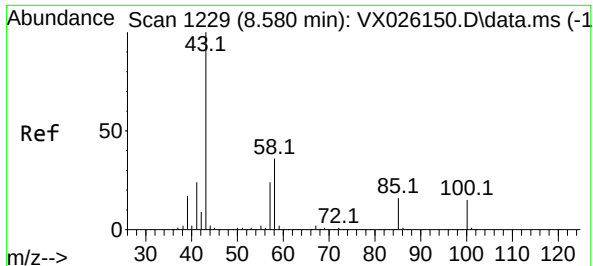

#51
4-Methyl-2-Pentanone
Concen: 17.227 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.031 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 61604
Ion Ratio Lower Upper
43 100
58 8.3 30.8 46.2#

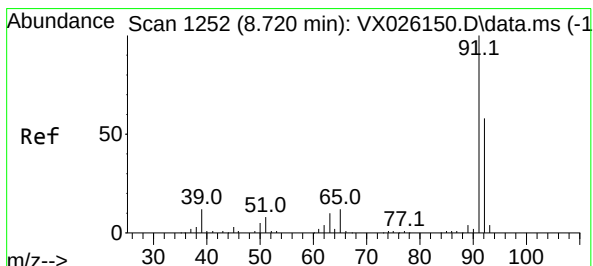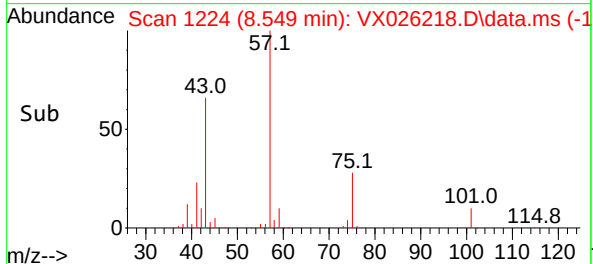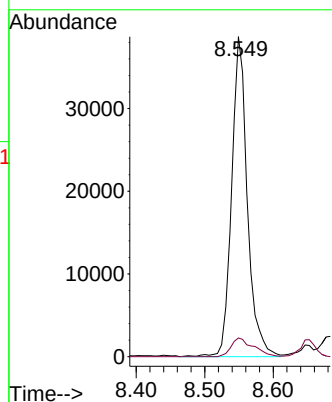

#52
Toluene
Concen: 3.668 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 92 Resp: 19595
Ion Ratio Lower Upper
92 100
91 171.9 136.0 204.0

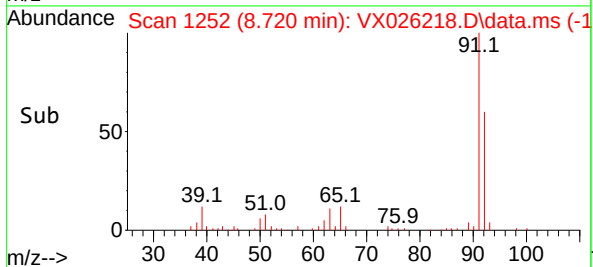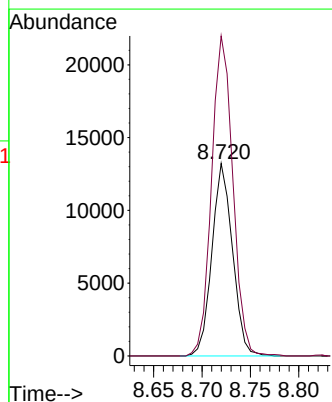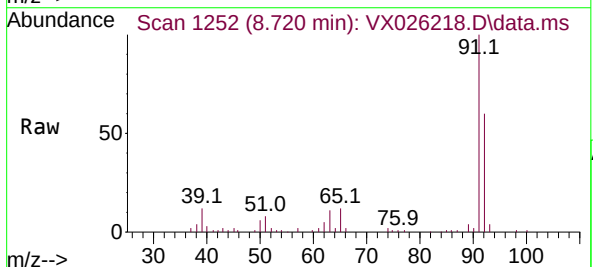



#53

t-1,3-Dichloropropene

Concen: 1.970 ug/l

RT: 8.714 min Scan# 11

Delta R.T. -0.268 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 286

Ion Ratio Lower Upper

75 100

77 95.1 25.1 37.7#

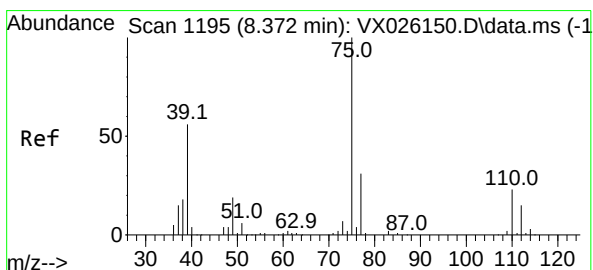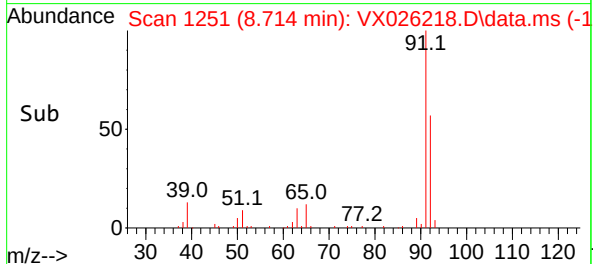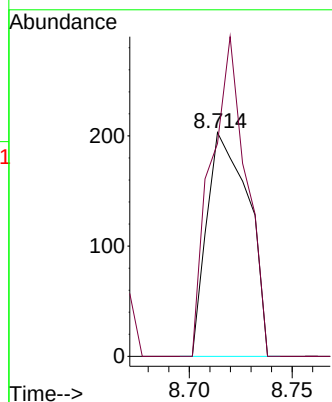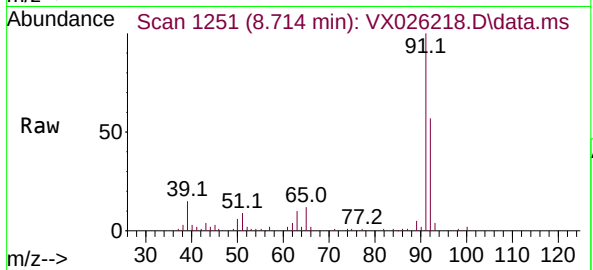

#54

cis-1,3-Dichloropropene

Concen: 6.878 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.177 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28




Tgt Ion: 75 Resp: 24354


Ion Ratio Lower Upper

75 100

77 0.4 25.3 37.9#

39 41.3 41.4 62.0#

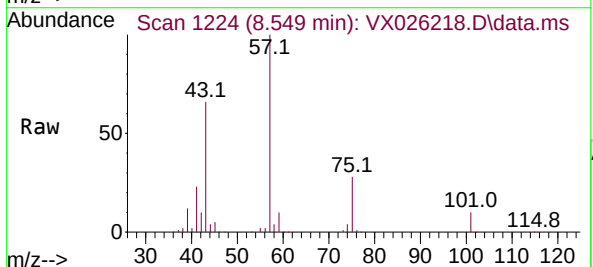



#57

1,3-Dichloropropane

Concen: 3.562 ug/l

RT: 9.482 min Scan# 13397

Delta R.T. 0.171 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 76 Resp: 13397

Ion Ratio Lower Upper

76 100

78 0.2 26.0 39.0#



#59

2-Hexanone

Concen: 2.799 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.055 min

Lab File: VX026218.D




Acq: 03 Jan 2022 14:28


Tgt Ion: 43 Resp: 7581

Ion Ratio Lower Upper

43 100

58 0.0 26.9 80.6#









#62
4-Bromofluorobenzene
Concen: 52.013 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 129849
Ion Ratio Lower Upper
95 100
174 73.7 0.0 157.4
176 71.5 0.0 154.6

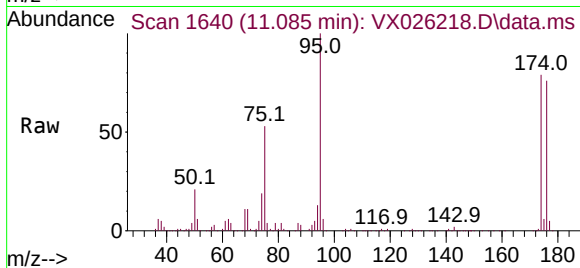

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 117 Resp: 262134
Ion Ratio Lower Upper
117 100
82 57.5 43.8 65.6
119 32.0 25.2 37.8




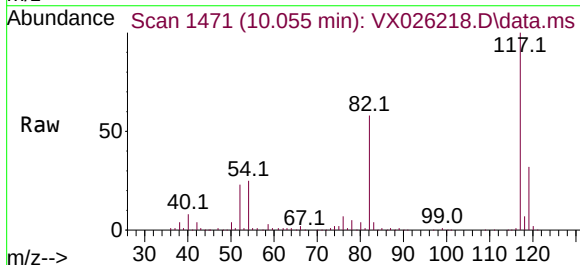




#67
Ethyl Benzene
Concen: 14.262 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 146849
Ion Ratio Lower Upper
91 100
106 31.3 25.7 38.5



#68
m/p-Xylenes
Concen: 79.387 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion:106 Resp: 305204
Ion Ratio Lower Upper
106 100
91 209.5 158.6 238.0









#69
o-Xylene
Concen: 182.576 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 686778
Ion Ratio Lower Upper
106 100
91 221.0 105.5 316.4

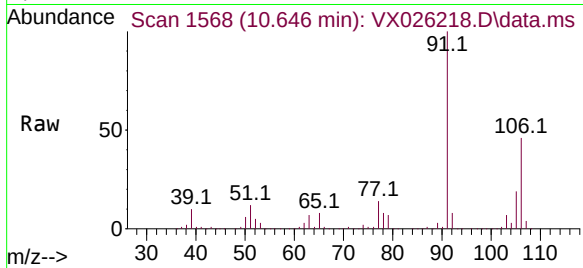

#70
Styrene
Concen: 7.877 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.013 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion:104 Resp: 48574
Ion Ratio Lower Upper
104 100
78 254.7 39.8 59.6#
103 209.6 43.0 64.6#




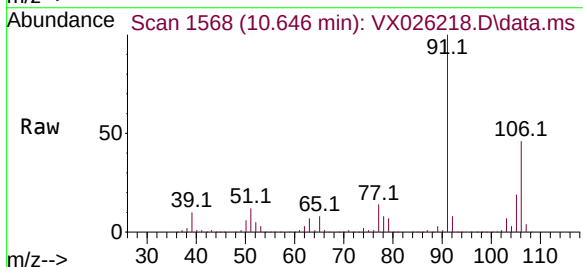




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 130742
Ion Ratio Lower Upper
152 100
115 65.0 41.3 123.9
150 157.0 0.0 351.8

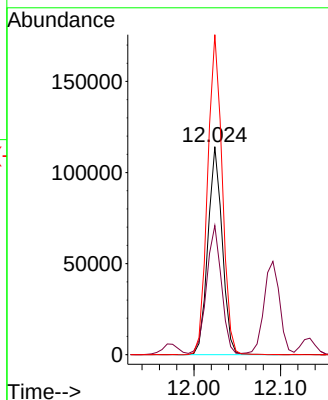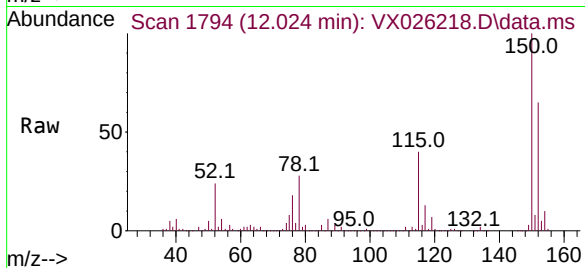

#73
Isopropylbenzene
Concen: 3.101 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion:105 Resp: 31517
Ion Ratio Lower Upper
105 100
120 25.7 13.6 40.7



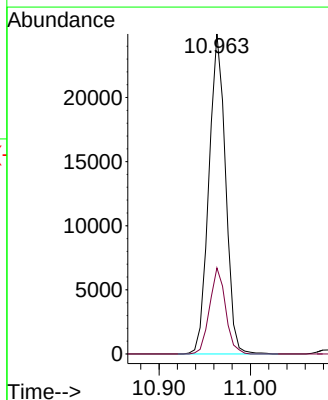
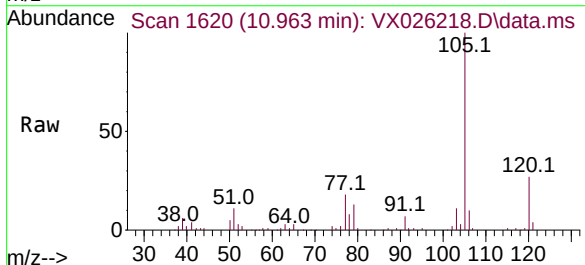




#74
N-amy1 acetate
Concen: 0.256 ug/l
RT: 10.860 min Scan# 1
Delta R.T. 0.012 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 1195
Ion Ratio Lower Upper
43 100
70 129.0 34.1 51.1#
55 142.3 19.2 28.8#
61 0.0 19.0 28.4#



#76
1,2,3-Trichloropropane
Concen: 2.640 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.134 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 75 Resp: 8330
Ion Ratio Lower Upper
75 100
77 1319.9 19.0 57.0#





#78

n-propylbenzene

Concen: 3.708 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 43326

Ion Ratio Lower Upper

91 100

120 0.0 12.0 36.1#

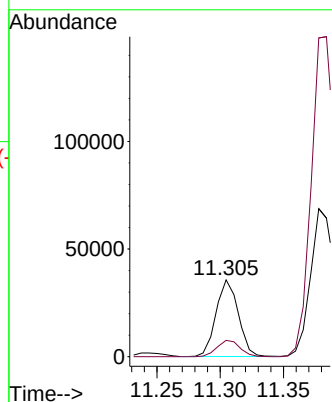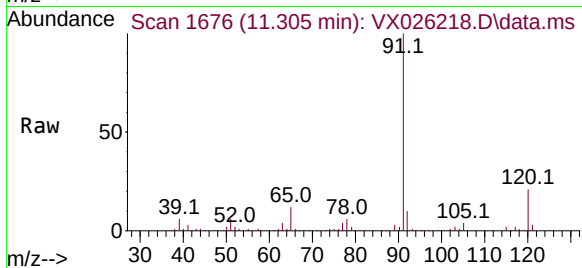

#79

2-Chlorotoluene

Concen: 15.788 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.012 min

Lab File: VX026218.D




Acq: 03 Jan 2022 14:28


Tgt Ion: 91 Resp: 113555

Ion Ratio Lower Upper

91 100

126 0.5 17.8 53.3#




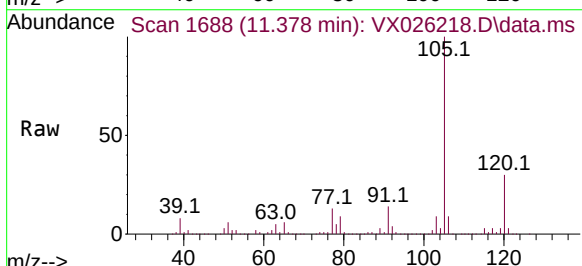




#80
1,3,5-Trimethylbenzene
Concen: 143.827 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 1212980
Ion Ratio Lower Upper
105 100
120 47.7 24.9 74.7

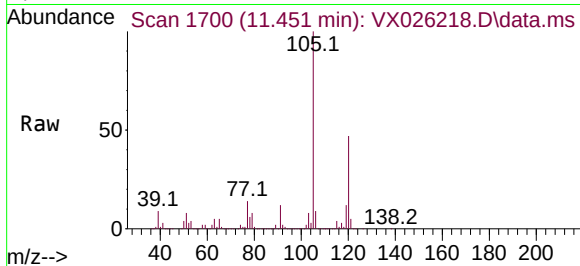

#81
trans-1,4-Dichloro-2-butene
Concen: 65.077 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 75 Resp: 70988
Ion Ratio Lower Upper
75 100
53 0.1 79.5 119.3#
89 0.0 38.3 57.5#

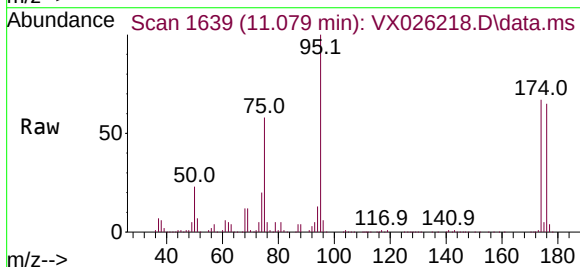



#82

4-Chlorotoluene

Concen: 17.554 ug/l

RT: 11.451 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 142595

Ion Ratio Lower Upper

91 100

126 0.0 15.6 46.7#

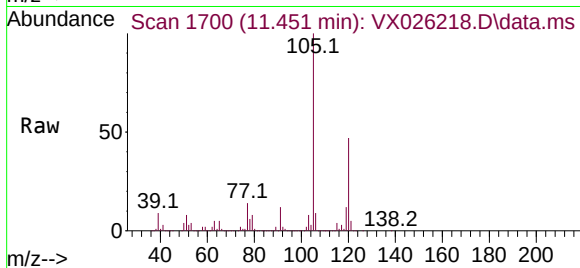

#83

tert-Butylbenzene

Concen: 23.006 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. 0.037 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28




Tgt Ion: 119 Resp: 188327


Ion Ratio Lower Upper

119 100

91 100.9 28.7 86.1#

134 0.0 11.9 35.9#




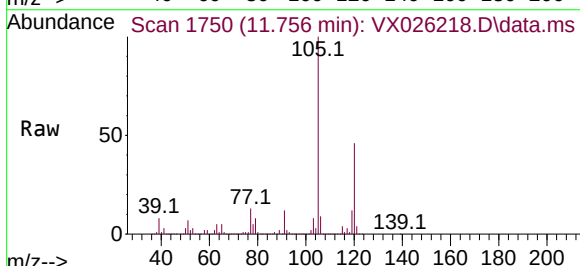




#84
1,2,4-Trimethylbenzene
Concen: 187.379 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 1579017
Ion Ratio Lower Upper
105 100
120 44.8 22.9 68.7

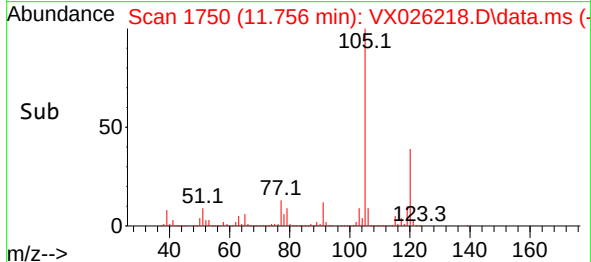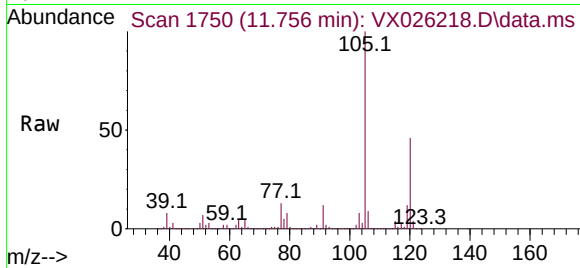

#85
sec-Butylbenzene
Concen: 154.572 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion:105 Resp: 1579017
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#




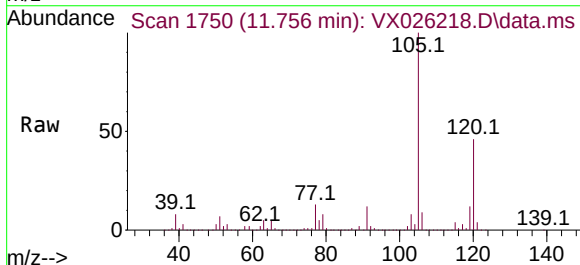




#86
p-Isopropyltoluene
Concen: 6.466 ug/l
RT: 12.012 min Scan# 119
Delta R.T. -0.000 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:119 Resp: 55066
Ion Ratio Lower Upper
119 100
134 26.6 13.2 39.6
91 26.6 11.9 35.9

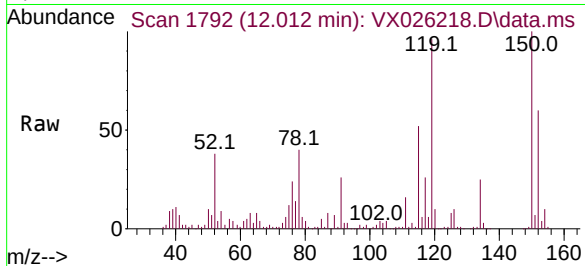

#89
n-Butylbenzene
Concen: 7.373 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX026218.D
Acq: 03 Jan 2022 14:28

Tgt Ion: 91 Resp: 55800
Ion Ratio Lower Upper
91 100
92 21.6 27.3 81.8#
134 141.9 13.5 40.4#

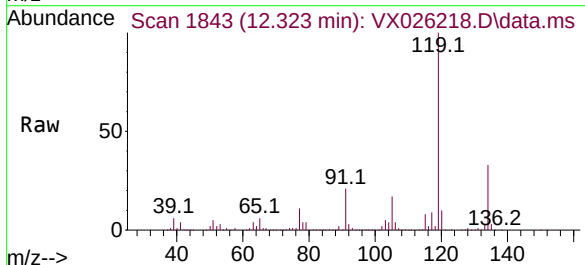



#90

Hexachloroethane

Concen: 15.356 ug/l

RT: 12.554 min Scan# 117

Delta R.T. 0.012 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:117 Resp: 26119

Ion Ratio Lower Upper

117 100

201 0.0 35.4 106.3#

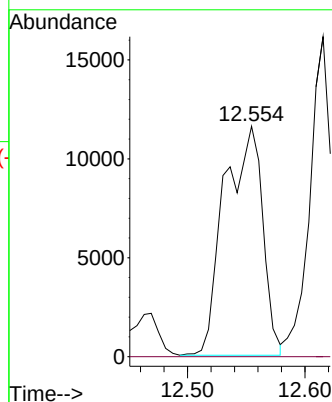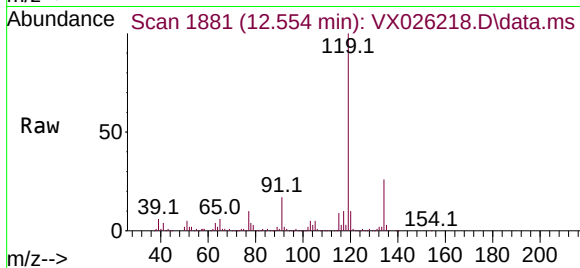

#92

1,2-Dibromo-3-Chloropropane

Concen: 22.883 ug/l

RT: 12.969 min Scan# 1949

Delta R.T. 0.024 min

Lab File: VX026218.D

Acq: 03 Jan 2022 14:28




Tgt Ion: 75 Resp: 20246


Ion Ratio Lower Upper

75 100

155 0.0 44.0 131.8#

157 0.0 55.5 166.5#

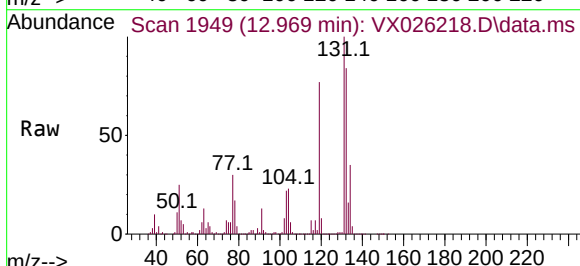



#95

Naphthalene

Concen: 502.726 ug/l

RT: 13.780 min Scan# 20

Delta R.T. -0.000 min


Lab File: VX026218.D

Acq: 03 Jan 2022 14:28

Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion:128 Resp: 5079868

Ion Ratio Lower Upper

128 100

127 14.3 10.3 15.5

129 12.2 8.8 13.2

