

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
 Data File : VX026235.D
 Acq On : 03 Jan 2022 21:01
 Operator : JC/MD
 Sample : M5333-02 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-2R

Quant Time: Jan 04 03:55:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	197226	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	344149	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	302088	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	128032	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	153125	53.666	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 107.340%	
35) Dibromofluoromethane	5.391	113	112338	50.209	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.420%	
50) Toluene-d8	8.653	98	406055	48.791	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 97.580%	
62) 4-Bromofluorobenzene	11.079	95	141846	47.878	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 95.760%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
Data File : VX026235.D
Acq On : 03 Jan 2022 21:01
Operator : JC/MD
Sample : M5333-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2R

Quant Time: Jan 04 03:55:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration




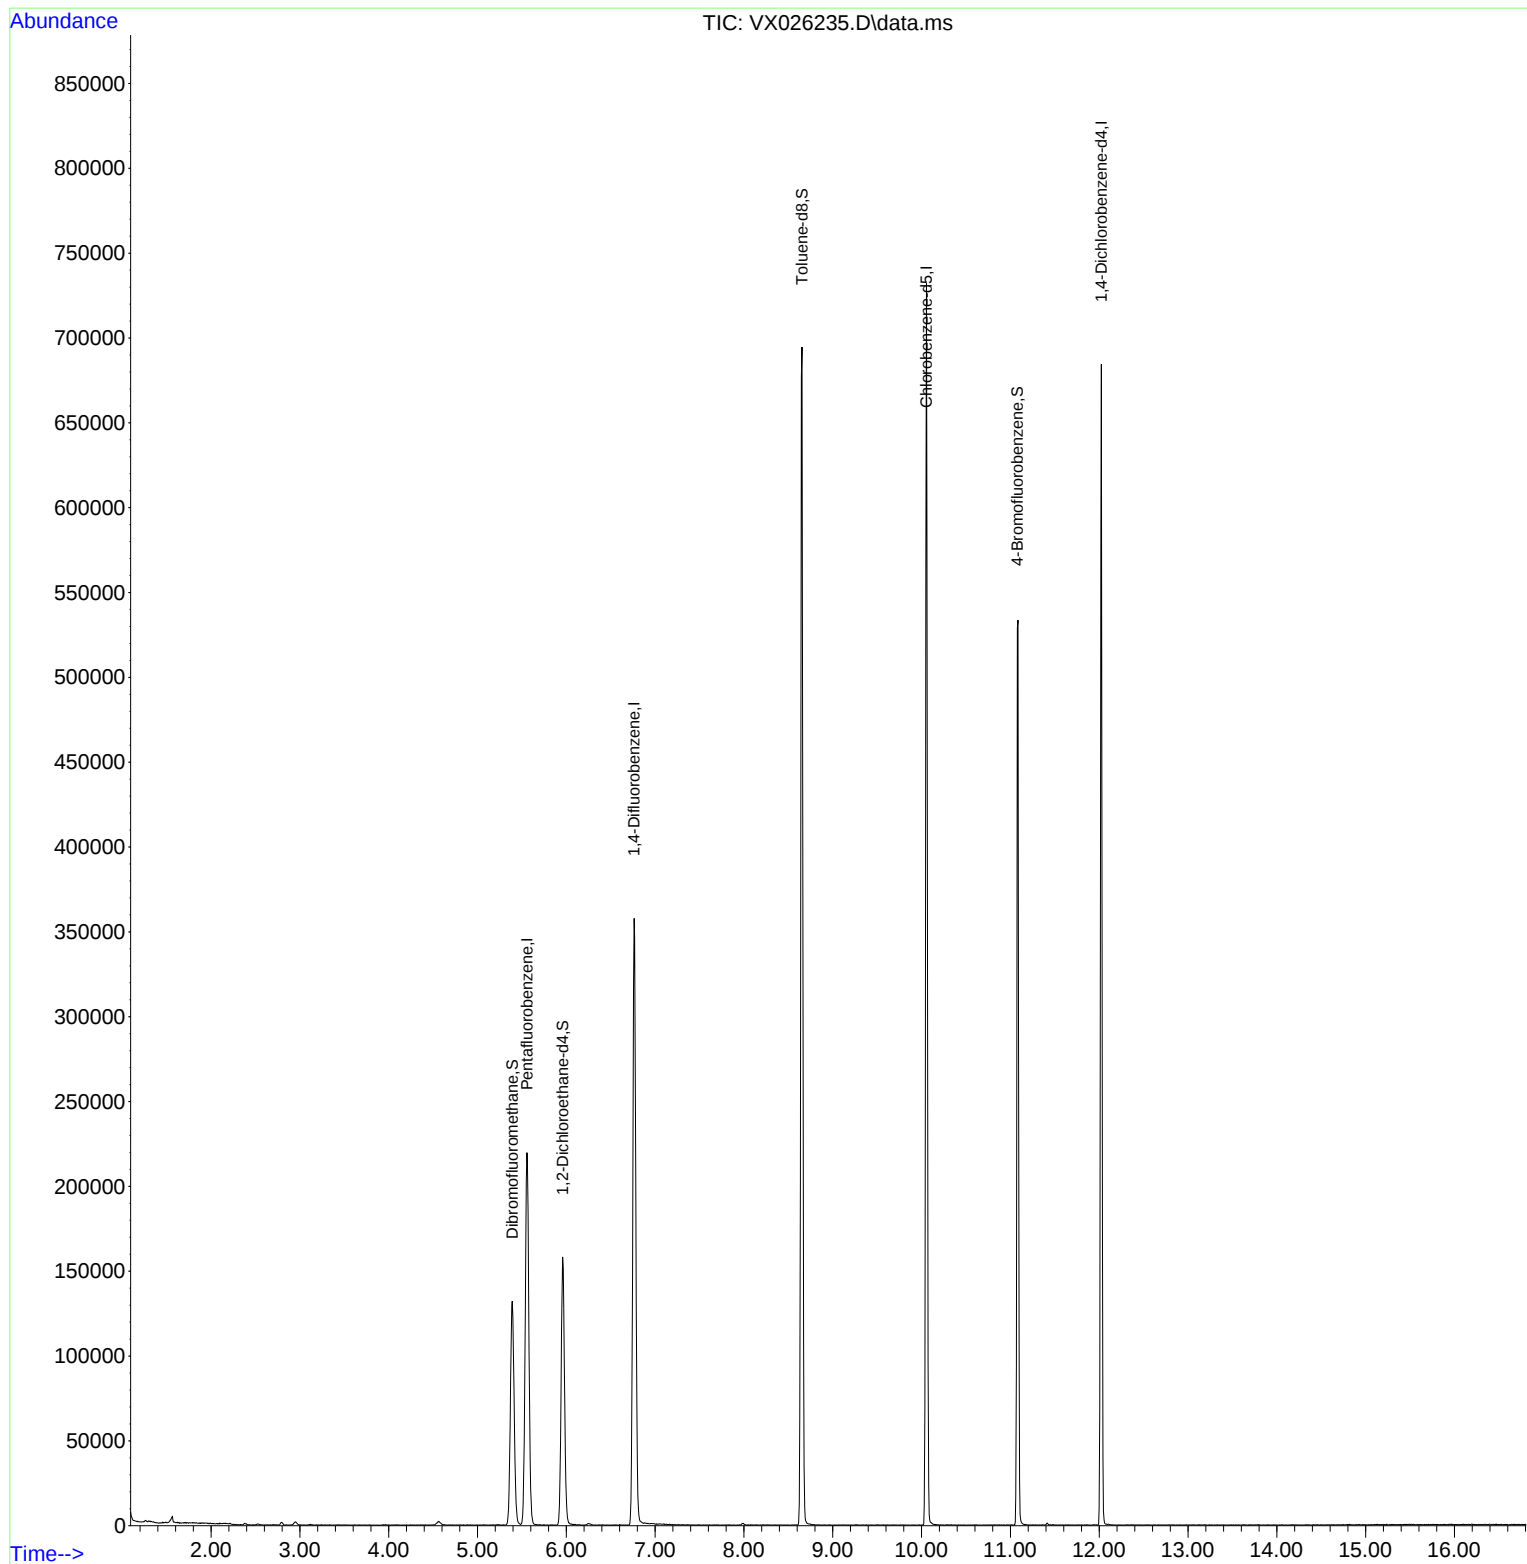


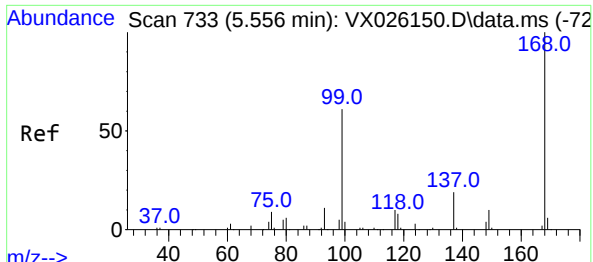

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026235.D
Acq: 03 Jan 2022 21:01




Instrument :
MSVOA_X
ClientSampleId :
MW-2R


Tgt Ion:168 Resp: 197226
Ion Ratio Lower Upper
168 100
99 65.2 45.8 68.8

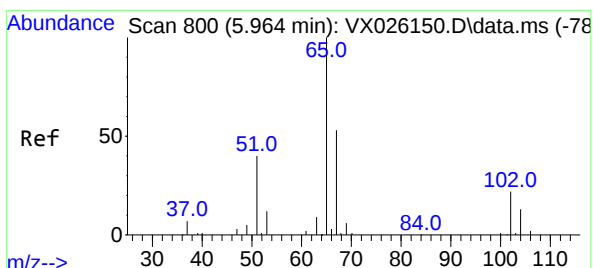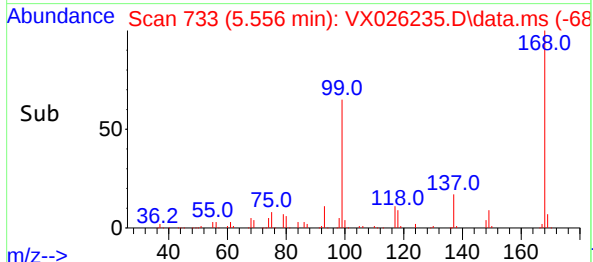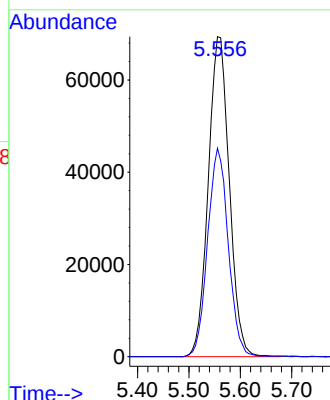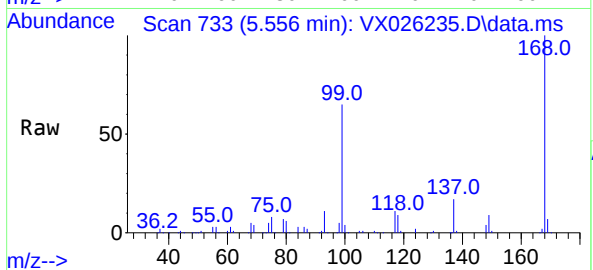

#33
1,2-Dichloroethane-d4
Concen: 53.666 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX026235.D
Acq: 03 Jan 2022 21:01

Tgt Ion: 65 Resp: 153125
Ion Ratio Lower Upper
65 100
67 50.4 0.0 103.4


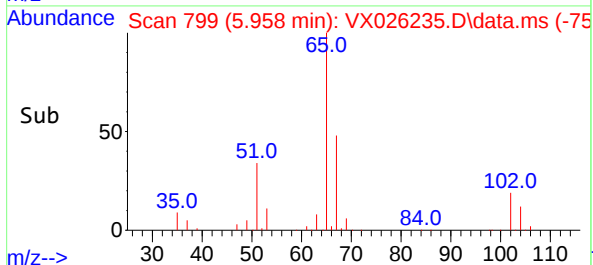
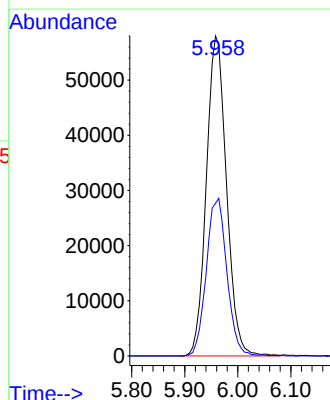
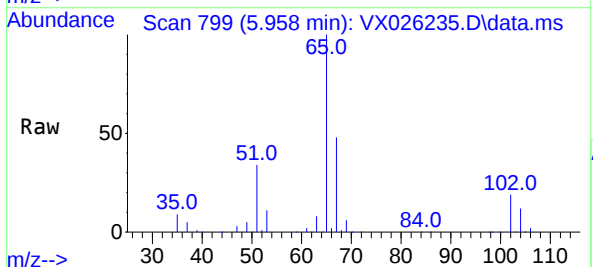


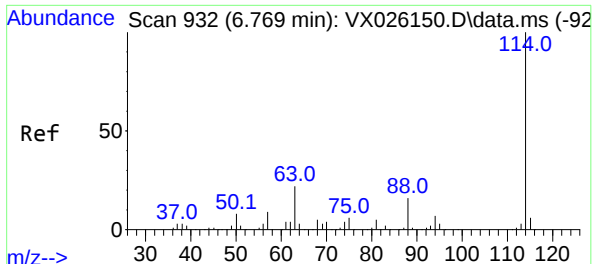

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX026235.D
Acq: 03 Jan 2022 21:01




Instrument :
MSVOA_X
ClientSampleId :
MW-2R


Tgt Ion:114 Resp: 344149
Ion Ratio Lower Upper
114 100
63 23.1 0.0 40.0
88 16.5 0.0 30.6

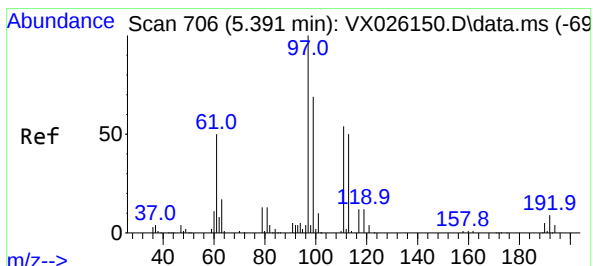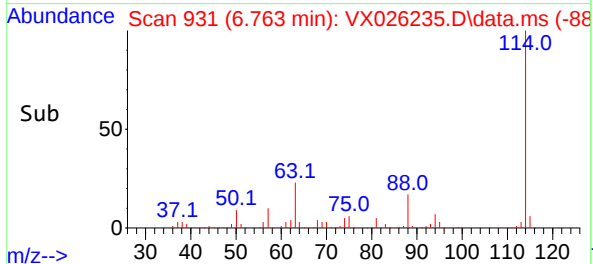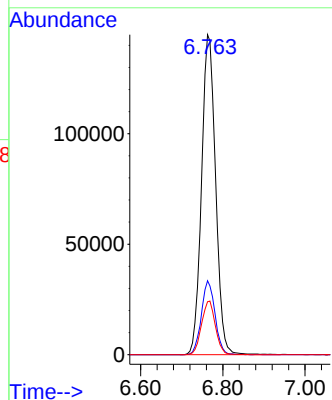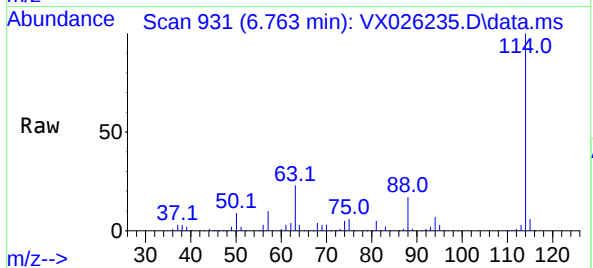

#35
Dibromofluoromethane
Concen: 50.209 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX026235.D
Acq: 03 Jan 2022 21:01

Tgt Ion:113 Resp: 112338
Ion Ratio Lower Upper
113 100
111 103.6 81.8 122.8
192 18.5 15.0 22.4


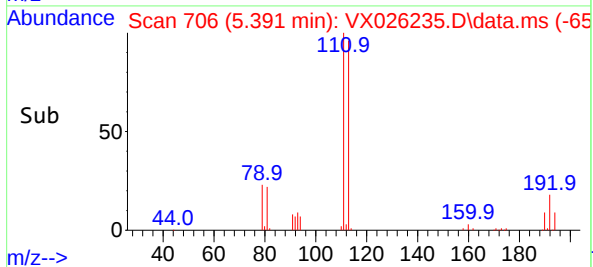
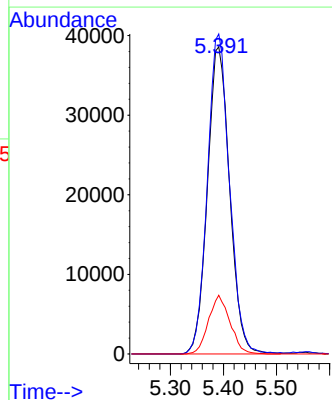
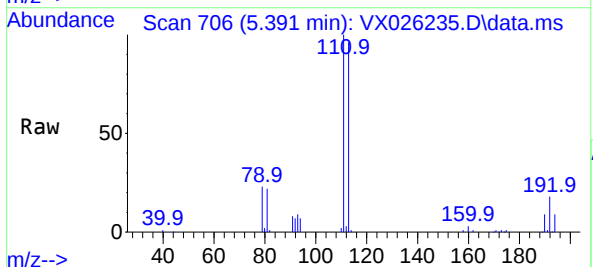


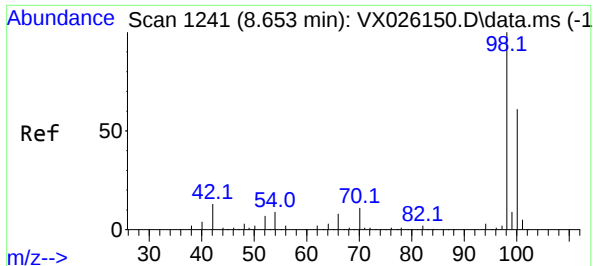

#50
Toluene-d8
Concen: 48.791 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX026235.D
Acq: 03 Jan 2022 21:01




Instrument :
MSVOA_X
ClientSampleId :
MW-2R


Tgt Ion: 98 Resp: 406055
Ion Ratio Lower Upper
98 100
100 65.1 52.6 78.8

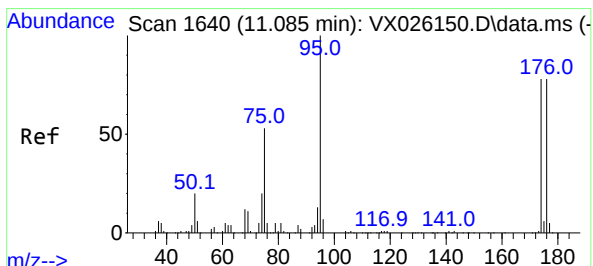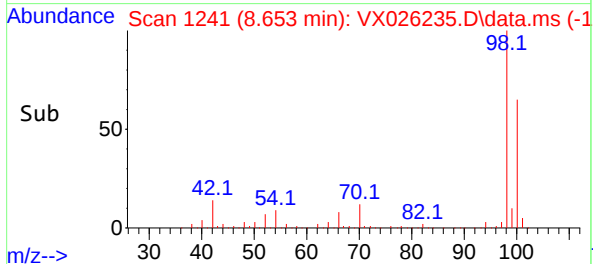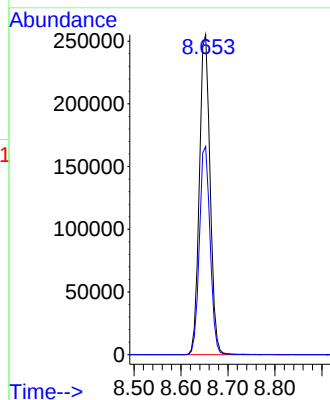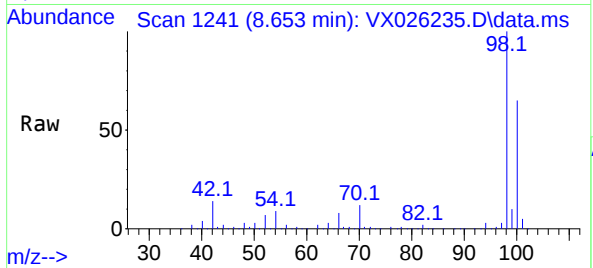

#62
4-Bromofluorobenzene
Concen: 47.878 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX026235.D
Acq: 03 Jan 2022 21:01

Tgt Ion: 95 Resp: 141846
Ion Ratio Lower Upper
95 100
174 73.2 0.0 157.4
176 70.3 0.0 154.6


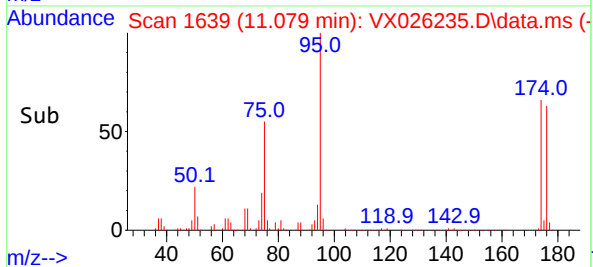
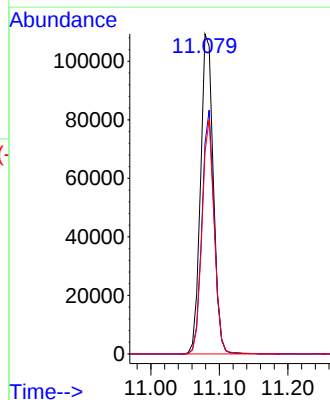
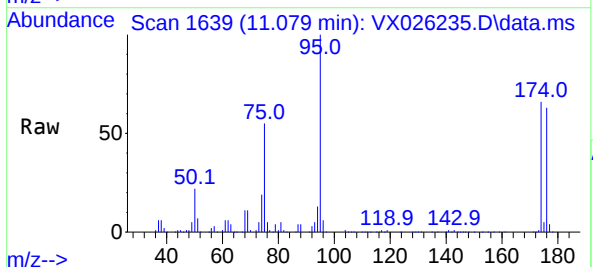


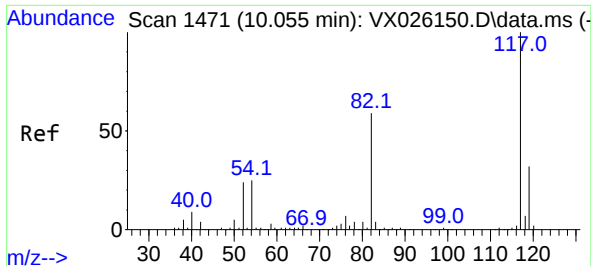

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026235.D
Acq: 03 Jan 2022 21:01

Instrument :
MSVOA_X
ClientSampleId :
MW-2R

Tgt Ion:117 Resp: 302088
Ion Ratio Lower Upper
117 100
82 57.7 43.8 65.6
119 31.9 25.2 37.8

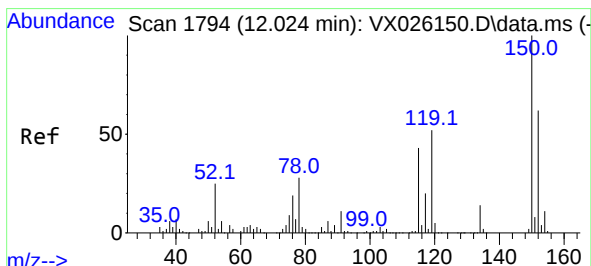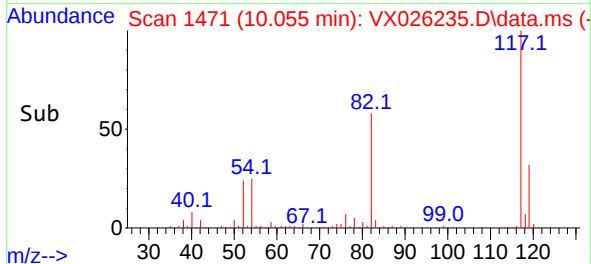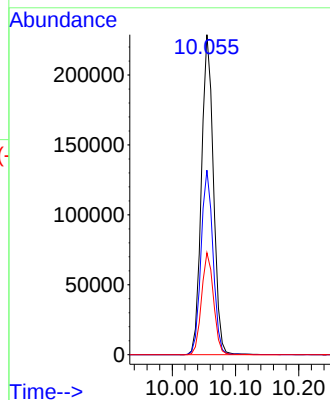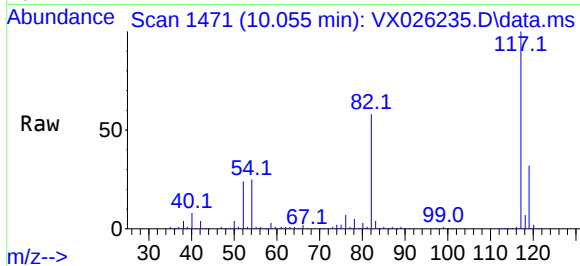

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX026235.D
Acq: 03 Jan 2022 21:01

Tgt Ion:152 Resp: 128032
Ion Ratio Lower Upper
152 100
115 60.9 41.3 123.9
150 156.2 0.0 351.8

