

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
 Data File : VX026229.D
 Acq On : 03 Jan 2022 18:42
 Operator : JC/MD
 Sample : M5328-10 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 20995

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M

Title : SW846 8260

Signal : TIC: VX026229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	72	rBV	324131	363140	33.84%	5.817%
2	2.050	152	158	169	rBV	20438	33850	3.15%	0.542%
3	2.294	192	198	207	rBV	60518	98790	9.21%	1.582%
4	2.380	207	212	224	rVB	8053	14317	1.33%	0.229%
5	4.562	560	570	585	rBV2	11754	35129	3.27%	0.563%
6	5.391	690	706	720	rBV	127718	369432	34.43%	5.917%
7	5.556	720	733	746	rVV2	214590	596804	55.62%	9.559%
8	5.958	787	799	812	rBV	149900	398639	37.15%	6.385%
9	6.763	919	931	944	rBV	341697	818078	76.24%	13.104%
10	8.647	1233	1240	1250	rBV	667020	1073054	100.00%	17.188%
11	10.055	1465	1471	1482	rBV	700511	929790	86.65%	14.893%
12	11.079	1634	1639	1653	rBV	537714	687071	64.03%	11.005%
13	12.024	1788	1794	1806	rBV	663946	825051	76.89%	13.215%




Sum of corrected areas: 6243145

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
Data File : VX026229.D
Acq On : 03 Jan 2022 18:42
Operator : JC/MD
Sample : M5328-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20995

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

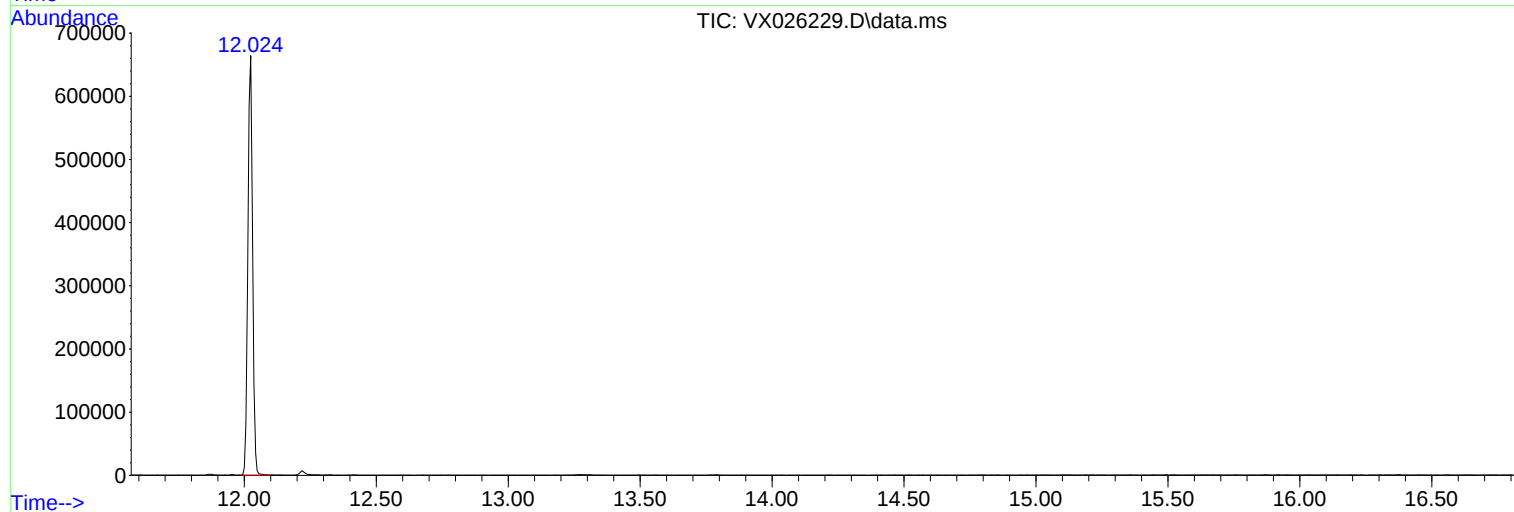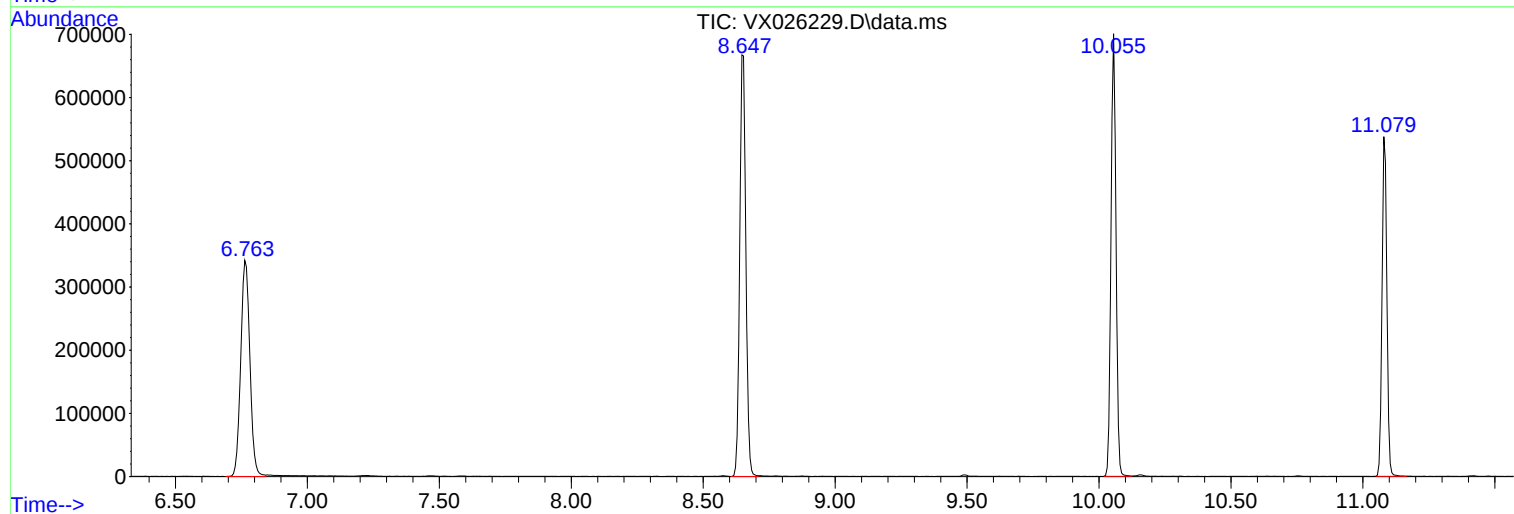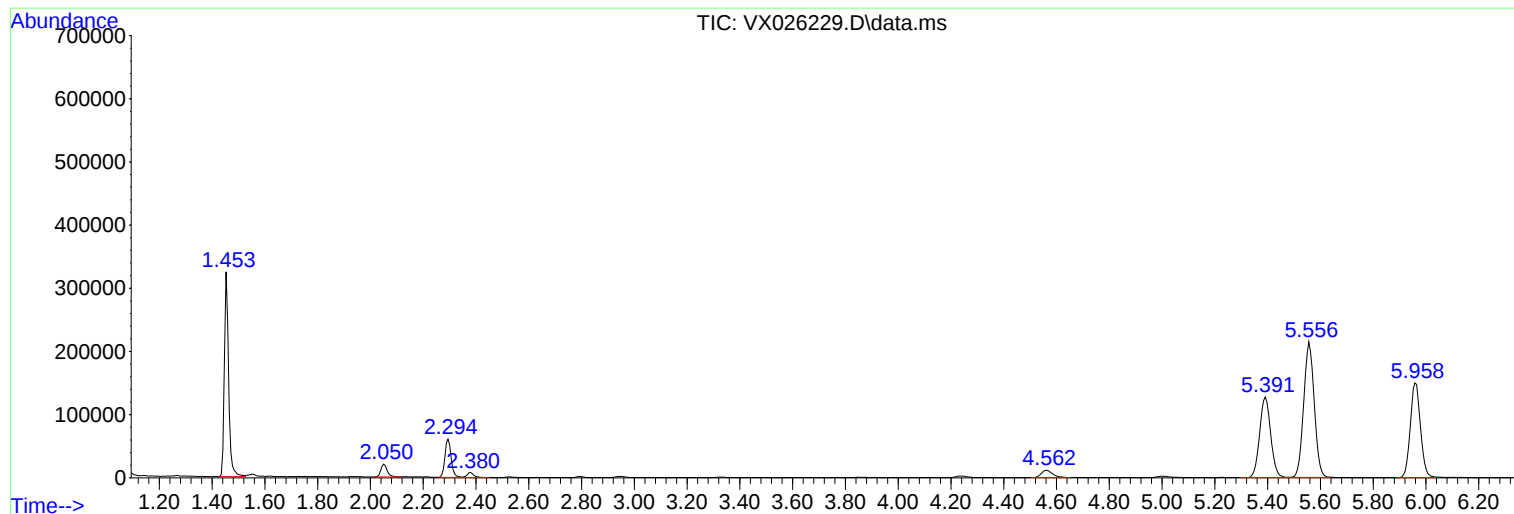

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
Data File : VX026229.D
Acq On : 03 Jan 2022 18:42
Operator : JC/MD
Sample : M5328-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20995










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propanal Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.294	8.28 ug/l	98790	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanal	58	C3H6O	000123-38-6	78
2			2-(Aminomethyl)-4-methylpentanoi...	187	C10H21NO2	1891211-54-3	9
3			Oxirane, methyl-, (S)-	58	C3H6O	016088-62-3	7
4			Propylene oxide	58	C3H6O	000075-56-9	7
5			Trimethylene oxide	58	C3H6O	000503-30-0	5

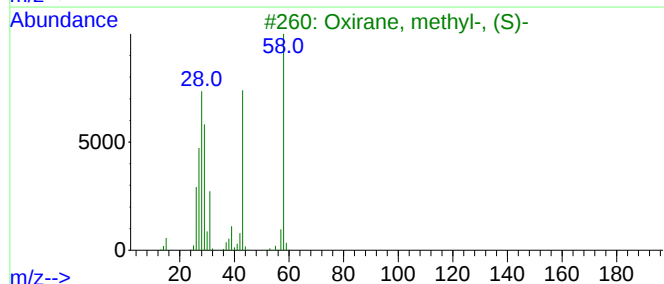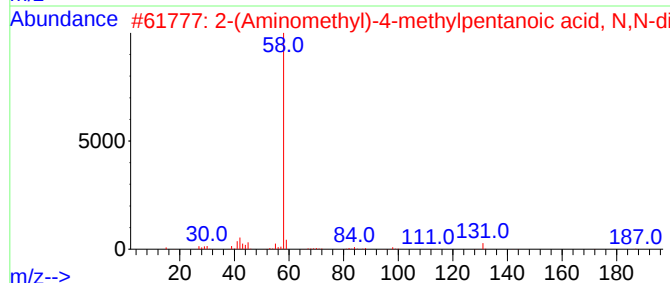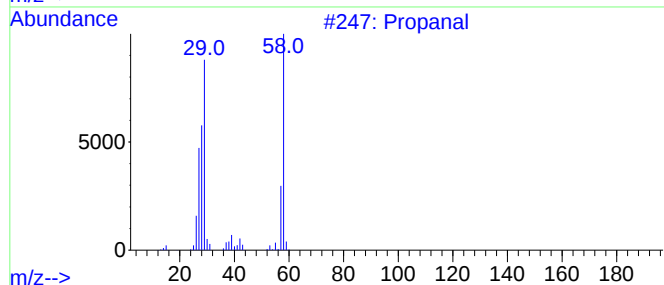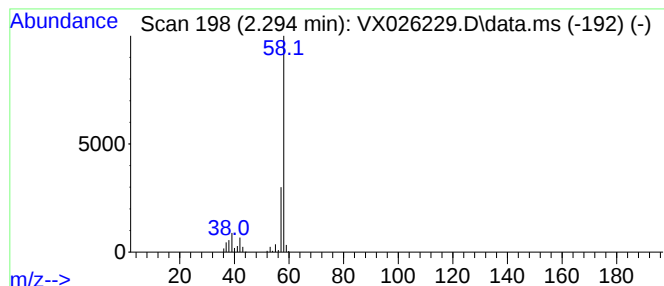

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
Data File : VX026229.D
Acq On : 03 Jan 2022 18:42
Operator : JC/MD
Sample : M5328-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20995

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propanal	2.294	8.3	ug/l	98790	1	5.556	596804	50.0