
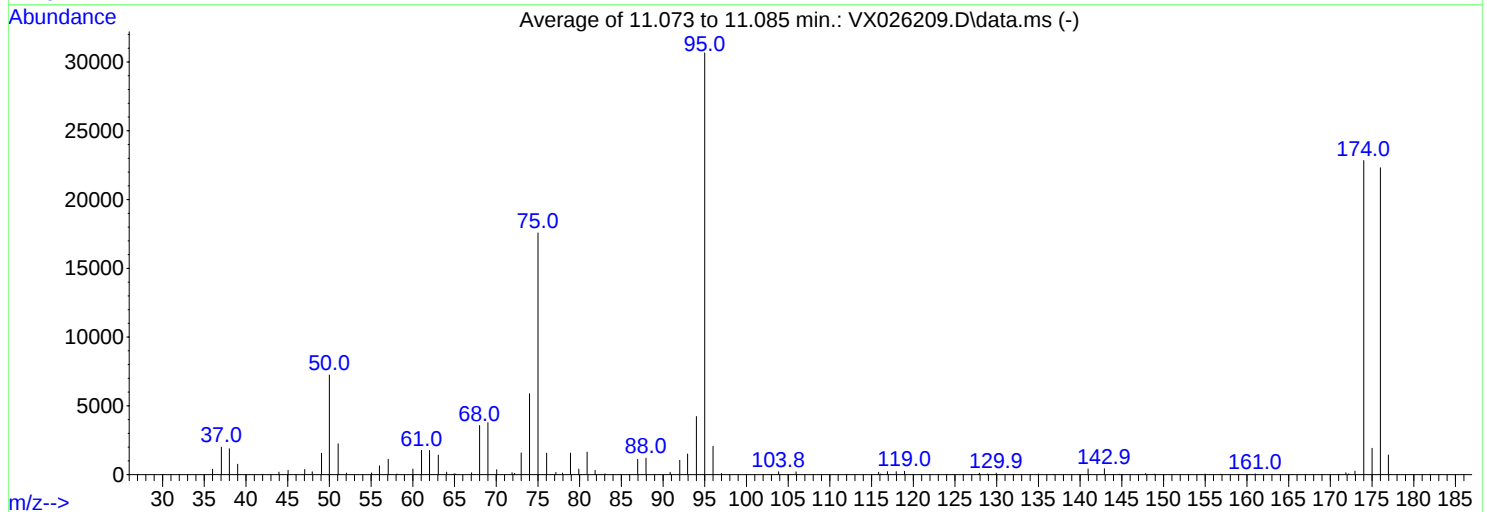


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010322\
 Data File : VX026209.D
 Acq On : 03 Jan 2022 09:47
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Title : SW846 8260
 Last Update : Thu Dec 30 08:02:21 2021

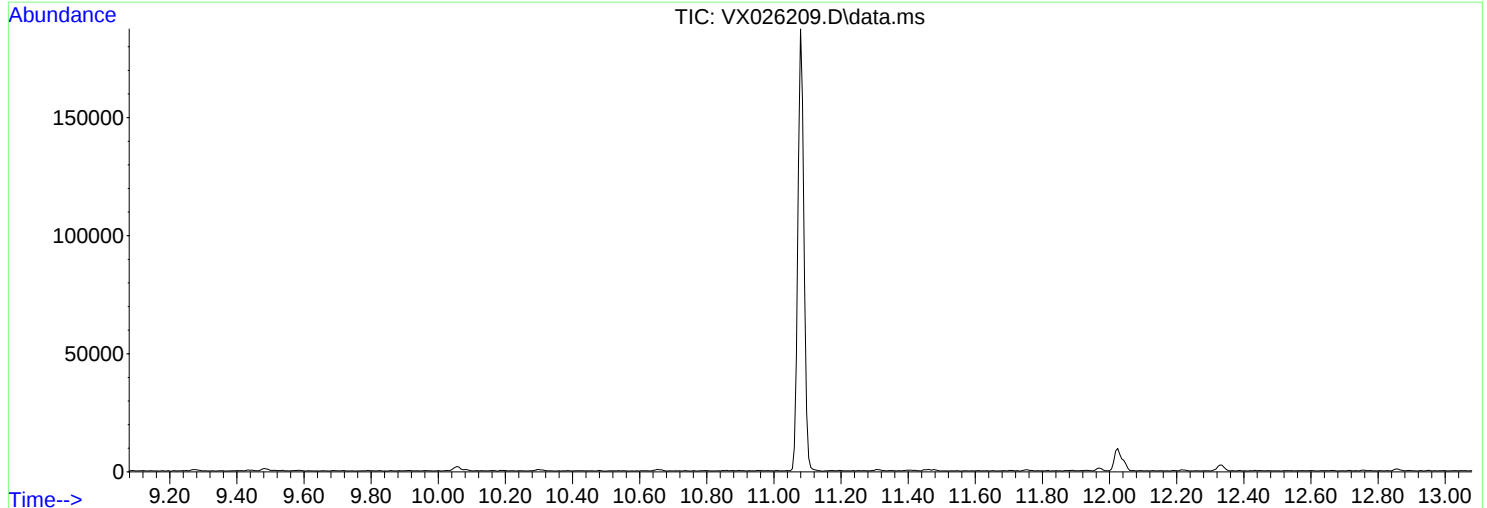

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	7251	PASS
75	95	30	60	57.3	17578	PASS
95	95	100	100	100.0	30669	PASS
96	95	5	9	6.7	2059	PASS
173	174	0.00	2	1.1	260	PASS
174	95	50	100	74.5	22834	PASS
175	174	5	9	8.4	1920	PASS
176	174	95	101	97.7	22317	PASS
177	176	5	9	6.4	1434	PASS