

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010422\
 Data File : VX026276.D
 Acq On : 04 Jan 2022 17:00
 Operator : JC/MD
 Sample : M5333-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FIELD-BLANK

Quant Time: Jan 05 07:29:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	149907	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	257606	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	226271	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	98077	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	116129	53.547	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 107.100%	
35) Dibromofluoromethane	5.391	113	84150	50.245	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.500%	
50) Toluene-d8	8.653	98	304984	48.958	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 97.920%	
62) 4-Bromofluorobenzene	11.079	95	113338	51.107	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 102.220%	
Target Compounds						
16) Acetone	2.379	43	3611	3.073	ug/l	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010422\
Data File : VX026276.D
Acq On : 04 Jan 2022 17:00
Operator : JC/MD
Sample : M5333-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANK

Quant Time: Jan 05 07:29:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration




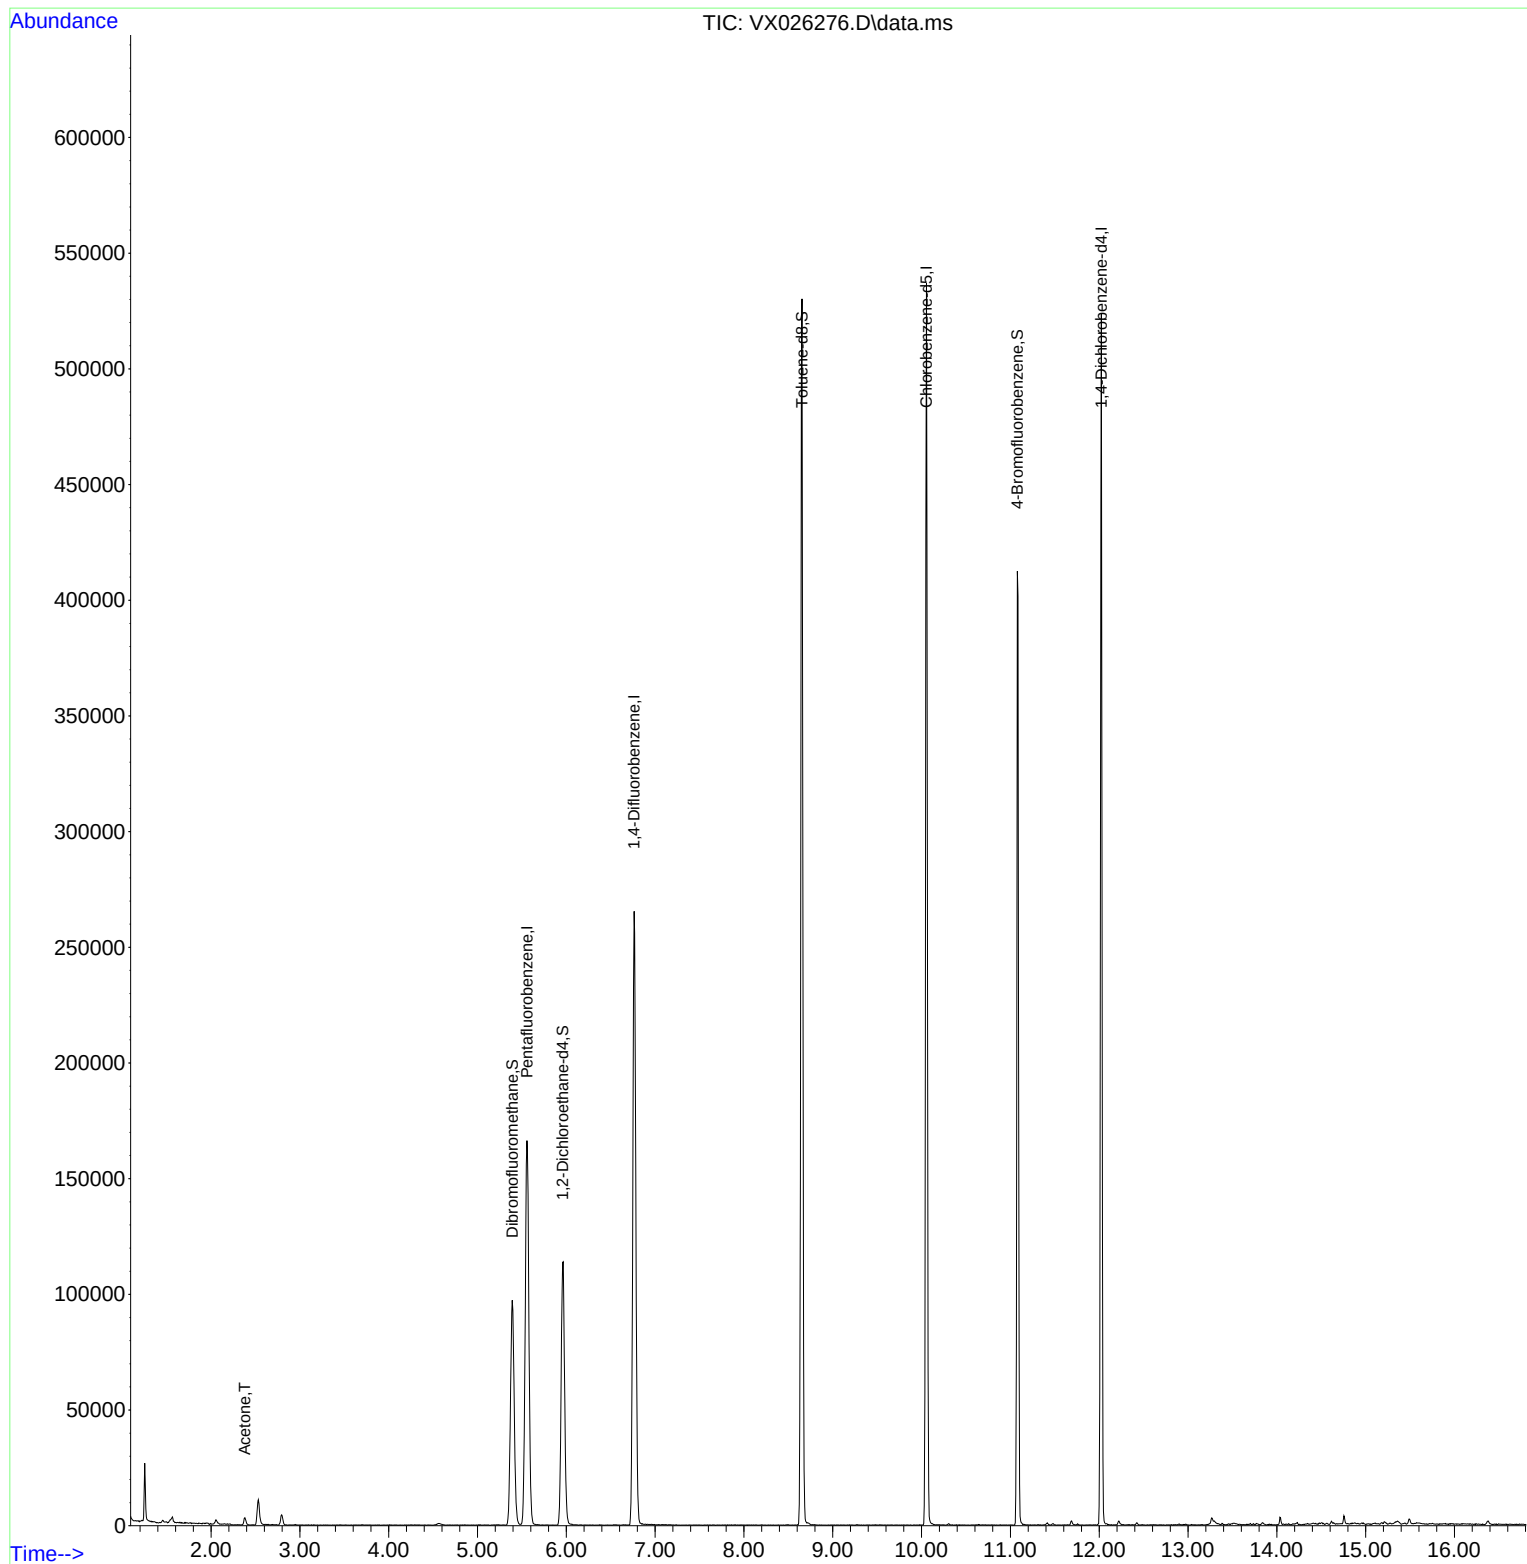


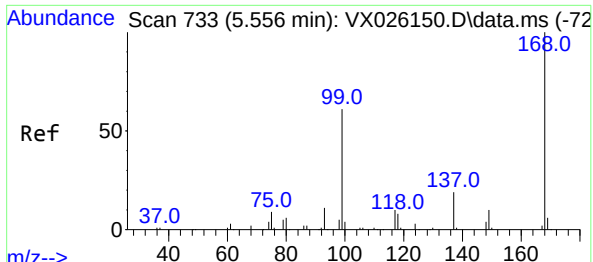

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026276.D
Acq: 04 Jan 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANK


Tgt Ion:168 Resp: 149907
Ion Ratio Lower Upper
168 100
99 65.8 45.8 68.8

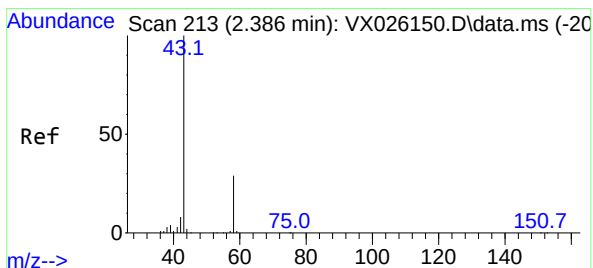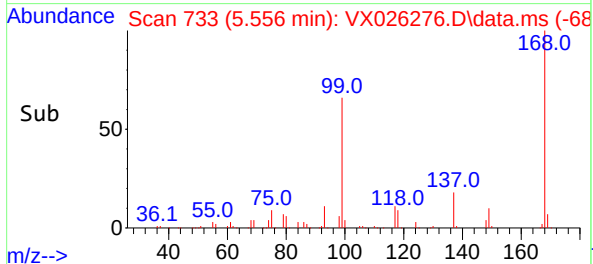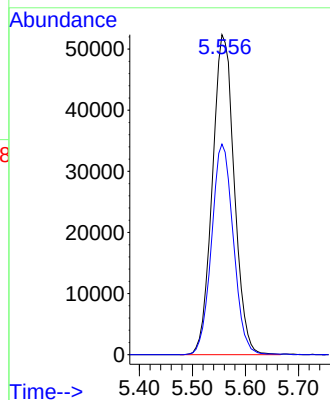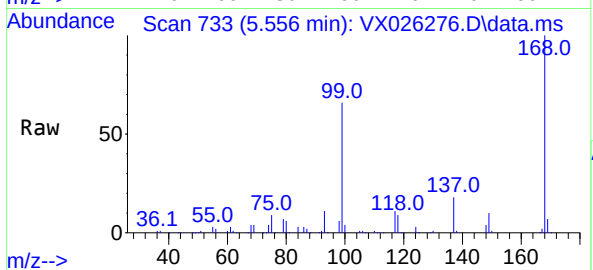

#16
Acetone
Concen: 3.073 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.007 min
Lab File: VX026276.D
Acq: 04 Jan 2022 17:00

Tgt Ion: 43 Resp: 3611
Ion Ratio Lower Upper
43 100
58 27.6 24.8 37.2

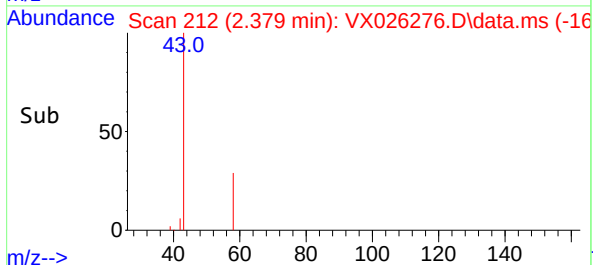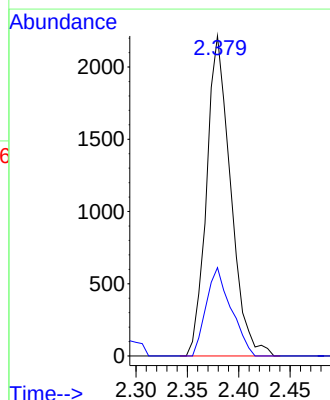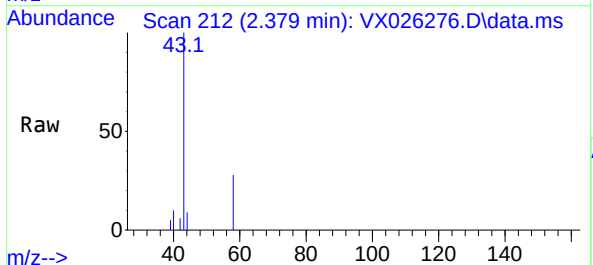

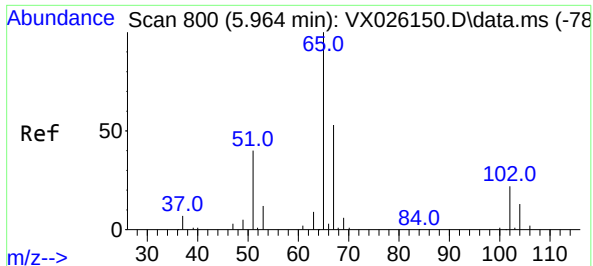

#33

1,2-Dichloroethane-d4

Concen: 53.547 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX026276.D

Acq: 04 Jan 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :





FIELD-BLANK

Tgt Ion: 65 Resp: 116129

Ion Ratio Lower Upper

65 100

67 49.1 0.0 103.4

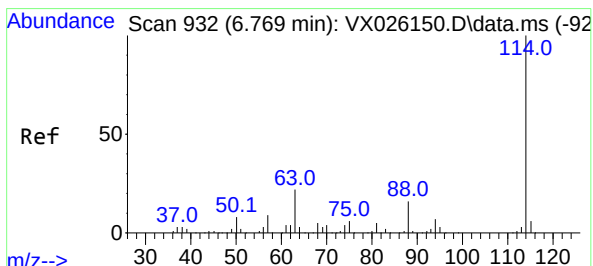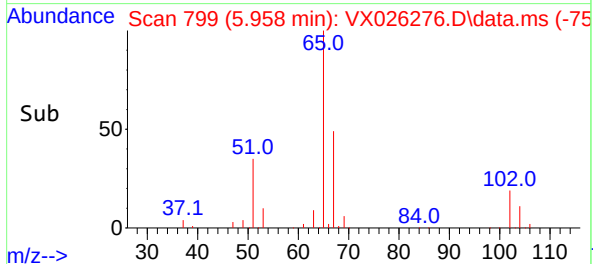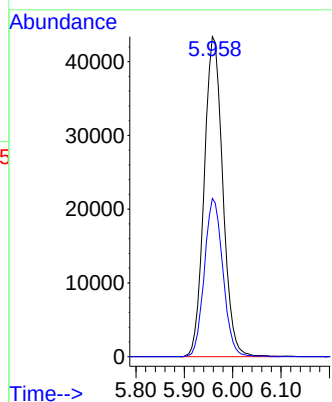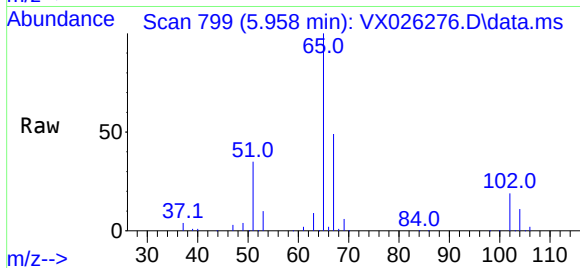

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX026276.D

Acq: 04 Jan 2022 17:00




Tgt Ion: 114 Resp: 257606


Ion Ratio Lower Upper

114 100

63 22.3 0.0 40.0

88 16.9 0.0 30.6

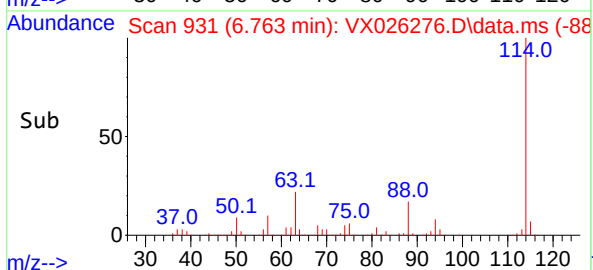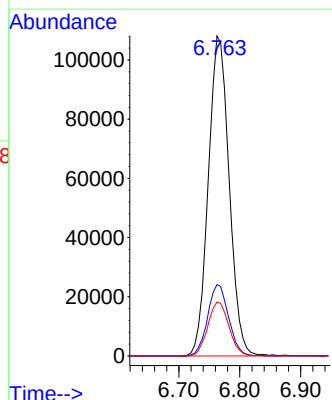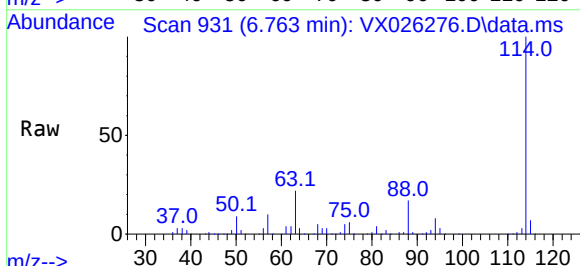

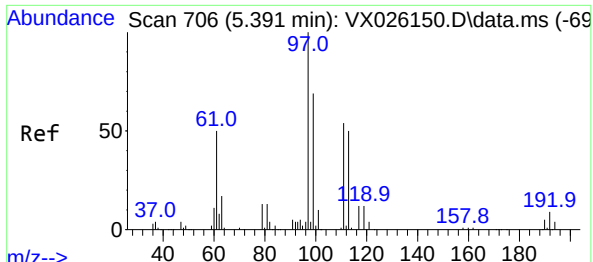

#35

Dibromofluoromethane

Concen: 50.245 ug/l

RT: 5.391 min Scan# 706

Delta R.T. -0.000 min

Lab File: VX026276.D


Acq: 04 Jan 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :

FIELD-BLANK

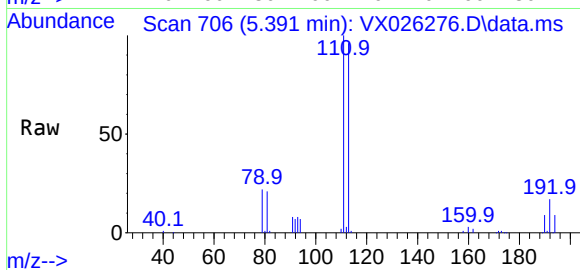




Tgt Ion:113 Resp: 84150

Ion Ratio Lower Upper

113 100

111 102.7 81.8 122.8

192 18.5 15.0 22.4

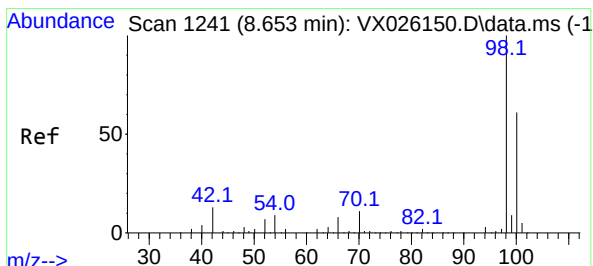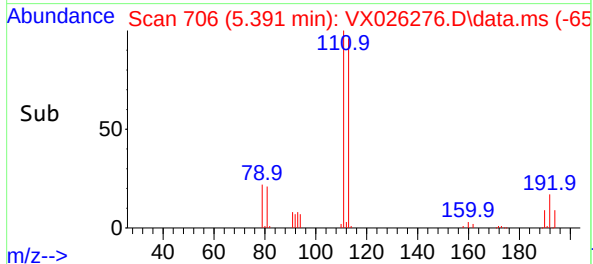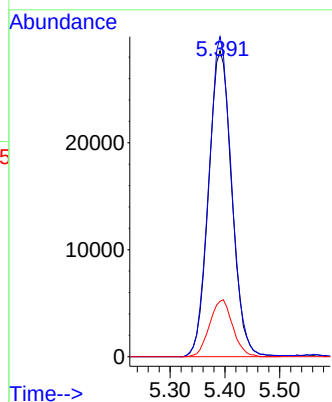

#50

Toluene-d8

Concen: 48.958 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX026276.D




Acq: 04 Jan 2022 17:00


Tgt Ion: 98 Resp: 304984

Ion Ratio Lower Upper

98 100

100 65.4 52.6 78.8


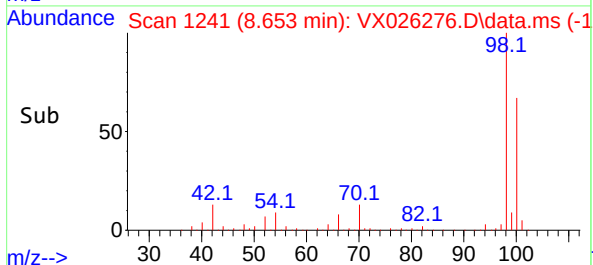
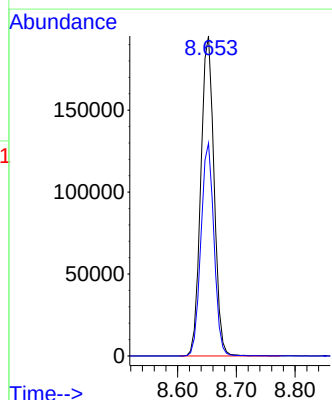
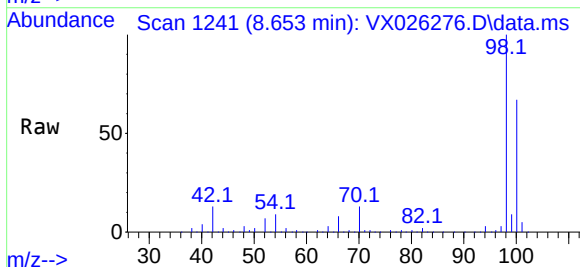


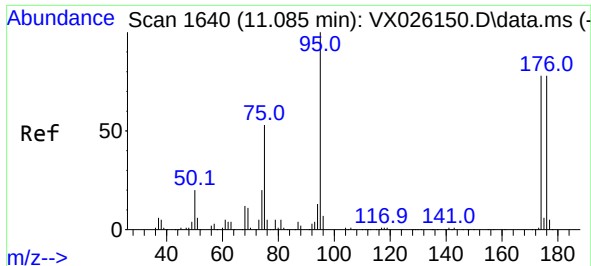

#62
4-Bromofluorobenzene
Concen: 51.107 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX026276.D
Acq: 04 Jan 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANK


Tgt Ion: 95 Resp: 113338
Ion Ratio Lower Upper
95 100
174 70.8 0.0 157.4
176 68.5 0.0 154.6

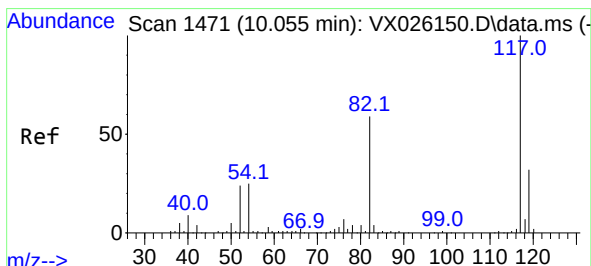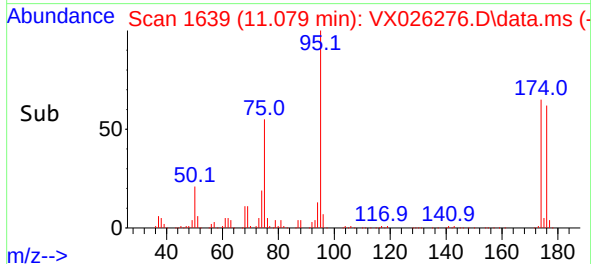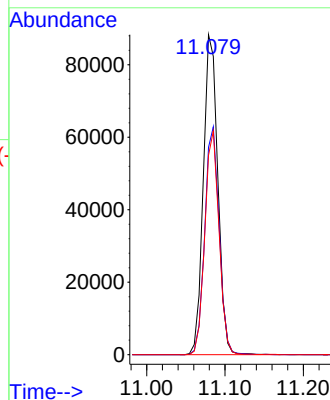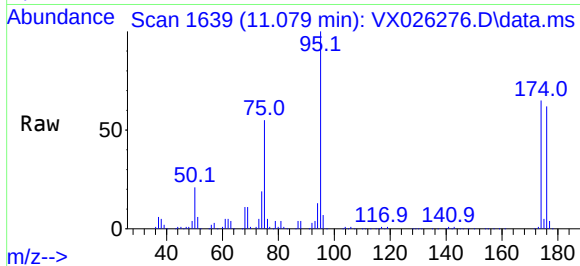

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026276.D
Acq: 04 Jan 2022 17:00

Tgt Ion: 117 Resp: 226271
Ion Ratio Lower Upper
117 100
82 59.4 43.8 65.6
119 32.8 25.2 37.8

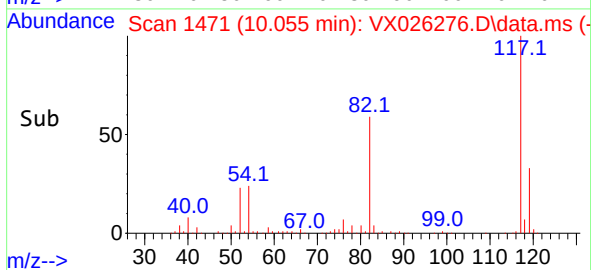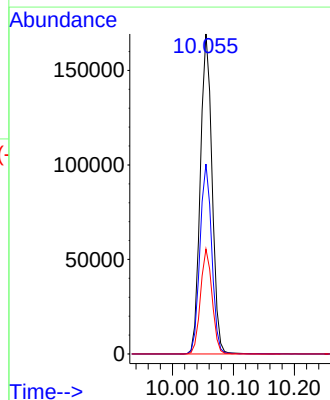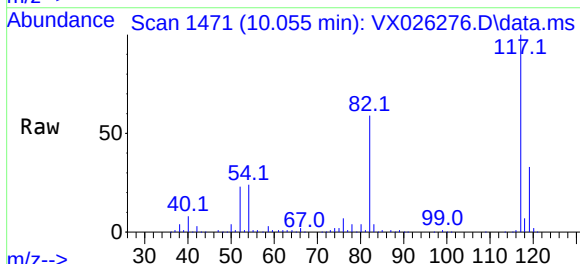

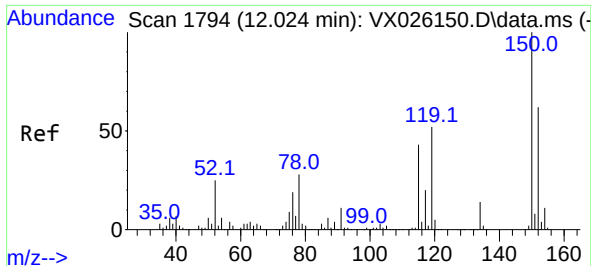

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX026276.D


Acq: 04 Jan 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :

FIELD-BLANK

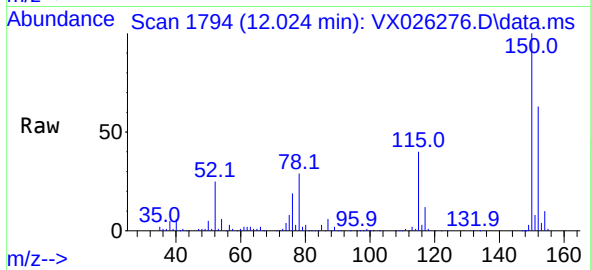

Tgt Ion:152 Resp: 98077

Ion Ratio Lower Upper

152 100

115 63.3 41.3 123.9

150 158.3 0.0 351.8

