

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010422\
 Data File : VX026284.D
 Acq On : 04 Jan 2022 20:28
 Operator : JC/MD
 Sample : N1005-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WANA-SB

Quant Time: Jan 05 06:16:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 01/05/2022
 Supervised By : Mahesh Dadoda 01/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	162481	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	6.775	114	273627	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	243083	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.030	152	120556	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.983	65	115437	49.109	ug/l	0.02
Spiked Amount 50.000	Range 78 - 117		Recovery =	98.220%		
35) Dibromofluoromethane	5.410	113	73669	41.412	ug/l	0.02
Spiked Amount 50.000	Range 75 - 124		Recovery =	82.820%		
50) Toluene-d8	8.665	98	322769	48.779	ug/l	0.01
Spiked Amount 50.000	Range 92 - 112		Recovery =	97.560%		
62) 4-Bromofluorobenzene	11.085	95	124374	52.800	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	105.600%		
Target Compounds					Qvalue	
8) Diethyl Ether	2.136	74	927737	749.929	ug/l	99
11) Tert butyl alcohol	2.983	59	1820127	3876.766	ug/l #	64
16) Acetone	2.386	43	7403636	5813.149	ug/l	99
17) Carbon Disulfide	2.514	76	9551	1.850	ug/l #	93
18) Methyl Acetate	2.709	43	689986	167.022	ug/l	98
19) Methyl tert-butyl Ether	3.123	73	2012250	320.195	ug/l	93
20) Methylene Chloride	2.800	84	8793	3.438	ug/l #	90
25) 2-Butanone	4.574	43	1744374	983.232	ug/l	97
29) Tetrahydrofuran	5.026	42	56752	50.752	ug/l	88
31) Cyclohexane	5.483	56	107806	32.205	ug/l	94
39) Methylcyclohexane	7.391	83	106519	32.911	ug/l	96
40) Benzene	6.068	78	12195041	1489.226	ug/l	91
43) Isopropyl Acetate	6.348	43	482897	89.061	ug/l #	77
52) Toluene	8.763	92	19939661	3955.299	ug/l #	72
67) Ethyl Benzene	10.201	91	4560980	477.680	ug/l	96
68) m/p-Xylenes	10.323	106	8271535	2320.142	ug/l	79
69) o-Xylene	10.653	106	3364481	964.528	ug/l	91
73) Isopropylbenzene	10.970	105	609017	64.991	ug/l	98
78) n-propylbenzene	11.305	91	437300m	40.588	ug/l	
80) 1,3,5-Trimethylbenzene	11.457	105	1501182	193.039	ug/l	98
84) 1,2,4-Trimethylbenzene	11.756	105	3257333	419.201	ug/l	98
85) sec-Butylbenzene	11.896	105	148346	15.749	ug/l	87
86) p-Isopropyltoluene	12.018	119	186888m	23.800	ug/l	
89) n-Butylbenzene	12.323	91	255002	36.541	ug/l #	17
95) Naphthalene	13.780	128	622833	66.846	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010422\
Data File : VX026284.D
Acq On : 04 Jan 2022 20:28
Operator : JC/MD
Sample : N1005-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
WANA-SB

Quant Time: Jan 05 06:16:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : John Carlone 01/05/2022
Supervised By : Mahesh Dadoda 01/05/2022

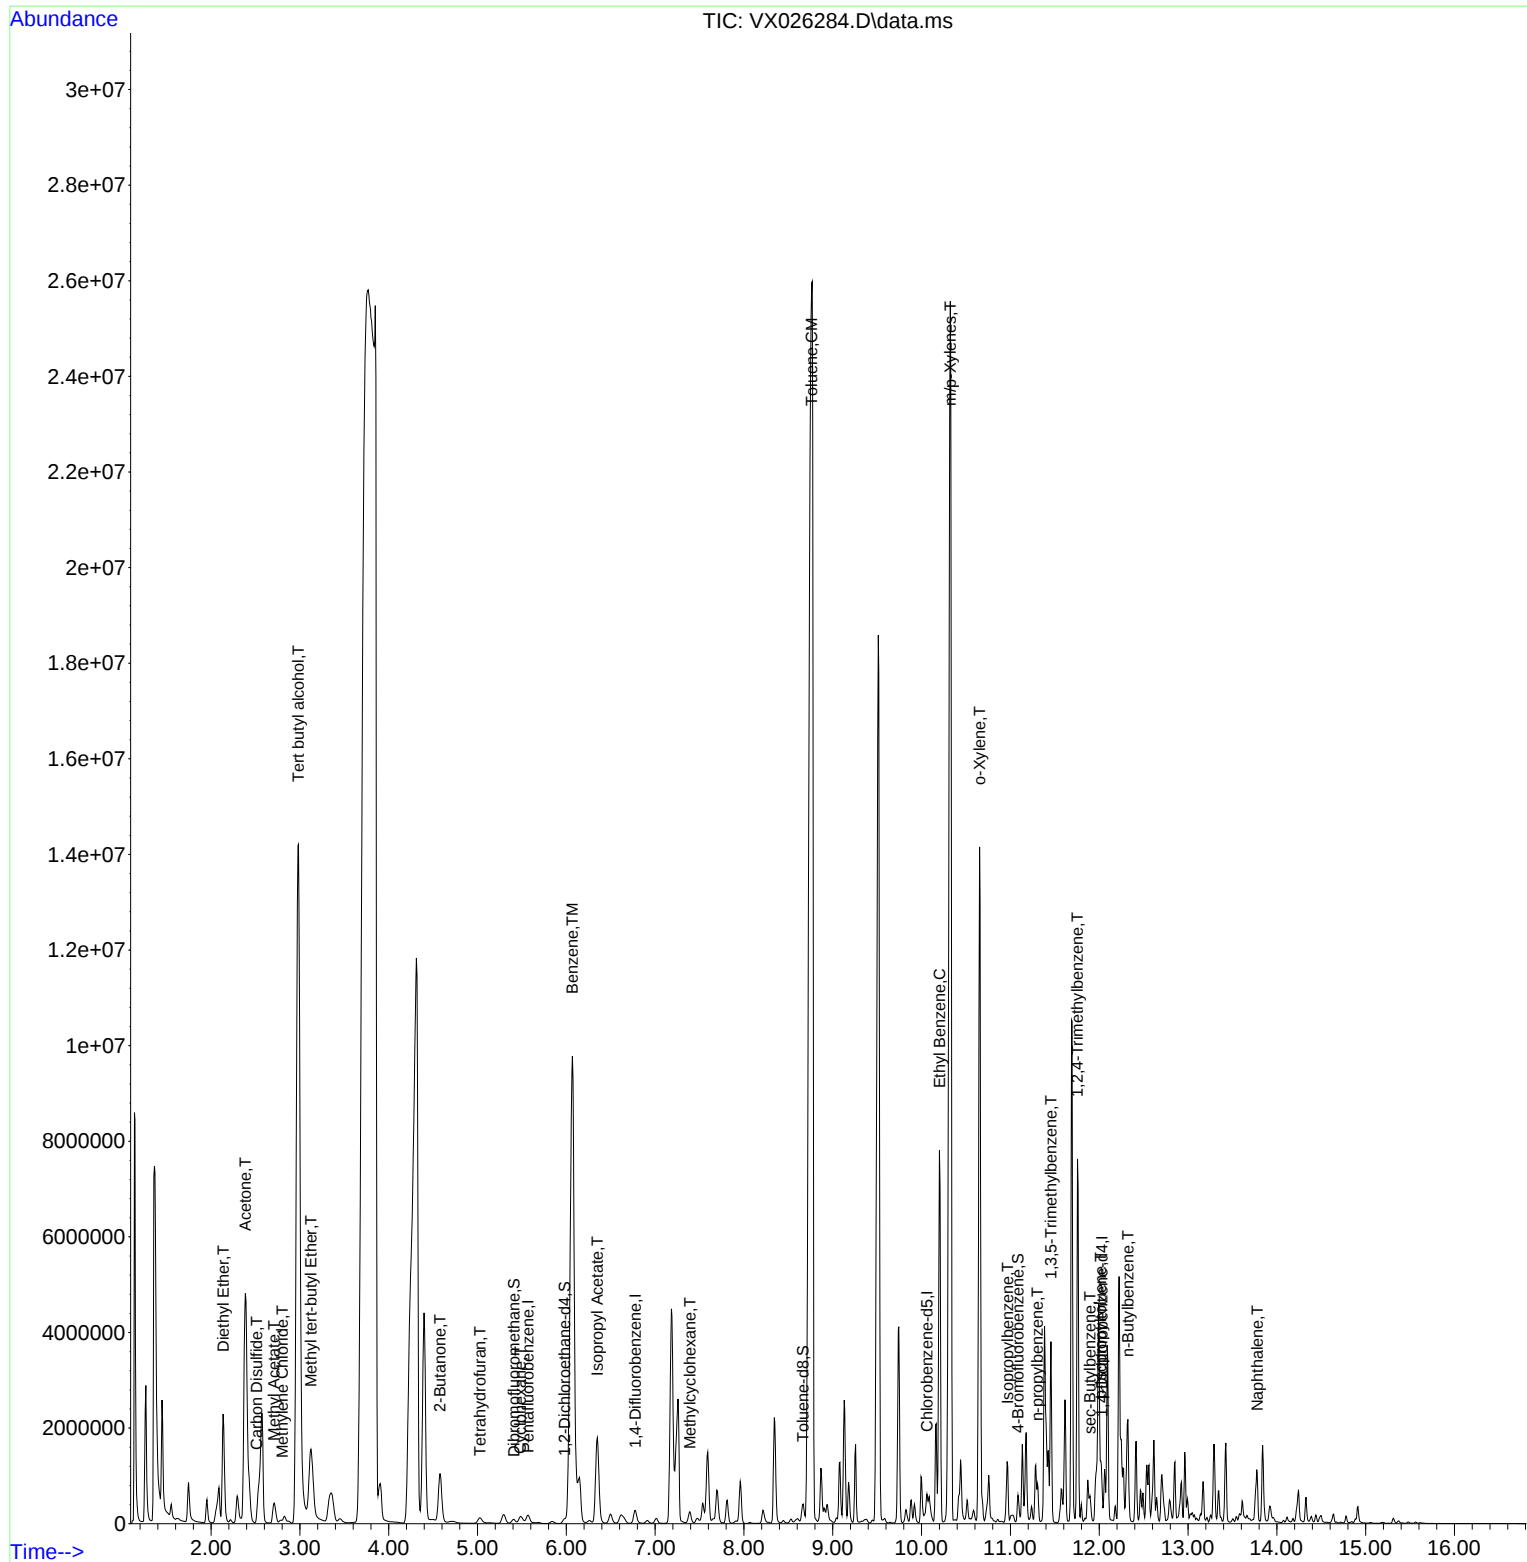

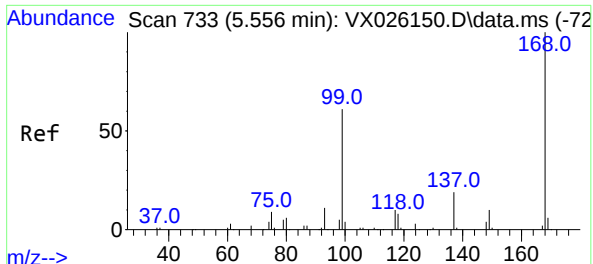

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.012 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB

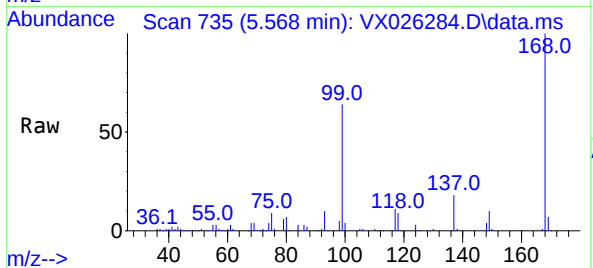


Tgt Ion:168 Resp: 16248
Ion Ratio Lower Upper
168 100
99 64.0 45.8 68.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

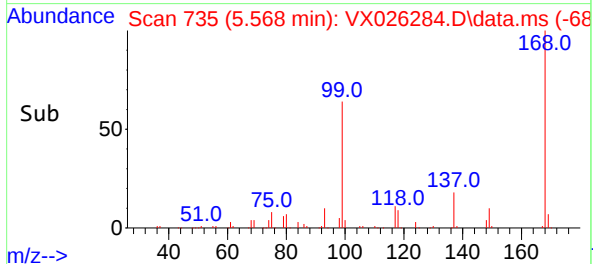


#8
Diethyl Ether
Concen: 749.929 ug/l
RT: 2.136 min Scan# 172
Delta R.T. -0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28

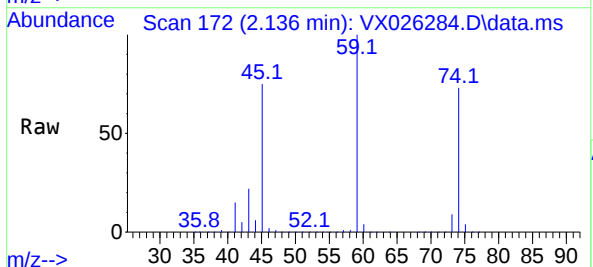


Tgt Ion: 74 Resp: 927737
Ion Ratio Lower Upper
74 100
45 99.6 50.4 151.2

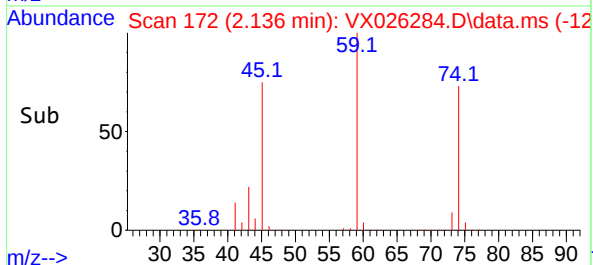



#11
Tert butyl alcohol
Concen: 3876.766 ug/l
RT: 2.983 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB



Tgt Ion: 59 Resp: 182012
Ion Ratio Lower Upper
59 100
57 23.4 8.2 12.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022



#16
Acetone
Concen: 5813.149 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28


Tgt Ion: 43 Resp: 7403636
Ion Ratio Lower Upper
43 100
58 31.5 24.8 37.2

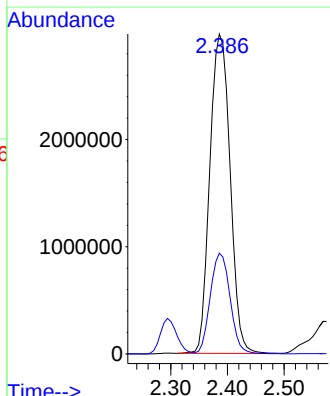



#17
Carbon Disulfide
Concen: 1.850 ug/l
RT: 2.514 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB




Tgt Ion: 76 Resp: 955
Ion Ratio Lower Upper
76 100
78 6.4 7.2 10.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

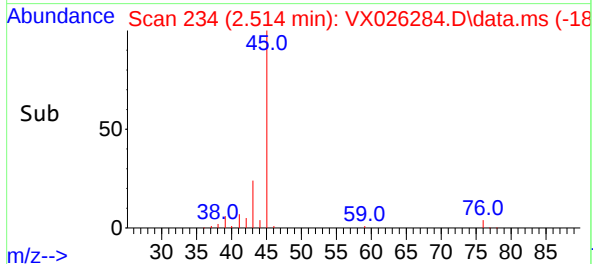


#18
Methyl Acetate
Concen: 167.022 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28

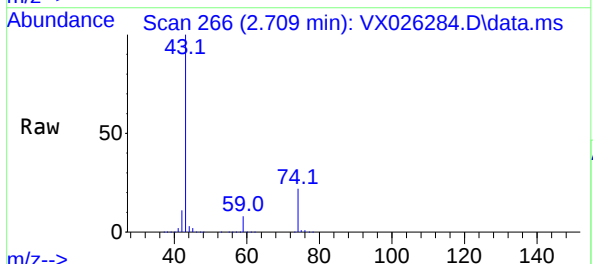


Tgt Ion: 43 Resp: 689986
Ion Ratio Lower Upper
43 100
74 22.7 19.1 28.7

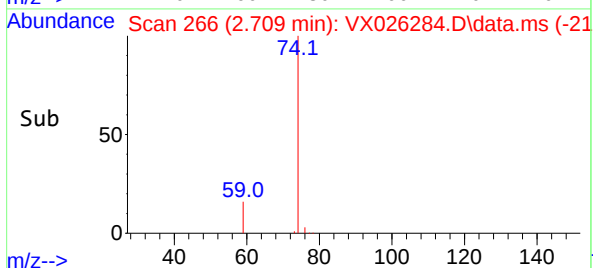



#19
Methyl tert-butyl Ether
Concen: 320.195 ug/l
RT: 3.123 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB



Tgt Ion: 73 Resp: 2012250
Ion Ratio Lower Upper
73 100
57 24.7 17.0 25.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

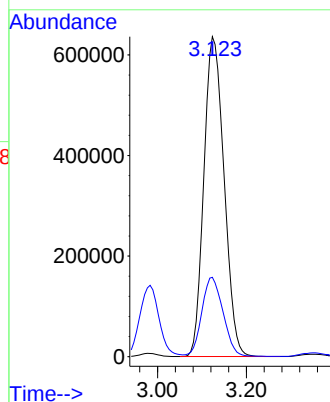

#20
Methylene Chloride
Concen: 3.438 ug/l
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28

Tgt Ion: 84 Resp: 8793
Ion Ratio Lower Upper
84 100
49 117.8 97.1 145.7
51 44.4 29.3 43.9#
86 80.7 50.8 76.2#





#25

2-Butanone

Concen: 983.232 ug/l

RT: 4.574 min Scan# 51

Delta R.T. 0.012 min

Lab File: VX026284.D

Acq: 04 Jan 2022 20:28

Instrument :

MSVOA_X

ClientSampleId :

WANA-SB

Tgt Ion: 43 Resp: 1744374

Ion Ratio Lower Upper

43 100





72 24.9 21.0 31.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/05/2022

Supervised By :Mahesh Dadoda 01/05/2022

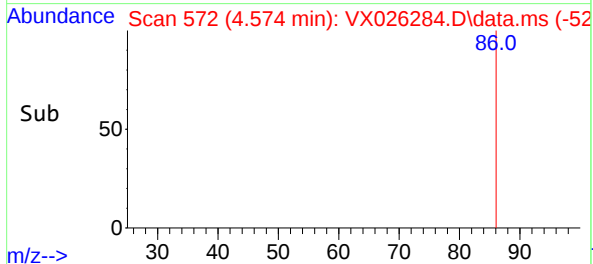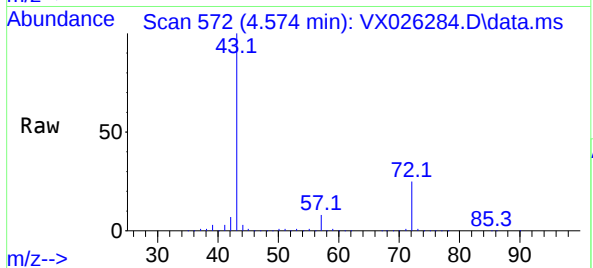

#29

Tetrahydrofuran

Concen: 50.752 ug/l

RT: 5.026 min Scan# 646

Delta R.T. 0.013 min

Lab File: VX026284.D

Acq: 04 Jan 2022 20:28




Tgt Ion: 42 Resp: 56752


Ion Ratio Lower Upper

42 100

72 38.6 37.0 55.6


71 34.3 34.1 51.1

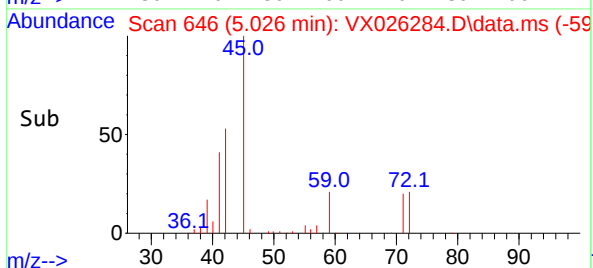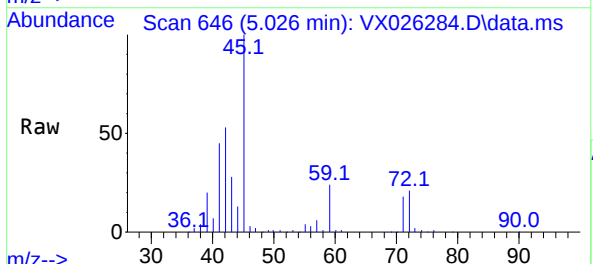



#31
Cyclohexane
Concen: 32.205 ug/l
RT: 5.483 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB




Tgt Ion: 56 Resp: 107800
Ion Ratio Lower Upper
56 100
69 30.7 23.9 35.9
84 84.7 73.2 109.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

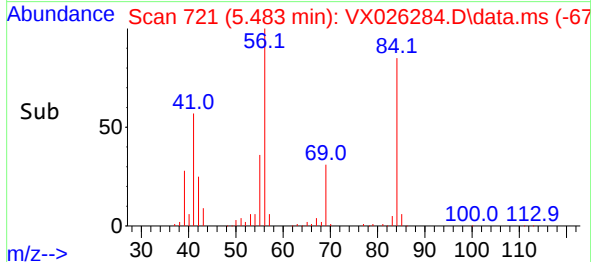


#33
1,2-Dichloroethane-d4
Concen: 49.109 ug/l
RT: 5.983 min Scan# 803
Delta R.T. 0.019 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Tgt Ion: 65 Resp: 115437
Ion Ratio Lower Upper
65 100
67 50.0 0.0 103.4





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.775 min Scan# 911
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB

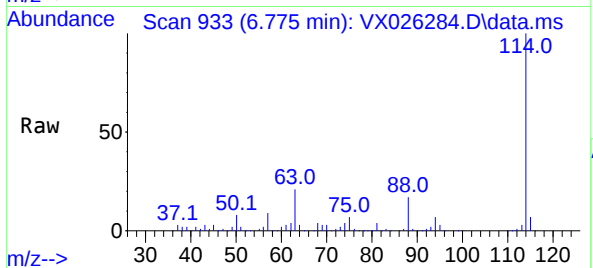


Tgt Ion:114 Resp: 27362
Ion Ratio Lower Upper
114 100
63 21.3 0.0 40.0
88 16.9 0.0 30.6

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

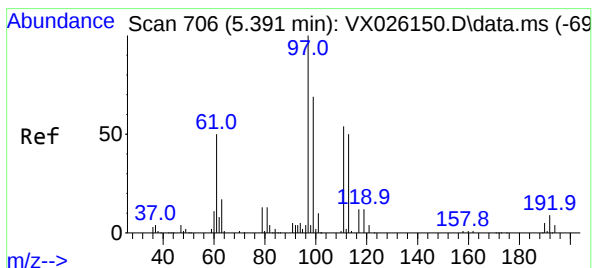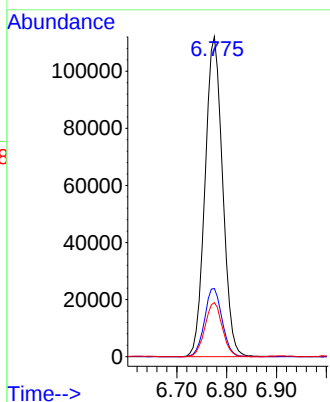


#35
Dibromofluoromethane
Concen: 41.412 ug/l
RT: 5.410 min Scan# 709
Delta R.T. 0.019 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28

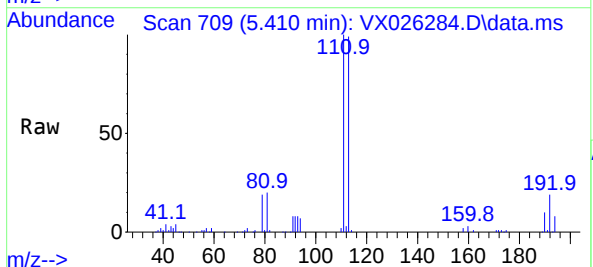

Tgt Ion:113 Resp: 73669
Ion Ratio Lower Upper
113 100
111 103.5 81.8 122.8
192 19.3 15.0 22.4

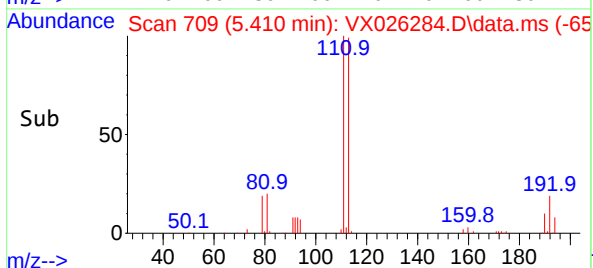



#39

Methylcyclohexane

Concen: 32.911 ug/l

RT: 7.391 min Scan# 1033

Delta R.T. 0.006 min

Lab File: VX026284.D

Acq: 04 Jan 2022 20:28

Instrument :

MSVOA_X

ClientSampleId :

WANA-SB

Tgt Ion: 83 Resp: 106519

Ion Ratio Lower Upper

83 100

55 77.8 57.8 86.8





98 50.1 40.5 60.7

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/05/2022

Supervised By :Mahesh Dadoda 01/05/2022

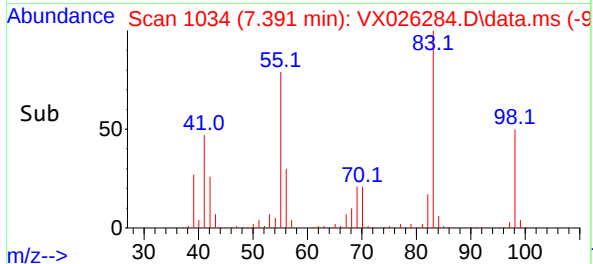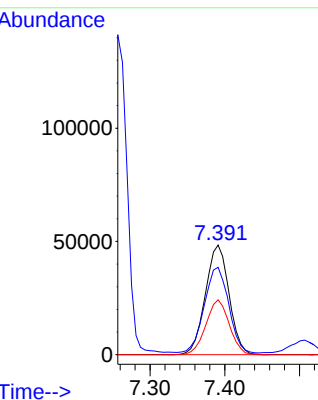

#40

Benzene

Concen: 1489.226 ug/l

RT: 6.068 min Scan# 817

Delta R.T. 0.024 min

Lab File: VX026284.D




Acq: 04 Jan 2022 20:28


Tgt Ion: 78 Resp:12195041

Ion Ratio Lower Upper

78 100


77 27.7 18.6 27.8

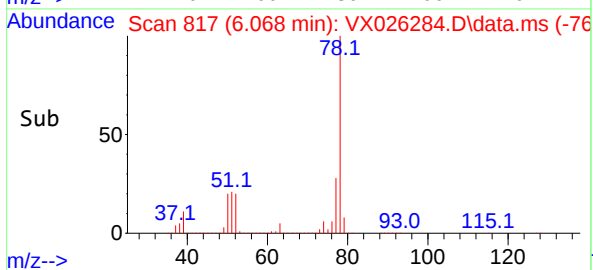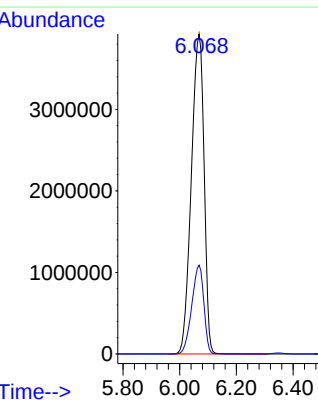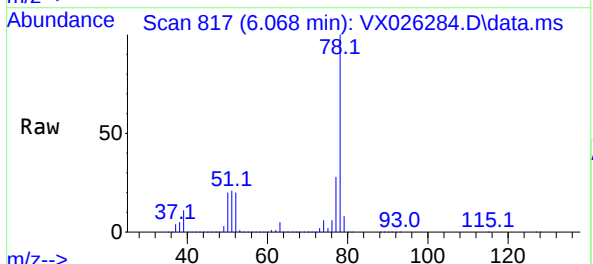



#43
Isopropyl Acetate
Concen: 89.061 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB




Tgt Ion: 43 Resp: 482897
Ion Ratio Lower Upper
43 100
61 11.5 15.7 23.5
87 2.0 11.2 16.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022




#50
Toluene-d8
Concen: 48.779 ug/l
RT: 8.665 min Scan# 1243
Delta R.T. 0.012 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Tgt Ion: 98 Resp: 322769
Ion Ratio Lower Upper
98 100
100 65.2 52.6 78.8





#52
Toluene
Concen: 3955.299 ug/l
RT: 8.763 min Scan# 1252
Delta R.T. 0.043 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB




Tgt Ion: 92 Resp: 1993966
Ion Ratio Lower Upper
92 100
91 131.6 136.0 204.0

Manual Integrations
APPROVED



Reviewed By : John Carlone 01/05/2022
Supervised By : Mahesh Dadoda 01/05/2022




#62
4-Bromofluorobenzene
Concen: 52.800 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28



Tgt Ion: 95 Resp: 124374
Ion Ratio Lower Upper
95 100
174 73.2 0.0 157.4
176 70.1 0.0 154.6









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28

Instrument :
MSVOA_X
ClientSampleId :
WANA-SB

Tgt Ion:117 Resp: 243083
Ion Ratio Lower Upper
117 100
82 56.2 43.8 65.6
119 32.0 25.2 37.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

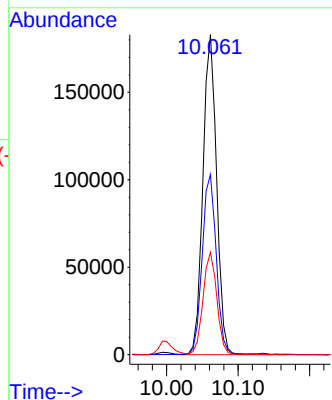

#67
Ethyl Benzene
Concen: 477.680 ug/l
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28


Tgt Ion: 91 Resp: 4560980
Ion Ratio Lower Upper
91 100
106 34.1 25.7 38.5

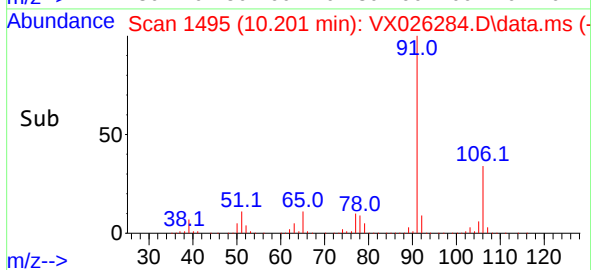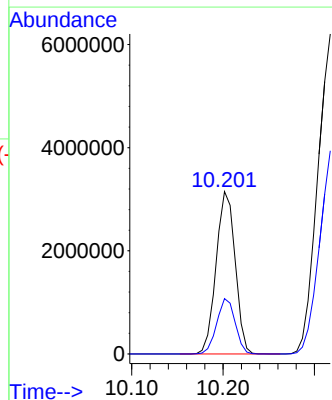



#68
m/p-Xylenes
Concen: 2320.142 ug/l
RT: 10.323 min Scan# 1512
Delta R.T. 0.018 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB

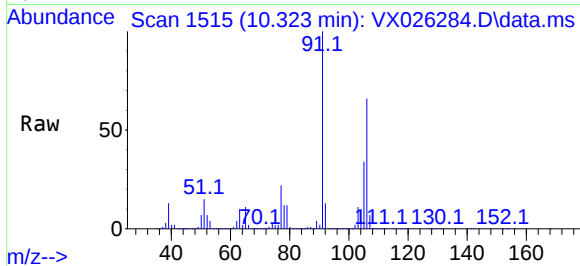


Tgt Ion:106 Resp: 827153
Ion Ratio Lower Upper
106 100
91 166.3 158.6 238.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022




#69
o-Xylene
Concen: 964.528 ug/l
RT: 10.653 min Scan# 1569
Delta R.T. 0.007 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28

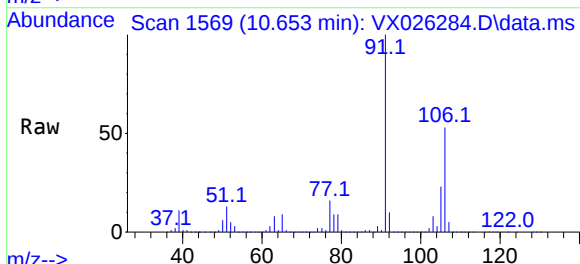


Tgt Ion:106 Resp: 3364481
Ion Ratio Lower Upper
106 100
91 197.3 105.5 316.4





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.030 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB




Tgt Ion:152 Resp: 120550
Ion Ratio Lower Upper
152 100
115 71.8 41.3 123.9
150 175.1 0.0 351.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

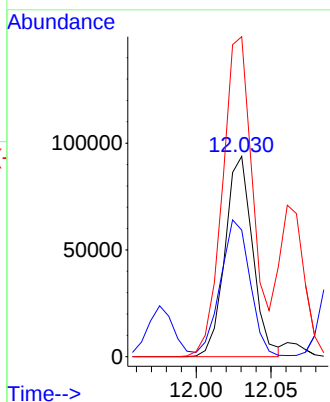


#73
Isopropylbenzene
Concen: 64.991 ug/l
RT: 10.970 min Scan# 1621
Delta R.T. 0.007 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Tgt Ion:105 Resp: 609017
Ion Ratio Lower Upper
105 100
120 26.1 13.6 40.7





#78
n-propylbenzene
Concen: 40.588 ug/l m
RT: 11.305 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB

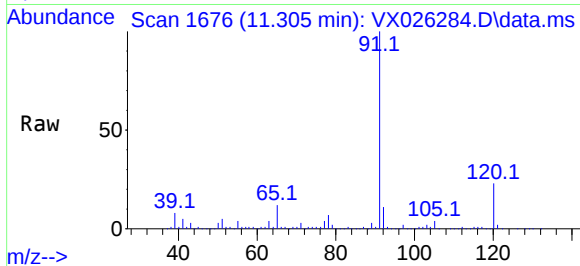


Tgt Ion: 91 Resp: 437300
Ion Ratio Lower Upper
91 100
120 0.0 12.0 36.1

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022




#80
1,3,5-Trimethylbenzene
Concen: 193.039 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28

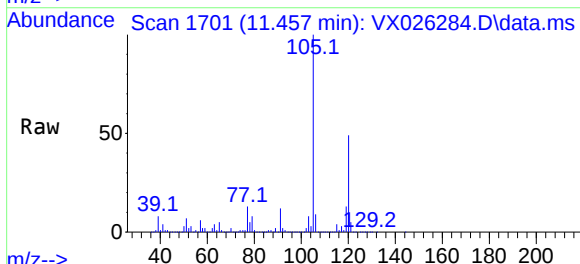


Tgt Ion:105 Resp: 1501182
Ion Ratio Lower Upper
105 100
120 48.6 24.9 74.7





#84
1,2,4-Trimethylbenzene
Concen: 419.201 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB




Tgt Ion:105 Resp: 325733
Ion Ratio Lower Upper
105 100
120 46.8 22.9 68.7

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022




#85
sec-Butylbenzene
Concen: 15.749 ug/l
RT: 11.896 min Scan# 1773
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Tgt Ion:105 Resp: 148346
Ion Ratio Lower Upper
105 100
134 26.8 10.4 31.1





#86
p-Isopropyltoluene
Concen: 23.800 ug/l m
RT: 12.018 min Scan# 1792
Delta R.T. 0.006 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28




Instrument :
MSVOA_X
ClientSampleId :
WANA-SB

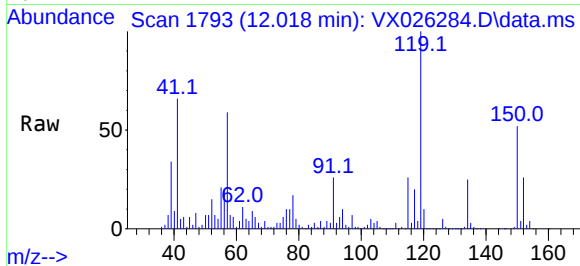


Tgt Ion:119 Resp: 186888
Ion Ratio Lower Upper
119 100
134 21.6 13.2 39.6
91 20.1 11.9 35.9

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

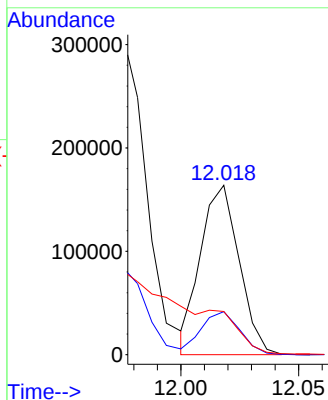


#89
n-Butylbenzene
Concen: 36.541 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28

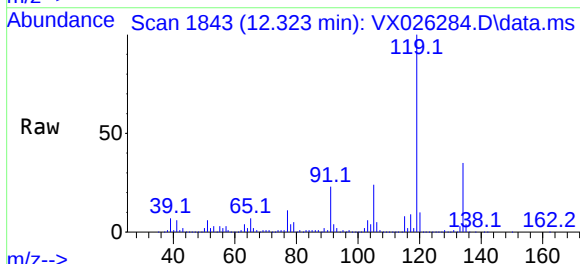


Tgt Ion: 91 Resp: 255002
Ion Ratio Lower Upper
91 100
92 27.2 27.3 81.8#
134 117.4 13.5 40.4#

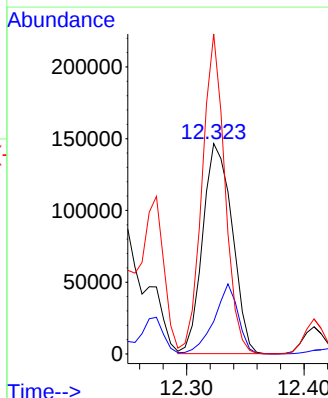

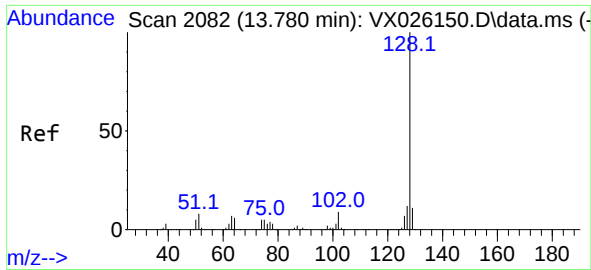

#95
Naphthalene
Concen: 66.846 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX026284.D
Acq: 04 Jan 2022 20:28

Instrument :
MSVOA_X
ClientSampleId :
WANA-SB



Tgt Ion:128 Resp: 622833
Ion Ratio Lower Upper
128 100
127 13.1 10.3 15.5
129 11.1 8.8 13.2

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/05/2022
Supervised By :Mahesh Dadoda 01/05/2022

