

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010423\
 Data File : VX033616.D
 Acq On : 04 Jan 2023 13:24
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
 Title : SW846 8260

Signal : TIC: VX033616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.325	31	39	40	rBV3	4572	8433	1.13%	0.225%
2	2.514	229	234	241	rBV	5767	8514	1.14%	0.227%
3	2.965	299	308	316	rBV5	4116	9721	1.30%	0.259%
4	3.093	319	329	335	rVB5	3438	7898	1.05%	0.211%
5	3.696	417	428	441	rBV	38046	106276	14.19%	2.836%
6	5.385	693	705	722	rBV	88435	261000	34.86%	6.964%
7	5.550	722	732	748	rVB	167612	482619	64.45%	12.878%
8	5.958	789	799	812	rBV	91880	249039	33.26%	6.645%
9	6.763	921	931	945	rBV	235017	561463	74.98%	14.981%
10	8.647	1233	1240	1249	rBV	483610	748791	100.00%	19.980%
11	10.055	1465	1471	1483	rBV	337882	453771	60.60%	12.108%
12	11.079	1634	1639	1649	rBV	290805	357977	47.81%	9.552%
13	11.457	1697	1701	1709	rVB3	6015	7654	1.02%	0.204%
14	12.024	1788	1794	1805	rVB	332189	433667	57.92%	11.571%
15	12.335	1841	1845	1851	rVB2	8497	10283	1.37%	0.274%
16	13.591	2046	2051	2057	rVB	7727	9561	1.28%	0.255%
17	13.725	2068	2073	2077	rBV	11420	13439	1.79%	0.359%
18	13.780	2077	2082	2090	rBV	5907	8015	1.07%	0.214%
19	13.963	2107	2112	2117	rVB	7471	9647	1.29%	0.257%




Sum of corrected areas: 3747768

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010423\
Data File : VX033616.D
Acq On : 04 Jan 2023 13:24
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

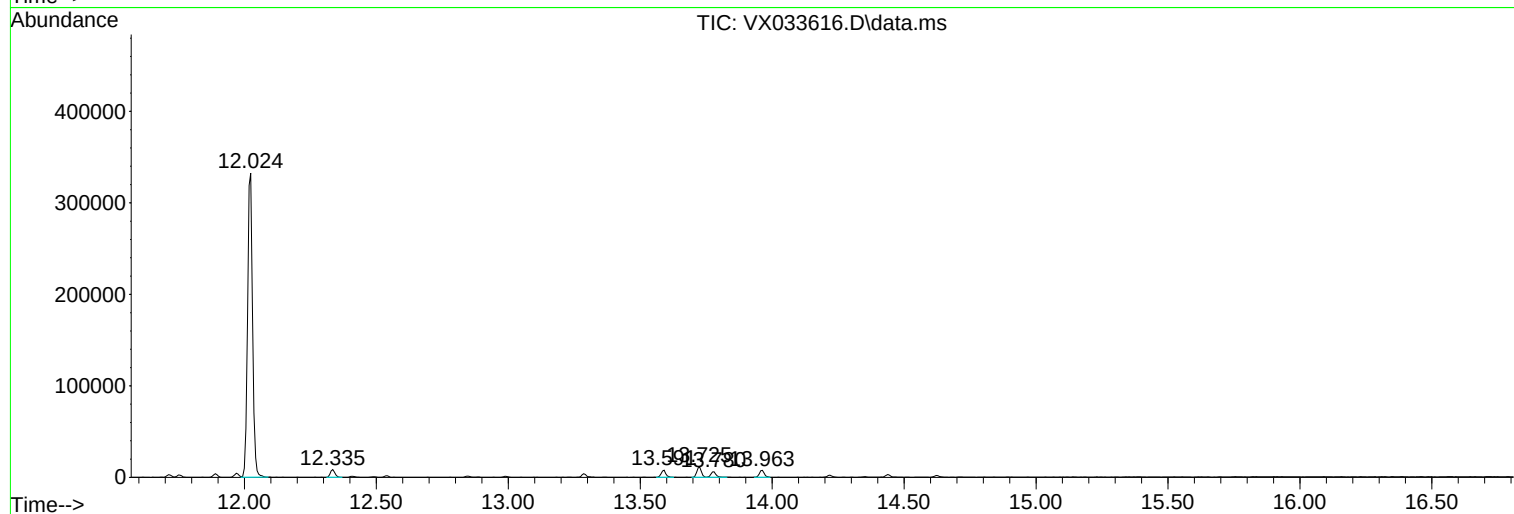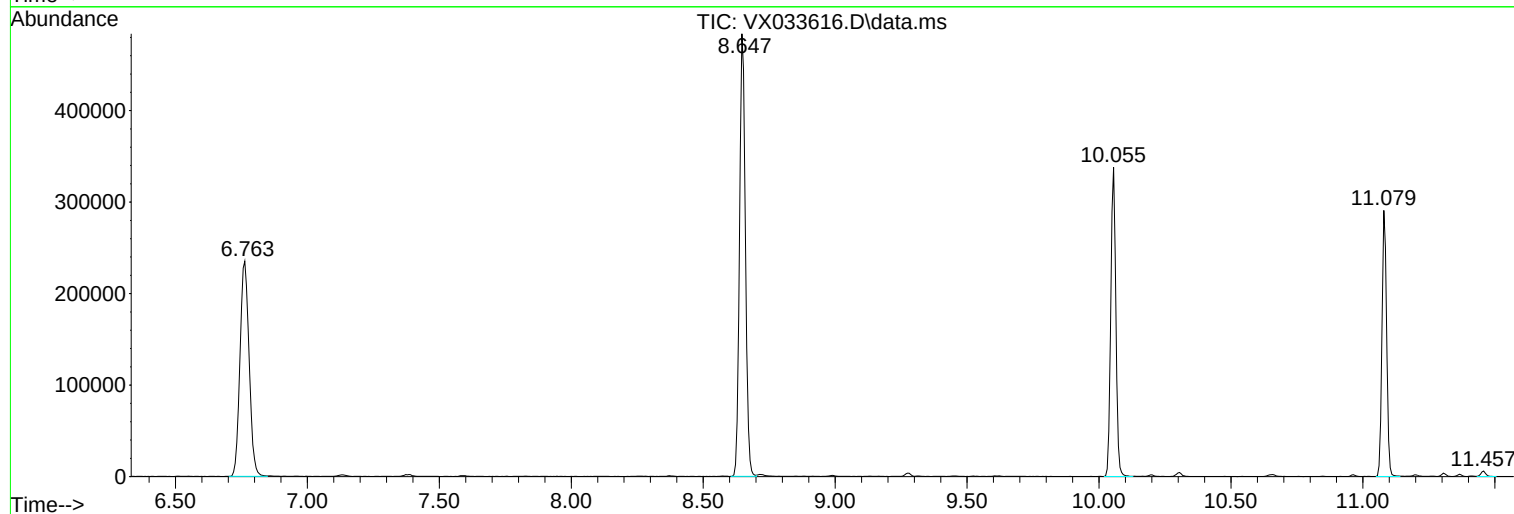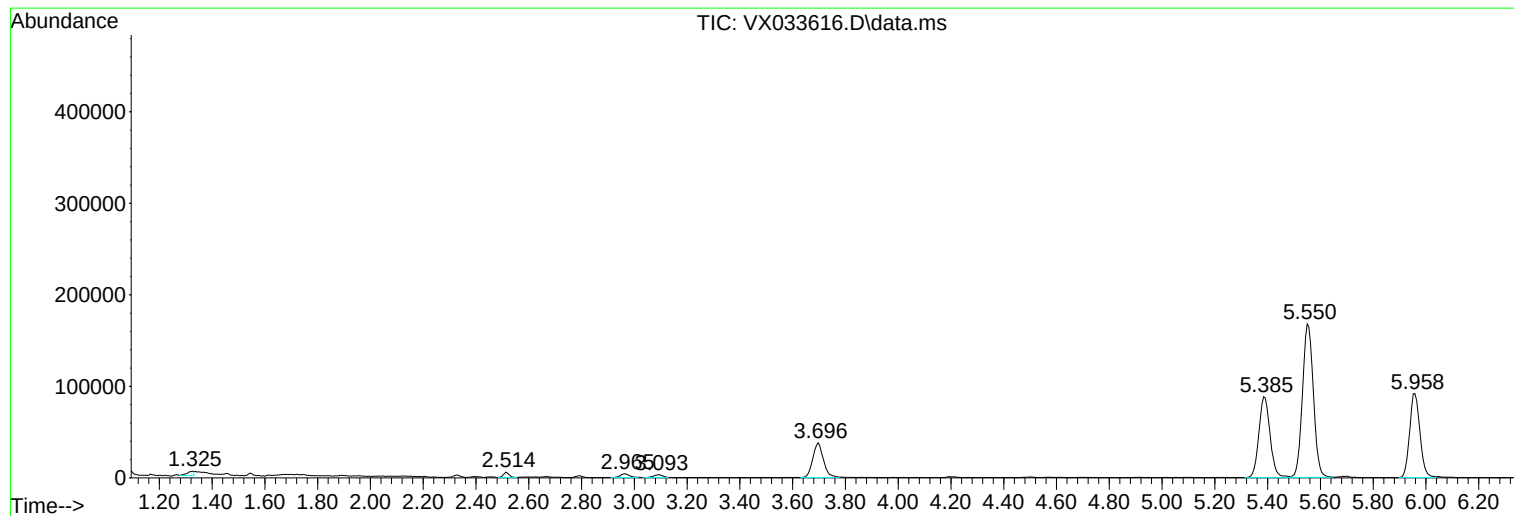

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010423\
Data File : VX033616.D
Acq On : 04 Jan 2023 13:24
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown3.696 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.696	11.01 ug/l	106276	Pentafluorobenzene	5.556

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		1-Propene, 2-methyl-	56	C4H8	000115-11-7	49
2		1-Butene	56	C4H8	000106-98-9	49
3		2-Propanethiol, 2-methyl-	90	C4H10S	000075-66-1	43
4		2-Butanethiol	90	C4H10S	000513-53-1	35
5		Propane, 2-methyl-1-nitro-	103	C4H9NO2	000625-74-1	33

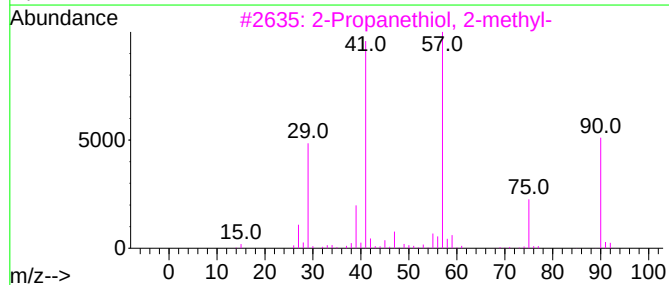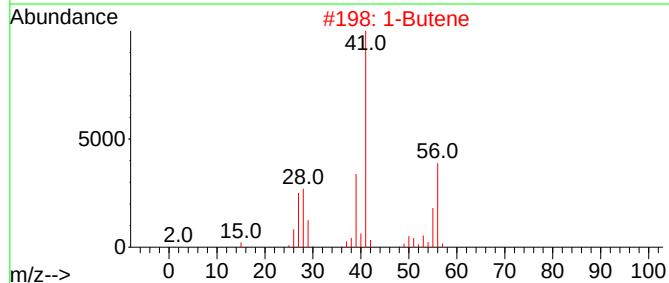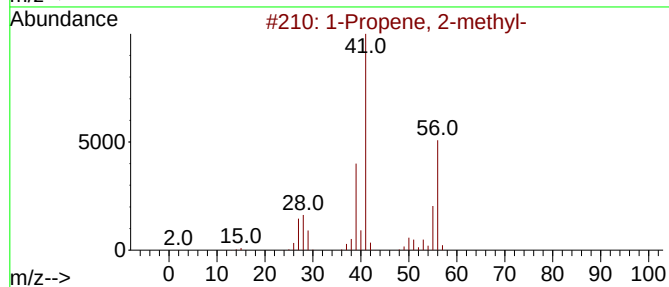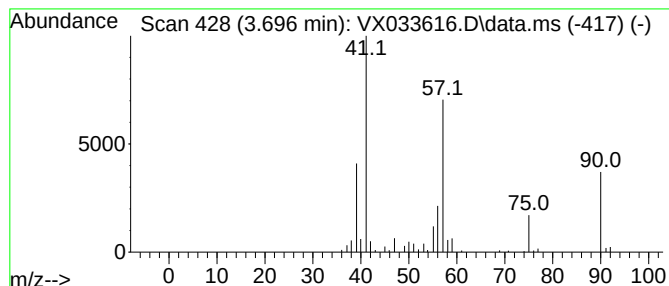

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010423\
Data File : VX033616.D
Acq On : 04 Jan 2023 13:24
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.696	3.696	11.0	ug/l	106276	1	5.556	482619	50.0