

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010424\
 Data File : VX039632.D
 Acq On : 04 Jan 2024 19:43
 Operator : JC/MD
 Sample : P1034-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB

Quant Time: Jan 05 00:47:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	87312	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	183850	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	201398	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	100861	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	76325	47.718	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.440%
35) Dibromofluoromethane	5.385	113	60468	47.608	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.220%
50) Toluene-d8	8.647	98	234093	49.645	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.280%
62) 4-Bromofluorobenzene	11.079	95	109409	56.236	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	112.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010424\
Data File : VX039632.D
Acq On : 04 Jan 2024 19:43
Operator : JC/MD
Sample : P1034-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Time: Jan 05 00:47:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




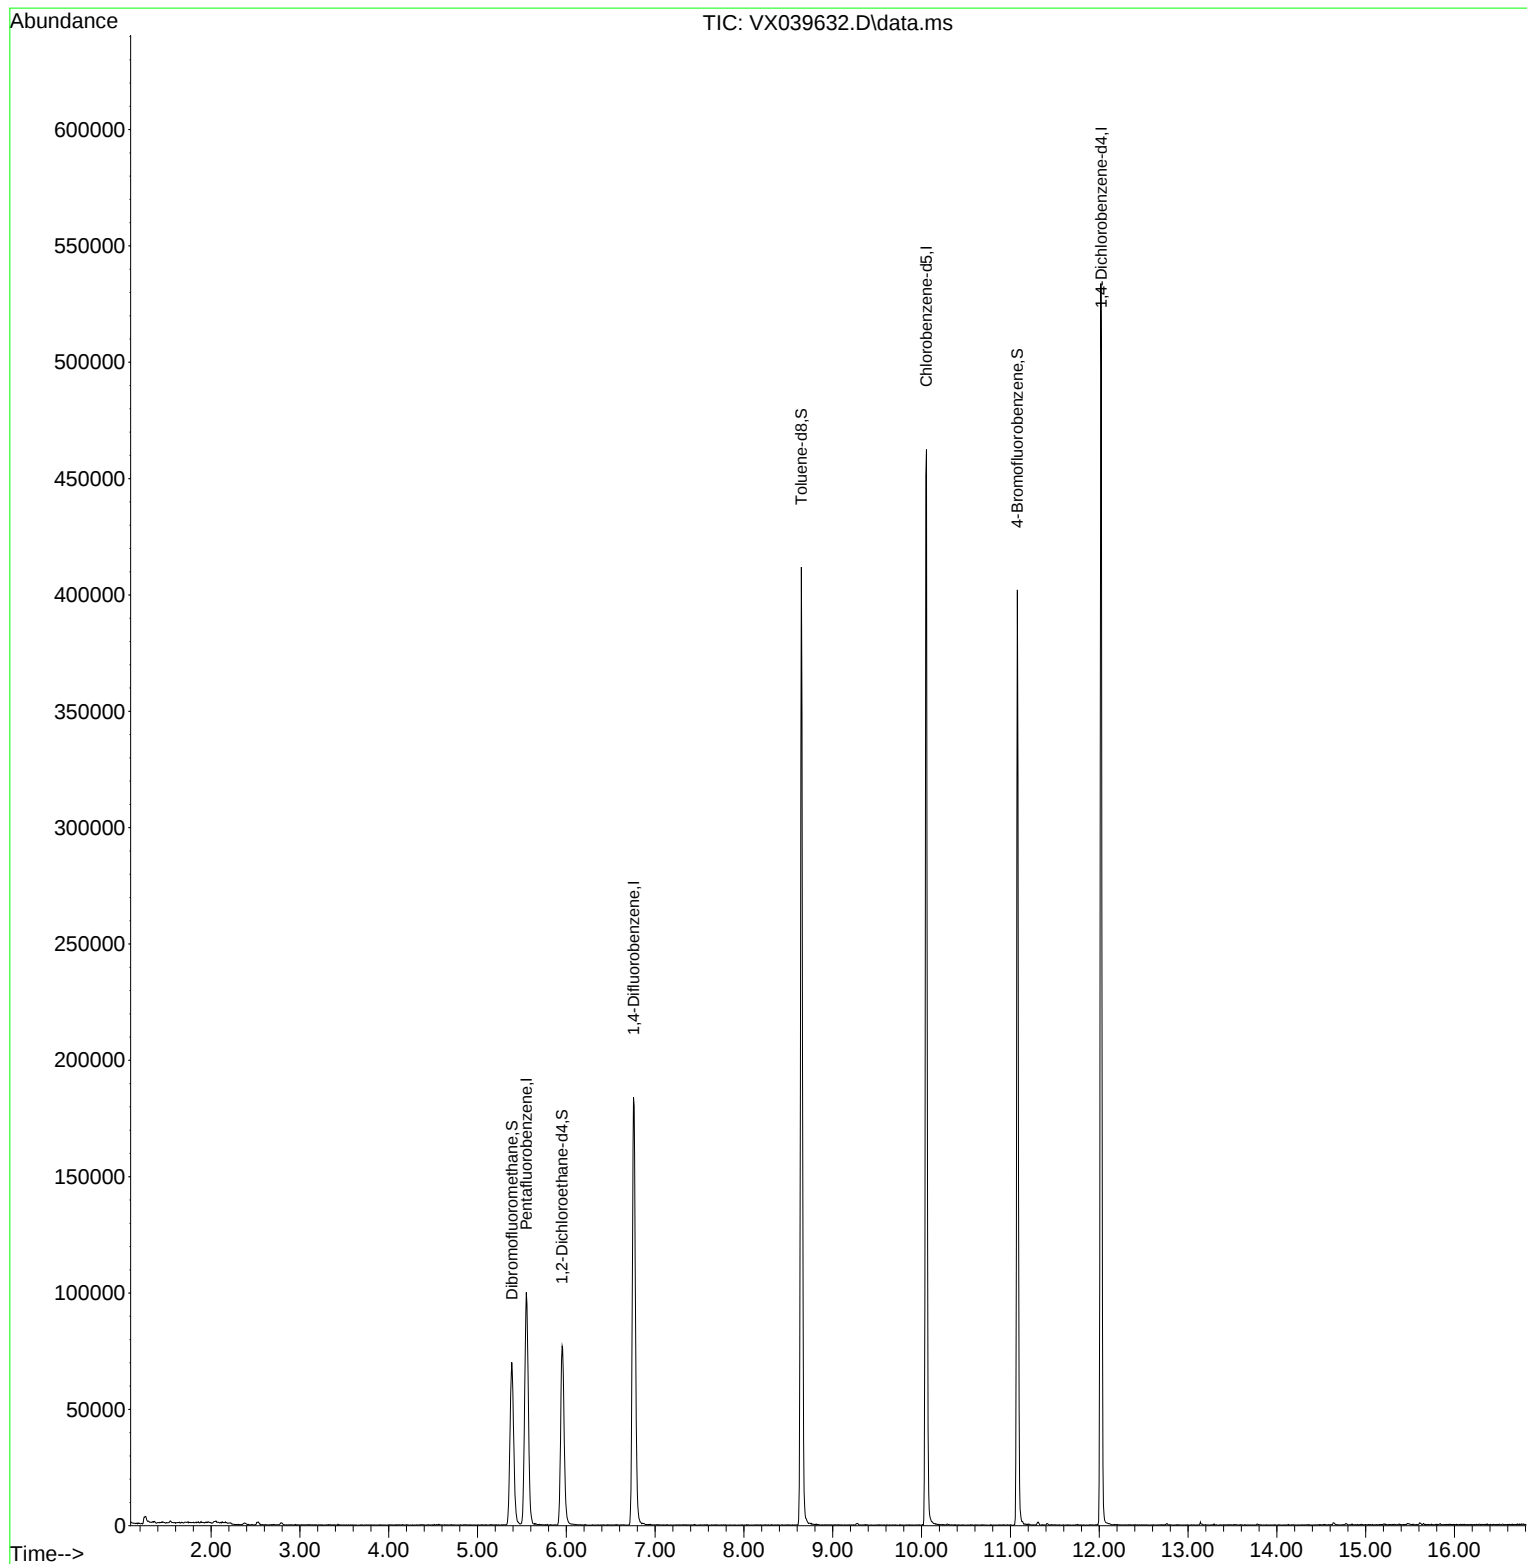


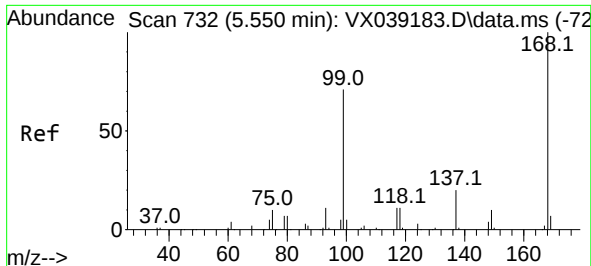

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX039632.D
Acq: 04 Jan 2024 19:43




Instrument :
MSVOA_X
ClientSampleId :
TB

Tgt Ion:168 Resp: 87312
Ion Ratio Lower Upper
168 100
99 68.4 56.6 85.0

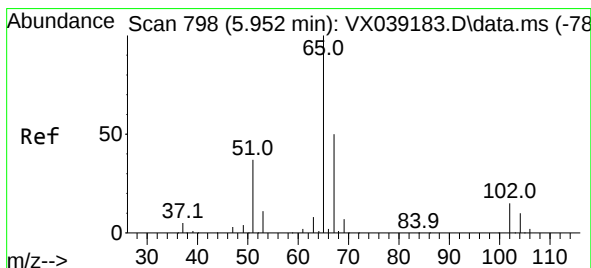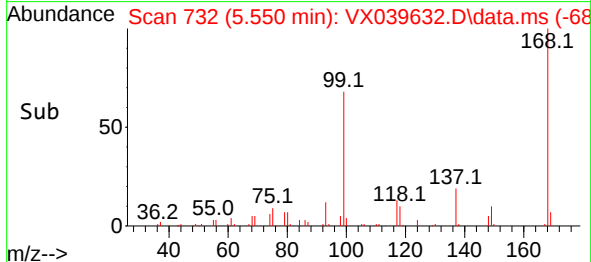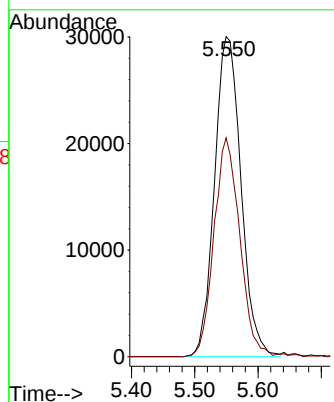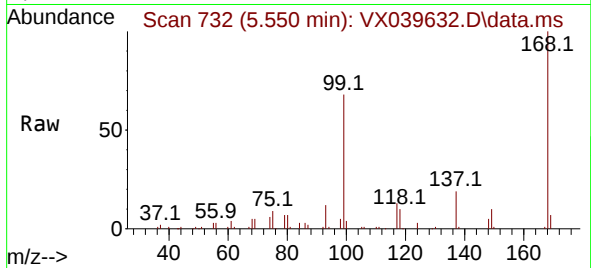

#33
1,2-Dichloroethane-d4
Concen: 47.718 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039632.D
Acq: 04 Jan 2024 19:43

Tgt Ion: 65 Resp: 76325
Ion Ratio Lower Upper
65 100
67 51.7 0.0 100.2


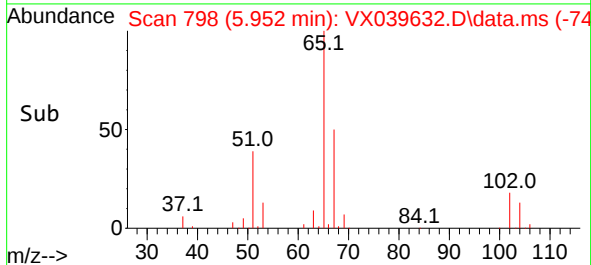
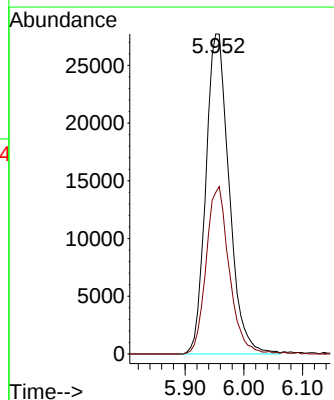
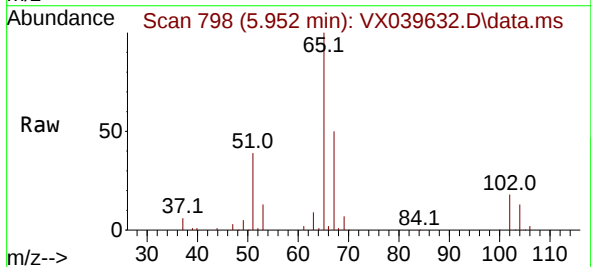




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX039632.D
Acq: 04 Jan 2024 19:43




Instrument :
MSVOA_X
ClientSampleId :
TB

Tgt Ion:114 Resp: 183850
Ion Ratio Lower Upper
114 100
63 21.1 0.0 45.0
88 17.4 0.0 36.6

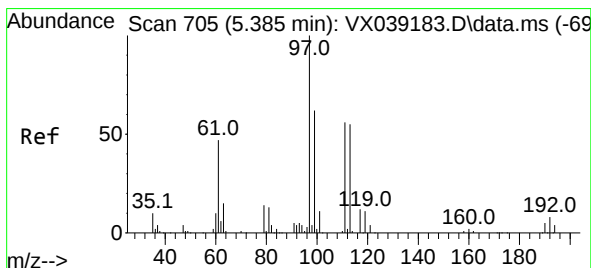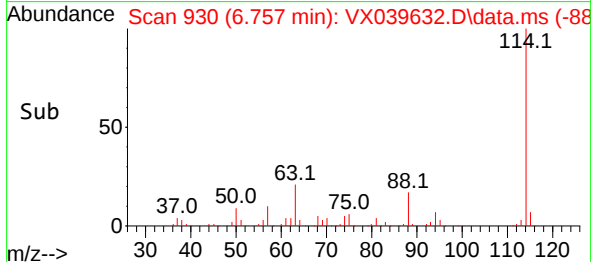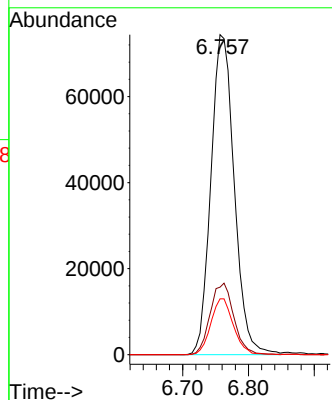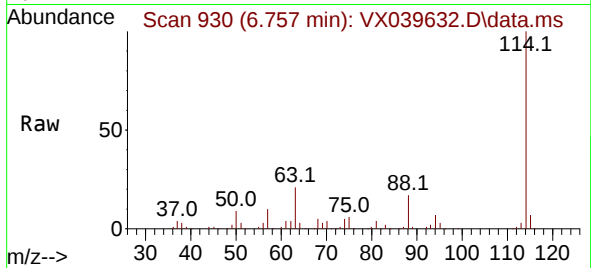

#35
Dibromofluoromethane
Concen: 47.608 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039632.D
Acq: 04 Jan 2024 19:43

Tgt Ion:113 Resp: 60468
Ion Ratio Lower Upper
113 100
111 104.3 82.9 124.3
192 15.6 13.3 19.9

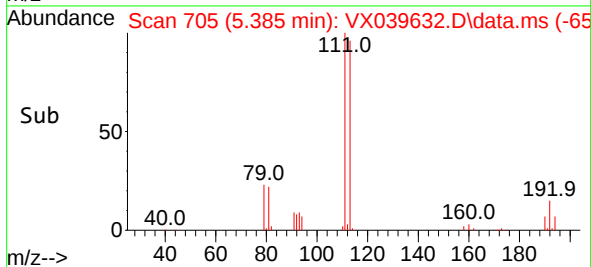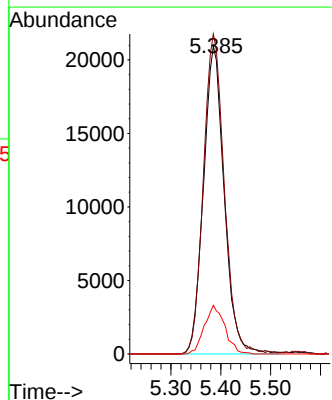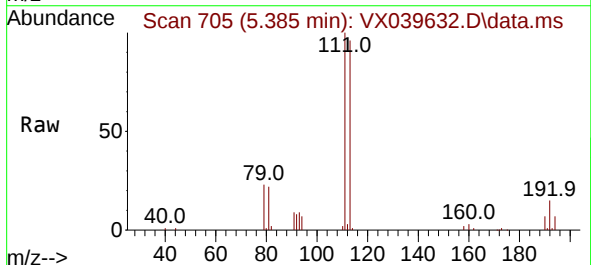



#50

Toluene-d8

Concen: 49.645 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX039632.D

Acq: 04 Jan 2024 19:43

Instrument :

MSVOA_X

ClientSampleId :





TB

Tgt Ion: 98 Resp: 234093

Ion Ratio Lower Upper

98 100

100 64.1 53.1 79.7

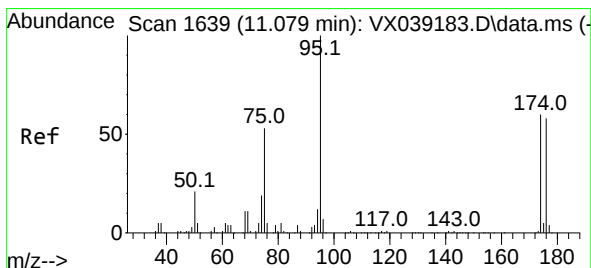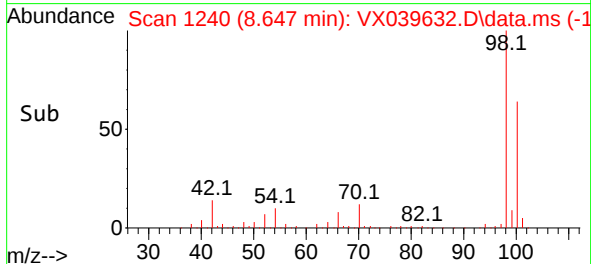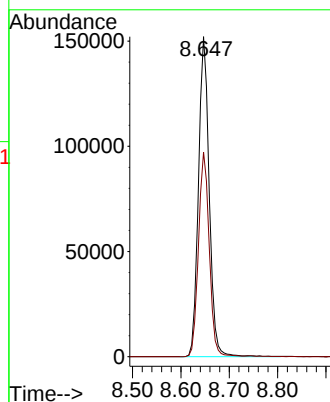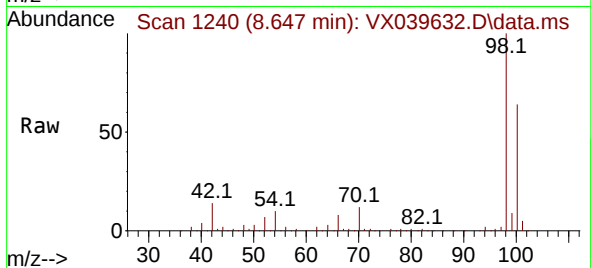

#62

4-Bromofluorobenzene

Concen: 56.236 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX039632.D

Acq: 04 Jan 2024 19:43




Tgt Ion: 95 Resp: 109409


Ion Ratio Lower Upper

95 100

174 65.1 0.0 135.6

176 62.4 0.0 131.0

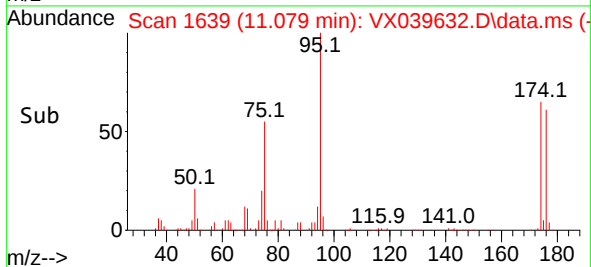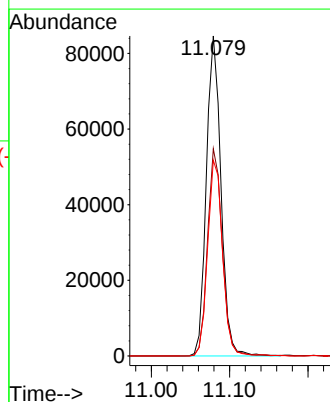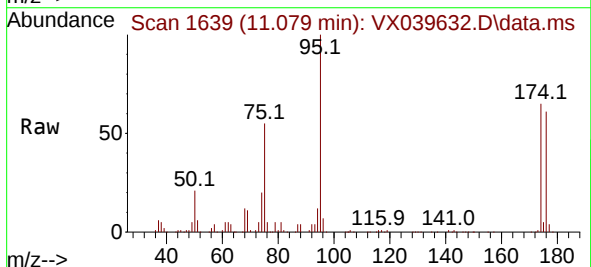

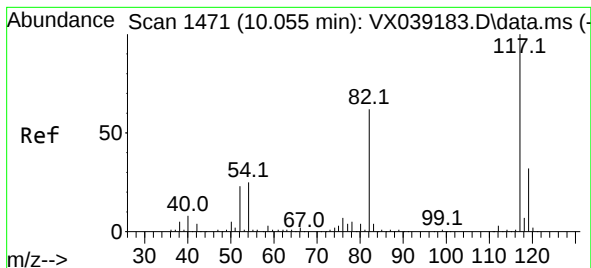

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX039632.D

Acq: 04 Jan 2024 19:43

Instrument :

MSVOA_X

ClientSampleId :

TB





Tgt Ion:117 Resp: 201398

Ion Ratio Lower Upper

117 100

82 60.4 46.2 69.4

119 32.6 25.5 38.3

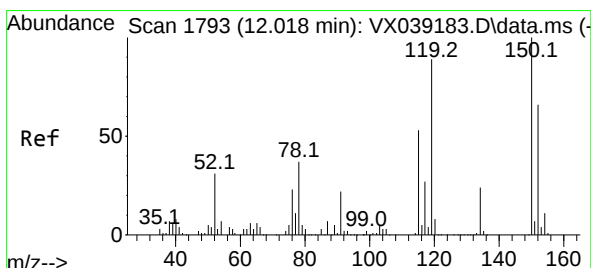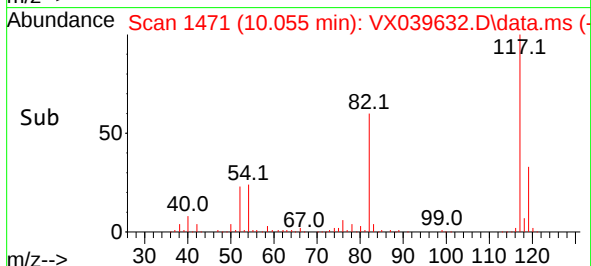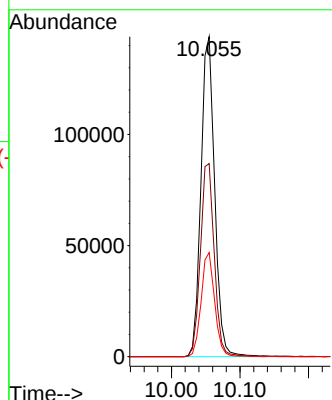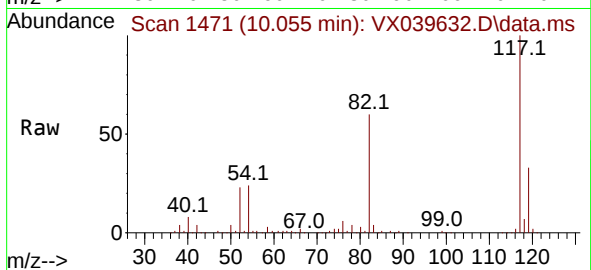

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.006 min

Lab File: VX039632.D

Acq: 04 Jan 2024 19:43

Tgt Ion:152 Resp: 100861

Ion Ratio Lower Upper

152 100

115 67.9 43.3 129.9

150 159.1 0.0 345.0

