



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010424\
Data File : VX039615.D
Acq On : 04 Jan 2024 08:45
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Title : SW846 8260
Last Update : Thu Dec 14 01:28:15 2023

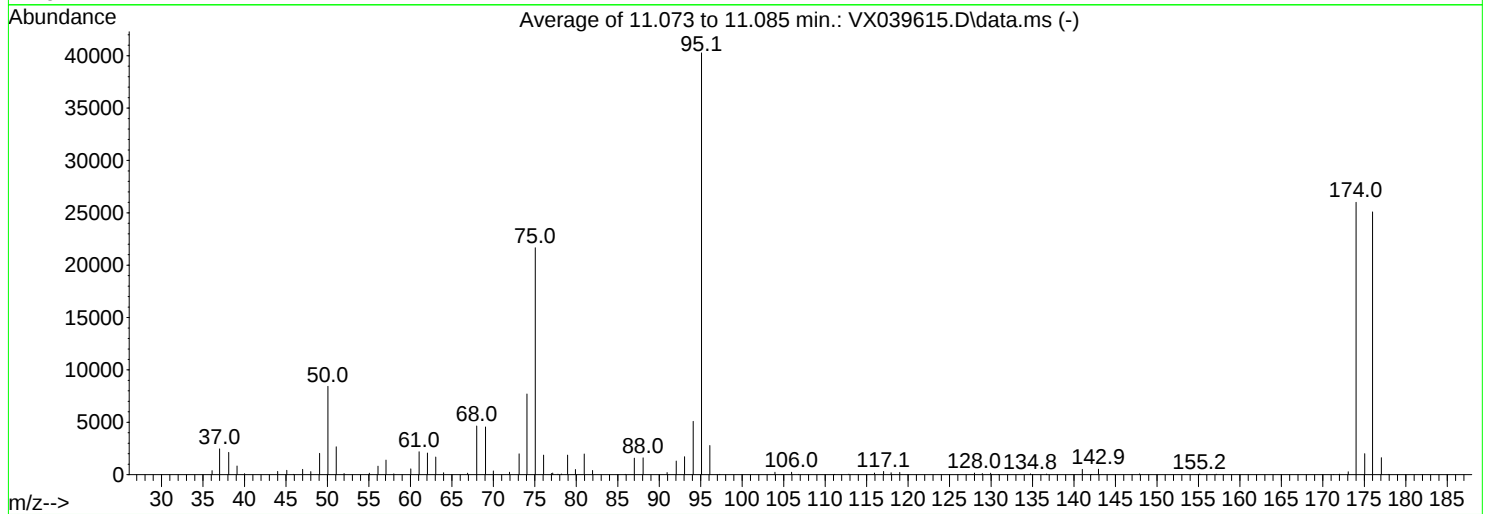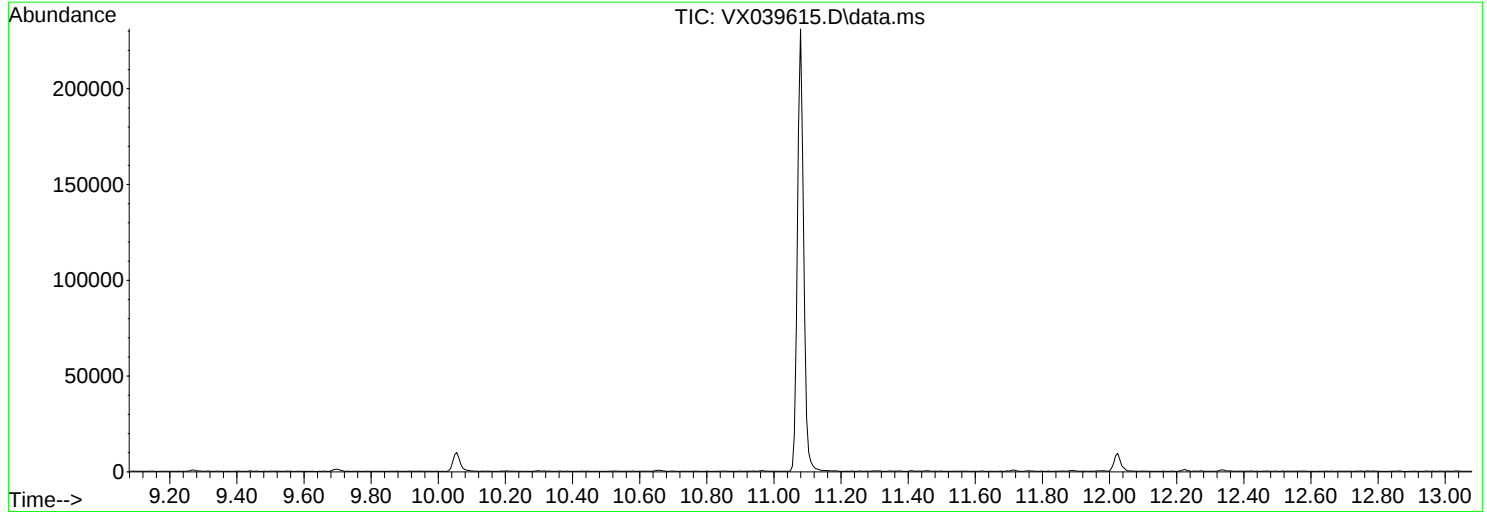

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	8430	PASS
75	95	30	60	53.8	21661	PASS
95	95	100	100	100.0	40275	PASS
96	95	5	9	6.9	2788	PASS
173	174	0.00	2	1.1	274	PASS
174	95	50	100	64.6	26011	PASS
175	174	5	9	7.7	2001	PASS
176	174	95	101	96.4	25085	PASS
177	176	5	9	6.5	1621	PASS