


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX010521\
 Data File : VX020499.D
 Acq On : 05 Jan 2021 15:12
 Operator : JC/MD
 Sample : BFB62
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB62

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR010521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jan 06 04:48:03 2021

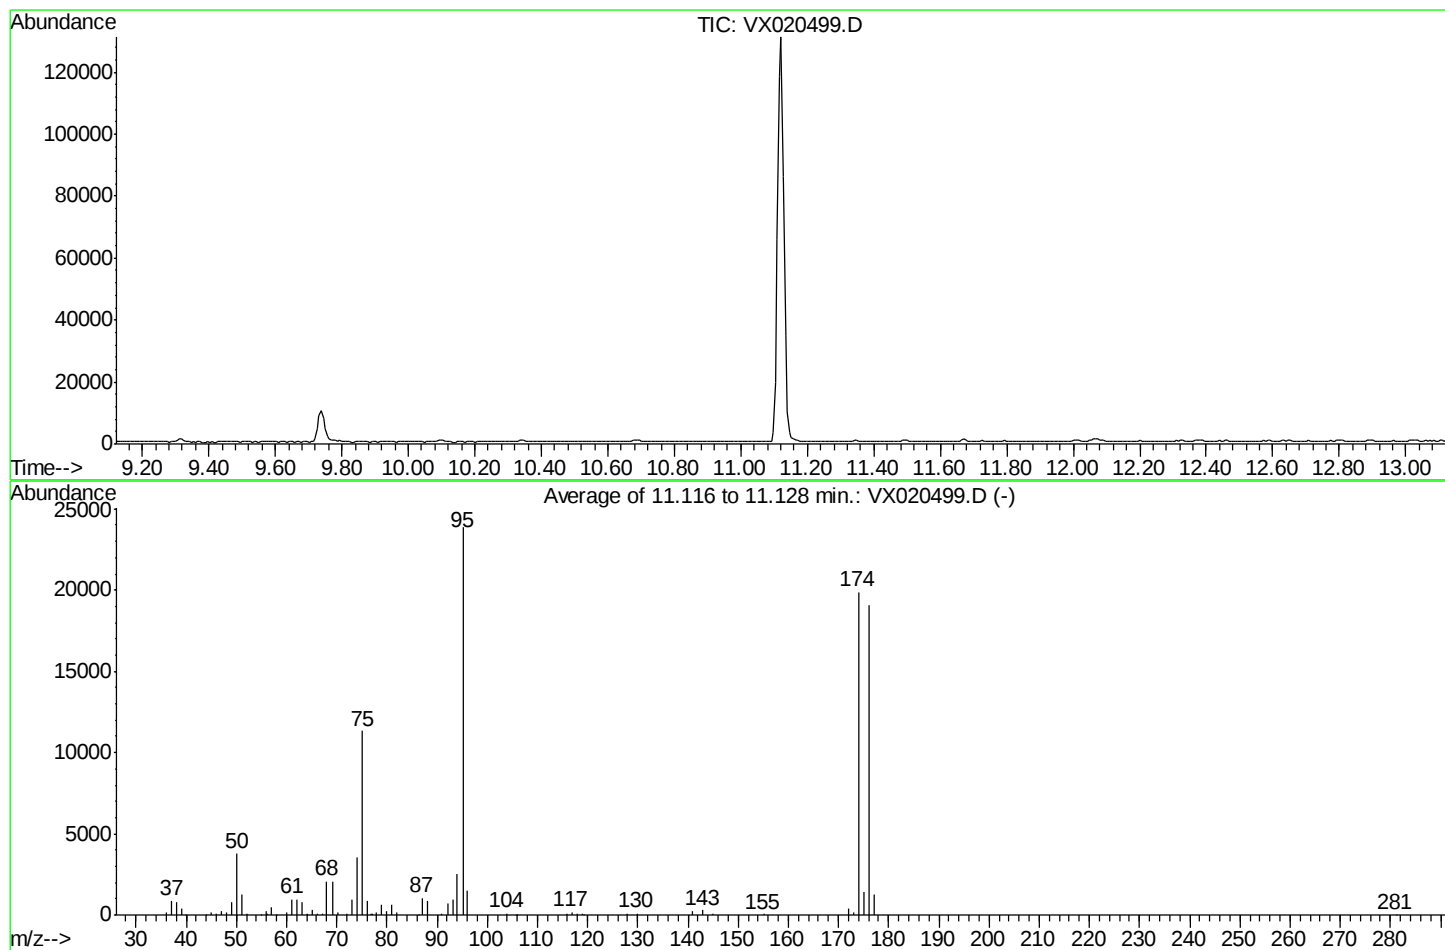

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	3748	PASS
75	95	30	80	47.4	11323	PASS
95	95	100	100	100.0	23864	PASS
96	95	5	9	6.2	1471	PASS
173	174	0.00	2	0.7	134	PASS
174	95	50	120	83.3	19874	PASS
175	174	5	9	7.1	1405	PASS
176	174	95	105	96.1	19090	PASS
177	176	5	10	6.6	1258	PASS

m/z	Abundance
36.10	189.0
37.10	1015.0
38.00	935.0
39.00	431.0
39.90	146.0
44.10	741.0
45.10	202.0
46.10	72.0
47.00	299.0
48.00	141.0
49.00	1030.0
50.10	4469.0
51.10	1540.0
52.10	111.0
54.90	83.0
56.00	347.0
57.00	683.0
60.00	267.0
61.00	1012.0
62.00	1056.0
63.10	912.0
64.00	182.0
65.10	351.0
67.20	97.0
68.10	2381.0
69.10	2253.0
70.00	119.0
72.00	130.0
73.00	959.0
74.10	3941.0
75.10	12954.0
76.10	1001.0
77.20	185.0
77.90	132.0
79.00	688.0
79.90	250.0
81.00	676.0
82.00	220.0
86.20	56.0
87.00	1284.0
88.00	974.0
91.00	70.0
92.10	740.0
93.10	1095.0
94.10	2830.0
95.10	26248.0
96.10	1682.0
104.00	115.0
105.70	62.0
106.10	69.0
116.00	117.0
116.90	146.0
117.80	84.0
119.00	124.0
128.00	68.0
129.90	70.0
141.00	215.0
143.00	309.0
145.10	169.0
172.00	338.0
173.10	194.0
174.00	19400.0
175.00	1213.0
176.00	17480.0
177.00	1135.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62

m/z	Abundance
36.00	147.0
37.10	1051.0
38.10	839.0
39.00	440.0
39.90	180.0
44.00	771.0
45.00	153.0
46.10	79.0
47.10	290.0
48.10	170.0
49.00	951.0
50.10	4243.0
51.10	1352.0
52.00	56.0
56.00	254.0
57.10	527.0
58.00	59.0
60.10	197.0
61.10	1073.0
62.00	1005.0
63.00	864.0
64.00	180.0
65.10	334.0
66.10	84.0
67.20	65.0
68.00	2462.0
69.10	2359.0
70.10	194.0
72.10	164.0
73.00	1166.0
74.10	4284.0
75.10	13134.0
76.10	1023.0
76.90	151.0
77.90	138.0
78.90	720.0
80.00	263.0
81.00	735.0
81.90	203.0
87.00	1182.0
88.00	1150.0
91.00	80.0
92.10	888.0
93.10	1154.0
94.10	2813.0
95.10	27336.0
96.10	1610.0
103.90	89.0
105.60	58.0
106.00	52.0
116.00	88.0
116.90	216.0
117.90	105.0
118.80	148.0
127.90	93.0
129.90	138.0
140.90	324.0
143.00	348.0
144.90	96.0
155.00	80.0
172.00	420.0
172.90	210.0
174.00	23808.0
175.00	1855.0
176.00	23056.0
177.00	1577.0
281.20	52.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62

m/z	Abundance
36.20	85.0
37.10	551.0
38.10	532.0
39.00	260.0
40.00	187.0
44.10	696.0
45.00	134.0
47.10	198.0
48.00	113.0
49.10	464.0
50.10	2533.0
51.00	847.0
52.20	54.0
56.20	187.0
56.90	264.0
60.10	101.0
61.00	759.0
62.10	771.0
63.00	579.0
64.20	115.0
65.10	362.0
66.10	57.0
67.20	60.0
68.00	1373.0
69.10	1589.0
70.20	104.0
73.00	796.0
74.10	2496.0
75.10	7882.0
76.00	568.0
77.00	176.0
77.80	98.0
79.00	396.0
80.10	171.0
80.90	397.0
82.00	122.0
87.00	673.0
88.00	546.0
90.90	63.0
92.00	477.0
93.10	706.0
94.00	1890.0
95.10	18008.0
96.10	1122.0
103.90	64.0
116.90	152.0
118.00	78.0
119.10	87.0
129.90	88.0
140.90	152.0
142.90	221.0
144.90	74.0
155.10	60.0
172.00	395.0
174.00	16416.0
175.10	1148.0
176.00	16736.0
177.00	1064.0
281.20	59.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62

Scan 1638 (11.073 min): VX020499.D
BFB62

m/z	Abundance
40.00	153.0
44.10	703.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62