

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
 Data File : VX026322.D
 Acq On : 05 Jan 2022 15:14
 Operator : JC/MD
 Sample : M5336-15DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 06 03:09:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	144386	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	242449	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	214662	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	104976	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	104516	50.035	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 100.080%	
35) Dibromofluoromethane	5.391	113	79166	50.225	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.440%	
50) Toluene-d8	8.653	98	284917	48.596	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 97.200%	
62) 4-Bromofluorobenzene	11.085	95	114787	54.997	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 110.000%	

Target Compounds				Qvalue		
3) Chloromethane	1.361	50	5856	3.318	ug/l #	83
5) Bromomethane	1.599	94	238	0.208	ug/l	98
10) Methyl Iodide	2.465	142	618	0.283	ug/l #	88
11) Tert butyl alcohol	2.971	59	60223	144.347	ug/l #	38
13) Acrolein	2.252	56	143	0.959	ug/l #	14
15) Acrylonitrile	3.123	53	3030	2.933	ug/l #	30
16) Acetone	2.386	43	148202	130.948	ug/l	95
17) Carbon Disulfide	2.514	76	1659	0.362	ug/l	96
18) Methyl Acetate	2.965	43	280852	76.505	ug/l #	52
19) Methyl tert-butyl Ether	3.117	73	310203	55.546	ug/l	99
20) Methylene Chloride	2.794	84	4969	1.835	ug/l	93
22) Diisopropyl ether	3.702	45	248413	41.192	ug/l #	1
23) Vinyl Acetate	3.696	43	14272	2.980	ug/l #	76
24) 1,1-Dichloroethane	3.696	63	1738	0.532	ug/l #	83
25) 2-Butanone	4.568	43	27254	17.287	ug/l	100
29) Tetrahydrofuran	5.025	42	326	0.328	ug/l #	32
31) Cyclohexane	5.470	56	1844	0.620	ug/l #	66
36) 1,1-Dichloropropene	5.556	75	12284	4.832	ug/l #	50
37) Ethyl Acetate	4.568	43	27254	9.246	ug/l #	69
38) Carbon Tetrachloride	5.562	117	15755	5.571	ug/l #	15
39) Methylcyclohexane	7.385	83	2389	0.833	ug/l #	89
40) Benzene	6.043	78	349348	48.148	ug/l	97
42) 1,2-Dichloroethane	6.050	62	5805	1.977	ug/l #	74
43) Isopropyl Acetate	6.336	43	10472	2.180	ug/l #	67
48) Methyl methacrylate	7.690	41	105012	45.576	ug/l #	30
49) 1,4-Dioxane	7.690	88	274	6.453	ug/l #	1
51) 4-Methyl-2-Pentanone	8.555	43	10226	3.420	ug/l #	46
52) Toluene	8.720	92	1365172	305.624	ug/l	98
53) t-1,3-Dichloropropene	9.080	75	570	2.077	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.336	63	377	10.068	ug/l #	44
59) 2-Hexanone	9.445	43	1183	0.522	ug/l	76
67) Ethyl Benzene	10.195	91	57420	6.810	ug/l	95
68) m/p-Xylenes	10.305	106	68934	21.896	ug/l	93
69) o-Xylene	10.646	106	24660	8.006	ug/l	86
70) Styrene	10.646	104	1475	0.292	ug/l #	1
76) 1,2,3-Trichloropropane	11.085	75	59801	23.601	ug/l #	39

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
 Data File : VX026322.D
 Acq On : 05 Jan 2022 15:14
 Operator : JC/MD
 Sample : M5336-15DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 06 03:09:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
81) trans-1,4-Dichloro-2-b...	11.085	75	59801	68.277	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.756	105	1751	0.259	ug/l	66
92) 1,2-Dibromo-3-Chloropr...	12.993	75	1512	2.128	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
Data File : VX026322.D
Acq On : 05 Jan 2022 15:14
Operator : JC/MD
Sample : M5336-15DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 06 03:09:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration

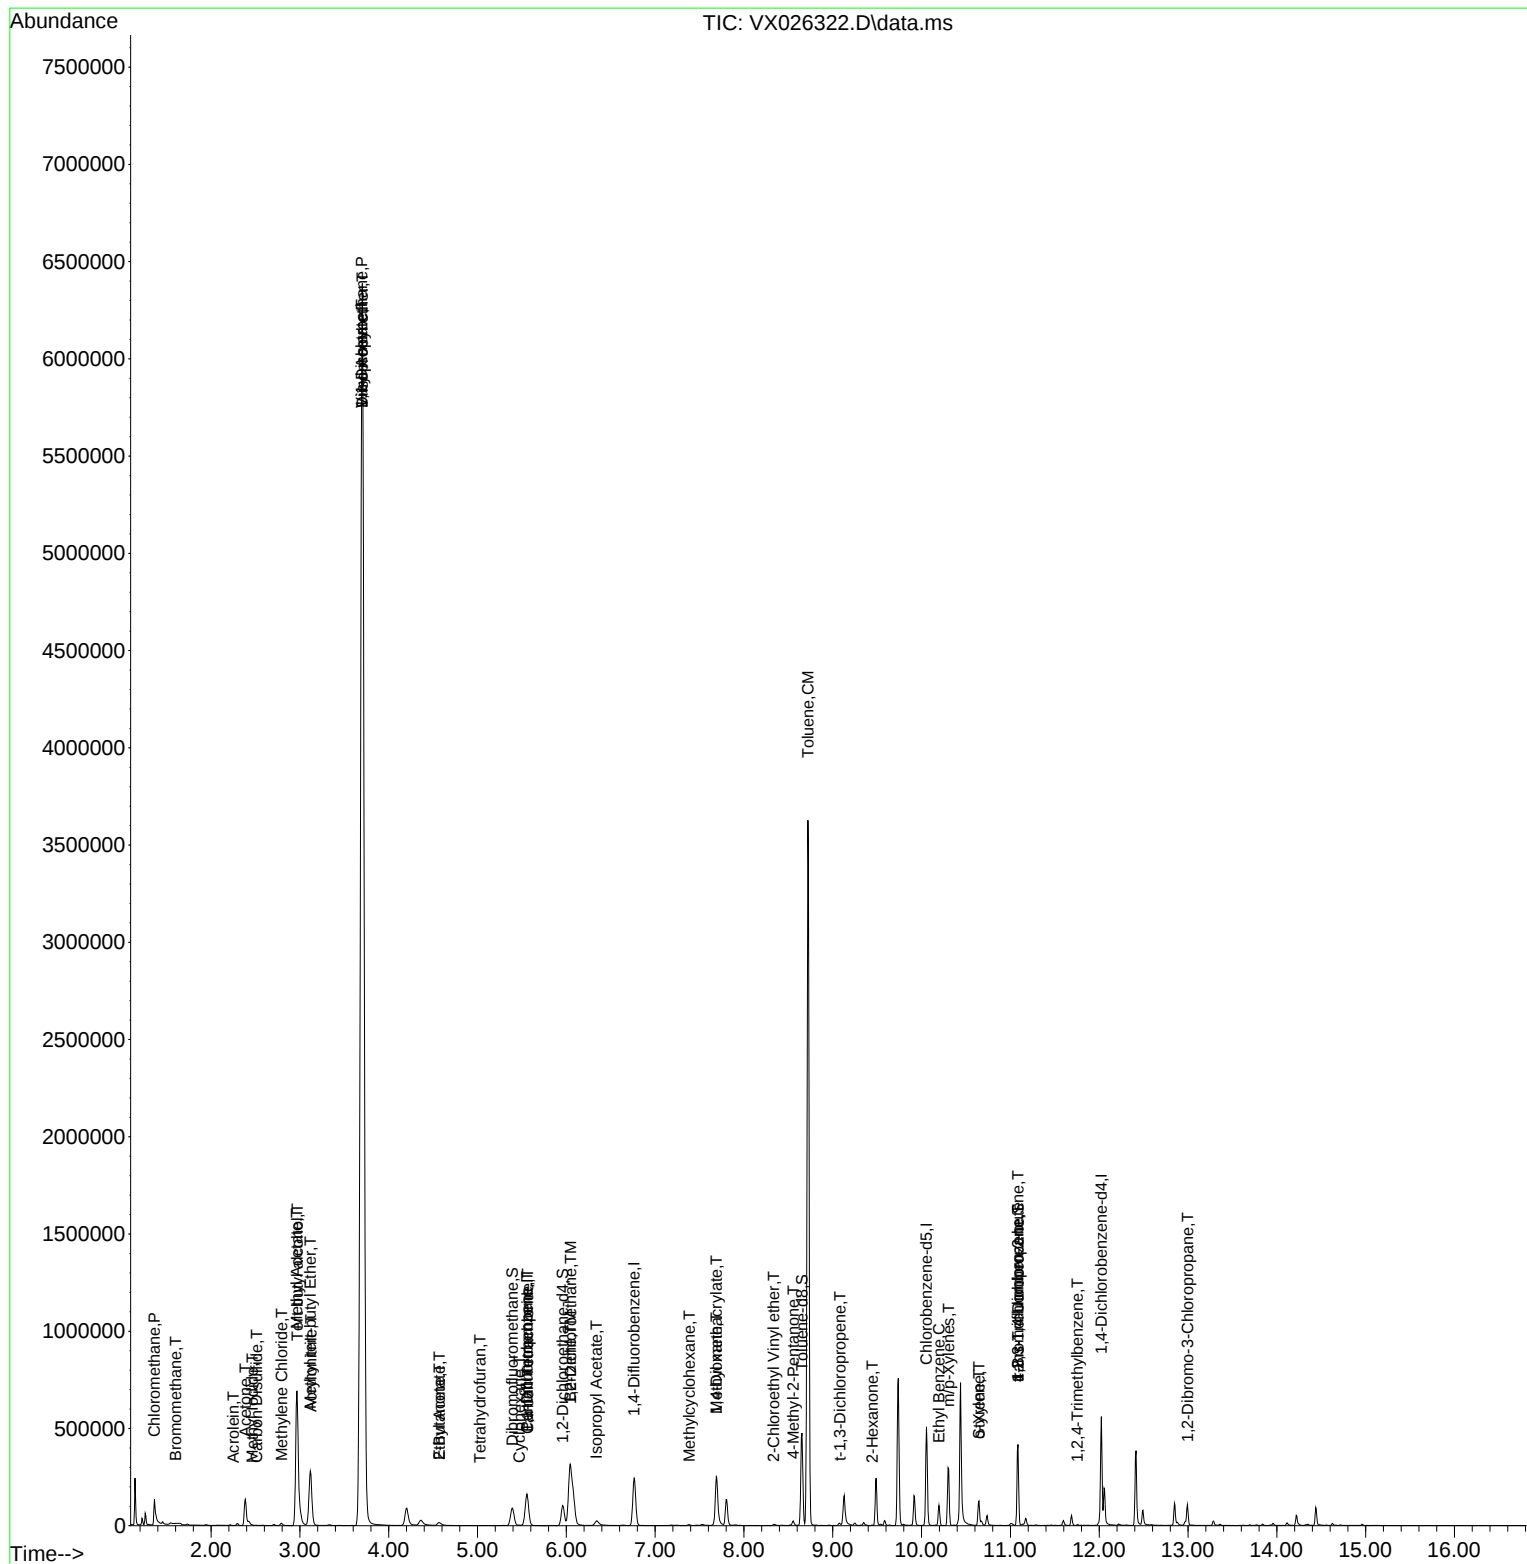






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Instrument :
MSVOA_X
ClientSampleId :



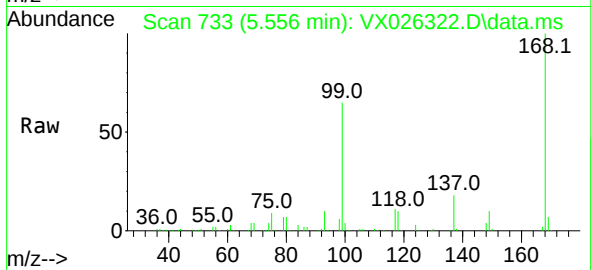



Tgt Ion:168 Resp: 144386
Ion Ratio Lower Upper
168 100
99 64.7 45.8 68.8

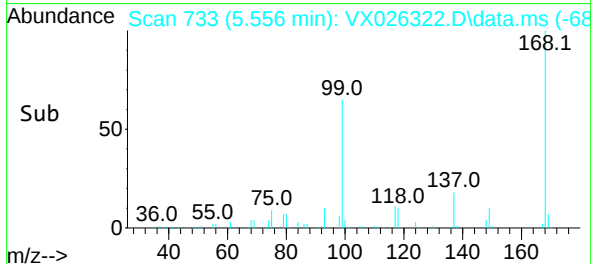

#3
Chloromethane
Concen: 3.318 ug/l
RT: 1.361 min Scan# 45
Delta R.T. 0.067 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Tgt Ion: 50 Resp: 5856
Ion Ratio Lower Upper
50 100
52 22.0 25.4 38.0#


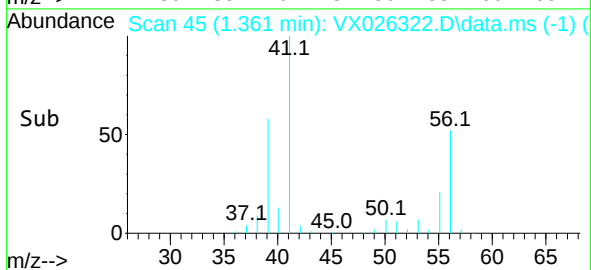

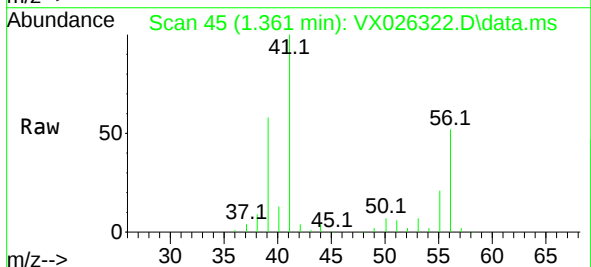


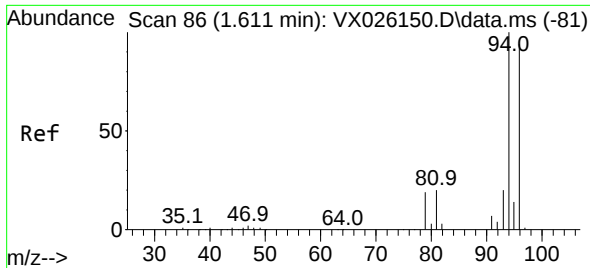

#5
Bromomethane
Concen: 0.208 ug/l
RT: 1.599 min Scan# 84
Delta R.T. -0.012 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 94 Resp: 238
Ion Ratio Lower Upper
94 100
96 95.4 75.0 112.4

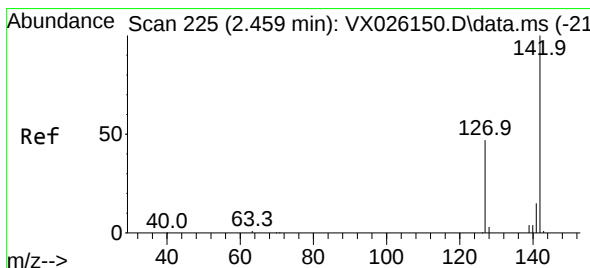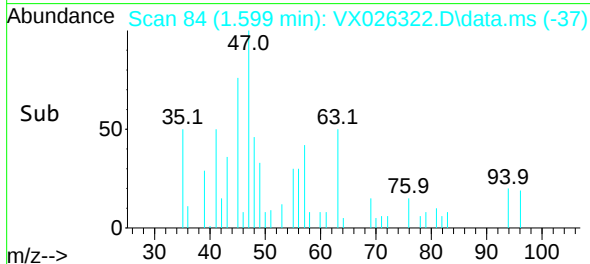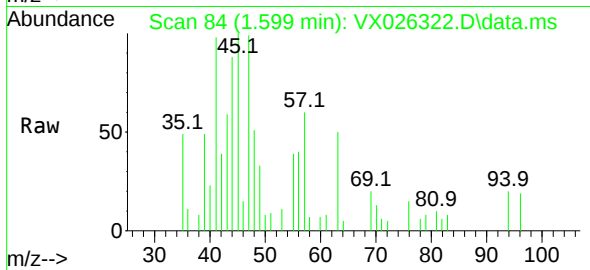

#10
Methyl Iodide
Concen: 0.283 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.006 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14


Tgt Ion: 142 Resp: 618
Ion Ratio Lower Upper
142 100
127 43.4 37.5 56.3
141 0.0 11.4 17.0#

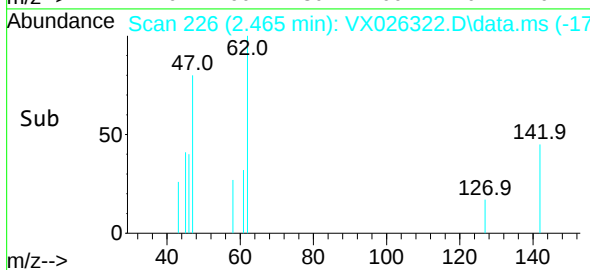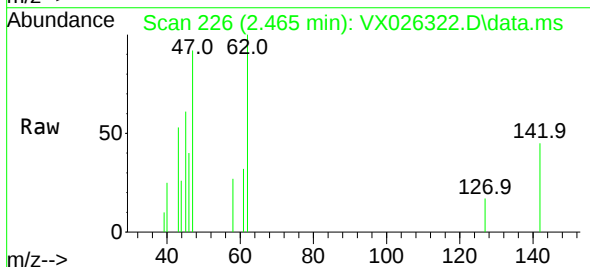






#11
Tert butyl alcohol
Concen: 144.347 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 59 Resp: 60223
Ion Ratio Lower Upper
59 100
57 33.2 8.2 12.2#

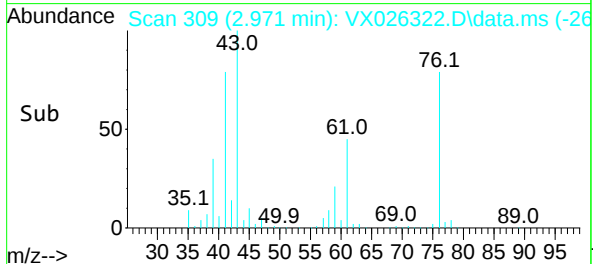

#13
Acrolein
Concen: 0.959 ug/l
RT: 2.252 min Scan# 191
Delta R.T. 0.013 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Tgt Ion: 56 Resp: 143
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.2#

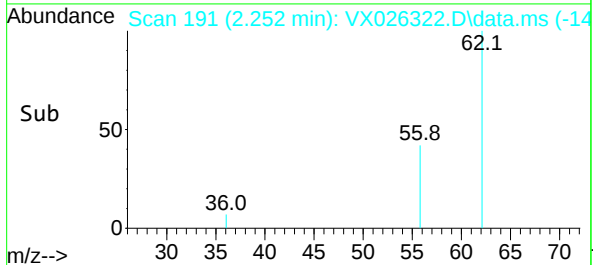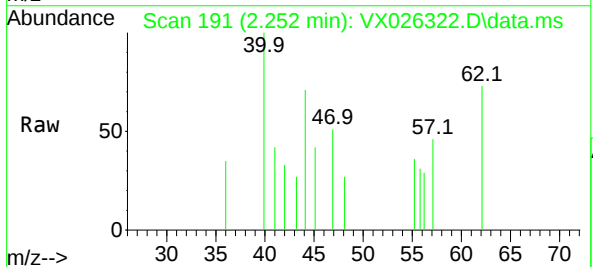



#15

Acrylonitrile

Concen: 2.933 ug/l

RT: 3.123 min Scan# 31

Delta R.T. 0.054 min


Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Instrument :

MSVOA_X

ClientSampleId :

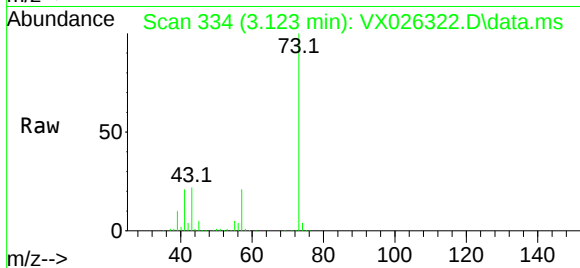




Tgt Ion: 53 Resp: 3030

Ion Ratio Lower Upper

53 100

52 21.0 66.2 99.2#

51 79.5 29.4 44.0#

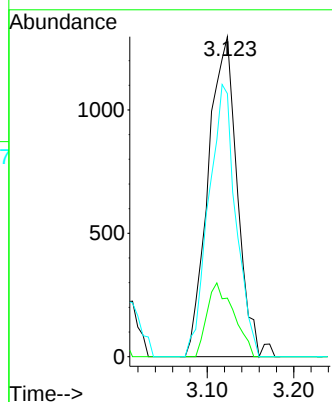

#16

Acetone

Concen: 130.948 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.000 min

Lab File: VX026322.D




Acq: 05 Jan 2022 15:14


Tgt Ion: 43 Resp: 148202

Ion Ratio Lower Upper

43 100


58 28.1 24.8 37.2

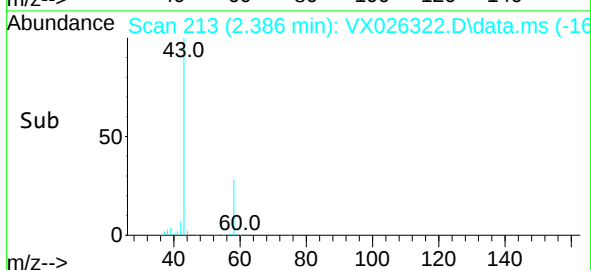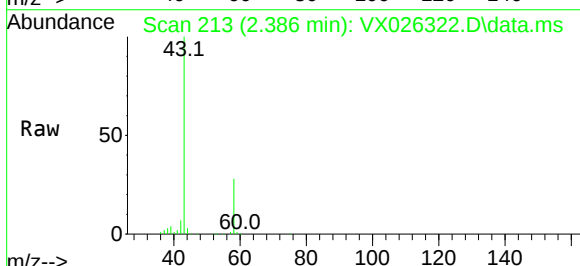






#17
Carbon Disulfide
Concen: 0.362 ug/l
RT: 2.514 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 76 Resp: 1659
Ion Ratio Lower Upper
76 100
78 10.4 7.2 10.8

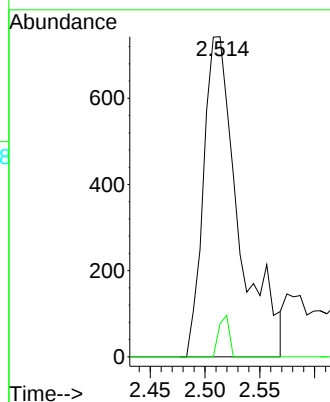


#18
Methyl Acetate
Concen: 76.505 ug/l
RT: 2.965 min Scan# 308
Delta R.T. 0.256 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14



Tgt Ion: 43 Resp: 280852
Ion Ratio Lower Upper
43 100
74 0.3 19.1 28.7#

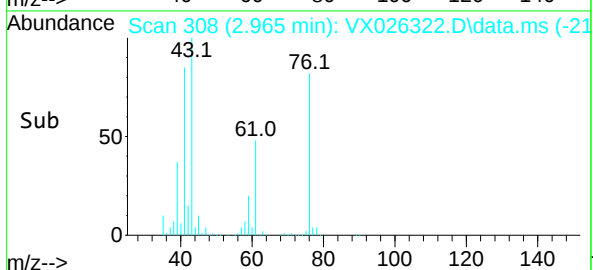



#19

Methyl tert-butyl Ether

Concen: 55.546 ug/l

RT: 3.117 min Scan# 31

Delta R.T. 0.000 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 73 Resp: 310203

Ion Ratio Lower Upper

73 100

57 21.6 17.0 25.6

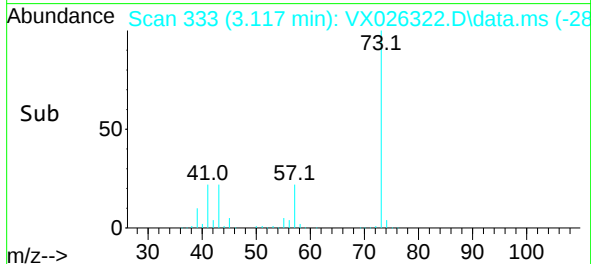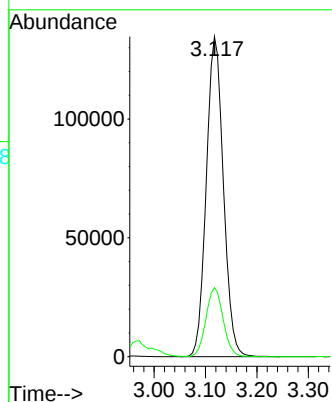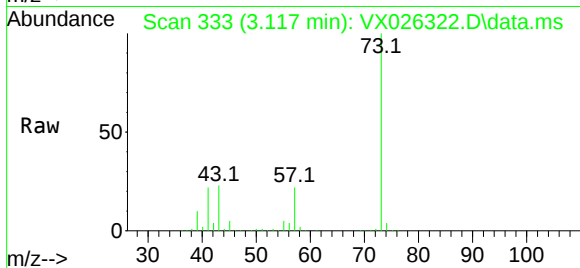

#20

Methylene Chloride

Concen: 1.835 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.000 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Tgt Ion: 84 Resp: 4969




Ion Ratio Lower Upper


84 100

49 127.5 97.1 145.7

51 41.2 29.3 43.9


86 71.8 50.8 76.2

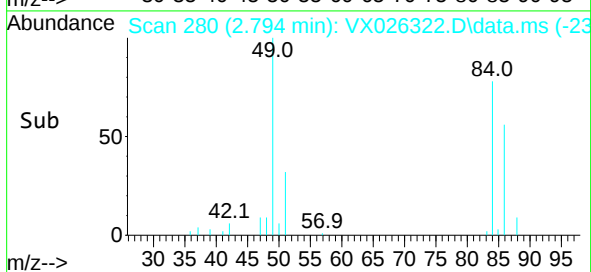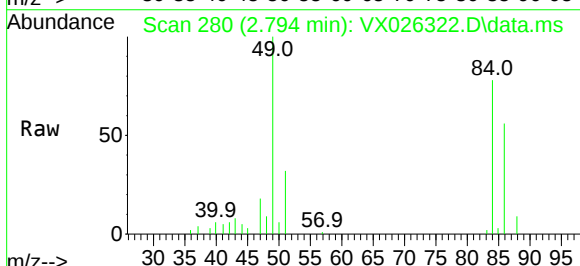






#22
Diisopropyl ether
Concen: 41.192 ug/l
RT: 3.702 min Scan# 41
Delta R.T. -0.068 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 45 Resp: 248413
Ion Ratio Lower Upper
45 100
43 5.0 63.8 95.6#
87 0.7 24.2 36.4#
59 194.9 9.4 14.2#




#23
Vinyl Acetate
Concen: 2.980 ug/l
RT: 3.696 min Scan# 428
Delta R.T. -0.031 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

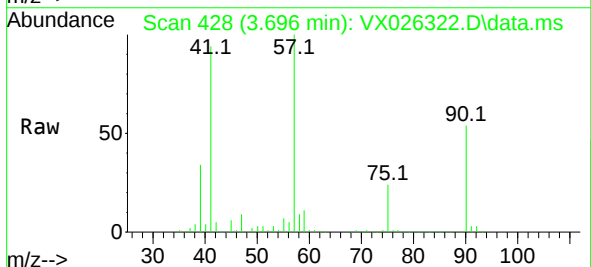

Tgt Ion: 43 Resp: 14272
Ion Ratio Lower Upper
43 100
86 2.0 9.0 13.6#









#24
1,1-Dichloroethane
Concen: 0.532 ug/l
RT: 3.696 min Scan# 415
Delta R.T. 0.079 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 63 Resp: 1738
Ion Ratio Lower Upper
63 100
98 0.0 3.3 9.9#
100 0.0 2.2 6.6#

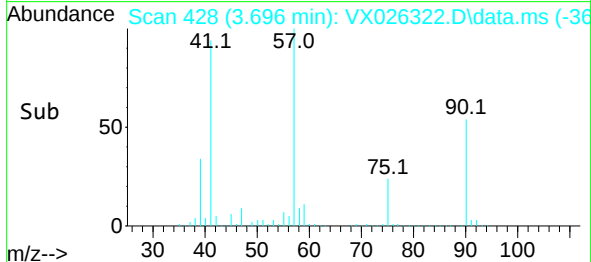

#25
2-Butanone
Concen: 17.287 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.006 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Tgt Ion: 43 Resp: 27254
Ion Ratio Lower Upper
43 100
72 26.1 21.0 31.4

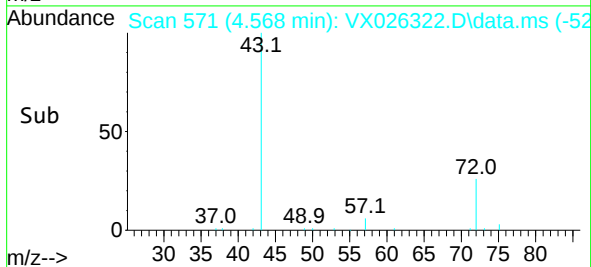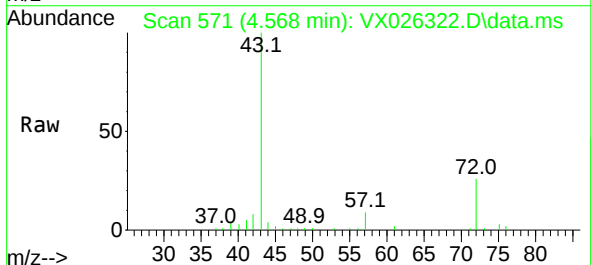



#29

Tetrahydrofuran

Concen: 0.328 ug/l

RT: 5.025 min Scan# 64

Delta R.T. 0.012 min


Lab File: VX026322.D

Acq: 05 Jan 2022 15:14




Instrument :

MSVOA_X

ClientSampleId :

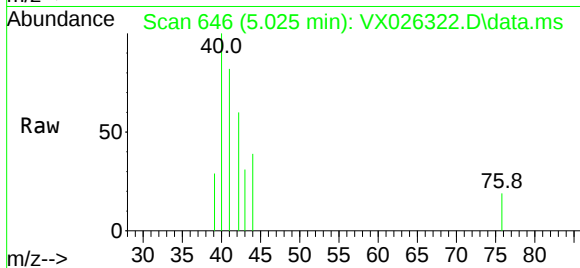

Tgt Ion:	42	Resp:	326
Ion Ratio	Lower	Upper	
42	100		
72	0.0	37.0	55.6#
71	0.0	34.1	51.1#

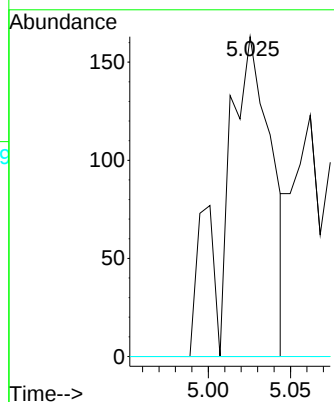

#31

Cyclohexane

Concen: 0.620 ug/l




RT: 5.470 min Scan# 719


Delta R.T. -0.007 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Tgt Ion:	56	Resp:	1844
Ion Ratio	Lower	Upper	
56	100		
69	23.5	23.9	35.9#
84	52.5	73.2	109.8#

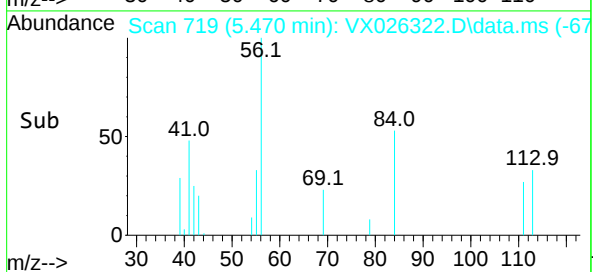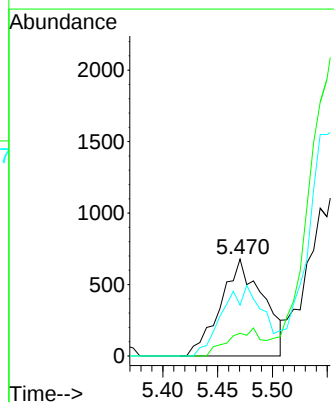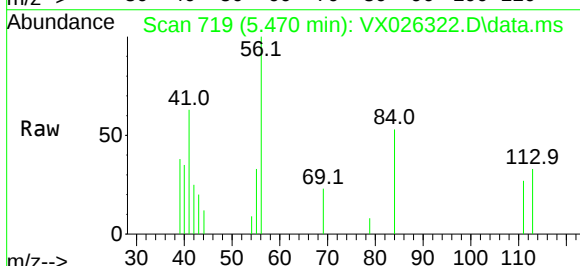



#33

1,2-Dichloroethane-d4

Concen: 50.035 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 104516

Ion Ratio Lower Upper

65 100

67 50.2 0.0 103.4

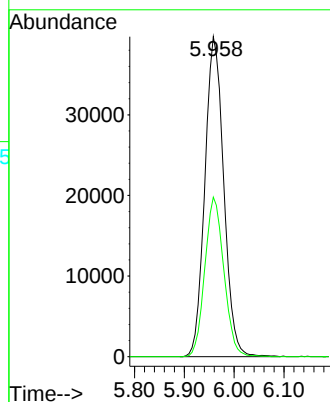

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14




Tgt Ion: 114 Resp: 242449


Ion Ratio Lower Upper

114 100

63 22.1 0.0 40.0

88 16.8 0.0 30.6

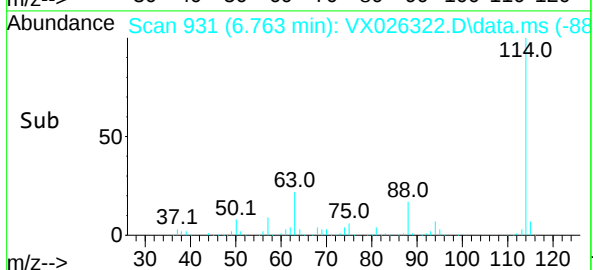



#35

Dibromofluoromethane

Concen: 50.225 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min


Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Instrument :

MSVOA_X

ClientSampleId :

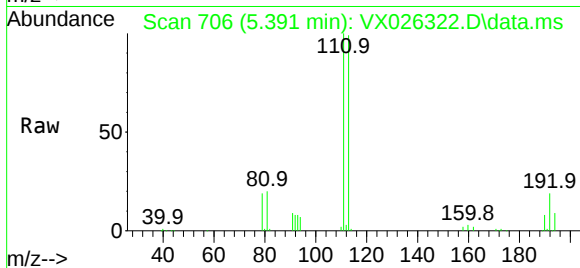




Tgt Ion:113 Resp: 79166

Ion Ratio Lower Upper

113 100

111 101.5 81.8 122.8

192 18.5 15.0 22.4

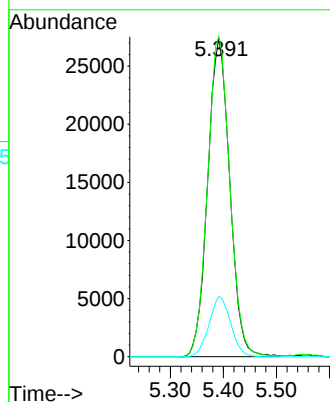

#36

1,1-Dichloropropene

Concen: 4.832 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.146 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14




Tgt Ion: 75 Resp: 12284


Ion Ratio Lower Upper

75 100

110 9.9 18.2 54.6#

77 0.0 24.7 37.1#

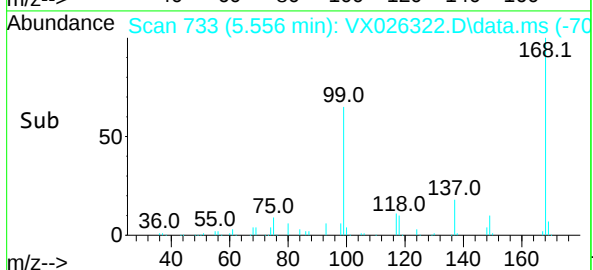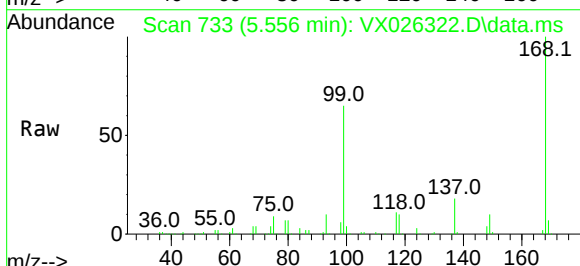



#37

Ethyl Acetate

Concen: 9.246 ug/l

RT: 4.568 min Scan# 51

Delta R.T. -0.153 min


Lab File: VX026322.D

Acq: 05 Jan 2022 15:14




Instrument :

MSVOA_X

ClientSampleId :

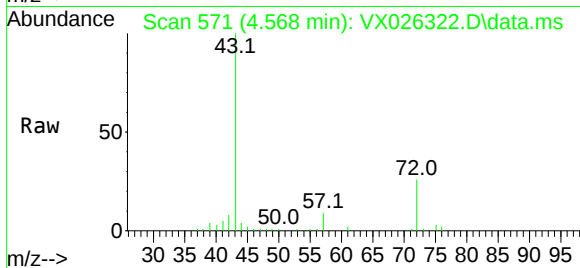

Tgt Ion: 43	Resp: 27254
Ion Ratio	Lower Upper
43	100
61	0.0 10.7 16.1#
70	0.0 8.5 12.7#

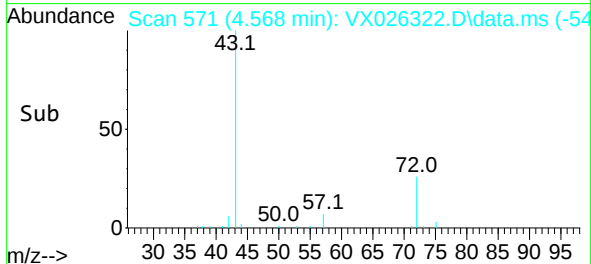

#38

Carbon Tetrachloride

Concen: 5.571 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.122 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Tgt Ion: 117	Resp: 15755
Ion Ratio	Lower Upper
117	100
119	4.0 77.2 115.8#
121	0.0 23.8 35.8#

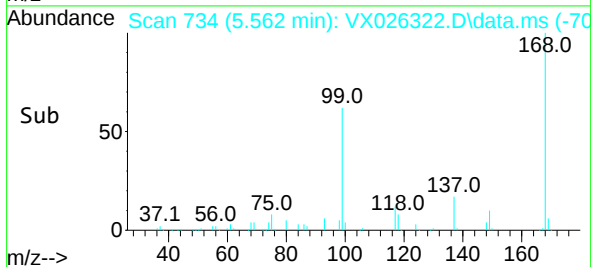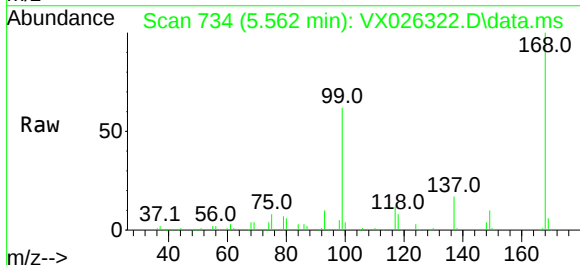



#39

Methylcyclohexane

Concen: 0.833 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. -0.000 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 2389

Ion Ratio Lower Upper

83 100

55 87.7 57.8 86.8#

98 50.6 40.5 60.7

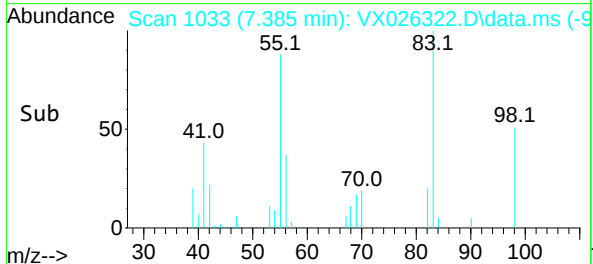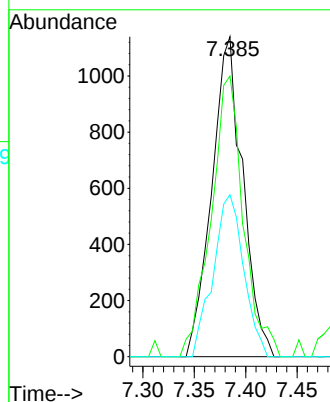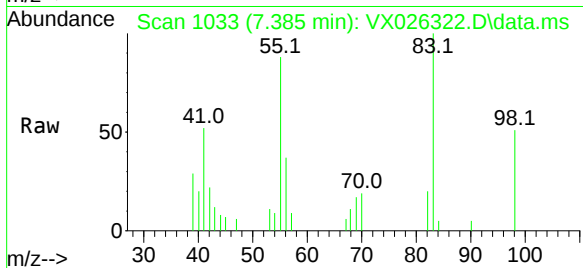

#40

Benzene

Concen: 48.148 ug/l

RT: 6.043 min Scan# 813

Delta R.T. -0.000 min

Lab File: VX026322.D




Acq: 05 Jan 2022 15:14


Tgt Ion: 78 Resp: 349348

Ion Ratio Lower Upper

78 100

77 24.7 18.6 27.8

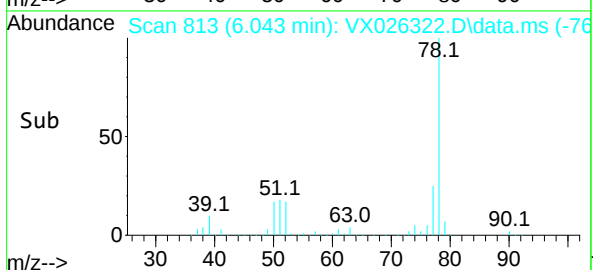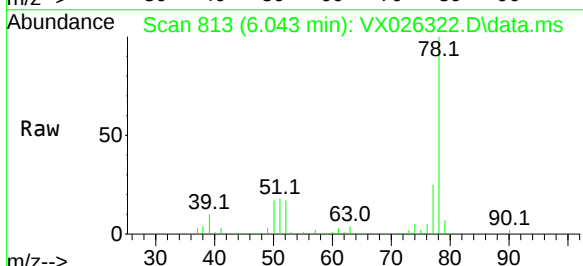



#42

1,2-Dichloroethane

Concen: 1.977 ug/l

RT: 6.050 min Scan# 81

Delta R.T. -0.042 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 62 Resp: 5805

Ion Ratio Lower Upper

62 100

98 0.0 0.0 18.8

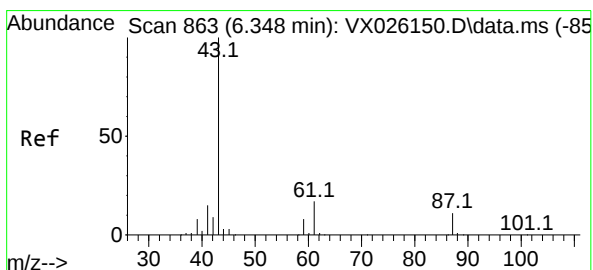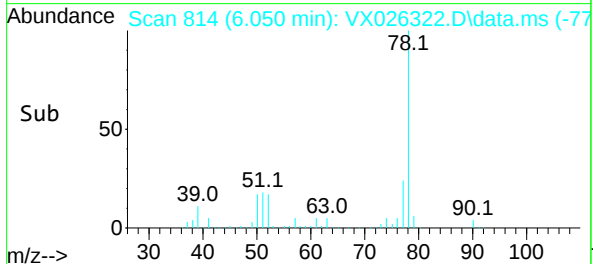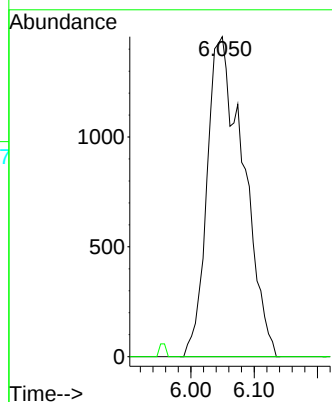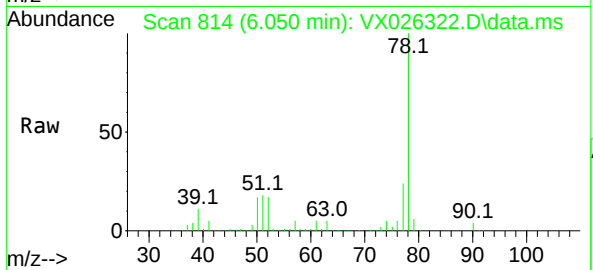

#43

Isopropyl Acetate

Concen: 2.180 ug/l

RT: 6.336 min Scan# 861

Delta R.T. -0.012 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14




Tgt Ion: 43 Resp: 10472


Ion Ratio Lower Upper

43 100

61 0.0 15.7 23.5#

87 6.3 11.2 16.8#

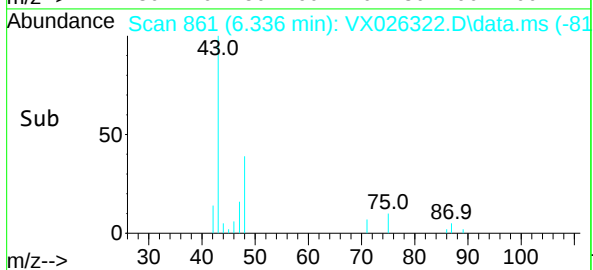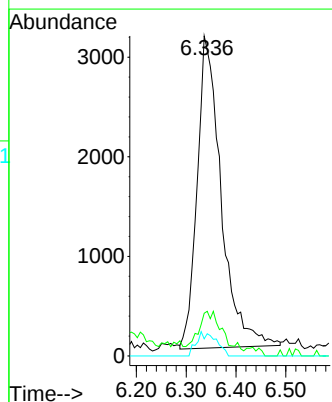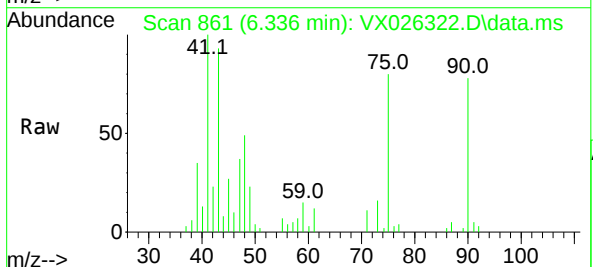



#48

Methyl methacrylate

Concen: 45.576 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. -0.006 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 41 Resp: 105012

Ion Ratio Lower Upper

41 100

69 0.7 67.3 100.9#

39 31.9 50.2 75.2#

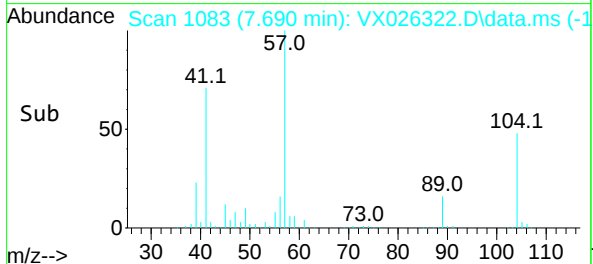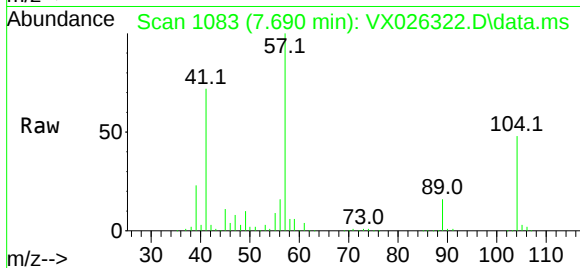

#49

1,4-Dioxane

Concen: 6.453 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. 0.006 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14




Tgt Ion: 88 Resp: 274


Ion Ratio Lower Upper

88 100

43 0.0 25.3 37.9#

58 3400.7 51.8 77.6#

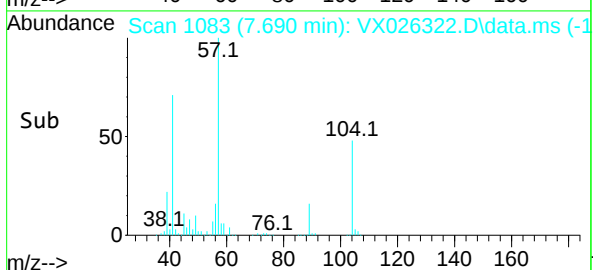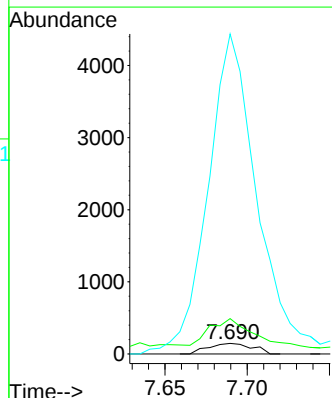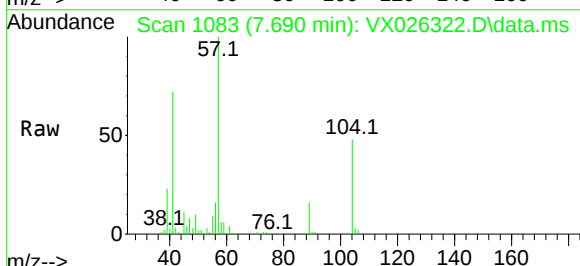



#50

Toluene-d8

Concen: 48.596 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX026322.D

Acq: 05 Jan 2022 15:14

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 98 Resp: 284917

Ion Ratio Lower Upper

98 100

100 65.9 52.6 78.8

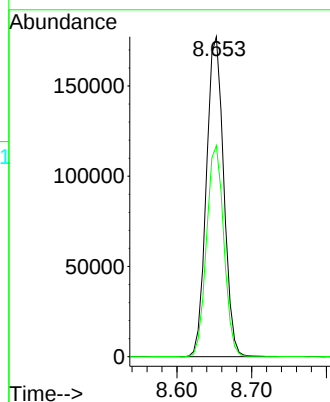

#51

4-Methyl-2-Pentanone

Concen: 3.420 ug/l

RT: 8.555 min Scan# 1225

Delta R.T. -0.025 min

Lab File: VX026322.D




Acq: 05 Jan 2022 15:14


Tgt Ion: 43 Resp: 10226

Ion Ratio Lower Upper

43 100


58 5.5 30.8 46.2#

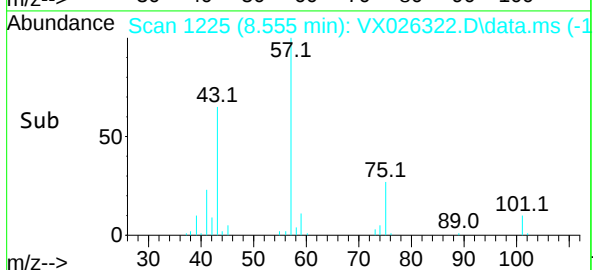






#52
Toluene
Concen: 305.624 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 92 Resp: 1365172
Ion Ratio Lower Upper
92 100
91 167.2 136.0 204.0

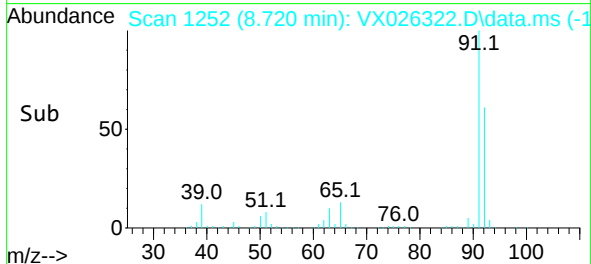

#53
t-1,3-Dichloropropene
Concen: 2.077 ug/l
RT: 9.080 min Scan# 1311
Delta R.T. 0.098 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Tgt Ion: 75 Resp: 570
Ion Ratio Lower Upper
75 100
77 31.8 25.1 37.7


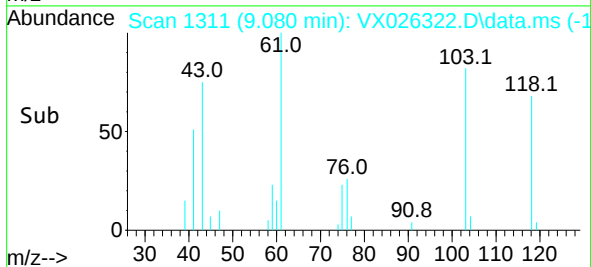

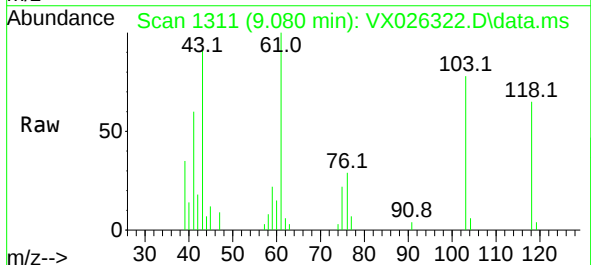




#58
2-Chloroethyl Vinyl ether
Concen: 10.068 ug/l
RT: 8.336 min Scan# 1174
Delta R.T. 0.092 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 63 Resp: 377
Ion Ratio Lower Upper
63 100
106 0.0 24.4 36.6#

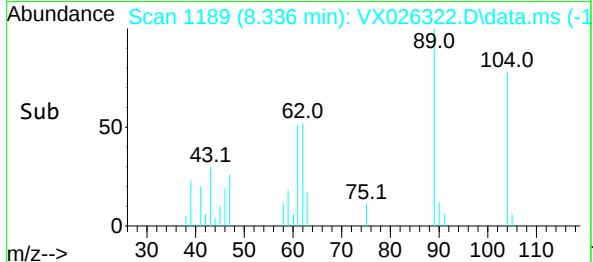

#59
2-Hexanone
Concen: 0.522 ug/l
RT: 9.445 min Scan# 1371
Delta R.T. 0.012 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Tgt Ion: 43 Resp: 1183
Ion Ratio Lower Upper
43 100
58 70.6 26.9 80.6


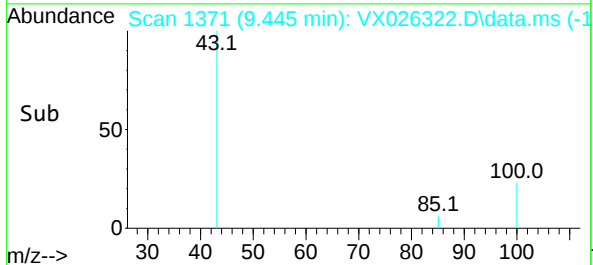

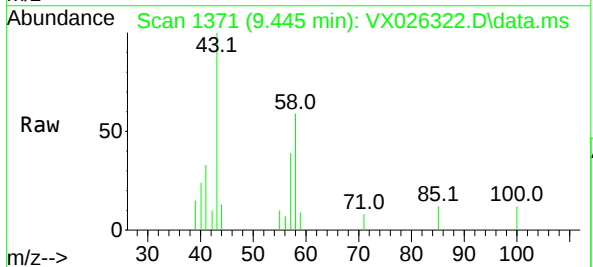




#62
4-Bromofluorobenzene
Concen: 54.997 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 114787
Ion Ratio Lower Upper
95 100
174 71.9 0.0 157.4
176 69.1 0.0 154.6

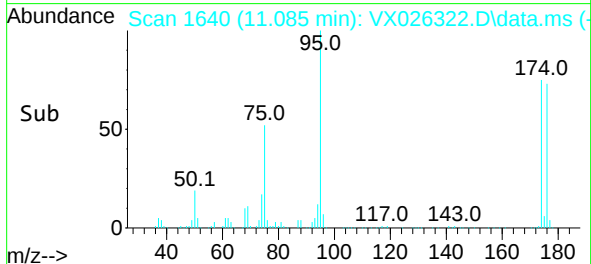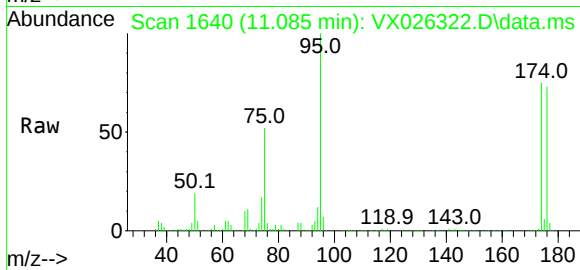

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Tgt Ion: 117 Resp: 214662
Ion Ratio Lower Upper
117 100
82 59.7 43.8 65.6
119 32.5 25.2 37.8




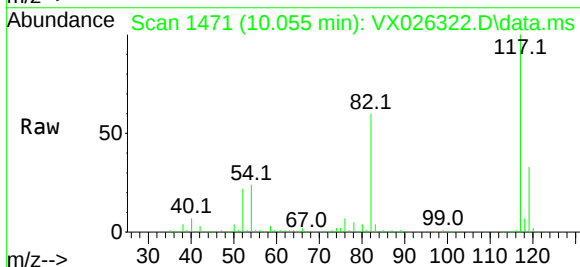




#67
Ethyl Benzene
Concen: 6.810 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 57420
Ion Ratio Lower Upper
91 100
106 29.5 25.7 38.5

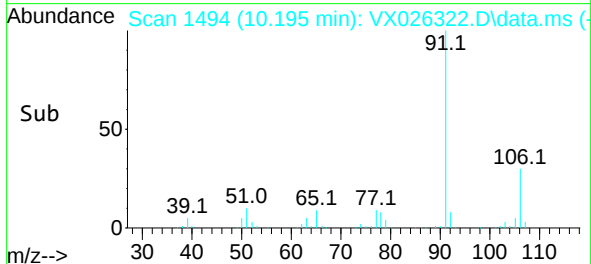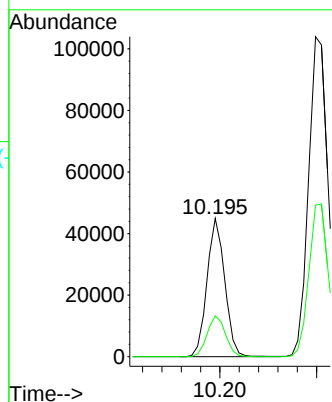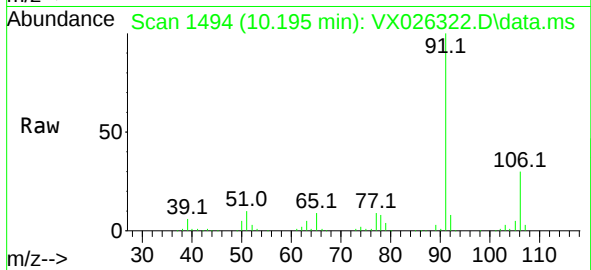

#68
m/p-Xylenes
Concen: 21.896 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14

Tgt Ion:106 Resp: 68934
Ion Ratio Lower Upper
106 100
91 208.6 158.6 238.0


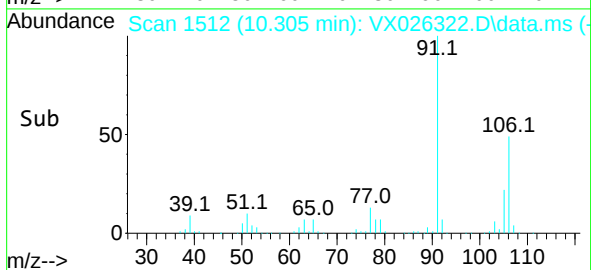
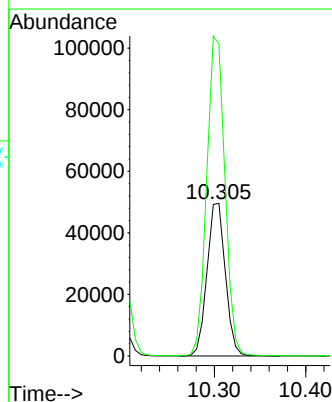
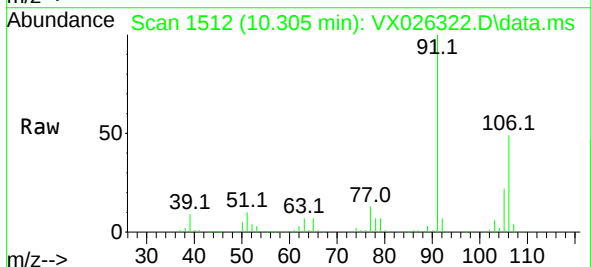




#69
o-Xylene
Concen: 8.006 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 24660
Ion Ratio Lower Upper
106 100
91 232.9 105.5 316.4

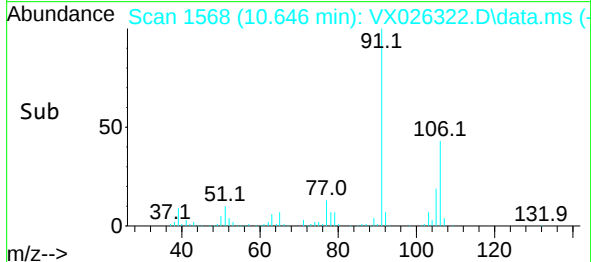

#70
Styrene
Concen: 0.292 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.013 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14


Tgt Ion:104 Resp: 1475
Ion Ratio Lower Upper
104 100
78 281.4 39.8 59.6#
103 252.9 43.0 64.6#

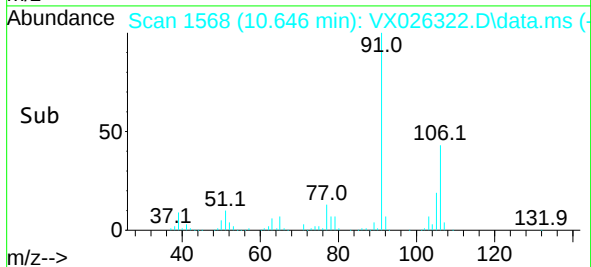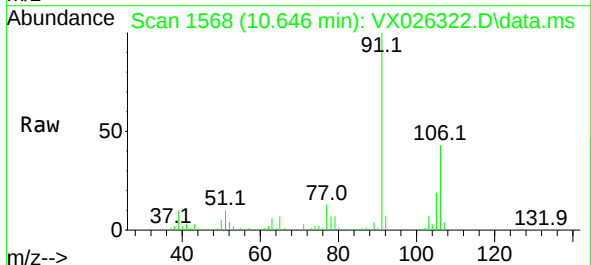






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX026322.D
 Acq: 05 Jan 2022 15:14

Instrument :
 MSVOA_X
 ClientSampleId :



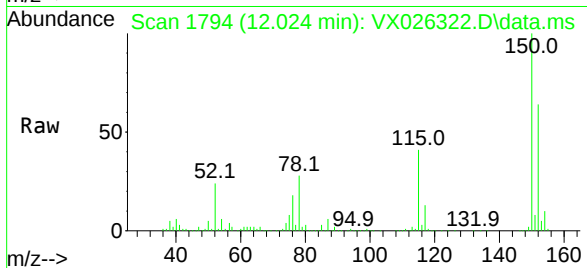



Tgt Ion:152 Resp: 104976
 Ion Ratio Lower Upper
 152 100
 115 61.6 41.3 123.9
 150 157.9 0.0 351.8

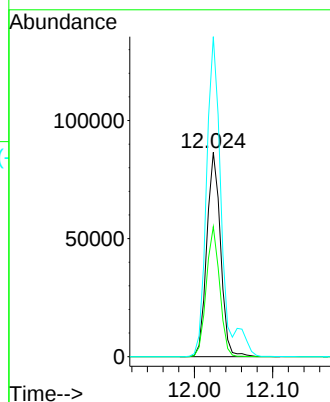

#76
 1,2,3-Trichloropropane
 Concen: 23.601 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. -0.159 min
 Lab File: VX026322.D
 Acq: 05 Jan 2022 15:14

Tgt Ion: 75 Resp: 59801
 Ion Ratio Lower Upper
 75 100
 77 1.2 19.0 57.0#



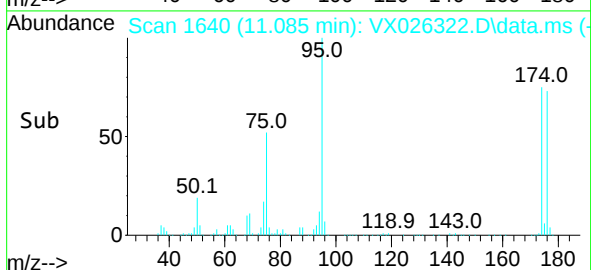
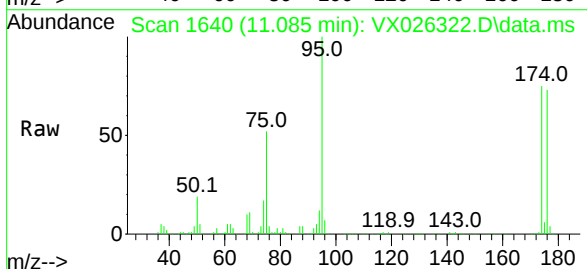




#81
trans-1,4-Dichloro-2-butene
Concen: 68.277 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 59801
Ion Ratio Lower Upper
75 100
53 0.0 79.5 119.3#
89 0.0 38.3 57.5#

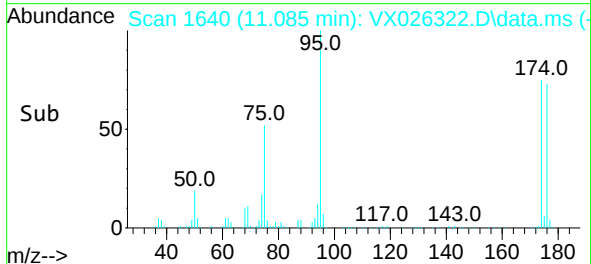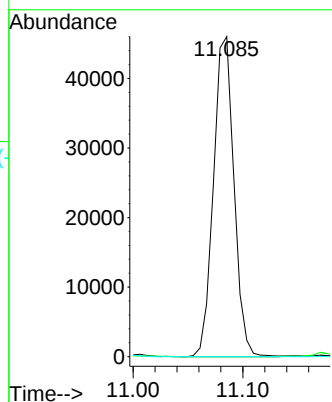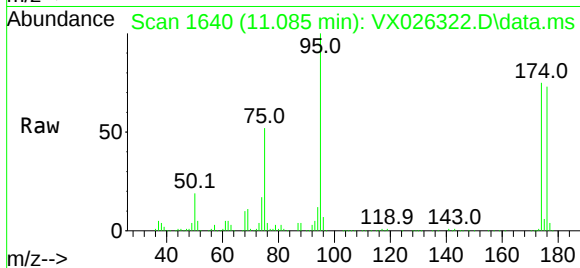

#84
1,2,4-Trimethylbenzene
Concen: 0.259 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX026322.D
Acq: 05 Jan 2022 15:14


Tgt Ion: 105 Resp: 1751
Ion Ratio Lower Upper
105 100
120 23.4 22.9 68.7

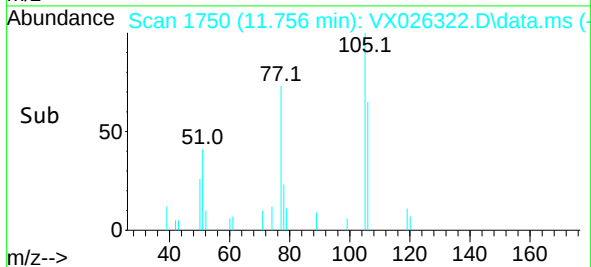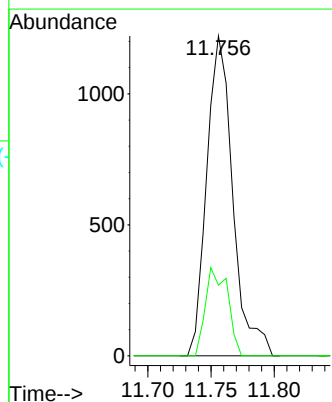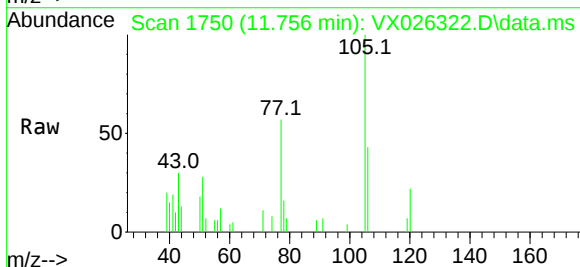



#92
 1,2-Dibromo-3-Chloropropane
 Concen: 2.128 ug/l
 RT: 12.993 min Scan# 1953
 Delta R.T. 0.048 min
 Lab File: VX026322.D
 Acq: 05 Jan 2022 15:14

Instrument :
 MSVOA_X
 ClientSampleId :



Tgt Ion: 75 Resp: 1512
 Ion Ratio Lower Upper
 75 100
 155 0.0 44.0 131.8#
 157 0.0 55.5 166.5#

