

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
 Data File : VX026357.D
 Acq On : 06 Jan 2022 05:30
 Operator : JC/MD
 Sample : N1020-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 06 12:22:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	149094	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	247603	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	214438	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	94932	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	106499	49.375	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.740%
35) Dibromofluoromethane	5.391	113	79629	49.467	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.940%
50) Toluene-d8	8.653	98	285388	47.663	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.320%
62) 4-Bromofluorobenzene	11.079	95	107755	50.553	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	101.100%
Target Compounds						
					Qvalue	
3) Chloromethane	1.270	50	458	0.251	ug/l	89
6) Chloroethane	1.538	64	31589	23.418	ug/l #	51
11) Tert butyl alcohol	2.983	59	776	1.801	ug/l #	73
13) Acrolein	2.221	56	7890	51.217	ug/l #	1
14) Allyl chloride	2.758	41	18960	5.811	ug/l #	15
15) Acrylonitrile	3.105	53	571	0.535	ug/l #	26
16) Acetone	2.386	43	18724	16.022	ug/l	96
17) Carbon Disulfide	2.538	76	1335	0.282	ug/l #	93
18) Methyl Acetate	2.715	43	2129	0.562	ug/l #	51
20) Methylene Chloride	2.721	84	902	Below Cal	#	15
23) Vinyl Acetate	3.739	43	1903	0.385	ug/l #	70
25) 2-Butanone	4.574	43	2147	1.319	ug/l #	88
26) 2,2-Dichloropropane	4.312	77	717	0.282	ug/l #	52
30) Chloroform	5.190	83	2538	0.711	ug/l #	19
31) Cyclohexane	5.477	56	32912	10.715	ug/l	91
36) 1,1-Dichloropropene	5.562	75	12398	4.775	ug/l #	50
38) Carbon Tetrachloride	5.562	117	16075	5.566	ug/l #	15
39) Methylcyclohexane	7.379	83	6604	2.255	ug/l #	84
40) Benzene	6.044	78	810857	109.427	ug/l	99
42) 1,2-Dichloroethane	6.044	62	8204	2.736	ug/l #	74
48) Methyl methacrylate	7.659	41	765	0.325	ug/l #	77
51) 4-Methyl-2-Pentanone	8.574	43	616	0.202	ug/l #	70
52) Toluene	8.720	92	159233	34.906	ug/l	100
53) t-1,3-Dichloropropene	8.720	75	2226	2.597	ug/l #	1
58) 2-Chloroethyl Vinyl ether	8.190	63	53	9.862	ug/l #	44
59) 2-Hexanone	9.458	43	693	0.300	ug/l	92
67) Ethyl Benzene	10.195	91	1221370	145.004	ug/l	98
68) m/p-Xylenes	10.305	106	648620	206.239	ug/l	94
69) o-Xylene	10.640	106	224577	72.982	ug/l	92
70) Styrene	10.646	104	11955	2.370	ug/l #	1
73) Isopropylbenzene	10.963	105	27872	3.777	ug/l	98
76) 1,2,3-Trichloropropane	11.378	75	2041	0.891	ug/l #	1
78) n-propylbenzene	11.305	91	44626	5.260	ug/l	97
79) 2-Chlorotoluene	11.378	91	26365	5.048	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	84206	13.751	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	55850	70.513	ug/l #	10

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
 Data File : VX026357.D
 Acq On : 06 Jan 2022 05:30
 Operator : JC/MD
 Sample : N1020-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 06 12:22:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


82) 4-Chlorotoluene	11.451	91	9041	1.533	ug/l #	44
83) tert-Butylbenzene	11.756	119	53781	9.048	ug/l #	51
84) 1,2,4-Trimethylbenzene	11.750	105	453026	74.039	ug/l	98
85) sec-Butylbenzene	11.750	105	453026	61.076	ug/l #	56
86) p-Isopropyltoluene	11.975	119	3168	0.512	ug/l #	75
89) n-Butylbenzene	12.317	91	2633	0.479	ug/l #	1
90) Hexachloroethane	12.701	117	23737	19.220	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	12.963	75	146	0.227	ug/l #	1
95) Naphthalene	13.780	128	240952	32.841	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
Data File : VX026357.D
Acq On : 06 Jan 2022 05:30
Operator : JC/MD
Sample : N1020-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 06 12:22:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration

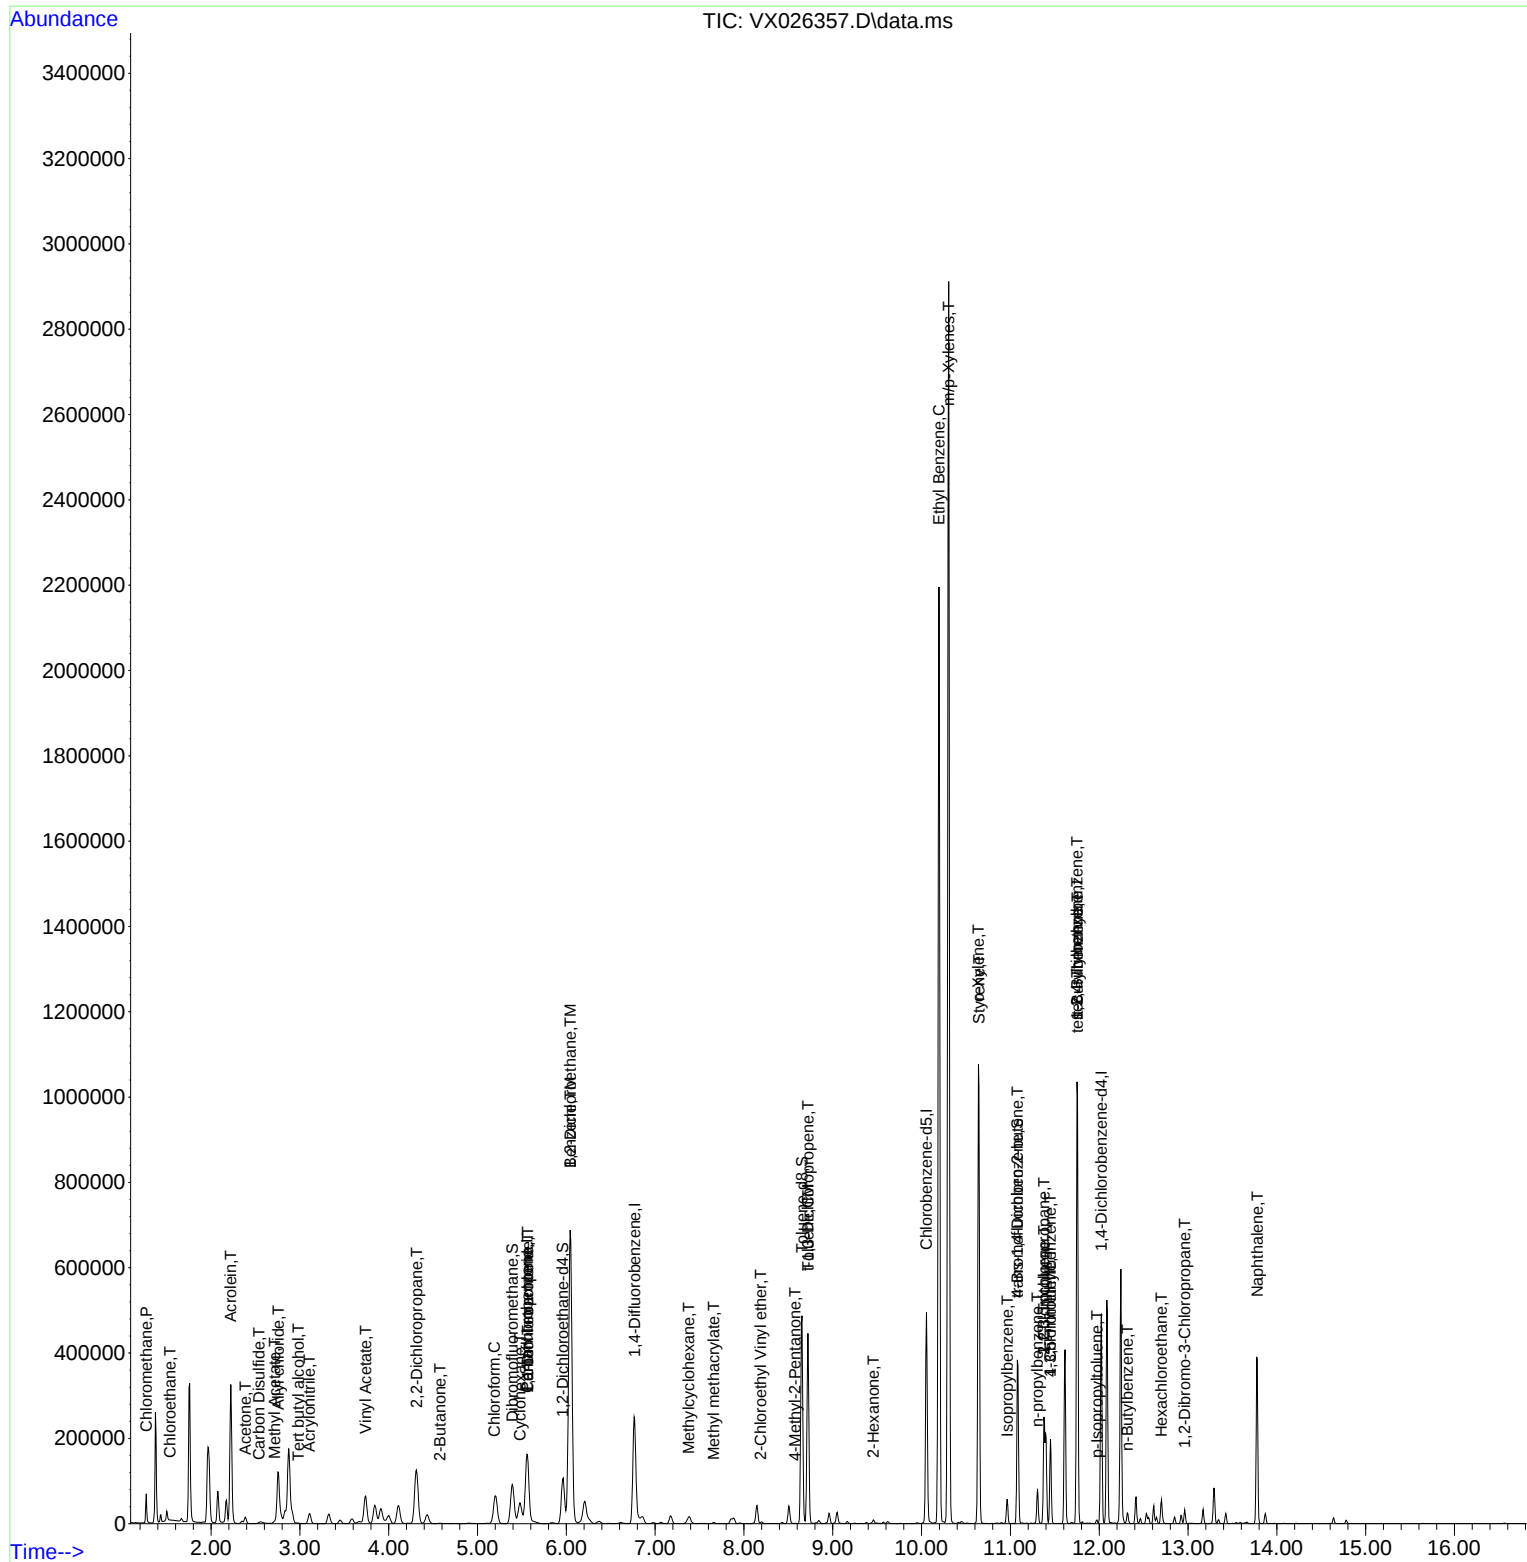






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Instrument :
MSVOA_X
ClientSampleId :






Tgt Ion:168 Resp: 149094
Ion Ratio Lower Upper
168 100
99 63.6 45.8 68.8




#3
Chloromethane
Concen: 0.251 ug/l
RT: 1.270 min Scan# 30
Delta R.T. -0.024 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 50 Resp: 458
Ion Ratio Lower Upper
50 100
52 25.6 25.4 38.0

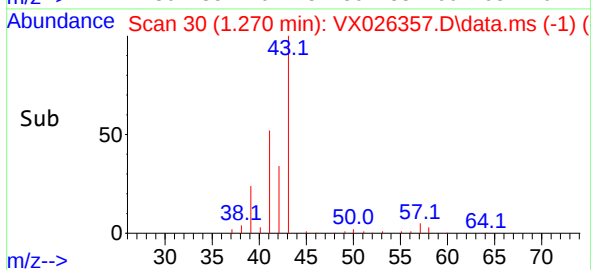





Abundance Scan 99 (1.691 min): VX026150.D\data.ms (-93)

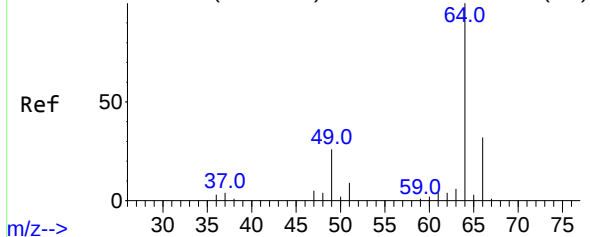

#6
Chloroethane
Concen: 23.418 ug/l
RT: 1.538 min Scan# 74
Delta R.T. -0.153 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 64 Resp: 31589
Ion Ratio Lower Upper
64 100
66 4.9 25.9 38.9#

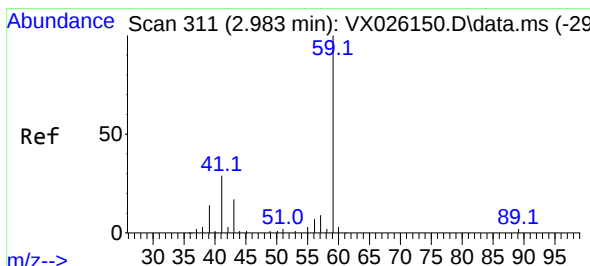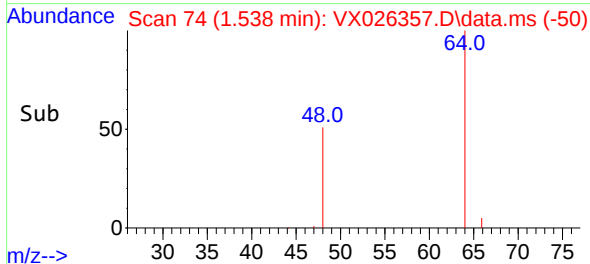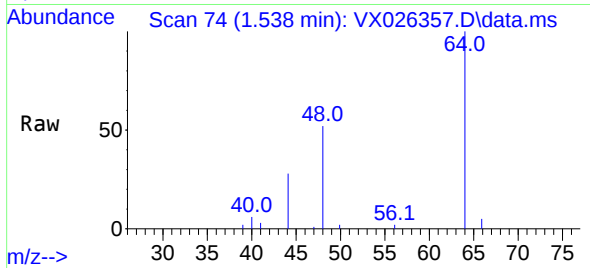

#11
Tert butyl alcohol
Concen: 1.801 ug/l
RT: 2.983 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30


Tgt Ion: 59 Resp: 776
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

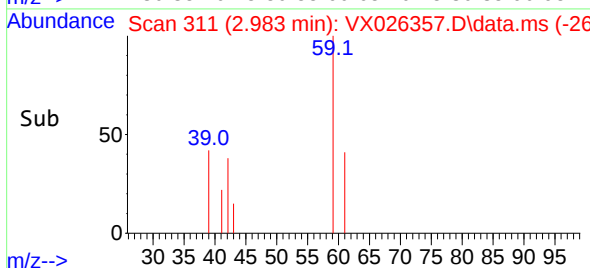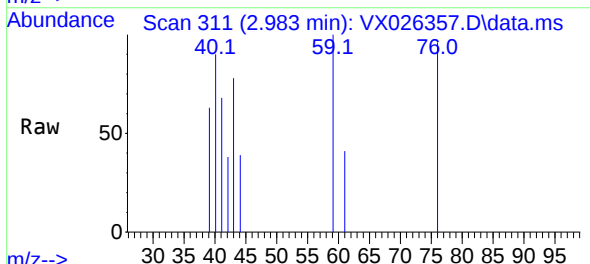






#13
Acrolein
Concen: 51.217 ug/l
RT: 2.221 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 7890
Ion Ratio Lower Upper
56 100
55 2180.6 57.4 86.2#



#14
Allyl chloride
Concen: 5.811 ug/l
RT: 2.758 min Scan# 274
Delta R.T. 0.086 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 41 Resp: 18960
Ion Ratio Lower Upper
41 100
39 148.2 55.4 83.0#
76 0.0 27.6 41.4#


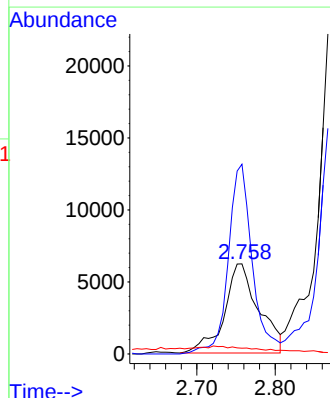






#15
Acrylonitrile
Concen: 0.535 ug/l
RT: 3.105 min Scan# 31
Delta R.T. 0.036 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 53 Resp: 571
Ion Ratio Lower Upper
53 100
52 0.0 66.2 99.2#
51 56.9 29.4 44.0#



#16
Acetone
Concen: 16.022 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30


Tgt Ion: 43 Resp: 18724
Ion Ratio Lower Upper
43 100
58 28.7 24.8 37.2








#17
Carbon Disulfide
Concen: 0.282 ug/l
RT: 2.538 min Scan# 21
Delta R.T. 0.024 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 76 Resp: 1335
Ion Ratio Lower Upper
76 100
78 11.5 7.2 10.8#

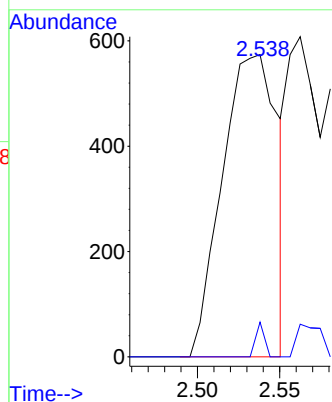

#18
Methyl Acetate
Concen: 0.562 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30


Tgt Ion: 43 Resp: 2129
Ion Ratio Lower Upper
43 100
74 0.0 19.1 28.7#

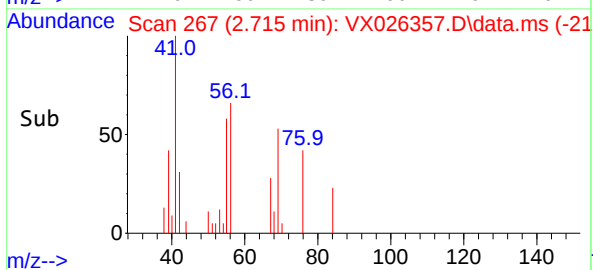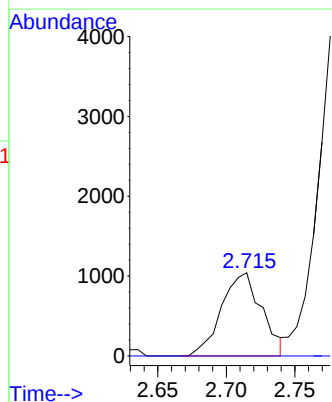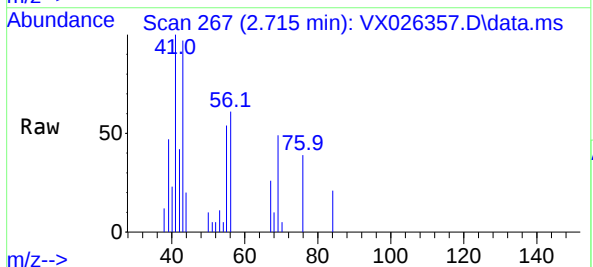






#20
Methylene Chloride
Concen: Below Cal
RT: 2.721 min Scan# 20
Delta R.T. -0.073 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion: 84 Resp: 902




Ion	Ratio	Lower	Upper
84	100		
49	0.0	97.1	145.7#
51	30.1	29.3	43.9
86	0.0	50.8	76.2#




#23
Vinyl Acetate
Concen: 0.385 ug/l
RT: 3.739 min Scan# 435
Delta R.T. 0.012 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 43 Resp: 1903

Ion	Ratio	Lower	Upper
43	100		
86	0.0	9.0	13.6#

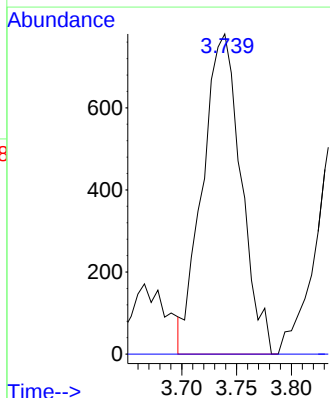

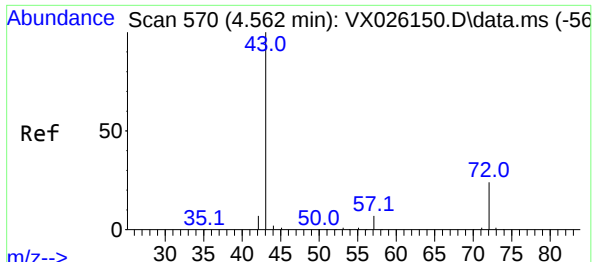

#25

2-Butanone

Concen: 1.319 ug/l

RT: 4.574 min Scan# 51

Delta R.T. 0.012 min

Lab File: VX026357.D

Acq: 06 Jan 2022 05:30

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 2147

Ion Ratio Lower Upper

43 100

72 20.2 21.0 31.4#

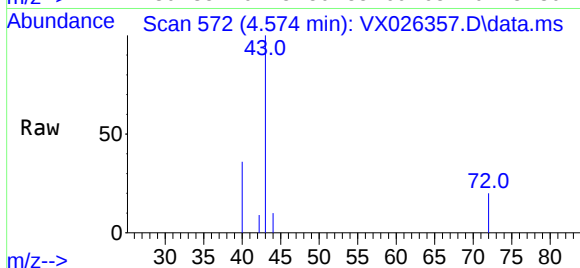

#26

2,2-Dichloropropane

Concen: 0.282 ug/l

RT: 4.312 min Scan# 529

Delta R.T. -0.171 min

Lab File: VX026357.D




Acq: 06 Jan 2022 05:30


Tgt Ion: 77 Resp: 717

Ion Ratio Lower Upper

77 100

97 0.0 11.7 35.0#


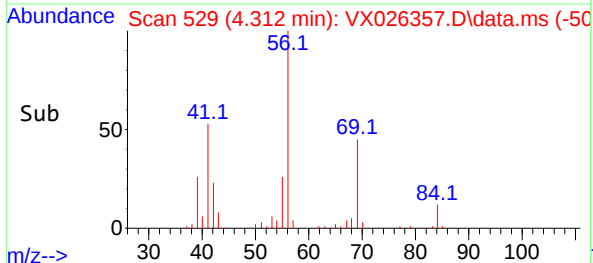
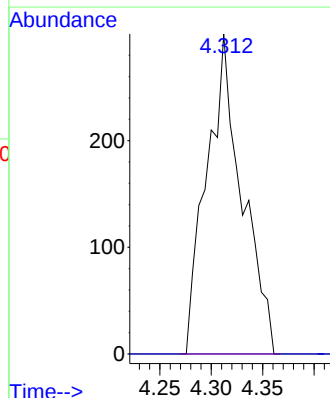
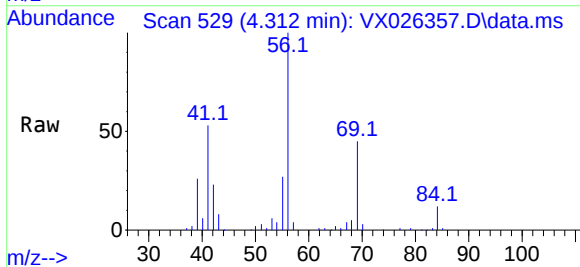




#30
Chloroform
Concen: 0.711 ug/l
RT: 5.190 min Scan# 61
Delta R.T. 0.085 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 83 Resp: 2538
Ion Ratio Lower Upper
83 100
85 0.0 50.6 75.8#



#31
Cyclohexane
Concen: 10.715 ug/l
RT: 5.477 min Scan# 720
Delta R.T. -0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 56 Resp: 32912
Ion Ratio Lower Upper
56 100
69 27.9 23.9 35.9
84 81.9 73.2 109.8

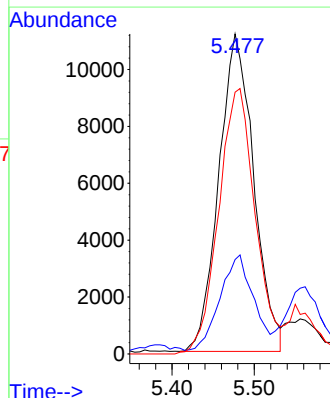



#33

1,2-Dichloroethane-d4

Concen: 49.375 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX026357.D

Acq: 06 Jan 2022 05:30

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 106499

Ion Ratio Lower Upper

65 100

67 49.9 0.0 103.4

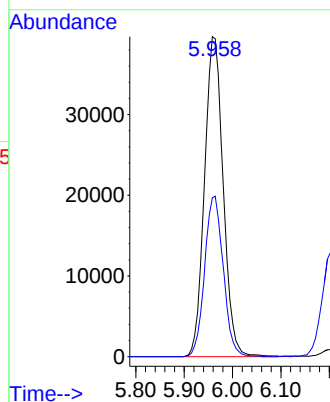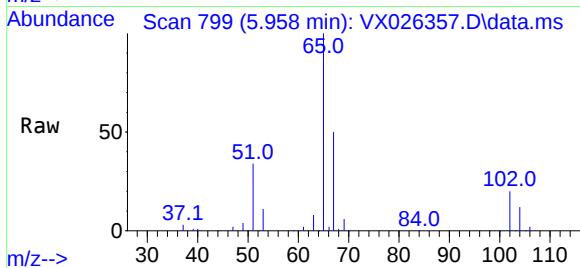

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX026357.D

Acq: 06 Jan 2022 05:30




Tgt Ion: 114 Resp: 247603


Ion Ratio Lower Upper

114 100

63 21.8 0.0 40.0


88 16.5 0.0 30.6

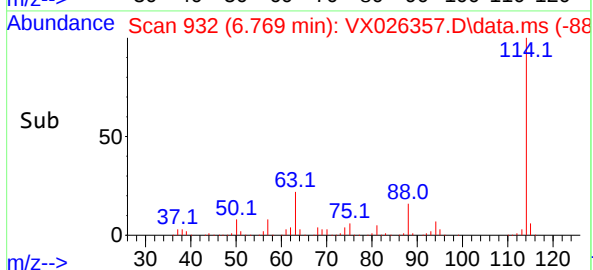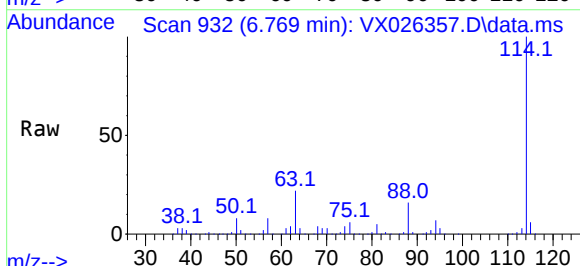



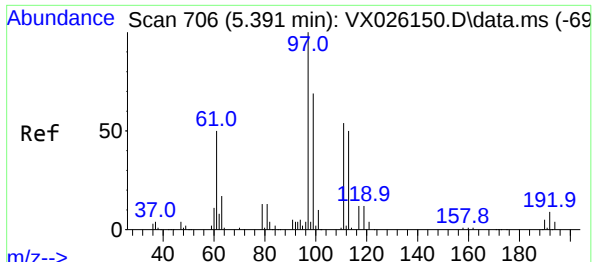


#35
Dibromofluoromethane
Concen: 49.467 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Instrument :
MSVOA_X
ClientSampleId :



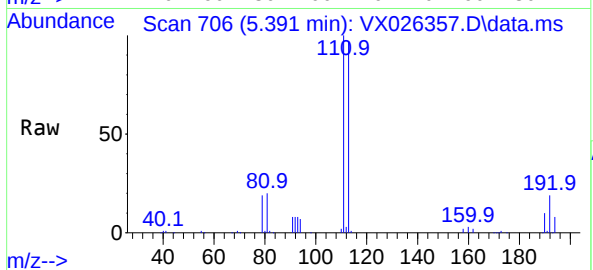



Tgt Ion:113 Resp: 79629
Ion Ratio Lower Upper
113 100
111 103.2 81.8 122.8
192 18.7 15.0 22.4

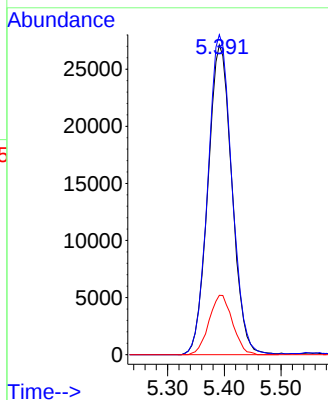

#36
1,1-Dichloropropene
Concen: 4.775 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30


Tgt Ion: 75 Resp: 12398
Ion Ratio Lower Upper
75 100
110 9.7 18.2 54.6#
77 0.0 24.7 37.1#

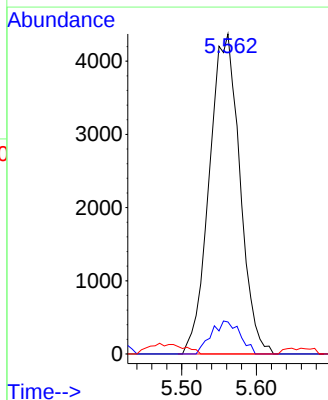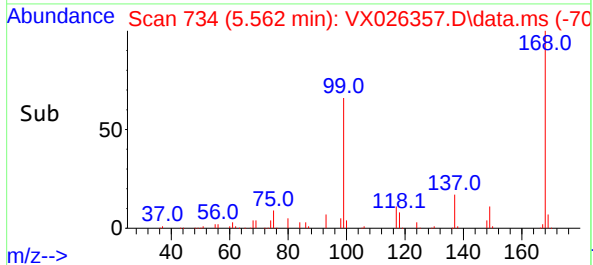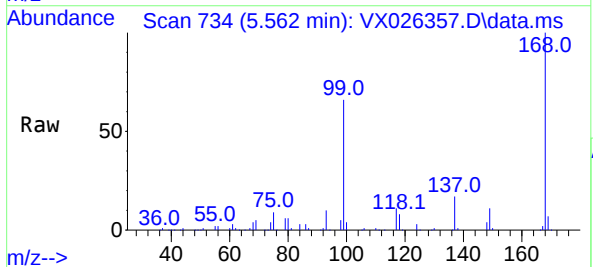



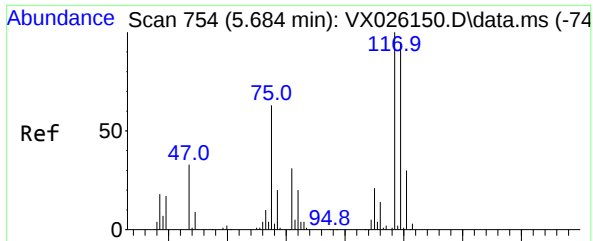


#38
Carbon Tetrachloride
Concen: 5.566 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Instrument :
MSVOA_X
ClientSampleId :



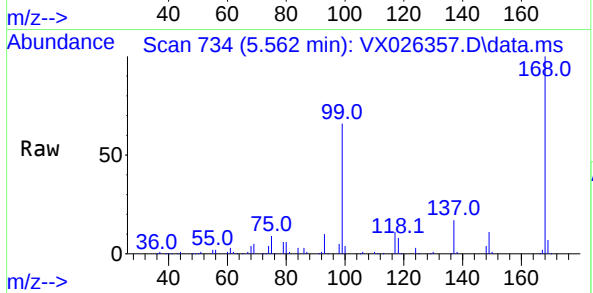



Tgt Ion:117 Resp: 16075
Ion Ratio Lower Upper
117 100
119 3.5 77.2 115.8#
121 0.0 23.8 35.8#



#39
Methylcyclohexane
Concen: 2.255 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 83 Resp: 6604
Ion Ratio Lower Upper
83 100
55 88.7 57.8 86.8#
98 43.7 40.5 60.7


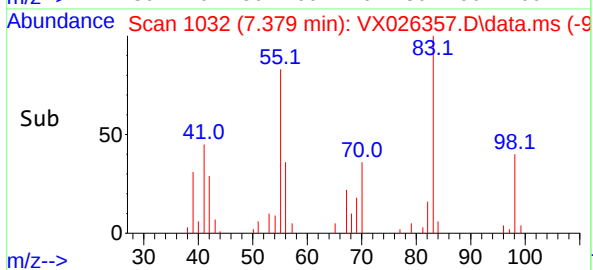

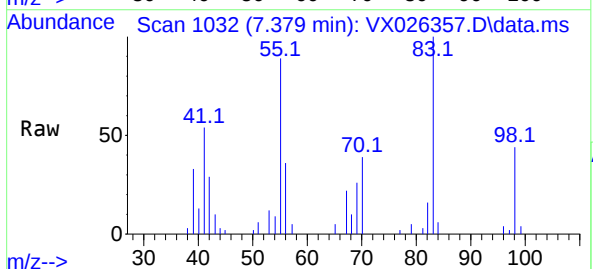




#40
Benzene
Concen: 109.427 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 78 Resp: 810857
Ion Ratio Lower Upper
78 100
77 23.5 18.6 27.8

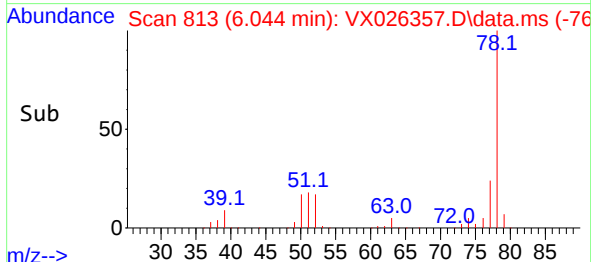

#42
1,2-Dichloroethane
Concen: 2.736 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.048 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 62 Resp: 8204
Ion Ratio Lower Upper
62 100
98 0.0 0.0 18.8

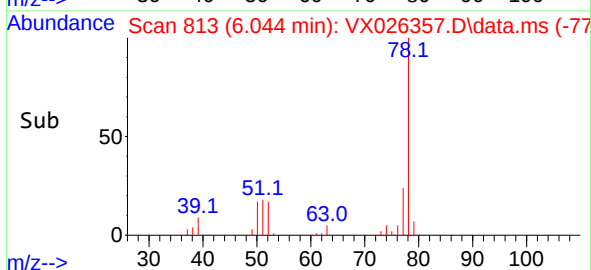



#48

Methyl methacrylate

Concen: 0.325 ug/l

RT: 7.659 min Scan# 1084

Delta R.T. -0.037 min

Lab File: VX026357.D

Acq: 06 Jan 2022 05:30

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 41 Resp: 765

Ion Ratio Lower Upper

41 100

69 113.2 67.3 100.9#

39 54.0 50.2 75.2



#50

Toluene-d8

Concen: 47.663 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX026357.D




Acq: 06 Jan 2022 05:30


Tgt Ion: 98 Resp: 285388

Ion Ratio Lower Upper

98 100

100 66.2 52.6 78.8

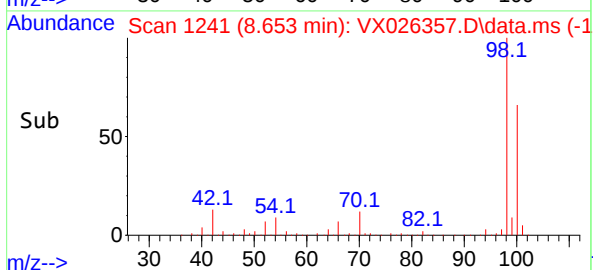



#51

4-Methyl-2-Pentanone

Concen: 0.202 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. -0.006 min

Lab File: VX026357.D

Acq: 06 Jan 2022 05:30

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 616

Ion Ratio Lower Upper

43 100

58 20.1 30.8 46.2#



#52

Toluene

Concen: 34.906 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX026357.D




Acq: 06 Jan 2022 05:30


Tgt Ion: 92 Resp: 159233

Ion Ratio Lower Upper

92 100

91 169.8 136.0 204.0

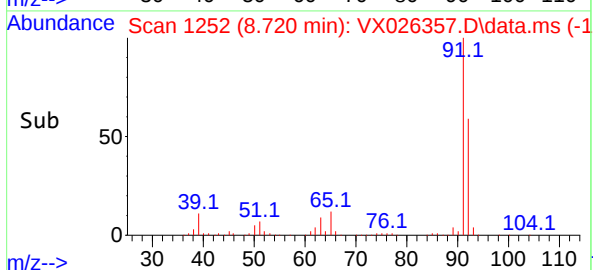



#53

t-1,3-Dichloropropene

Concen: 2.597 ug/l

RT: 8.720 min Scan# 1165

Delta R.T. -0.262 min

Lab File: VX026357.D

Acq: 06 Jan 2022 05:30

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 2226

Ion Ratio Lower Upper

75 100

77 159.5 25.1 37.7#

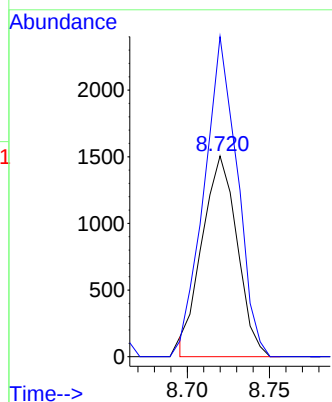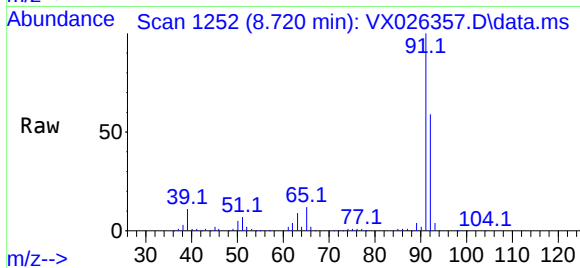

#58

2-Chloroethyl Vinyl ether

Concen: 9.862 ug/l

RT: 8.190 min Scan# 1165

Delta R.T. -0.054 min

Lab File: VX026357.D




Acq: 06 Jan 2022 05:30


Tgt Ion: 63 Resp: 53

Ion Ratio Lower Upper

63 100

106 0.0 24.4 36.6#

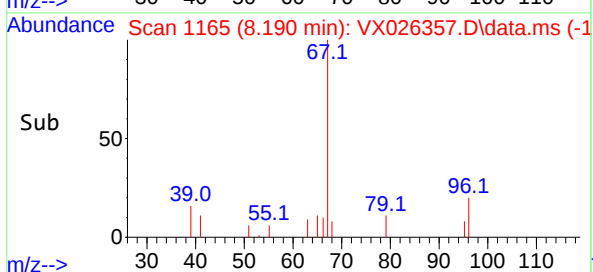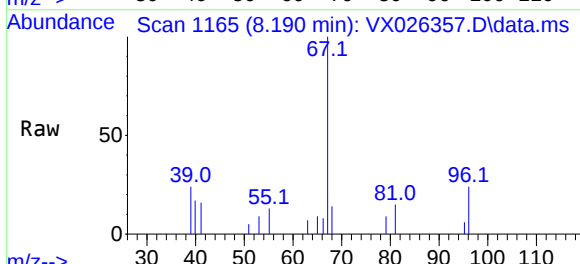



#59

2-Hexanone

Concen: 0.300 ug/l

RT: 9.458 min Scan# 1

Delta R.T. 0.025 min

Lab File: VX026357.D

Acq: 06 Jan 2022 05:30

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 693

Ion Ratio Lower Upper

43 100

58 48.2 26.9 80.6

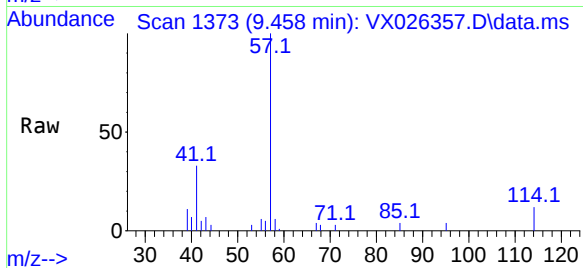

#62

4-Bromofluorobenzene

Concen: 50.553 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX026357.D

Acq: 06 Jan 2022 05:30




Tgt Ion: 95 Resp: 107755


Ion Ratio Lower Upper

95 100

174 71.6 0.0 157.4


176 68.7 0.0 154.6

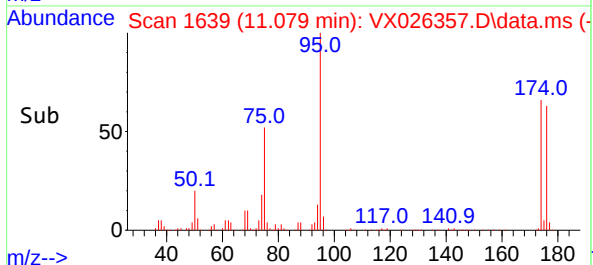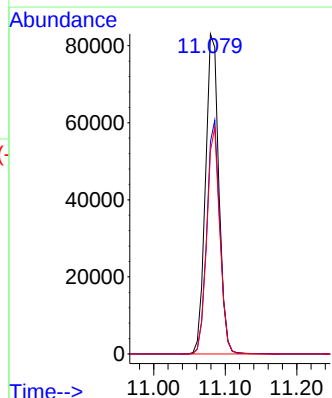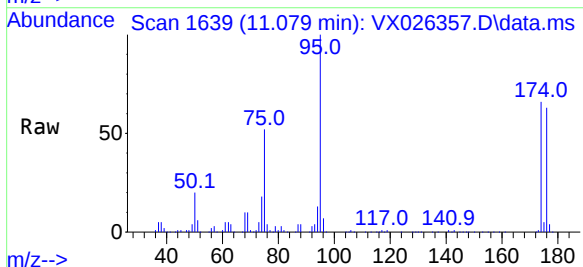






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 214438
Ion Ratio Lower Upper
117 100
82 58.0 43.8 65.6
119 32.8 25.2 37.8

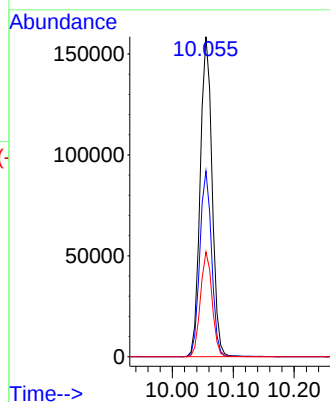

#67
Ethyl Benzene
Concen: 145.004 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 91 Resp: 1221370
Ion Ratio Lower Upper
91 100
106 30.9 25.7 38.5


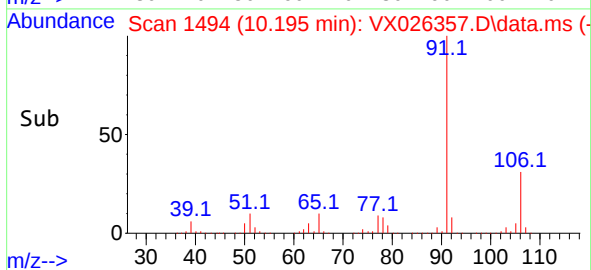
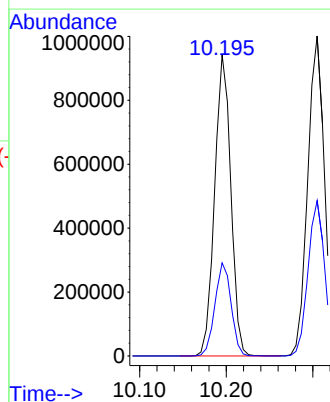
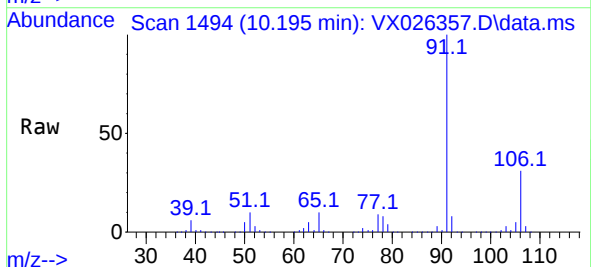




#68
m/p-Xylenes
Concen: 206.239 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 648620
Ion Ratio Lower Upper
106 100
91 206.7 158.6 238.0

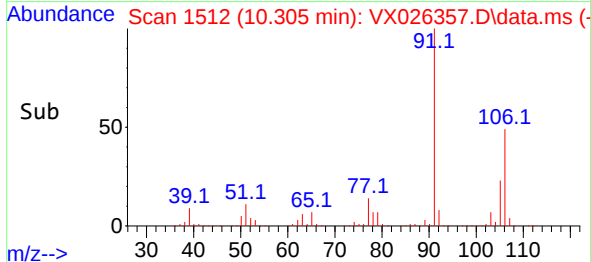

#69
o-Xylene
Concen: 72.982 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion:106 Resp: 224577
Ion Ratio Lower Upper
106 100
91 223.3 105.5 316.4


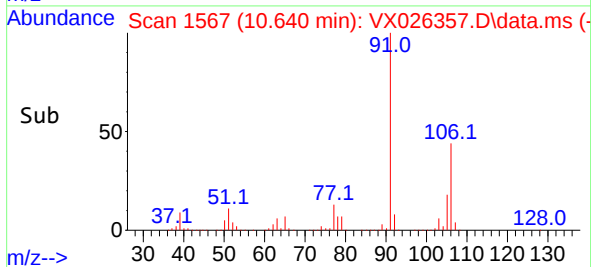

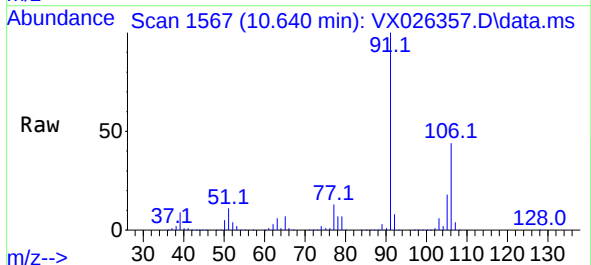




#70
Styrene
Concen: 2.370 ug/l
RT: 10.646 min Scan# 11
Delta R.T. -0.013 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:104 Resp: 11955
Ion Ratio Lower Upper
104 100
78 307.9 39.8 59.6#
103 262.9 43.0 64.6#

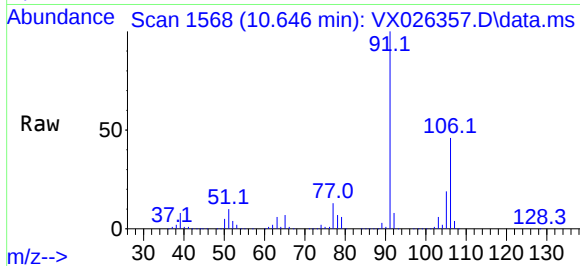

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion:152 Resp: 94932
Ion Ratio Lower Upper
152 100
115 62.7 41.3 123.9
150 157.9 0.0 351.8


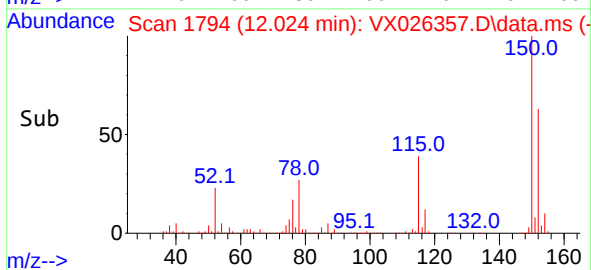

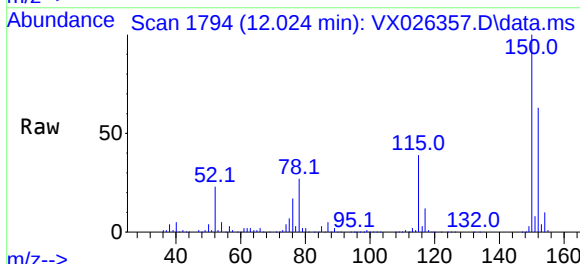




#73
Isopropylbenzene
Concen: 3.777 ug/l
RT: 10.963 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 27872
Ion Ratio Lower Upper
105 100
120 26.2 13.6 40.7

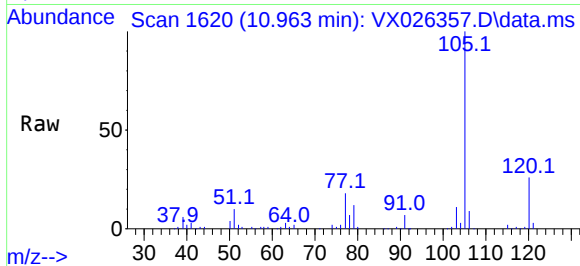

#76
1,2,3-Trichloropropane
Concen: 0.891 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.134 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 75 Resp: 2041
Ion Ratio Lower Upper
75 100
77 1269.6 19.0 57.0#


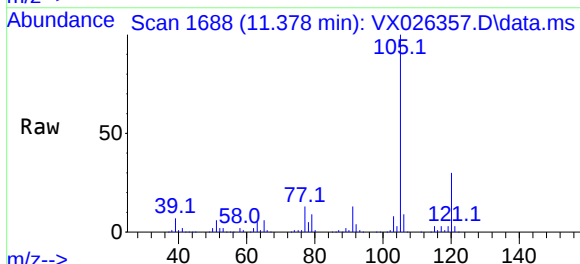




#78
n-propylbenzene
Concen: 5.260 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30


Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 44626
Ion Ratio Lower Upper
91 100
120 22.7 12.0 36.1

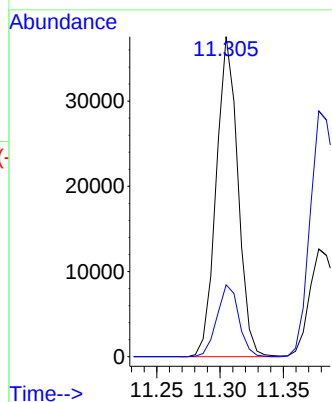

#79
2-Chlorotoluene
Concen: 5.048 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 91 Resp: 26365
Ion Ratio Lower Upper
91 100
126 0.2 17.8 53.3#




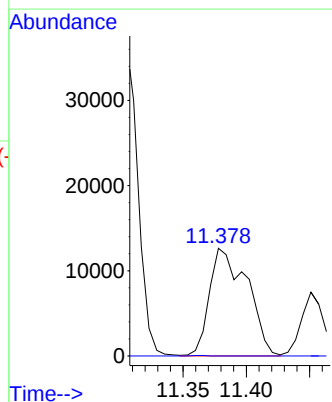




#80
1,3,5-Trimethylbenzene
Concen: 13.751 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 84206
Ion Ratio Lower Upper
105 100
120 47.6 24.9 74.7

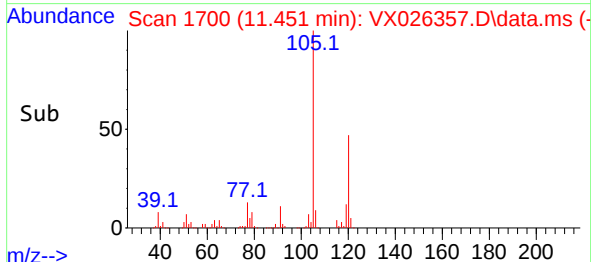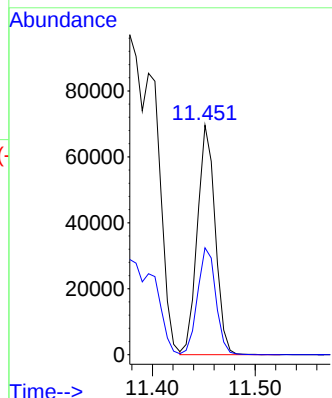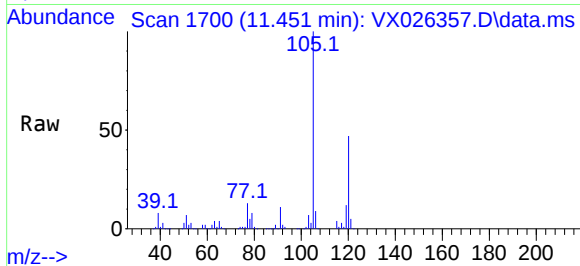

#81
trans-1,4-Dichloro-2-butene
Concen: 70.513 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 75 Resp: 55850
Ion Ratio Lower Upper
75 100
53 0.0 79.5 119.3#
89 0.0 38.3 57.5#




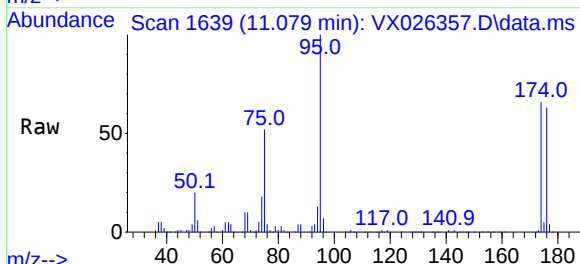




#82
4-Chlorotoluene
Concen: 1.533 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 9041
Ion Ratio Lower Upper
91 100
126 0.0 15.6 46.7#

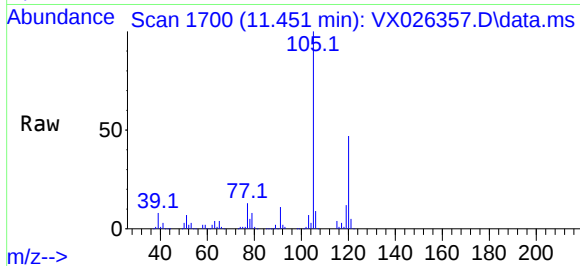

#83
tert-Butylbenzene
Concen: 9.048 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 119 Resp: 53781
Ion Ratio Lower Upper
119 100
91 93.3 28.7 86.1#
134 0.0 11.9 35.9#


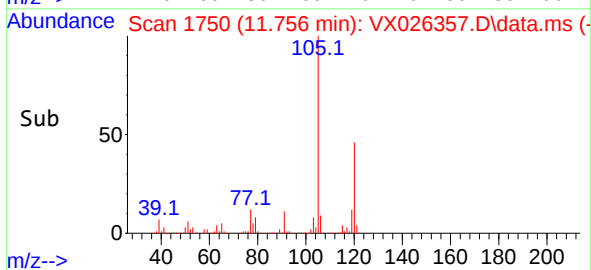

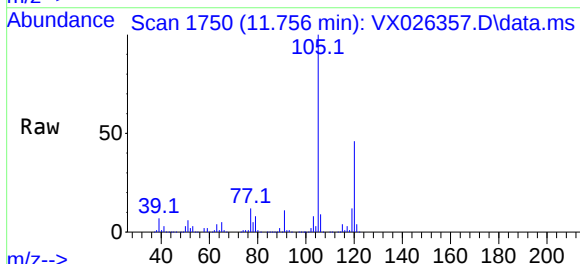




#84
1,2,4-Trimethylbenzene
Concen: 74.039 ug/l
RT: 11.750 min Scan# 1750
Delta R.T. -0.006 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 453026
Ion Ratio Lower Upper
105 100
120 44.7 22.9 68.7

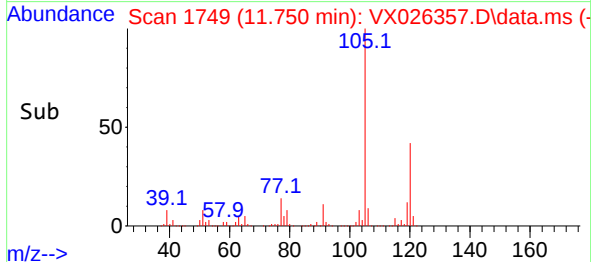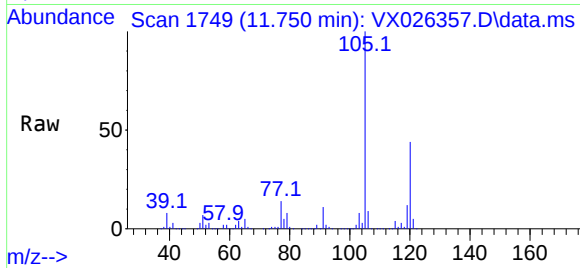

#85
sec-Butylbenzene
Concen: 61.076 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion:105 Resp: 453026
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


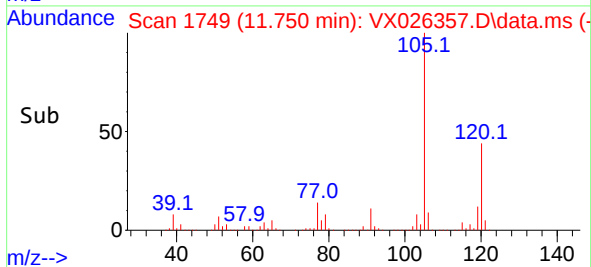

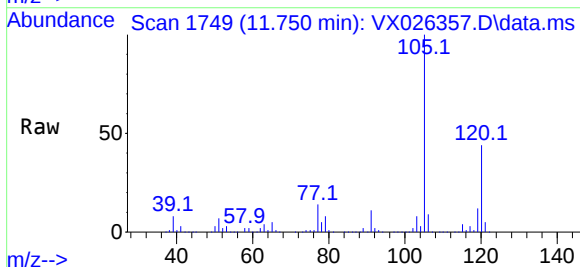




#86
p-Isopropyltoluene
Concen: 0.512 ug/l
RT: 11.975 min Scan# 11
Delta R.T. -0.037 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:119 Resp: 3168
Ion Ratio Lower Upper
119 100
134 28.3 13.2 39.6
91 0.0 11.9 35.9#

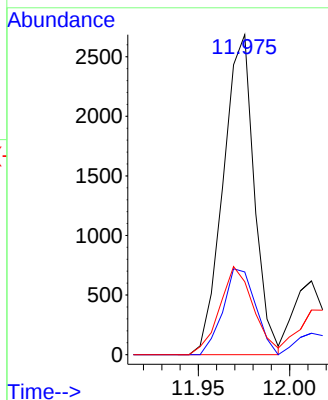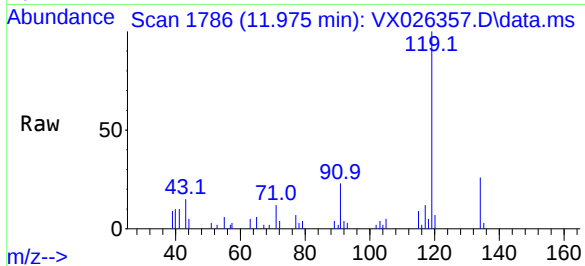

#89
n-Butylbenzene
Concen: 0.479 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. -0.018 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 91 Resp: 2633
Ion Ratio Lower Upper
91 100
92 19.4 27.3 81.8#
134 135.2 13.5 40.4#



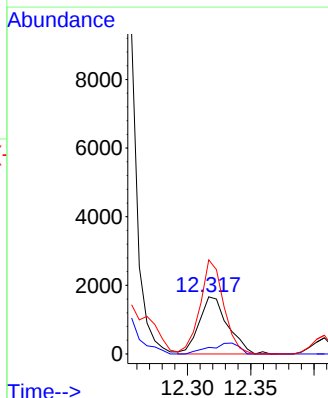
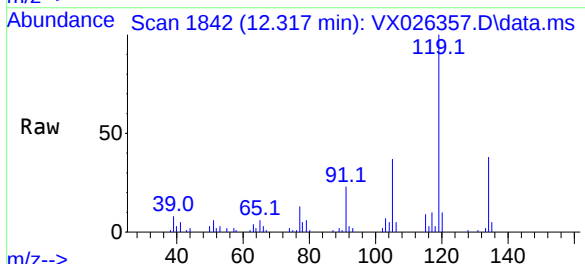




#90
Hexachloroethane
Concen: 19.220 ug/l
RT: 12.701 min Scan# 1905
Delta R.T. 0.159 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 23737
Ion Ratio Lower Upper
117 100
201 0.0 35.4 106.3#

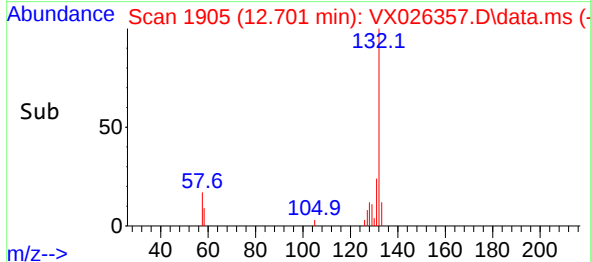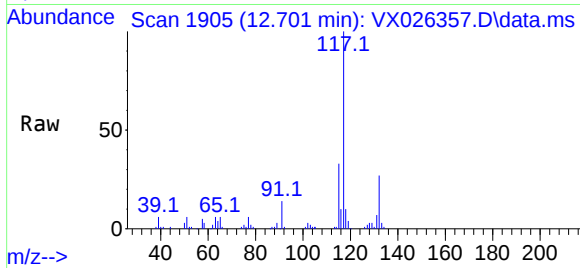

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.227 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX026357.D
Acq: 06 Jan 2022 05:30

Tgt Ion: 75 Resp: 146
Ion Ratio Lower Upper
75 100
155 0.0 44.0 131.8#
157 0.0 55.5 166.5#

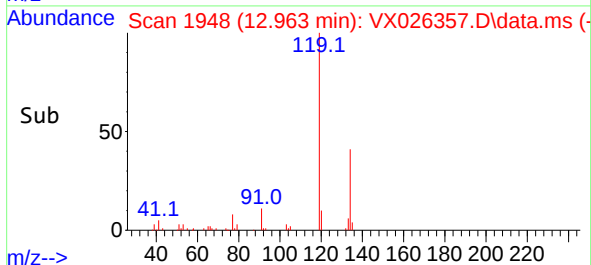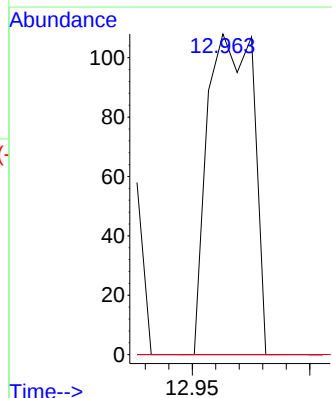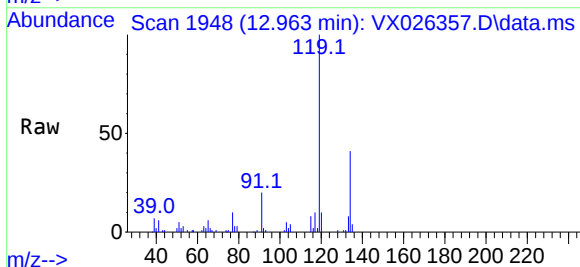



#95

Naphthalene

Concen: 32.841 ug/l

RT: 13.780 min Scan# 20

Delta R.T. -0.000 min


Lab File: VX026357.D

Acq: 06 Jan 2022 05:30

Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion:128 Resp: 240952

Ion Ratio Lower Upper

128 100

127 12.8 10.3 15.5

129 10.9 8.8 13.2

