

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
 Data File : VX026361.D
 Acq On : 06 Jan 2022 07:02
 Operator : JC/MD
 Sample : N1020-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 06 12:24:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	157175	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	264106	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	228258	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	101786	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	113026	49.707	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	99.420%
35) Dibromofluoromethane	5.391	113	85064	49.541	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.080%
50) Toluene-d8	8.653	98	304547	47.684	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.360%
62) 4-Bromofluorobenzene	11.079	95	113190	49.785	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.560%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.977	59	301	0.663	ug/l #	73
13) Acrolein	2.221	56	20484	126.132	ug/l #	1
14) Allyl chloride	2.752	41	38961	11.328	ug/l #	6
15) Acrylonitrile	3.105	53	960	0.854	ug/l #	36
16) Acetone	2.386	43	6967	5.655	ug/l	95
18) Methyl Acetate	2.709	43	2871	0.718	ug/l #	51
20) Methylene Chloride	2.721	84	1581	Below Cal	#	17
23) Vinyl Acetate	3.733	43	3973	0.762	ug/l #	70
24) 1,1-Dichloroethane	3.745	63	1236	0.347	ug/l #	83
25) 2-Butanone	4.434	43	2067	1.204	ug/l #	49
29) Tetrahydrofuran	5.202	42	2862	2.646	ug/l #	32
30) Chloroform	5.190	83	4695	1.248	ug/l #	19
31) Cyclohexane	5.477	56	50465	15.584	ug/l	96
36) 1,1-Dichloropropene	5.550	75	13165	4.754	ug/l #	50
37) Ethyl Acetate	4.721	43	4709	1.466	ug/l	96
38) Carbon Tetrachloride	5.556	117	17017	5.524	ug/l #	16
39) Methylcyclohexane	7.379	83	6380	2.042	ug/l #	87
40) Benzene	6.044	78	1843178	233.198	ug/l	98
41) Methacrylonitrile	4.904	41	447	0.247	ug/l #	17
42) 1,2-Dichloroethane	6.044	62	18429	5.761	ug/l #	74
48) Methyl methacrylate	7.665	41	817	0.326	ug/l #	83
51) 4-Methyl-2-Pentanone	8.561	43	2228	0.684	ug/l #	54
52) Toluene	8.720	92	207157	42.574	ug/l	99
53) t-1,3-Dichloropropene	8.720	75	3291	2.869	ug/l #	1
58) 2-Chloroethyl Vinyl ether	8.141	63	732	10.255	ug/l #	44
59) 2-Hexanone	9.567	43	1233	0.500	ug/l	77
67) Ethyl Benzene	10.195	91	206021	22.978	ug/l	97
68) m/p-Xylenes	10.305	106	334641	99.962	ug/l	93
69) o-Xylene	10.640	106	22238	6.789	ug/l	93
70) Styrene	10.646	104	1148	0.214	ug/l #	1
73) Isopropylbenzene	10.963	105	74648	9.435	ug/l	97
76) 1,2,3-Trichloropropane	11.079	75	59491	24.214	ug/l #	39
78) n-propylbenzene	11.305	91	124320	13.666	ug/l	97
79) 2-Chlorotoluene	11.402	91	6413	1.145	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.451	105	29588	4.506	ug/l	95
81) trans-1,4-Dichloro-2-b...	11.079	75	59491	70.052	ug/l #	10

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
 Data File : VX026361.D
 Acq On : 06 Jan 2022 07:02
 Operator : JC/MD
 Sample : N1020-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 06 12:24:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
82) 4-Chlorotoluene	11.402	91	6413	1.014	ug/l #	44
83) tert-Butylbenzene	11.750	119	11057	1.735	ug/l #	49
84) 1,2,4-Trimethylbenzene	11.750	105	95438	14.547	ug/l	97
85) sec-Butylbenzene	11.750	105	95438	12.000	ug/l #	56
89) n-Butylbenzene	12.329	91	1847	0.313	ug/l #	60
90) Hexachloroethane	12.701	117	30891	23.328	ug/l #	14
95) Naphthalene	13.774	128	246651	31.354	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
Data File : VX026361.D
Acq On : 06 Jan 2022 07:02
Operator : JC/MD
Sample : N1020-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 06 12:24:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration

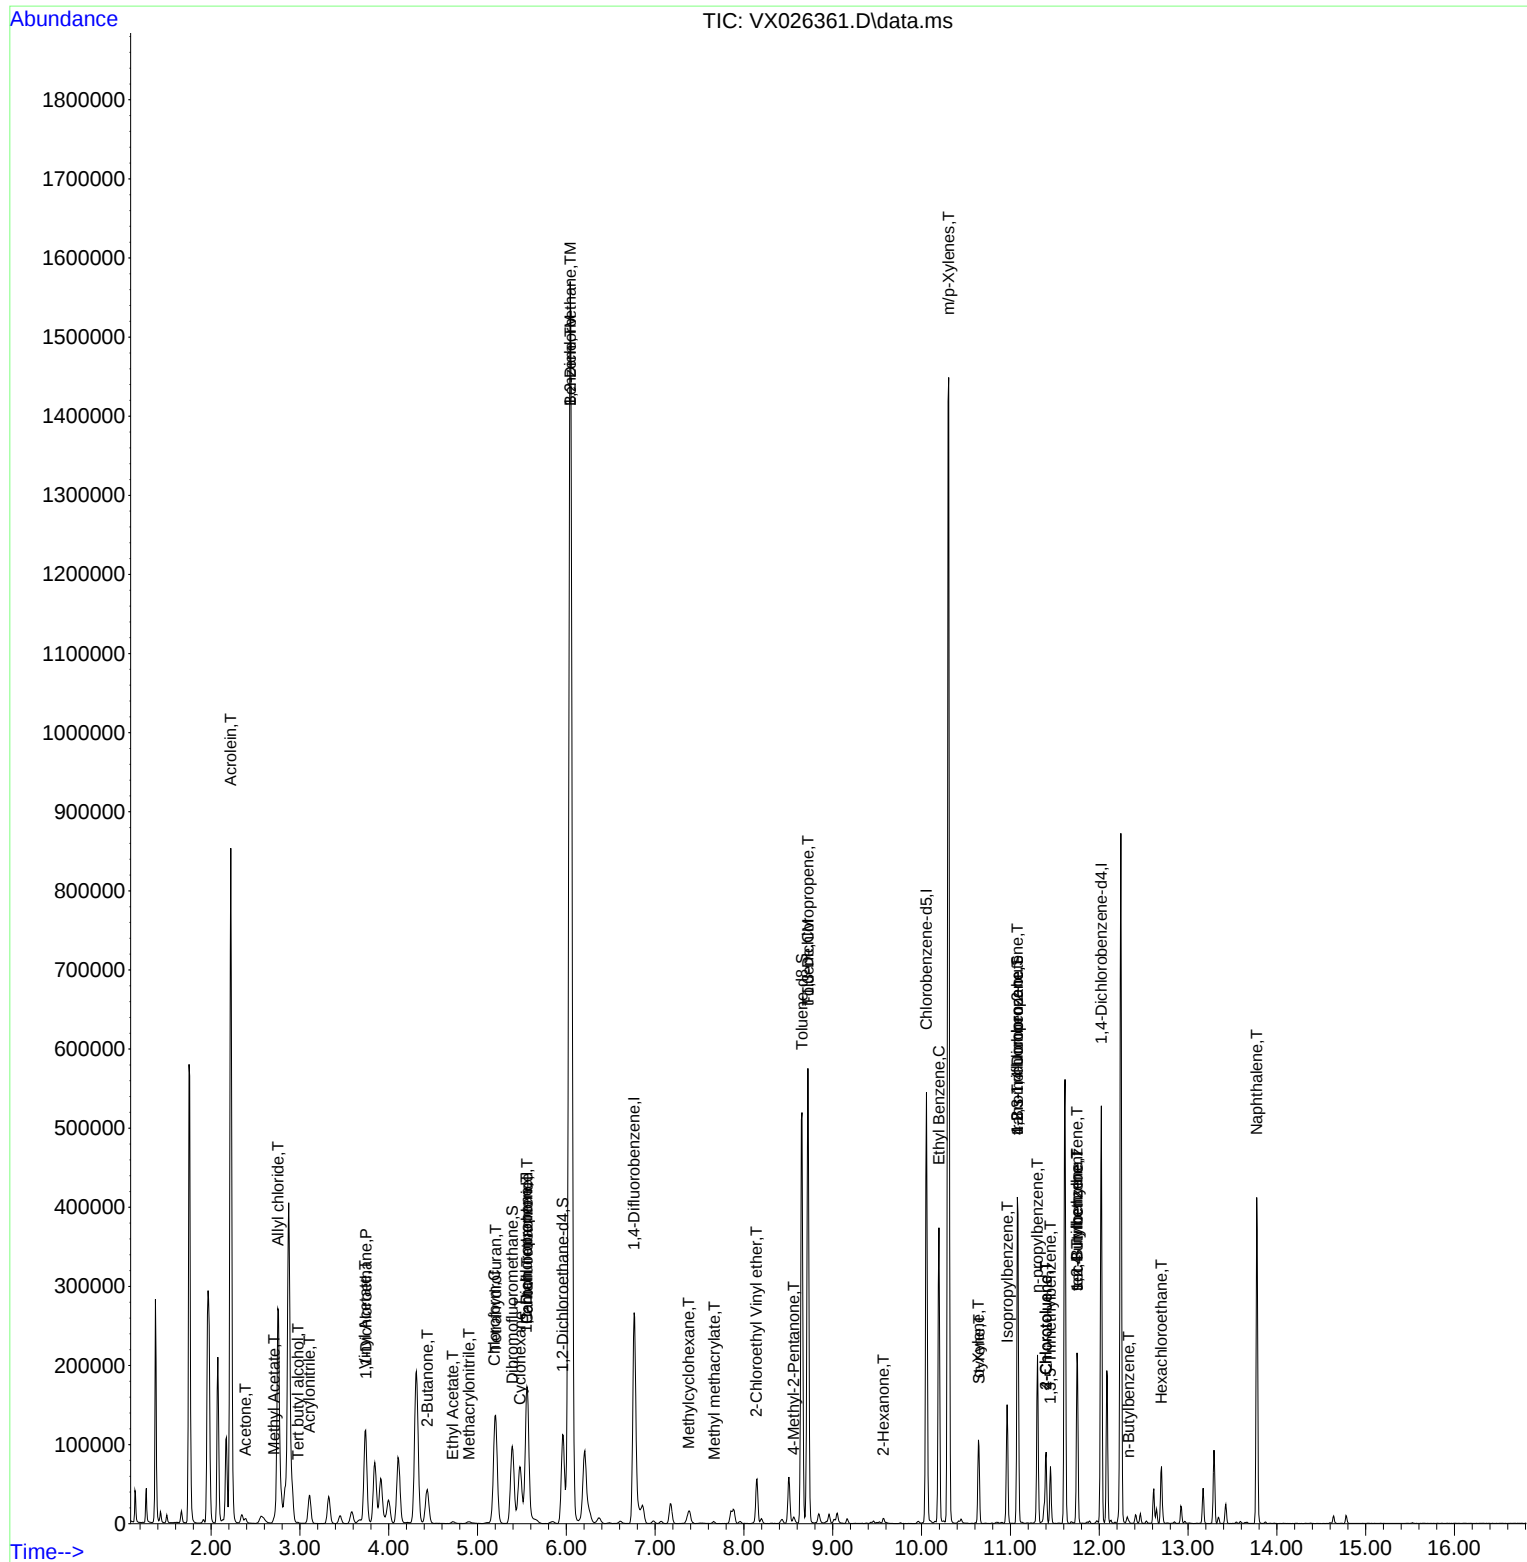






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Instrument :
MSVOA_X
ClientSampleId :



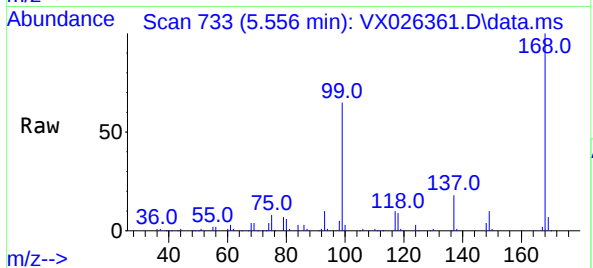



Tgt Ion:168 Resp: 157175
Ion Ratio Lower Upper
168 100
99 64.6 45.8 68.8

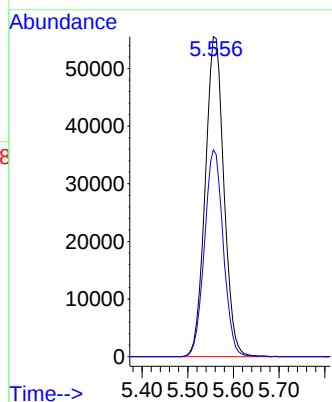

#11
Tert butyl alcohol
Concen: 0.663 ug/l
RT: 2.977 min Scan# 310
Delta R.T. -0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 59 Resp: 301
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#


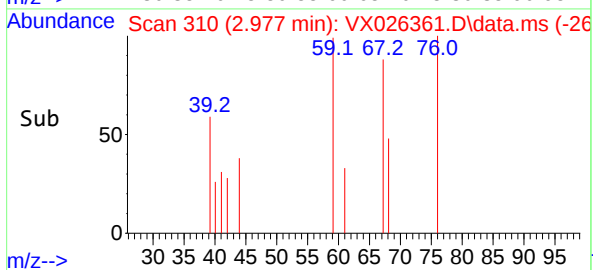






#13
Acrolein
Concen: 126.132 ug/l
RT: 2.221 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 56 Resp: 20484
Ion Ratio Lower Upper
56 100
55 2178.5 57.4 86.2#

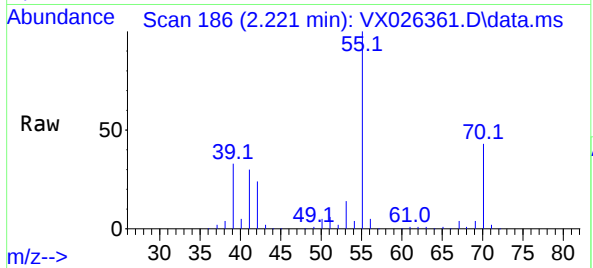

#14
Allyl chloride
Concen: 11.328 ug/l
RT: 2.752 min Scan# 273
Delta R.T. 0.080 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02


Tgt Ion: 41 Resp: 38961
Ion Ratio Lower Upper
41 100
39 159.4 55.4 83.0#
76 0.0 27.6 41.4#

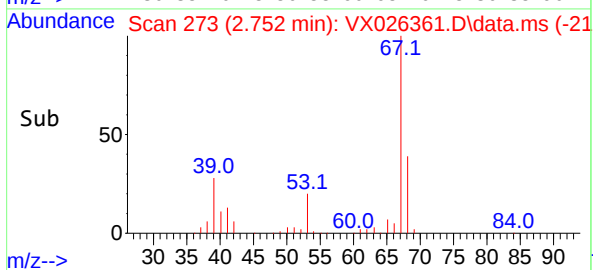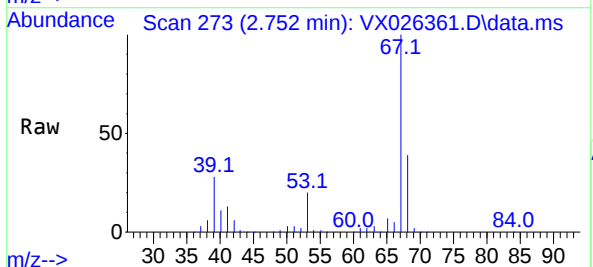






#15
Acrylonitrile
Concen: 0.854 ug/l
RT: 3.105 min Scan# 31
Delta R.T. 0.036 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 53 Resp: 960
Ion Ratio Lower Upper
53 100
52 8.8 66.2 99.2#
51 49.4 29.4 44.0#



#16
Acetone
Concen: 5.655 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 43 Resp: 6967
Ion Ratio Lower Upper
43 100
58 28.4 24.8 37.2


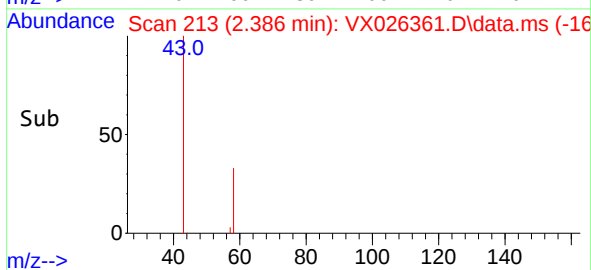






#18
Methyl Acetate
Concen: 0.718 ug/l
RT: 2.709 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2871
Ion Ratio Lower Upper
43 100
74 0.0 19.1 28.7#

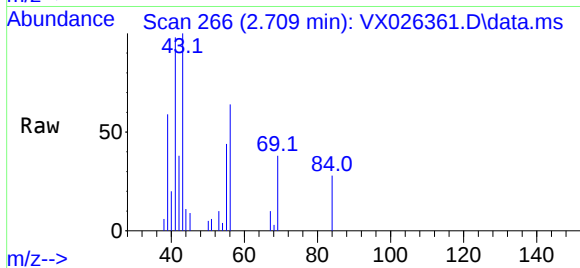

#23
Vinyl Acetate
Concen: 0.762 ug/l
RT: 3.733 min Scan# 434
Delta R.T. 0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 43 Resp: 3973
Ion Ratio Lower Upper
43 100
86 0.0 9.0 13.6#


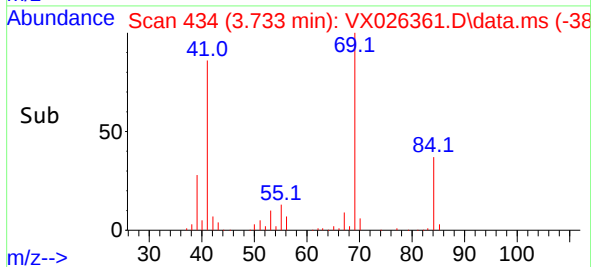

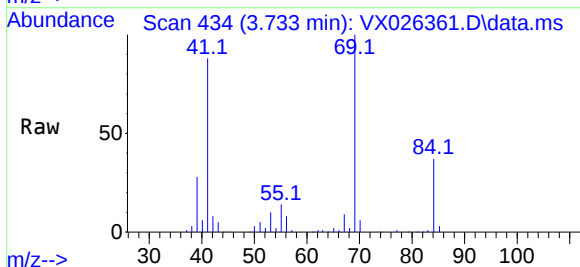




#24
1,1-Dichloroethane
Concen: 0.347 ug/l
RT: 3.745 min Scan# 41
Delta R.T. 0.128 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 63 Resp: 1236
Ion Ratio Lower Upper
63 100
98 0.0 3.3 9.9#
100 0.0 2.2 6.6#

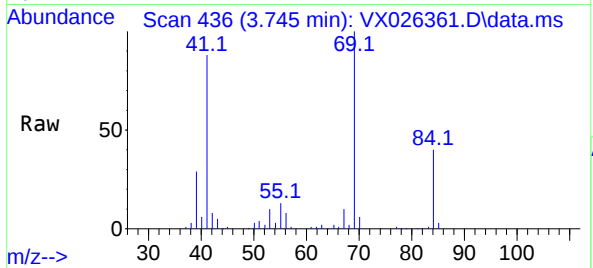

#25
2-Butanone
Concen: 1.204 ug/l
RT: 4.434 min Scan# 549
Delta R.T. -0.128 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 43 Resp: 2067
Ion Ratio Lower Upper
43 100
72 0.0 21.0 31.4#


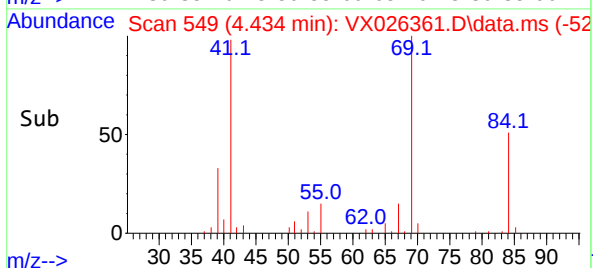
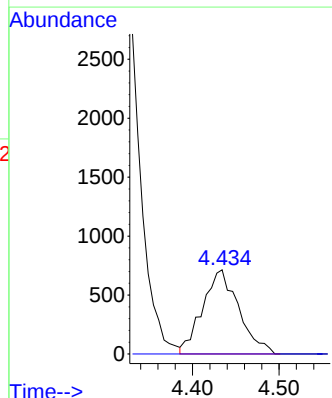





#29
Tetrahydrofuran
Concen: 2.646 ug/l
RT: 5.202 min Scan# 61
Delta R.T. 0.189 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 42 Resp: 2862
Ion Ratio Lower Upper
42 100
72 0.0 37.0 55.6#
71 0.0 34.1 51.1#

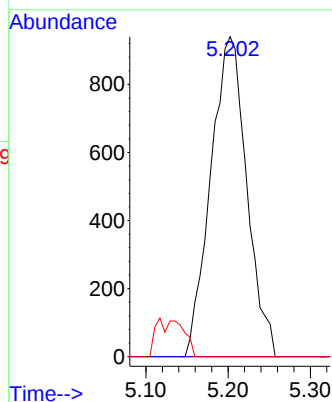

#30
Chloroform
Concen: 1.248 ug/l
RT: 5.190 min Scan# 673
Delta R.T. 0.085 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02


Tgt Ion: 83 Resp: 4695
Ion Ratio Lower Upper
83 100
85 0.0 50.6 75.8#

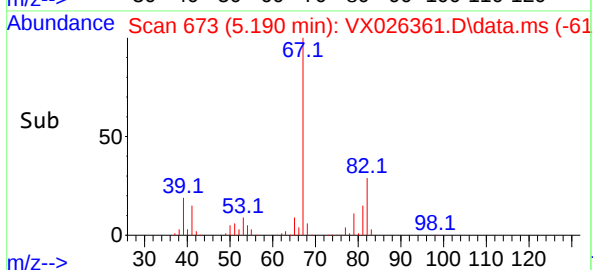






#31
Cyclohexane
Concen: 15.584 ug/l
RT: 5.477 min Scan# 719
Delta R.T. -0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 50465
Ion Ratio Lower Upper
56 100
69 29.5 23.9 35.9
84 86.8 73.2 109.8

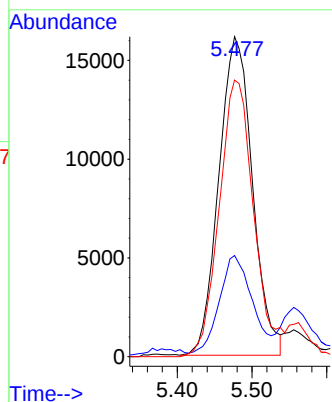

#33
1,2-Dichloroethane-d4
Concen: 49.707 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 65 Resp: 113026
Ion Ratio Lower Upper
65 100
67 49.7 0.0 103.4


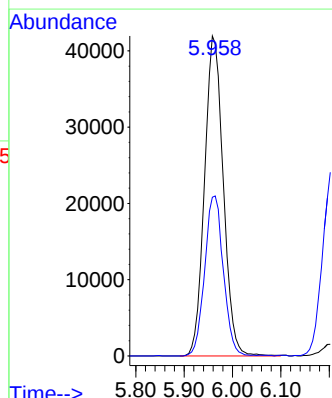






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 264106
Ion Ratio Lower Upper
114 100
63 21.9 0.0 40.0
88 16.7 0.0 30.6

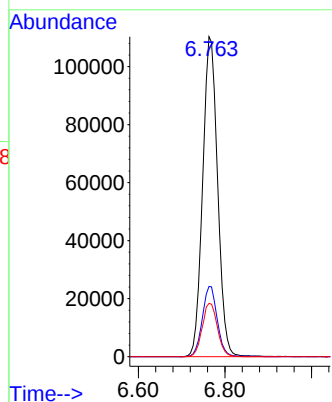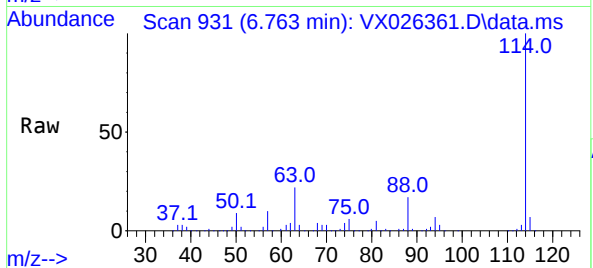

#35
Dibromofluoromethane
Concen: 49.541 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion:113 Resp: 85064
Ion Ratio Lower Upper
113 100
111 101.9 81.8 122.8
192 18.8 15.0 22.4

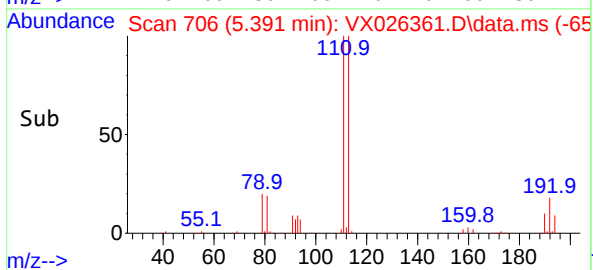

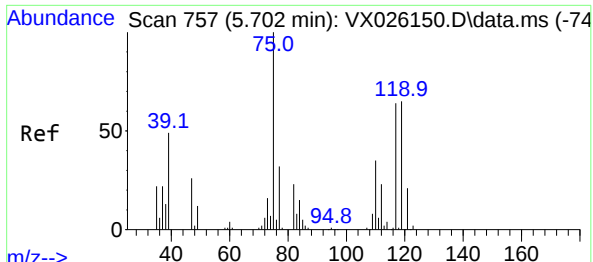

#36

1,1-Dichloropropene

Concen: 4.754 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.152 min

Lab File: VX026361.D

Acq: 06 Jan 2022 07:02

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 75 Resp: 13165

Ion Ratio Lower Upper

75 100

110 10.1 18.2 54.6#

77 0.0 24.7 37.1#

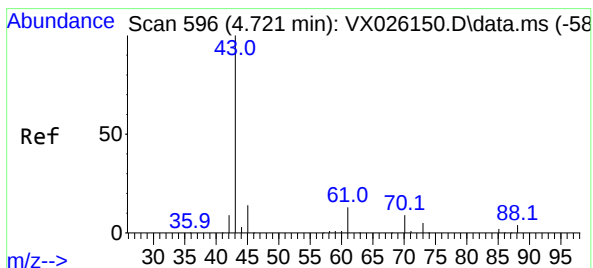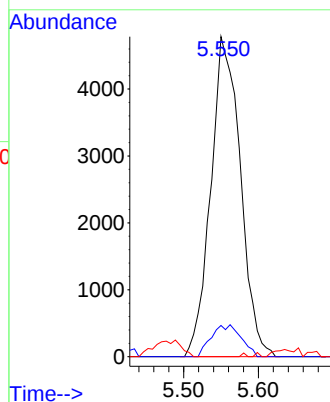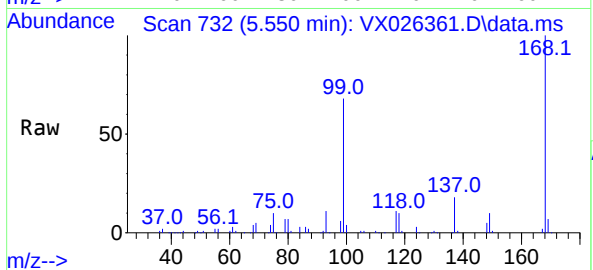

#37

Ethyl Acetate

Concen: 1.466 ug/l

RT: 4.721 min Scan# 596

Delta R.T. -0.000 min

Lab File: VX026361.D

Acq: 06 Jan 2022 07:02




Tgt Ion: 43 Resp: 4709


Ion Ratio Lower Upper

43 100

61 11.2 10.7 16.1


70 11.3 8.5 12.7

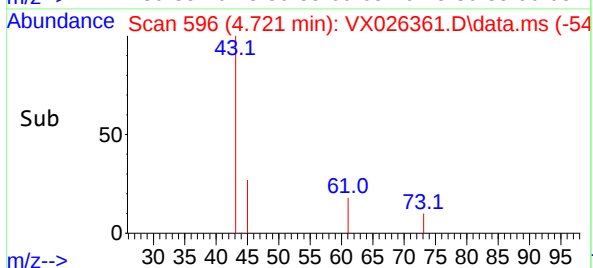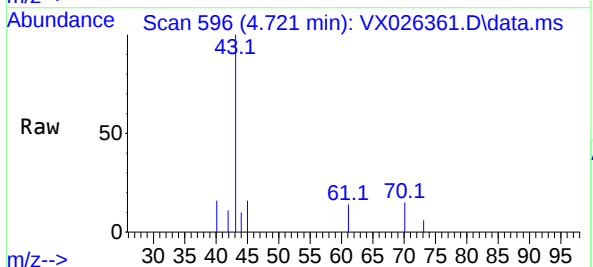



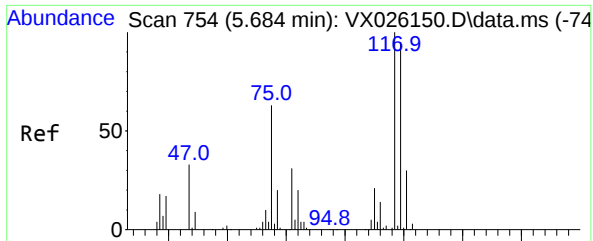


#38
Carbon Tetrachloride
Concen: 5.524 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Instrument :
MSVOA_X
ClientSampleId :



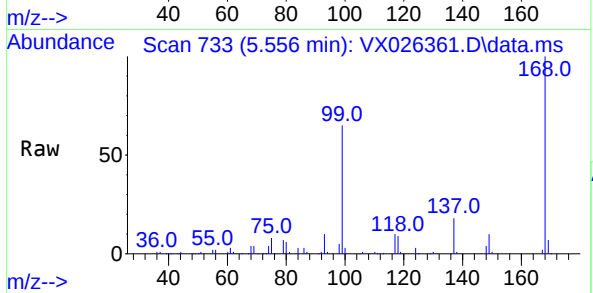



Tgt Ion:117 Resp: 17017
Ion Ratio Lower Upper
117 100
119 5.9 77.2 115.8#
121 0.0 23.8 35.8#

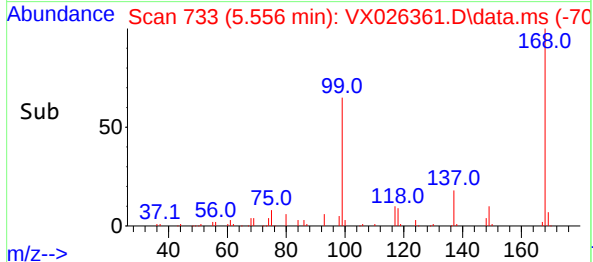

#39
Methylcyclohexane
Concen: 2.042 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02


Tgt Ion: 83 Resp: 6380
Ion Ratio Lower Upper
83 100
55 88.3 57.8 86.8#
98 52.7 40.5 60.7

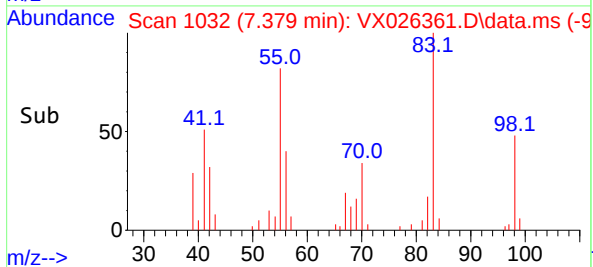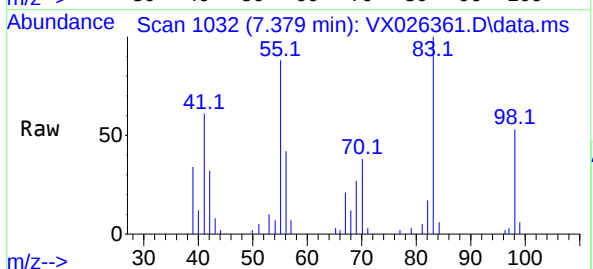






#40
Benzene
Concen: 233.198 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02


Instrument :
MSVOA_X
ClientSampleId :

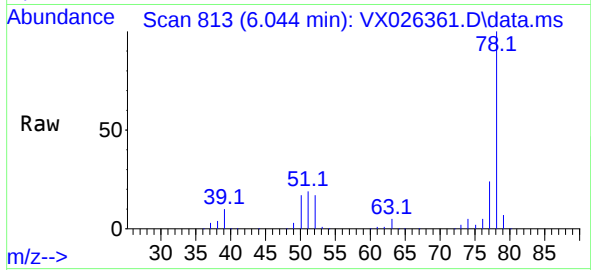



Tgt Ion: 78 Resp: 1843178
Ion Ratio Lower Upper
78 100
77 24.1 18.6 27.8

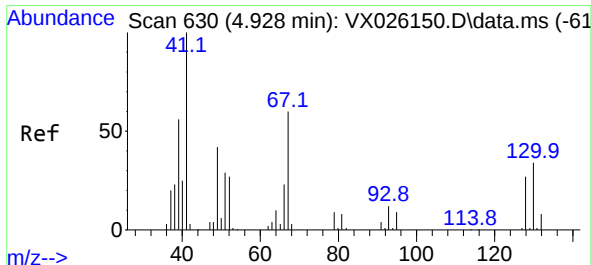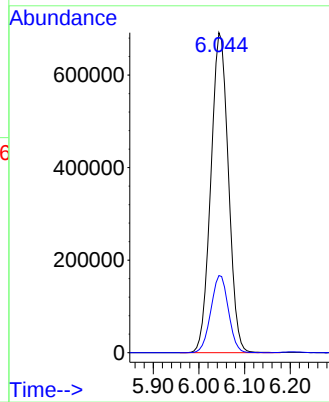


#41
Methacrylonitrile
Concen: 0.247 ug/l
RT: 4.904 min Scan# 626
Delta R.T. -0.024 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

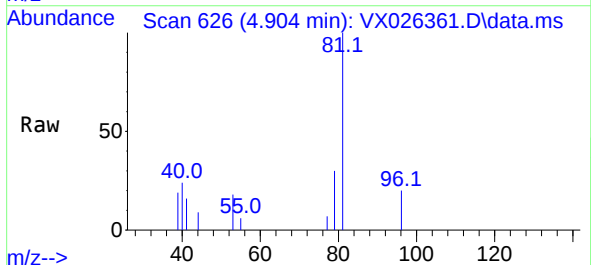

Tgt Ion: 41 Resp: 447
Ion Ratio Lower Upper
41 100
39 122.4 44.2 66.2#
67 0.0 59.7 89.5#
52 0.0 24.2 36.2#

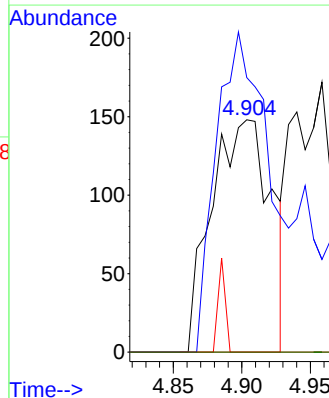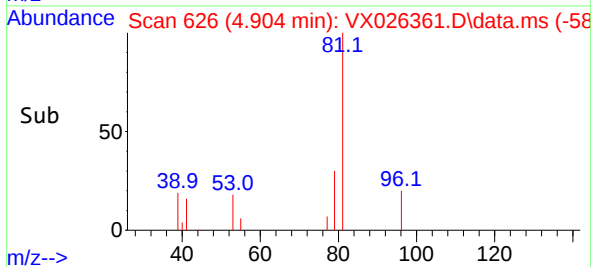



#42

1,2-Dichloroethane

Concen: 5.761 ug/l

RT: 6.044 min Scan# 81

Delta R.T. -0.048 min

Lab File: VX026361.D

Acq: 06 Jan 2022 07:02

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 62 Resp: 18429

Ion Ratio Lower Upper

62 100

98 0.0 0.0 18.8

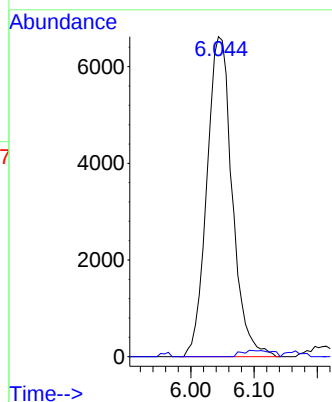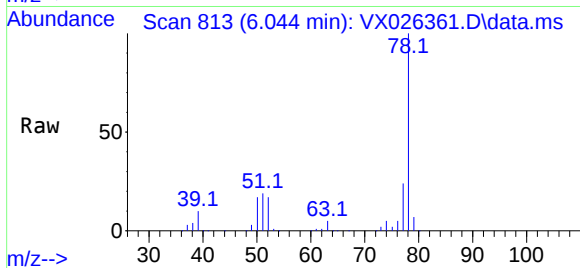

#48

Methyl methacrylate

Concen: 0.326 ug/l

RT: 7.665 min Scan# 1079

Delta R.T. -0.031 min

Lab File: VX026361.D

Acq: 06 Jan 2022 07:02




Tgt Ion: 41 Resp: 817


Ion Ratio Lower Upper

41 100

69 97.6 67.3 100.9

39 47.6 50.2 75.2#


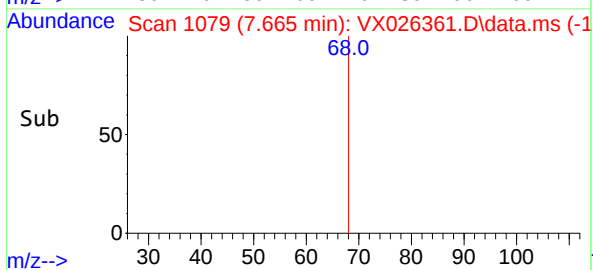

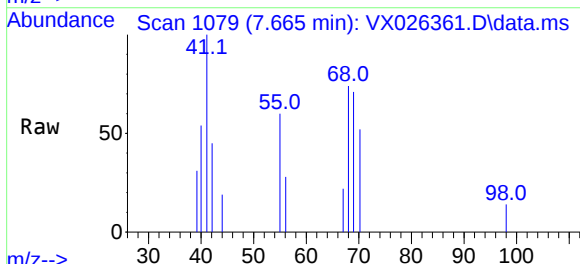




#50
Toluene-d8
Concen: 47.684 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 304547
Ion Ratio Lower Upper
98 100
100 66.4 52.6 78.8

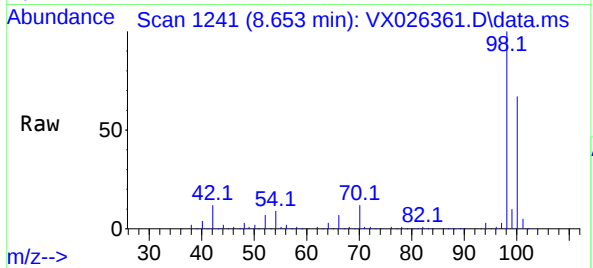

#51
4-Methyl-2-Pentanone
Concen: 0.684 ug/l
RT: 8.561 min Scan# 1226
Delta R.T. -0.019 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 43 Resp: 2228
Ion Ratio Lower Upper
43 100
58 10.5 30.8 46.2#


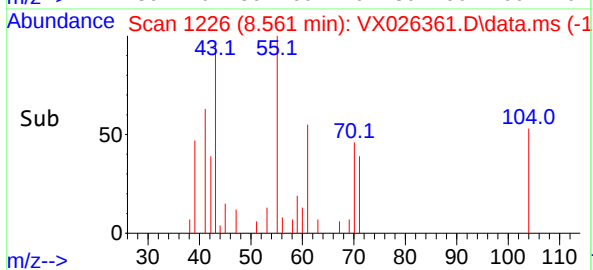

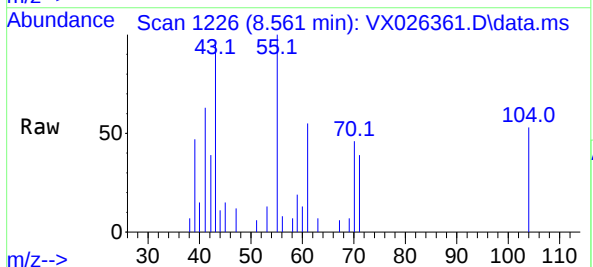




#52
Toluene
Concen: 42.574 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 207157
Ion Ratio Lower Upper
92 100
91 171.7 136.0 204.0

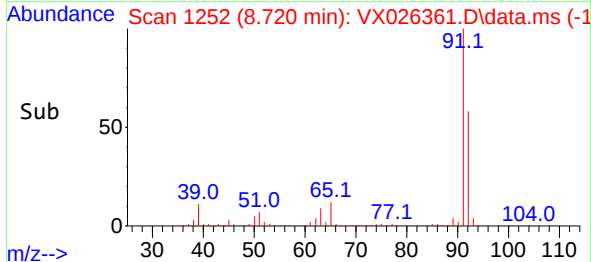

#53
t-1,3-Dichloropropene
Concen: 2.869 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.262 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 75 Resp: 3291
Ion Ratio Lower Upper
75 100
77 153.7 25.1 37.7#


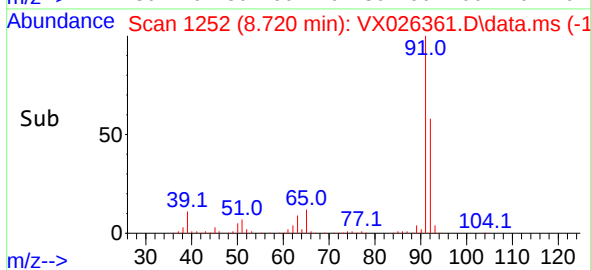






#58
2-Chloroethyl Vinyl ether
Concen: 10.255 ug/l
RT: 8.141 min Scan# 1157
Delta R.T. -0.103 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 63 Resp: 732
Ion Ratio Lower Upper
63 100
106 0.0 24.4 36.6#

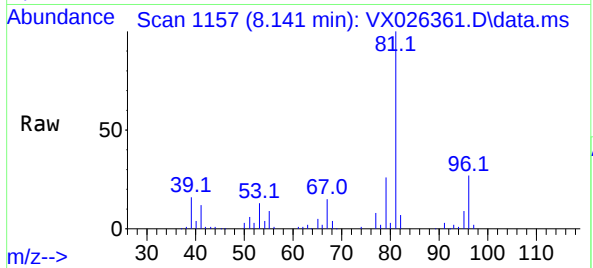

#59
2-Hexanone
Concen: 0.500 ug/l
RT: 9.567 min Scan# 1391
Delta R.T. 0.134 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 43 Resp: 1233
Ion Ratio Lower Upper
43 100
58 70.5 26.9 80.6


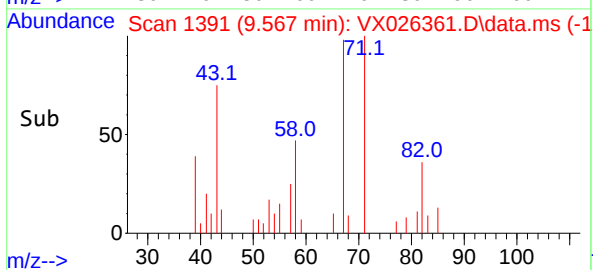

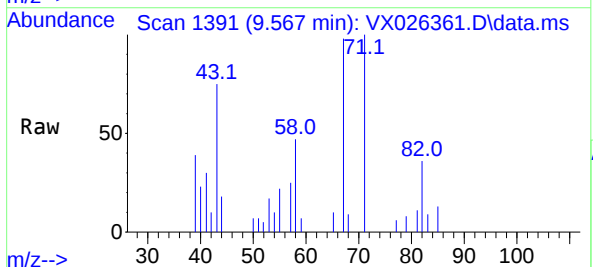




#62
4-Bromofluorobenzene
Concen: 49.785 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 113190
Ion Ratio Lower Upper
95 100
174 72.2 0.0 157.4
176 70.0 0.0 154.6



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 117 Resp: 228258
Ion Ratio Lower Upper
117 100
82 57.6 43.8 65.6
119 31.8 25.2 37.8


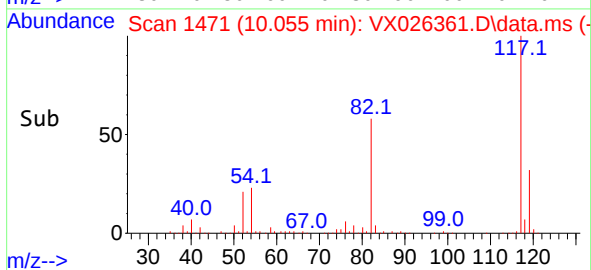






#67
Ethyl Benzene
Concen: 22.978 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 206021
Ion Ratio Lower Upper
91 100
106 30.6 25.7 38.5

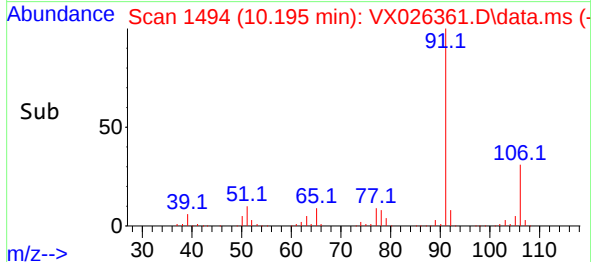

#68
m/p-Xylenes
Concen: 99.962 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion:106 Resp: 334641
Ion Ratio Lower Upper
106 100
91 209.5 158.6 238.0


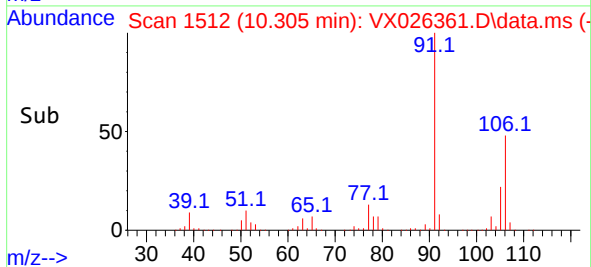

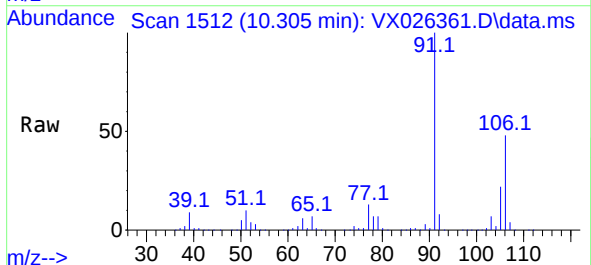




#69
o-Xylene
Concen: 6.789 ug/l
RT: 10.640 min Scan# 1568
Delta R.T. -0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 22238
Ion Ratio Lower Upper
106 100
91 221.2 105.5 316.4

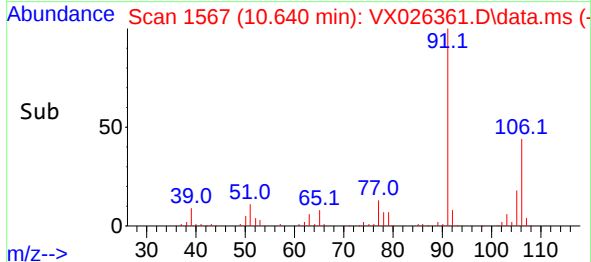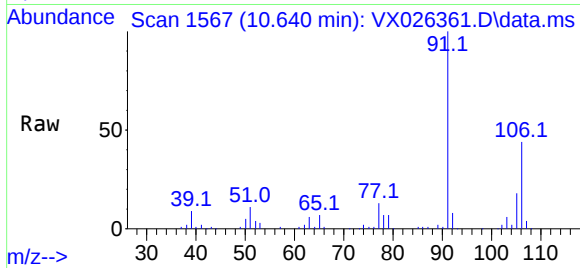

#70
Styrene
Concen: 0.214 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.013 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02


Tgt Ion:104 Resp: 1148
Ion Ratio Lower Upper
104 100
78 319.2 39.8 59.6#
103 250.0 43.0 64.6#

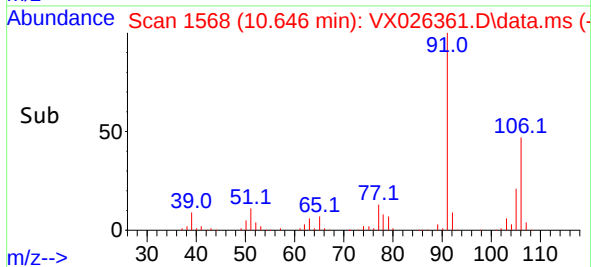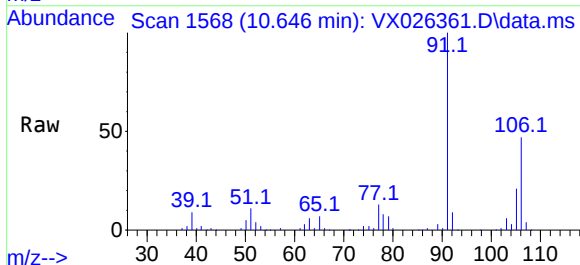






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02


Instrument :
MSVOA_X
ClientSampleId :

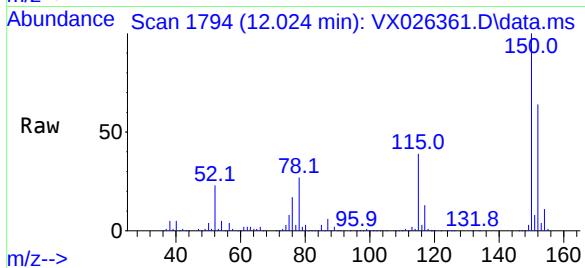



Tgt Ion:152 Resp: 101786
Ion Ratio Lower Upper
152 100
115 62.5 41.3 123.9
150 156.8 0.0 351.8

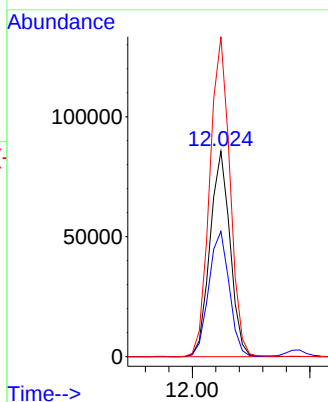


#73
Isopropylbenzene
Concen: 9.435 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

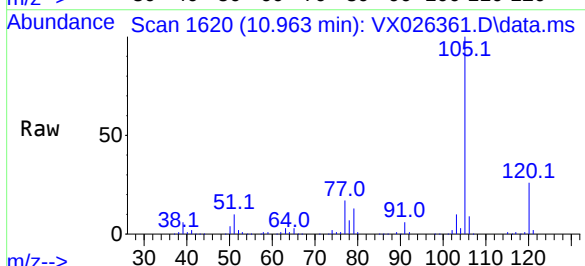

Tgt Ion:105 Resp: 74648
Ion Ratio Lower Upper
105 100
120 25.8 13.6 40.7



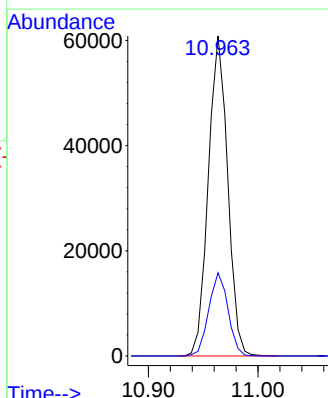





#76
1,2,3-Trichloropropane
Concen: 24.214 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 59491
Ion Ratio Lower Upper
75 100
77 1.0 19.0 57.0#

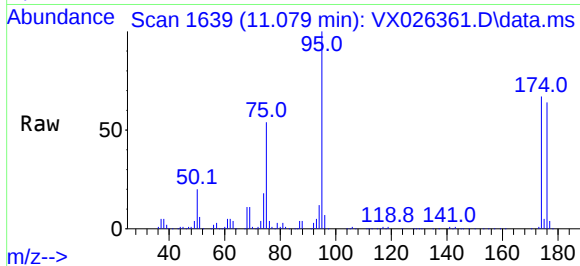

#78
n-propylbenzene
Concen: 13.666 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 91 Resp: 124320
Ion Ratio Lower Upper
91 100
120 22.5 12.0 36.1



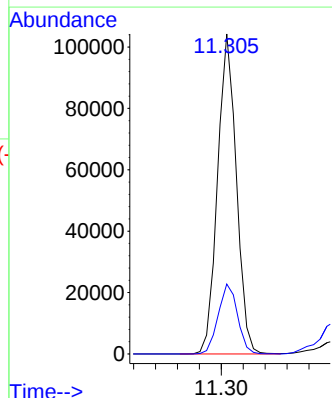
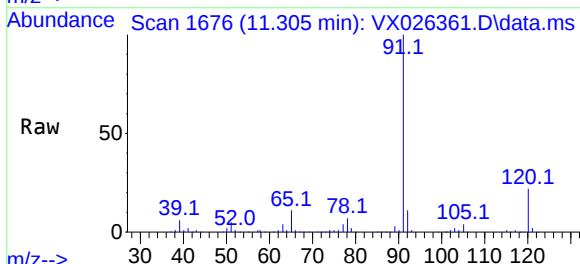




#79
2-Chlorotoluene
Concen: 1.145 ug/l
RT: 11.402 min Scan# 11
Delta R.T. 0.036 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 6413
Ion Ratio Lower Upper
91 100
126 0.0 17.8 53.3#

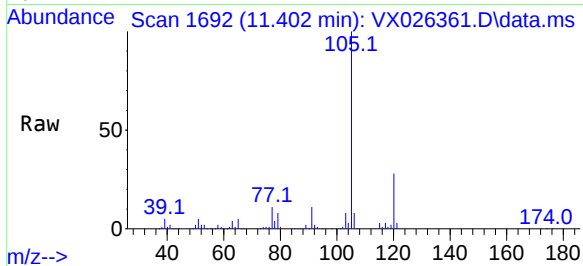

#80
1,3,5-Trimethylbenzene
Concen: 4.506 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion:105 Resp: 29588
Ion Ratio Lower Upper
105 100
120 46.5 24.9 74.7


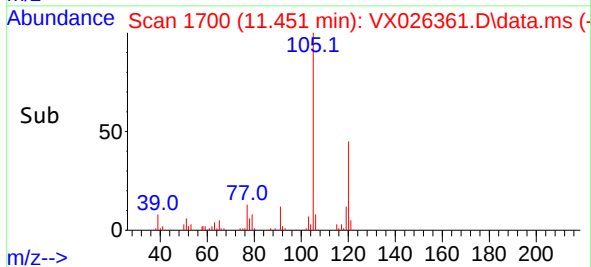

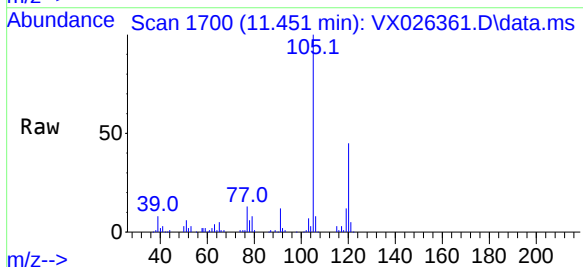




#81
trans-1,4-Dichloro-2-butene
Concen: 70.052 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 59491
Ion Ratio Lower Upper
75 100
53 0.0 79.5 119.3#
89 0.0 38.3 57.5#

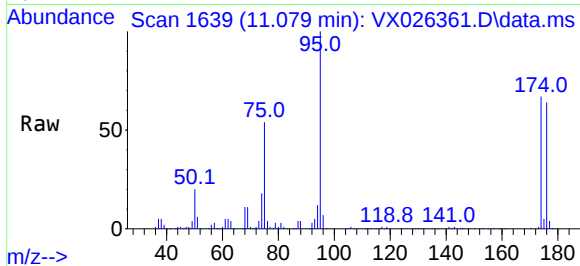

#82
4-Chlorotoluene
Concen: 1.014 ug/l
RT: 11.402 min Scan# 1692
Delta R.T. -0.055 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 91 Resp: 6413
Ion Ratio Lower Upper
91 100
126 0.0 15.6 46.7#


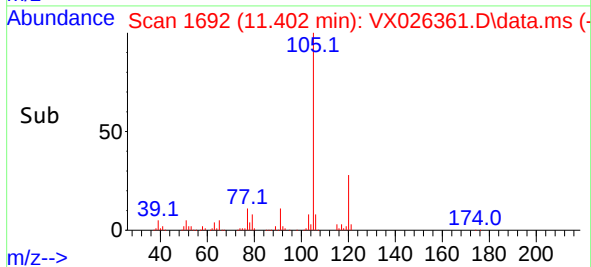

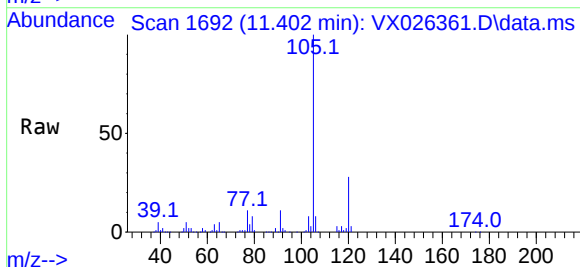




#83
tert-Butylbenzene
Concen: 1.735 ug/l
RT: 11.750 min Scan# 11
Delta R.T. 0.031 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:119 Resp: 11057
Ion Ratio Lower Upper
119 100
91 95.4 28.7 86.1#
134 0.0 11.9 35.9#

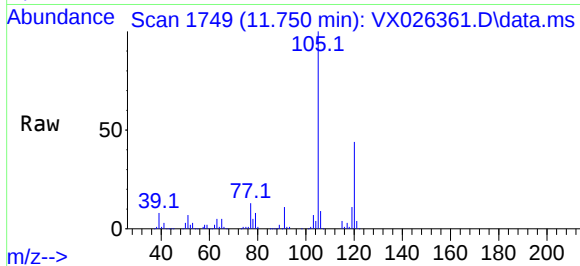

#84
1,2,4-Trimethylbenzene
Concen: 14.547 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion:105 Resp: 95438
Ion Ratio Lower Upper
105 100
120 44.0 22.9 68.7



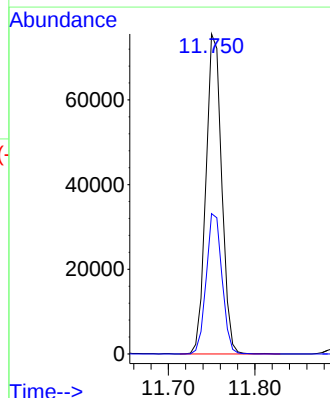
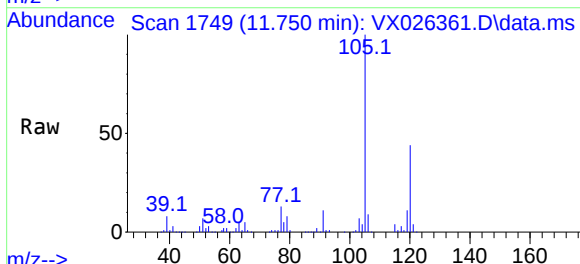




#85
sec-Butylbenzene
Concen: 12.000 ug/l
RT: 11.750 min Scan# 11
Delta R.T. -0.140 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 95438
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#

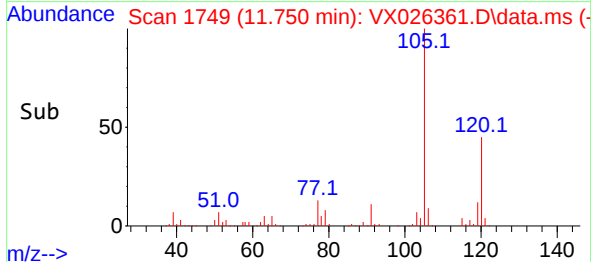

#89
n-Butylbenzene
Concen: 0.313 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion: 91 Resp: 1847
Ion Ratio Lower Upper
91 100
92 35.4 27.3 81.8
134 62.0 13.5 40.4#


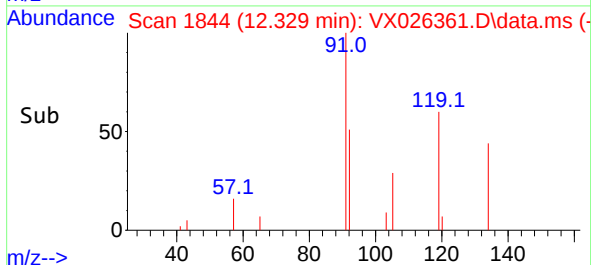
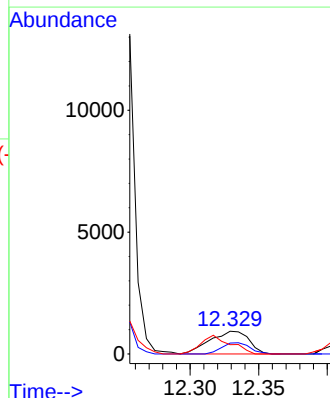
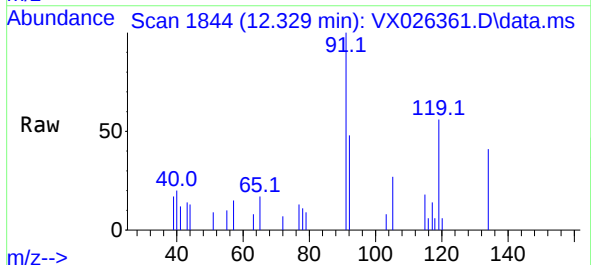




#90
Hexachloroethane
Concen: 23.328 ug/l
RT: 12.701 min Scan# 1905
Delta R.T. 0.159 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:117 Resp: 30891
Ion Ratio Lower Upper
117 100
201 0.0 35.4 106.3#

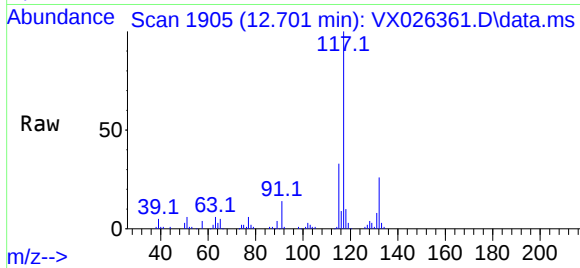

#95
Naphthalene
Concen: 31.354 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX026361.D
Acq: 06 Jan 2022 07:02

Tgt Ion:128 Resp: 246651
Ion Ratio Lower Upper
128 100
127 12.9 10.3 15.5
129 11.0 8.8 13.2

