

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
 Data File : VX026348.D
 Acq On : 06 Jan 2022 02:02
 Operator : JC/MD
 Sample : N1019-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-26I

Quant Time: Jan 06 05:04:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	153380	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	255986	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	221122	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	96317	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	110936	49.995	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	99.980%
35) Dibromofluoromethane	5.391	113	83056	49.906	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.820%
50) Toluene-d8	8.653	98	295794	47.783	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.560%
62) 4-Bromofluorobenzene	11.079	95	109910	49.875	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.760%
Target Compounds						
16) Acetone	2.386	43	8375	6.966	ug/l	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
Data File : VX026348.D
Acq On : 06 Jan 2022 02:02
Operator : JC/MD
Sample : N1019-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-26I

Quant Time: Jan 06 05:04:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration




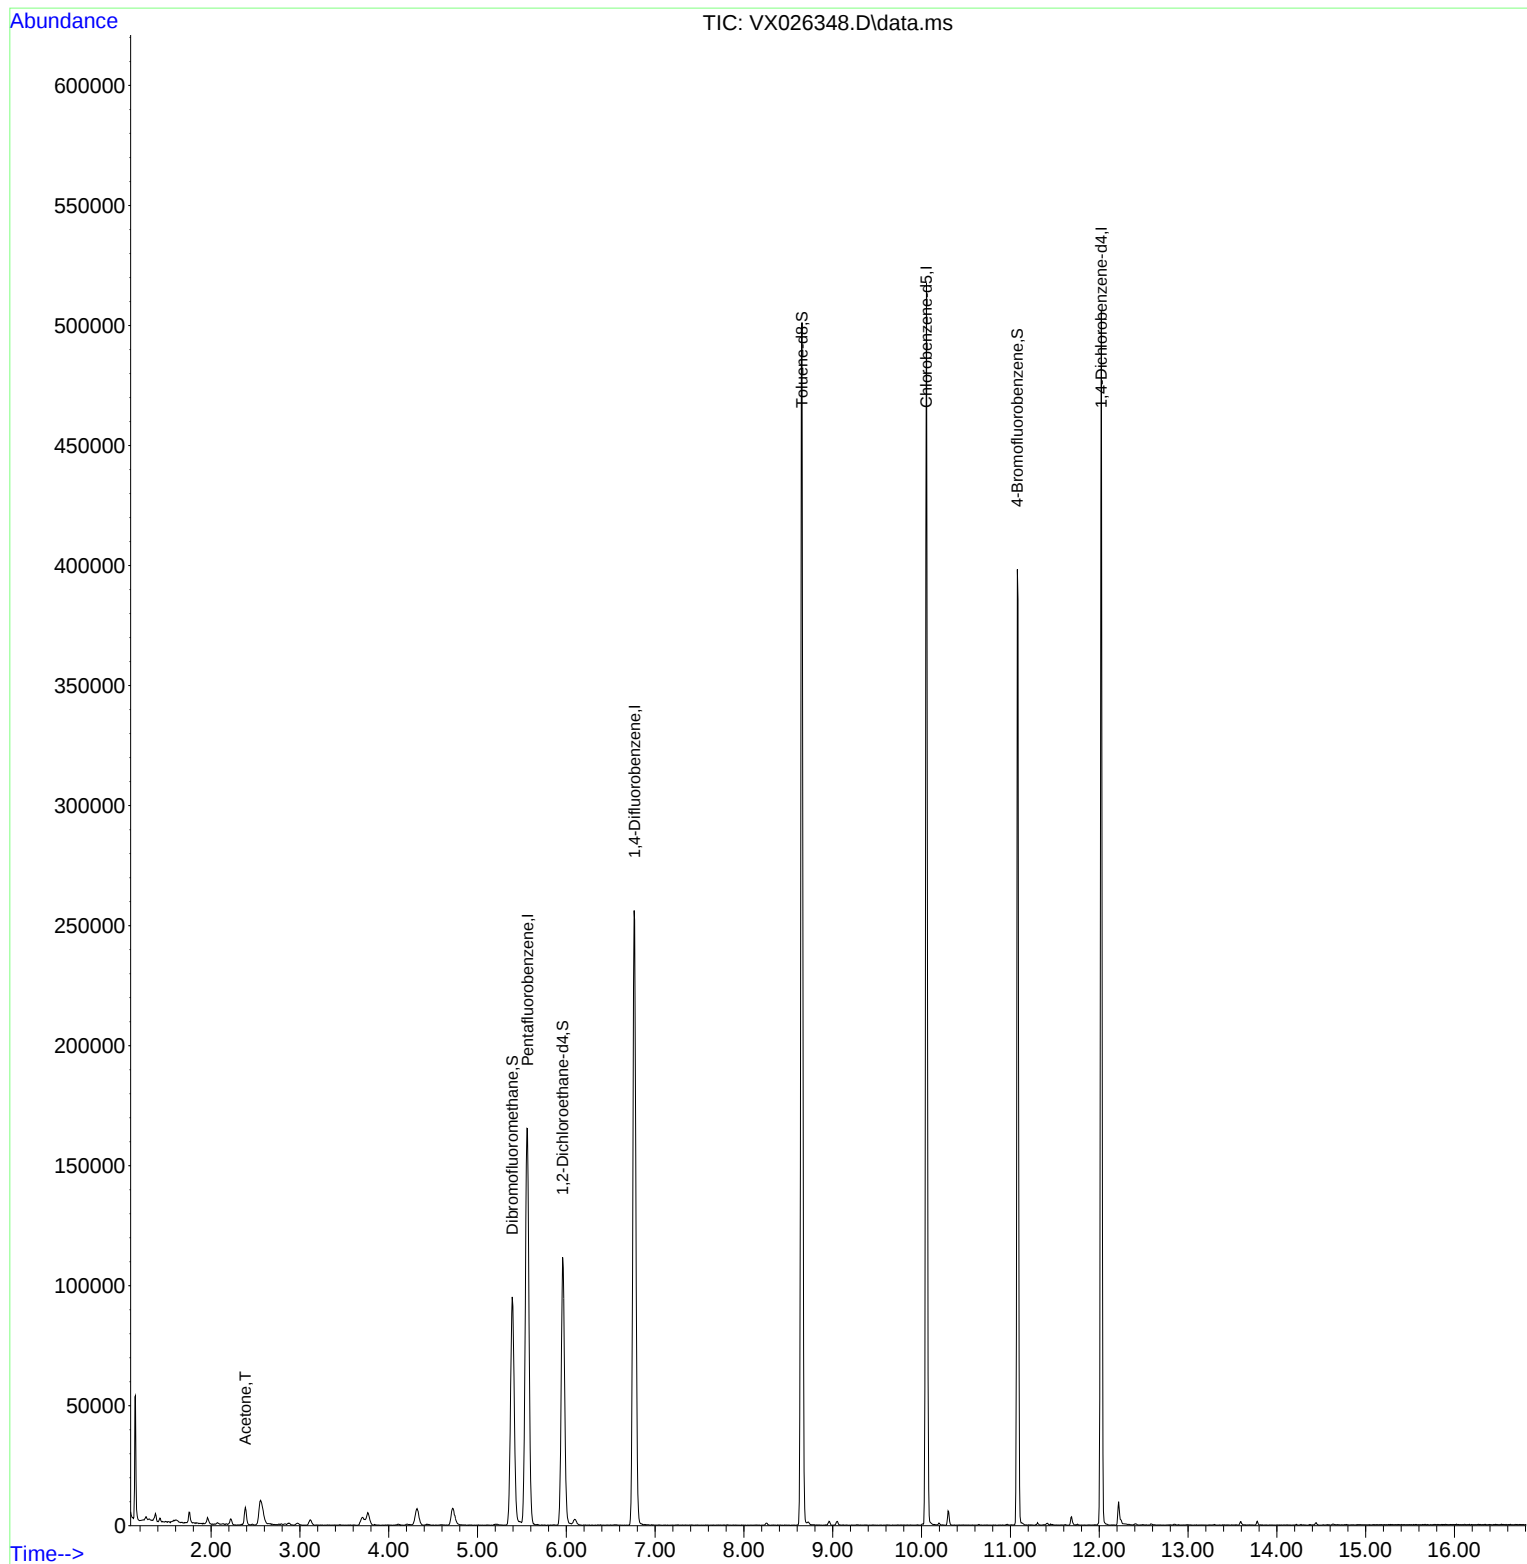




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX026348.D
Acq: 06 Jan 2022 02:02




Instrument :
MSVOA_X
ClientSampleId :
MW-26l


Tgt Ion:168 Resp: 153380
Ion Ratio Lower Upper
168 100
99 63.6 45.8 68.8

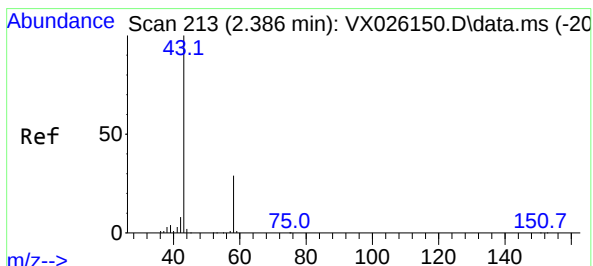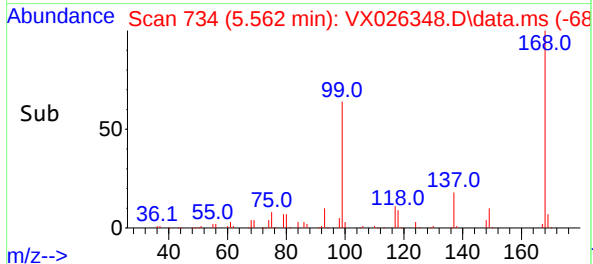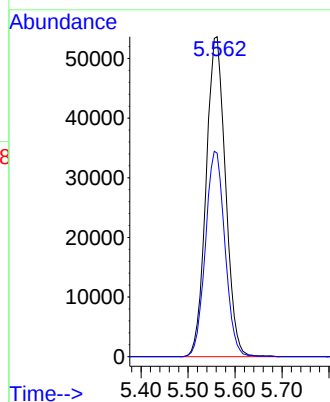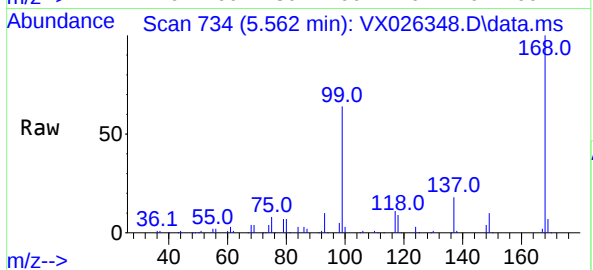

#16
Acetone
Concen: 6.966 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX026348.D
Acq: 06 Jan 2022 02:02

Tgt Ion: 43 Resp: 8375
Ion Ratio Lower Upper
43 100
58 26.1 24.8 37.2

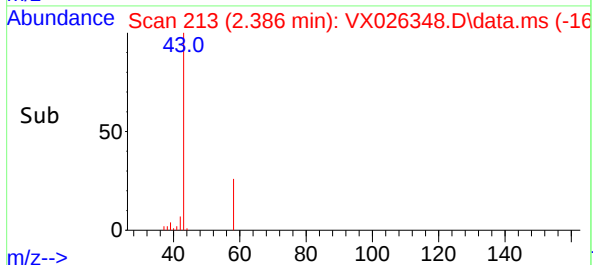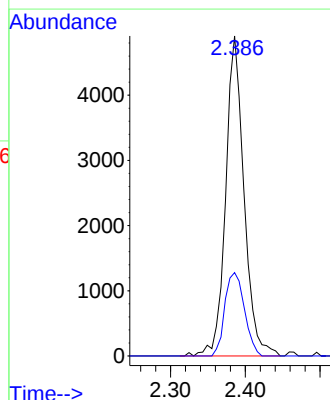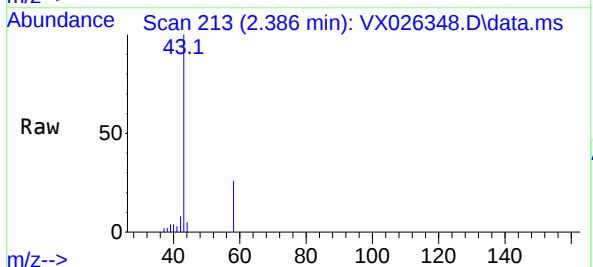

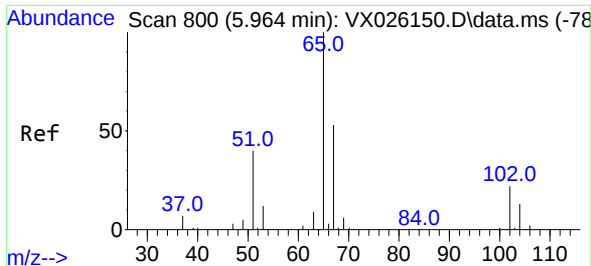

#33

1,2-Dichloroethane-d4

Concen: 49.995 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX026348.D

Acq: 06 Jan 2022 02:02

Instrument :

MSVOA_X

ClientSampleId :





MW-26I

Tgt Ion: 65 Resp: 110936

Ion Ratio Lower Upper

65 100

67 50.1 0.0 103.4

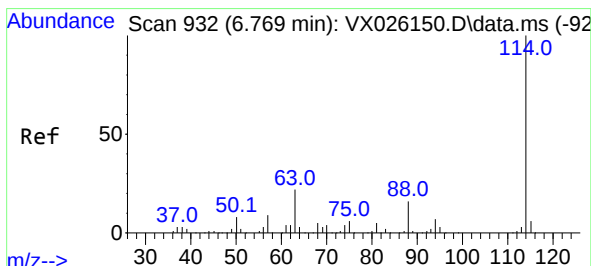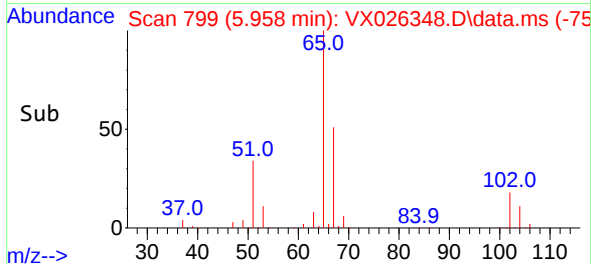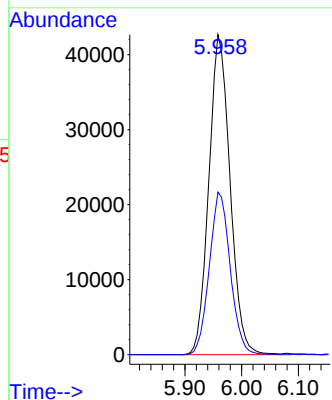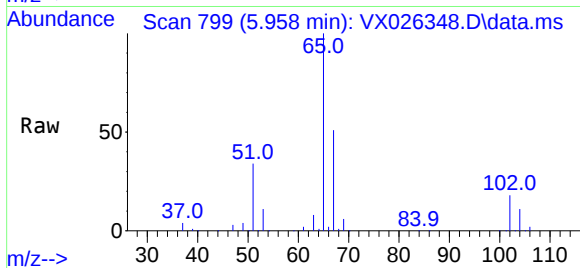

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. -0.000 min

Lab File: VX026348.D

Acq: 06 Jan 2022 02:02




Tgt Ion: 114 Resp: 255986


Ion Ratio Lower Upper

114 100

63 21.0 0.0 40.0


88 16.3 0.0 30.6

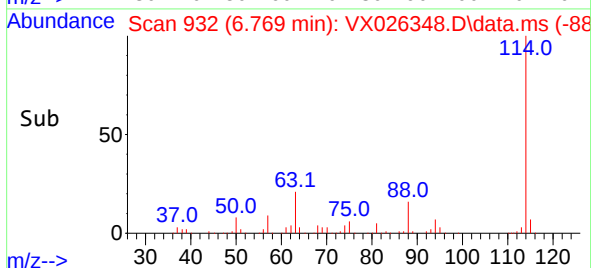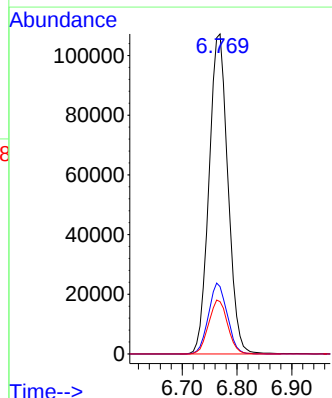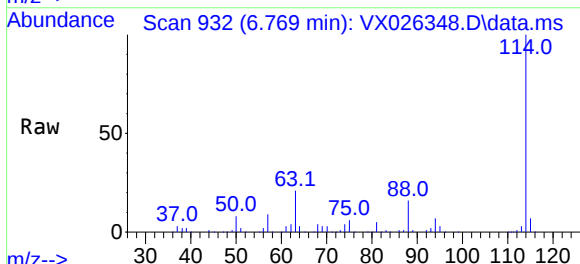



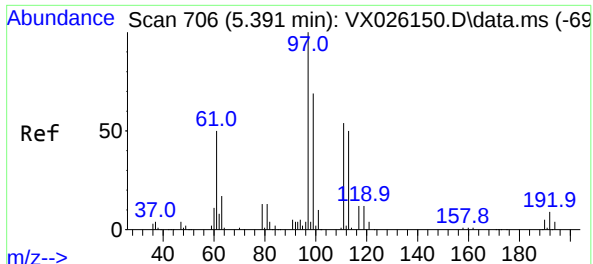


#35
Dibromofluoromethane
Concen: 49.906 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026348.D
Acq: 06 Jan 2022 02:02

Instrument :
MSVOA_X
ClientSampleId :
MW-26l



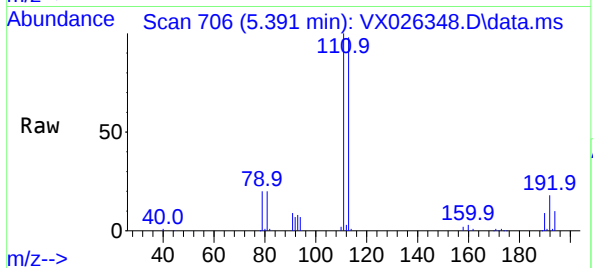



Tgt Ion:113 Resp: 83056
Ion Ratio Lower Upper
113 100
111 101.9 81.8 122.8
192 19.0 15.0 22.4

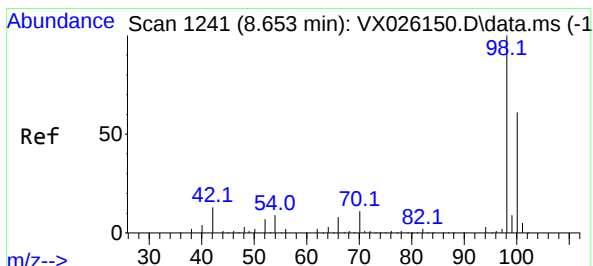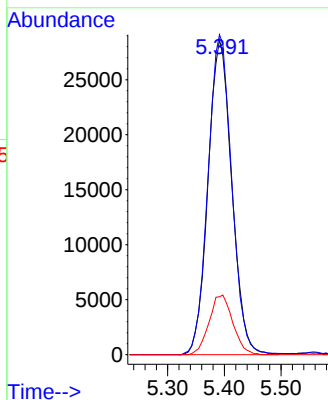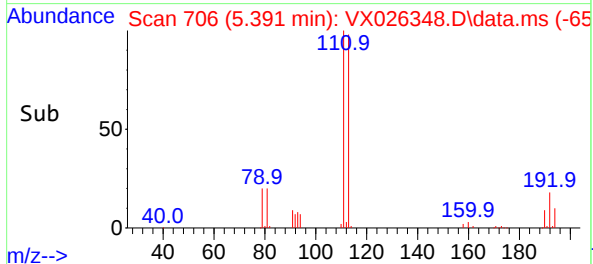

#50
Toluene-d8
Concen: 47.783 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX026348.D
Acq: 06 Jan 2022 02:02

Tgt Ion: 98 Resp: 295794
Ion Ratio Lower Upper
98 100
100 65.8 52.6 78.8


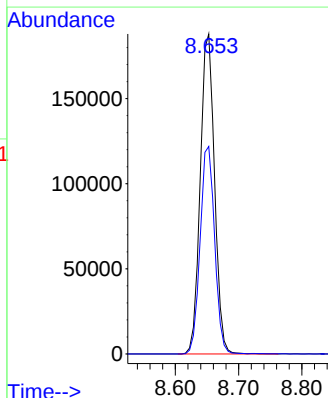
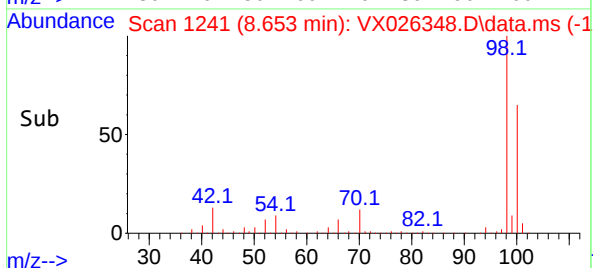
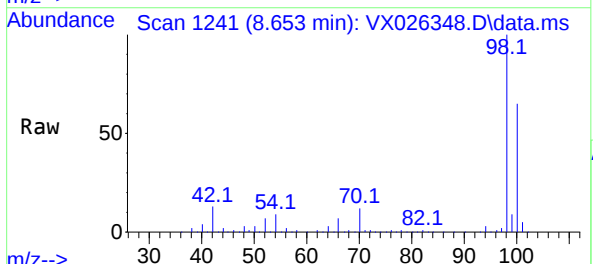


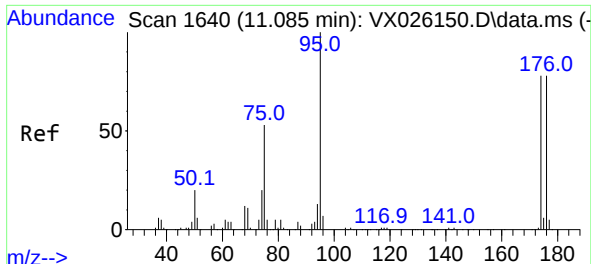

#62
4-Bromofluorobenzene
Concen: 49.875 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX026348.D
Acq: 06 Jan 2022 02:02




Instrument :
MSVOA_X
ClientSampleId :
MW-26I


Tgt Ion: 95 Resp: 109910
Ion Ratio Lower Upper
95 100
174 72.2 0.0 157.4
176 69.5 0.0 154.6

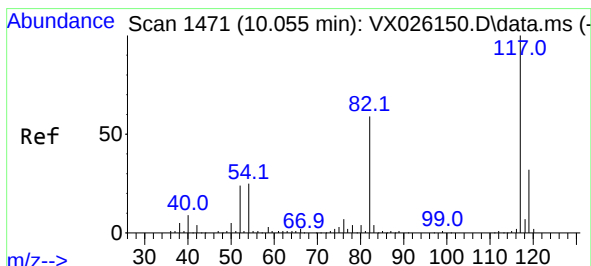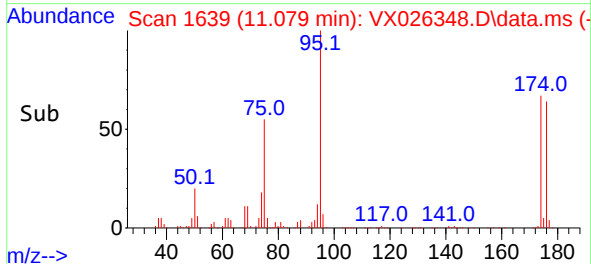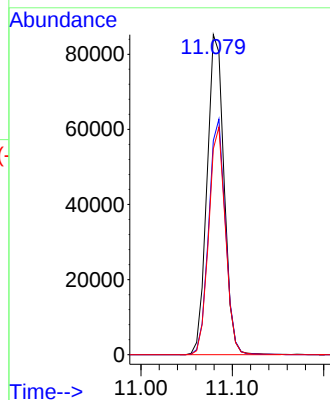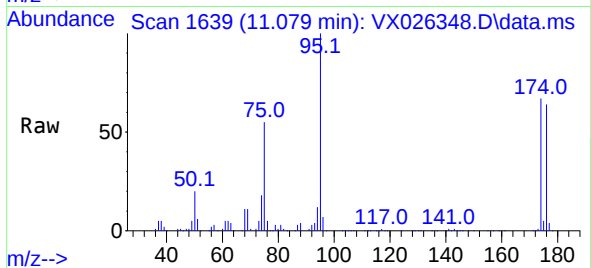

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026348.D
Acq: 06 Jan 2022 02:02


Tgt Ion: 117 Resp: 221122
Ion Ratio Lower Upper
117 100
82 58.2 43.8 65.6
119 32.1 25.2 37.8

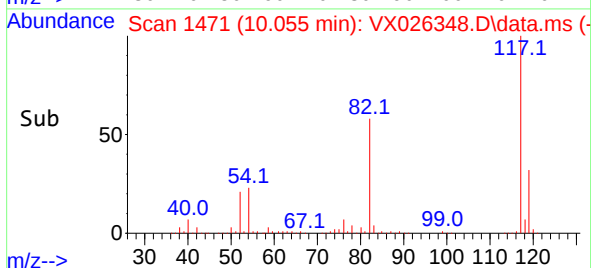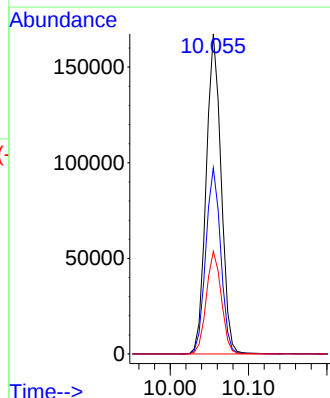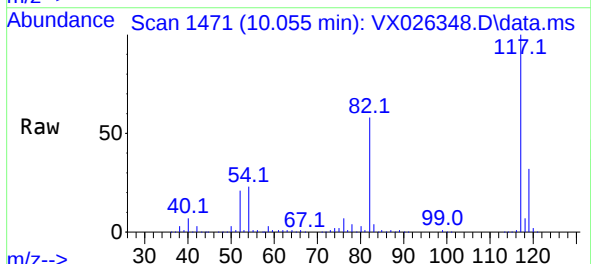

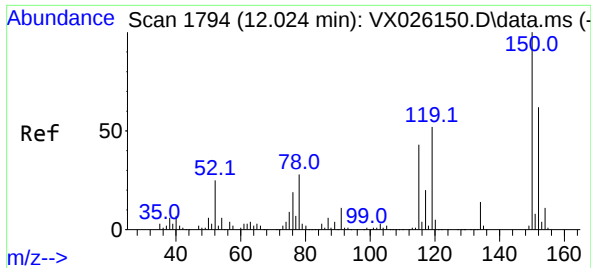

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX026348.D
 Acq: 06 Jan 2022 02:02

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-26I

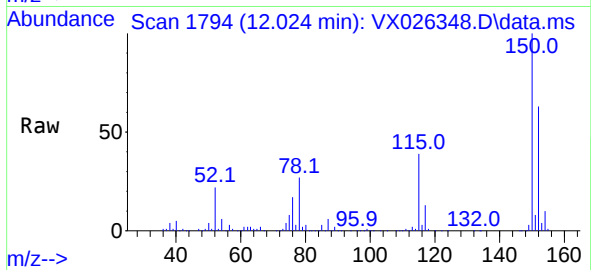

Tgt Ion:152 Resp: 96317
 Ion Ratio Lower Upper
 152 100
 115 62.7 41.3 123.9
 150 158.7 0.0 351.8

