

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
 Data File : VX026321.D
 Acq On : 05 Jan 2022 14:51
 Operator : JC/MD
 Sample : M5336-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 40563DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Title : SW846 8260

Signal : TIC: VX026321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	41	47	53	rBV2	256944	427533	1.31%	0.432%
2	2.380	205	212	218	rBV	966847	1615220	4.95%	1.631%
3	2.971	298	309	324	rBV2	970542	2138505	6.55%	2.159%
4	3.117	324	333	356	rVV	250625	616021	1.89%	0.622%
5	3.709	415	430	445	rBV	11057458	32650015	100.00%	32.962%
6	4.233	501	516	530	rBV2	1261951	3705813	11.35%	3.741%
7	5.556	723	733	750	rVB	155276	443443	1.36%	0.448%
8	6.050	805	814	817	rBV	354065	944101	2.89%	0.953%
9	6.769	919	932	944	rBV	238681	590811	1.81%	0.596%
10	7.226	991	1007	1026	rBV	1413115	3308854	10.13%	3.341%
11	7.580	1058	1065	1072	rBV	273055	508803	1.56%	0.514%
12	7.952	1119	1126	1136	rVB	467206	788338	2.41%	0.796%
13	8.653	1235	1241	1246	rBV	488656	758881	2.32%	0.766%
14	8.720	1246	1252	1257	rBV	1531323	2296444	7.03%	2.318%
15	8.769	1257	1260	1270	rVB	286629	411854	1.26%	0.416%
16	9.238	1332	1337	1346	rBV	1113221	1451264	4.44%	1.465%
17	9.488	1372	1378	1390	rBV	1708584	2498561	7.65%	2.522%
18	9.738	1409	1419	1426	rBV	614607	945979	2.90%	0.955%
19	10.055	1463	1471	1473	rBV	500092	737739	2.26%	0.745%
20	10.159	1482	1488	1491	rBV	1563958	1977528	6.06%	1.996%
21	10.195	1491	1494	1504	rVV	388363	504996	1.55%	0.510%
22	10.299	1506	1511	1519	rVB	1849483	2552188	7.82%	2.577%
23	10.439	1526	1534	1541	rBV	732517	1005643	3.08%	1.015%
24	10.506	1541	1545	1554	rVB	390488	487947	1.49%	0.493%
25	10.640	1562	1567	1572	rBV	1097581	1459692	4.47%	1.474%
26	10.756	1578	1586	1594	rBV	657619	959105	2.94%	0.968%
27	10.951	1613	1618	1623	rBV2	245858	337644	1.03%	0.341%
28	11.079	1635	1639	1643	rBV	397422	496810	1.52%	0.502%
29	11.134	1643	1648	1652	rVV	1748866	2130422	6.53%	2.151%
30	11.280	1668	1672	1681	rVB2	978097	1292799	3.96%	1.305%
31	11.384	1681	1689	1692	rBV	250263	444681	1.36%	0.449%
32	11.421	1692	1695	1698	rVV	543500	690904	2.12%	0.698%
33	11.457	1698	1701	1707	rVB2	314118	385853	1.18%	0.390%
34	11.573	1713	1720	1723	rBV	538364	672707	2.06%	0.679%
35	11.610	1723	1726	1734	rVB2	349099	460480	1.41%	0.465%
36	11.689	1734	1739	1745	rBV	9064481	10685062	32.73%	10.787%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
Data File : VX026321.D
Acq On : 05 Jan 2022 14:51
Operator : JC/MD
Sample : M5336-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
40563DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Title : SW846 8260

37	11.750	1745	1749	1753	rVV	404496	494602	1.51%	0.499%
38	11.872	1765	1769	1772	rVV	900194	1103655	3.38%	1.114%
39	11.957	1779	1783	1785	rVV	747232	908018	2.78%	0.917%
40	11.994	1785	1789	1792	rVV	3736251	4784369	14.65%	4.830%
41	12.024	1792	1794	1797	rVV	617164	735256	2.25%	0.742%
42	12.219	1822	1826	1833	rBV	3939961	4807239	14.72%	4.853%
43	12.305	1836	1840	1852	rVB3	482915	739347	2.26%	0.746%
44	12.414	1852	1858	1863	rBV	1060008	1337631	4.10%	1.350%
45	12.792	1915	1920	1926	rBV4	231890	377749	1.16%	0.381%
46	12.847	1926	1929	1935	rVV	303916	381922	1.17%	0.386%




Sum of corrected areas: 99052428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
Data File : VX026321.D
Acq On : 05 Jan 2022 14:51
Operator : JC/MD
Sample : M5336-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
40563DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

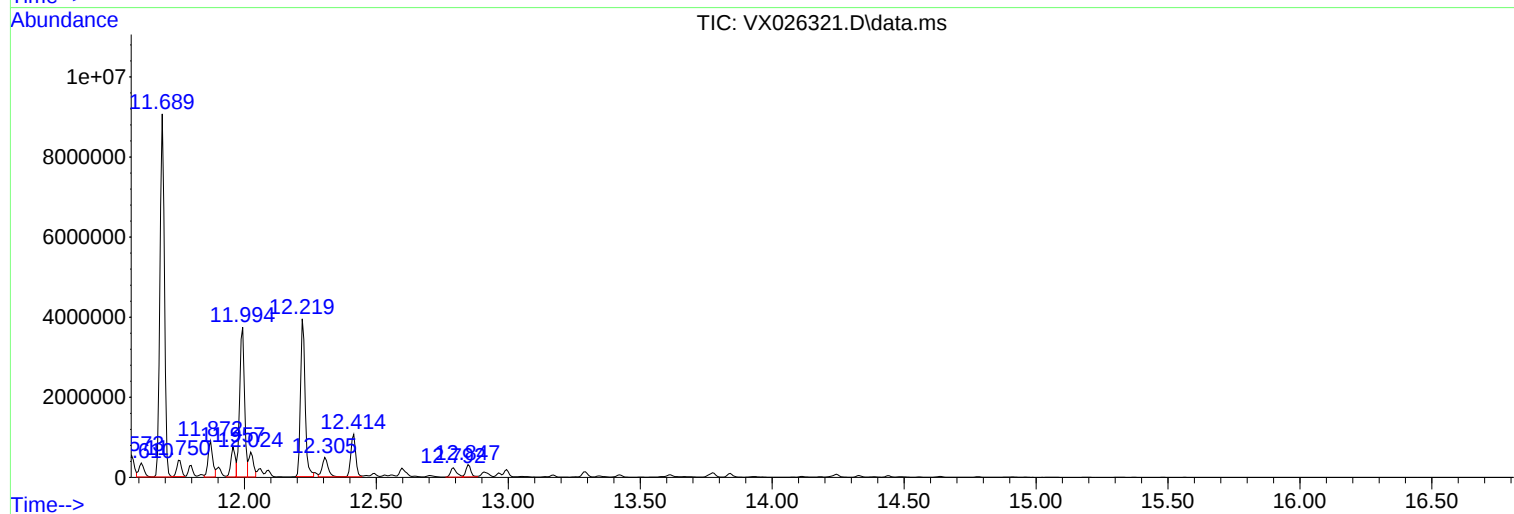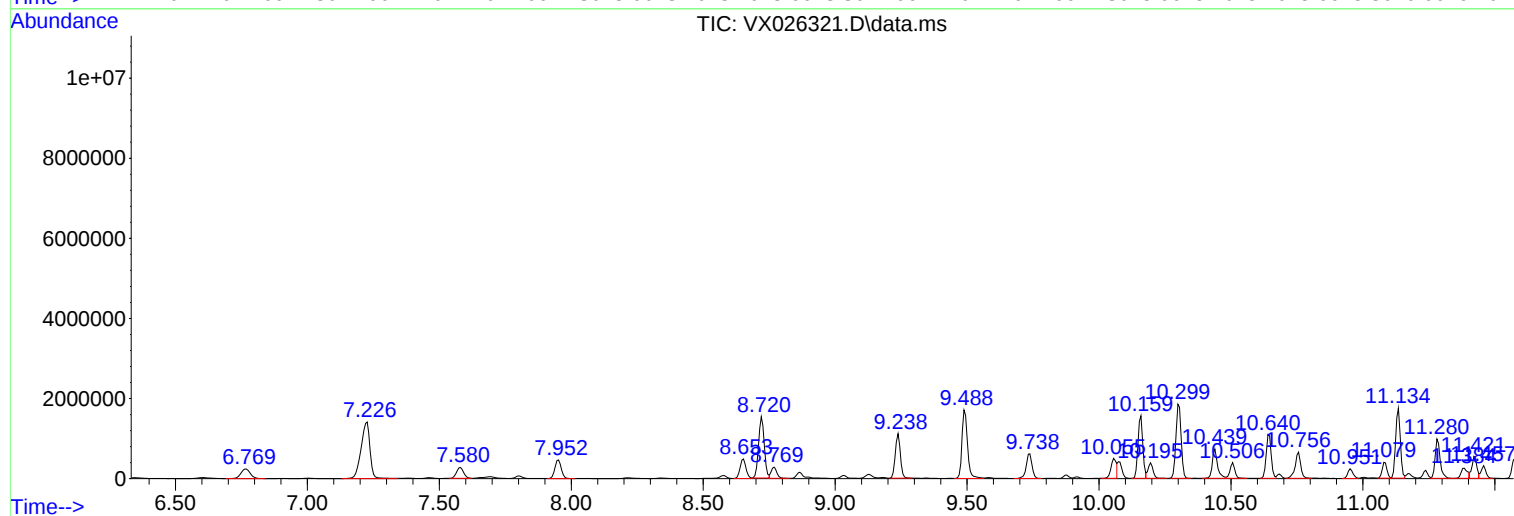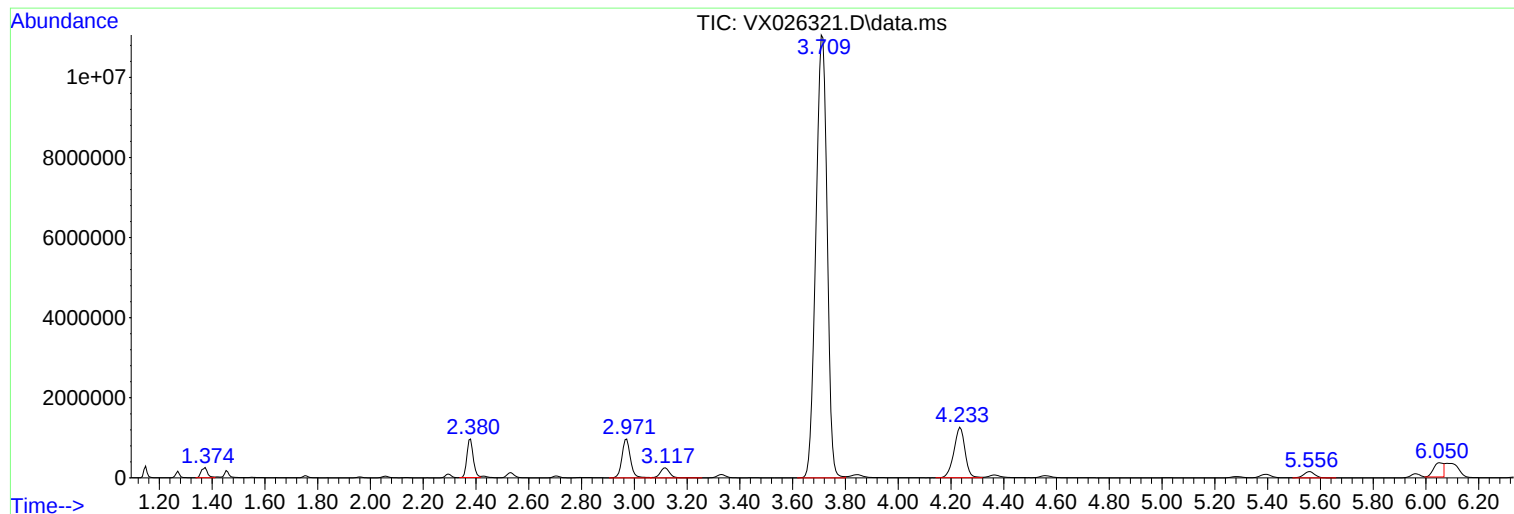

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
Data File : VX026321.D
Acq On : 05 Jan 2022 14:51
Operator : JC/MD
Sample : M5336-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
40563DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
Data File : VX026321.D
Acq On : 05 Jan 2022 14:51
Operator : JC/MD
Sample : M5336-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
40563DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc