
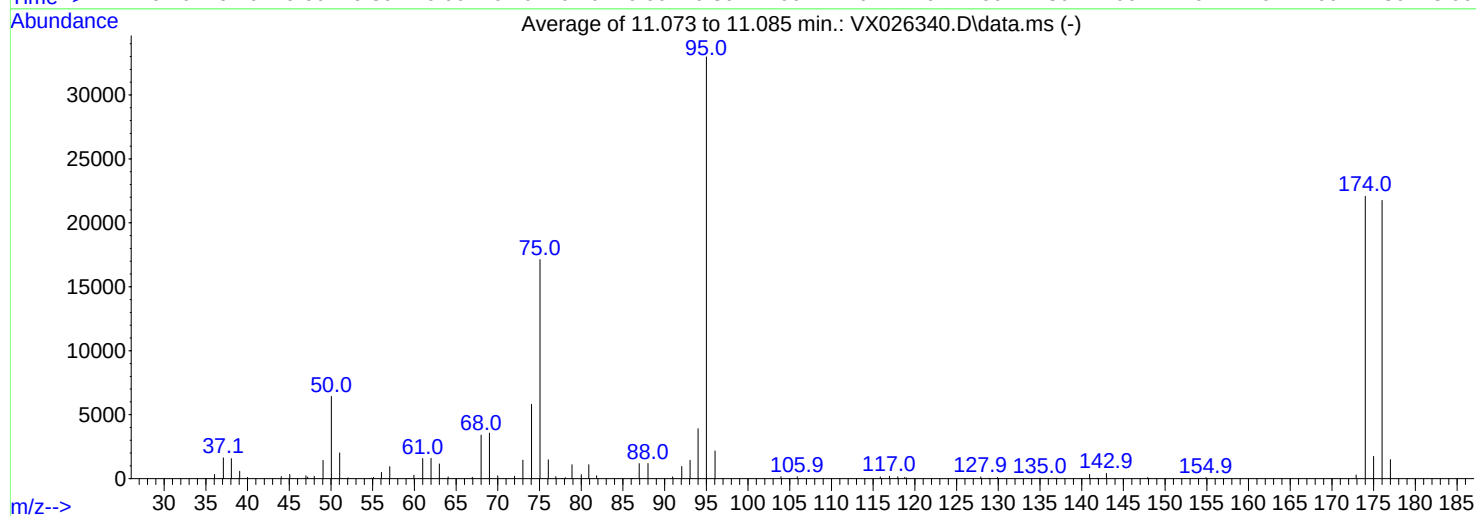


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010522\
Data File : VX026340.D
Acq On : 05 Jan 2022 22:34
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Title : SW846 8260
Last Update : Thu Dec 30 08:02:21 2021

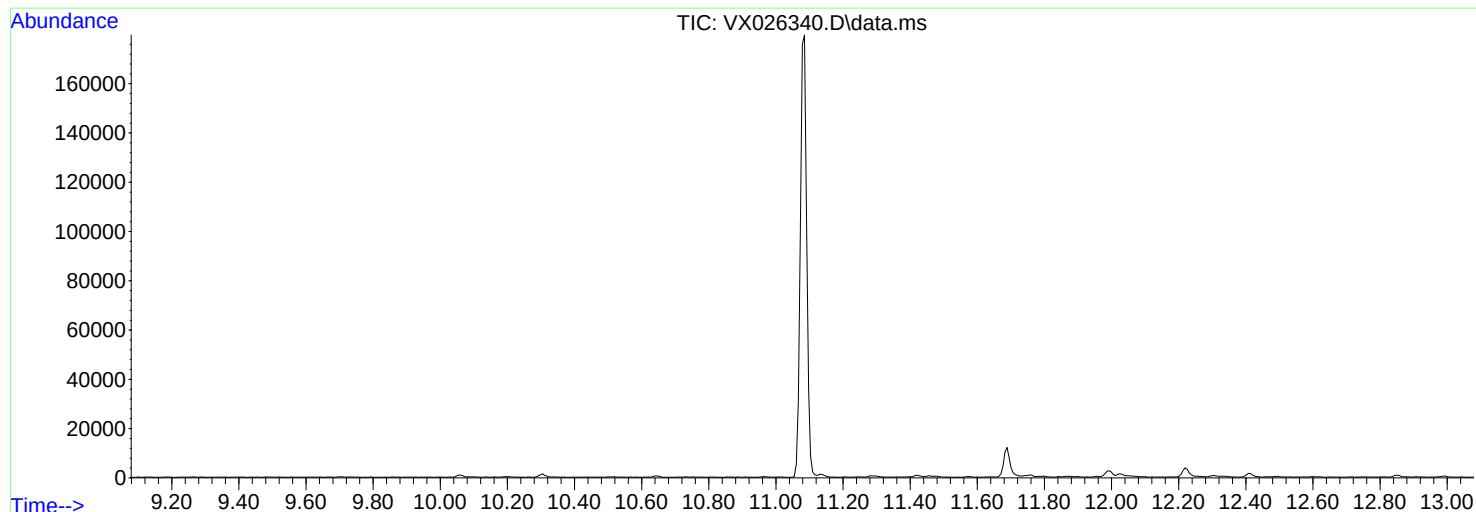

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	6428	PASS
75	95	30	60	51.9	17128	PASS
95	95	100	100	100.0	32979	PASS
96	95	5	9	6.6	2166	PASS
173	174	0.00	2	1.3	292	PASS
174	95	50	100	67.0	22085	PASS
175	174	5	9	7.9	1743	PASS
176	174	95	101	98.5	21751	PASS
177	176	5	9	6.8	1487	PASS