


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX010620\  
 Data File : VX014416.D  
 Acq On : 06 Jan 2020 09:19  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121319W.M  
 Title : SW846 8260  
 Last Update : Tue Dec 17 03:01:07 2019

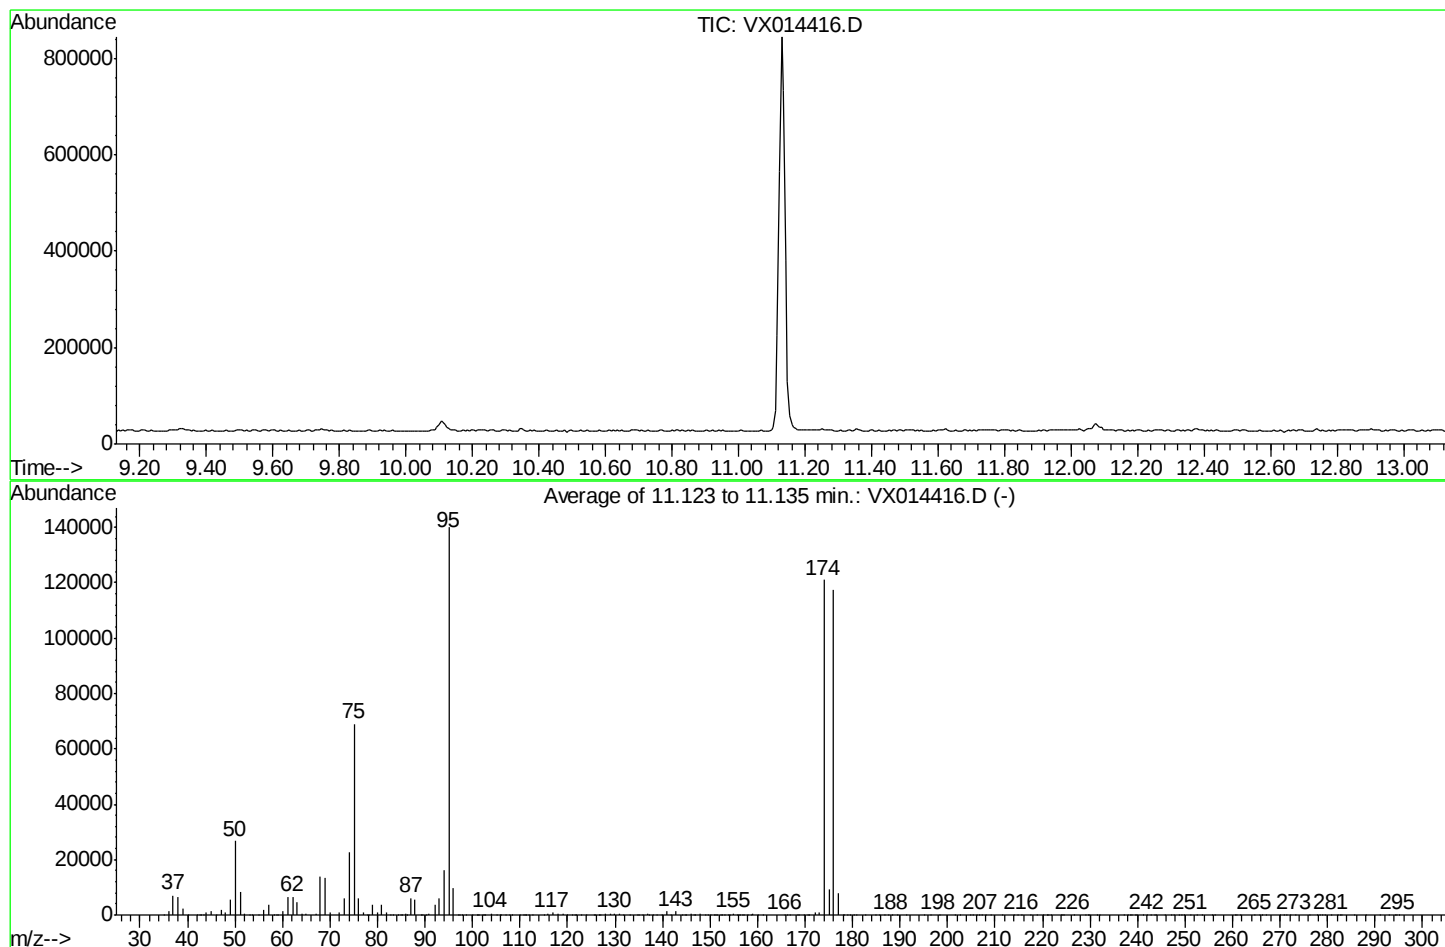

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1670

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.1      | 26789   | PASS             |
| 75          | 95           | 30           | 60           | 49.4      | 69111   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 140037  | PASS             |
| 96          | 95           | 5            | 9            | 7.0       | 9764    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 1058    | PASS             |
| 174         | 95           | 50           | 100          | 86.4      | 120976  | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 9051    | PASS             |
| 176         | 174          | 95           | 101          | 97.1      | 117451  | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 7791    | PASS             |