

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX010621\
 Data File : VX020511.D
 Acq On : 06 Jan 2021 10:12
 Operator : JC/MD
 Sample : VX0106WBL01
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0106WBL01

Quant Time: Jan 07 01:52:50 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR010521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 07 01:47:26 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.82	114	152834	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.09	117	155254	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	64804	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	59390	4.83	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.60%
7) Chloroethane-d5	1.69	69	55960	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.00%
11) 1,1-Dichloroethene-d2	2.34	63	92993	3.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.00%
20) 2-Butanone-d5	4.54	46	137039	51.44	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.88%
24) Chloroform-d	5.13	84	120698	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	6.03	65	60391	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
32) Benzene-d6	6.04	84	243085	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	7.36	67	73509	4.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.40%
41) Toluene-d8	8.69	98	201190	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.40%
43) trans-1,3-Dichloropropene-	8.99	79	24520	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	9.43	63	116251	48.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.48%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	52456	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.60%
66) 1,2-Dichlorobenzene-d4	12.36	152	70892	5.61	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.20%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	3926	0.280 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX010621\
Data File : VX020511.D
Acq On : 06 Jan 2021 10:12
Operator : JC/MD
Sample : VX0106WBL01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0106WBL01

Quant Time: Jan 07 01:52:50 2021
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR010521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 07 01:47:26 2021
Response via : Initial Calibration

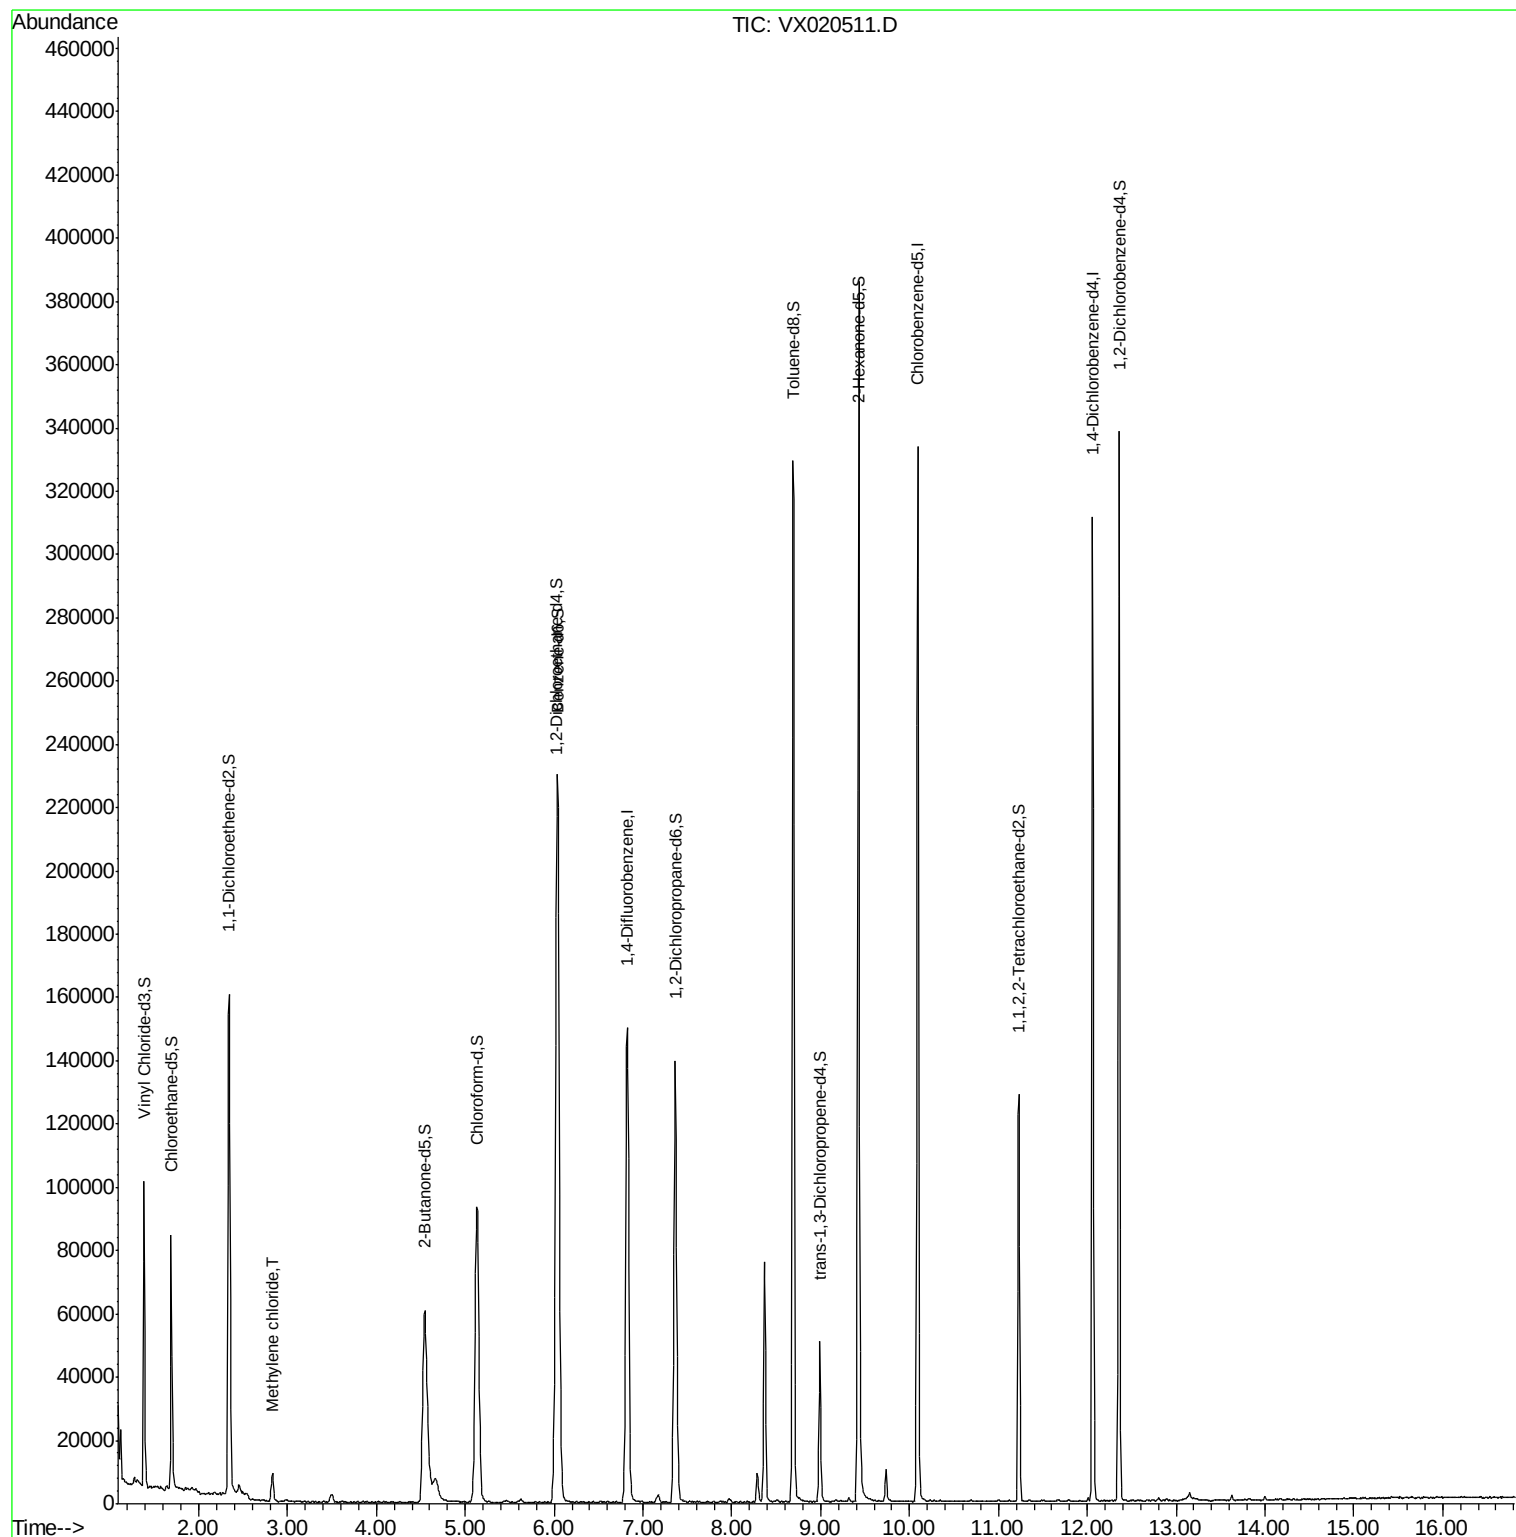

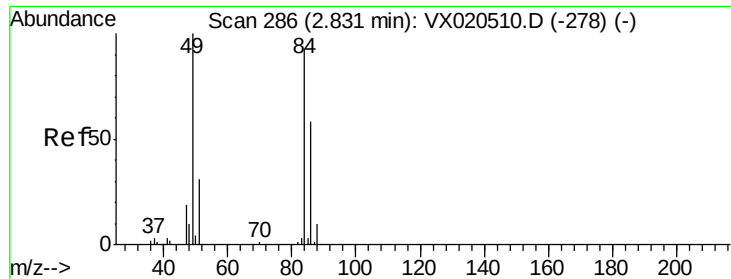

#16
 Methylene chloride
 Concen: 0.280 ug/L
 RT: 2.83 min Scan# 286
 Delta R.T. 0.00 min
 Lab File: VX020511.D
 Acq: 06 Jan 2021 10:12

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0106WBL01

Tot Ion: 84 Resp: 3926
 Ion Ratio Lower Upper
 84 100
 86 70.7 44.6 82.8
 49 116.4 79.5 147.6

