


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX010621\
 Data File : VX020509.D
 Acq On : 06 Jan 2021 08:55
 Operator : JC/MD
 Sample : BFB63
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB63

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR010521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Jan 07 17:08:59 2021

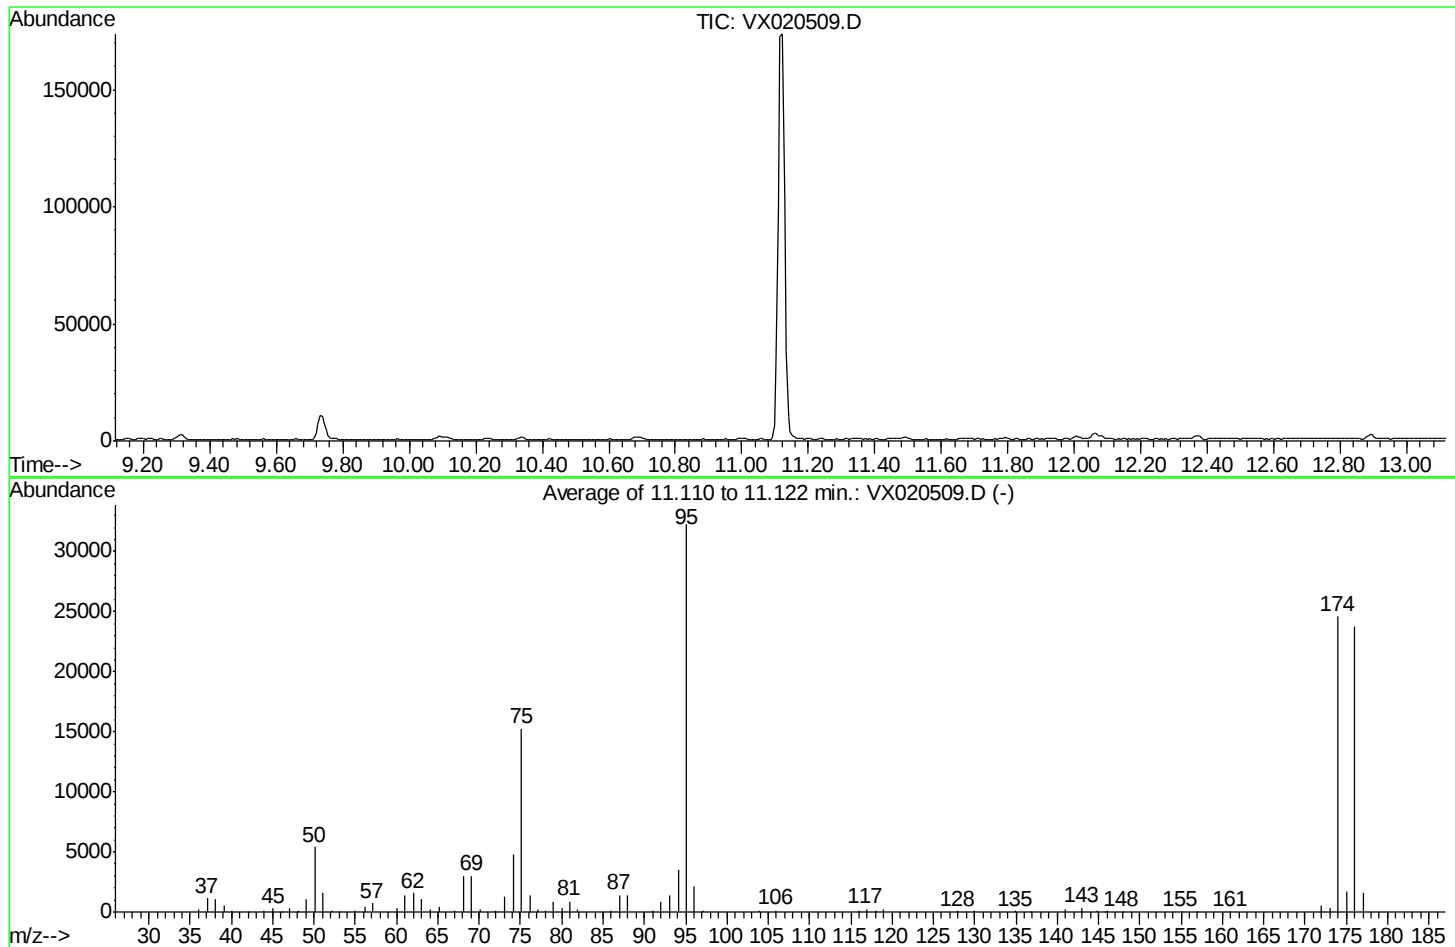

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	5391	PASS
75	95	30	80	47.2	15239	PASS
95	95	100	100	100.0	32264	PASS
96	95	5	9	6.5	2109	PASS
173	174	0.00	2	1.2	288	PASS
174	95	50	120	76.2	24575	PASS
175	174	5	9	7.1	1746	PASS
176	174	95	105	96.7	23752	PASS
177	176	5	10	6.6	1561	PASS

m/z	Abundance
35.10	181.0
37.10	863.0
38.10	854.0
39.10	385.0
40.00	196.0
44.10	561.0
45.10	250.0
47.00	286.0
48.00	128.0
49.00	795.0
50.10	4363.0
51.10	1339.0
52.20	98.0
55.00	77.0
56.10	413.0
57.10	567.0
60.10	175.0
61.00	1069.0
62.00	1147.0
63.10	747.0
64.00	148.0
65.10	264.0
67.00	60.0
68.00	1996.0
69.00	2290.0
70.10	223.0
72.00	84.0
73.00	917.0
74.10	3655.0
75.10	10646.0
76.10	1092.0
77.10	156.0
78.10	156.0
79.00	559.0
80.00	139.0
81.00	708.0
82.00	193.0
87.00	979.0
87.90	957.0
91.00	92.0
92.00	591.0
93.00	891.0
94.10	2649.0
95.10	22384.0
96.10	1622.0
97.00	54.0
103.90	62.0
105.90	88.0
116.00	110.0
116.90	176.0
117.90	87.0
118.90	134.0
128.00	78.0
134.90	55.0
141.10	174.0
143.00	234.0
145.00	73.0
146.00	58.0
172.00	241.0
173.00	157.0
174.00	14495.0
175.00	967.0
176.00	13425.0
177.00	1118.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63

m/z	Abundance
36.00	218.0
37.00	1155.0
38.10	1097.0
39.10	593.0
40.10	243.0
44.00	658.0
45.00	271.0
46.20	78.0
47.10	329.0
48.10	163.0
49.00	1121.0
50.10	5405.0
51.10	1735.0
52.20	82.0
53.00	77.0
54.90	73.0
56.10	351.0
57.00	682.0
60.10	275.0
61.00	1474.0
62.10	1704.0
63.10	1161.0
64.10	291.0
65.10	516.0
67.00	82.0
68.10	3229.0
69.10	3341.0
70.00	221.0
72.00	187.0
73.10	1513.0
74.10	5141.0
75.10	16936.0
76.10	1366.0
77.10	199.0
77.80	126.0
78.90	1060.0
80.00	305.0
81.00	971.0
81.90	278.0
85.90	82.0
87.00	1651.0
87.90	1547.0
91.00	134.0
92.10	1021.0
93.10	1707.0
94.10	3903.0
95.10	36608.0
96.00	2250.0
97.10	54.0
104.00	153.0
105.90	170.0
115.80	91.0
116.90	221.0
118.10	133.0
118.90	219.0
127.90	77.0
128.90	101.0
129.90	119.0
134.90	75.0
140.90	283.0
143.00	441.0
144.90	168.0
145.70	55.0
146.10	58.0
147.80	82.0
155.00	59.0
157.00	52.0
171.90	638.0
173.10	417.0
174.00	31024.0
175.00	2228.0
176.00	31520.0
177.00	1715.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63

m/z	Abundance
35.90	322.0
37.10	1473.0
38.00	1377.0
39.10	553.0
40.00	231.0
42.00	57.0
44.00	666.0
45.10	380.0
46.10	61.0
47.10	453.0
48.20	164.0
49.00	1412.0
50.10	6407.0
51.10	1864.0
52.00	83.0
55.00	110.0
56.10	424.0
57.00	875.0
60.10	361.0
61.10	1676.0
62.10	1815.0
63.00	1363.0
64.00	254.0
65.10	451.0
67.00	68.0
68.00	3703.0
69.10	3485.0
70.00	271.0
72.10	146.0
73.00	1474.0
74.10	5753.0
75.10	18136.0
76.10	1762.0
77.00	245.0
77.90	112.0
79.00	932.0
80.00	395.0
80.90	1047.0
81.90	226.0
85.90	93.0
87.00	1649.0
88.00	1504.0
91.00	107.0
92.00	928.0
93.00	1534.0
94.10	4003.0
95.10	37800.0
96.10	2456.0
97.00	78.0
104.00	140.0
106.00	127.0
116.00	144.0
116.90	301.0
118.00	122.0
119.00	166.0
127.90	147.0
128.80	71.0
129.90	157.0
135.00	87.0
136.80	68.0
141.00	350.0
143.00	437.0
144.80	203.0
146.10	64.0
148.00	88.0
161.00	56.0
172.00	588.0
173.10	290.0
174.00	28208.0
175.00	2044.0
176.00	26312.0
177.00	1850.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63

Scan 1638 (11.073 min): VX020509.D
BFB63

m/z	Abundance
40.00	161.0
44.00	527.0
207.10	70.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63