

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
 Data File : VX026371.D
 Acq On : 06 Jan 2022 14:21
 Operator : JC/MD
 Sample : N1019-07DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 07 04:13:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	156598	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	259982	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	218598	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	92684	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	110518	48.783	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.560%
35) Dibromofluoromethane	5.391	113	83648	49.489	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.980%
50) Toluene-d8	8.653	98	299182	47.587	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.180%
62) 4-Bromofluorobenzene	11.079	95	107104	47.855	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.700%
Target Compounds						
					Qvalue	
5) Bromomethane	1.624	94	341	0.274	ug/l	86
10) Methyl Iodide	2.465	142	1059	0.448	ug/l #	94
11) Tert butyl alcohol	2.947	59	672	1.485	ug/l #	73
13) Acrolein	2.221	56	1164	7.194	ug/l #	1
14) Allyl chloride	2.721	41	847	0.247	ug/l #	54
15) Acrylonitrile	3.105	53	396	0.353	ug/l #	33
16) Acetone	2.392	43	2509	2.044	ug/l	99
18) Methyl Acetate	2.715	43	908	0.228	ug/l #	56
20) Methylene Chloride	2.800	84	777	Below Cal	#	92
25) 2-Butanone	4.599	43	374	0.219	ug/l #	49
31) Cyclohexane	5.477	56	9035	2.800	ug/l	92
36) 1,1-Dichloropropene	5.556	75	13167	4.830	ug/l #	49
37) Ethyl Acetate	4.733	43	2239	0.708	ug/l #	88
38) Carbon Tetrachloride	5.556	117	16603	5.475	ug/l #	15
39) Methylcyclohexane	7.379	83	2045	0.665	ug/l #	77
40) Benzene	6.037	78	3132	0.403	ug/l	95
52) Toluene	8.720	92	12850	2.683	ug/l	98
53) t-1,3-Dichloropropene	8.720	75	163	1.942	ug/l #	1
58) 2-Chloroethyl Vinyl ether	8.147	63	124	9.902	ug/l #	44
67) Ethyl Benzene	10.195	91	310634	36.177	ug/l	98
68) m/p-Xylenes	10.305	106	86319	26.924	ug/l	90
69) o-Xylene	10.640	106	50860	16.214	ug/l	92
70) Styrene	10.640	104	2841	0.552	ug/l #	1
73) Isopropylbenzene	10.963	105	10578	1.468	ug/l	95
76) 1,2,3-Trichloropropane	11.079	75	56207	25.124	ug/l #	39
78) n-propylbenzene	11.305	91	12600	1.521	ug/l	97
79) 2-Chlorotoluene	11.378	91	3992	0.783	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	3937	0.659	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	56207	72.685	ug/l #	10
83) tert-Butylbenzene	11.750	119	18529	3.193	ug/l #	49
84) 1,2,4-Trimethylbenzene	11.750	105	156166	26.141	ug/l	97
85) sec-Butylbenzene	11.750	105	156166	21.565	ug/l #	56
90) Hexachloroethane	12.701	117	5142	4.264	ug/l #	14
94) Hexachlorobutadiene	13.725	225	212	0.260	ug/l	69
95) Naphthalene	13.780	128	42020	5.866	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
Data File : VX026371.D
Acq On : 06 Jan 2022 14:21
Operator : JC/MD
Sample : N1019-07DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jan 07 04:13:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
Data File : VX026371.D
Acq On : 06 Jan 2022 14:21
Operator : JC/MD
Sample : N1019-07DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 07 04:13:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration

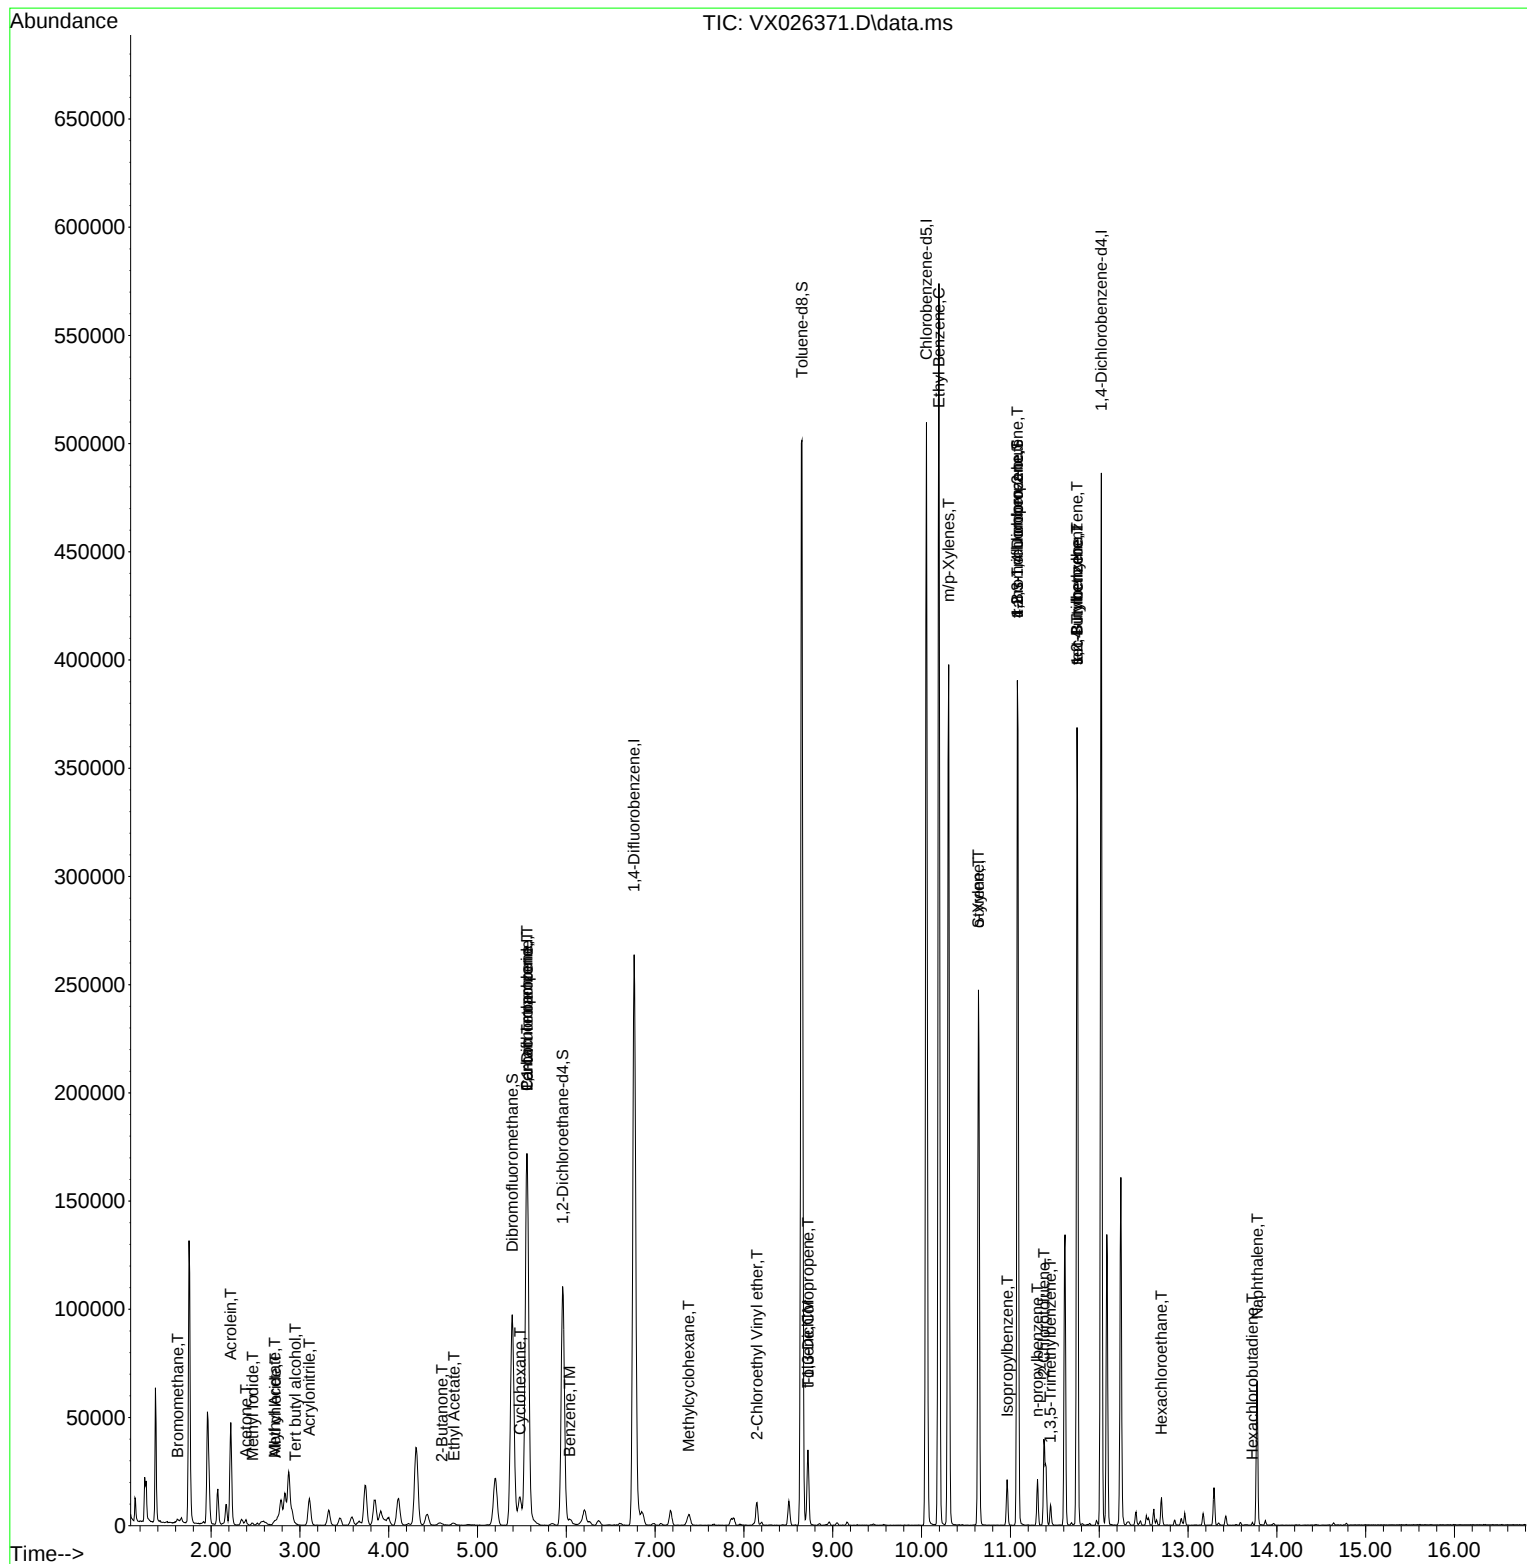






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 156598
Ion Ratio Lower Upper
168 100
99 63.2 45.8 68.8

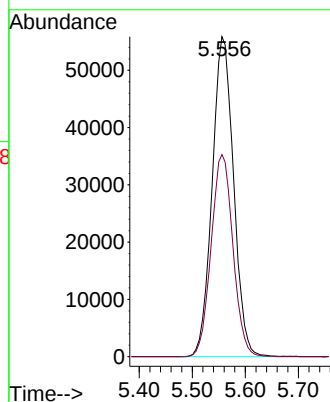

#5
Bromomethane
Concen: 0.274 ug/l
RT: 1.624 min Scan# 88
Delta R.T. 0.013 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21


Tgt Ion: 94 Resp: 341
Ion Ratio Lower Upper
94 100
96 80.1 75.0 112.4

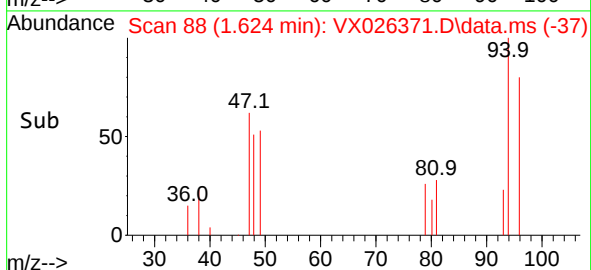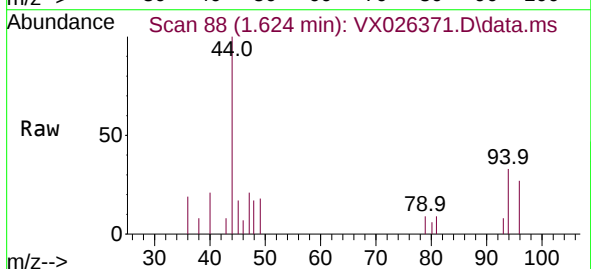






#10
Methyl Iodide
Concen: 0.448 ug/l
RT: 2.465 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:142 Resp: 1059
Ion Ratio Lower Upper
142 100
127 43.1 37.5 56.3
141 11.0 11.4 17.0#

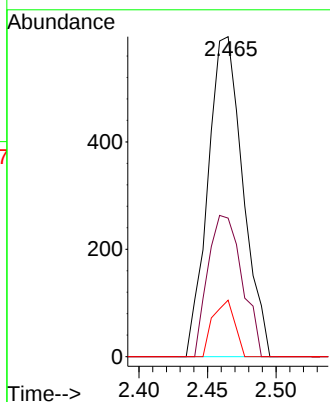


#11
Tert butyl alcohol
Concen: 1.485 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.036 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21



Tgt Ion: 59 Resp: 672
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

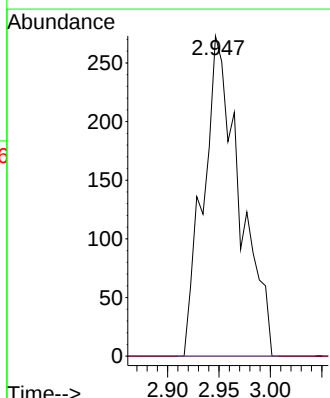



#13

Acrolein

Concen: 7.194 ug/l

RT: 2.221 min Scan# 186

Delta R.T. -0.018 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 56 Resp: 1164

Ion Ratio Lower Upper

56 100

55 2126.7 57.4 86.2#

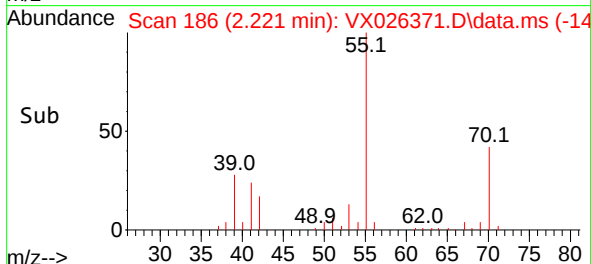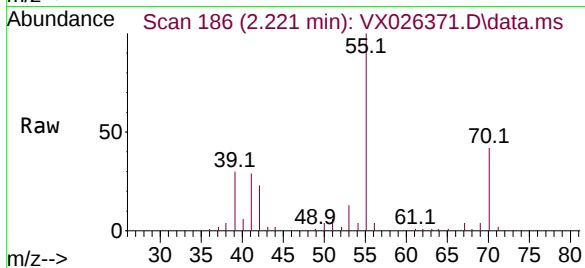

#14

Allyl chloride

Concen: 0.247 ug/l

RT: 2.721 min Scan# 268

Delta R.T. 0.049 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21




Tgt Ion: 41 Resp: 847


Ion Ratio Lower Upper

41 100

39 37.8 55.4 83.0#


76 0.0 27.6 41.4#

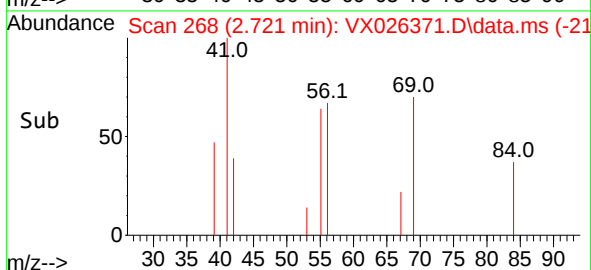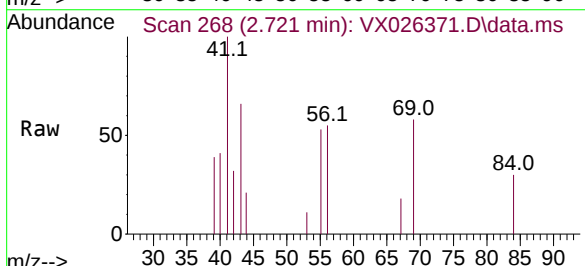






#15
Acrylonitrile
Concen: 0.353 ug/l
RT: 3.105 min Scan# 31
Delta R.T. 0.036 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 53 Resp: 396
Ion Ratio Lower Upper
53 100
52 0.0 66.2 99.2#
51 42.9 29.4 44.0



#16
Acetone
Concen: 2.044 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Tgt Ion: 43 Resp: 2509
Ion Ratio Lower Upper
43 100
58 30.5 24.8 37.2


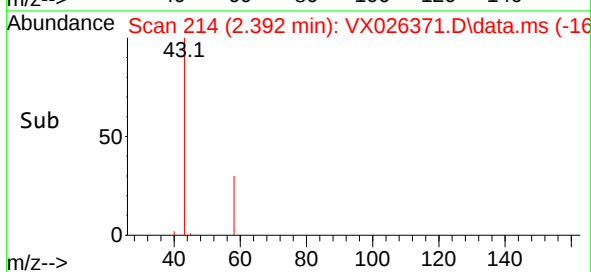






#18
Methyl Acetate
Concen: 0.228 ug/l
RT: 2.715 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 908
Ion Ratio Lower Upper
43 100
74 2.4 19.1 28.7#

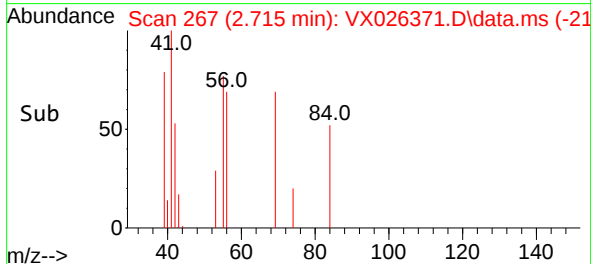

#20
Methylene Chloride
Concen: Below Cal
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Tgt Ion: 84 Resp: 777
Ion Ratio Lower Upper
84 100
49 113.9 97.1 145.7
51 25.4 29.3 43.9#
86 66.6 50.8 76.2

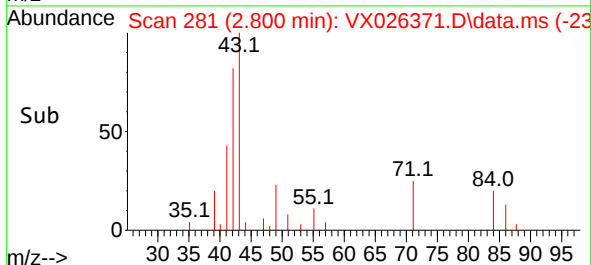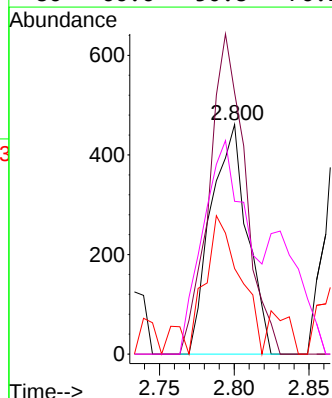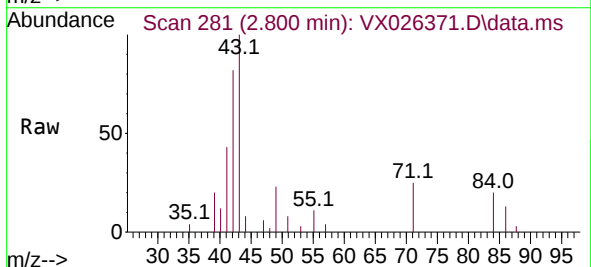



#25

2-Butanone

Concen: 0.219 ug/l

RT: 4.599 min Scan# 51

Delta R.T. 0.037 min


Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 43 Resp: 374

Ion Ratio Lower Upper

43 100

72 0.0 21.0 31.4#



#31

Cyclohexane

Concen: 2.800 ug/l

RT: 5.477 min Scan# 720

Delta R.T. -0.000 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21




Tgt Ion: 56 Resp: 9035


Ion Ratio Lower Upper

56 100

69 27.1 23.9 35.9

84 83.6 73.2 109.8


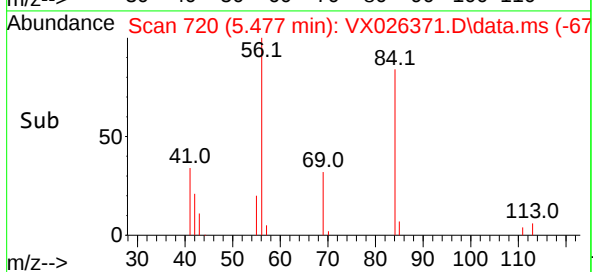






#33
 1,2-Dichloroethane-d4
 Concen: 48.783 ug/l
 RT: 5.958 min Scan# 799
 Delta R.T. -0.006 min
 Lab File: VX026371.D
 Acq: 06 Jan 2022 14:21




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 65 Resp: 110518
 Ion Ratio Lower Upper
 65 100
 67 50.8 0.0 103.4

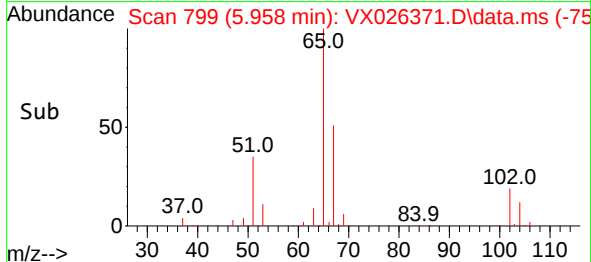

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. -0.006 min
 Lab File: VX026371.D
 Acq: 06 Jan 2022 14:21

Tgt Ion: 114 Resp: 259982
 Ion Ratio Lower Upper
 114 100
 63 22.4 0.0 40.0
 88 17.1 0.0 30.6

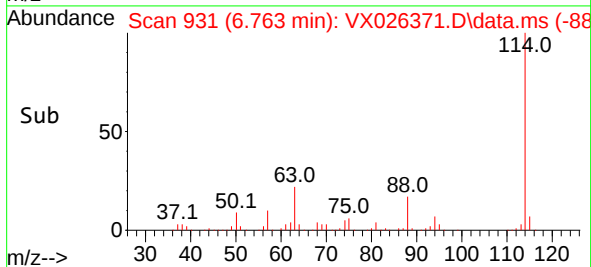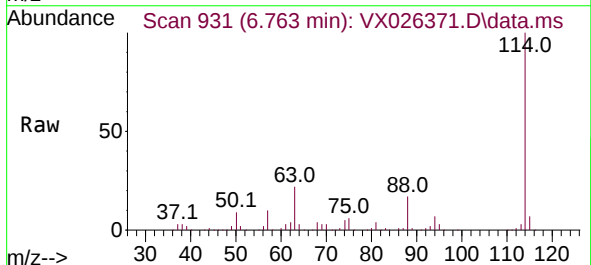



#35

Dibromofluoromethane

Concen: 49.489 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min


Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X

ClientSampleId :

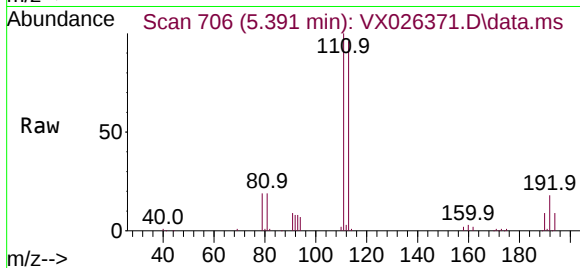




Tgt Ion:113 Resp: 83648

Ion Ratio Lower Upper

113 100

111 102.8 81.8 122.8

192 18.7 15.0 22.4



#36

1,1-Dichloropropene

Concen: 4.830 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.146 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21




Tgt Ion: 75 Resp: 13167


Ion Ratio Lower Upper

75 100

110 9.4 18.2 54.6#

77 0.0 24.7 37.1#

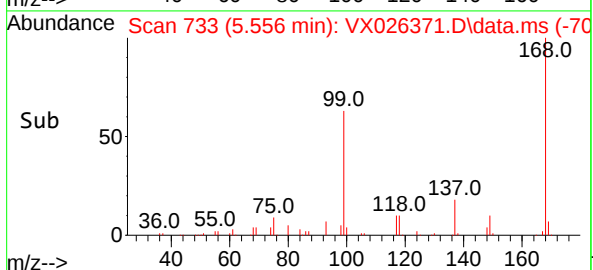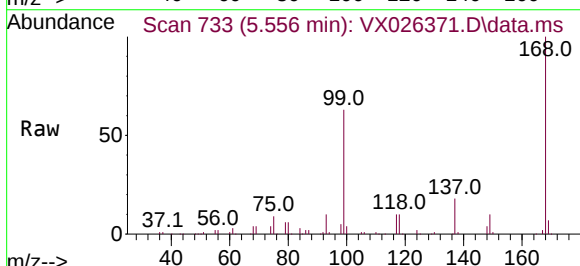



#37

Ethyl Acetate

Concen: 0.708 ug/l

RT: 4.733 min Scan# 596

Delta R.T. 0.012 min


Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X

ClientSampleId :

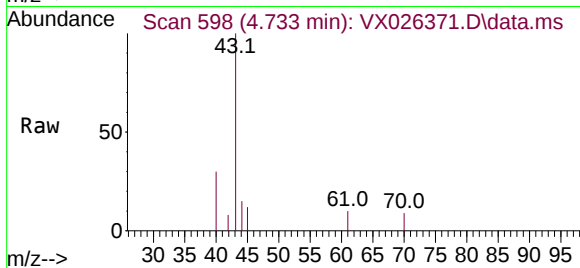




Tgt Ion: 43 Resp: 2239

Ion Ratio Lower Upper

43 100

61 9.1 10.7 16.1#

70 5.1 8.5 12.7#



#38

Carbon Tetrachloride

Concen: 5.475 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21




Tgt Ion: 117 Resp: 16603


Ion Ratio Lower Upper

117 100

119 4.1 77.2 115.8#

121 0.0 23.8 35.8#

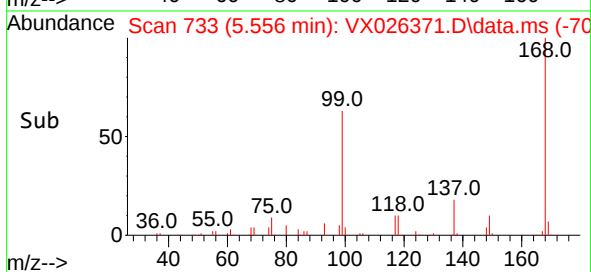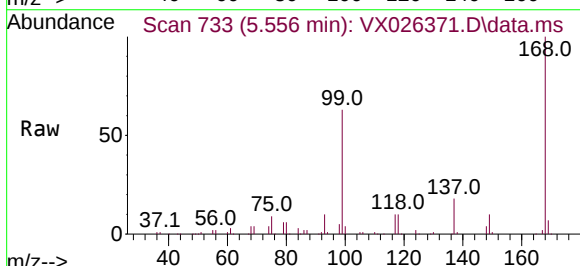



#39

Methylcyclohexane

Concen: 0.665 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. -0.006 min


Lab File: VX026371.D

Acq: 06 Jan 2022 14:21




Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion:	83	Resp:	2045
Ion	Ratio	Lower	Upper
83	100		
55	88.9	57.8	86.8#
98	31.8	40.5	60.7#



#40

Benzene

Concen: 0.403 ug/l




RT: 6.037 min Scan# 812


Delta R.T. -0.007 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Tgt Ion:	78	Resp:	3132
Ion	Ratio	Lower	Upper
78	100		
77	25.4	18.6	27.8


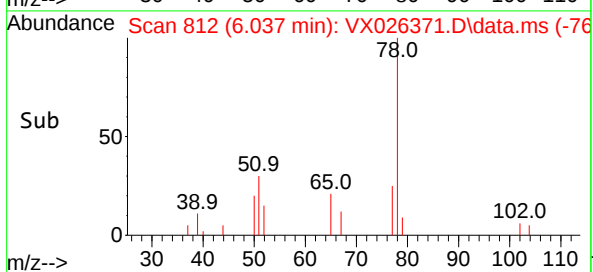






#50
Toluene-d8
Concen: 47.587 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 299182
Ion Ratio Lower Upper
98 100
100 66.5 52.6 78.8

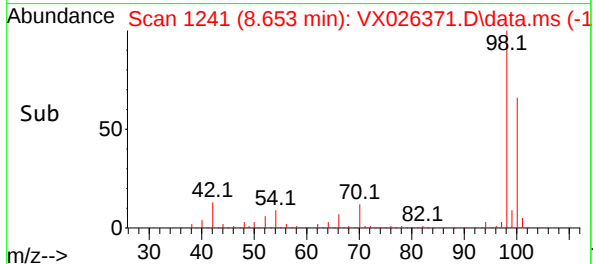

#52
Toluene
Concen: 2.683 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Tgt Ion: 92 Resp: 12850
Ion Ratio Lower Upper
92 100
91 167.3 136.0 204.0

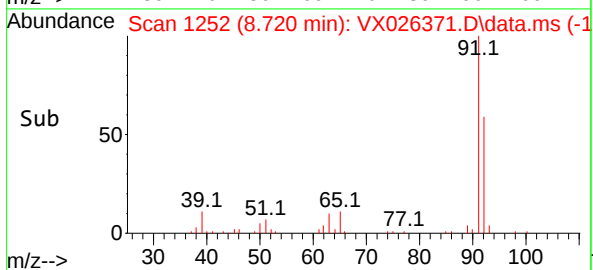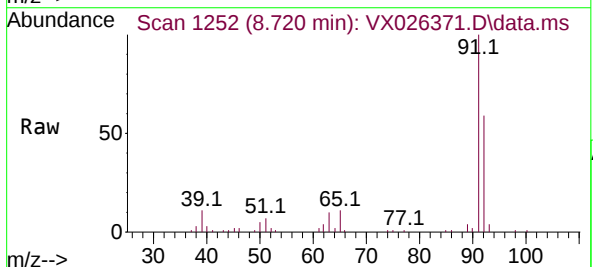



#53

t-1,3-Dichloropropene

Concen: 1.942 ug/l

RT: 8.720 min Scan# 1158

Delta R.T. -0.262 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 163

Ion Ratio Lower Upper

75 100

77 130.8 25.1 37.7#

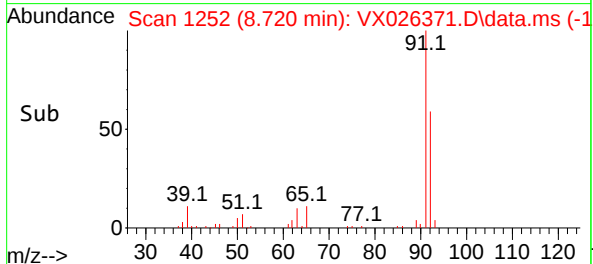

#58

2-Chloroethyl Vinyl ether

Concen: 9.902 ug/l

RT: 8.147 min Scan# 1158

Delta R.T. -0.097 min

Lab File: VX026371.D




Acq: 06 Jan 2022 14:21


Tgt Ion: 63 Resp: 124

Ion Ratio Lower Upper

63 100

106 0.0 24.4 36.6#









#62
4-Bromofluorobenzene
Concen: 47.855 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 107104
Ion Ratio Lower Upper
95 100
174 71.8 0.0 157.4
176 70.0 0.0 154.6

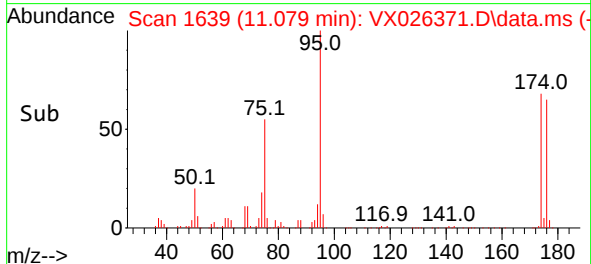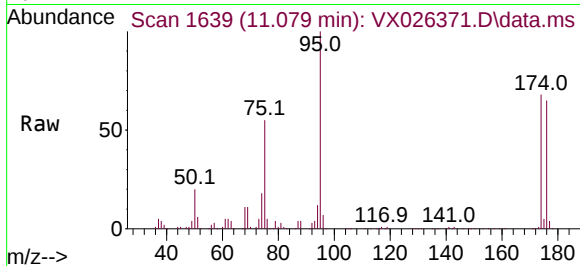

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Tgt Ion: 117 Resp: 218598
Ion Ratio Lower Upper
117 100
82 57.6 43.8 65.6
119 32.2 25.2 37.8

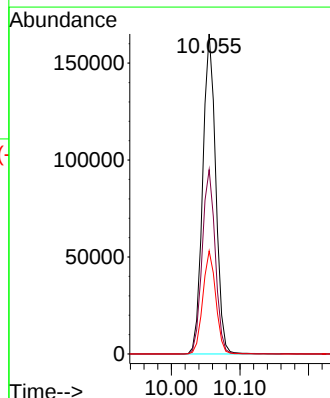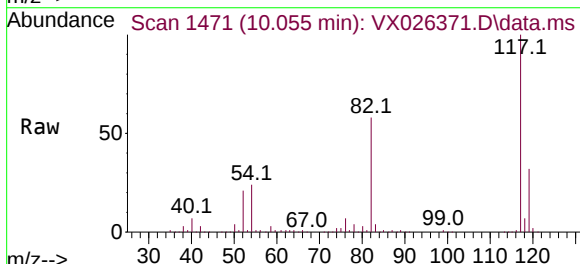



#67

Ethyl Benzene

Concen: 36.177 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 310634

Ion Ratio Lower Upper

91 100

106 30.8 25.7 38.5

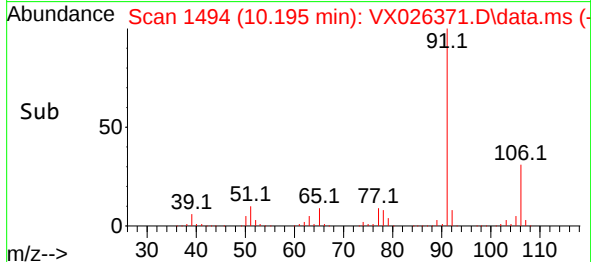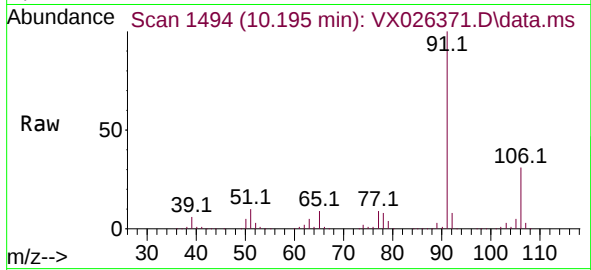

#68

m/p-Xylenes

Concen: 26.924 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. -0.000 min

Lab File: VX026371.D




Acq: 06 Jan 2022 14:21


Tgt Ion:106 Resp: 86319

Ion Ratio Lower Upper

106 100

91 212.8 158.6 238.0

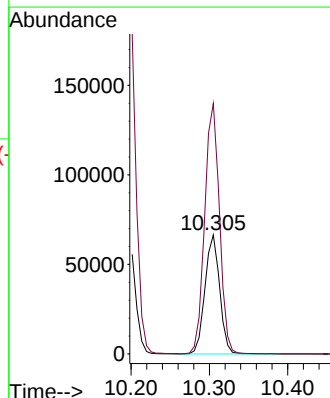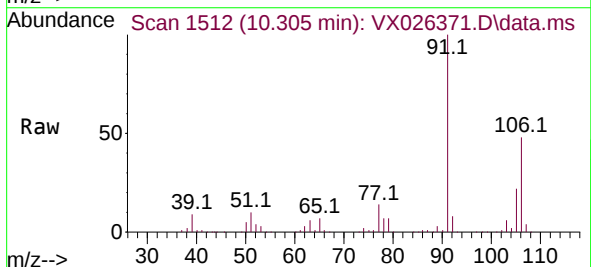



#69

o-Xylene

Concen: 16.214 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.006 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:106 Resp: 50860

Ion Ratio Lower Upper

106 100

91 223.5 105.5 316.4



#70

Styrene

Concen: 0.552 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.019 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21




Tgt Ion:104 Resp: 2841


Ion Ratio Lower Upper

104 100

78 293.4 39.8 59.6#

103 253.4 43.0 64.6#


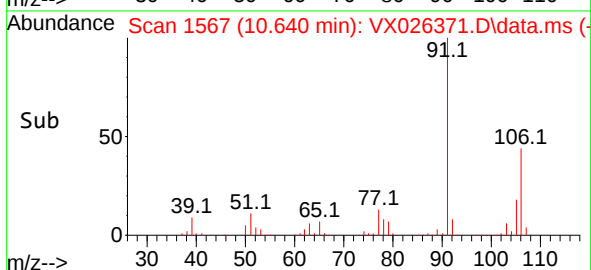






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 92684
Ion Ratio Lower Upper
152 100
115 62.7 41.3 123.9
150 157.7 0.0 351.8

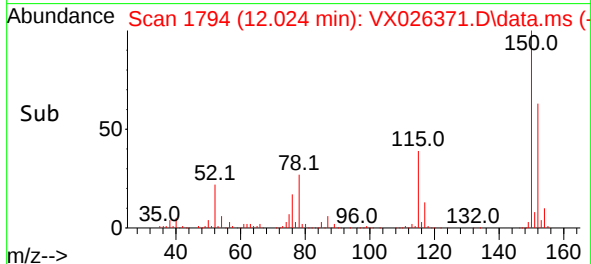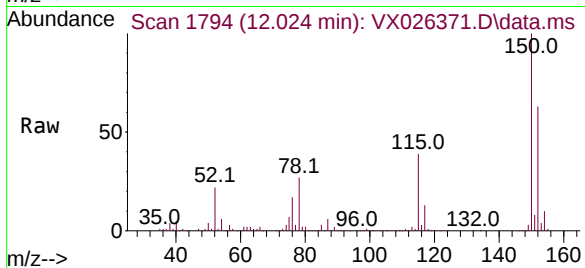

#73
Isopropylbenzene
Concen: 1.468 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Tgt Ion:105 Resp: 10578
Ion Ratio Lower Upper
105 100
120 24.8 13.6 40.7


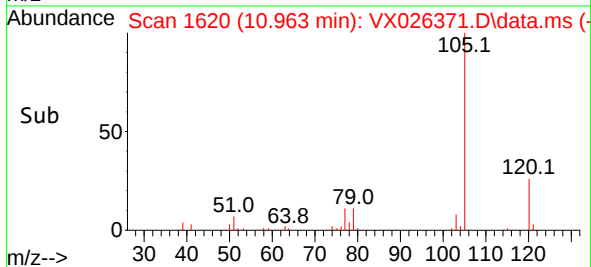

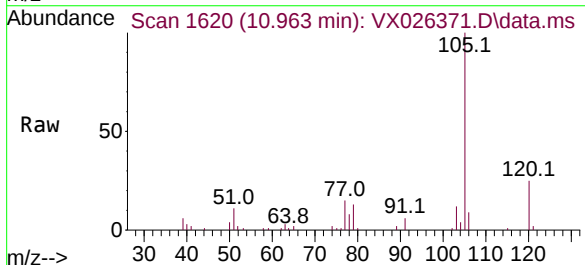




#76
1,2,3-Trichloropropane
Concen: 25.124 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 56207
Ion Ratio Lower Upper
75 100
77 1.0 19.0 57.0#

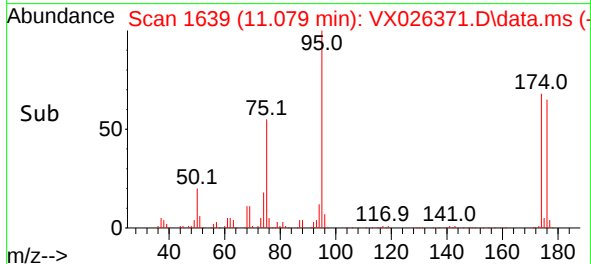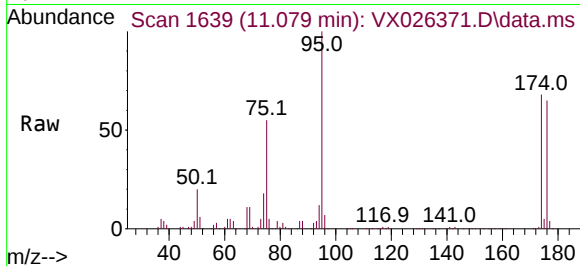

#78
n-propylbenzene
Concen: 1.521 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Tgt Ion: 91 Resp: 12600
Ion Ratio Lower Upper
91 100
120 22.5 12.0 36.1

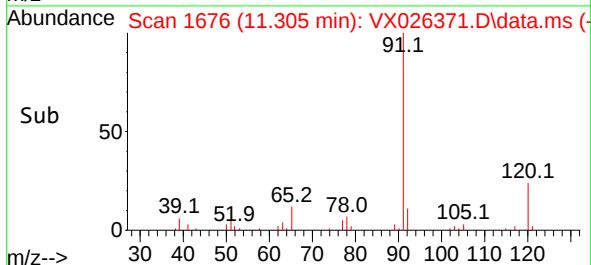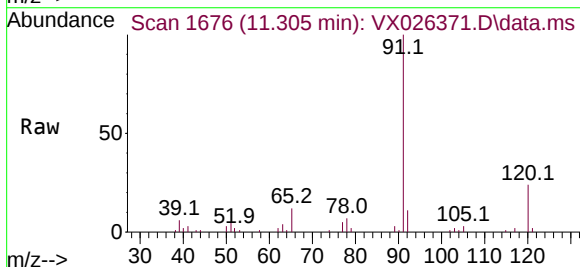



#79

2-Chlorotoluene

Concen: 0.783 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 3992

Ion Ratio Lower Upper

91 100

126 1.5 17.8 53.3#

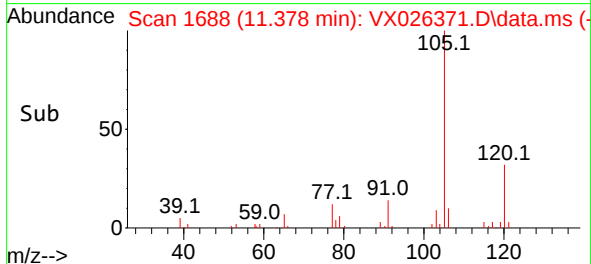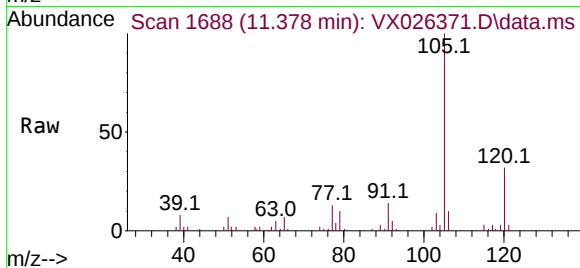

#80

1,3,5-Trimethylbenzene

Concen: 0.659 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX026371.D




Acq: 06 Jan 2022 14:21


Tgt Ion: 105 Resp: 3937

Ion Ratio Lower Upper

105 100

120 49.6 24.9 74.7


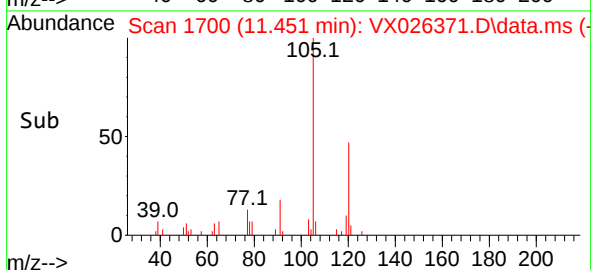

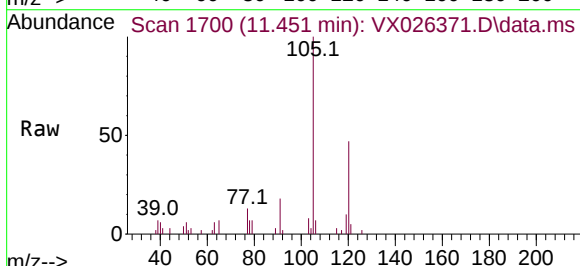




#81
trans-1,4-Dichloro-2-butene
Concen: 72.685 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 56207
Ion Ratio Lower Upper
75 100
53 0.0 79.5 119.3#
89 0.0 38.3 57.5#

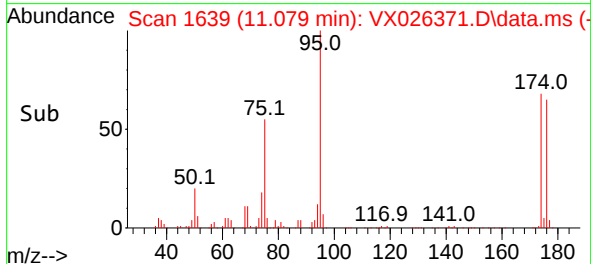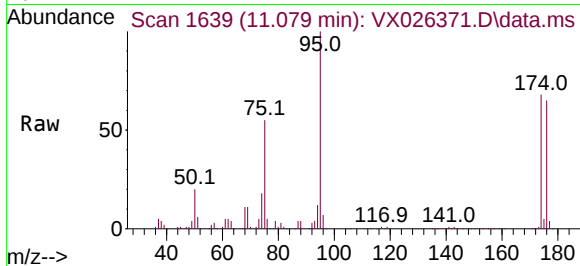

#83
tert-Butylbenzene
Concen: 3.193 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.031 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Tgt Ion: 119 Resp: 18529
Ion Ratio Lower Upper
119 100
91 95.6 28.7 86.1#
134 0.0 11.9 35.9#


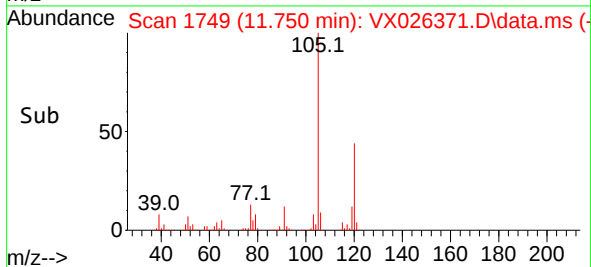

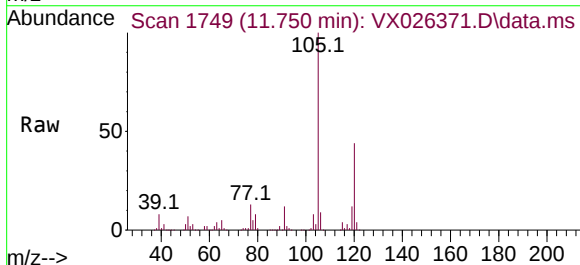




#84
1,2,4-Trimethylbenzene
Concen: 26.141 ug/l
RT: 11.750 min Scan# 1750
Delta R.T. -0.006 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 156166
Ion Ratio Lower Upper
105 100
120 43.9 22.9 68.7

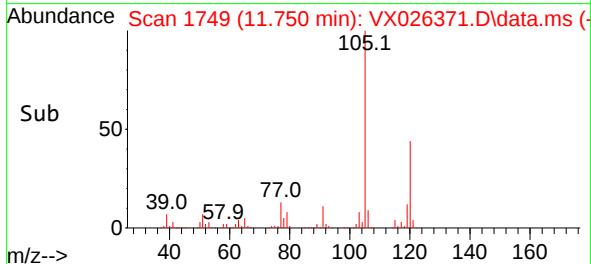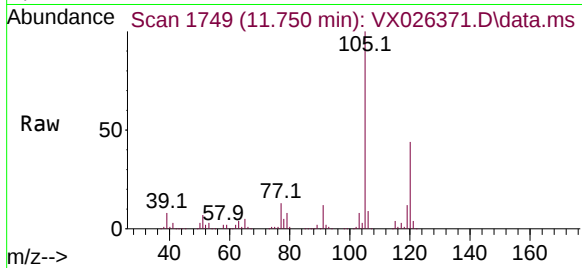

#85
sec-Butylbenzene
Concen: 21.565 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX026371.D
Acq: 06 Jan 2022 14:21

Tgt Ion:105 Resp: 156166
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#

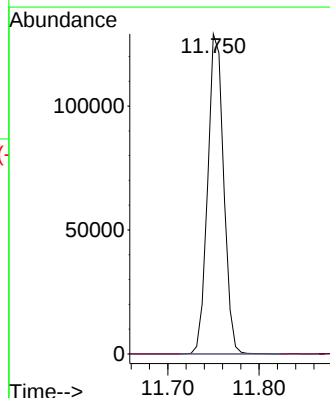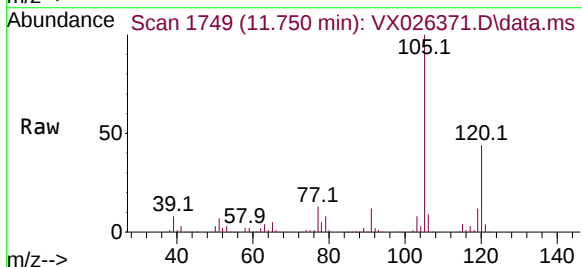



#90

Hexachloroethane

Concen: 4.264 ug/l

RT: 12.701 min Scan# 1905

Delta R.T. 0.159 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:117 Resp: 5142

Ion Ratio Lower Upper

117 100

201 0.0 35.4 106.3#

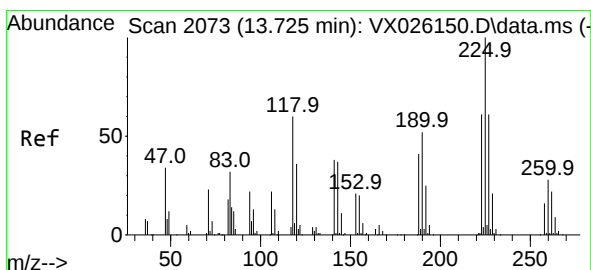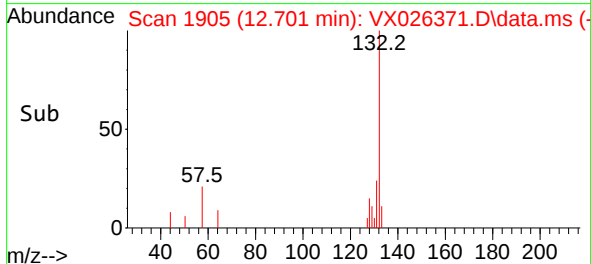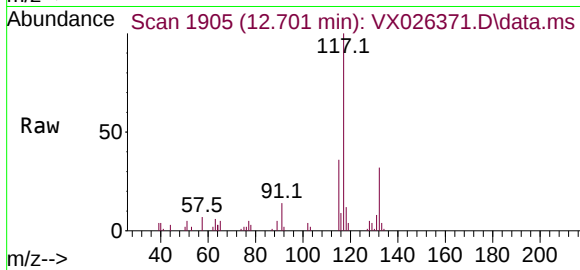

#94

Hexachlorobutadiene

Concen: 0.260 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. 0.000 min

Lab File: VX026371.D

Acq: 06 Jan 2022 14:21




Tgt Ion:225 Resp: 212


Ion Ratio Lower Upper

225 100

223 88.2 31.6 95.0

227 88.7 32.5 97.5

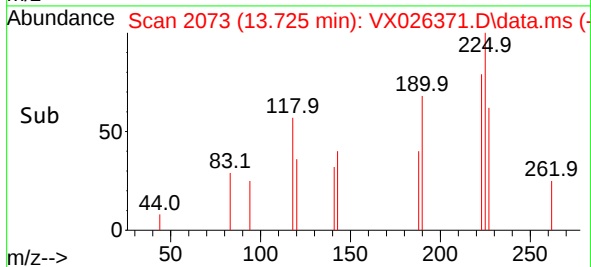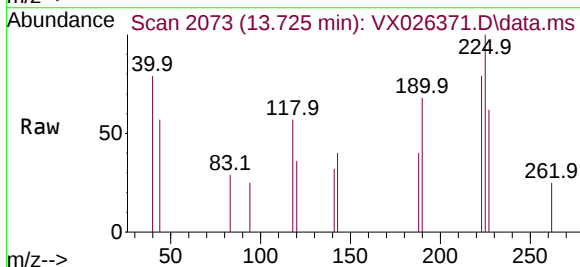



#95

Naphthalene

Concen: 5.866 ug/l

RT: 13.780 min Scan# 20

Delta R.T. -0.000 min


Lab File: VX026371.D

Acq: 06 Jan 2022 14:21

Instrument :

MSVOA_X

ClientSampleId :

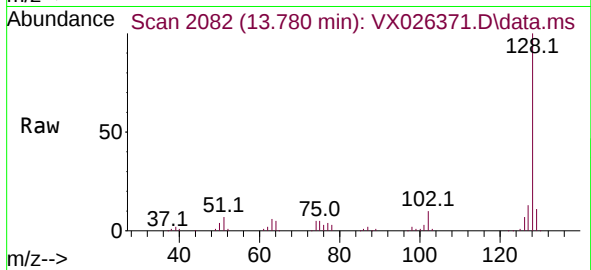

Tgt Ion:128 Resp: 42020

Ion Ratio Lower Upper

128 100

127 12.9 10.3 15.5

129 10.6 8.8 13.2

