

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
 Data File : VX026376.D
 Acq On : 06 Jan 2022 16:17
 Operator : JC/MD
 Sample : N1020-01DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 07 04:15:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	156528	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	260576	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	224090	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	96574	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	111086	49.055	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	98.120%		
35) Dibromofluoromethane	5.391	113	83271	49.154	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.300%		
50) Toluene-d8	8.653	98	300192	47.639	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	95.280%		
62) 4-Bromofluorobenzene	11.079	95	111312	49.622	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	99.240%		
Target Compounds						Qvalue
5) Bromomethane	1.624	94	303	0.244	ug/l #	64
11) Tert butyl alcohol	2.947	59	534	1.181	ug/l #	73
13) Acrolein	2.221	56	2999	18.543	ug/l #	1
14) Allyl chloride	2.752	41	4377	1.278	ug/l #	14
16) Acetone	2.386	43	1379	1.124	ug/l	95
20) Methylene Chloride	2.794	84	523	Below Cal	#	84
29) Tetrahydrofuran	5.196	42	350	0.325	ug/l #	32
31) Cyclohexane	5.483	56	4844	1.502	ug/l	97
36) 1,1-Dichloropropene	5.562	75	13129	4.805	ug/l #	49
37) Ethyl Acetate	4.727	43	708	0.223	ug/l #	69
38) Carbon Tetrachloride	5.556	117	16731	5.505	ug/l #	16
39) Methylcyclohexane	7.385	83	1007	0.327	ug/l	87
40) Benzene	6.044	78	744891	95.520	ug/l	99
42) 1,2-Dichloroethane	6.044	62	7435	2.356	ug/l #	74
52) Toluene	8.720	92	99237	20.671	ug/l	99
53) t-1,3-Dichloropropene	8.720	75	1269	2.274	ug/l #	1
59) 2-Hexanone	9.378	43	982	0.403	ug/l #	25
67) Ethyl Benzene	10.195	91	43264	4.915	ug/l	98
68) m/p-Xylenes	10.305	106	79199	24.098	ug/l	91
69) o-Xylene	10.640	106	34940	10.866	ug/l	91
70) Styrene	10.640	104	1926	0.365	ug/l #	1
76) 1,2,3-Trichloropropane	11.079	75	57379	24.615	ug/l #	39
78) n-propylbenzene	11.305	91	1759	0.204	ug/l	96
79) 2-Chlorotoluene	11.378	91	3048	0.574	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.451	105	9366	1.503	ug/l	93
81) trans-1,4-Dichloro-2-b...	11.079	75	57379	71.211	ug/l #	10
83) tert-Butylbenzene	11.750	119	3238	0.536	ug/l #	52
84) 1,2,4-Trimethylbenzene	11.750	105	26149	4.201	ug/l	98
85) sec-Butylbenzene	11.750	105	26149	3.465	ug/l #	56
90) Hexachloroethane	12.646	117	331	0.263	ug/l #	14
95) Naphthalene	13.780	128	4904	0.657	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
Data File : VX026376.D
Acq On : 06 Jan 2022 16:17
Operator : JC/MD
Sample : N1020-01DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 07 04:15:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration

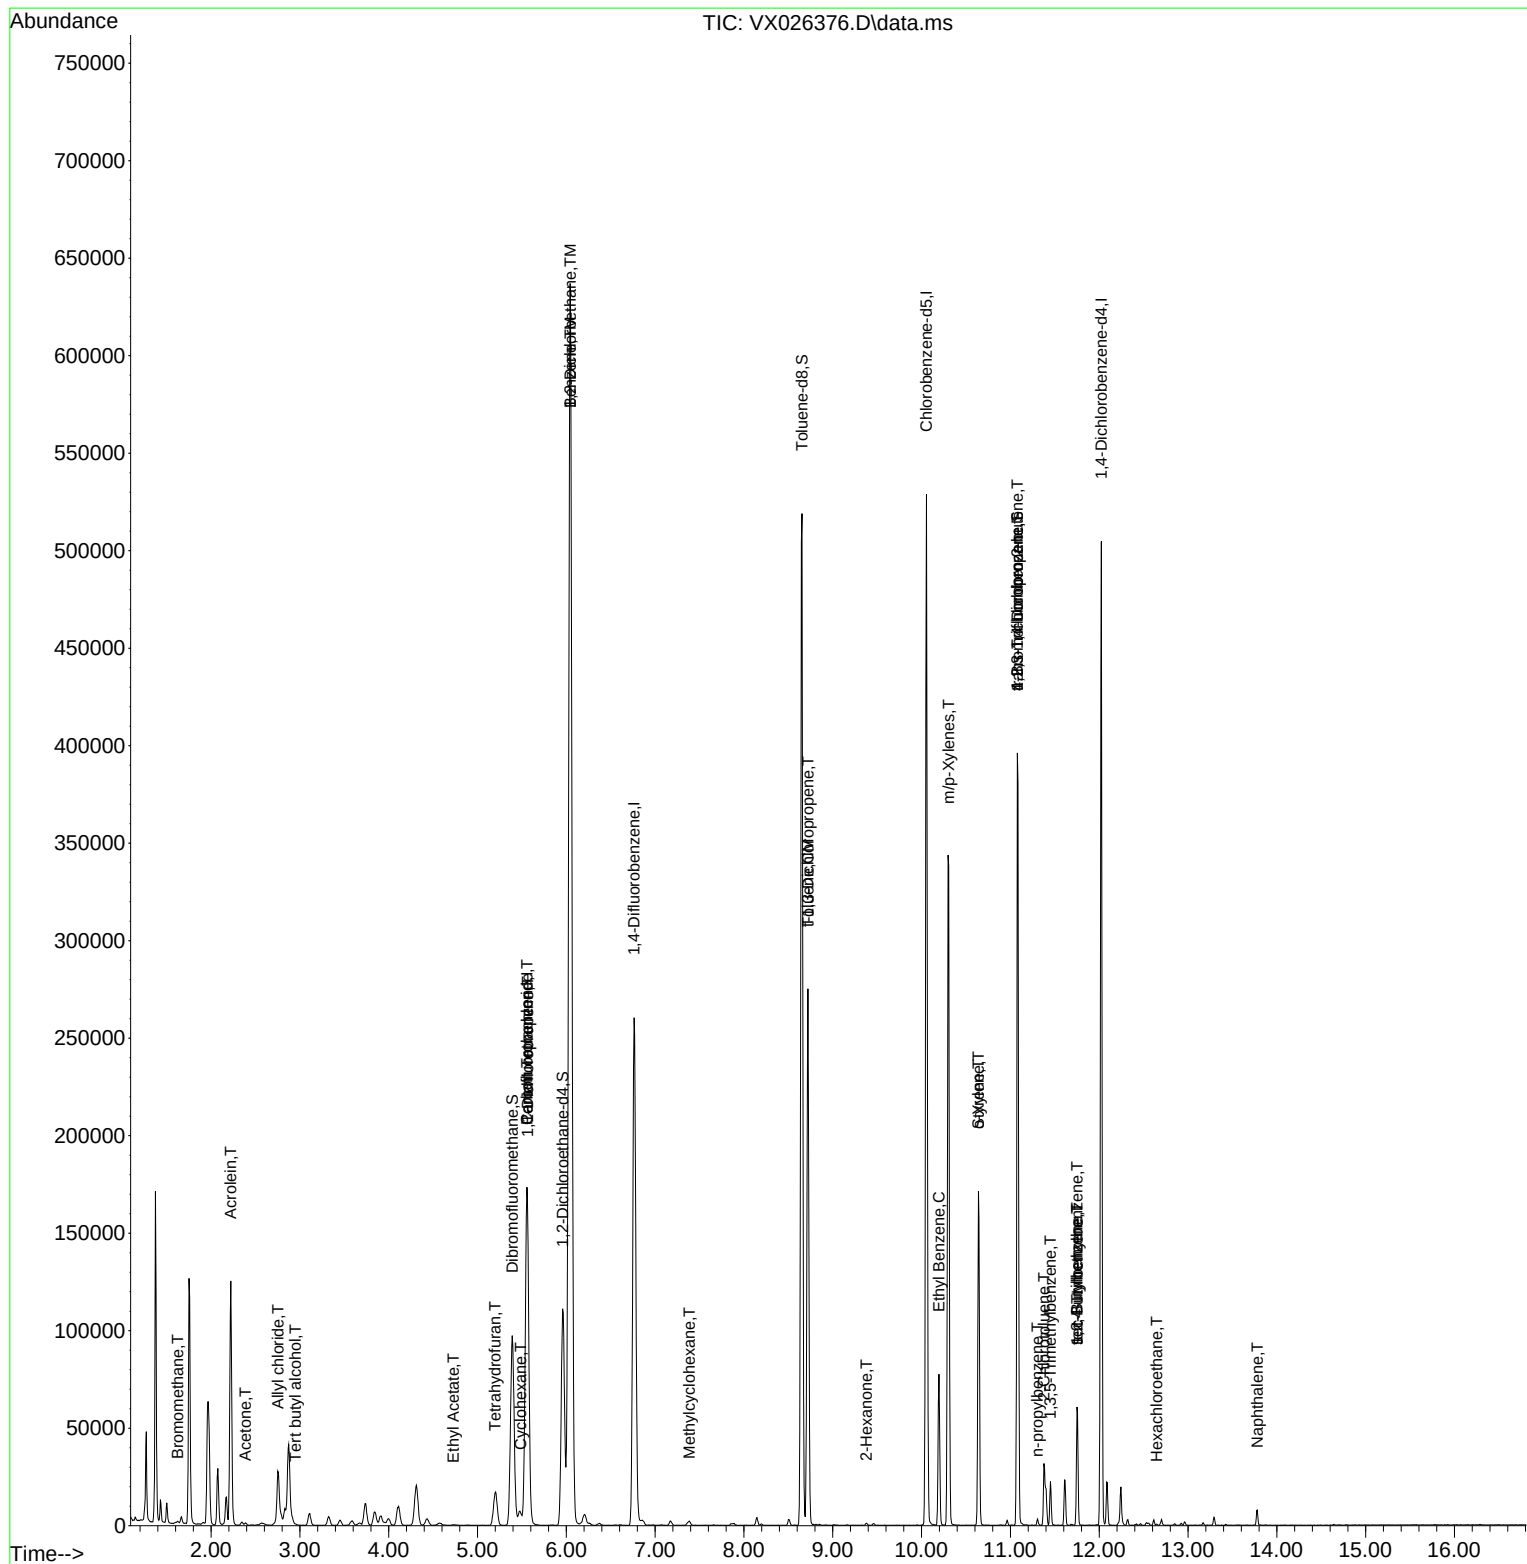






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 156528
Ion Ratio Lower Upper
168 100
99 64.6 45.8 68.8



#5
Bromomethane
Concen: 0.244 ug/l
RT: 1.624 min Scan# 88
Delta R.T. 0.013 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17


Tgt Ion: 94 Resp: 303
Ion Ratio Lower Upper
94 100
96 59.4 75.0 112.4#

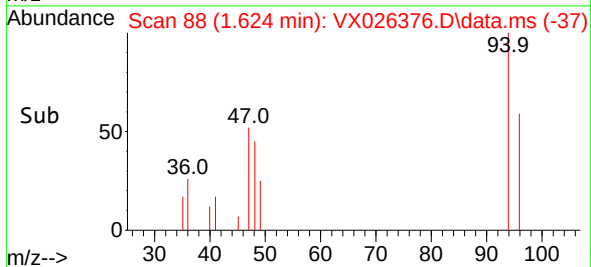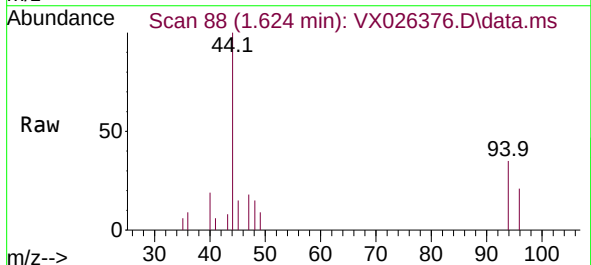



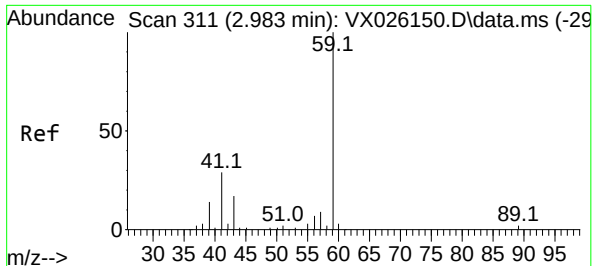


#11
Tert butyl alcohol
Concen: 1.181 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.036 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 59 Resp: 534
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

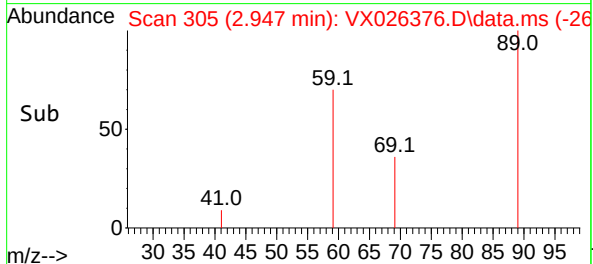

#13
Acrolein
Concen: 18.543 ug/l
RT: 2.221 min Scan# 186
Delta R.T. -0.018 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17


Tgt Ion: 56 Resp: 2999
Ion Ratio Lower Upper
56 100
55 2182.7 57.4 86.2#

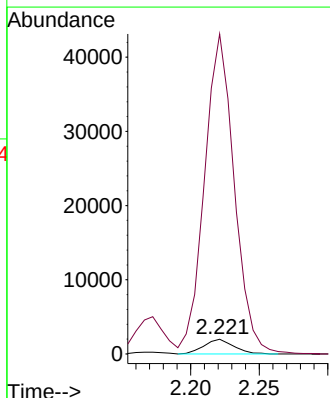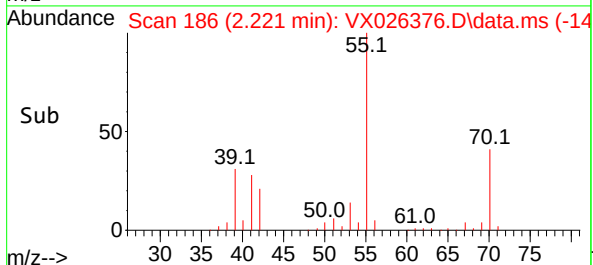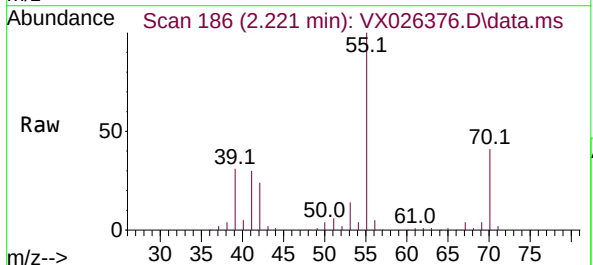



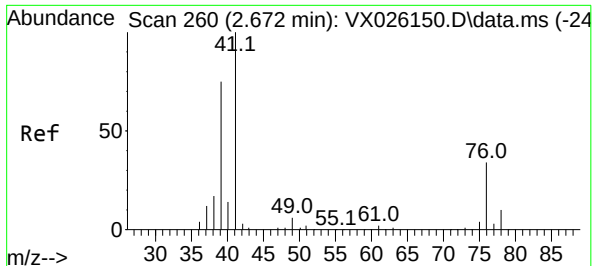


#14
 Allyl chloride
 Concen: 1.278 ug/l
 RT: 2.752 min Scan# 213
 Delta R.T. 0.079 min
 Lab File: VX026376.D
 Acq: 06 Jan 2022 16:17

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion: 41 Resp: 4377
 Ion Ratio Lower Upper
 41 100
 39 149.7 55.4 83.0#
 76 0.0 27.6 41.4#

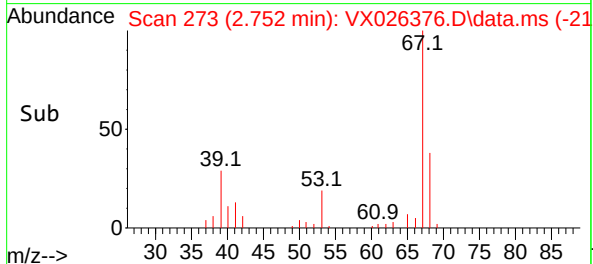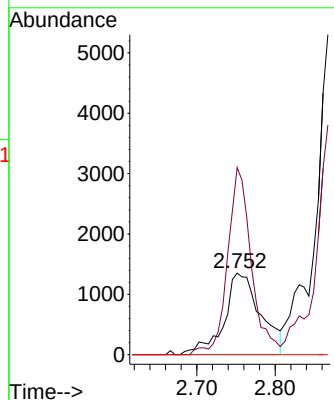

#16
 Acetone
 Concen: 1.124 ug/l
 RT: 2.386 min Scan# 213
 Delta R.T. -0.000 min
 Lab File: VX026376.D
 Acq: 06 Jan 2022 16:17


Tgt Ion: 43 Resp: 1379
 Ion Ratio Lower Upper
 43 100
 58 33.8 24.8 37.2

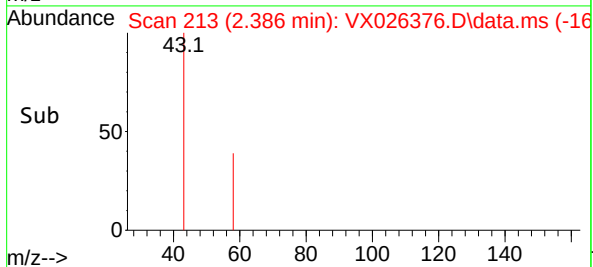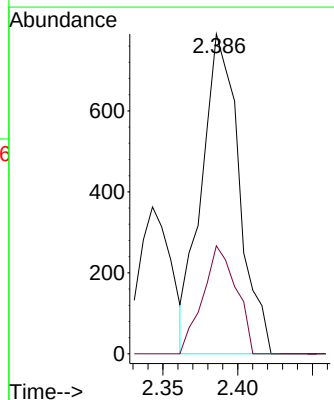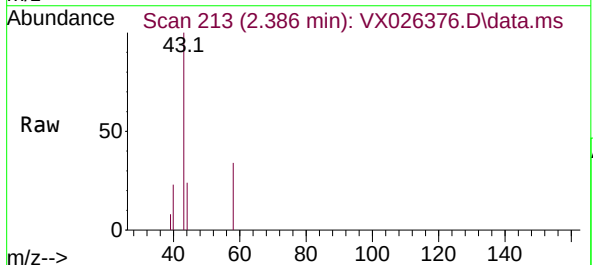






#20
Methylene Chloride
Concen: Below Cal
RT: 2.794 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:	84	Resp:	523
Ion	Ratio	Lower	Upper
84	100		
49	108.9	97.1	145.7
51	46.4	29.3	43.9#
86	82.7	50.8	76.2#



#29
Tetrahydrofuran
Concen: 0.325 ug/l
RT: 5.196 min Scan# 674
Delta R.T. 0.183 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17


Tgt Ion:	42	Resp:	350
Ion	Ratio	Lower	Upper
42	100		
72	0.0	37.0	55.6#
71	0.0	34.1	51.1#








#31
Cyclohexane
Concen: 1.502 ug/l
RT: 5.483 min Scan# 719
Delta R.T. 0.006 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Instrument :
MSVOA_X
ClientSampleId :

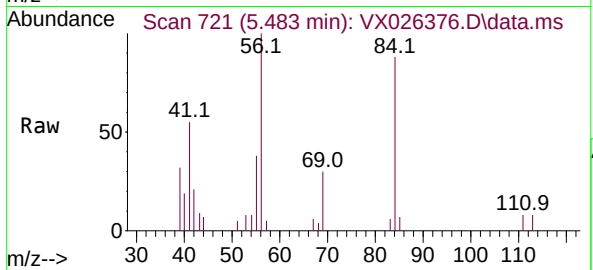

Tgt Ion: 56 Resp: 4844




Ion	Ratio	Lower	Upper
56	100		
69	30.1	23.9	35.9
84	87.6	73.2	109.8

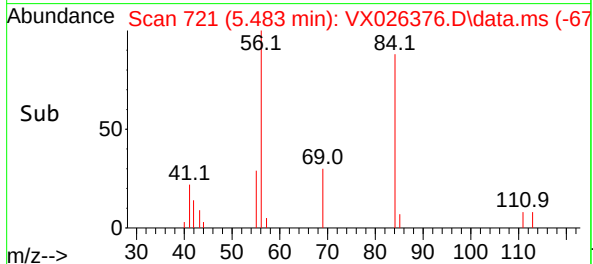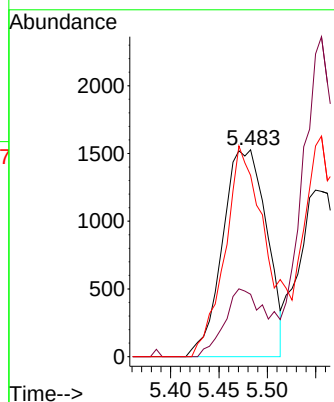


#33
1,2-Dichloroethane-d4
Concen: 49.055 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Tgt Ion: 65 Resp: 111086

Ion	Ratio	Lower	Upper
65	100		
67	50.2	0.0	103.4


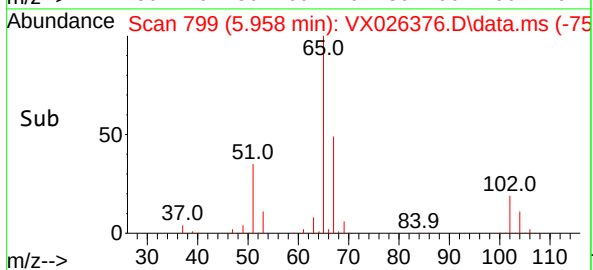
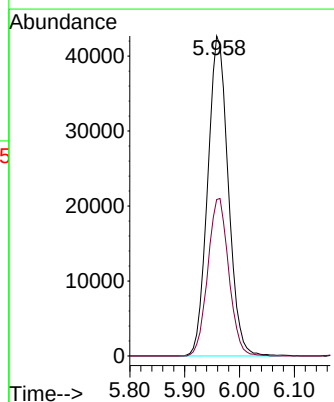
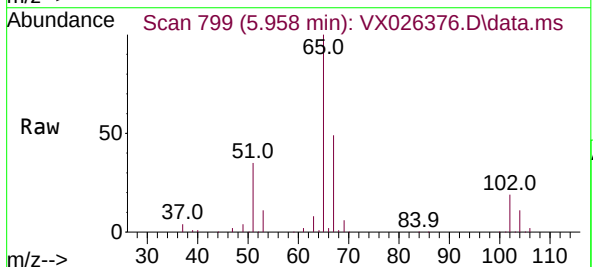




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 260576
Ion Ratio Lower Upper
114 100
63 22.5 0.0 40.0
88 16.8 0.0 30.6



#35
Dibromofluoromethane
Concen: 49.154 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Tgt Ion:113 Resp: 83271
Ion Ratio Lower Upper
113 100
111 102.5 81.8 122.8
192 19.2 15.0 22.4





#36

1,1-Dichloropropene

Concen: 4.805 ug/l

RT: 5.562 min Scan# 71

Delta R.T. -0.140 min


Lab File: VX026376.D

Acq: 06 Jan 2022 16:17

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 75 Resp: 13129

Ion Ratio Lower Upper

75 100

110 8.8 18.2 54.6#

77 0.0 24.7 37.1#

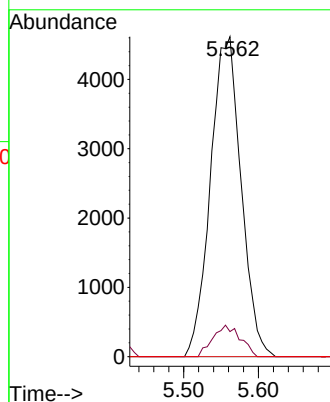

#37

Ethyl Acetate

Concen: 0.223 ug/l

RT: 4.727 min Scan# 597

Delta R.T. 0.006 min

Lab File: VX026376.D

Acq: 06 Jan 2022 16:17




Tgt Ion: 43 Resp: 708


Ion Ratio Lower Upper

43 100

61 0.0 10.7 16.1#


70 0.0 8.5 12.7#





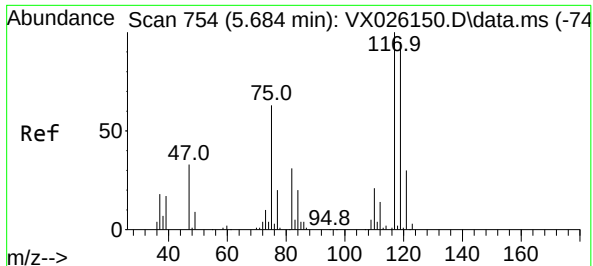


#38
Carbon Tetrachloride
Concen: 5.505 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 16731
Ion Ratio Lower Upper
117 100
119 5.5 77.2 115.8#
121 0.0 23.8 35.8#

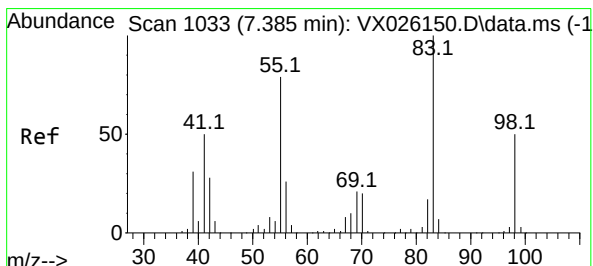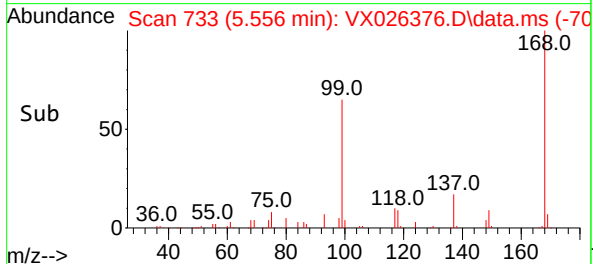

#39
Methylcyclohexane
Concen: 0.327 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Tgt Ion: 83 Resp: 1007
Ion Ratio Lower Upper
83 100
55 85.7 57.8 86.8
98 44.7 40.5 60.7


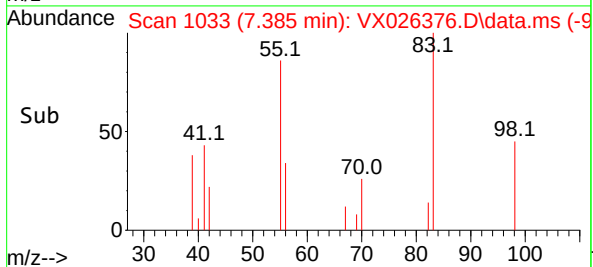

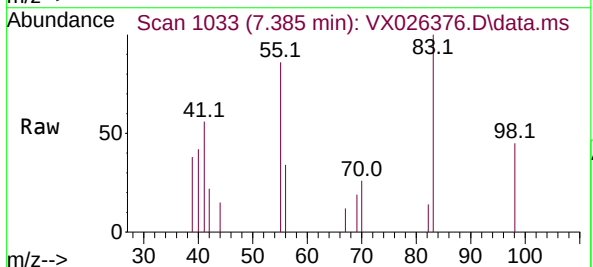




#40
Benzene
Concen: 95.520 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 78 Resp: 744891
Ion Ratio Lower Upper
78 100
77 23.8 18.6 27.8

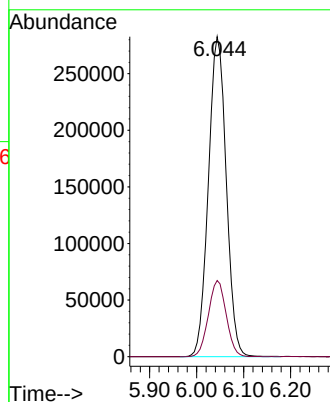

#42
1,2-Dichloroethane
Concen: 2.356 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.048 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Tgt Ion: 62 Resp: 7435
Ion Ratio Lower Upper
62 100
98 0.0 0.0 18.8









#50
Toluene-d8
Concen: 47.639 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 300192
Ion Ratio Lower Upper
98 100
100 66.4 52.6 78.8

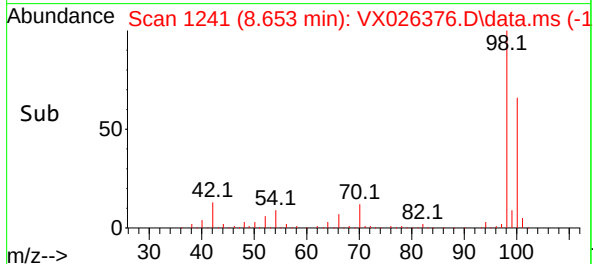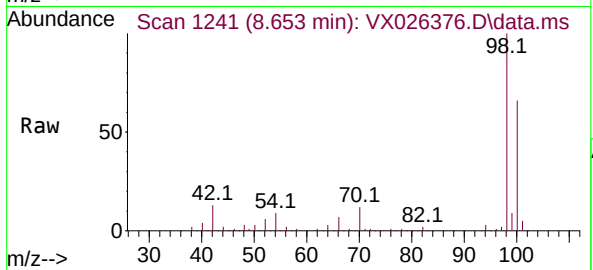

#52
Toluene
Concen: 20.671 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Tgt Ion: 92 Resp: 99237
Ion Ratio Lower Upper
92 100
91 171.3 136.0 204.0

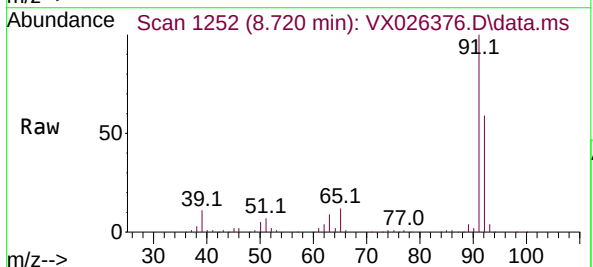



#53

t-1,3-Dichloropropene

Concen: 2.274 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX026376.D

Acq: 06 Jan 2022 16:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 1269

Ion Ratio Lower Upper

75 100

77 145.7 25.1 37.7#

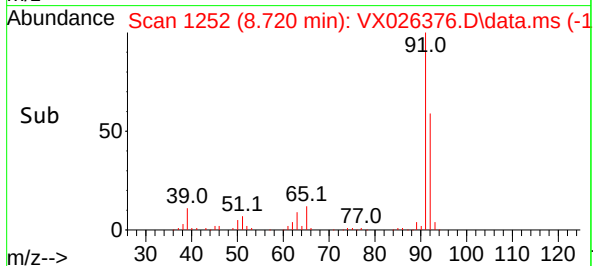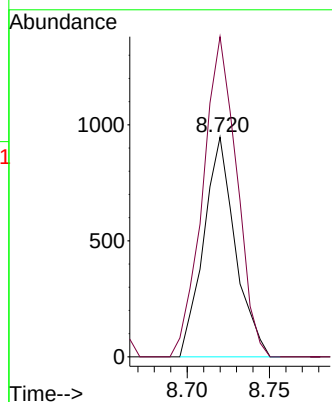

#59

2-Hexanone

Concen: 0.403 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.055 min

Lab File: VX026376.D




Acq: 06 Jan 2022 16:17


Tgt Ion: 43 Resp: 982

Ion Ratio Lower Upper

43 100

58 0.0 26.9 80.6#


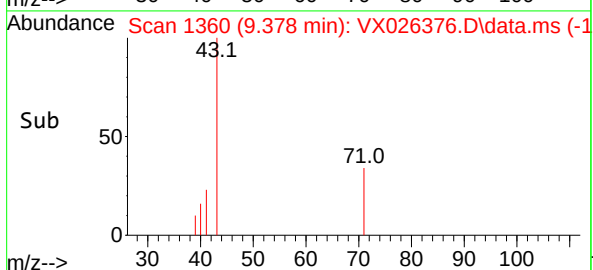
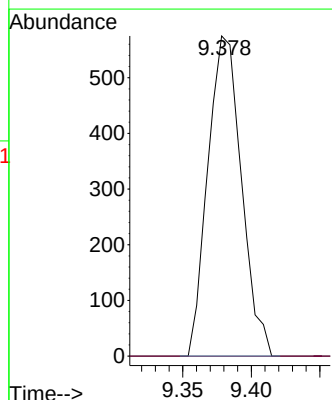
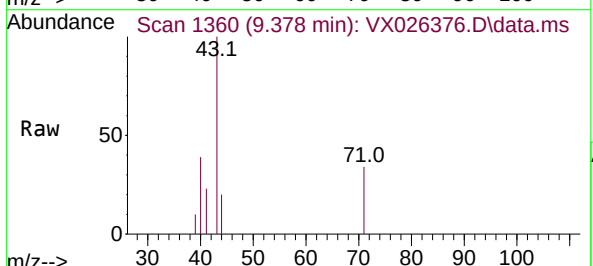




#62
4-Bromofluorobenzene
Concen: 49.622 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 111312
Ion Ratio Lower Upper
95 100
174 70.7 0.0 157.4
176 68.3 0.0 154.6

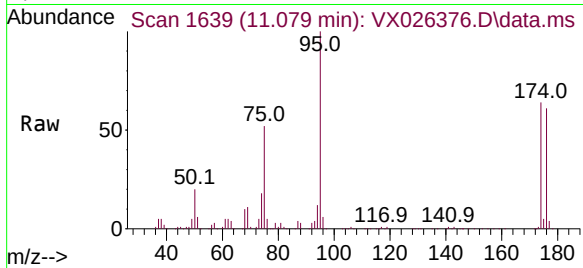

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17

Tgt Ion: 117 Resp: 224090
Ion Ratio Lower Upper
117 100
82 58.7 43.8 65.6
119 31.8 25.2 37.8

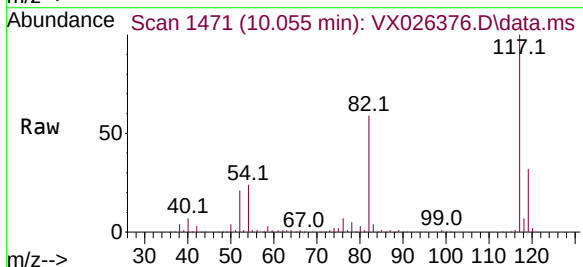



#67

Ethyl Benzene

Concen: 4.915 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX026376.D

Acq: 06 Jan 2022 16:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 43264

Ion Ratio Lower Upper

91 100

106 30.7 25.7 38.5

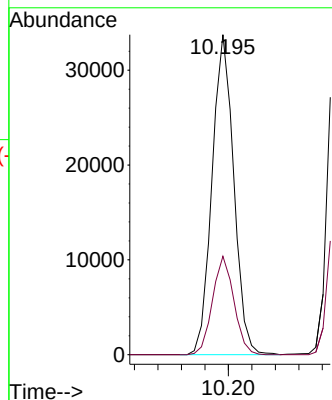

#68

m/p-Xylenes

Concen: 24.098 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.000 min

Lab File: VX026376.D




Acq: 06 Jan 2022 16:17


Tgt Ion:106 Resp: 79199

Ion Ratio Lower Upper

106 100

91 211.3 158.6 238.0


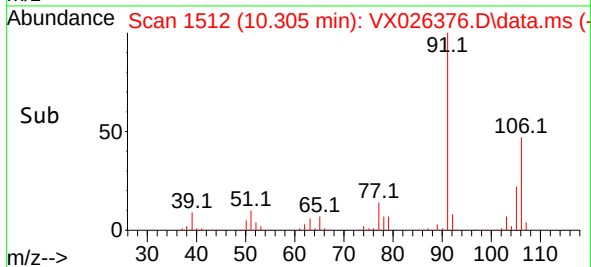
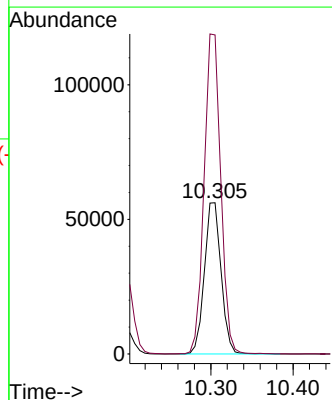
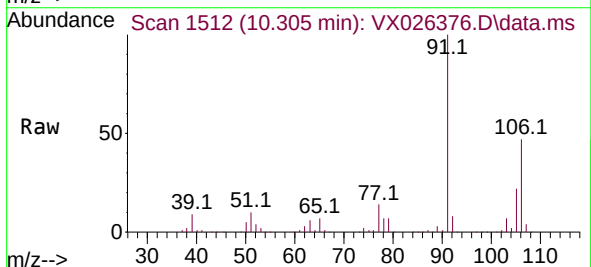




#69
o-Xylene
Concen: 10.866 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 34940
Ion Ratio Lower Upper
106 100
91 225.2 105.5 316.4

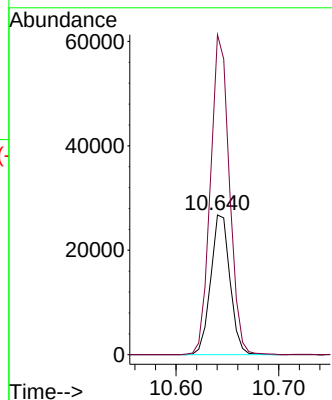

#70
Styrene
Concen: 0.365 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.019 min
Lab File: VX026376.D
Acq: 06 Jan 2022 16:17


Tgt Ion:104 Resp: 1926
Ion Ratio Lower Upper
104 100
78 292.9 39.8 59.6#
103 254.0 43.0 64.6#

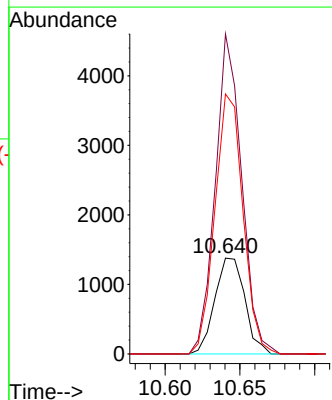






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VX026376.D
 Acq: 06 Jan 2022 16:17

Instrument :
 MSVOA_X
 ClientSampleId :



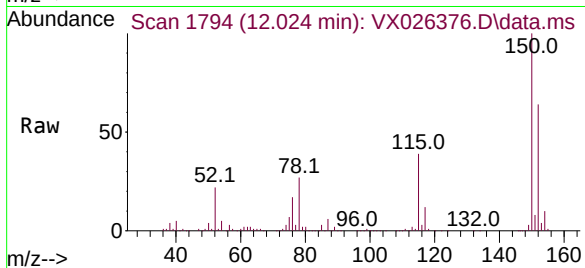



Tgt Ion:152 Resp: 96574
 Ion Ratio Lower Upper
 152 100
 115 62.6 41.3 123.9
 150 157.2 0.0 351.8

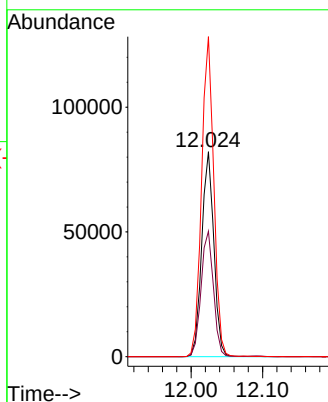

#76
 1,2,3-Trichloropropane
 Concen: 24.615 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.165 min
 Lab File: VX026376.D
 Acq: 06 Jan 2022 16:17

Tgt Ion: 75 Resp: 57379
 Ion Ratio Lower Upper
 75 100
 77 1.1 19.0 57.0#

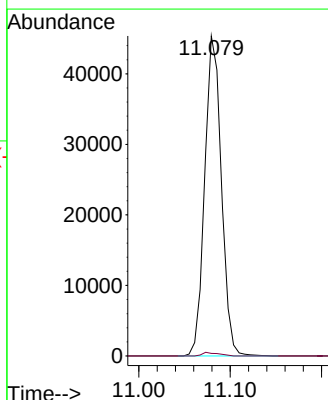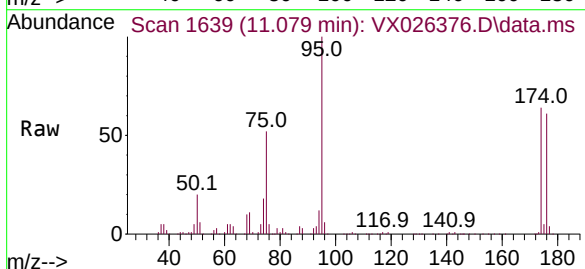



#78

n-propylbenzene

Concen: 0.204 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX026376.D

Acq: 06 Jan 2022 16:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 1759

Ion Ratio Lower Upper

91 100

120 22.3 12.0 36.1

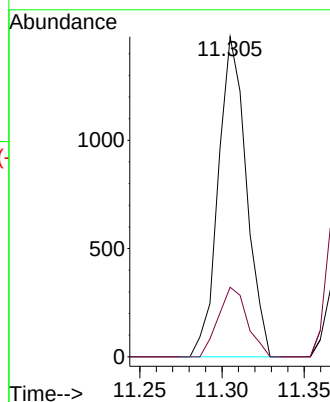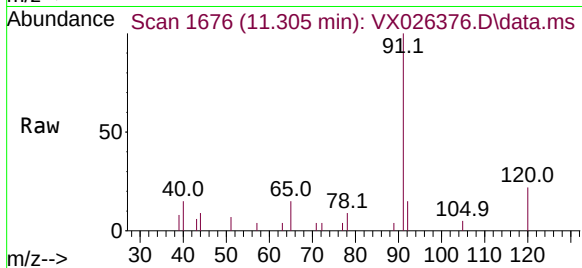

#79

2-Chlorotoluene

Concen: 0.574 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.012 min

Lab File: VX026376.D




Acq: 06 Jan 2022 16:17


Tgt Ion: 91 Resp: 3048

Ion Ratio Lower Upper

91 100

126 0.0 17.8 53.3#

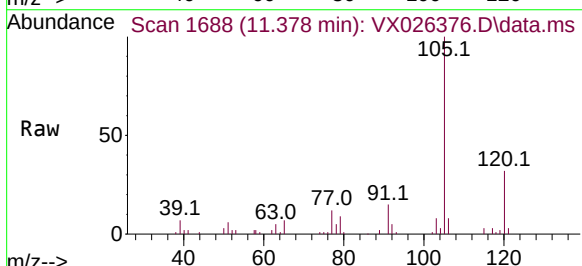



#80

1,3,5-Trimethylbenzene

Concen: 1.503 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX026376.D

Acq: 06 Jan 2022 16:17

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 9366

Ion Ratio Lower Upper

105 100

120 45.2 24.9 74.7

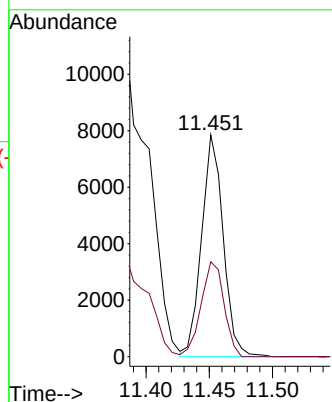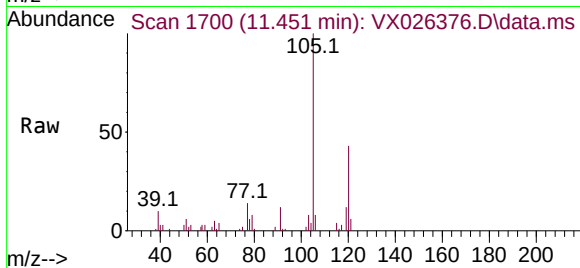

#81

trans-1,4-Dichloro-2-butene

Concen: 71.211 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX026376.D

Acq: 06 Jan 2022 16:17




Tgt Ion: 75 Resp: 57379


Ion Ratio Lower Upper

75 100

53 0.0 79.5 119.3#

89 0.0 38.3 57.5#



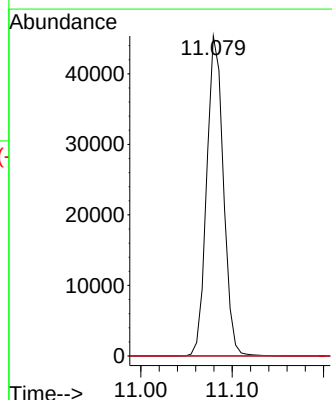
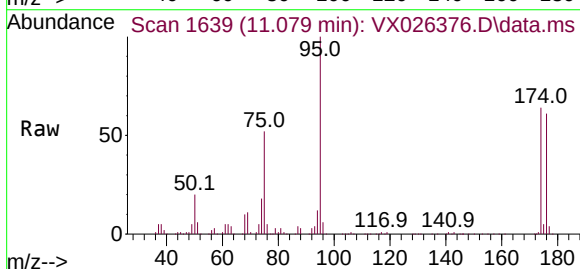




#83
 tert-Butylbenzene
 Concen: 0.536 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. 0.031 min
 Lab File: VX026376.D
 Acq: 06 Jan 2022 16:17




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:119 Resp: 3238
 Ion Ratio Lower Upper
 119 100
 91 92.4 28.7 86.1#
 134 0.0 11.9 35.9#

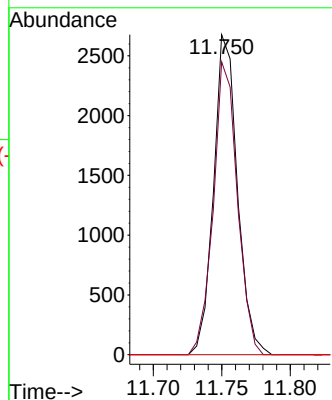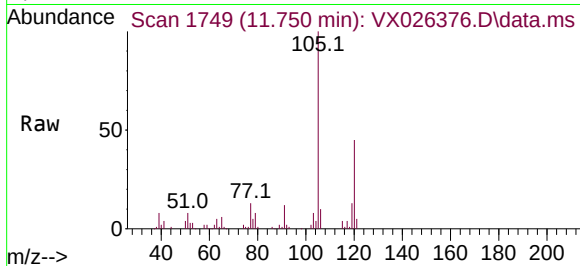

#84
 1,2,4-Trimethylbenzene
 Concen: 4.201 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.006 min
 Lab File: VX026376.D
 Acq: 06 Jan 2022 16:17

Tgt Ion:105 Resp: 26149
 Ion Ratio Lower Upper
 105 100
 120 44.3 22.9 68.7


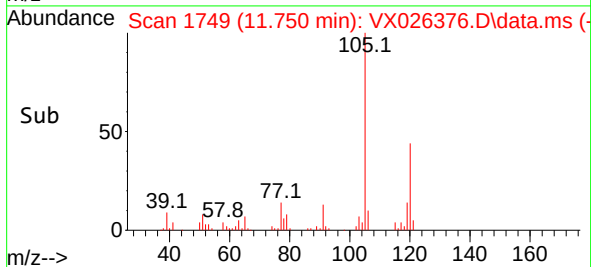
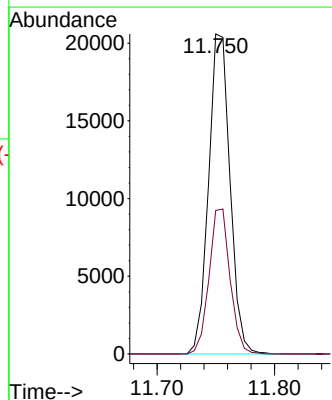
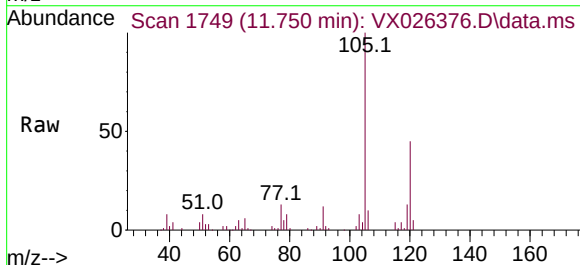




#85
 sec-Butylbenzene
 Concen: 3.465 ug/l
 RT: 11.750 min Scan# 11
 Delta R.T. -0.140 min
 Lab File: VX026376.D
 Acq: 06 Jan 2022 16:17




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 26149
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.1#



#90
 Hexachloroethane
 Concen: 0.263 ug/l
 RT: 12.646 min Scan# 1896
 Delta R.T. 0.104 min
 Lab File: VX026376.D
 Acq: 06 Jan 2022 16:17


Tgt Ion:117 Resp: 331
 Ion Ratio Lower Upper
 117 100
 201 0.0 35.4 106.3#

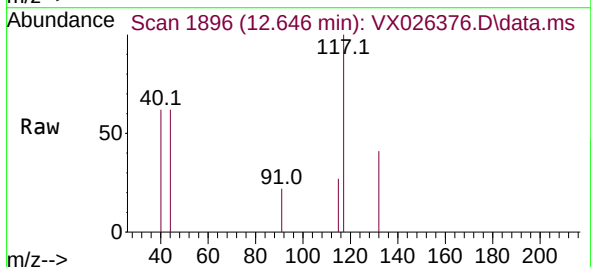



#95
 Naphthalene
 Concen: 0.657 ug/l
 RT: 13.780 min Scan# 2082
 Delta R.T. 0.000 min
 Lab File: VX026376.D
 Acq: 06 Jan 2022 16:17

Instrument :
 MSVOA_X
 ClientSampleId :



Tgt Ion:128 Resp: 4904
 Ion Ratio Lower Upper
 128 100
 127 13.1 10.3 15.5
 129 9.7 8.8 13.2

