

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
 Data File : VX026377.D
 Acq On : 06 Jan 2022 16:40
 Operator : JC/MD
 Sample : N1020-10DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :


Quant Time: Jan 07 04:15:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 30 08:02:21 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	147637	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	247969	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	210269	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	93594	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	107481	50.322	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 100.640%			
35) Dibromofluoromethane	5.391	113	79512	49.321	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 98.640%			
50) Toluene-d8	8.653	98	285707	47.646	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 95.300%			
62) 4-Bromofluorobenzene	11.079	95	105196	49.280	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 98.560%			
Target Compounds						Qvalue
11) Tert butyl alcohol	2.947	59	299	0.701	ug/l #	73
13) Acrolein	2.221	56	1554	10.187	ug/l #	1
14) Allyl chloride	2.758	41	3762	1.164	ug/l #	3
15) Acrylonitrile	2.873	53	1021	0.967	ug/l #	38
16) Acetone	2.392	43	856	0.740	ug/l	95
20) Methylene Chloride	2.794	84	650	Below Cal	#	81
29) Tetrahydrofuran	5.196	42	253	0.249	ug/l #	32
31) Cyclohexane	5.489	56	3415	1.123	ug/l #	89
36) 1,1-Dichloropropene	5.550	75	12653	4.866	ug/l #	49
38) Carbon Tetrachloride	5.556	117	15982	5.526	ug/l #	14
39) Methylcyclohexane	7.391	83	593	0.202	ug/l	96
40) Benzene	6.044	78	699502	94.260	ug/l	98
42) 1,2-Dichloroethane	6.038	62	6758	2.250	ug/l #	74
52) Toluene	8.720	92	16234	3.553	ug/l	100
53) t-1,3-Dichloropropene	8.726	75	199	1.956	ug/l #	1
55) 1,1,2-Trichloroethane	9.019	97	408	0.217	ug/l #	15
67) Ethyl Benzene	10.195	91	274623	33.250	ug/l	97
68) m/p-Xylenes	10.299	106	341381	110.700	ug/l	93
69) o-Xylene	10.640	106	40186	13.318	ug/l	91
70) Styrene	10.640	104	1904	0.385	ug/l #	1
73) Isopropylbenzene	10.964	105	6110	0.840	ug/l	95
76) 1,2,3-Trichloropropane	11.079	75	55661	24.638	ug/l #	39
78) n-propylbenzene	11.305	91	12098	1.446	ug/l	95
79) 2-Chlorotoluene	11.378	91	9562	1.857	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.451	105	19811	3.281	ug/l	95
81) trans-1,4-Dichloro-2-b...	11.079	75	55661	71.279	ug/l #	10
82) 4-Chlorotoluene	11.451	91	2272	0.391	ug/l #	44
83) tert-Butylbenzene	11.756	119	9707	1.656	ug/l #	49
84) 1,2,4-Trimethylbenzene	11.756	105	82675	13.705	ug/l	97
85) sec-Butylbenzene	11.756	105	82675	11.305	ug/l #	56
90) Hexachloroethane	12.701	117	2311	1.898	ug/l #	14
95) Naphthalene	13.780	128	29536	4.083	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 07 04:15:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 30 08:02:21 2021
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 147637
Ion Ratio Lower Upper
168 100
99 63.6 45.8 68.8



#11
Tert butyl alcohol
Concen: 0.701 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.036 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 59 Resp: 299
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

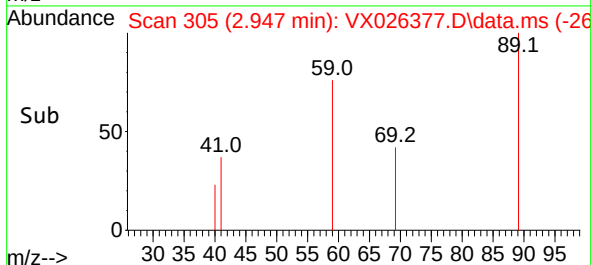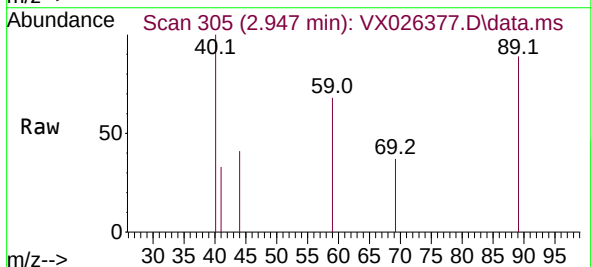



#13

Acrolein

Concen: 10.187 ug/l

RT: 2.221 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX026377.D

Acq: 06 Jan 2022 16:40

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 56 Resp: 1554

Ion Ratio Lower Upper

56 100

55 2183.3 57.4 86.2#

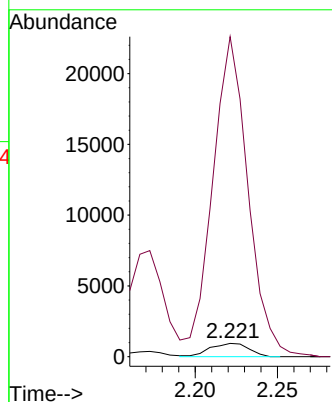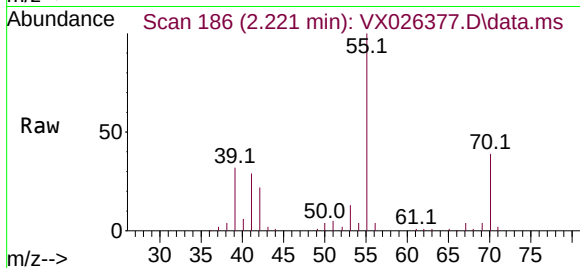

#14

Allyl chloride

Concen: 1.164 ug/l

RT: 2.758 min Scan# 274

Delta R.T. 0.086 min

Lab File: VX026377.D

Acq: 06 Jan 2022 16:40




Tgt Ion: 41 Resp: 3762


Ion Ratio Lower Upper

41 100

39 163.3 55.4 83.0#


76 0.0 27.6 41.4#

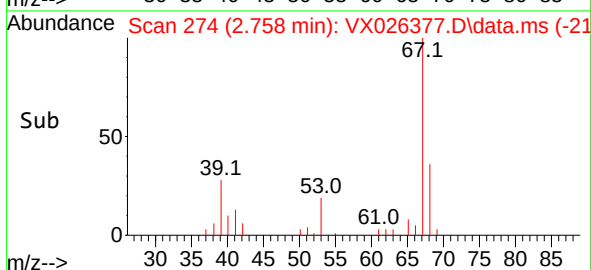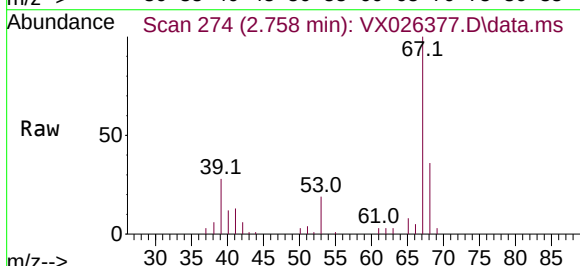






#15
Acrylonitrile
Concen: 0.967 ug/l
RT: 2.873 min Scan# 24
Delta R.T. -0.196 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 53 Resp: 1021
Ion Ratio Lower Upper
53 100
52 9.6 66.2 99.2#
51 47.0 29.4 44.0#



#16
Acetone
Concen: 0.740 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 43 Resp: 856
Ion Ratio Lower Upper
43 100
58 28.5 24.8 37.2

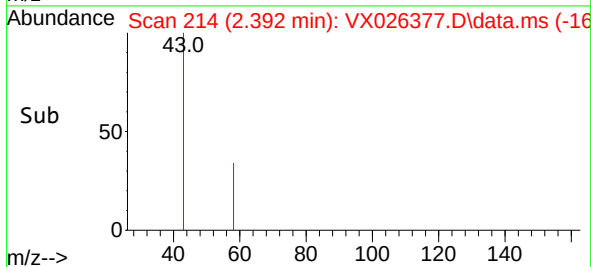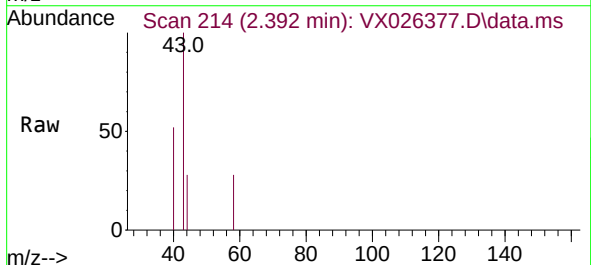



#20

Methylene Chloride

Concen: Below Cal

RT: 2.794 min Scan# 21

Delta R.T. 0.000 min


Lab File: VX026377.D

Acq: 06 Jan 2022 16:40

Instrument :

MSVOA_X

ClientSampleId :

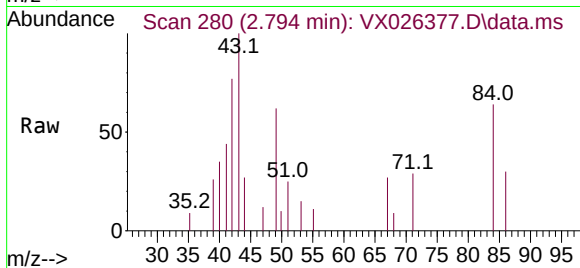

Tgt Ion: 84 Resp: 650




Ion Ratio Lower Upper

84 100

49 96.2 97.1 145.7#

51 39.2 29.3 43.9

86 46.2 50.8 76.2#



#29

Tetrahydrofuran

Concen: 0.249 ug/l

RT: 5.196 min Scan# 674

Delta R.T. 0.183 min

Lab File: VX026377.D

Acq: 06 Jan 2022 16:40




Tgt Ion: 42 Resp: 253


Ion Ratio Lower Upper

42 100

72 0.0 37.0 55.6#


71 0.0 34.1 51.1#

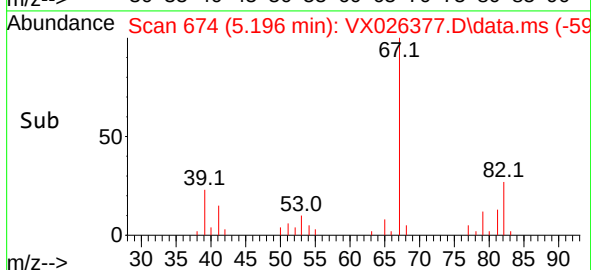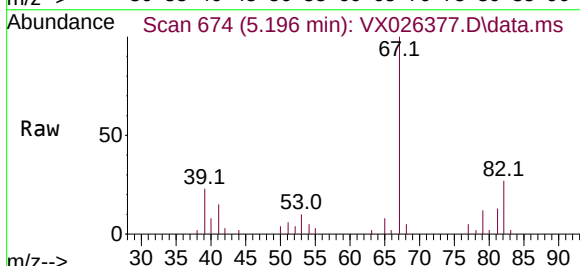



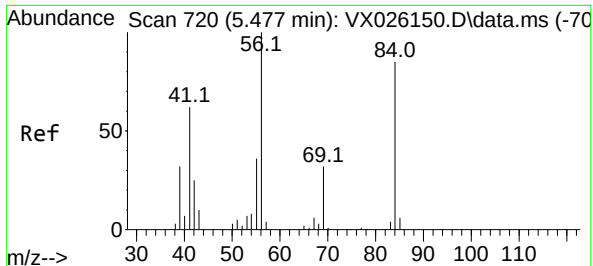


#31
Cyclohexane
Concen: 1.123 ug/l
RT: 5.489 min Scan# 719
Delta R.T. 0.012 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Instrument :
MSVOA_X
ClientSampleId :



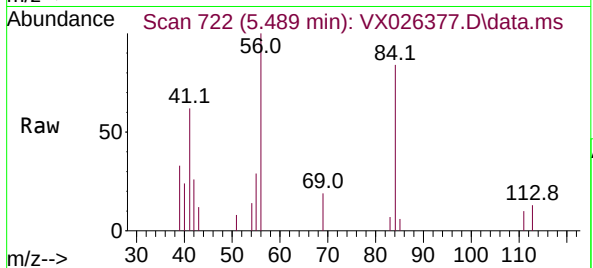



Tgt Ion: 56 Resp: 3415
Ion Ratio Lower Upper
56 100
69 19.0 23.9 35.9#
84 83.8 73.2 109.8

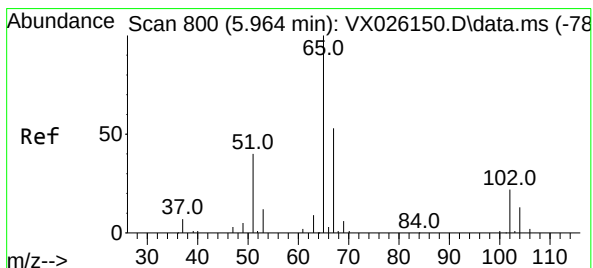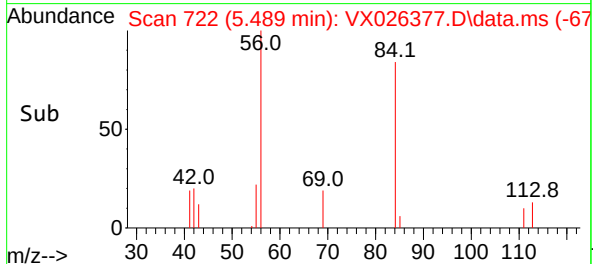

#33
1,2-Dichloroethane-d4
Concen: 50.322 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 65 Resp: 107481
Ion Ratio Lower Upper
65 100
67 49.9 0.0 103.4


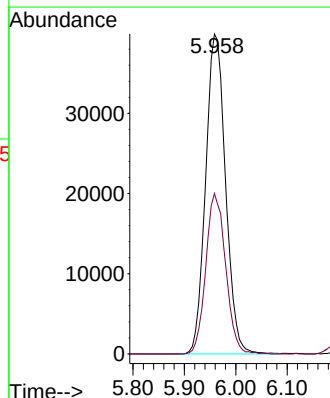
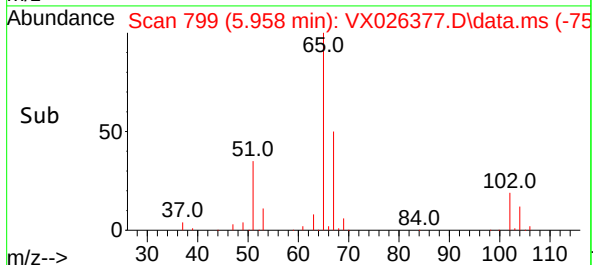
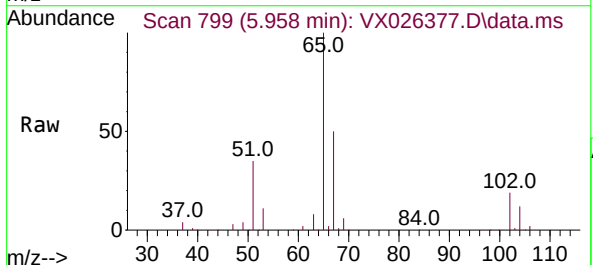




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 247969
Ion Ratio Lower Upper
114 100
63 22.2 0.0 40.0
88 16.7 0.0 30.6

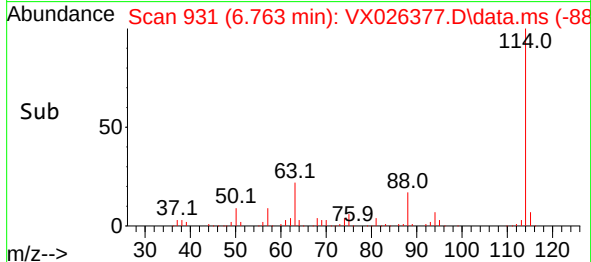

#35
Dibromofluoromethane
Concen: 49.321 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40


Tgt Ion:113 Resp: 79512
Ion Ratio Lower Upper
113 100
111 102.1 81.8 122.8
192 18.7 15.0 22.4

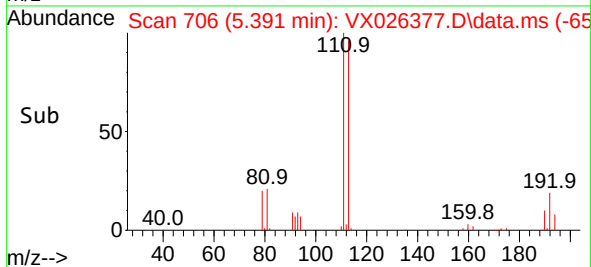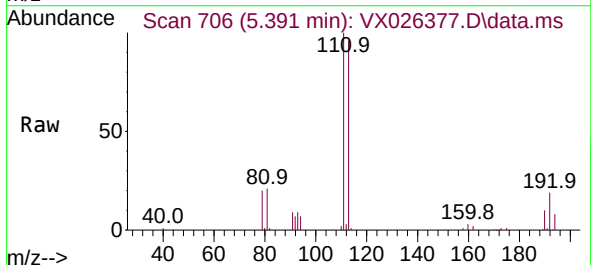






#36
1,1-Dichloropropene
Concen: 4.866 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.152 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 75 Resp: 12653
Ion Ratio Lower Upper
75 100
110 8.6 18.2 54.6#
77 0.0 24.7 37.1#



#38
Carbon Tetrachloride
Concen: 5.526 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 117 Resp: 15982
Ion Ratio Lower Upper
117 100
119 3.5 77.2 115.8#
121 0.0 23.8 35.8#


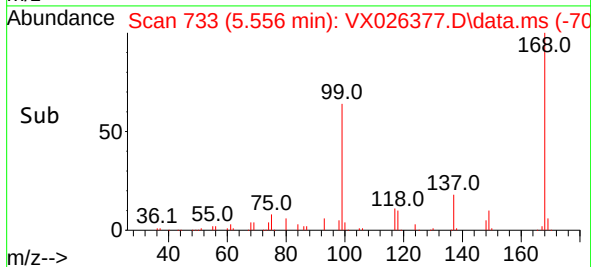

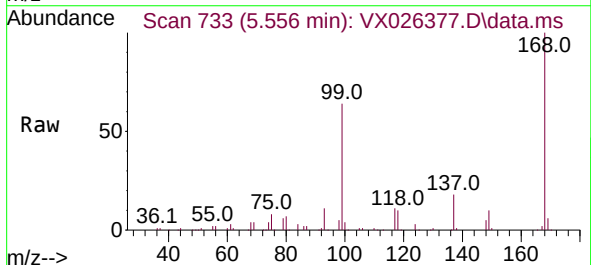


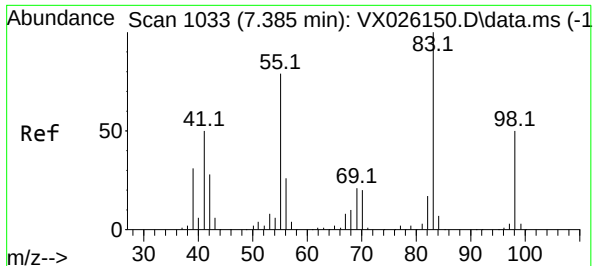

#39
Methylcyclohexane
Concen: 0.202 ug/l
RT: 7.391 min Scan# 1034
Delta R.T. 0.006 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 83 Resp: 593
Ion Ratio Lower Upper
83 100
55 69.4 57.8 86.8
98 48.0 40.5 60.7

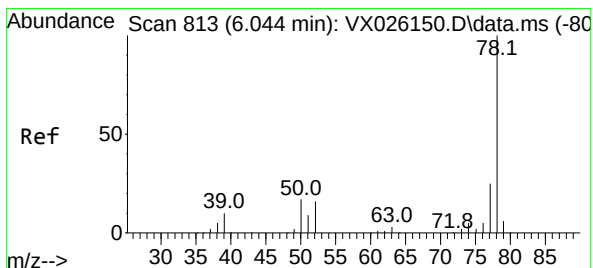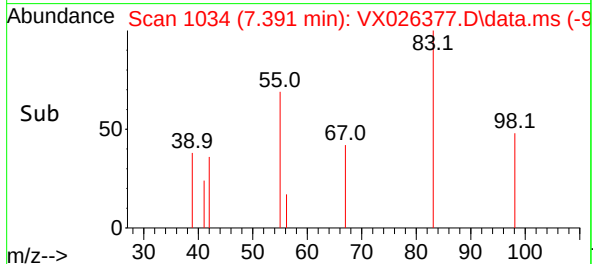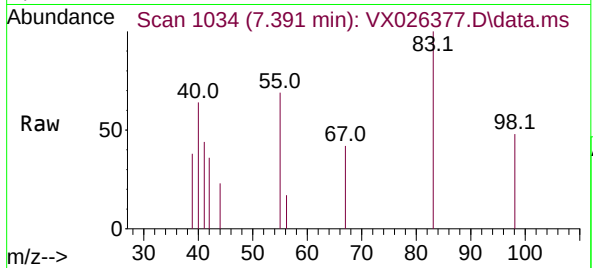

#40
Benzene
Concen: 94.260 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 78 Resp: 699502
Ion Ratio Lower Upper
78 100
77 24.2 18.6 27.8


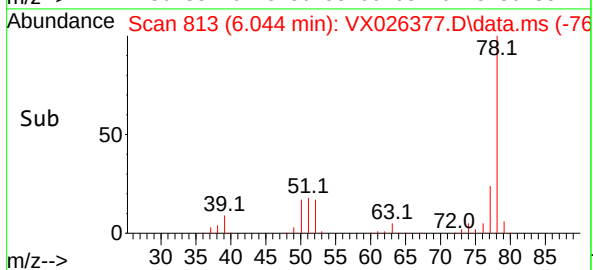

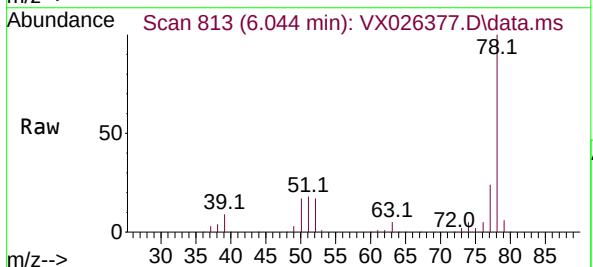




#42
1,2-Dichloroethane
Concen: 2.250 ug/l
RT: 6.038 min Scan# 81
Delta R.T. -0.054 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 62 Resp: 6758
Ion Ratio Lower Upper
62 100
98 0.0 0.0 18.8

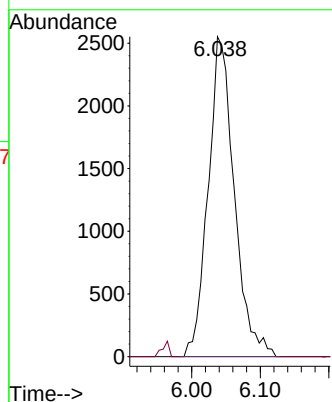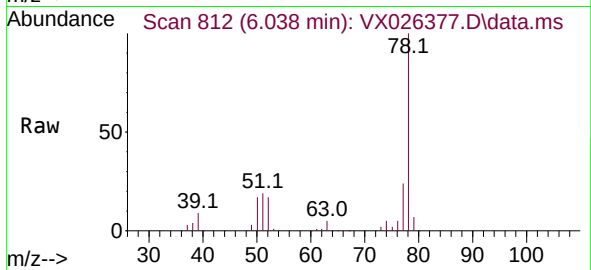

#50
Toluene-d8
Concen: 47.646 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 98 Resp: 285707
Ion Ratio Lower Upper
98 100
100 66.1 52.6 78.8

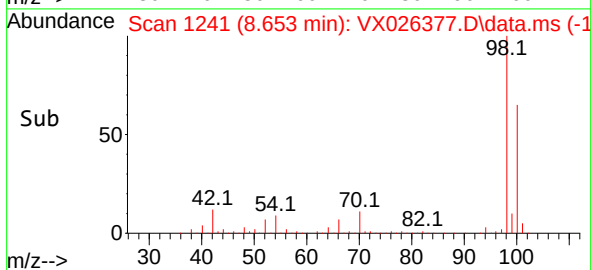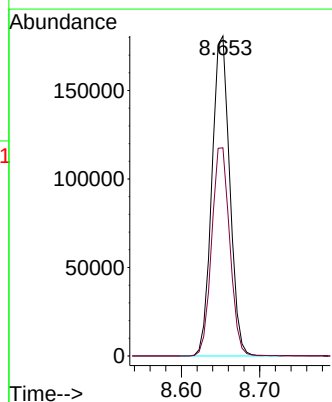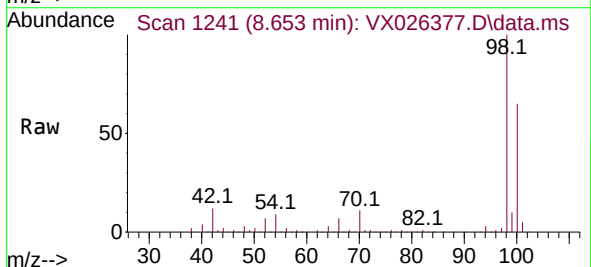

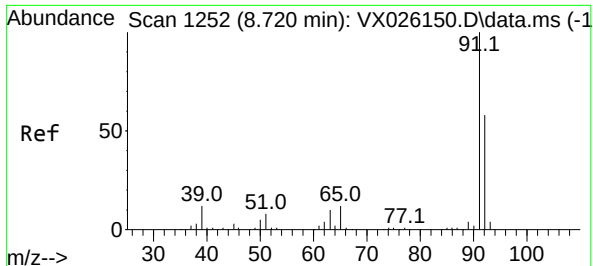

#52

Toluene

Concen: 3.553 ug/l

RT: 8.720 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX026377.D

Acq: 06 Jan 2022 16:40

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 92 Resp: 16234

Ion Ratio Lower Upper

92 100

91 170.1 136.0 204.0

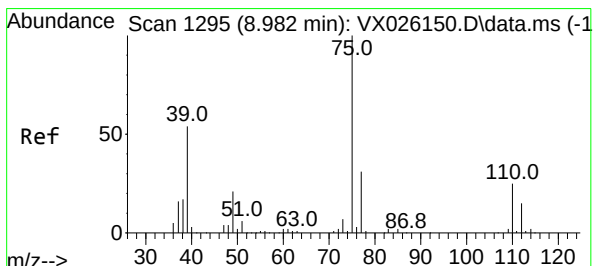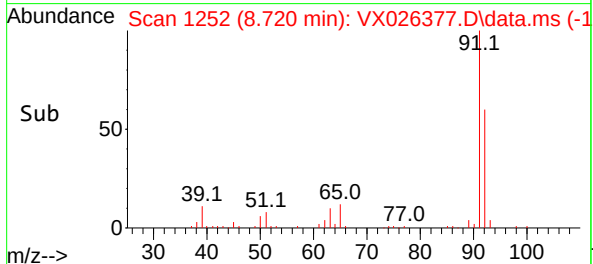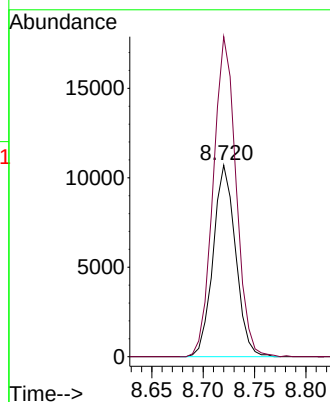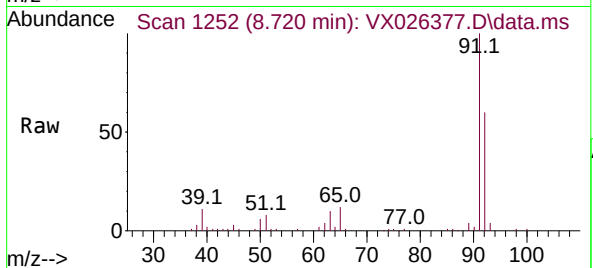

#53

t-1,3-Dichloropropene

Concen: 1.956 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. -0.256 min

Lab File: VX026377.D




Acq: 06 Jan 2022 16:40


Tgt Ion: 75 Resp: 199

Ion Ratio Lower Upper

75 100

77 95.9 25.1 37.7#

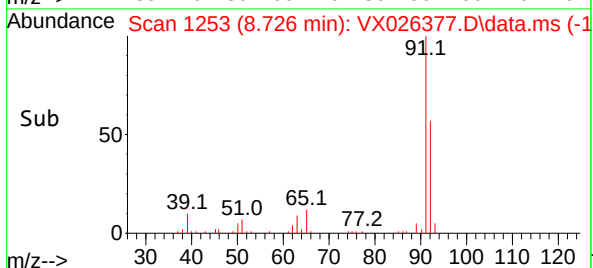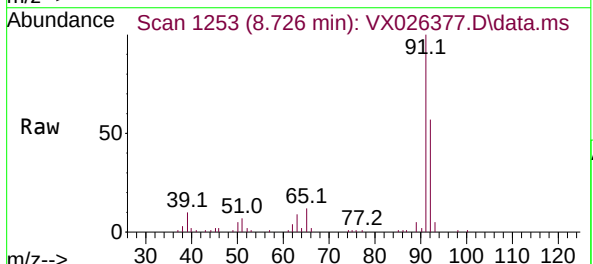

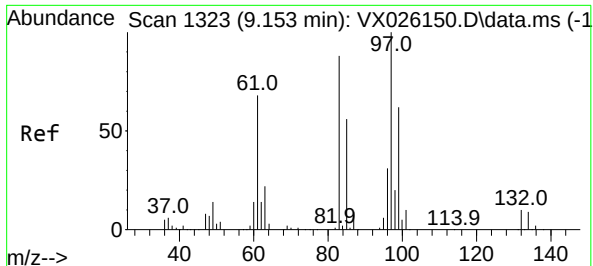

#55

1,1,2-Trichloroethane

Concen: 0.217 ug/l

RT: 9.019 min Scan# 1

Delta R.T. -0.134 min

Lab File: VX026377.D

Acq: 06 Jan 2022 16:40

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 97 Resp: 408





Ion Ratio Lower Upper

97 100

83 0.0 70.5 105.7#

85 0.0 43.8 65.6#

99 0.0 49.4 74.2#

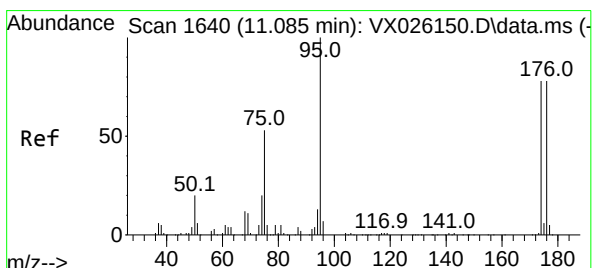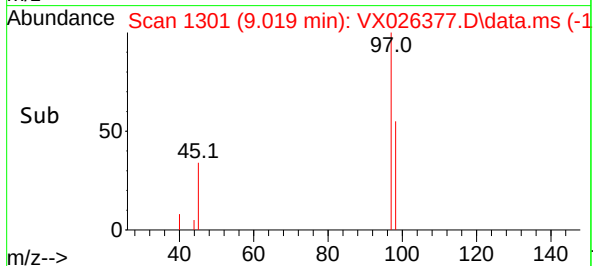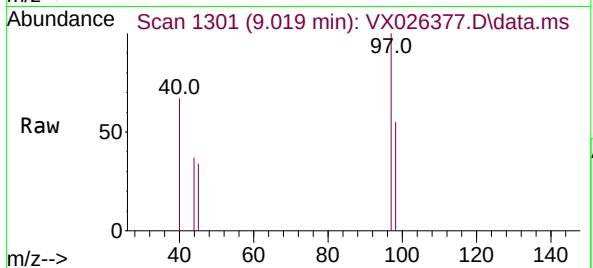

#62

4-Bromofluorobenzene

Concen: 49.280 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX026377.D

Acq: 06 Jan 2022 16:40




Tgt Ion: 95 Resp: 105196


Ion Ratio Lower Upper

95 100

174 72.8 0.0 157.4


176 69.8 0.0 154.6

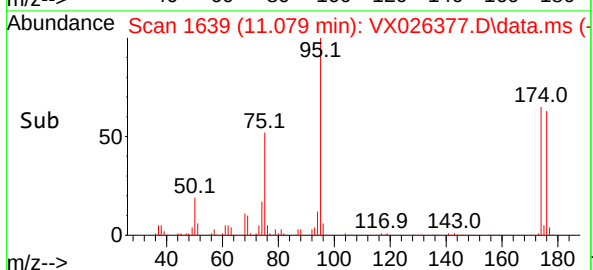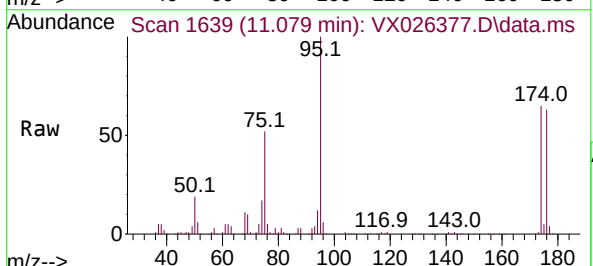






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Instrument :
MSVOA_X
ClientSampleId :



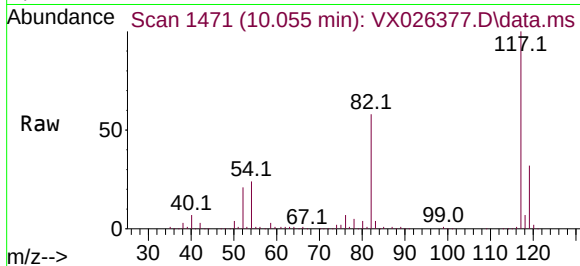



Tgt Ion:117 Resp: 210269
Ion Ratio Lower Upper
117 100
82 58.2 43.8 65.6
119 31.9 25.2 37.8



#67
Ethyl Benzene
Concen: 33.250 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 91 Resp: 274623
Ion Ratio Lower Upper
91 100
106 30.2 25.7 38.5


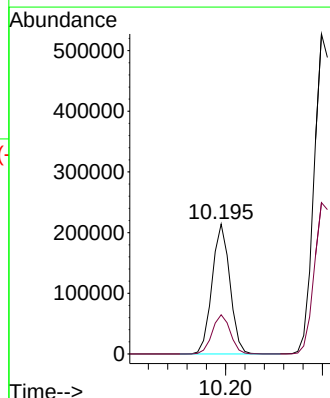
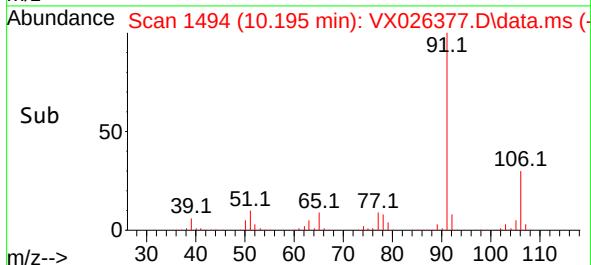
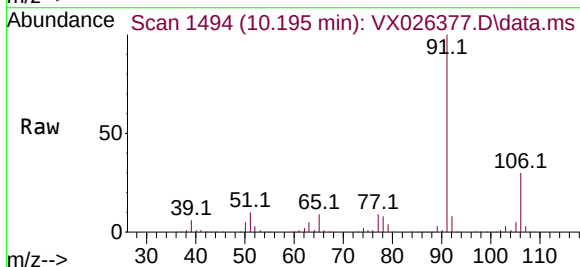




#68
m/p-Xylenes
Concen: 110.700 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 341381
Ion Ratio Lower Upper
106 100
91 209.3 158.6 238.0

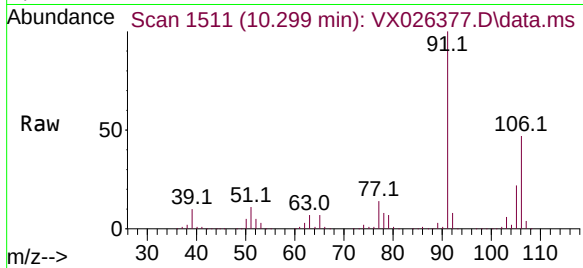

#69
o-Xylene
Concen: 13.318 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion:106 Resp: 40186
Ion Ratio Lower Upper
106 100
91 224.5 105.5 316.4


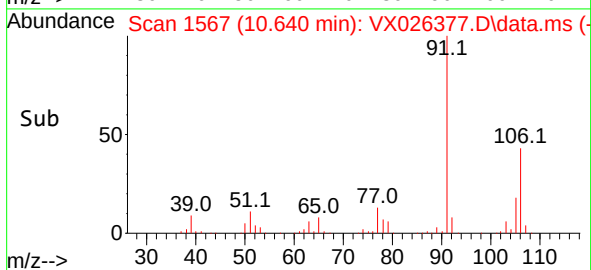

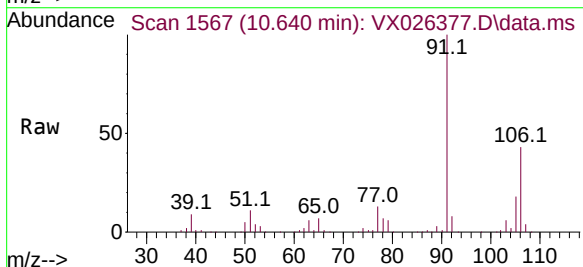




#70
Styrene
Concen: 0.385 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.019 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:104 Resp: 1904
Ion Ratio Lower Upper
104 100
78 334.0 39.8 59.6#
103 285.5 43.0 64.6#

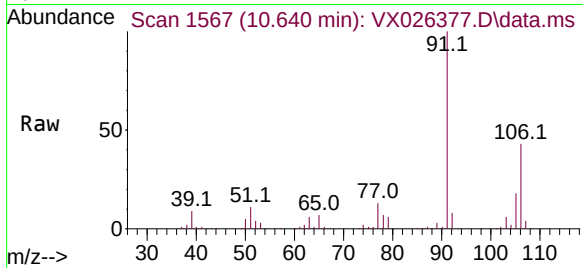

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40


Tgt Ion:152 Resp: 93594
Ion Ratio Lower Upper
152 100
115 62.2 41.3 123.9
150 157.2 0.0 351.8

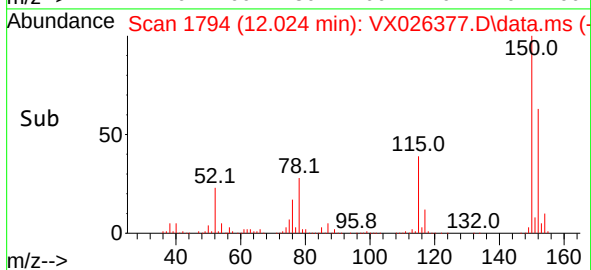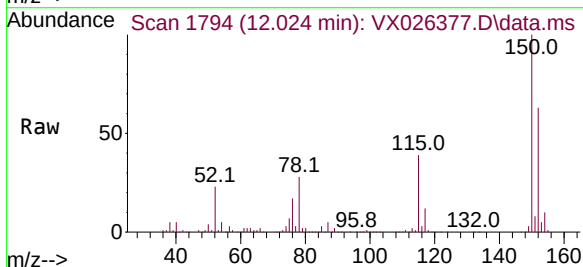






#73
Isopropylbenzene
Concen: 0.840 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.001 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Instrument :
MSVOA_X
ClientSampleId :



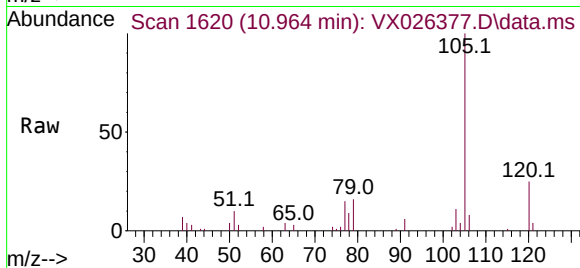



Tgt Ion:105 Resp: 6110
Ion Ratio Lower Upper
105 100
120 24.5 13.6 40.7

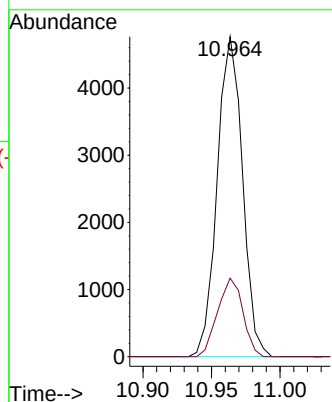

#76
1,2,3-Trichloropropane
Concen: 24.638 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 75 Resp: 55661
Ion Ratio Lower Upper
75 100
77 1.0 19.0 57.0#


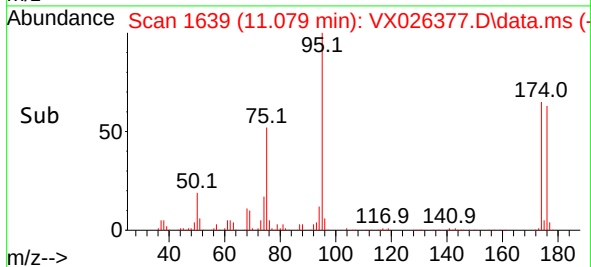
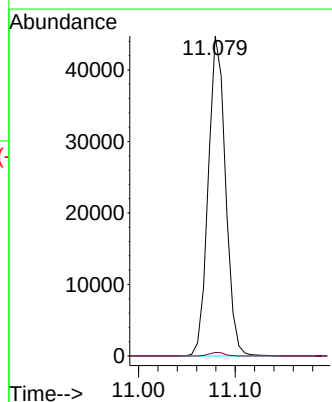
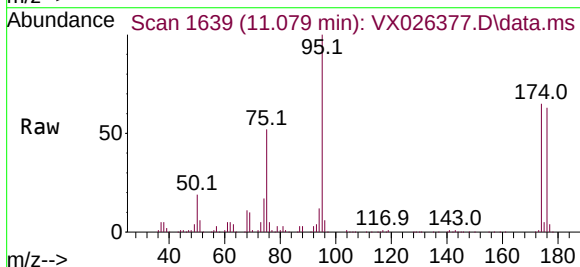




#78
n-propylbenzene
Concen: 1.446 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 12098
Ion Ratio Lower Upper
91 100
120 21.8 12.0 36.1

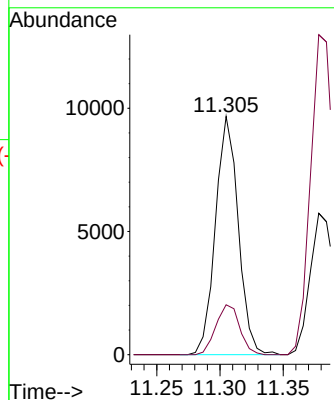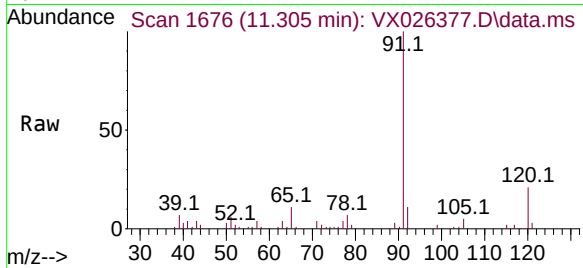

#79
2-Chlorotoluene
Concen: 1.857 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 91 Resp: 9562
Ion Ratio Lower Upper
91 100
126 0.0 17.8 53.3#


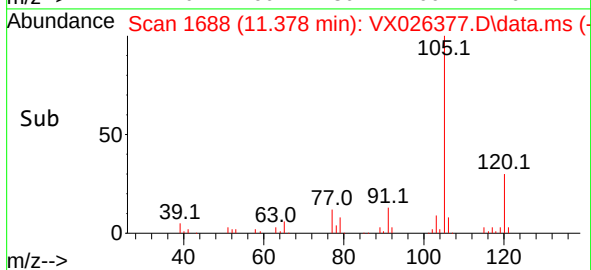
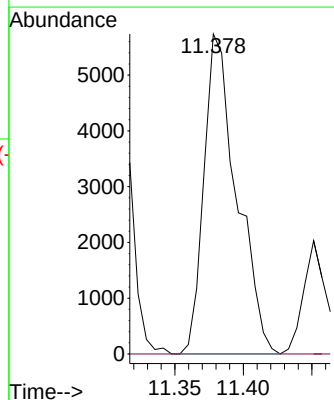
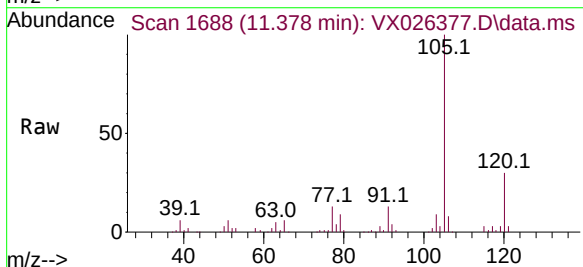




#80
 1,3,5-Trimethylbenzene
 Concen: 3.281 ug/l
 RT: 11.451 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX026377.D
 Acq: 06 Jan 2022 16:40




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 19811
 Ion Ratio Lower Upper
 105 100
 120 46.5 24.9 74.7

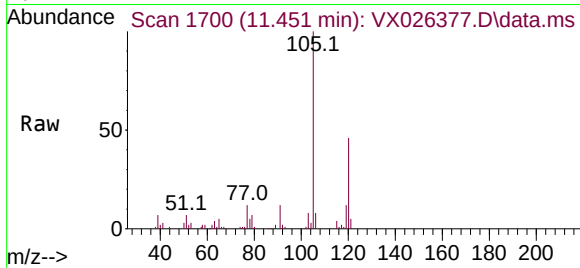

#81
 trans-1,4-Dichloro-2-butene
 Concen: 71.279 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. 0.061 min
 Lab File: VX026377.D
 Acq: 06 Jan 2022 16:40

Tgt Ion: 75 Resp: 55661
 Ion Ratio Lower Upper
 75 100
 53 0.0 79.5 119.3#
 89 0.0 38.3 57.5#


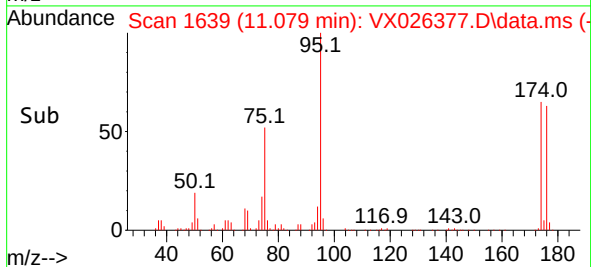

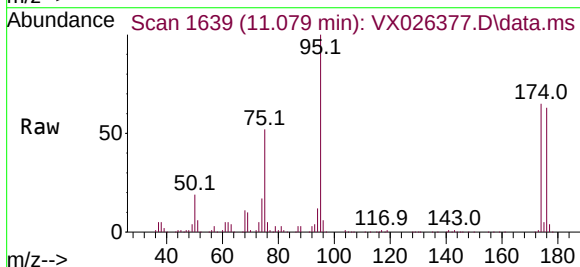




#82
4-Chlorotoluene
Concen: 0.391 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 2272
Ion Ratio Lower Upper
91 100
126 0.0 15.6 46.7#

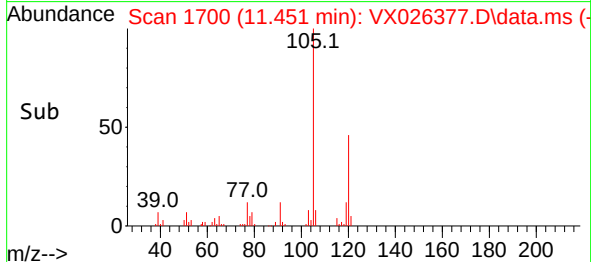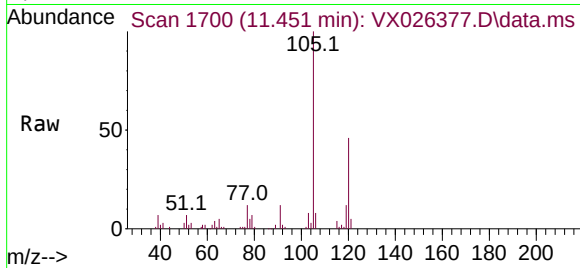

#83
tert-Butylbenzene
Concen: 1.656 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX026377.D
Acq: 06 Jan 2022 16:40

Tgt Ion: 119 Resp: 9707
Ion Ratio Lower Upper
119 100
91 95.9 28.7 86.1#
134 0.0 11.9 35.9#


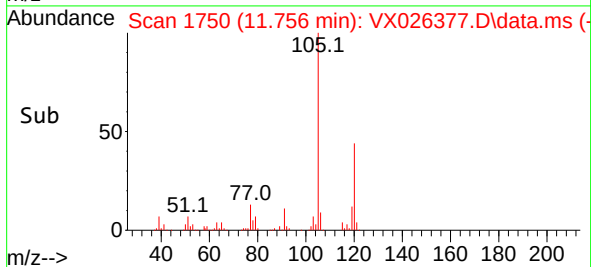

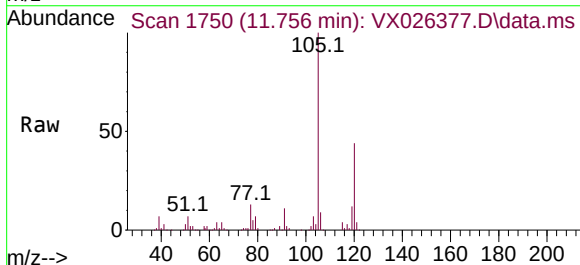




#84
 1,2,4-Trimethylbenzene
 Concen: 13.705 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.000 min
 Lab File: VX026377.D
 Acq: 06 Jan 2022 16:40




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 82675
 Ion Ratio Lower Upper
 105 100
 120 43.6 22.9 68.7

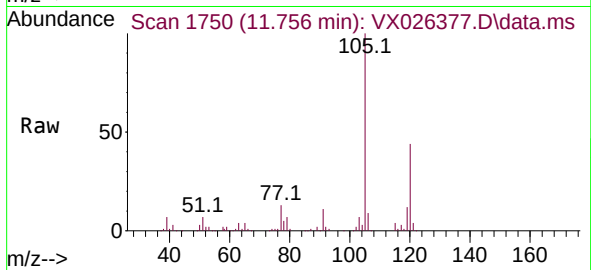

#85
 sec-Butylbenzene
 Concen: 11.305 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.134 min
 Lab File: VX026377.D
 Acq: 06 Jan 2022 16:40

Tgt Ion:105 Resp: 82675
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.1#

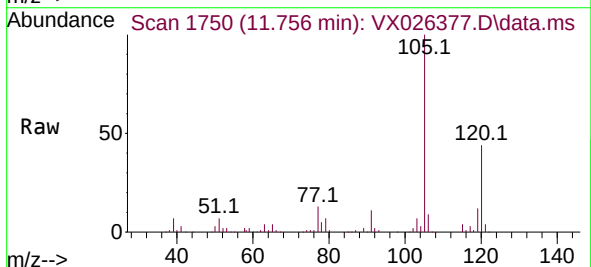



#90

Hexachloroethane

Concen: 1.898 ug/l

RT: 12.701 min Scan# 1905

Delta R.T. 0.159 min

Lab File: VX026377.D

Acq: 06 Jan 2022 16:40

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:117 Resp: 2311

Ion Ratio Lower Upper

117 100

201 0.0 35.4 106.3#

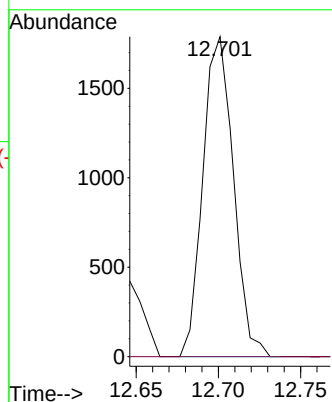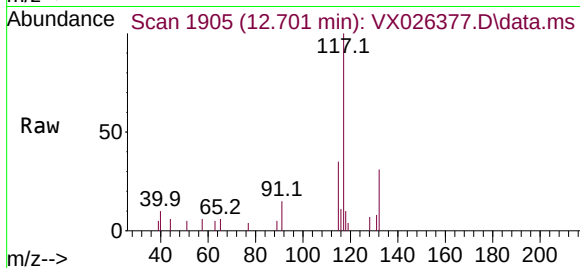

#95

Naphthalene

Concen: 4.083 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.000 min

Lab File: VX026377.D

Acq: 06 Jan 2022 16:40

Tgt Ion:128 Resp: 29536

Ion Ratio Lower Upper

128 100

127 12.5 10.3 15.5

129 10.4 8.8 13.2

