

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
 Data File : VX026384.D
 Acq On : 06 Jan 2022 19:21
 Operator : JC/MD
 Sample : N1020-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-12

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Title : SW846 8260

Signal : TIC: VX026384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rBV	33491	33691	4.23%	0.768%
2	1.362	37	45	52	rBV2	15219	61939	7.78%	1.413%
3	2.386	207	213	218	rBV	5827	9702	1.22%	0.221%
4	2.563	231	242	256	rBV2	9293	35672	4.48%	0.814%
5	4.721	586	596	607	rBV2	3180	9469	1.19%	0.216%
6	5.391	694	706	720	rBV2	94512	271839	34.16%	6.200%
7	5.556	722	733	752	rVB	168895	474600	59.65%	10.824%
8	5.958	786	799	810	rBV	112369	290969	36.57%	6.636%
9	6.763	921	931	945	rBV	256441	612453	76.97%	13.968%
10	8.653	1234	1241	1251	rBV	504576	795696	100.00%	18.147%
11	10.055	1465	1471	1484	rBV	510622	677484	85.14%	15.451%
12	10.299	1506	1511	1521	rVB	10379	14701	1.85%	0.335%
13	11.079	1634	1639	1652	rBV	390069	499343	62.76%	11.388%
14	12.024	1788	1794	1800	rBV	463531	581544	73.09%	13.263%
15	12.219	1822	1826	1839	rBV2	10327	15538	1.95%	0.354%




Sum of corrected areas: 4384640

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
Data File : VX026384.D
Acq On : 06 Jan 2022 19:21
Operator : JC/MD
Sample : N1020-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

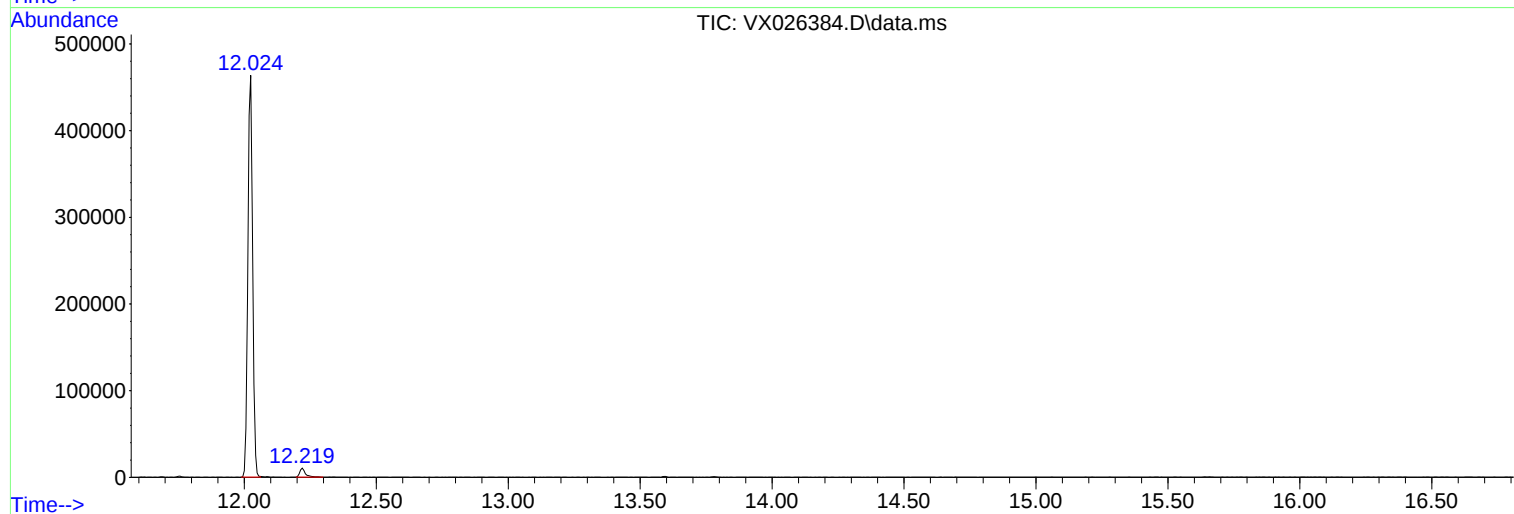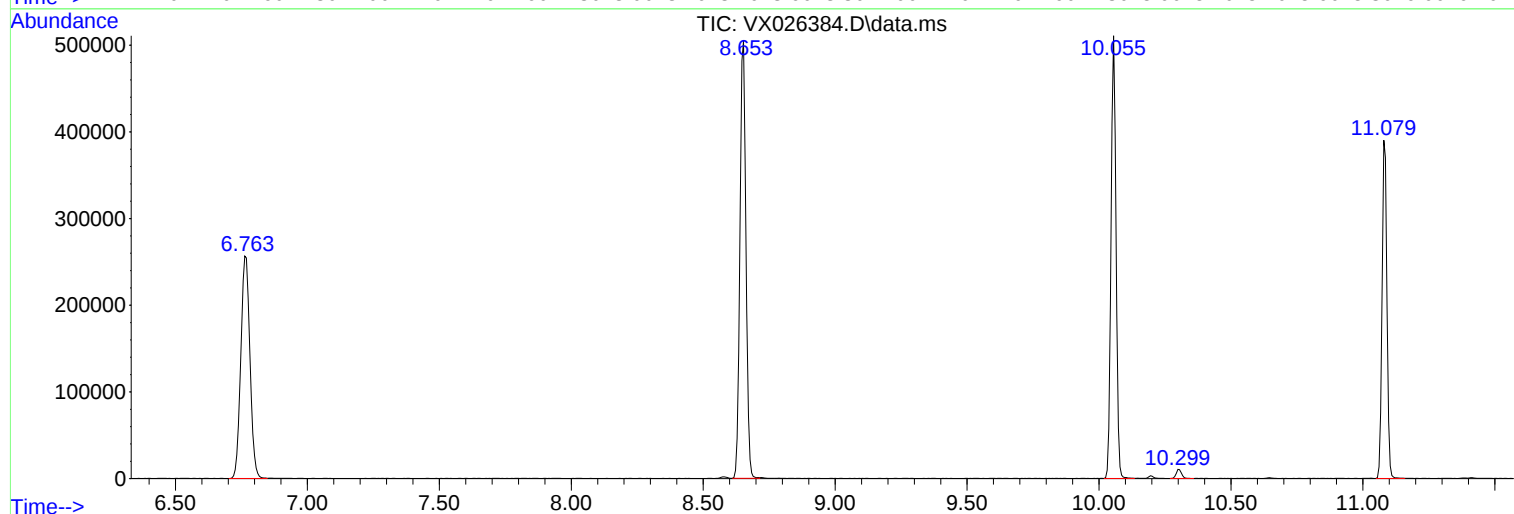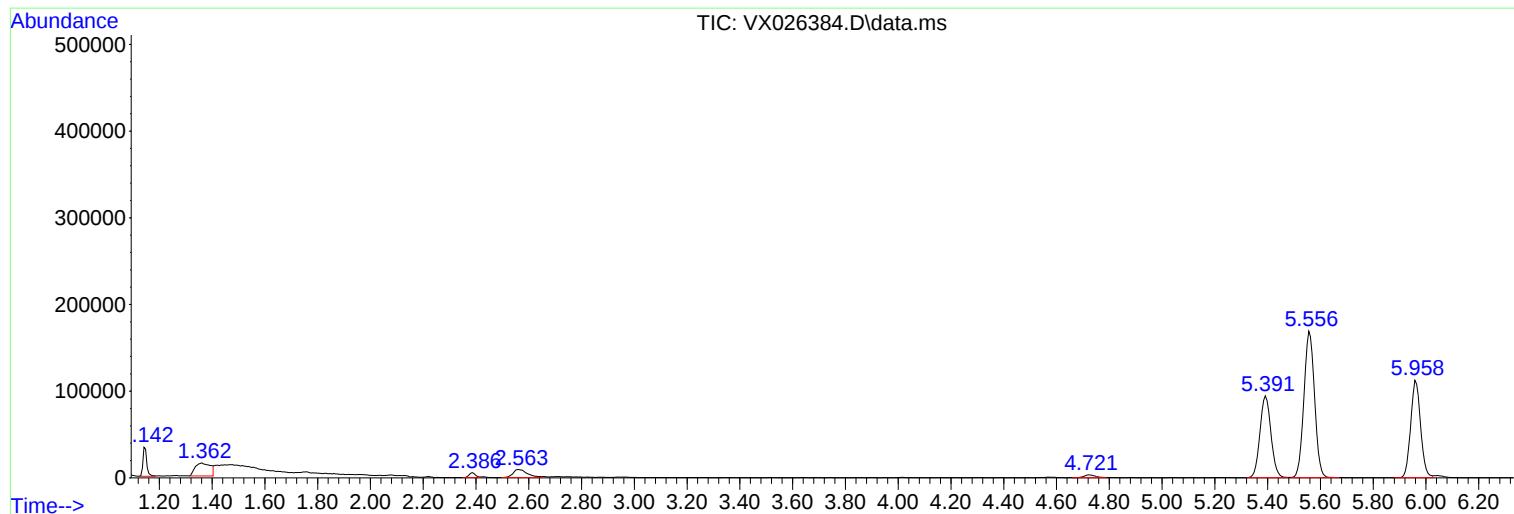

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
Data File : VX026384.D
Acq On : 06 Jan 2022 19:21
Operator : JC/MD
Sample : N1020-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-12










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.362	6.53 ug/l	61939	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

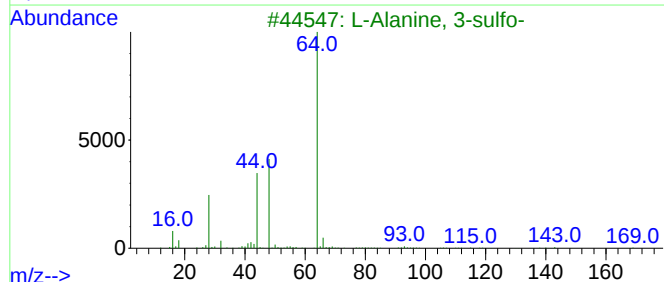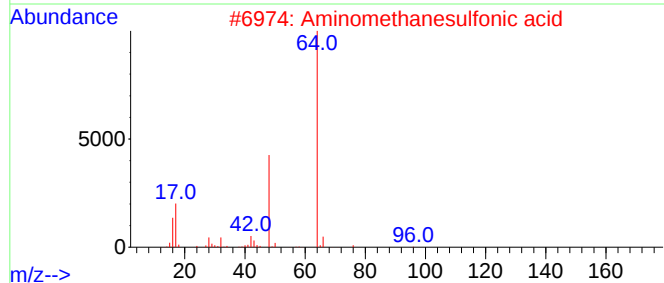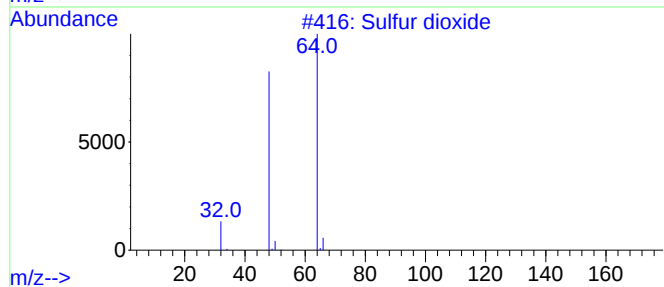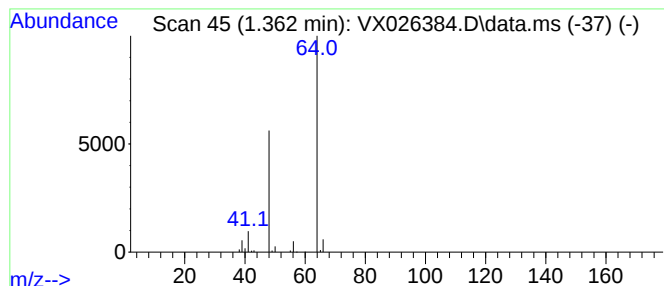

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010622\
Data File : VX026384.D
Acq On : 06 Jan 2022 19:21
Operator : JC/MD
Sample : N1020-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.362	6.5	ug/l	61939	1	5.556	474600	50.0