

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
 Data File : VX033631.D
 Acq On : 06 Jan 2023 15:25
 Operator : JC/MD
 Sample : PB050057ZHE#08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB050057ZHE#08

Quant Time: Jan 07 04:25:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 05 04:43:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	167999	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	241878	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	171675	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	105097	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	90053	47.484	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.960%
35) Dibromofluoromethane	5.385	113	74952	47.144	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.280%
50) Toluene-d8	8.647	98	283796	49.942	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.880%
62) 4-Bromofluorobenzene	11.079	95	100782	50.036	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.080%
Target Compounds						
					Qvalue	
3) Chloromethane	1.301	50	466	0.273	ug/l #	42
6) Chloroethane	1.679	64	193	0.221	ug/l #	43
11) Tert butyl alcohol	2.947	59	1436	4.609	ug/l #	80
14) Allyl chloride	2.672	41	538	0.205	ug/l #	32
16) Acetone	2.392	43	32891	39.851	ug/l	97
17) Carbon Disulfide	2.514	76	216	1.680	ug/l #	74
18) Methyl Acetate	2.703	43	2156	0.820	ug/l #	91
20) Methylene Chloride	2.788	84	5318	1.177	ug/l	96
25) 2-Butanone	4.574	43	6878	5.554	ug/l	100
29) Tetrahydrofuran	5.038	42	1075	1.369	ug/l #	78
31) Cyclohexane	5.556	56	2959	1.121	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	11009	5.112	ug/l #	50
37) Ethyl Acetate	4.715	43	23764	8.182	ug/l	98
38) Carbon Tetrachloride	5.550	117	15618	6.853	ug/l #	15
41) Methacrylonitrile	5.044	41	594	0.454	ug/l #	42
43) Isopropyl Acetate	6.336	43	101970	27.694	ug/l	99
48) Methyl methacrylate	7.793	41	91119	48.889	ug/l #	45
49) 1,4-Dioxane	7.799	88	63	1.589	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	86951	37.311	ug/l #	51
53) t-1,3-Dichloropropene	8.952	75	789	0.444	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	37750	15.507	ug/l #	60
56) Ethyl methacrylate	9.238	69	609	0.252	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	4598	1.658	ug/l #	42
59) 2-Hexanone	9.482	43	70028	40.678	ug/l #	50
74) N-amyl acetate	10.640	43	27637	9.190	ug/l #	52
76) 1,2,3-Trichloropropane	11.079	75	49758	25.843	ug/l #	35
81) trans-1,4-Dichloro-2-b...	11.079	75	49758	78.437	ug/l #	7
93) 1,2,4-Trichlorobenzene	13.591	180	120	1.643	ug/l #	12
95) Naphthalene	13.774	128	238	3.148	ug/l #	69
96) 1,2,3-Trichlorobenzene	13.957	180	40	3.764	ug/l #	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
Data File : VX033631.D
Acq On : 06 Jan 2023 15:25
Operator : JC/MD
Sample : PB050057ZHE#08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08

Quant Time: Jan 07 04:25:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 05 04:43:25 2023
Response via : Initial Calibration




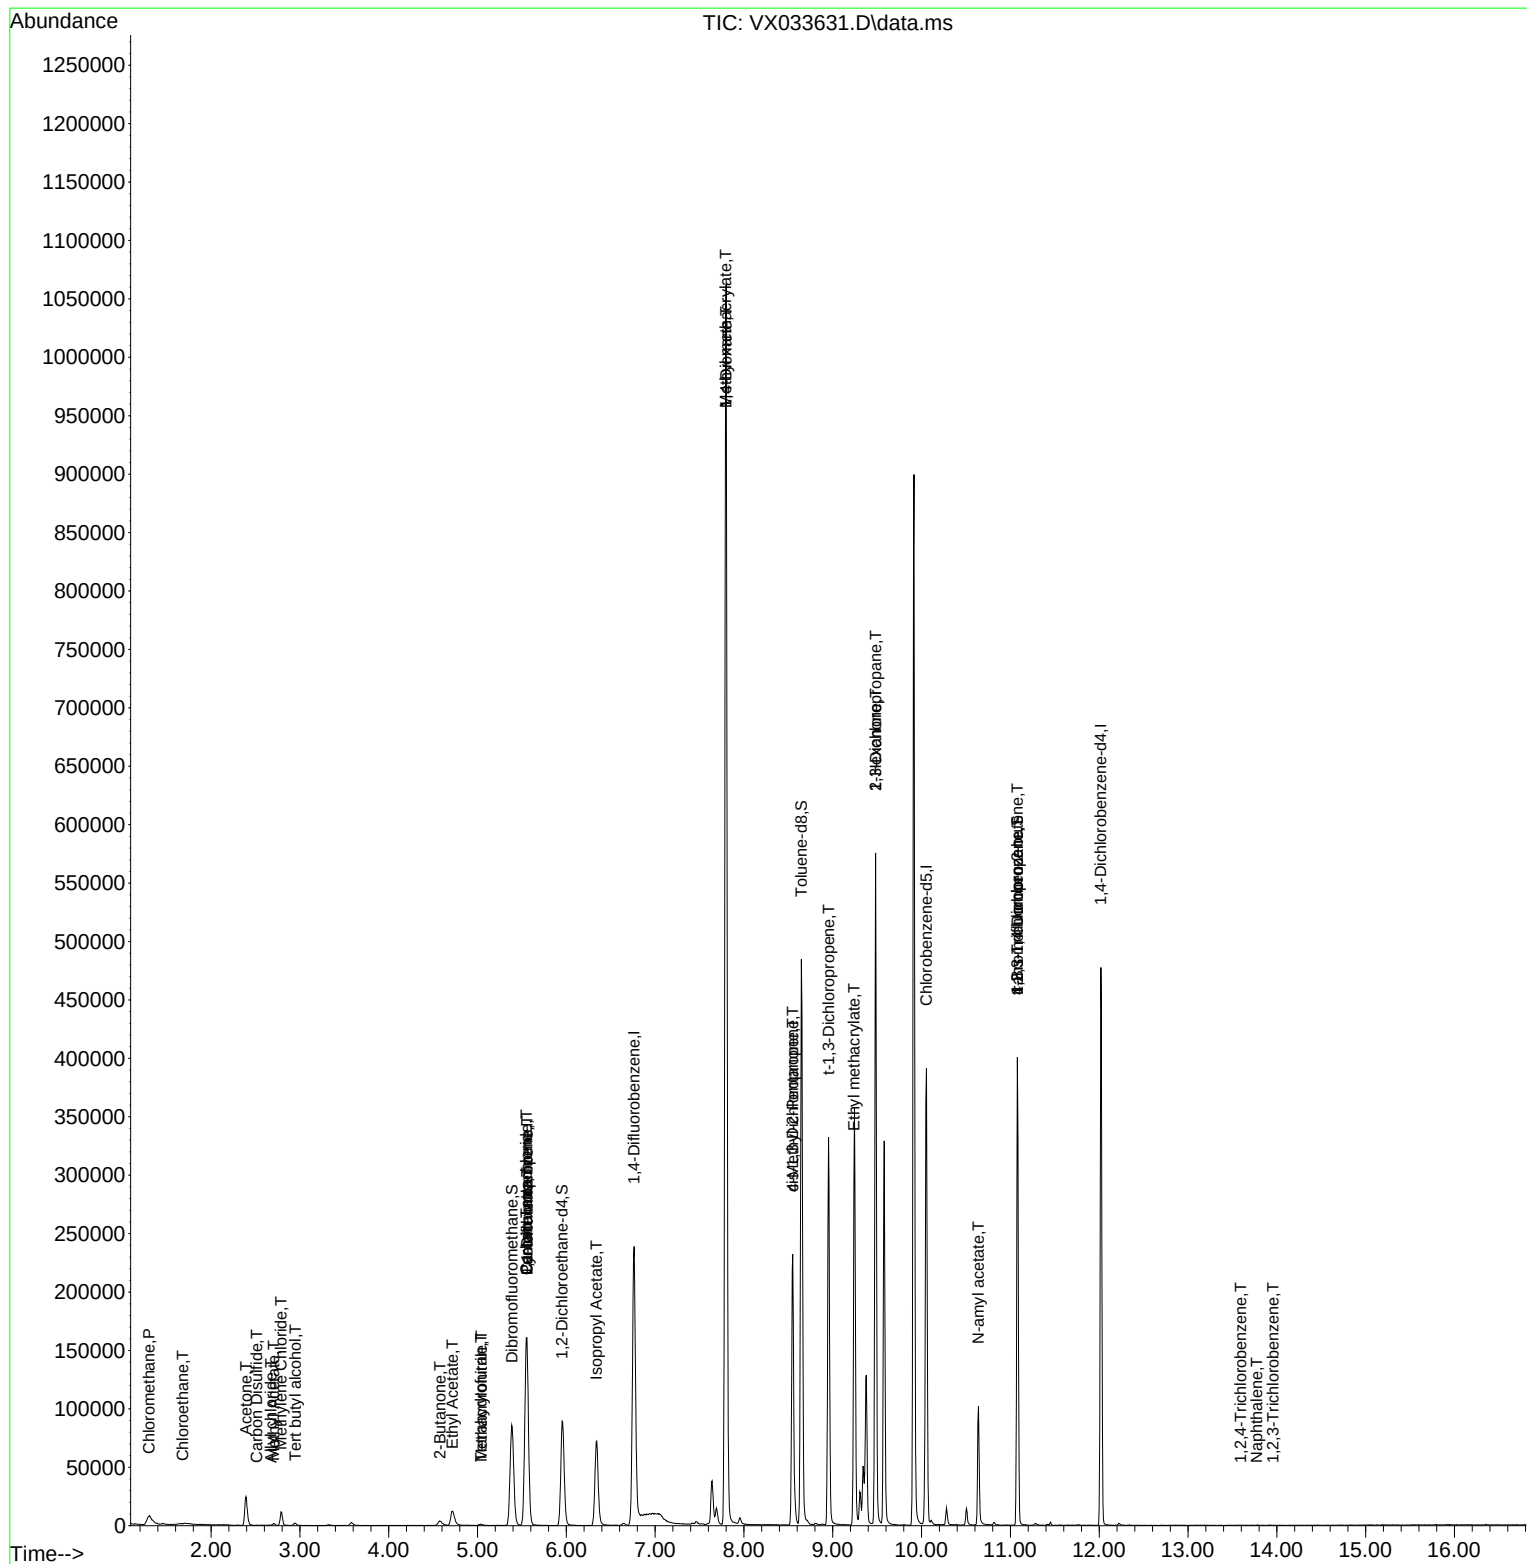




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion:168 Resp: 167999
Ion Ratio Lower Upper
168 100
99 51.3 41.4 62.2

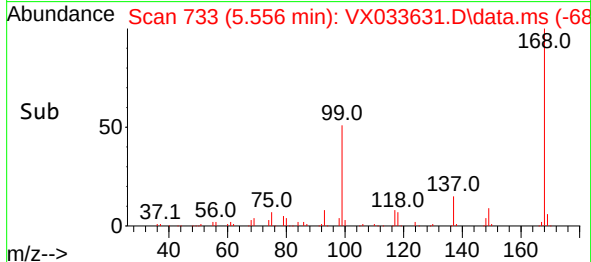

#3
Chloromethane
Concen: 0.273 ug/l
RT: 1.301 min Scan# 35
Delta R.T. 0.006 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion: 50 Resp: 466
Ion Ratio Lower Upper
50 100
52 0.0 26.1 39.1#



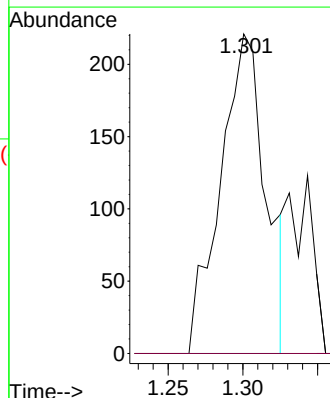



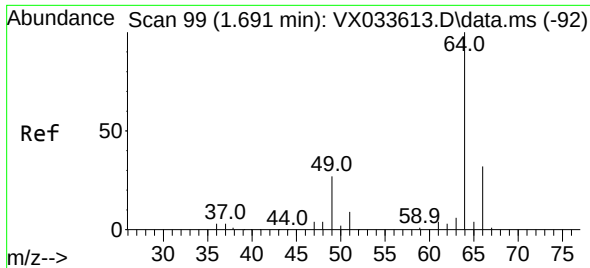

#6
Chloroethane
Concen: 0.221 ug/l
RT: 1.679 min Scan# 91
Delta R.T. -0.012 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion: 64 Resp: 193
Ion Ratio Lower Upper
64 100
66 0.0 25.7 38.5#

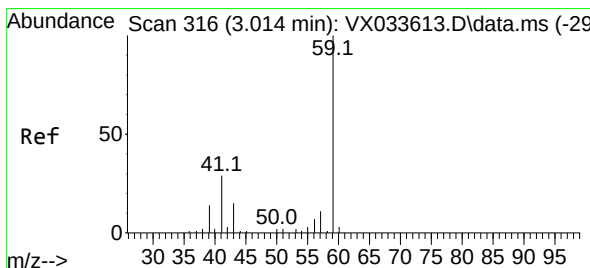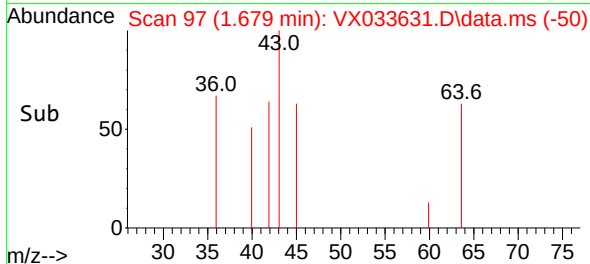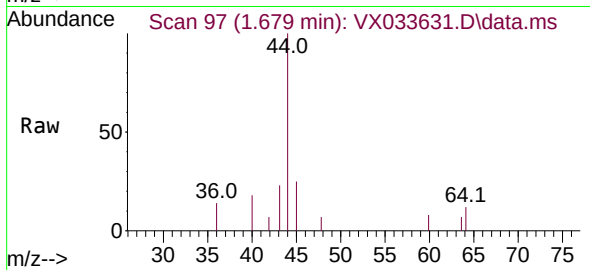

#11
Tert butyl alcohol
Concen: 4.609 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.067 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion: 59 Resp: 1436
Ion Ratio Lower Upper
59 100
57 0.0 5.5 8.3#


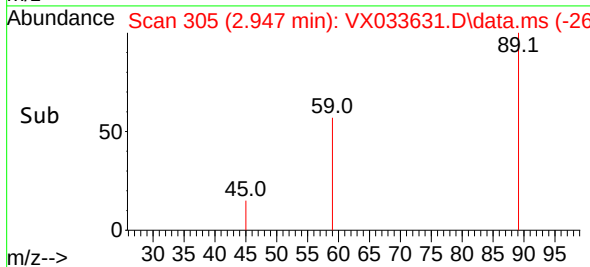

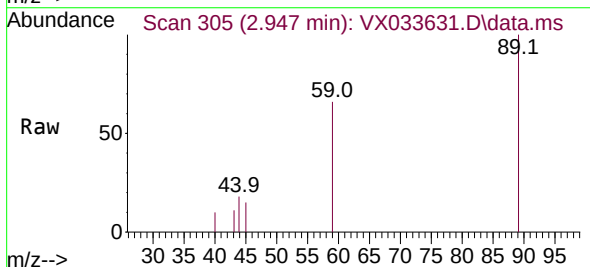




#14
 Allyl chloride
 Concen: 0.205 ug/l
 RT: 2.672 min Scan# 214
 Delta R.T. 0.006 min
 Lab File: VX033631.D
 Acq: 06 Jan 2023 15:25




Instrument :
 MSVOA_X
 ClientSampleId :
 PB050057ZHE#08


Tgt Ion: 41 Resp: 538
 Ion Ratio Lower Upper
 41 100
 39 7.8 53.3 79.9#
 76 0.0 25.0 37.4#



#16
 Acetone
 Concen: 39.851 ug/l
 RT: 2.392 min Scan# 214
 Delta R.T. -0.006 min
 Lab File: VX033631.D
 Acq: 06 Jan 2023 15:25

Tgt Ion: 43 Resp: 32891
 Ion Ratio Lower Upper
 43 100
 58 30.3 22.9 34.3

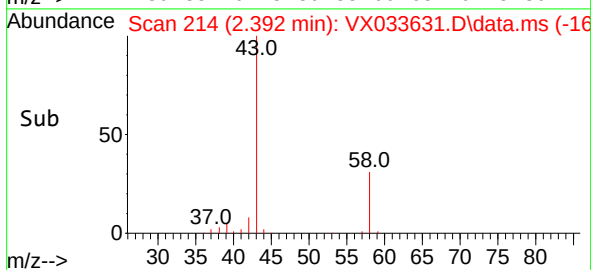



#17

Carbon Disulfide

Concen: 1.680 ug/l

RT: 2.514 min Scan# 216

Delta R.T. -0.000 min

Lab File: VX033631.D

Acq: 06 Jan 2023 15:25

Instrument :

MSVOA_X

ClientSampleId :





PB050057ZHE#08

Tgt Ion: 76 Resp: 216

Ion Ratio Lower Upper

76 100

78 0.0 7.6 11.4#

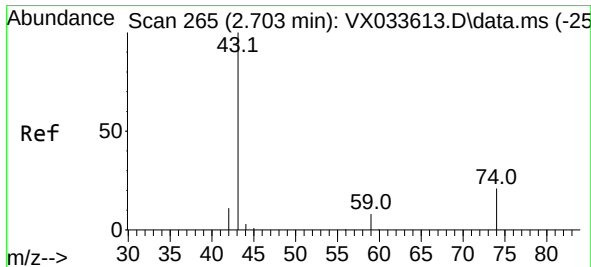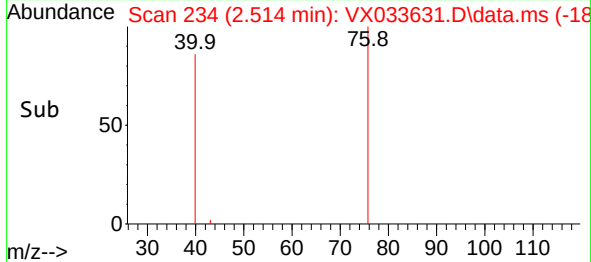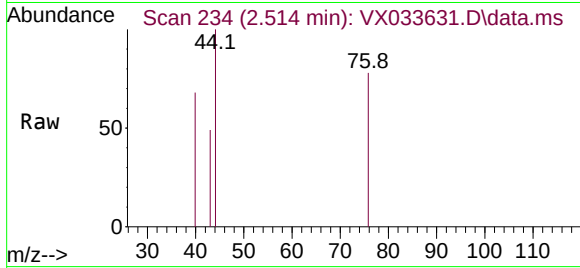

#18

Methyl Acetate

Concen: 0.820 ug/l

RT: 2.703 min Scan# 265

Delta R.T. -0.000 min

Lab File: VX033631.D




Acq: 06 Jan 2023 15:25


Tgt Ion: 43 Resp: 2156

Ion Ratio Lower Upper

43 100

74 17.9 17.9 26.9#

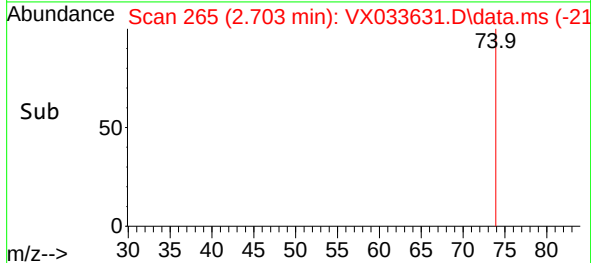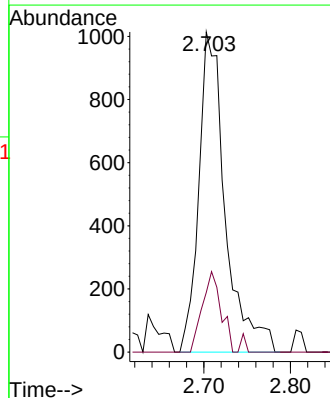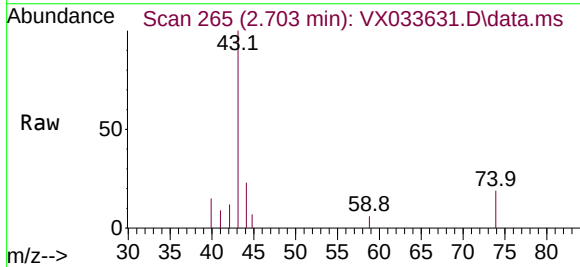



#20

Methylene Chloride

Concen: 1.177 ug/l

RT: 2.788 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX033631.D

Acq: 06 Jan 2023 15:25

Instrument :

MSVOA_X

ClientSampleId :

PB050057ZHE#08

Tgt Ion: 84 Resp: 5318





Ion Ratio Lower Upper

84 100

49 126.9 97.6 146.4

51 41.1 30.4 45.6

86 63.5 49.7 74.5



#25

2-Butanone

Concen: 5.554 ug/l

RT: 4.574 min Scan# 572

Delta R.T. 0.012 min

Lab File: VX033631.D




Acq: 06 Jan 2023 15:25


Tgt Ion: 43 Resp: 6878

Ion Ratio Lower Upper

43 100

72 24.8 19.8 29.6

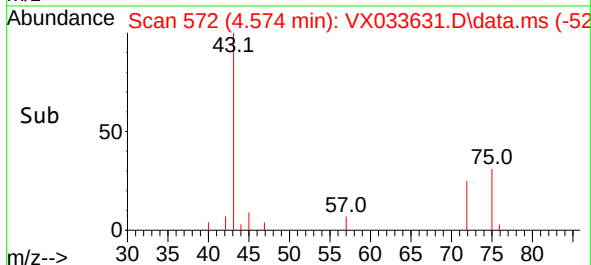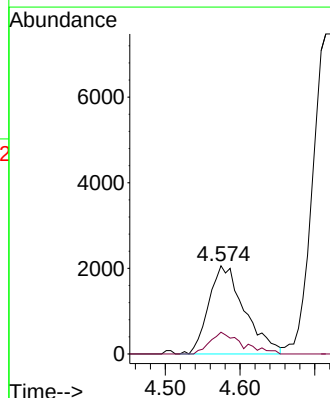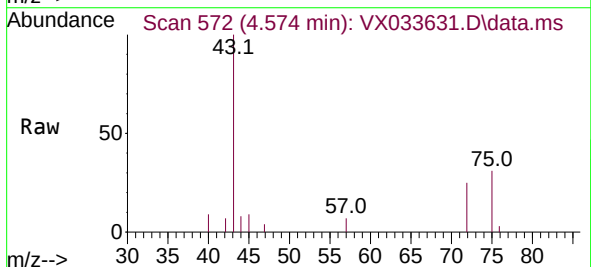

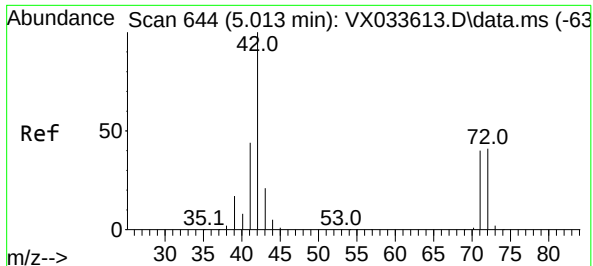

#29

Tetrahydrofuran

Concen: 1.369 ug/l

RT: 5.038 min Scan# 644

Delta R.T. 0.024 min

Lab File: VX033631.D

Acq: 06 Jan 2023 15:25

Instrument :

MSVOA_X

ClientSampleId :

PB050057ZHE#08





Tgt Ion: 42 Resp: 1075

Ion Ratio Lower Upper

42 100

72 30.8 34.2 51.4#

71 24.1 31.4 47.0#

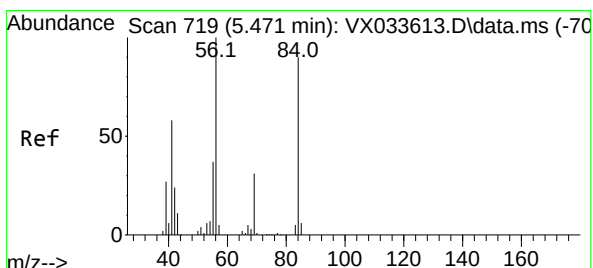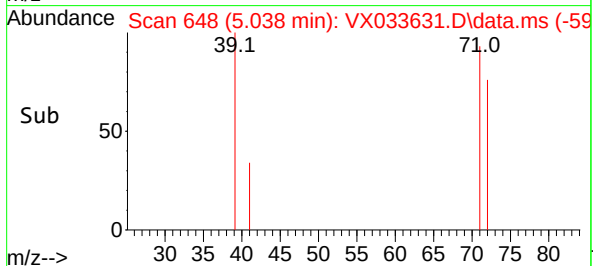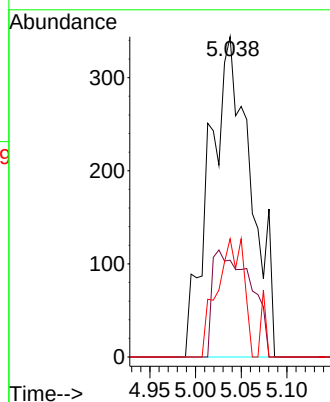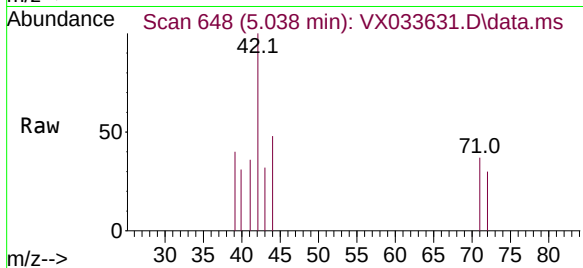

#31

Cyclohexane

Concen: 1.121 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.085 min

Lab File: VX033631.D

Acq: 06 Jan 2023 15:25




Tgt Ion: 56 Resp: 2959


Ion Ratio Lower Upper

56 100

69 225.8 24.6 36.8#

84 148.1 72.2 108.2#


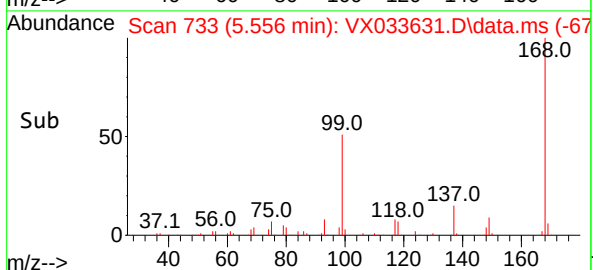

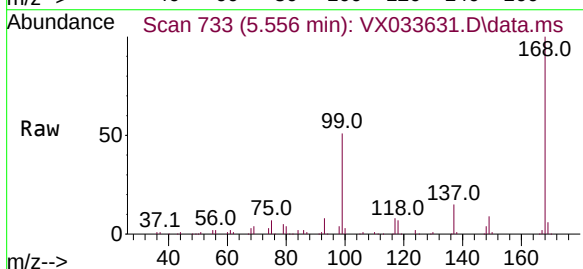




#33
 1,2-Dichloroethane-d4
 Concen: 47.484 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. -0.000 min
 Lab File: VX033613.D
 Acq: 06 Jan 2023 15:25




Instrument :
 MSVOA_X
 ClientSampleId :
 PB050057ZHE#08


Tgt Ion: 65 Resp: 90053
 Ion Ratio Lower Upper
 65 100
 67 49.9 0.0 104.8



#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. -0.000 min
 Lab File: VX033613.D
 Acq: 06 Jan 2023 15:25

Tgt Ion: 114 Resp: 241878
 Ion Ratio Lower Upper
 114 100
 63 19.8 0.0 40.0
 88 15.5 0.0 29.6


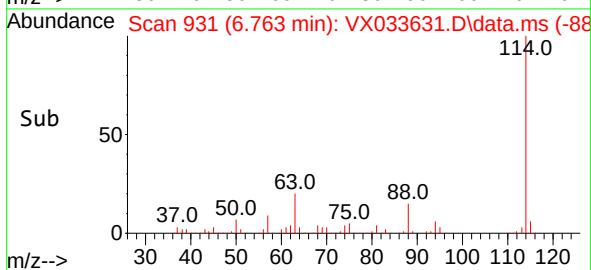

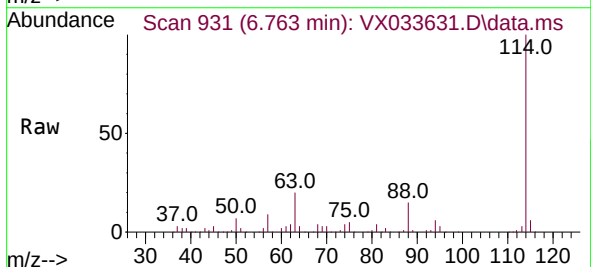


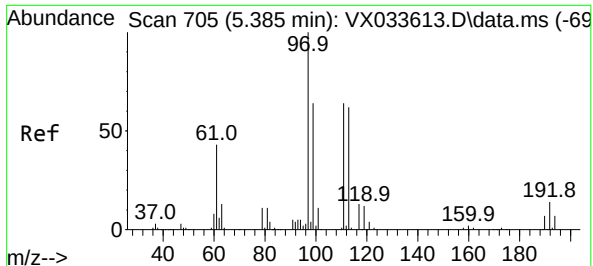

#35
Dibromofluoromethane
Concen: 47.144 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion:113 Resp: 74952
Ion Ratio Lower Upper
113 100
111 101.7 81.2 121.8
192 22.3 18.2 27.2

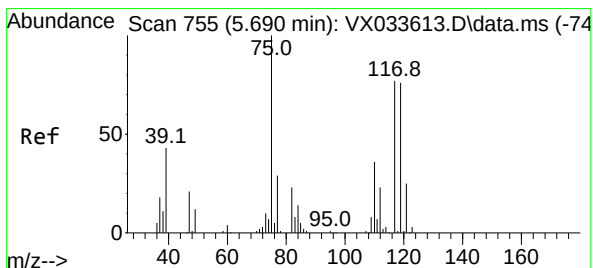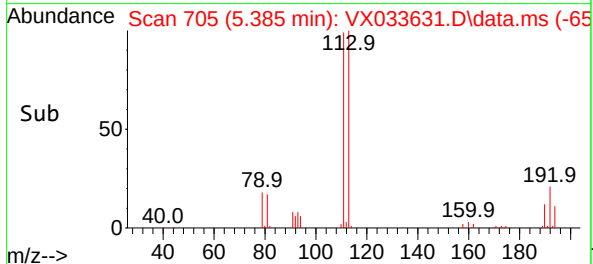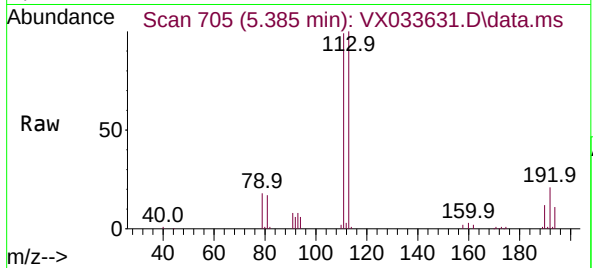

#36
1,1-Dichloropropene
Concen: 5.112 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion: 75 Resp: 11009
Ion Ratio Lower Upper
75 100
110 9.1 18.0 54.0#
77 0.0 24.5 36.7#


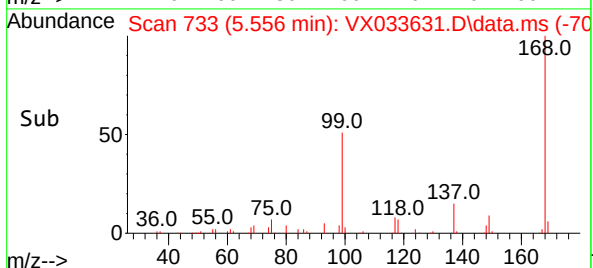
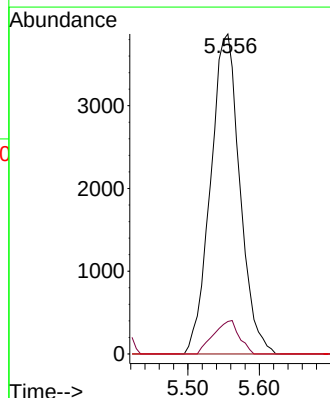
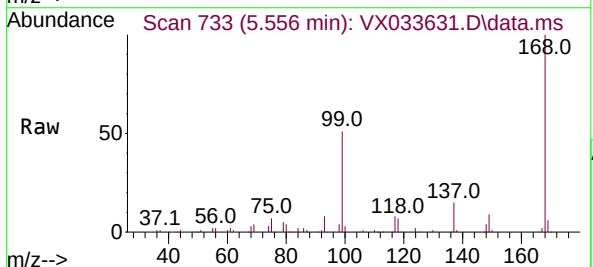




#37
Ethyl Acetate
Concen: 8.182 ug/l
RT: 4.715 min Scan# 595
Delta R.T. -0.000 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion:	43	Resp:	23764
Ion	Ratio	Lower	Upper
43	100		
61	12.6	10.6	16.0
70	11.1	8.1	12.1

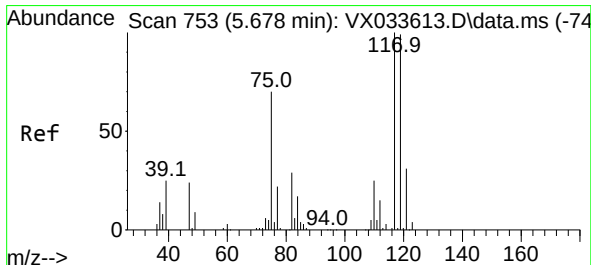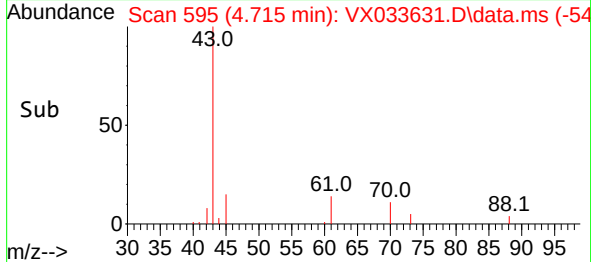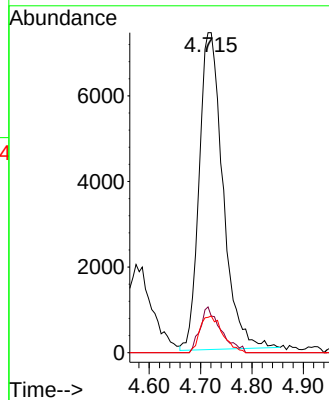

#38
Carbon Tetrachloride
Concen: 6.853 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion:	117	Resp:	15618
Ion	Ratio	Lower	Upper
117	100		
119	5.0	78.8	118.2#
121	0.0	24.9	37.3#


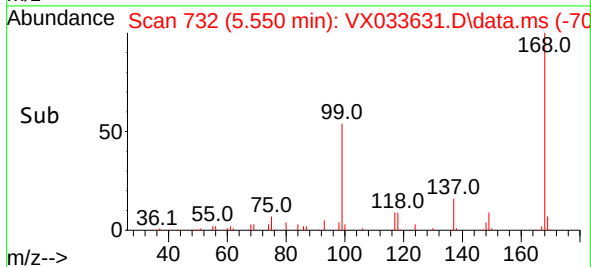
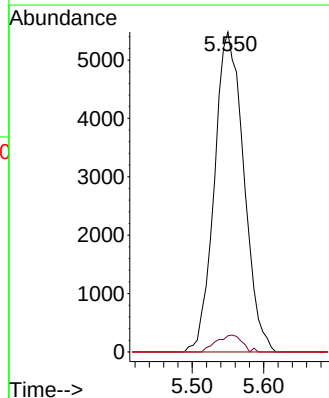
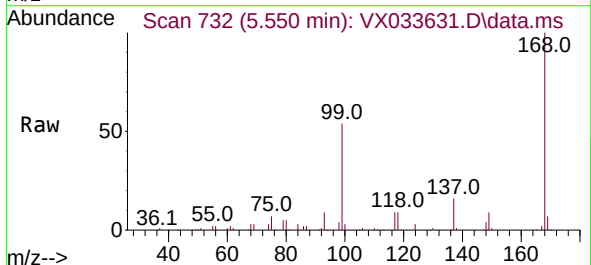




#41
Methacrylonitrile
Concen: 0.454 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.128 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion: 41	Resp: 594
Ion Ratio	Lower Upper
41 100	
39 33.8	44.1 66.1#
67 0.0	53.8 80.6#
52 0.0	23.1 34.7#

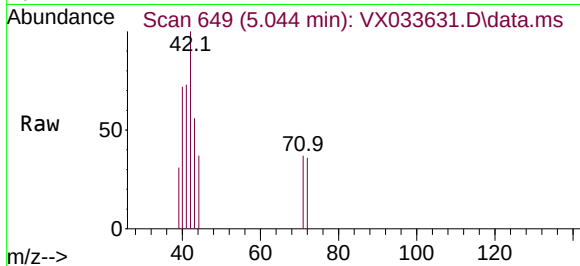

#43
Isopropyl Acetate
Concen: 27.694 ug/l
RT: 6.336 min Scan# 861
Delta R.T. -0.006 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion: 43	Resp: 101970
Ion Ratio	Lower Upper
43 100	
61 19.0	15.2 22.8
87 12.8	10.6 16.0

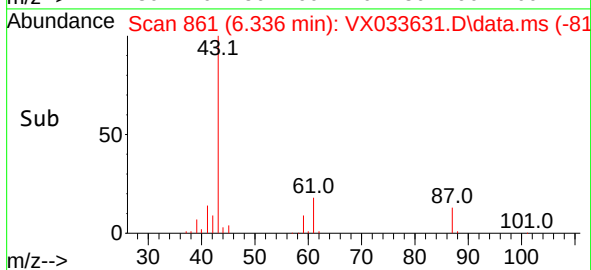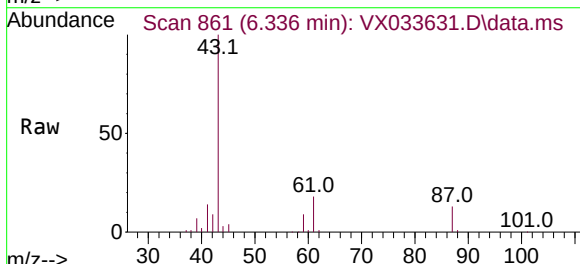

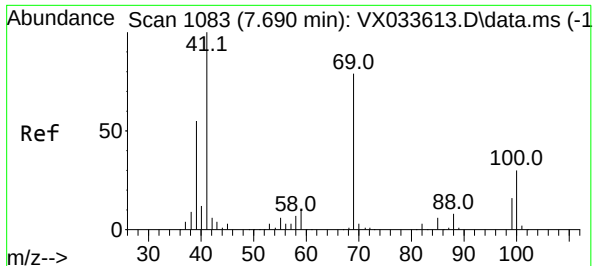

#48

Methyl methacrylate

Concen: 48.889 ug/l

RT: 7.793 min Scan# 1100

Delta R.T. 0.104 min

Lab File: VX033631.D

Acq: 06 Jan 2023 15:25

Instrument :

MSVOA_X

ClientSampleId :

PB050057ZHE#08





Tgt Ion: 41 Resp: 91119

Ion Ratio Lower Upper

41 100

69 0.2 63.1 94.7#

39 51.7 44.8 67.2

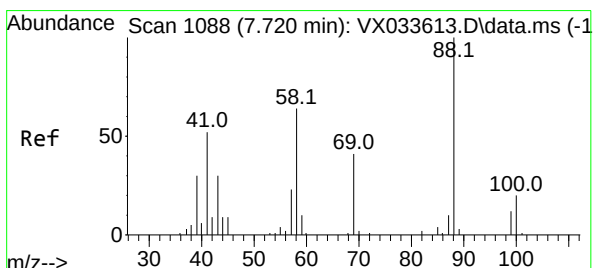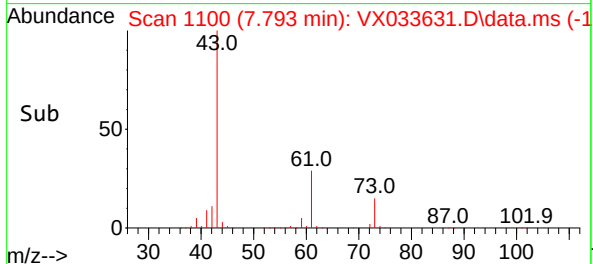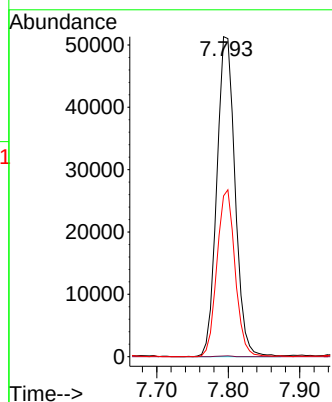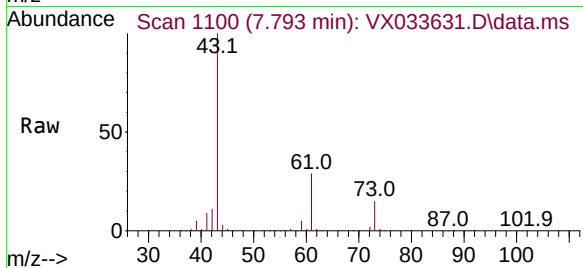

#49

1,4-Dioxane

Concen: 1.589 ug/l

RT: 7.799 min Scan# 1101

Delta R.T. 0.079 min

Lab File: VX033631.D

Acq: 06 Jan 2023 15:25




Tgt Ion: 88 Resp: 63


Ion Ratio Lower Upper

88 100

43 1597763.5 24.1 36.1#

58 6179.4 57.1 85.7#


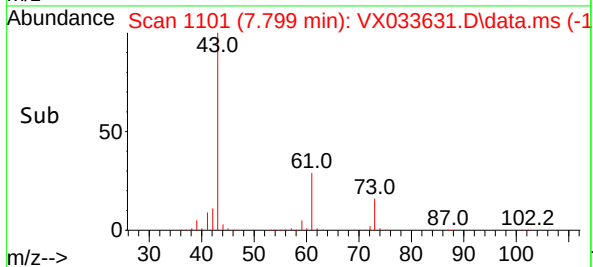

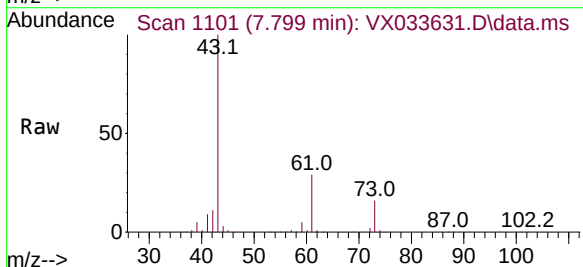




#50
Toluene-d8
Concen: 49.942 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033613.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion: 98 Resp: 283796
Ion Ratio Lower Upper
98 100
100 66.1 53.6 80.4



#51
4-Methyl-2-Pentanone
Concen: 37.311 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.024 min
Lab File: VX033613.D
Acq: 06 Jan 2023 15:25

Tgt Ion: 43 Resp: 86951
Ion Ratio Lower Upper
43 100
58 8.6 30.5 45.7#

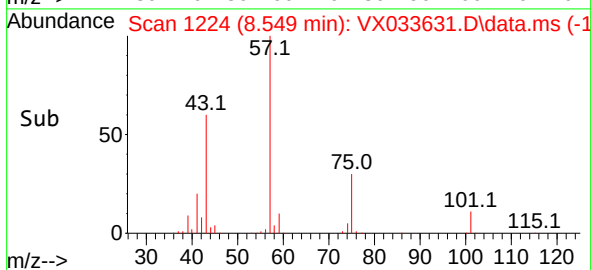

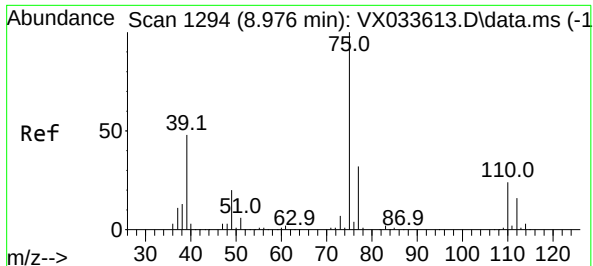

#53

t-1,3-Dichloropropene

Concen: 0.444 ug/l

RT: 8.952 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX033631.D

Acq: 06 Jan 2023 15:25

Instrument :

MSVOA_X

ClientSampleId :





PB050057ZHE#08

Tgt Ion: 75 Resp: 789

Ion Ratio Lower Upper

75 100

77 0.0 25.3 37.9#

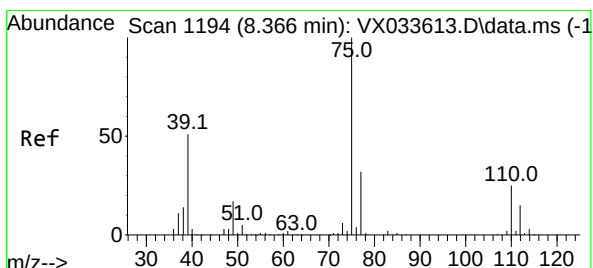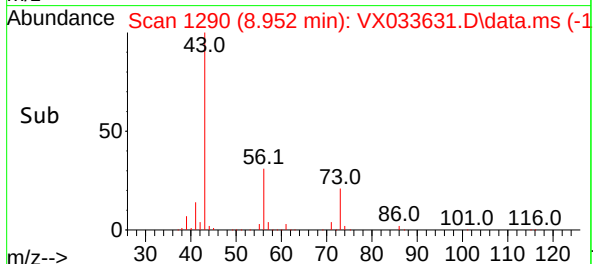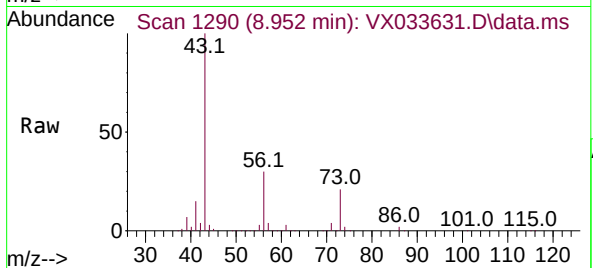

#54

cis-1,3-Dichloropropene

Concen: 15.507 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.183 min

Lab File: VX033631.D

Acq: 06 Jan 2023 15:25




Tgt Ion: 75 Resp: 37750


Ion Ratio Lower Upper

75 100

77 0.6 25.5 38.3#

39 30.6 40.6 61.0#


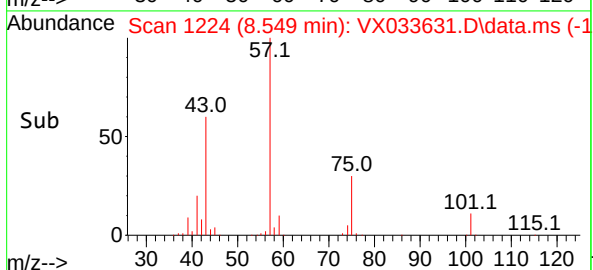

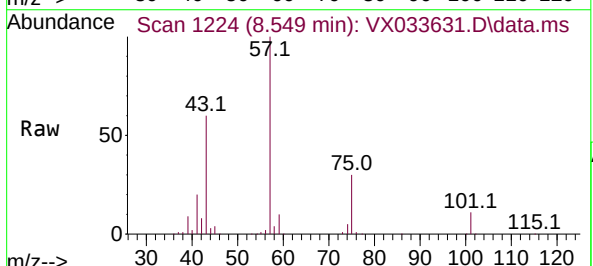


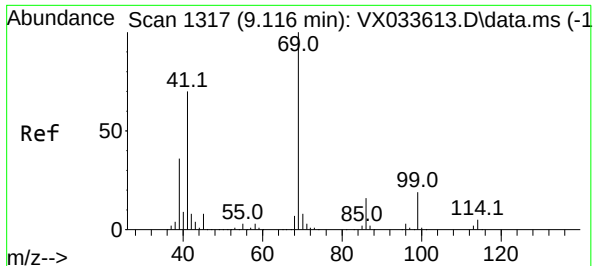

#56
Ethyl methacrylate
Concen: 0.252 ug/l
RT: 9.238 min Scan# 1337
Delta R.T. 0.122 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion: 69 Resp: 609
Ion Ratio Lower Upper
69 100
41 9000.7 56.6 84.8#
39 3604.8 29.4 44.0#

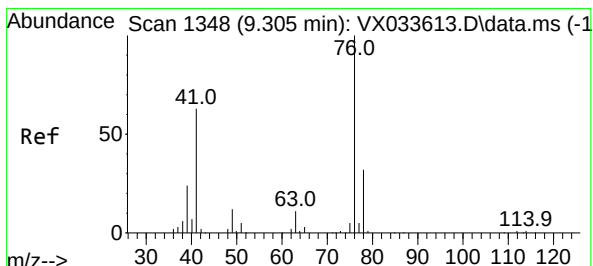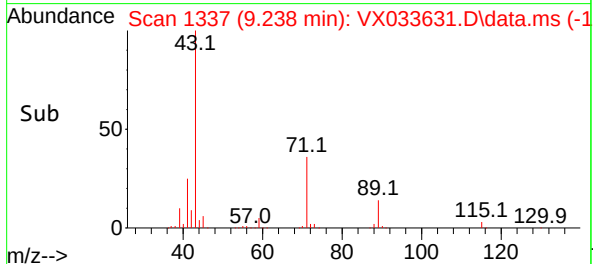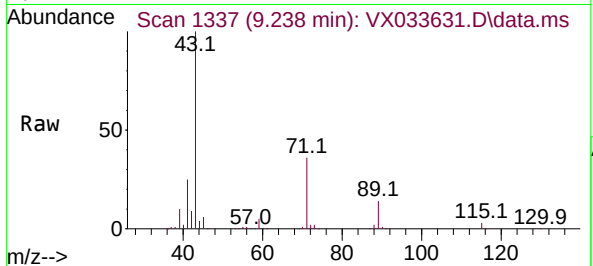

#57
1,3-Dichloropropane
Concen: 1.658 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.177 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion: 76 Resp: 4598
Ion Ratio Lower Upper
76 100
78 0.0 25.9 38.9#


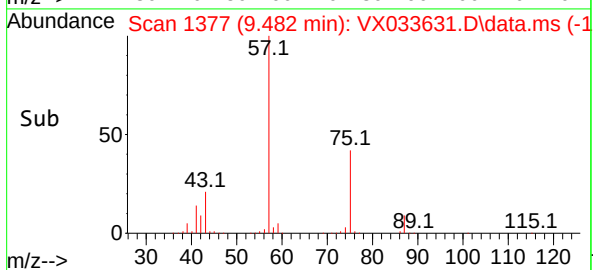

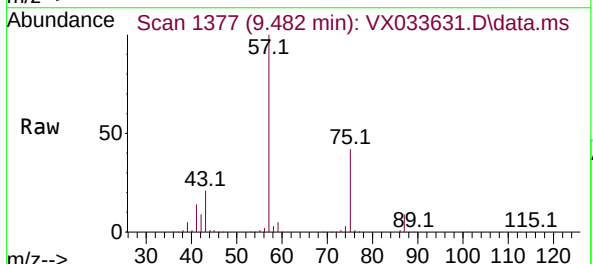




#59
2-Hexanone
Concen: 40.678 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.049 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion: 43 Resp: 70028
Ion Ratio Lower Upper
43 100
58 17.6 26.6 79.8#

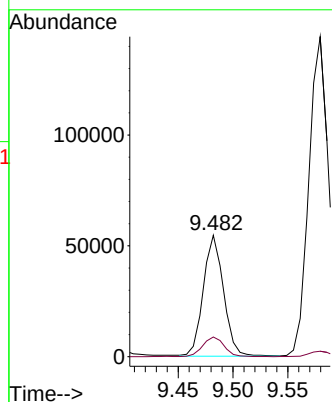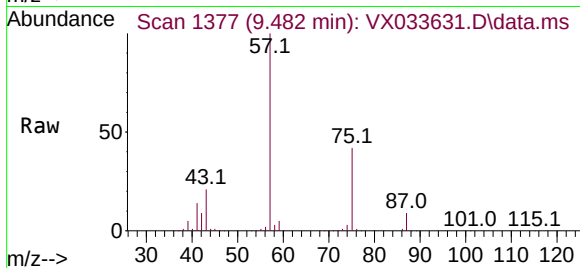

#62
4-Bromofluorobenzene
Concen: 50.036 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion: 95 Resp: 100782
Ion Ratio Lower Upper
95 100
174 89.7 0.0 180.4
176 86.8 0.0 176.2


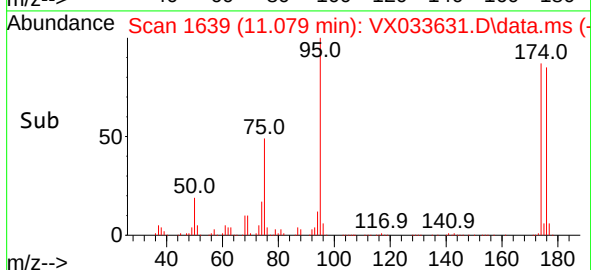

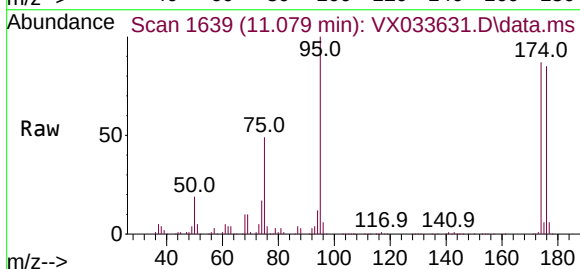




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion:117 Resp: 171675
Ion Ratio Lower Upper
117 100
82 53.6 42.2 63.2
119 31.9 26.2 39.4

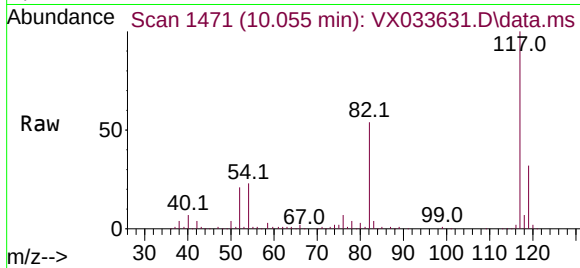

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion:152 Resp: 105097
Ion Ratio Lower Upper
152 100
115 54.9 38.5 115.5
150 155.2 0.0 340.4



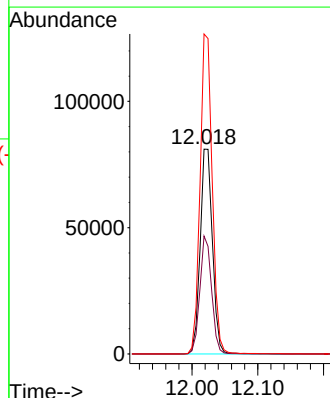
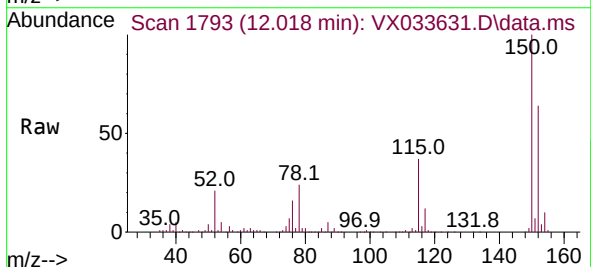


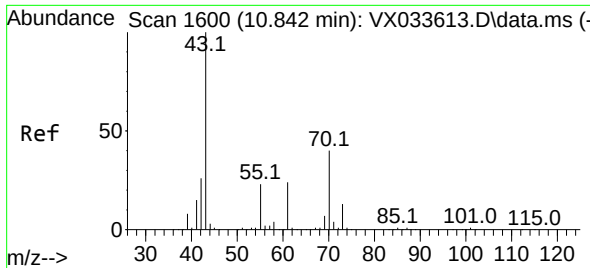

#74
N-amy1 acetate
Concen: 9.190 ug/l
RT: 10.640 min Scan# 1637
Delta R.T. -0.201 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion:	43	Resp:	27637
Ion	Ratio	Lower	Upper
43	100		
70	2.0	33.4	50.0#
55	4.3	18.6	27.8#
61	9.4	19.0	28.6#

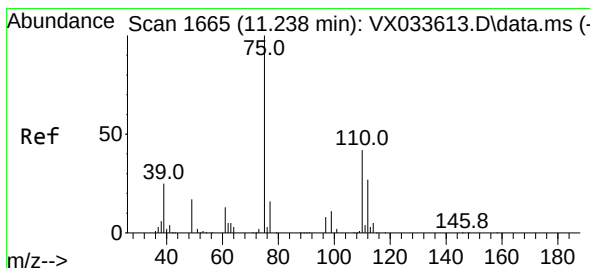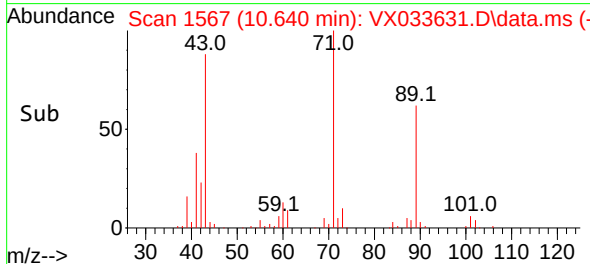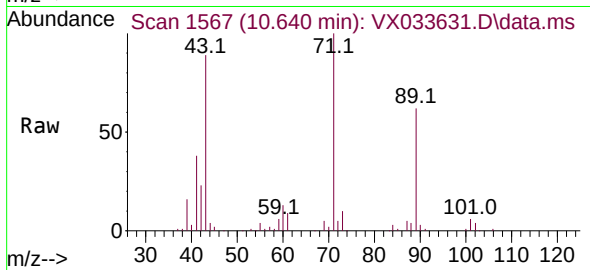

#76
1,2,3-Trichloropropane
Concen: 25.843 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion:	75	Resp:	49758
Ion	Ratio	Lower	Upper
75	100		
77	1.0	21.3	63.9#


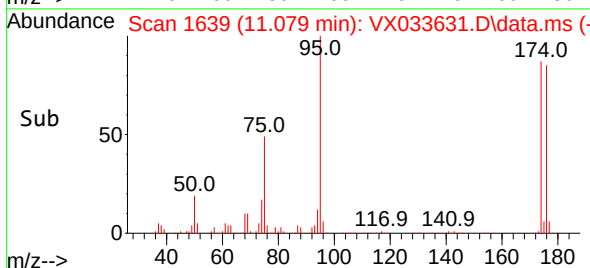

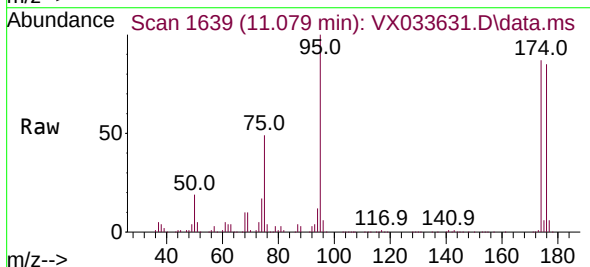




#81
trans-1,4-Dichloro-2-butene
Concen: 78.437 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25




Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08


Tgt Ion: 75 Resp: 49758
Ion Ratio Lower Upper
75 100
53 0.0 86.4 129.6#
89 0.0 37.4 56.2#

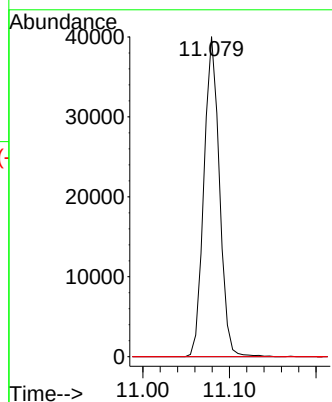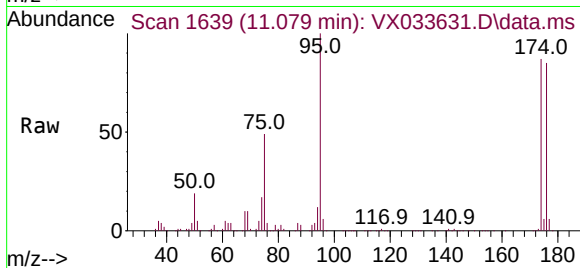

#93
1,2,4-Trichlorobenzene
Concen: 1.643 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25


Tgt Ion:180 Resp: 120
Ion Ratio Lower Upper
180 100
182 0.0 47.4 142.2#
145 0.0 14.1 42.2#

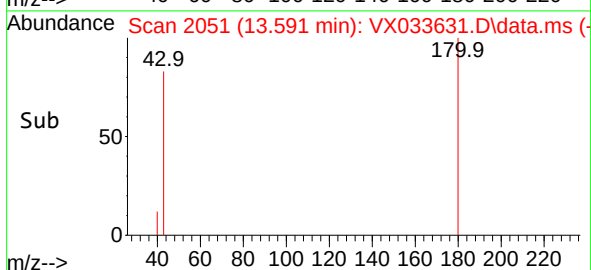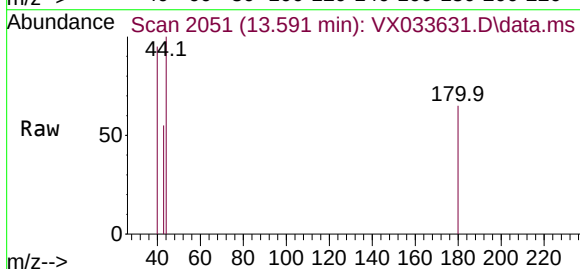






#95
Naphthalene
Concen: 3.148 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Instrument :
MSVOA_X
ClientSampleId :
PB050057ZHE#08

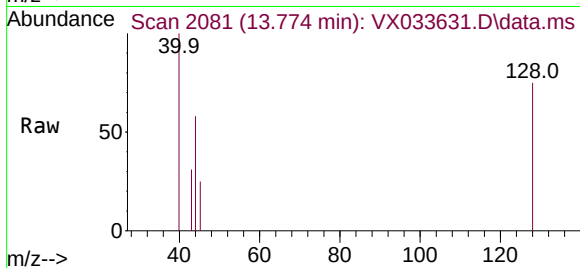

Tgt Ion:128 Resp: 238
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 0.0 9.0 13.4#



#96
1,2,3-Trichlorobenzene
Concen: 3.764 ug/l
RT: 13.957 min Scan# 2111
Delta R.T. -0.006 min
Lab File: VX033631.D
Acq: 06 Jan 2023 15:25

Tgt Ion:180 Resp: 40
Ion Ratio Lower Upper
180 100
182 75.0 47.2 141.6
145 0.0 15.0 45.0#

