

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
 Data File : VX033639.D
 Acq On : 06 Jan 2023 18:30
 Operator : JC/MD
 Sample : 01042-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WESTEND-SILICA-B

Quant Time: Jan 07 04:28:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 05 04:43:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	171059	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	251238	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	223564	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	110658	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	94361	48.865	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.740%
35) Dibromofluoromethane	5.385	113	77928	47.190	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.380%
50) Toluene-d8	8.647	98	289471	49.043	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.080%
62) 4-Bromofluorobenzene	11.079	95	105557	50.454	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.900%
Target Compounds						
					Qvalue	
8) Diethyl Ether	2.136	74	789	1.151	ug/l #	41
11) Tert butyl alcohol	3.032	59	1828	5.763	ug/l #	89
13) Acrolein	2.081	56	20	Below Cal	#	71
16) Acetone	2.404	43	7110	Below Cal		94
17) Carbon Disulfide	2.514	76	147	1.661	ug/l #	74
18) Methyl Acetate	2.709	43	1367	0.511	ug/l #	79
20) Methylene Chloride	2.788	84	320	Below Cal		98
25) 2-Butanone	4.587	43	6675	5.294	ug/l #	84
31) Cyclohexane	5.458	56	766	0.285	ug/l #	51
36) 1,1-Dichloropropene	5.550	75	11659	5.212	ug/l #	50
37) Ethyl Acetate	4.715	43	1747	Below Cal	#	76
38) Carbon Tetrachloride	5.556	117	15766	6.660	ug/l #	15
39) Methylcyclohexane	7.379	83	875	0.313	ug/l	90
40) Benzene	6.038	78	57735	8.831	ug/l	99
43) Isopropyl Acetate	6.342	43	7316	1.913	ug/l #	94
48) Methyl methacrylate	7.800	41	762	0.394	ug/l #	27
52) Toluene	8.720	92	64936	15.107	ug/l	99
53) t-1,3-Dichloropropene	8.903	75	426	0.289	ug/l #	43
59) 2-Hexanone	9.439	43	938	0.525	ug/l	96
67) Ethyl Benzene	10.195	91	6888	0.863	ug/l	98
68) m/p-Xylenes	10.299	106	18241	5.853	ug/l	99
69) o-Xylene	10.640	106	6010	1.945	ug/l	94
75) 1,1,2,2-Tetrachloroethane	11.281	83	582	0.239	ug/l #	26
76) 1,2,3-Trichloropropane	11.079	75	51988	25.644	ug/l #	35
80) 1,3,5-Trimethylbenzene	11.451	105	5480	0.852	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	51988	77.834	ug/l #	7
83) tert-Butylbenzene	11.750	119	1514	0.226	ug/l #	64
84) 1,2,4-Trimethylbenzene	11.750	105	12295	1.904	ug/l	97
95) Naphthalene	13.774	128	1209	3.263	ug/l #	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
Data File : VX033639.D
Acq On : 06 Jan 2023 18:30
Operator : JC/MD
Sample : 01042-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B

Quant Time: Jan 07 04:28:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 05 04:43:25 2023
Response via : Initial Calibration

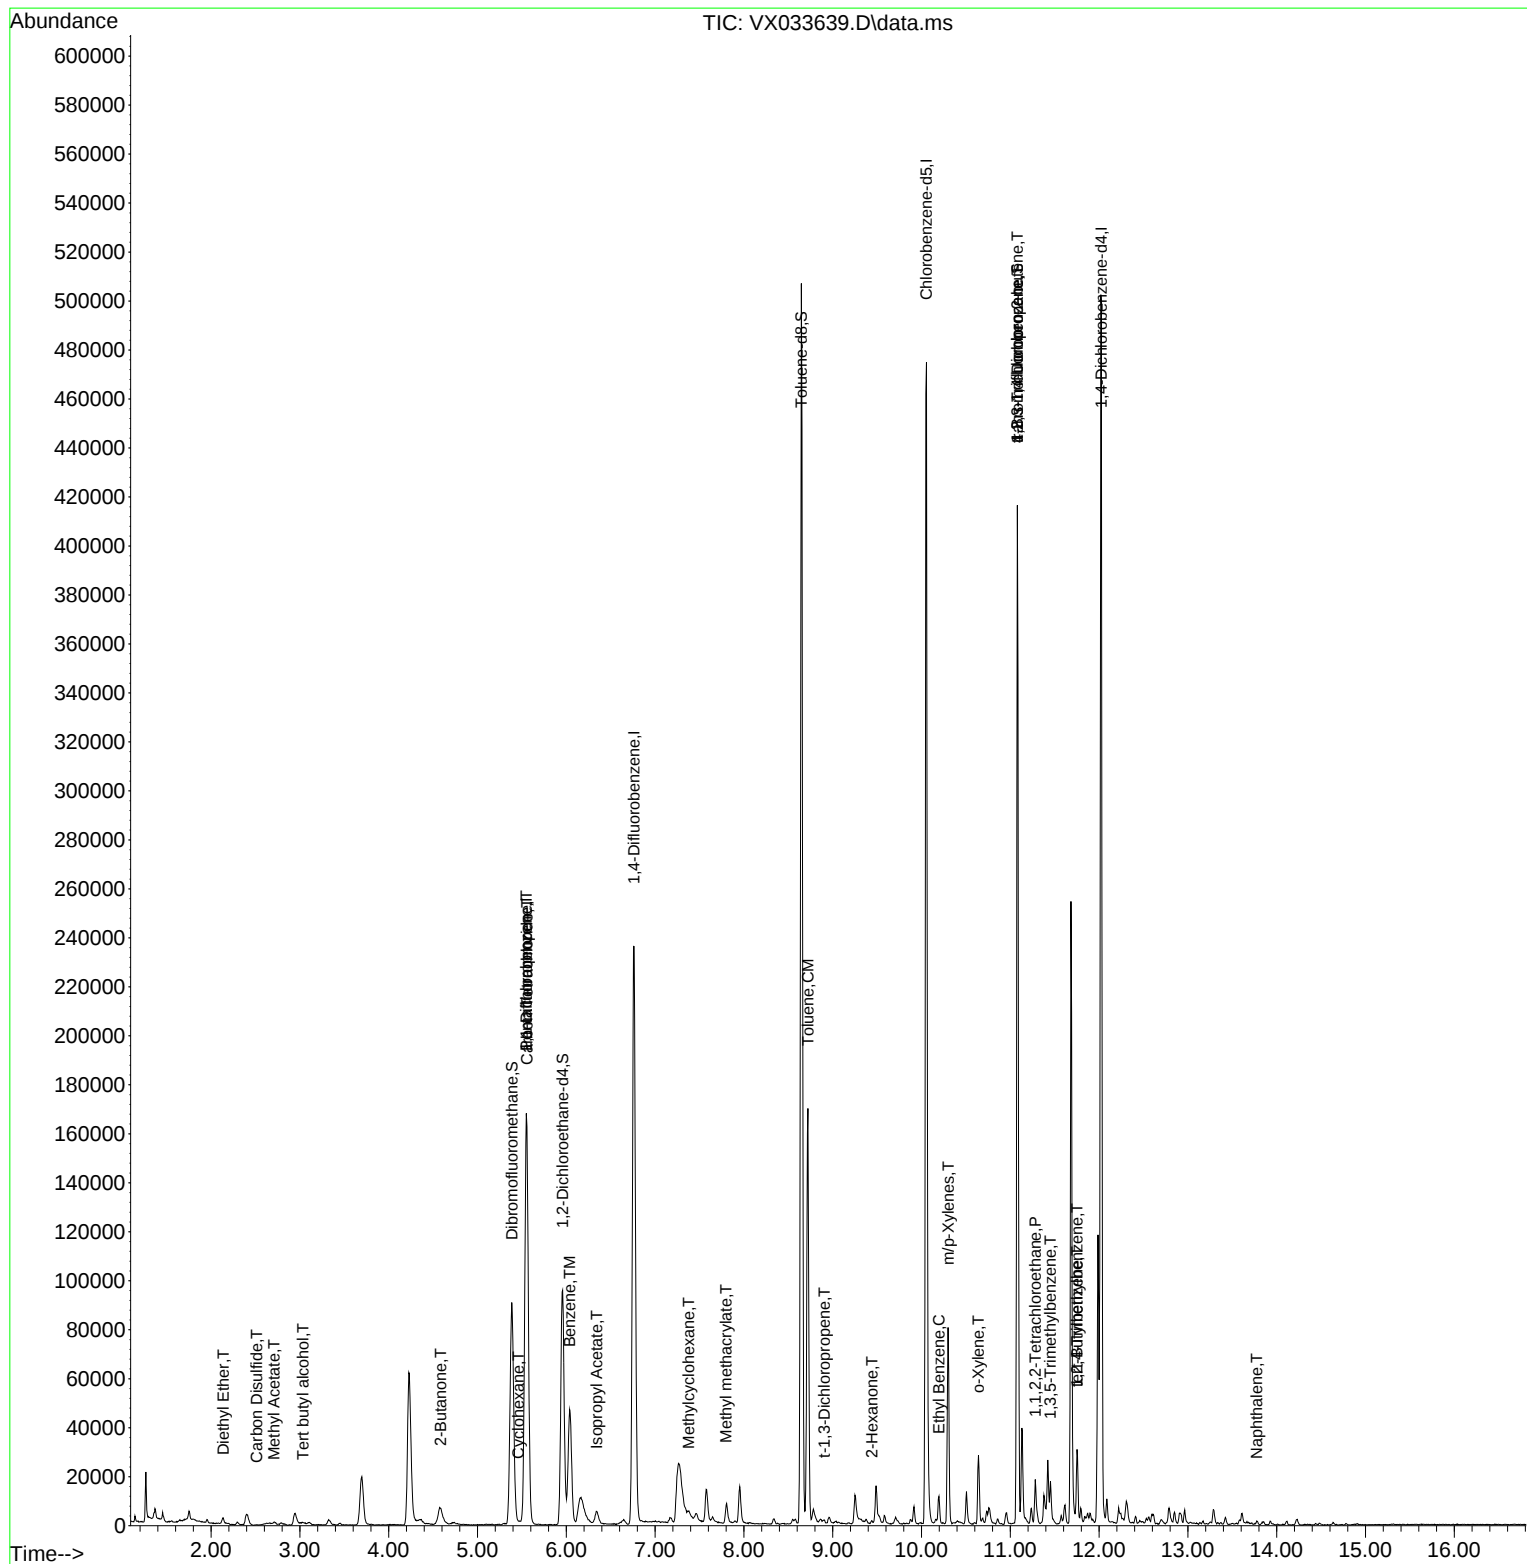



#1
Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.000 min

Lab File: VX033639.D

Acq: 06 Jan 2023 18:30

Instrument :

MSVOA_X

ClientSampleId :





WESTEND-SILICA-B

Tgt Ion:168 Resp: 171059

Ion Ratio Lower Upper

168 100

99 51.4 41.4 62.2

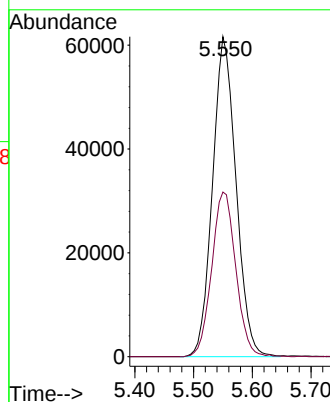

#8

Diethyl Ether

Concen: 1.151 ug/l

RT: 2.136 min Scan# 172

Delta R.T. 0.006 min

Lab File: VX033639.D




Acq: 06 Jan 2023 18:30


Tgt Ion: 74 Resp: 789

Ion Ratio Lower Upper

74 100

45 158.9 50.1 150.4#

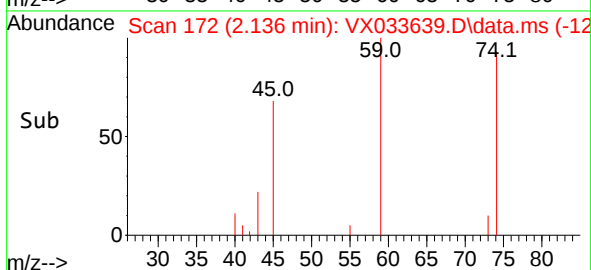

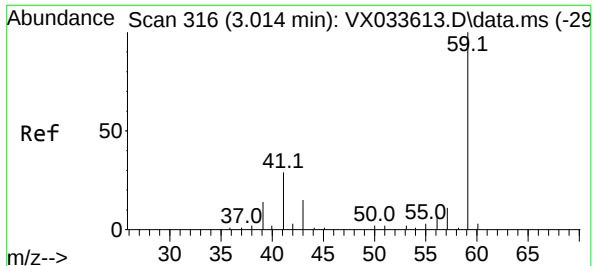

#11

Tert butyl alcohol

Concen: 5.763 ug/l

RT: 3.032 min Scan# 316

Delta R.T. 0.018 min

Lab File: VX033639.D

Acq: 06 Jan 2023 18:30

Instrument :

MSVOA_X

ClientSampleId :





WESTEND-SILICA-B

Tgt Ion: 59 Resp: 1828

Ion Ratio Lower Upper

59 100

57 3.2 5.5 8.3#

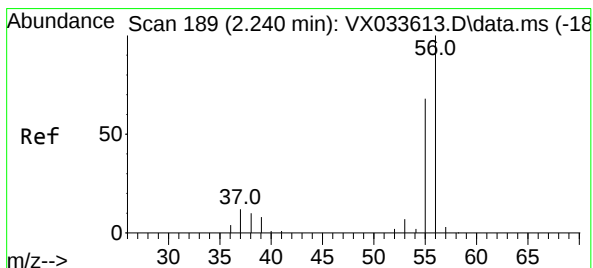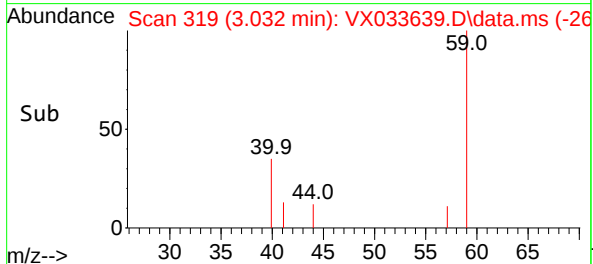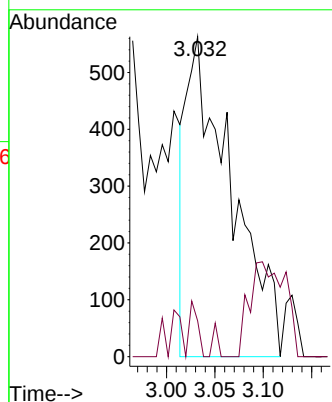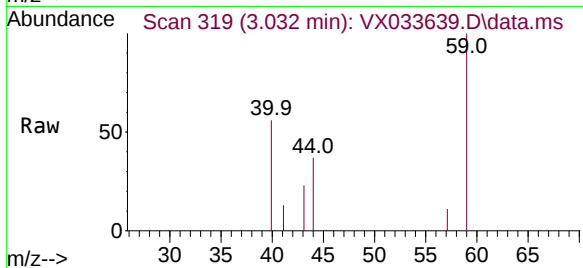

#13

Acrolein

Concen: Below Cal

RT: 2.081 min Scan# 163

Delta R.T. -0.159 min

Lab File: VX033639.D




Acq: 06 Jan 2023 18:30


Tgt Ion: 56 Resp: 20

Ion Ratio Lower Upper

56 100

55 95.0 56.9 85.3#


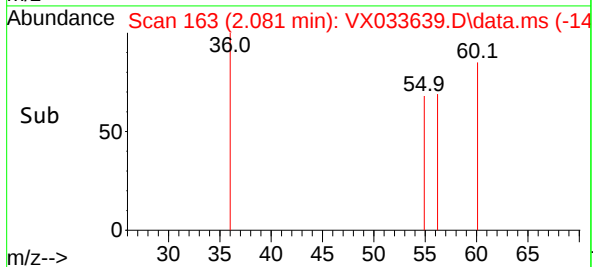

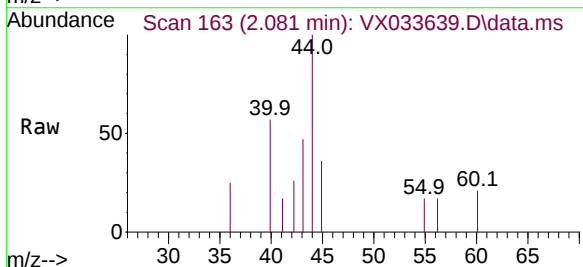




#16
Acetone
Concen: Below Cal
RT: 2.404 min Scan# 215
Delta R.T. 0.006 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion: 43 Resp: 7110
Ion Ratio Lower Upper
43 100
58 25.6 22.9 34.3

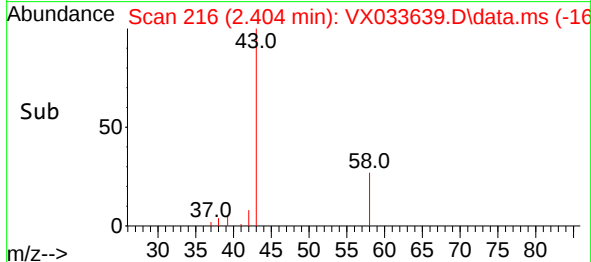

#17
Carbon Disulfide
Concen: 1.661 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion: 76 Resp: 147
Ion Ratio Lower Upper
76 100
78 0.0 7.6 11.4#




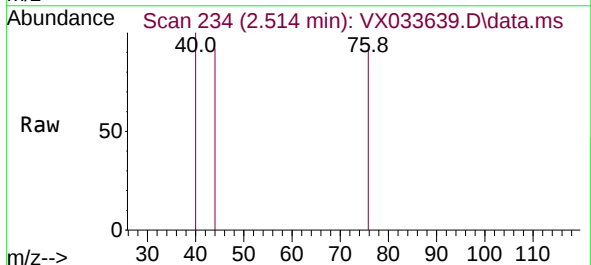




#18
Methyl Acetate
Concen: 0.511 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion: 43 Resp: 1367
Ion Ratio Lower Upper
43 100
74 12.4 17.9 26.9#



#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion: 84 Resp: 320
Ion Ratio Lower Upper
84 100
49 123.2 97.6 146.4
51 37.3 30.4 45.6
86 64.4 49.7 74.5

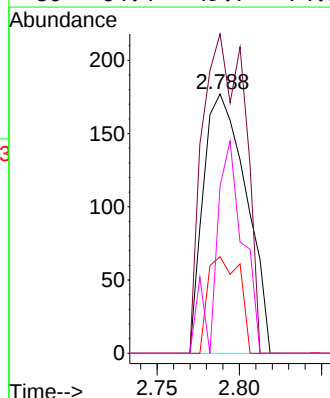



#25

2-Butanone

Concen: 5.294 ug/l

RT: 4.587 min Scan# 51

Delta R.T. 0.024 min

Lab File: VX033639.D

Acq: 06 Jan 2023 18:30

Instrument :

MSVOA_X

ClientSampleId :





WESTEND-SILICA-B

Tgt Ion: 43 Resp: 6675

Ion Ratio Lower Upper

43 100

72 32.8 19.8 29.6#

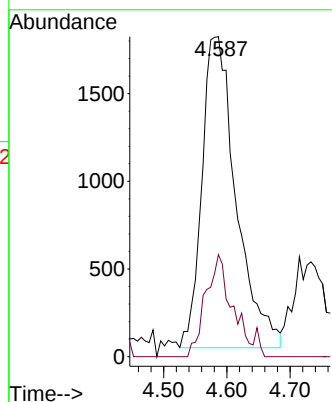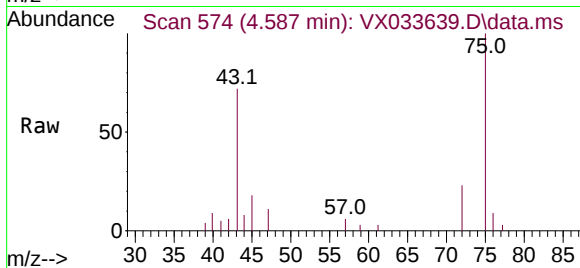

#31

Cyclohexane

Concen: 0.285 ug/l

RT: 5.458 min Scan# 717

Delta R.T. -0.012 min

Lab File: VX033639.D

Acq: 06 Jan 2023 18:30




Tgt Ion: 56 Resp: 766


Ion Ratio Lower Upper

56 100

69 0.0 24.6 36.8#

84 46.4 72.2 108.2#




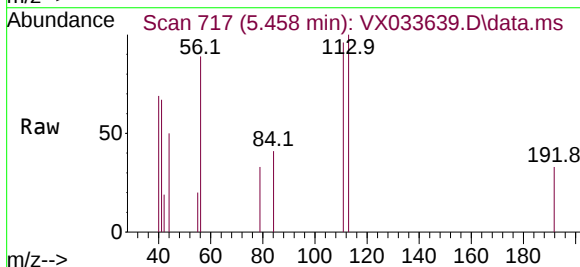




#33
 1,2-Dichloroethane-d4
 Concen: 48.865 ug/l
 RT: 5.958 min Scan# 798
 Delta R.T. 0.006 min
 Lab File: VX033639.D
 Acq: 06 Jan 2023 18:30




Instrument :
 MSVOA_X
 ClientSampleId :
 WESTEND-SILICA-B


Tgt Ion: 65 Resp: 94361
 Ion Ratio Lower Upper
 65 100
 67 51.6 0.0 104.8



#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. 0.000 min
 Lab File: VX033639.D
 Acq: 06 Jan 2023 18:30

Tgt Ion: 114 Resp: 251238
 Ion Ratio Lower Upper
 114 100
 63 19.0 0.0 40.0
 88 14.6 0.0 29.6

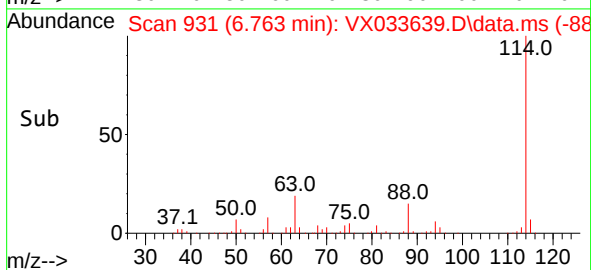

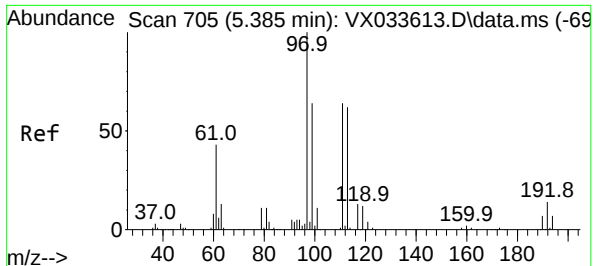

#35

Dibromofluoromethane

Concen: 47.190 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX033639.D

Acq: 06 Jan 2023 18:30

Instrument :

MSVOA_X

ClientSampleId :

WESTEND-SILICA-B





Tgt Ion:113 Resp: 77928

Ion Ratio Lower Upper

113 100

111 103.0 81.2 121.8

192 23.6 18.2 27.2

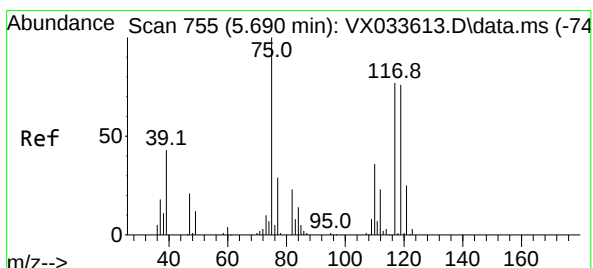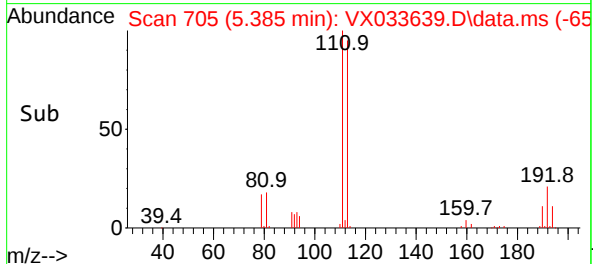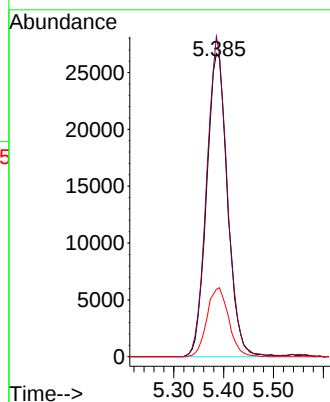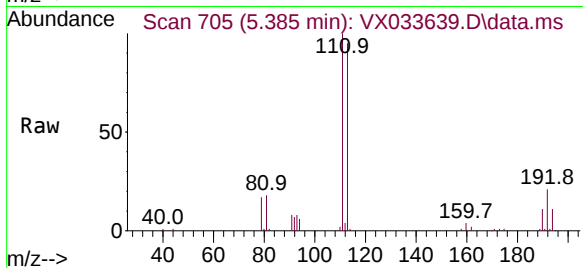

#36

1,1-Dichloropropene

Concen: 5.212 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.140 min

Lab File: VX033639.D

Acq: 06 Jan 2023 18:30




Tgt Ion: 75 Resp: 11659


Ion Ratio Lower Upper

75 100

110 9.3 18.0 54.0#

77 0.0 24.5 36.7#

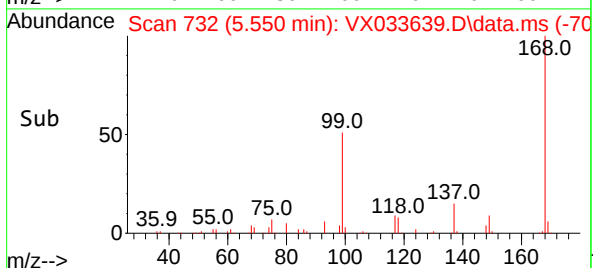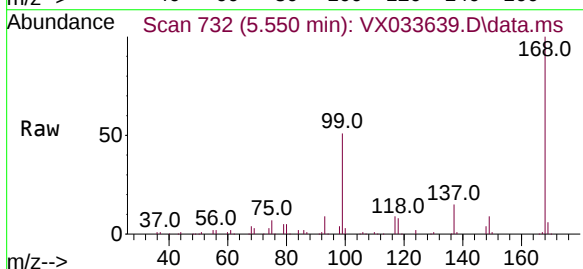

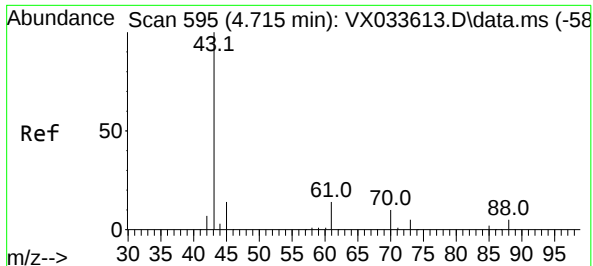

#37

Ethyl Acetate

Concen: Below Cal

RT: 4.715 min Scan# 595

Delta R.T. -0.000 min

Lab File: VX033639.D

Acq: 06 Jan 2023 18:30

Instrument :

MSVOA_X

ClientSampleId :

WESTEND-SILICA-B





Tgt Ion: 43 Resp: 1747

Ion Ratio Lower Upper

43 100

61 2.6 10.6 16.0#

70 2.3 8.1 12.1#

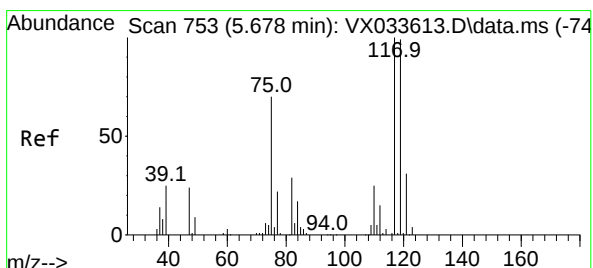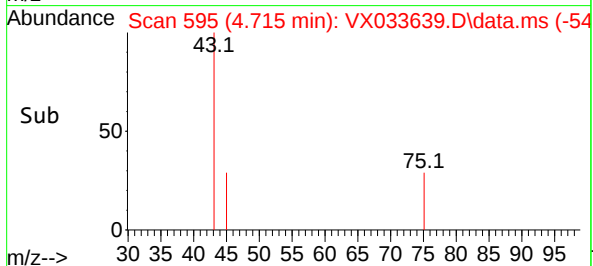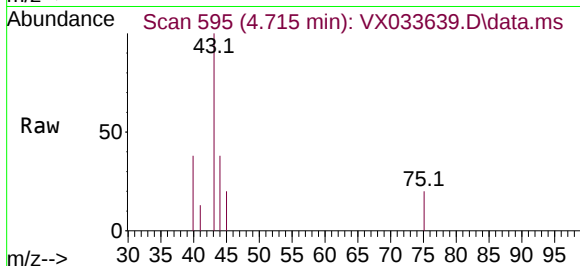

#38

Carbon Tetrachloride

Concen: 6.660 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.122 min

Lab File: VX033639.D

Acq: 06 Jan 2023 18:30




Tgt Ion: 117 Resp: 15766


Ion Ratio Lower Upper

117 100

119 5.2 78.8 118.2#

121 0.0 24.9 37.3#


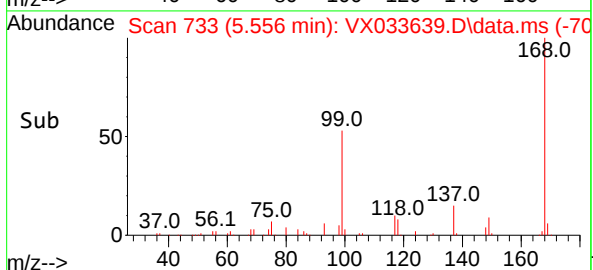

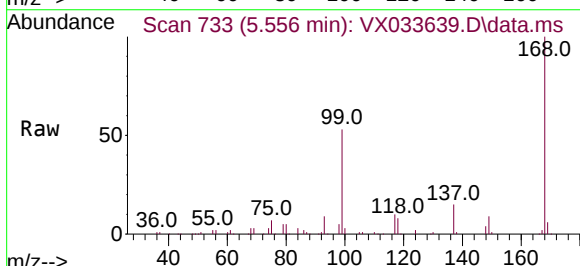




#39
Methylcyclohexane
Concen: 0.313 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion: 83	Resp:	875	
Ion	Ratio	Lower	Upper
83	100		
55	88.2	61.4	92.2
98	46.6	40.2	60.2

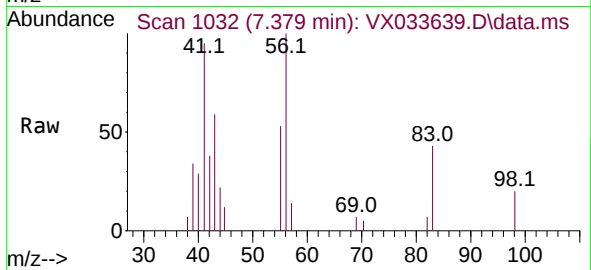

#40
Benzene
Concen: 8.831 ug/l
RT: 6.038 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion: 78	Resp: 57735
Ion Ratio	Lower Upper
78 100	
77 24.3	19.0 28.6


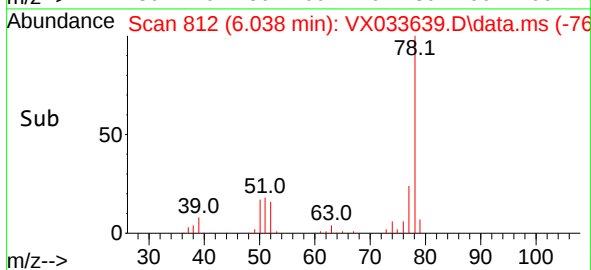






#43
Isopropyl Acetate
Concen: 1.913 ug/l
RT: 6.342 min Scan# 81
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion: 43 Resp: 7316
Ion Ratio Lower Upper
43 100
61 17.1 15.2 22.8
87 9.6 10.6 16.0#

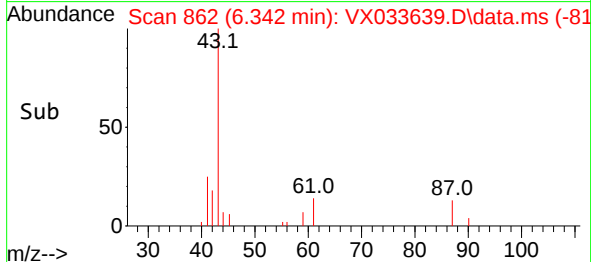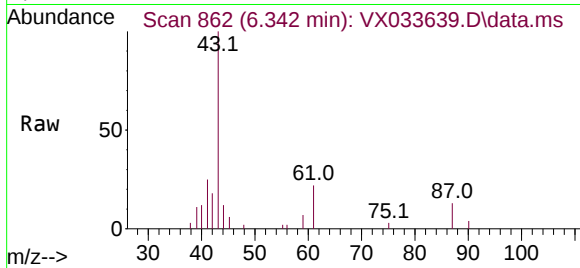

#48
Methyl methacrylate
Concen: 0.394 ug/l
RT: 7.800 min Scan# 1101
Delta R.T. 0.110 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion: 41 Resp: 762
Ion Ratio Lower Upper
41 100
69 0.0 63.1 94.7#
39 91.9 44.8 67.2#




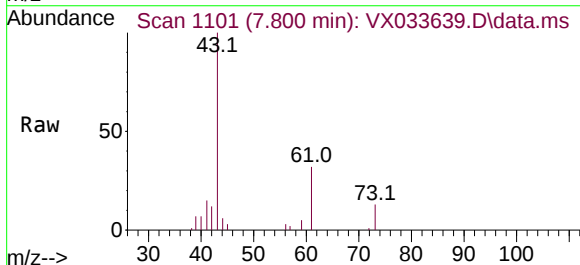




#50
Toluene-d8
Concen: 49.043 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion: 98 Resp: 289471
Ion Ratio Lower Upper
98 100
100 67.1 53.6 80.4



#52
Toluene
Concen: 15.107 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion: 92 Resp: 64936
Ion Ratio Lower Upper
92 100
91 168.3 135.4 203.2

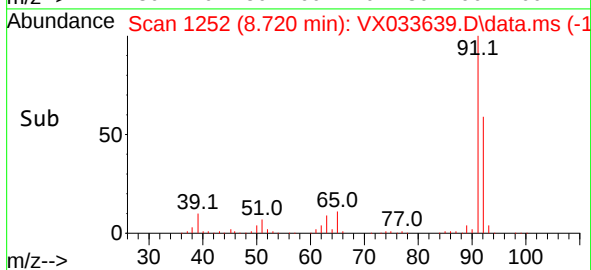

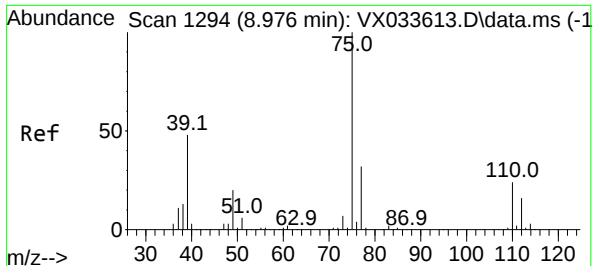

#53

t-1,3-Dichloropropene

Concen: 0.289 ug/l

RT: 8.903 min Scan# 11

Delta R.T. -0.073 min

Lab File: VX033639.D

Acq: 06 Jan 2023 18:30

Instrument :

MSVOA_X

ClientSampleId :





WESTEND-SILICA-B

Tgt Ion: 75 Resp: 426

Ion Ratio Lower Upper

75 100

77 0.0 25.3 37.9#

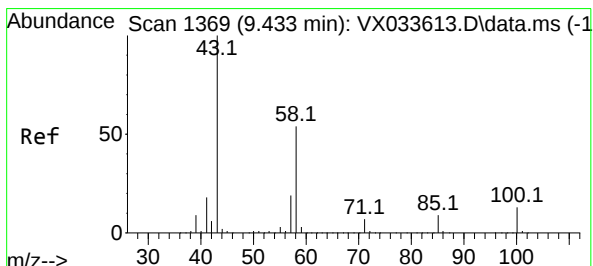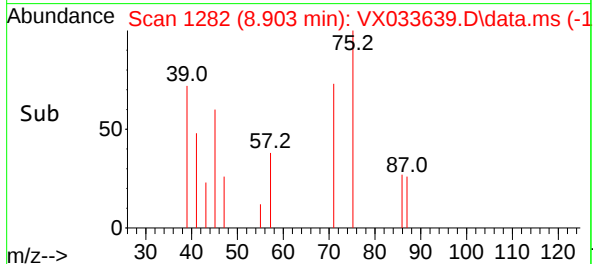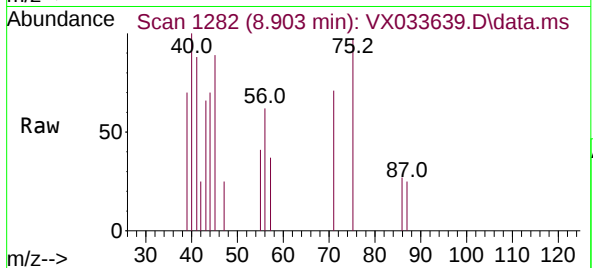

#59

2-Hexanone

Concen: 0.525 ug/l

RT: 9.439 min Scan# 1370

Delta R.T. 0.006 min

Lab File: VX033639.D




Acq: 06 Jan 2023 18:30


Tgt Ion: 43 Resp: 938

Ion Ratio Lower Upper

43 100

58 50.2 26.6 79.8


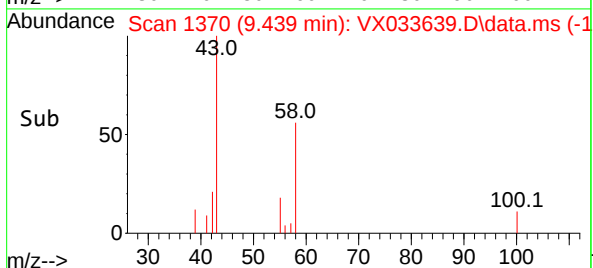
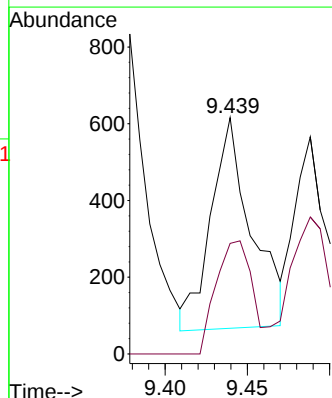
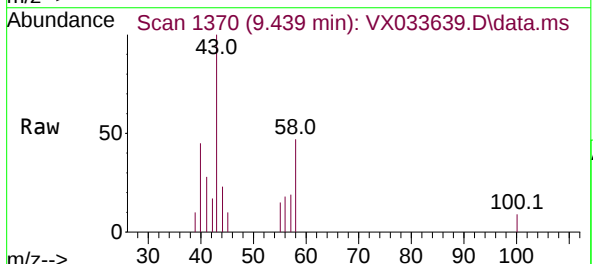




#62
4-Bromofluorobenzene
Concen: 50.454 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion: 95 Resp: 105557
Ion Ratio Lower Upper
95 100
174 88.9 0.0 180.4
176 85.4 0.0 176.2



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion: 117 Resp: 223564
Ion Ratio Lower Upper
117 100
82 52.6 42.2 63.2
119 33.2 26.2 39.4


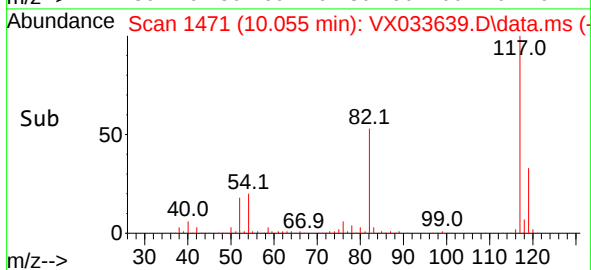






#67
Ethyl Benzene
Concen: 0.863 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion: 91 Resp: 6888
Ion Ratio Lower Upper
91 100
106 31.4 25.9 38.9



#68
m/p-Xylenes
Concen: 5.853 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion: 106 Resp: 18241
Ion Ratio Lower Upper
106 100
91 201.6 159.6 239.4


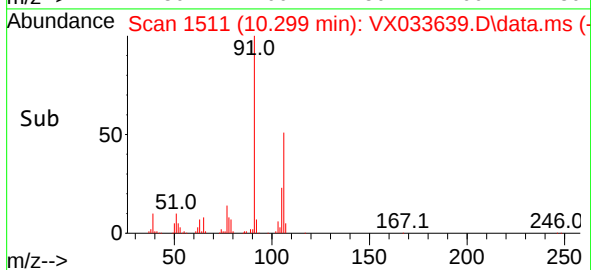






#69
o-Xylene
Concen: 1.945 ug/l
RT: 10.640 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion:106 Resp: 6010
Ion Ratio Lower Upper
106 100
91 217.9 104.1 312.3

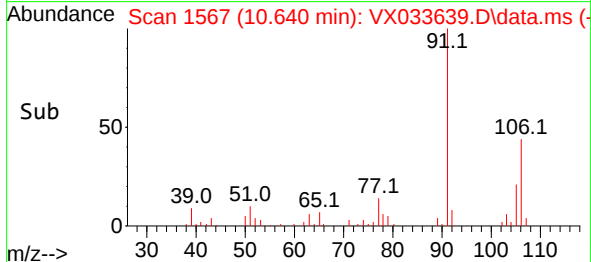

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion:152 Resp: 110658
Ion Ratio Lower Upper
152 100
115 55.5 38.5 115.5
150 156.5 0.0 340.4




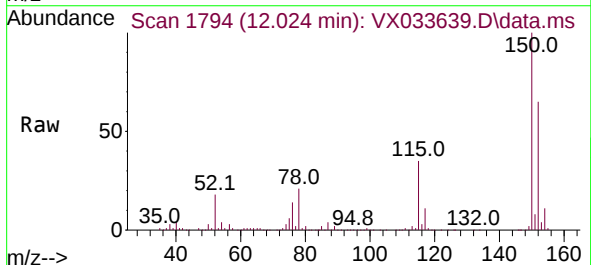




#75
1,1,2-Tetrachloroethane
Concen: 0.239 ug/l
RT: 11.281 min Scan# 1672
Delta R.T. 0.067 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion: 83 Resp: 582
Ion Ratio Lower Upper
83 100
131 0.0 5.5 16.5#
85 0.0 32.1 96.5#

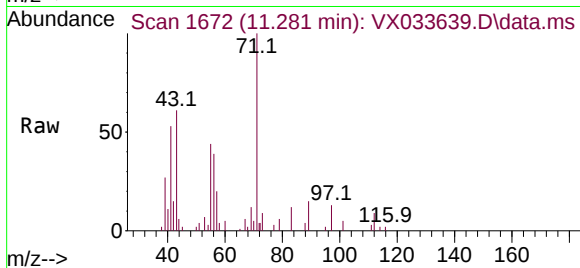

#76
1,2,3-Trichloropropane
Concen: 25.644 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion: 75 Resp: 51988
Ion Ratio Lower Upper
75 100
77 1.0 21.3 63.9#




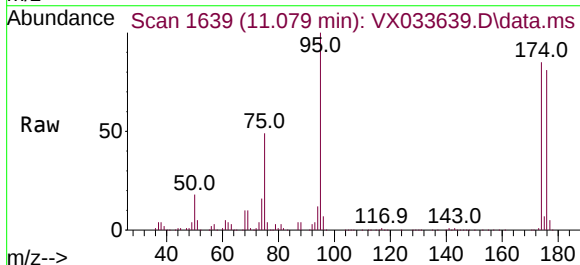




#80
1,3,5-Trimethylbenzene
Concen: 0.852 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion:105 Resp: 5480
Ion Ratio Lower Upper
105 100
120 51.4 25.5 76.5

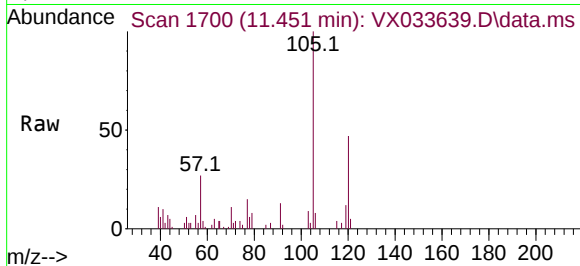

#81
trans-1,4-Dichloro-2-butene
Concen: 77.834 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion: 75 Resp: 51988
Ion Ratio Lower Upper
75 100
53 0.0 86.4 129.6#
89 0.0 37.4 56.2#




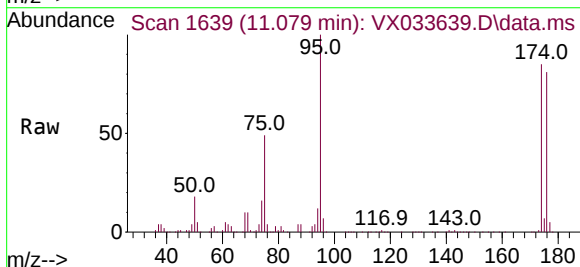




#83
tert-Butylbenzene
Concen: 0.226 ug/l
RT: 11.750 min Scan# 11
Delta R.T. 0.037 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30




Instrument :
MSVOA_X
ClientSampleId :
WESTEND-SILICA-B


Tgt Ion:119 Resp: 1514
Ion Ratio Lower Upper
119 100
91 78.1 27.9 83.6
134 0.0 12.2 36.6#

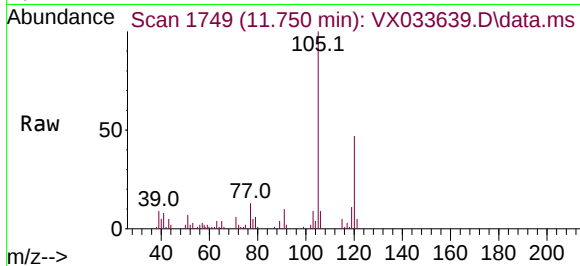

#84
1,2,4-Trimethylbenzene
Concen: 1.904 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VX033639.D
Acq: 06 Jan 2023 18:30

Tgt Ion:105 Resp: 12295
Ion Ratio Lower Upper
105 100
120 44.8 23.4 70.0

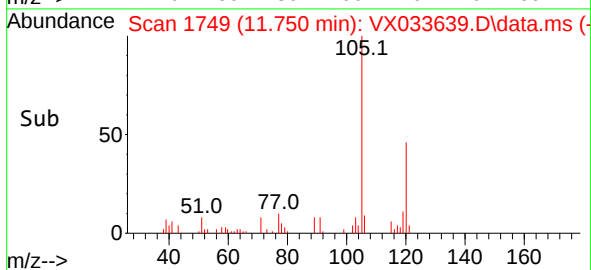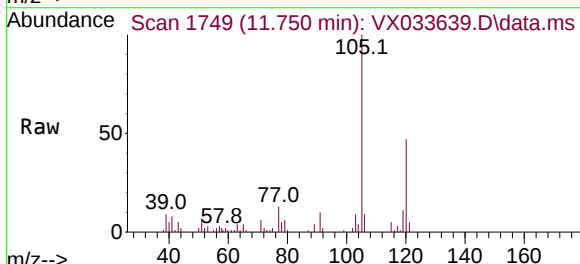



#95

Naphthalene

Concen: 3.263 ug/l

RT: 13.774 min Scan# 20

Delta R.T. 0.000 min

Lab File: VX033639.D


Acq: 06 Jan 2023 18:30

Instrument :

MSVOA_X

ClientSampleId :

WESTEND-SILICA-B

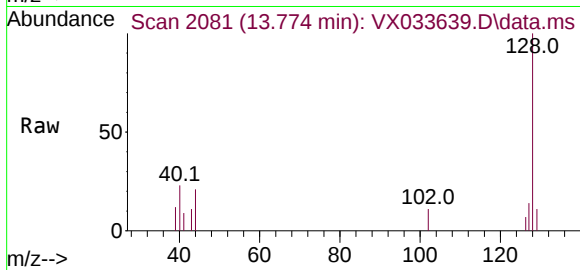

Tgt Ion:	128	Resp:	1209
Ion	Ratio	Lower	Upper
128	100		
127	12.7	10.3	15.5
129	8.6	9.0	13.4#

