

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
 Data File : VX033640.D
 Acq On : 06 Jan 2023 18:53
 Operator : JC/MD
 Sample : 01042-03 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 KEARNYGEN-SILICA

Quant Time: Jan 07 04:29:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 05 04:43:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	168226	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	245932	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	153262	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	107617	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	92778	48.855	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	97.700%		
35) Dibromofluoromethane	5.385	113	77767	48.109	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.220%		
50) Toluene-d8	8.647	98	283638	49.092	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	98.180%		
62) 4-Bromofluorobenzene	11.079	95	101790	49.703	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	99.400%		
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	3.026	59	80	0.256	ug/l #	80
13) Acrolein	2.343	56	447	Below Cal		89
14) Allyl chloride	2.782	41	944	0.360	ug/l #	73
16) Acetone	2.410	43	2555	Below Cal		97
17) Carbon Disulfide	2.520	76	84	1.645	ug/l #	74
18) Methyl Acetate	2.703	43	543	0.206	ug/l #	53
20) Methylene Chloride	2.788	84	411	Below Cal	#	73
22) Diisopropyl ether	3.697	45	7825	1.480	ug/l #	1
23) Vinyl Acetate	3.684	43	880	0.217	ug/l #	72
25) 2-Butanone	4.587	43	1303	1.051	ug/l #	87
31) Cyclohexane	5.477	56	6151	2.327	ug/l #	87
36) 1,1-Dichloropropene	5.550	75	11582	5.289	ug/l #	50
37) Ethyl Acetate	4.733	43	1788	Below Cal	#	73
38) Carbon Tetrachloride	5.550	117	15631	6.746	ug/l #	15
39) Methylcyclohexane	7.385	83	6157	2.252	ug/l	96
40) Benzene	6.038	78	134035	20.944	ug/l	100
43) Isopropyl Acetate	6.348	43	1050	0.280	ug/l #	65
51) 4-Methyl-2-Pentanone	8.549	43	785	0.331	ug/l #	37
52) Toluene	8.720	92	53571	12.732	ug/l	99
53) t-1,3-Dichloropropene	8.714	75	626	0.373	ug/l #	1
59) 2-Hexanone	9.488	43	356	0.203	ug/l	64
67) Ethyl Benzene	10.195	91	4293	0.784	ug/l	97
68) m/p-Xylenes	10.299	106	6701	3.136	ug/l	100
69) o-Xylene	10.640	106	2841	1.341	ug/l	97
76) 1,2,3-Trichloropropane	11.079	75	50467	25.597	ug/l #	35
81) trans-1,4-Dichloro-2-b...	11.079	75	50467	77.692	ug/l #	7
84) 1,2,4-Trimethylbenzene	11.750	105	2476	0.394	ug/l	89
93) 1,2,4-Trichlorobenzene	13.597	180	58	1.617	ug/l #	12
95) Naphthalene	13.780	128	2060	3.373	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
Data File : VX033640.D
Acq On : 06 Jan 2023 18:53
Operator : JC/MD
Sample : 01042-03 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KEARNYGEN-SILICA

Quant Time: Jan 07 04:29:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 05 04:43:25 2023
Response via : Initial Calibration




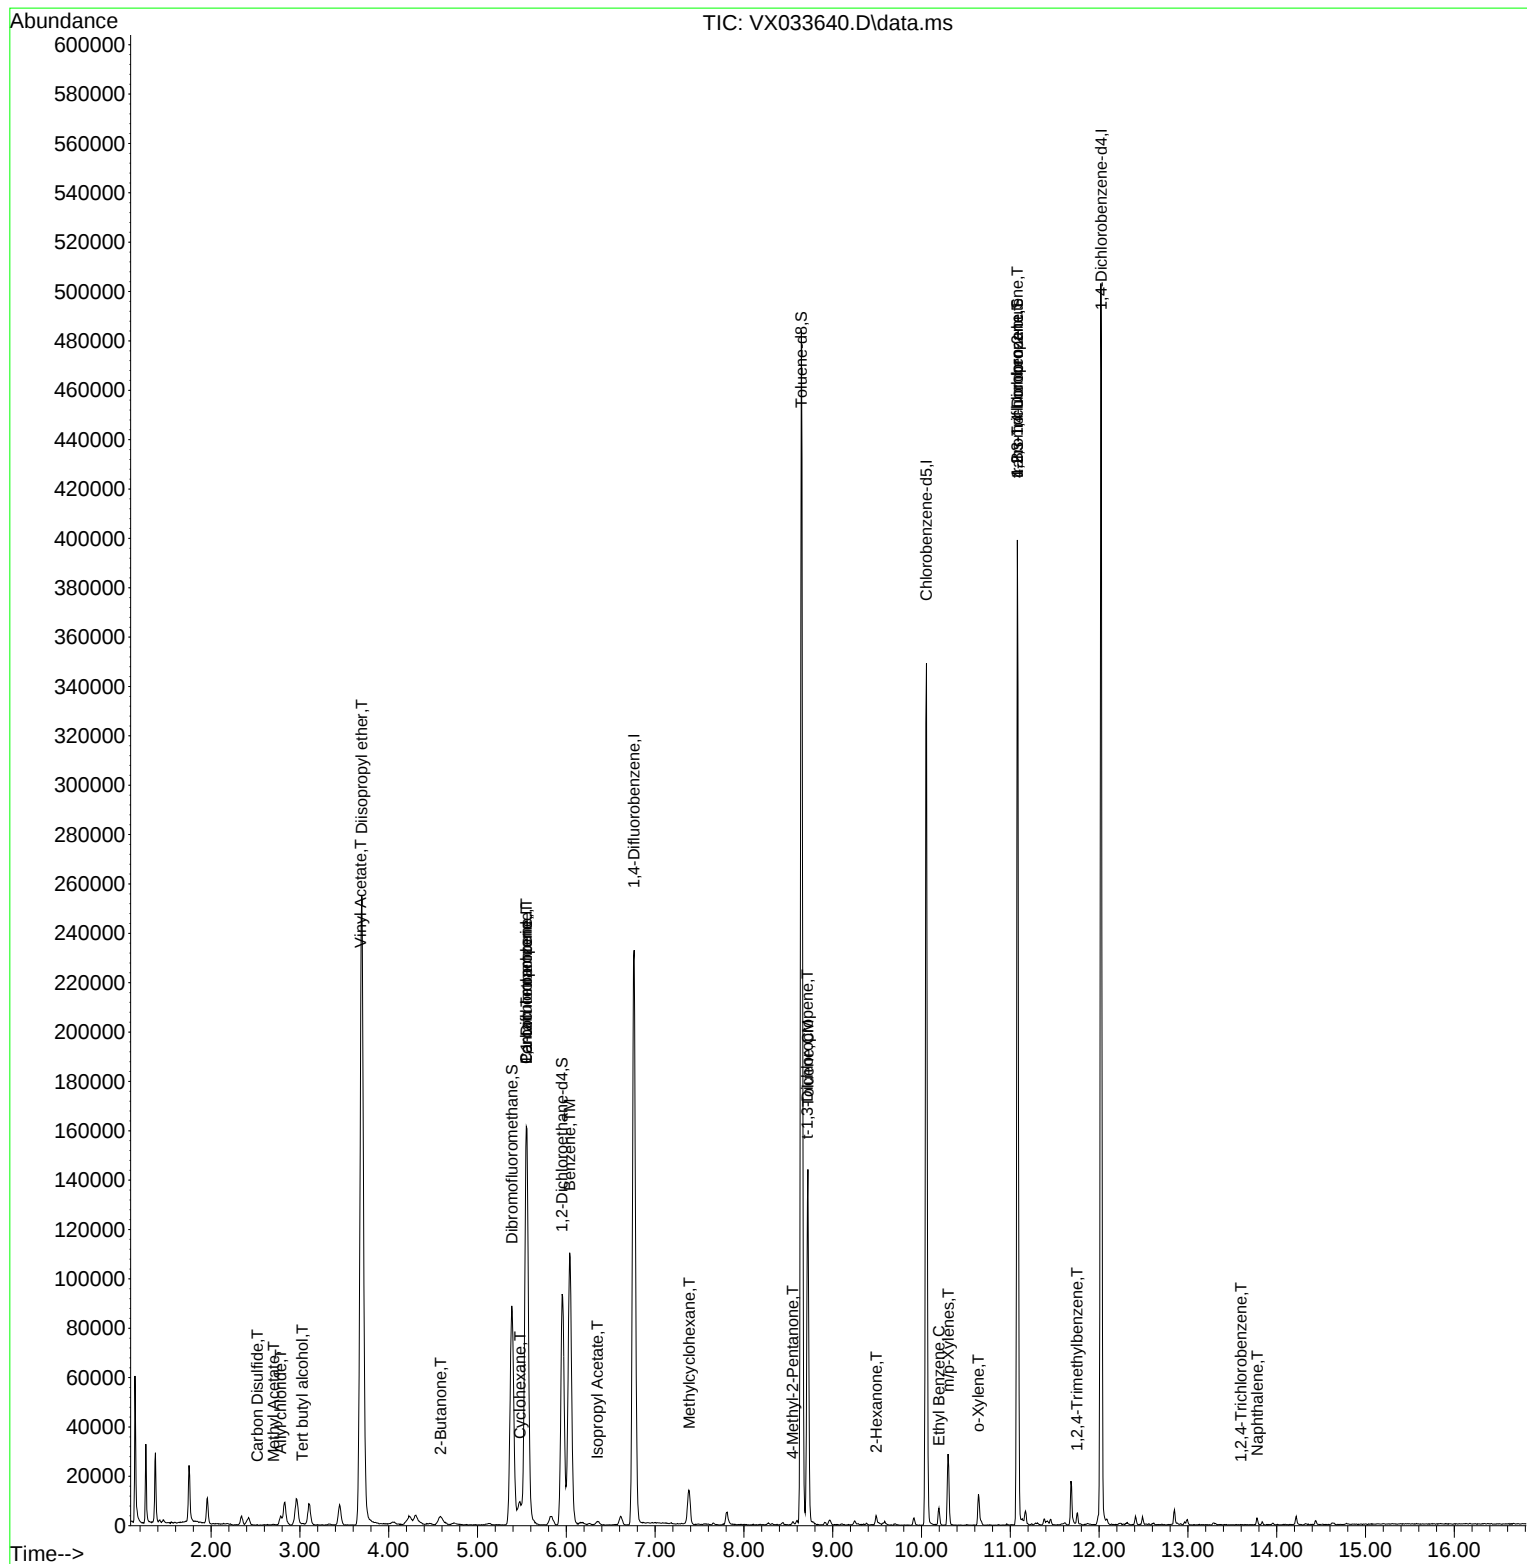


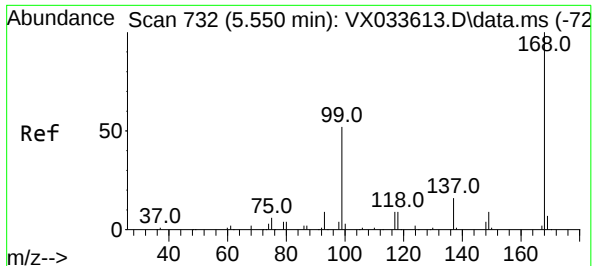

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53



Instrument :
MSVOA_X
ClientSampleId :
KEARNYGEN-SILICA


Tgt Ion:168 Resp: 168226
Ion Ratio Lower Upper
168 100
99 51.6 41.4 62.2

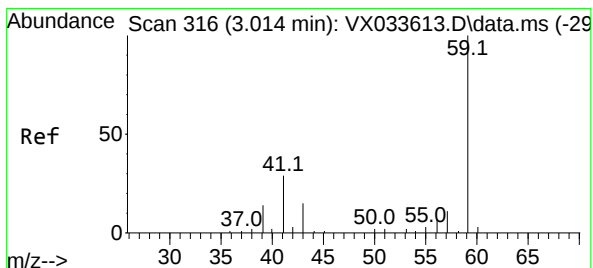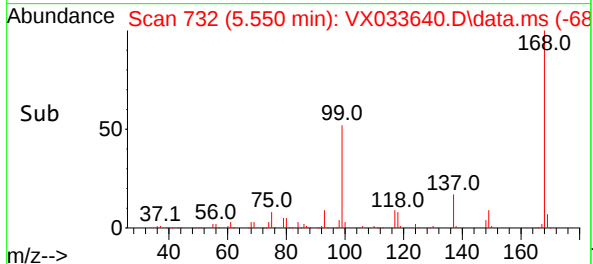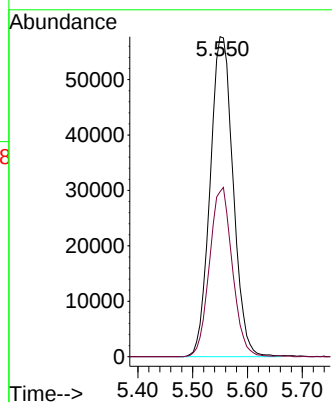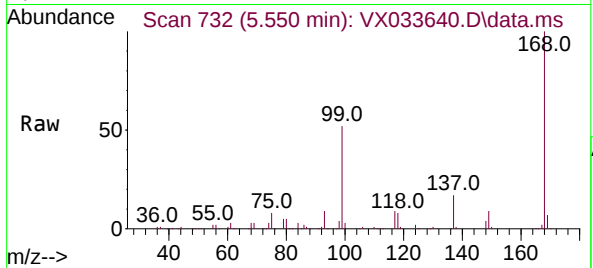

#11
Tert butyl alcohol
Concen: 0.256 ug/l
RT: 3.026 min Scan# 318
Delta R.T. 0.012 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53

Tgt Ion: 59 Resp: 80
Ion Ratio Lower Upper
59 100
57 0.0 5.5 8.3#

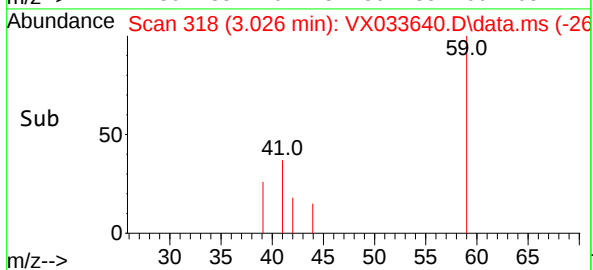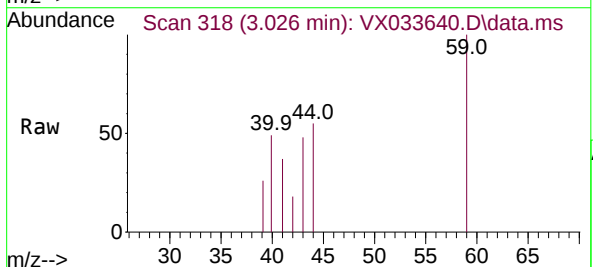



#13

Acrolein

Concen: Below Cal

RT: 2.343 min Scan# 206

Delta R.T. 0.103 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :





KEARNYGEN-SILICA

Tgt Ion: 56 Resp: 447

Ion Ratio Lower Upper

56 100

55 62.2 56.9 85.3

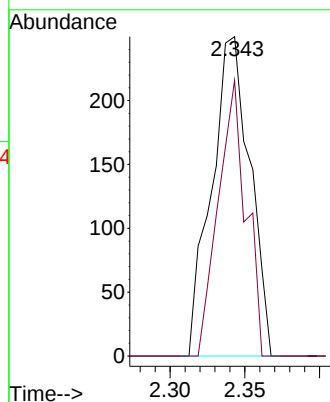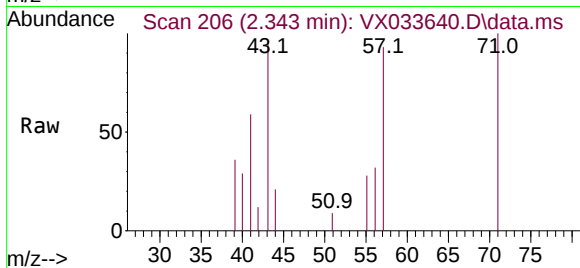

#14

Allyl chloride

Concen: 0.360 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.116 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53




Tgt Ion: 41 Resp: 944


Ion Ratio Lower Upper

41 100

39 55.9 53.3 79.9

76 0.0 25.0 37.4#


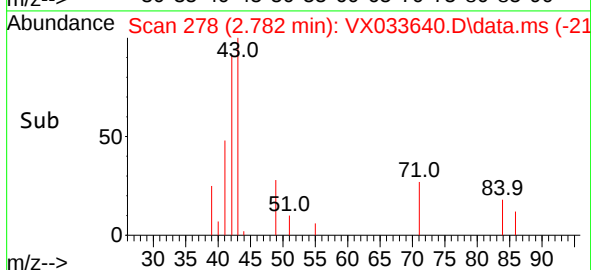

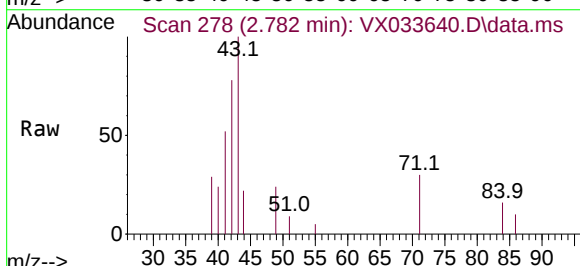




#16
Acetone
Concen: Below Cal
RT: 2.410 min Scan# 215
Delta R.T. 0.012 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53




Instrument :
MSVOA_X
ClientSampleId :
KEARNYGEN-SILICA


Tgt Ion: 43 Resp: 2555
Ion Ratio Lower Upper
43 100
58 27.1 22.9 34.3

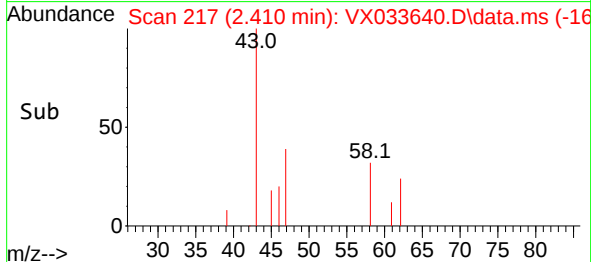

#17
Carbon Disulfide
Concen: 1.645 ug/l
RT: 2.520 min Scan# 235
Delta R.T. 0.006 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53

Tgt Ion: 76 Resp: 84
Ion Ratio Lower Upper
76 100
78 0.0 7.6 11.4#

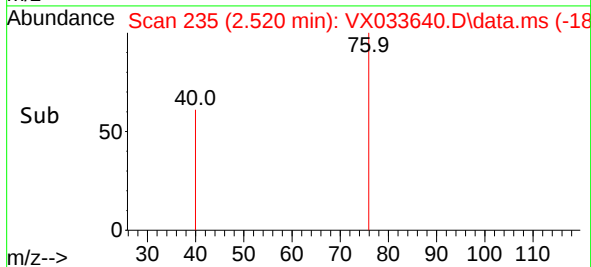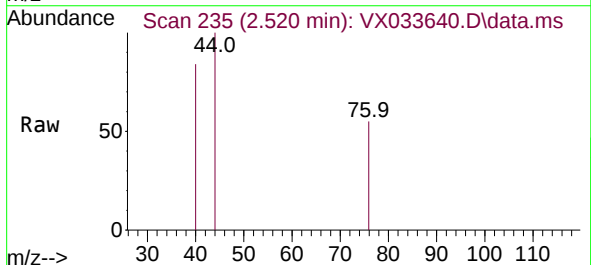



#18

Methyl Acetate

Concen: 0.206 ug/l

RT: 2.703 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :





KEARNYGEN-SILICA

Tgt Ion: 43 Resp: 543

Ion Ratio Lower Upper

43 100

74 0.0 17.9 26.9#

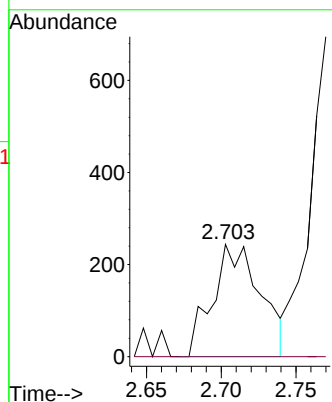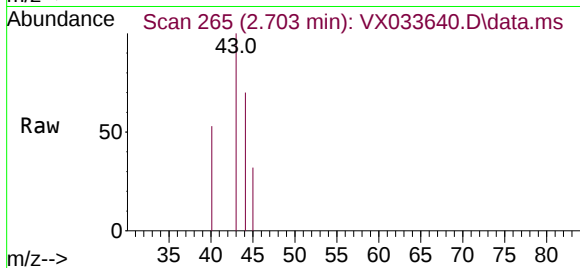

#20

Methylene Chloride

Concen: Below Cal

RT: 2.788 min Scan# 279

Delta R.T. 0.000 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Tgt Ion: 84 Resp: 411




Ion Ratio Lower Upper


84 100

49 89.8 97.6 146.4#

51 50.2 30.4 45.6#

86 41.7 49.7 74.5#


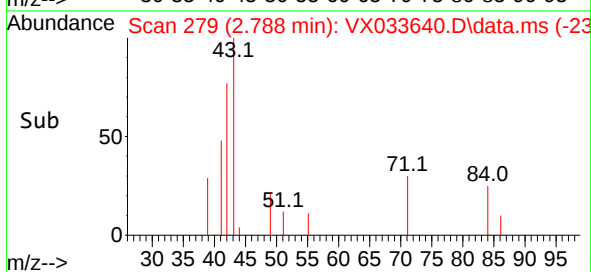

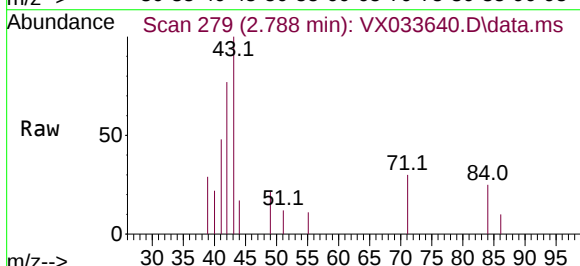




#22
Diisopropyl ether
Concen: 1.480 ug/l
RT: 3.697 min Scan# 41
Delta R.T. -0.061 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53




Instrument :
MSVOA_X
ClientSampleId :
KEARNYGEN-SILICA


Tgt Ion: 45	Resp: 7825
Ion Ratio	Lower Upper
45 100	
43 10.7	62.6 93.8#
87 0.0	22.1 33.1#
59 182.9	8.8 13.2#



#23
Vinyl Acetate
Concen: 0.217 ug/l
RT: 3.684 min Scan# 426
Delta R.T. -0.037 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53

Tgt Ion: 43	Resp: 880
Ion Ratio	Lower Upper
43 100	
86 0.0	8.3 12.5#





#25

2-Butanone

Concen: 1.051 ug/l

RT: 4.587 min Scan# 51

Delta R.T. 0.024 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :





KEARNYGEN-SILICA

Tgt Ion: 43 Resp: 1303

Ion Ratio Lower Upper

43 100

72 18.4 19.8 29.6#

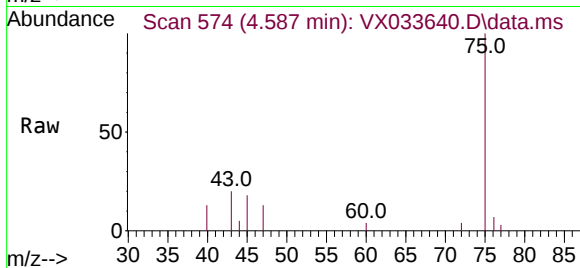

#31

Cyclohexane

Concen: 2.327 ug/l

RT: 5.477 min Scan# 720

Delta R.T. 0.006 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53




Tgt Ion: 56 Resp: 6151


Ion Ratio Lower Upper

56 100

69 40.7 24.6 36.8#

84 79.8 72.2 108.2


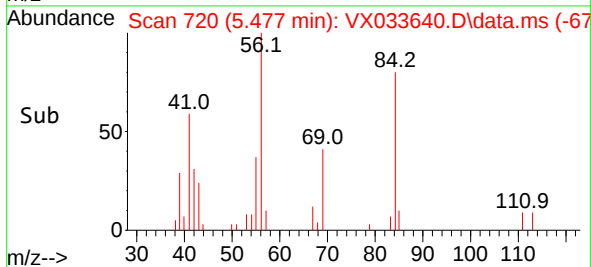

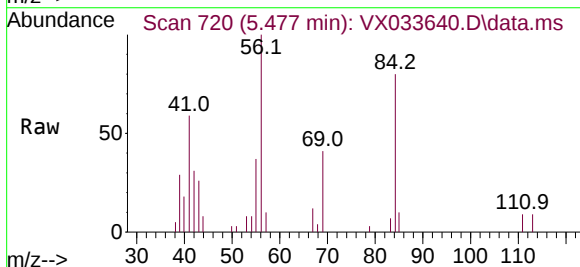




#33
 1,2-Dichloroethane-d4
 Concen: 48.855 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. -0.000 min
 Lab File: VX033640.D
 Acq: 06 Jan 2023 18:53




Instrument :
 MSVOA_X
 ClientSampleId :
 KEARNYGEN-SILICA


Tgt Ion: 65 Resp: 92778
 Ion Ratio Lower Upper
 65 100
 67 50.8 0.0 104.8

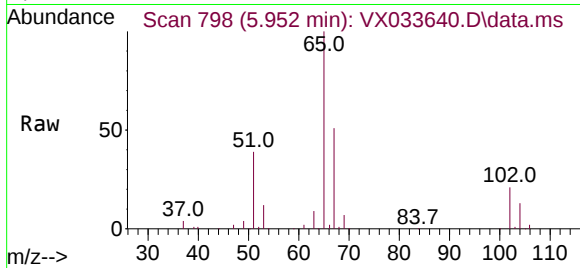

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. 0.000 min
 Lab File: VX033640.D
 Acq: 06 Jan 2023 18:53

Tgt Ion: 114 Resp: 245932
 Ion Ratio Lower Upper
 114 100
 63 19.2 0.0 40.0
 88 15.2 0.0 29.6

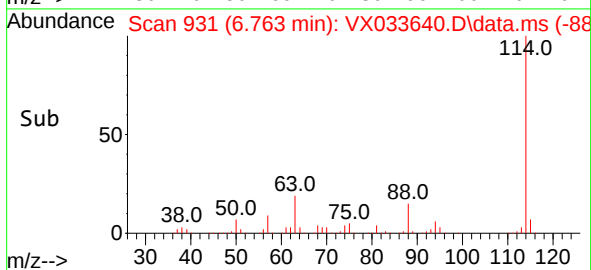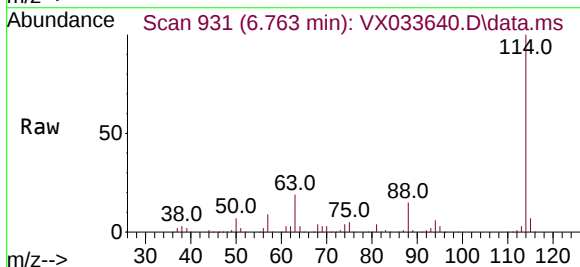

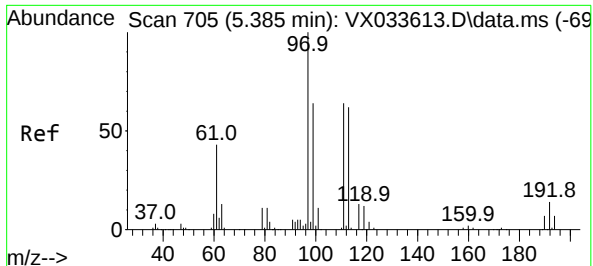

#35

Dibromofluoromethane

Concen: 48.109 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.000 min

Lab File: VX033640.D


Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :

KEARNYGEN-SILICA

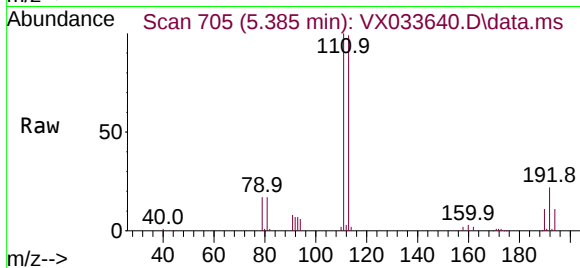




Tgt Ion:113 Resp: 77767

Ion Ratio Lower Upper

113 100

111 101.7 81.2 121.8

192 22.8 18.2 27.2

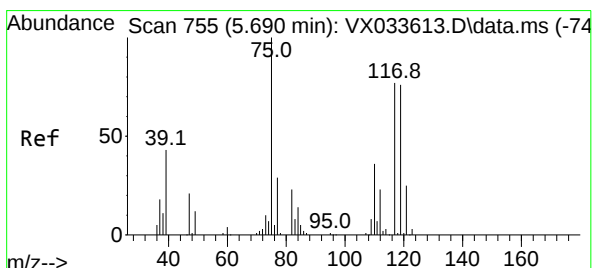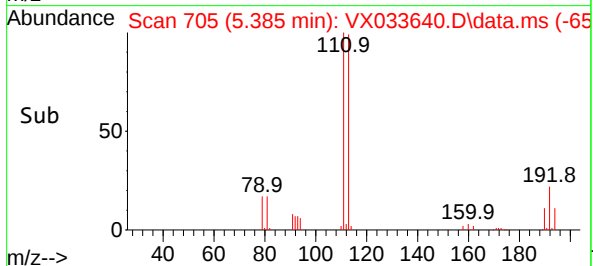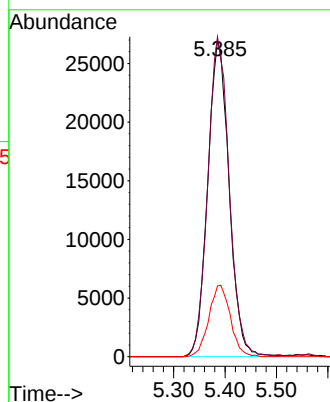

#36

1,1-Dichloropropene

Concen: 5.289 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.140 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53




Tgt Ion: 75 Resp: 11582


Ion Ratio Lower Upper

75 100

110 9.5 18.0 54.0#

77 0.0 24.5 36.7#

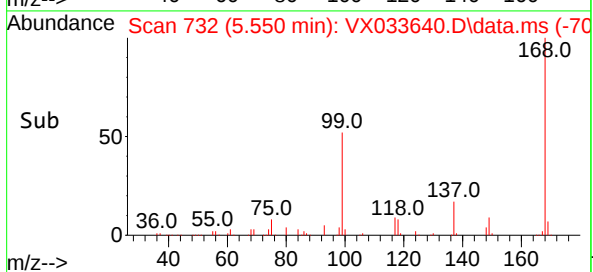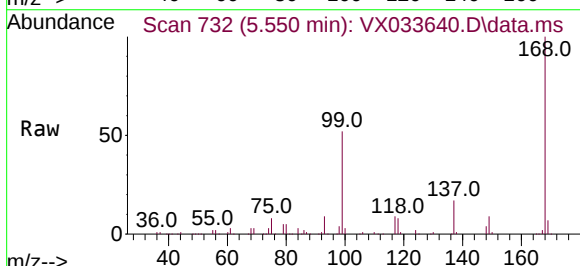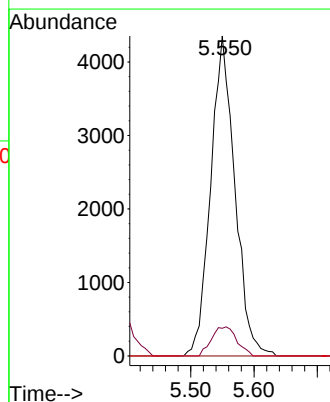



#37

Ethyl Acetate

Concen: Below Cal

RT: 4.733 min Scan# 51

Delta R.T. 0.018 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :

KEARNYGEN-SILICA





Tgt Ion: 43 Resp: 1788

Ion Ratio Lower Upper

43 100

61 1.2 10.6 16.0#

70 1.2 8.1 12.1#

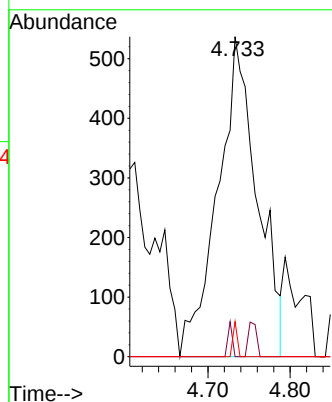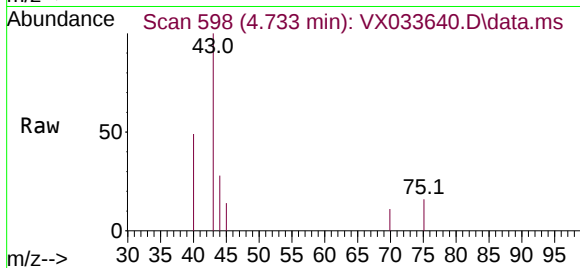

#38

Carbon Tetrachloride

Concen: 6.746 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.128 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53




Tgt Ion: 117 Resp: 15631


Ion Ratio Lower Upper

117 100

119 5.4 78.8 118.2#

121 0.0 24.9 37.3#

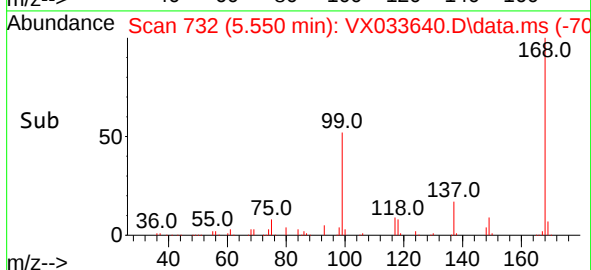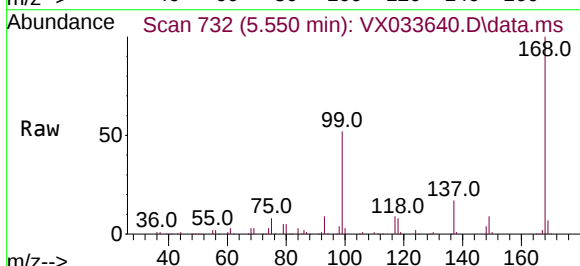

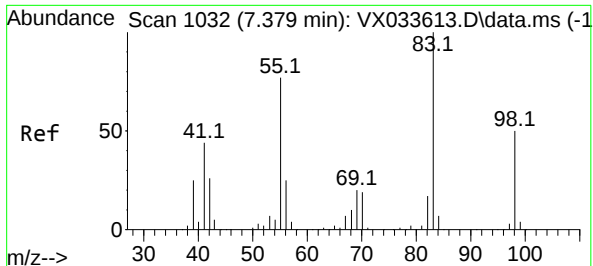

#39

Methylcyclohexane

Concen: 2.252 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. 0.006 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :

KEARNYGEN-SILICA





Tgt Ion: 83 Resp: 6157

Ion Ratio Lower Upper

83 100

55 78.7 61.4 92.2

98 45.9 40.2 60.2

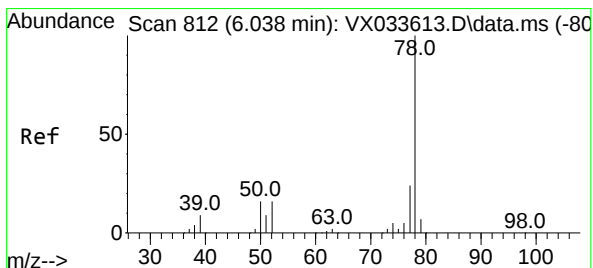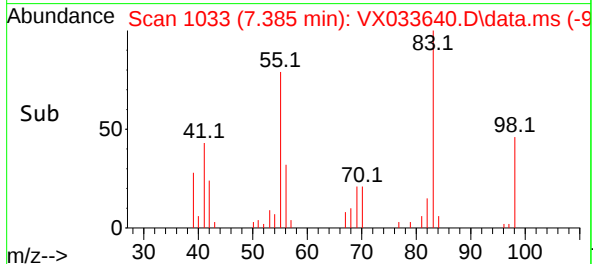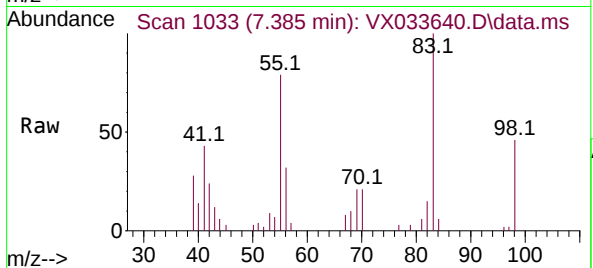

#40

Benzene

Concen: 20.944 ug/l

RT: 6.038 min Scan# 812

Delta R.T. -0.000 min

Lab File: VX033640.D




Acq: 06 Jan 2023 18:53


Tgt Ion: 78 Resp: 134035

Ion Ratio Lower Upper

78 100

77 23.9 19.0 28.6


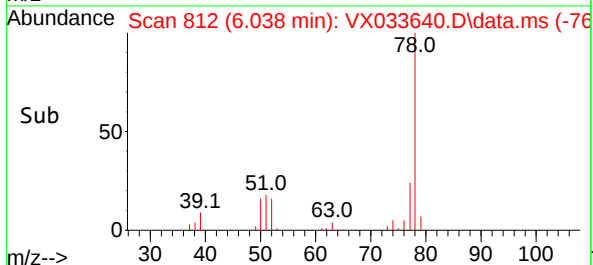

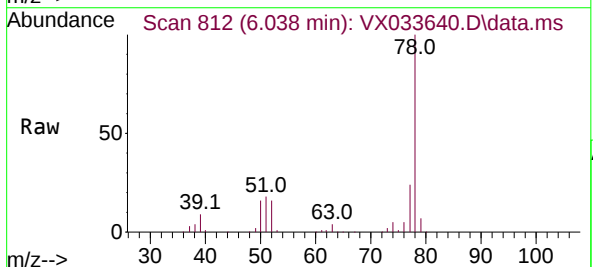




#43
Isopropyl Acetate
Concen: 0.280 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.006 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53




Instrument :
MSVOA_X
ClientSampleId :
KEARNYGEN-SILICA


Tgt Ion: 43 Resp: 1050
Ion Ratio Lower Upper
43 100
61 0.0 15.2 22.8#
87 3.7 10.6 16.0#

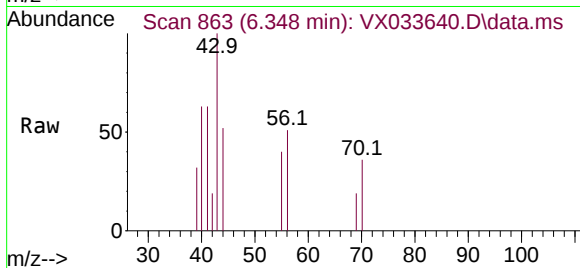

#50
Toluene-d8
Concen: 49.092 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53

Tgt Ion: 98 Resp: 283638
Ion Ratio Lower Upper
98 100
100 66.5 53.6 80.4

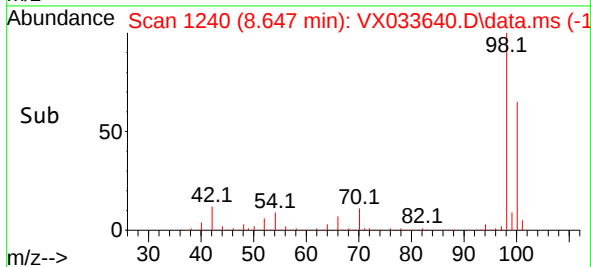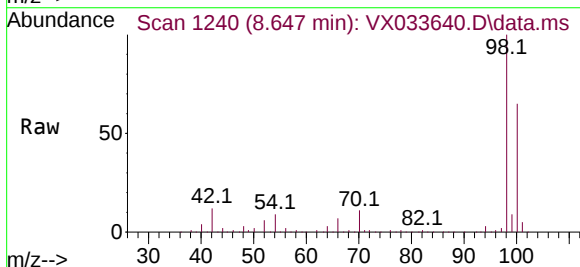



#51

4-Methyl-2-Pentanone

Concen: 0.331 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :





KEARNYGEN-SILICA

Tgt Ion: 43 Resp: 785

Ion Ratio Lower Upper

43 100

58 0.0 30.5 45.7#

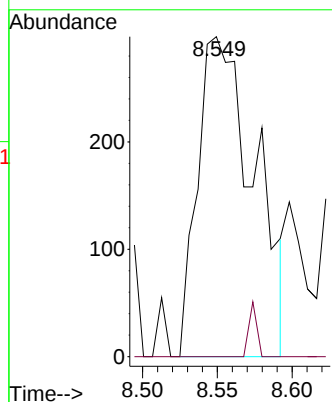

#52

Toluene

Concen: 12.732 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX033640.D




Acq: 06 Jan 2023 18:53


Tgt Ion: 92 Resp: 53571

Ion Ratio Lower Upper

92 100

91 170.5 135.4 203.2

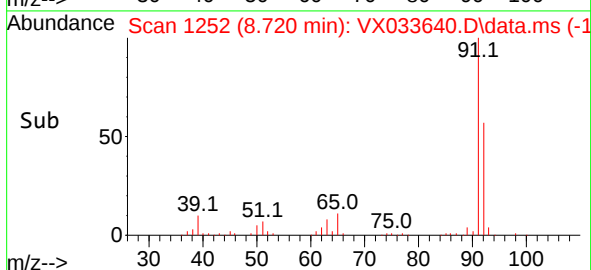

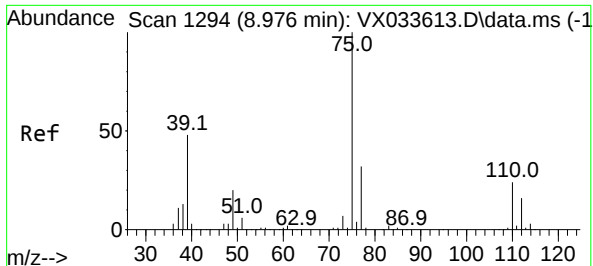

#53

t-1,3-Dichloropropene

Concen: 0.373 ug/l

RT: 8.714 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :





KEARNYGEN-SILICA

Tgt Ion: 75 Resp: 626

Ion Ratio Lower Upper

75 100

77 175.0 25.3 37.9#

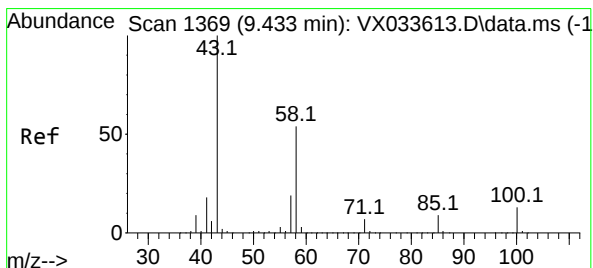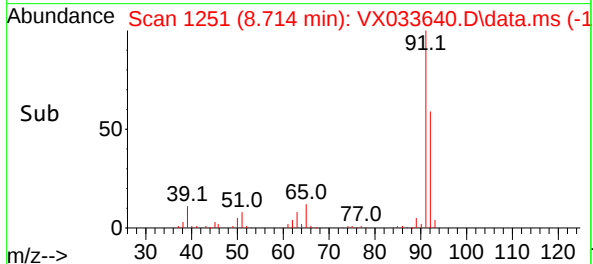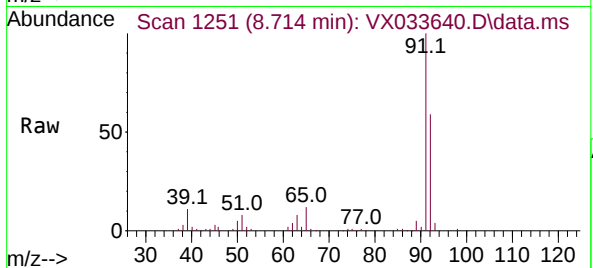

#59

2-Hexanone

Concen: 0.203 ug/l

RT: 9.488 min Scan# 1378

Delta R.T. 0.055 min

Lab File: VX033640.D




Acq: 06 Jan 2023 18:53


Tgt Ion: 43 Resp: 356

Ion Ratio Lower Upper

43 100

58 27.8 26.6 79.8


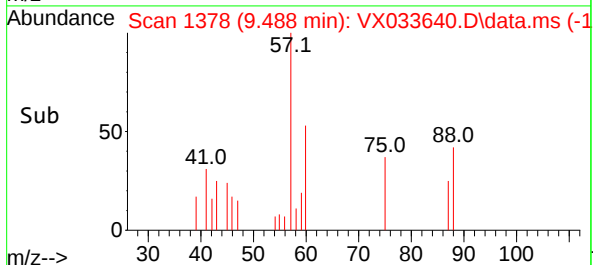

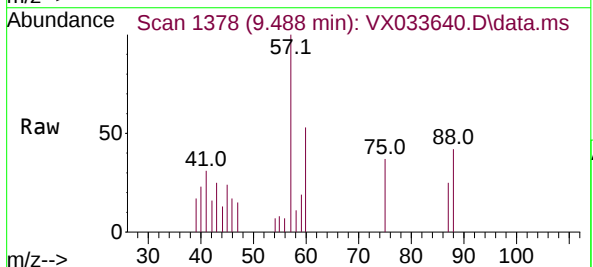




#62
4-Bromofluorobenzene
Concen: 49.703 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53




Instrument :
MSVOA_X
ClientSampleId :
KEARNYGEN-SILICA


Tgt Ion: 95 Resp: 101790
Ion Ratio Lower Upper
95 100
174 90.2 0.0 180.4
176 86.8 0.0 176.2

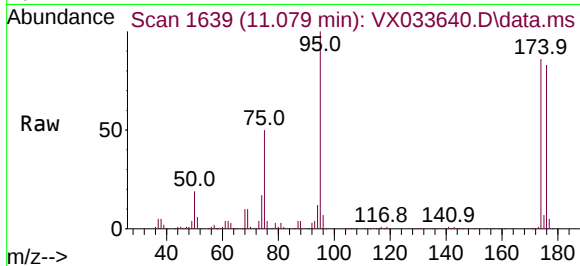

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53

Tgt Ion: 117 Resp: 153262
Ion Ratio Lower Upper
117 100
82 53.2 42.2 63.2
119 32.7 26.2 39.4

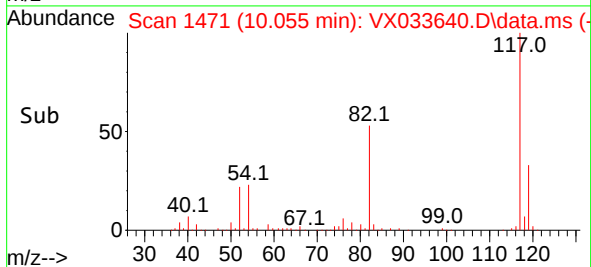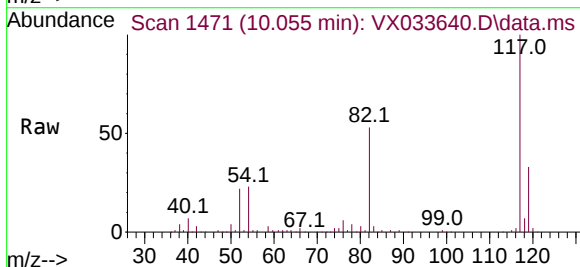



#67

Ethyl Benzene

Concen: 0.784 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. -0.000 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :





KEARNYGEN-SILICA

Tgt Ion: 91 Resp: 4293

Ion Ratio Lower Upper

91 100

106 30.8 25.9 38.9



#68

m/p-Xylenes

Concen: 3.136 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX033640.D




Acq: 06 Jan 2023 18:53


Tgt Ion: 106 Resp: 6701

Ion Ratio Lower Upper

106 100

91 199.5 159.6 239.4


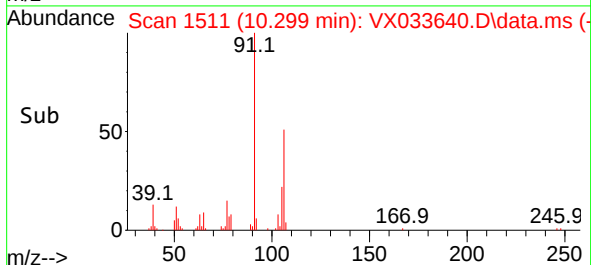
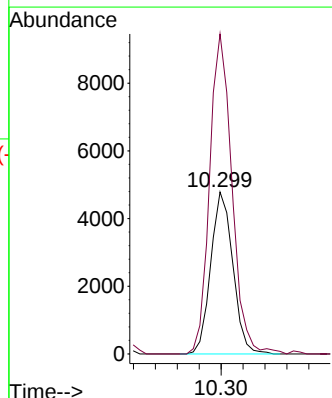
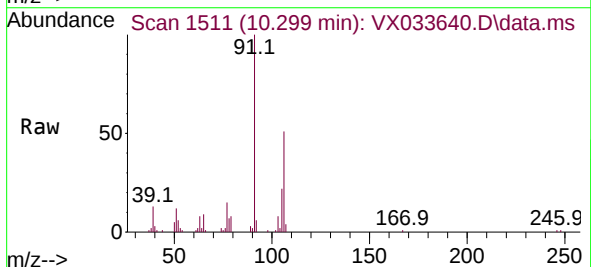




#69
o-Xylene
Concen: 1.341 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53




Instrument :
MSVOA_X
ClientSampleId :
KEARNYGEN-SILICA


Tgt Ion:106 Resp: 2841
Ion Ratio Lower Upper
106 100
91 203.1 104.1 312.3



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033640.D
Acq: 06 Jan 2023 18:53

Tgt Ion:152 Resp: 107617
Ion Ratio Lower Upper
152 100
115 55.7 38.5 115.5
150 156.6 0.0 340.4

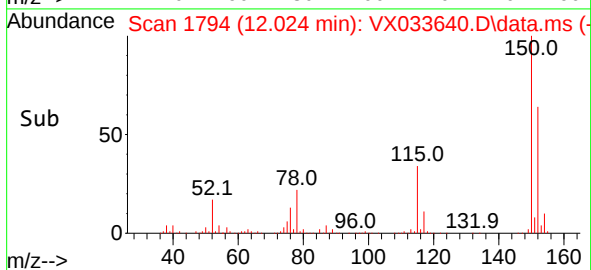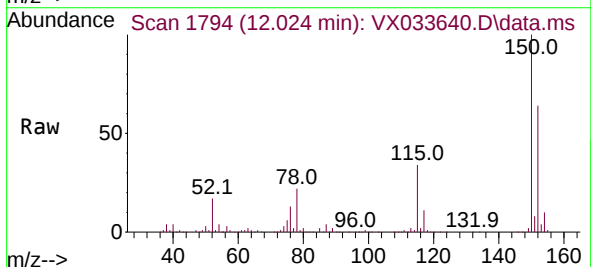



#76

1,2,3-Trichloropropane

Concen: 25.597 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :





KEARNYGEN-SILICA

Tgt Ion: 75 Resp: 50467

Ion Ratio Lower Upper

75 100

77 1.2 21.3 63.9#

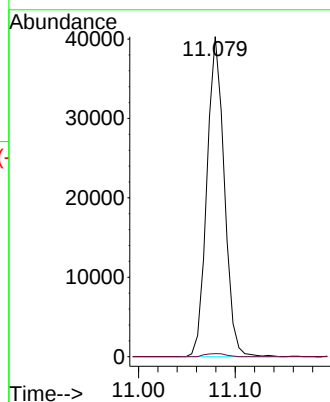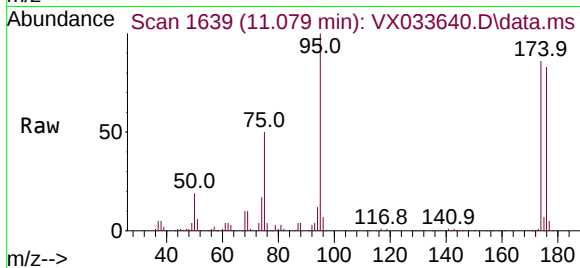

#81

trans-1,4-Dichloro-2-butene

Concen: 77.692 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53




Tgt Ion: 75 Resp: 50467


Ion Ratio Lower Upper

75 100

53 0.0 86.4 129.6#

89 0.0 37.4 56.2#

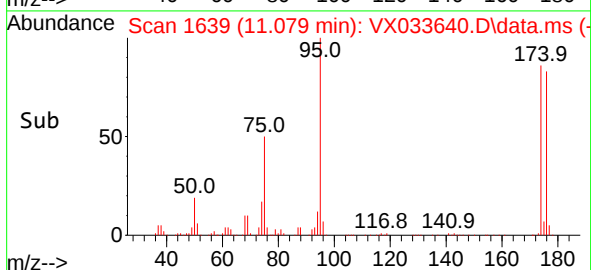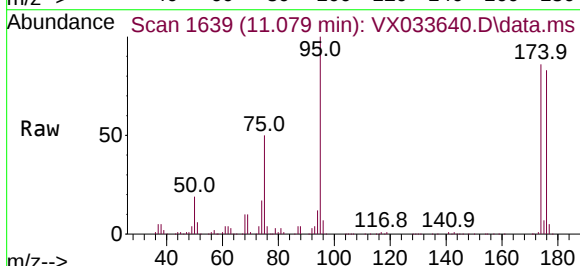



#84

1,2,4-Trimethylbenzene

Concen: 0.394 ug/l

RT: 11.750 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53

Instrument :

MSVOA_X

ClientSampleId :





KEARNYGEN-SILICA

Tgt Ion:105 Resp: 2476

Ion Ratio Lower Upper

105 100

120 39.3 23.4 70.0

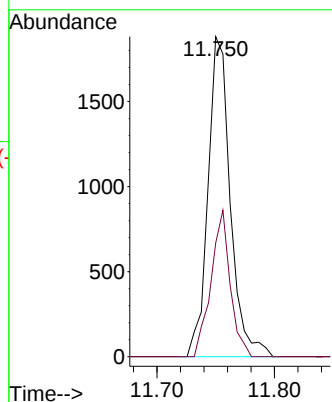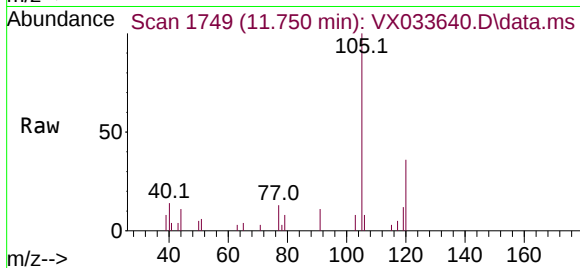

#93

1,2,4-Trichlorobenzene

Concen: 1.617 ug/l

RT: 13.597 min Scan# 2052

Delta R.T. 0.012 min

Lab File: VX033640.D

Acq: 06 Jan 2023 18:53




Tgt Ion:180 Resp: 58


Ion Ratio Lower Upper

180 100

182 0.0 47.4 142.2#


145 0.0 14.1 42.2#

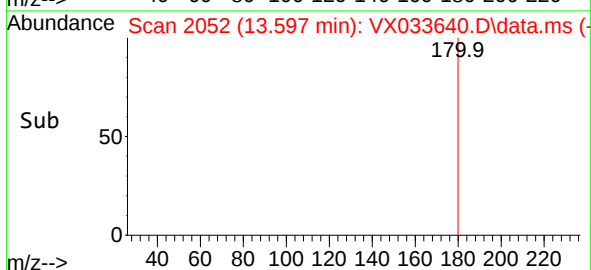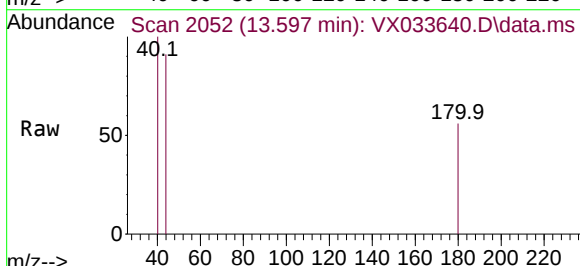



#95
 Naphthalene
 Concen: 3.373 ug/l
 RT: 13.780 min Scan# 2082
 Delta R.T. 0.006 min
 Lab File: VX033640.D
 Acq: 06 Jan 2023 18:53

Instrument :
 MSVOA_X
 ClientSampleId :
 KEARNYGEN-SILICA

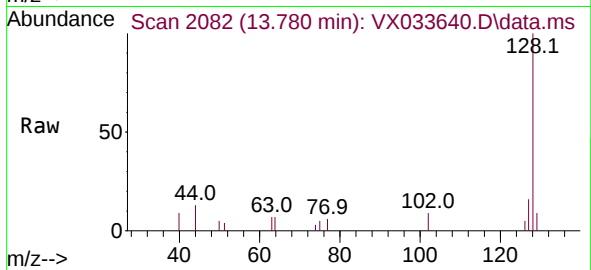

Tgt Ion:	128	Resp:	2060
Ion	Ratio	Lower	Upper
128	100		
127	12.7	10.3	15.5
129	9.5	9.0	13.4

