

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
 Data File : VX033641.D
 Acq On : 06 Jan 2023 19:16
 Operator : JC/MD
 Sample : 01042-04 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 HARRISON-SILICA

Quant Time: Jan 07 04:29:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 05 04:43:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	166884	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	243837	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	216356	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	109434	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	90783	48.189	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	96.380%		
35) Dibromofluoromethane	5.385	113	75863	47.334	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.660%		
50) Toluene-d8	8.647	98	283303	49.455	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	98.900%		
62) 4-Bromofluorobenzene	11.079	95	100939	49.711	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	99.420%		
Target Compounds						Qvalue
8) Diethyl Ether	2.136	74	855	1.279	ug/l	67
11) Tert butyl alcohol	3.007	59	1531	4.947	ug/l #	80
16) Acetone	2.398	43	6952	Below Cal		98
17) Carbon Disulfide	2.508	76	225	1.683	ug/l #	74
18) Methyl Acetate	2.709	43	1332	0.510	ug/l #	89
20) Methylene Chloride	2.788	84	430	Below Cal	#	88
25) 2-Butanone	4.586	43	4701	3.822	ug/l	100
36) 1,1-Dichloropropene	5.550	75	11203	5.160	ug/l #	50
37) Ethyl Acetate	4.733	43	1506	Below Cal	#	85
38) Carbon Tetrachloride	5.550	117	15616	6.797	ug/l #	16
39) Methylcyclohexane	7.385	83	687	0.253	ug/l #	78
40) Benzene	6.037	78	63880	10.067	ug/l	97
43) Isopropyl Acetate	6.342	43	2094	0.564	ug/l #	83
49) 1,4-Dioxane	7.726	88	19	0.475	ug/l #	23
51) 4-Methyl-2-Pentanone	8.573	43	5244	2.232	ug/l	89
52) Toluene	8.720	92	69044	16.551	ug/l	100
59) 2-Hexanone	9.433	43	2118	1.220	ug/l	98
67) Ethyl Benzene	10.195	91	5489	0.710	ug/l	97
68) m/p-Xylenes	10.299	106	12848	4.260	ug/l	95
69) o-Xylene	10.640	106	4351	1.455	ug/l	93
74) N-amyl acetate	10.756	43	3079	0.983	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.280	83	2411	1.001	ug/l #	26
76) 1,2,3-Trichloropropane	11.079	75	50368	25.123	ug/l #	35
80) 1,3,5-Trimethylbenzene	11.451	105	4412	0.693	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	50368	76.252	ug/l #	7
84) 1,2,4-Trimethylbenzene	11.750	105	9015	1.412	ug/l	93
93) 1,2,4-Trichlorobenzene	13.585	180	60	1.618	ug/l #	70
95) Naphthalene	13.780	128	1042	3.245	ug/l #	92
96) 1,2,3-Trichlorobenzene	13.963	180	46	3.766	ug/l #	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
Data File : VX033641.D
Acq On : 06 Jan 2023 19:16
Operator : JC/MD
Sample : 01042-04 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA

Quant Time: Jan 07 04:29:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 05 04:43:25 2023
Response via : Initial Calibration




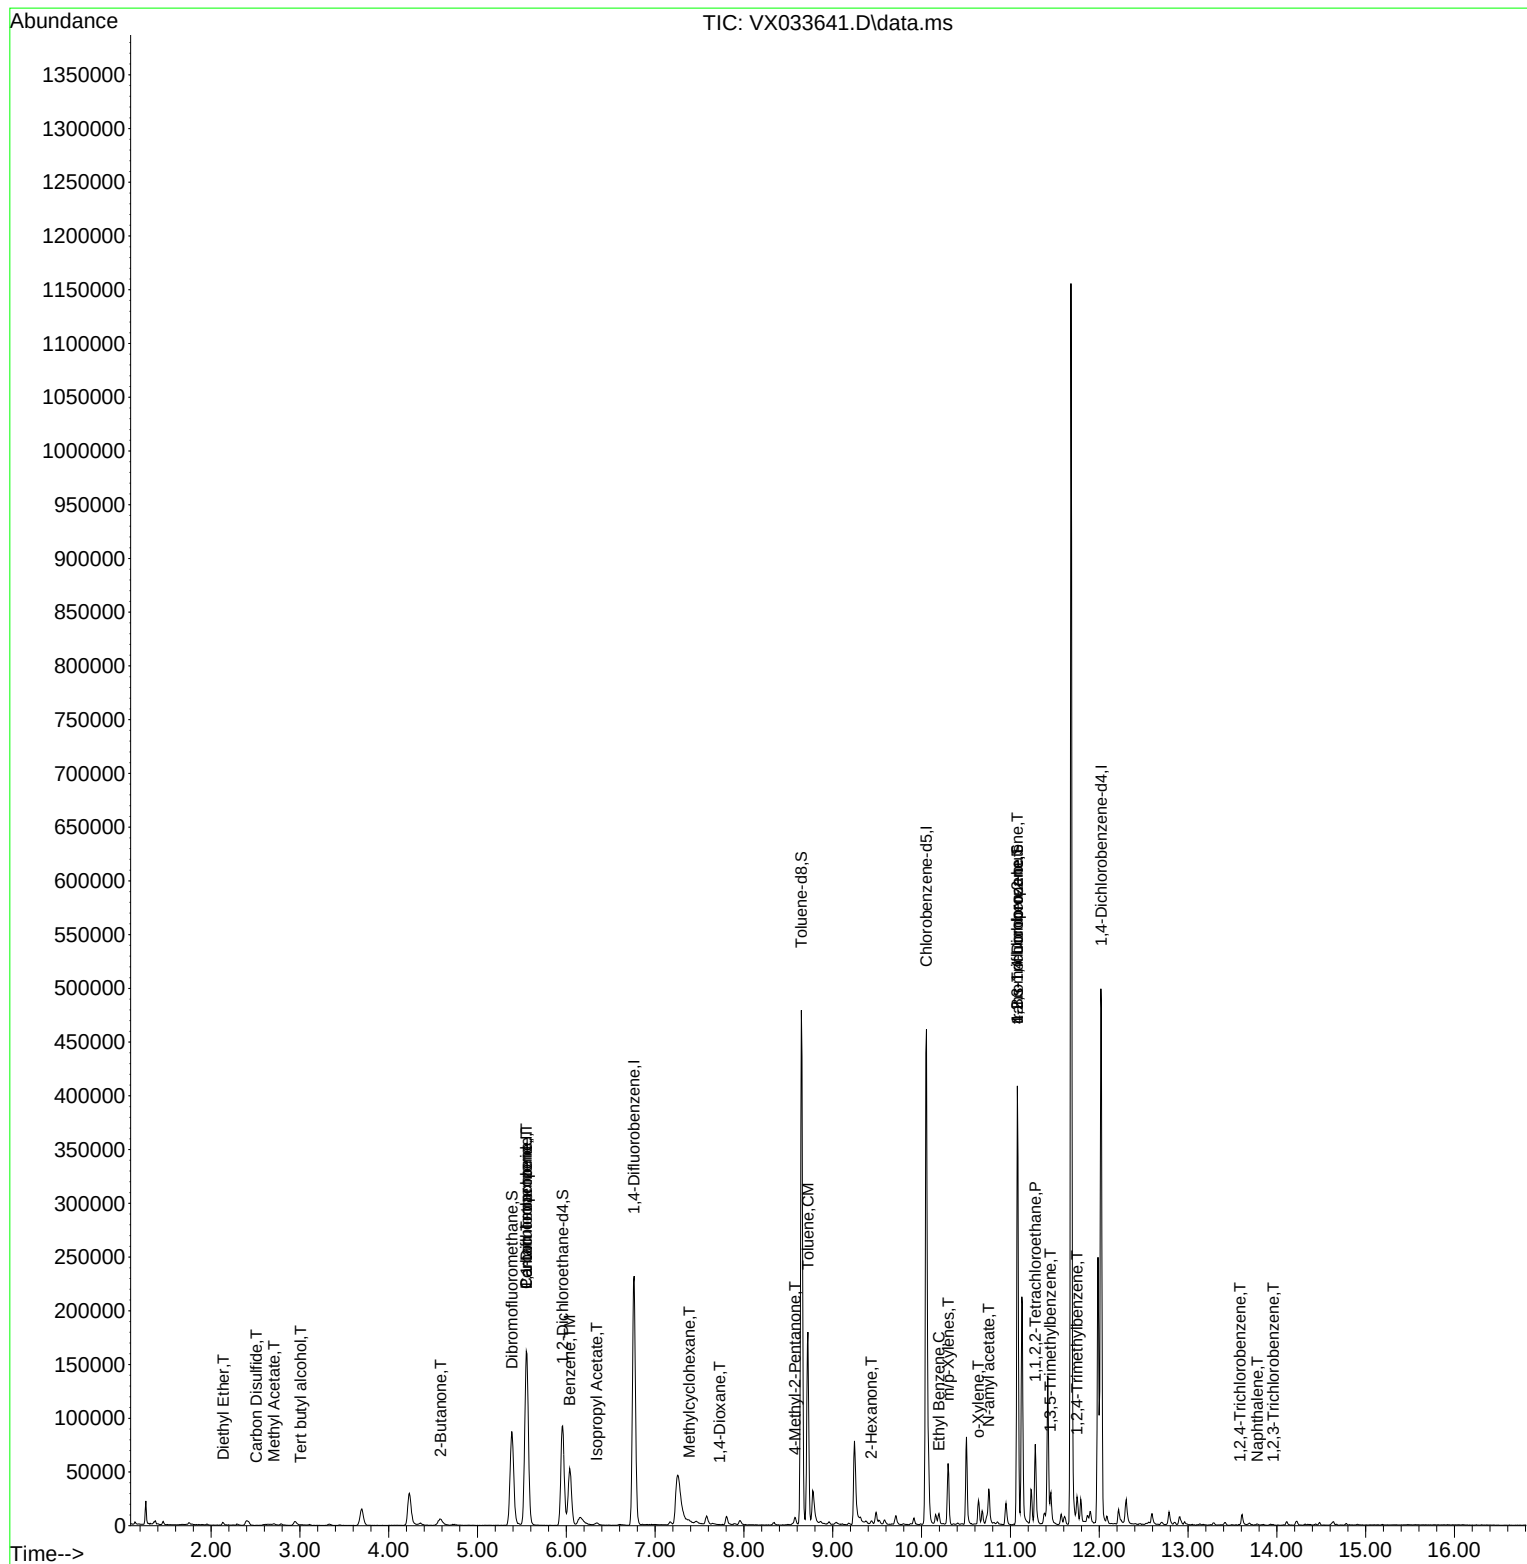


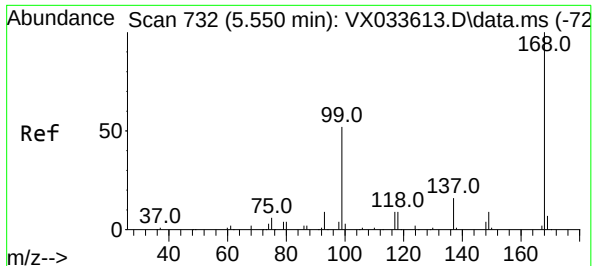

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion:168 Resp: 166884
Ion Ratio Lower Upper
168 100
99 51.7 41.4 62.2

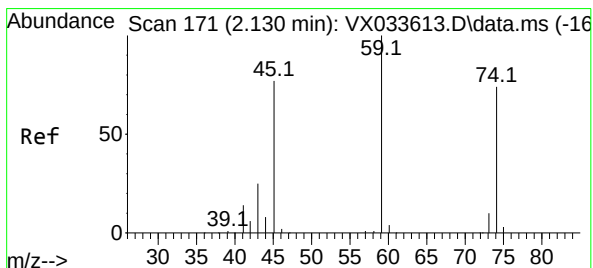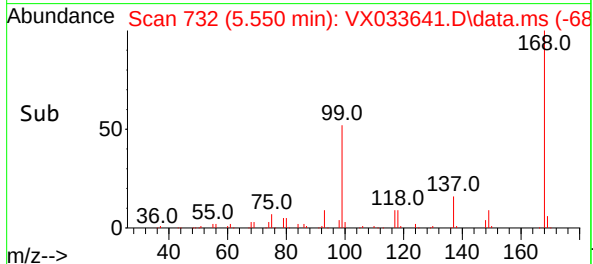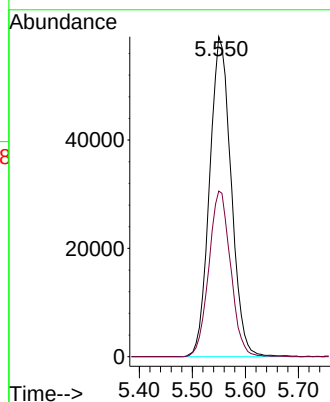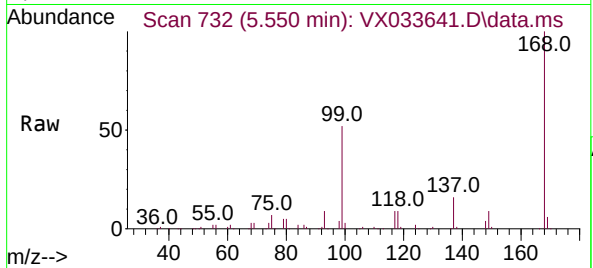

#8
Diethyl Ether
Concen: 1.279 ug/l
RT: 2.136 min Scan# 172
Delta R.T. 0.006 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 74 Resp: 855
Ion Ratio Lower Upper
74 100
45 133.0 50.1 150.4

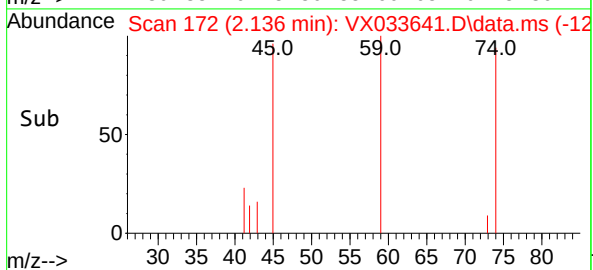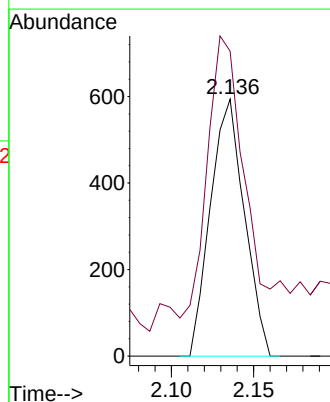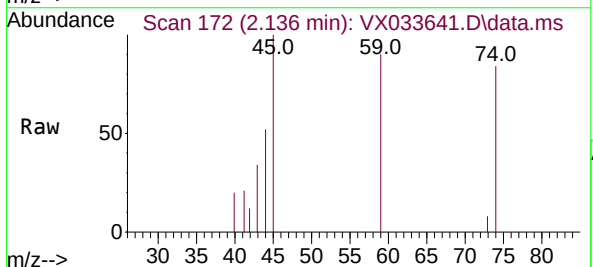



#11

Tert butyl alcohol

Concen: 4.947 ug/l

RT: 3.007 min Scan# 31

Delta R.T. -0.006 min

Lab File: VX033641.D

Acq: 06 Jan 2023 19:16

Instrument :

MSVOA_X

ClientSampleId :





HARRISON-SILICA

Tgt Ion: 59 Resp: 1531

Ion Ratio Lower Upper

59 100

57 0.0 5.5 8.3#

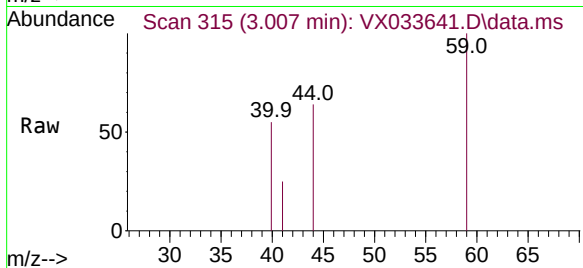

#16

Acetone

Concen: Below Cal

RT: 2.398 min Scan# 215

Delta R.T. -0.000 min

Lab File: VX033641.D




Acq: 06 Jan 2023 19:16


Tgt Ion: 43 Resp: 6952

Ion Ratio Lower Upper

43 100

58 27.6 22.9 34.3




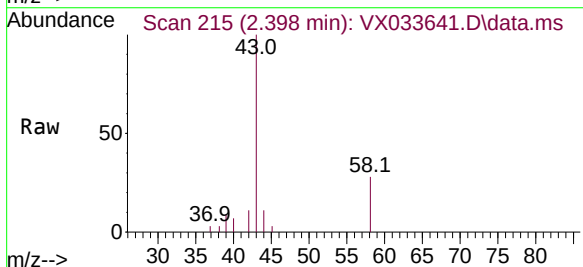


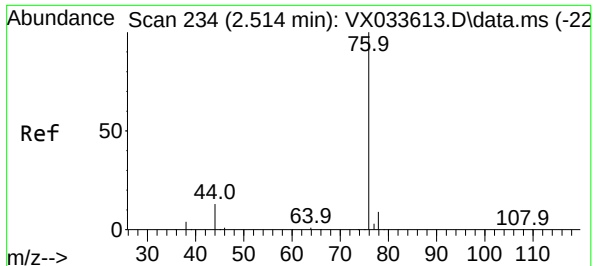

#17
Carbon Disulfide
Concen: 1.683 ug/l
RT: 2.508 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion: 76 Resp: 225
Ion Ratio Lower Upper
76 100
78 0.0 7.6 11.4#

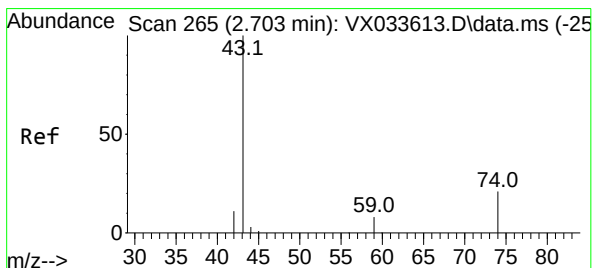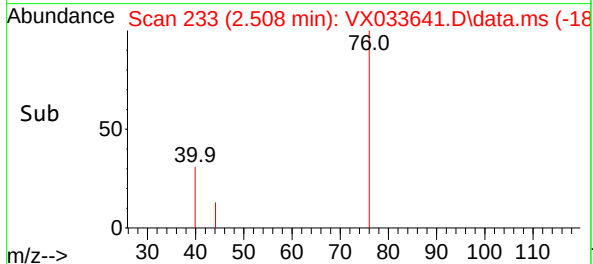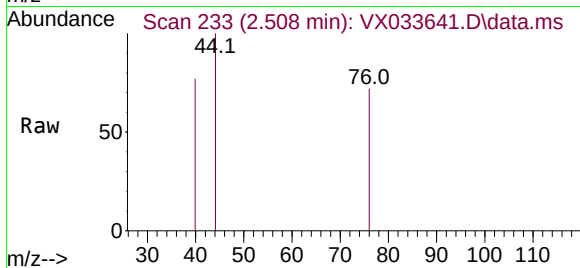

#18
Methyl Acetate
Concen: 0.510 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 43 Resp: 1332
Ion Ratio Lower Upper
43 100
74 17.0 17.9 26.9#


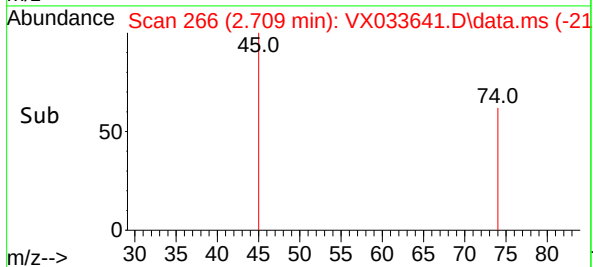

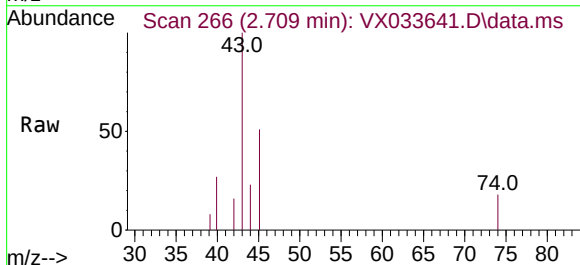




#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion:	84	Resp:	430
Ion	Ratio	Lower	Upper
84	100		
49	116.6	97.6	146.4
51	38.5	30.4	45.6
86	87.4	49.7	74.5

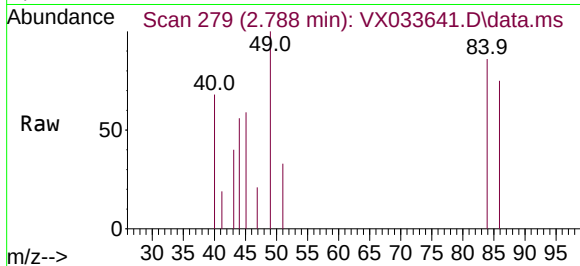

#25
2-Butanone
Concen: 3.822 ug/l
RT: 4.586 min Scan# 574
Delta R.T. 0.024 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion:	43	Resp:	4701
Ion	Ratio	Lower	Upper
43	100		
72	24.8	19.8	29.6


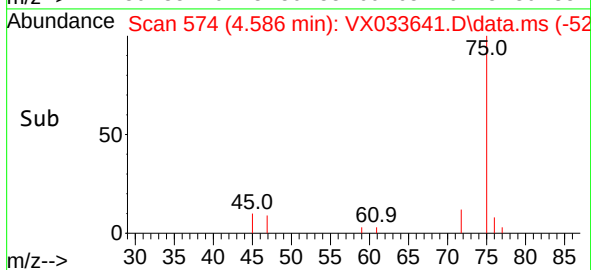

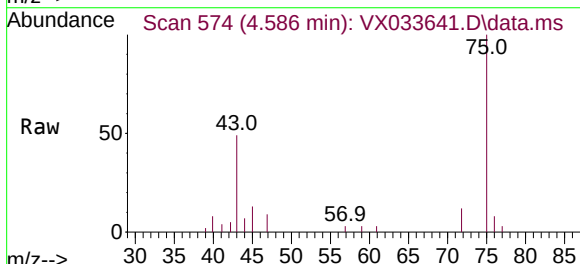


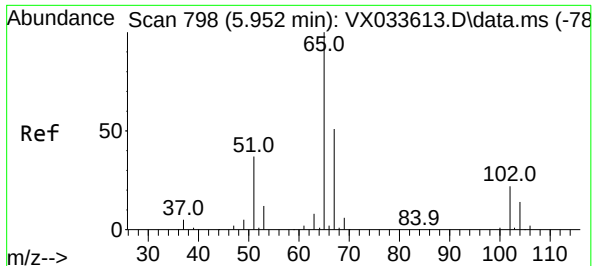

#33
 1,2-Dichloroethane-d4
 Concen: 48.189 ug/l
 RT: 5.958 min Scan# 798
 Delta R.T. 0.006 min
 Lab File: VX033641.D
 Acq: 06 Jan 2023 19:16




Instrument :
 MSVOA_X
 ClientSampleId :
 HARRISON-SILICA


Tgt Ion: 65 Resp: 90783
 Ion Ratio Lower Upper
 65 100
 67 52.0 0.0 104.8

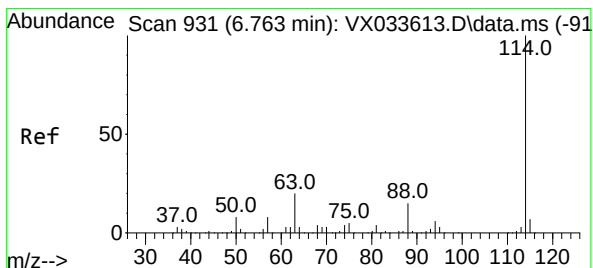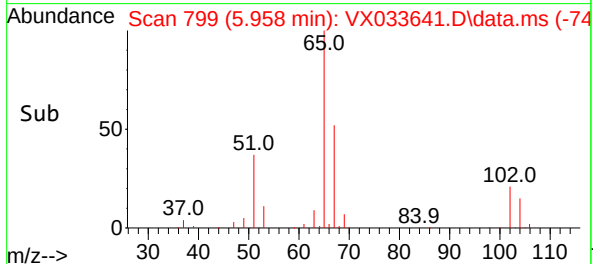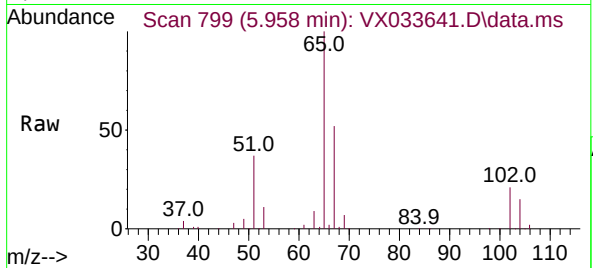

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. -0.000 min
 Lab File: VX033641.D
 Acq: 06 Jan 2023 19:16

Tgt Ion: 114 Resp: 243837
 Ion Ratio Lower Upper
 114 100
 63 19.3 0.0 40.0
 88 15.2 0.0 29.6

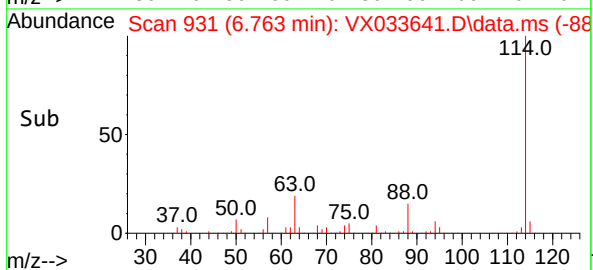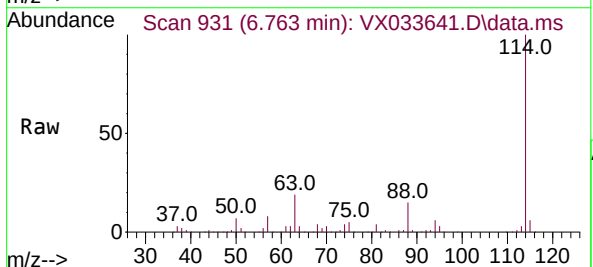

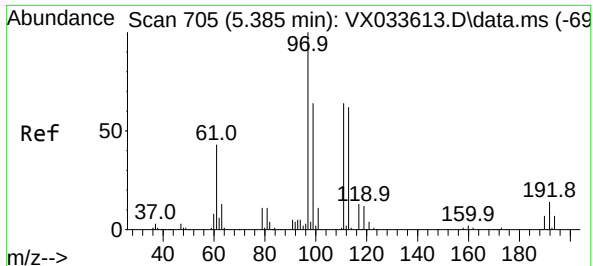

#35

Dibromofluoromethane

Concen: 47.334 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.000 min

Lab File: VX033641.D


Acq: 06 Jan 2023 19:16

Instrument :

MSVOA_X

ClientSampleId :

HARRISON-SILICA

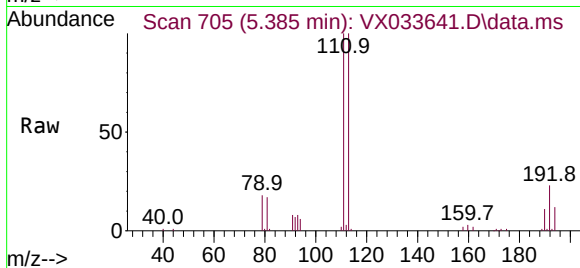




Tgt Ion:113 Resp: 75863

Ion Ratio Lower Upper

113 100

111 102.0 81.2 121.8

192 22.9 18.2 27.2

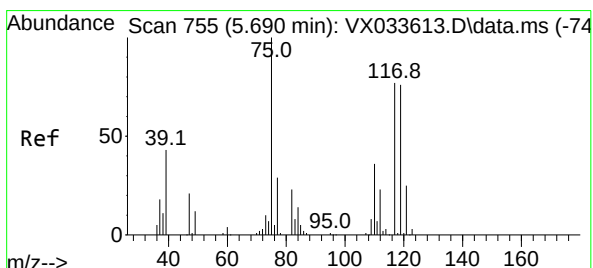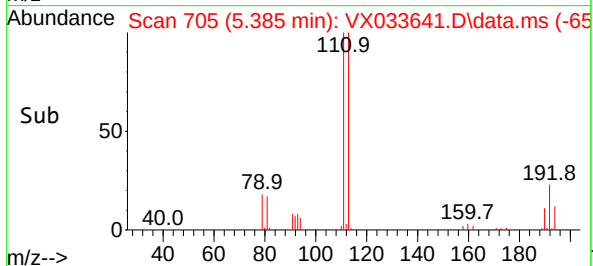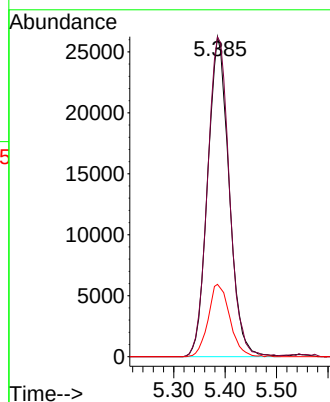

#36

1,1-Dichloropropene

Concen: 5.160 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.140 min

Lab File: VX033641.D

Acq: 06 Jan 2023 19:16




Tgt Ion: 75 Resp: 11203


Ion Ratio Lower Upper

75 100

110 9.5 18.0 54.0#

77 0.0 24.5 36.7#

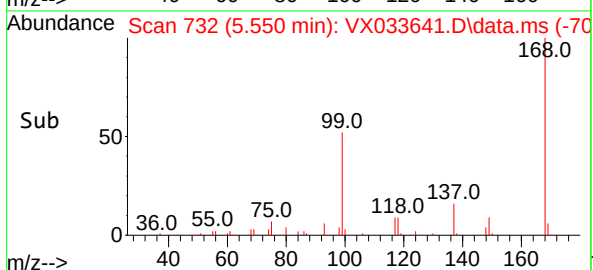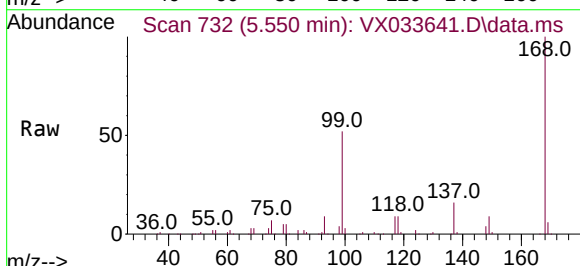



#37

Ethyl Acetate

Concen: Below Cal

RT: 4.733 min Scan# 595

Delta R.T. 0.018 min

Lab File: VX033641.D

Acq: 06 Jan 2023 19:16





Instrument :

MSVOA_X

ClientSampleId :

HARRISON-SILICA

Tgt Ion:	43	Resp:	1506
Ion	Ratio	Lower	Upper
43	100		
61	8.6	10.6	16.0#
70	2.6	8.1	12.1#

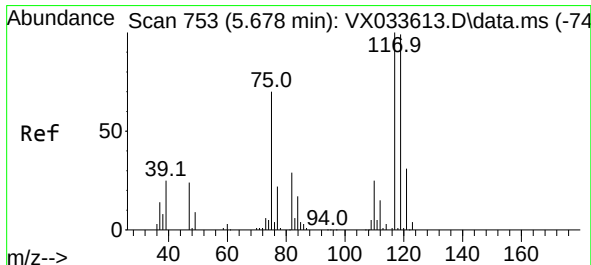

#38

Carbon Tetrachloride

Concen: 6.797 ug/l




RT: 5.550 min Scan# 732


Delta R.T. -0.128 min

Lab File: VX033641.D

Acq: 06 Jan 2023 19:16

Tgt Ion:	117	Resp:	15616
Ion	Ratio	Lower	Upper
117	100		
119	6.3	78.8	118.2#
121	0.0	24.9	37.3#




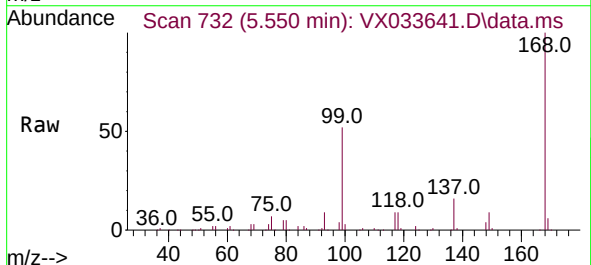




#39
Methylcyclohexane
Concen: 0.253 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. 0.006 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion: 83 Resp: 687
Ion Ratio Lower Upper
83 100
55 49.7 61.4 92.2#
98 55.8 40.2 60.2

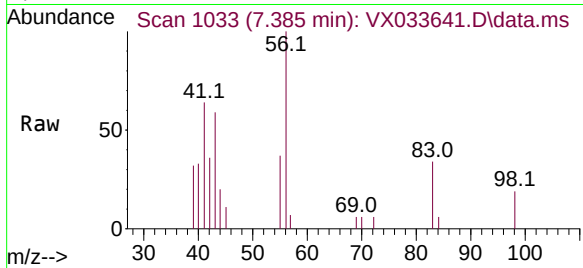

#40
Benzene
Concen: 10.067 ug/l
RT: 6.037 min Scan# 812
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 78 Resp: 63880
Ion Ratio Lower Upper
78 100
77 22.3 19.0 28.6


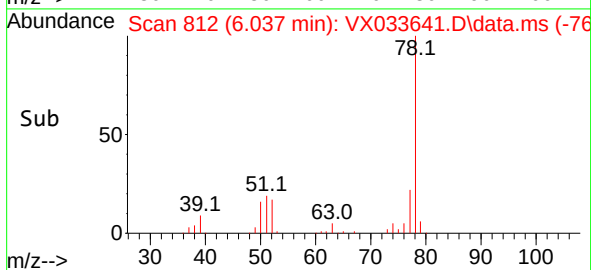

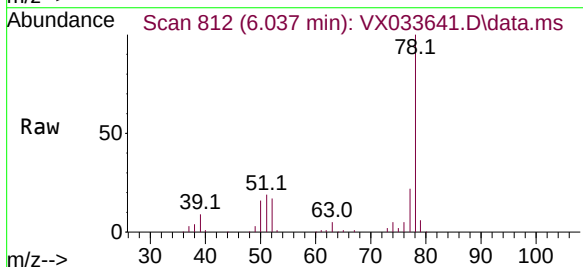




#43
Isopropyl Acetate
Concen: 0.564 ug/l
RT: 6.342 min Scan# 80
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion: 43 Resp: 2094
Ion Ratio Lower Upper
43 100
61 13.7 15.2 22.8#
87 3.6 10.6 16.0#

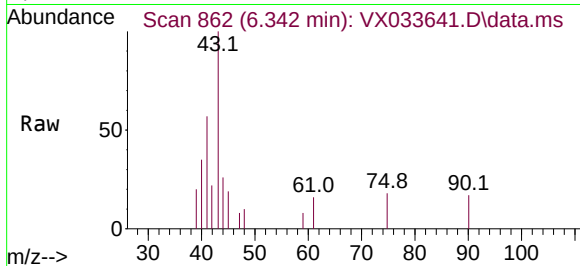

#49
1,4-Dioxane
Concen: 0.475 ug/l
RT: 7.726 min Scan# 1089
Delta R.T. 0.006 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 88 Resp: 19
Ion Ratio Lower Upper
88 100
43 0.0 24.1 36.1#
58 0.0 57.1 85.7#


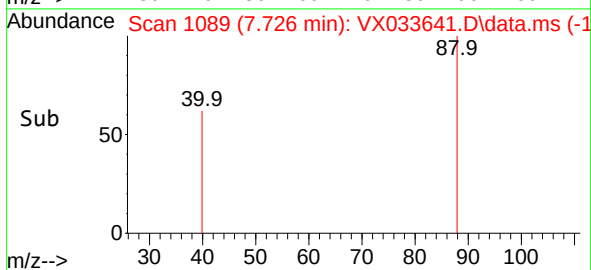

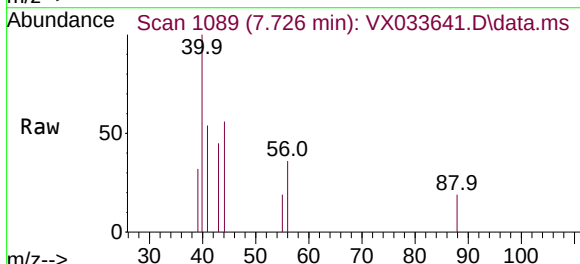




#50
Toluene-d8
Concen: 49.455 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion: 98 Resp: 283303
Ion Ratio Lower Upper
98 100
100 66.1 53.6 80.4



#51
4-Methyl-2-Pentanone
Concen: 2.232 ug/l
RT: 8.573 min Scan# 1228
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 43 Resp: 5244
Ion Ratio Lower Upper
43 100
58 31.5 30.5 45.7

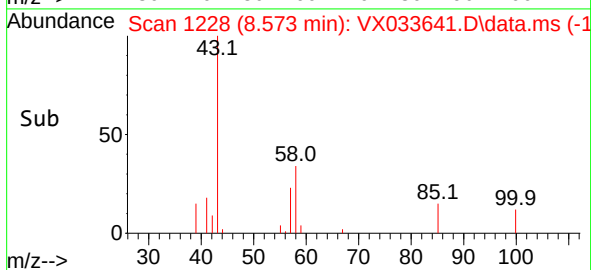



#52

Toluene

Concen: 16.551 ug/l

RT: 8.720 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX033641.D

Acq: 06 Jan 2023 19:16

Instrument :

MSVOA_X

ClientSampleId :





HARRISON-SILICA

Tgt Ion: 92 Resp: 69044

Ion Ratio Lower Upper

92 100

91 169.7 135.4 203.2



#59

2-Hexanone

Concen: 1.220 ug/l

RT: 9.433 min Scan# 1369

Delta R.T. -0.000 min

Lab File: VX033641.D




Acq: 06 Jan 2023 19:16


Tgt Ion: 43 Resp: 2118

Ion Ratio Lower Upper

43 100

58 51.8 26.6 79.8


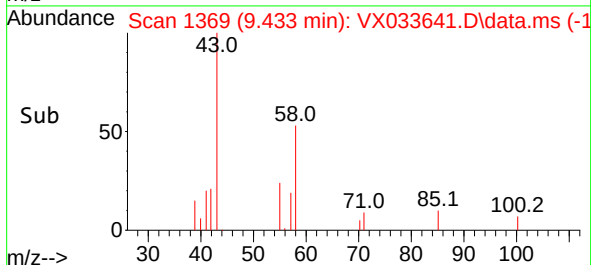






#62
4-Bromofluorobenzene
Concen: 49.711 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion: 95 Resp: 100939
Ion Ratio Lower Upper
95 100
174 89.4 0.0 180.4
176 88.1 0.0 176.2

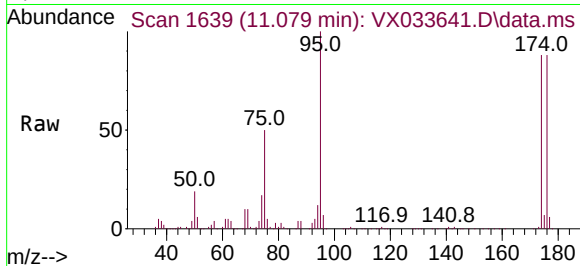

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 117 Resp: 216356
Ion Ratio Lower Upper
117 100
82 52.5 42.2 63.2
119 33.2 26.2 39.4




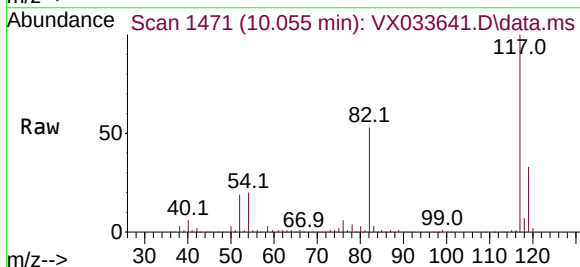




#67
Ethyl Benzene
Concen: 0.710 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion: 91 Resp: 5489
Ion Ratio Lower Upper
91 100
106 33.8 25.9 38.9



#68
m/p-Xylenes
Concen: 4.260 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 106 Resp: 12848
Ion Ratio Lower Upper
106 100
91 206.5 159.6 239.4

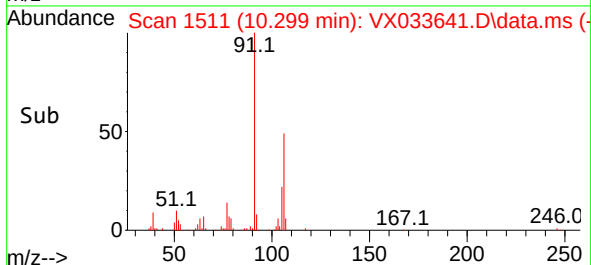

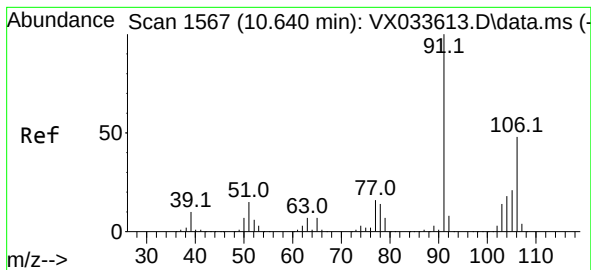

#69

o-Xylene

Concen: 1.455 ug/l

RT: 10.640 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX033641.D

Acq: 06 Jan 2023 19:16

Instrument :

MSVOA_X

ClientSampleId :





HARRISON-SILICA

Tgt Ion:106 Resp: 4351

Ion Ratio Lower Upper

106 100

91 218.5 104.1 312.3

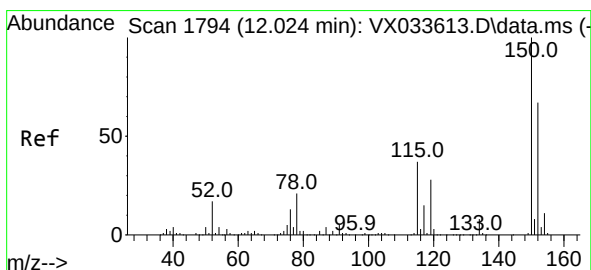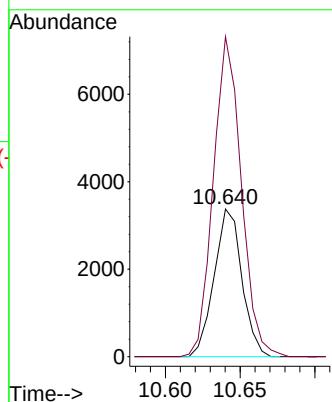

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX033641.D

Acq: 06 Jan 2023 19:16




Tgt Ion:152 Resp: 109434


Ion Ratio Lower Upper

152 100

115 55.6 38.5 115.5

150 155.8 0.0 340.4


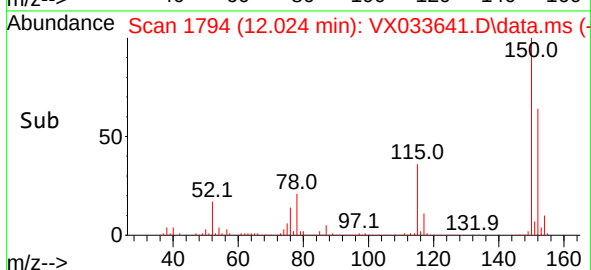

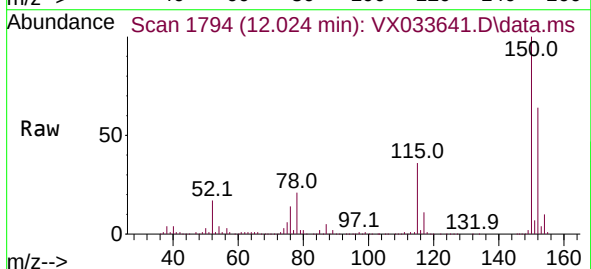




#74
N-amy1 acetate
Concen: 0.983 ug/l
RT: 10.756 min Scan# 1672
Delta R.T. -0.086 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion: 43	Resp: 3079
Ion Ratio	Lower Upper
43 100	
70 11.6	33.4 50.0#
55 191.1	18.6 27.8#
61 0.0	19.0 28.6#

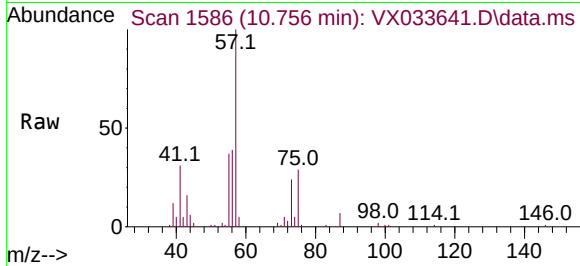

#75
1,1,2,2-Tetrachloroethane
Concen: 1.001 ug/l
RT: 11.280 min Scan# 1672
Delta R.T. 0.067 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 83	Resp: 2411
Ion Ratio	Lower Upper
83 100	
131 0.0	5.5 16.5#
85 0.0	32.1 96.5#




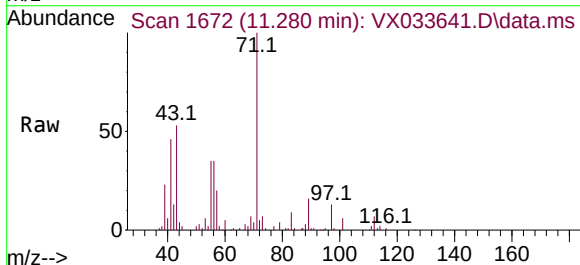




#76
1,2,3-Trichloropropane
Concen: 25.123 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion: 75 Resp: 50368
Ion Ratio Lower Upper
75 100
77 1.2 21.3 63.9#

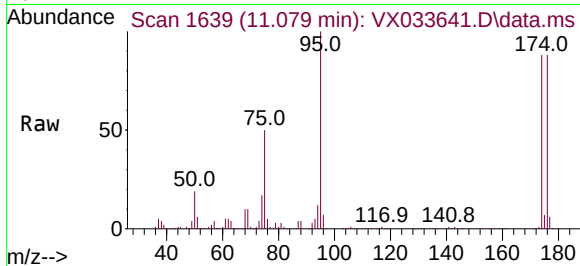

#80
1,3,5-Trimethylbenzene
Concen: 0.693 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 105 Resp: 4412
Ion Ratio Lower Upper
105 100
120 50.7 25.5 76.5




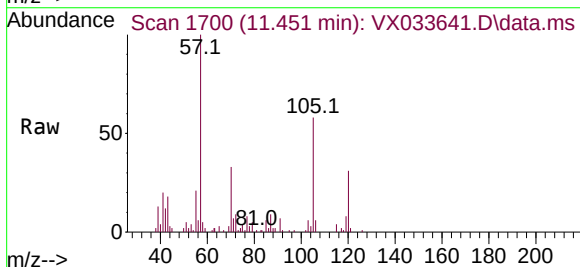




#81
trans-1,4-Dichloro-2-butene
Concen: 76.252 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16




Instrument :
MSVOA_X
ClientSampleId :
HARRISON-SILICA


Tgt Ion: 75 Resp: 50368
Ion Ratio Lower Upper
75 100
53 0.0 86.4 129.6#
89 0.0 37.4 56.2#

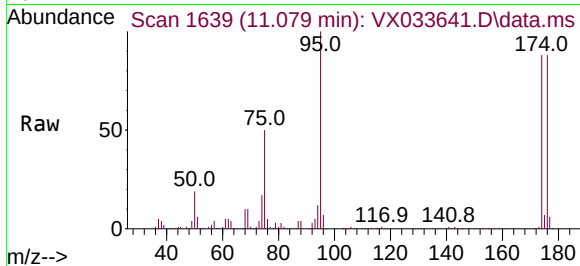

#84
1,2,4-Trimethylbenzene
Concen: 1.412 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX033641.D
Acq: 06 Jan 2023 19:16

Tgt Ion: 105 Resp: 9015
Ion Ratio Lower Upper
105 100
120 41.8 23.4 70.0

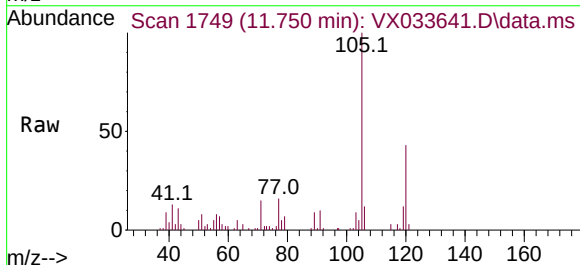



#93

1,2,4-Trichlorobenzene

Concen: 1.618 ug/l

RT: 13.585 min Scan# 2050

Delta R.T. -0.000 min

Lab File: VX033641.D

Acq: 06 Jan 2023 19:16





Instrument :

MSVOA_X

ClientSampleId :

HARRISON-SILICA

Tgt Ion:180	Resp:	60
Ion Ratio	Lower	Upper
180	100	
182	116.7	47.4 142.2
145	0.0	14.1 42.2#

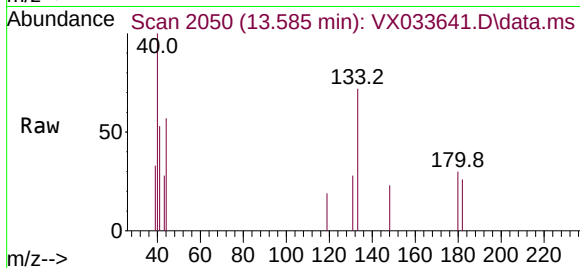

#95

Naphthalene

Concen: 3.245 ug/l




RT: 13.780 min Scan# 2082


Delta R.T. 0.006 min

Lab File: VX033641.D

Acq: 06 Jan 2023 19:16


Tgt Ion:128	Resp:	1042
Ion Ratio	Lower	Upper
128	100	
127	10.9	10.3 15.5
129	6.4	9.0 13.4#

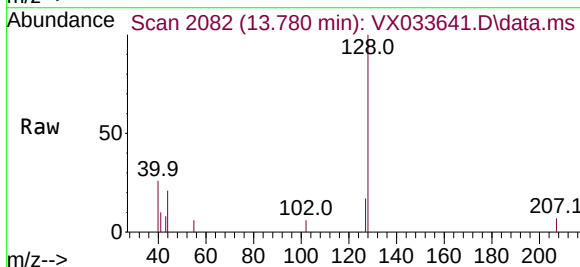



#96
 1,2,3-Trichlorobenzene
 Concen: 3.766 ug/l
 RT: 13.963 min Scan# 2112
 Delta R.T. -0.000 min
 Lab File: VX033641.D
 Acq: 06 Jan 2023 19:16

Instrument :
 MSVOA_X
 ClientSampleId :
 HARRISON-SILICA

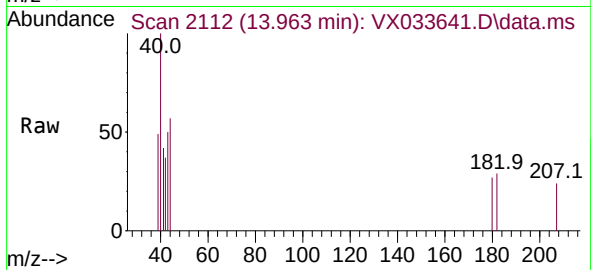

Tgt Ion:180 Resp: 46
 Ion Ratio Lower Upper
 180 100
 182 171.7 47.2 141.6#
 145 0.0 15.0 45.0#

