

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
 Data File : VX033644.D
 Acq On : 06 Jan 2023 20:26
 Operator : JC/MD
 Sample : 01042-07 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MARKETST-SILICA

Quant Time: Jan 07 04:31:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 05 04:43:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	169289	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	245514	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	220140	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	73045	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	91833	48.054	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	96.100%		
35) Dibromofluoromethane	5.385	113	76390	47.337	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.680%		
50) Toluene-d8	8.647	98	284222	49.276	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	98.560%		
62) 4-Bromofluorobenzene	11.079	95	101388	49.591	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	99.180%		
Target Compounds						Qvalue
11) Tert butyl alcohol	3.032	59	3753	11.955	ug/l #	80
13) Acrolein	2.337	56	1207	Below Cal	#	78
14) Allyl chloride	2.788	41	1770	0.670	ug/l #	65
15) Acrylonitrile	3.105	53	259	0.305	ug/l #	34
16) Acetone	2.404	43	4593	Below Cal		90
17) Carbon Disulfide	2.514	76	161	1.665	ug/l #	74
18) Methyl Acetate	2.782	43	4238	1.600	ug/l #	53
20) Methylene Chloride	2.794	84	424	Below Cal	#	74
23) Vinyl Acetate	3.447	43	2808	0.687	ug/l #	46
25) 2-Butanone	4.593	43	1974	1.582	ug/l #	89
31) Cyclohexane	5.477	56	9214	3.463	ug/l	93
36) 1,1-Dichloropropene	5.544	75	11304	5.171	ug/l #	50
37) Ethyl Acetate	4.733	43	1616	Below Cal	#	69
38) Carbon Tetrachloride	5.556	117	15302	6.615	ug/l #	16
39) Methylcyclohexane	7.385	83	9251	3.390	ug/l	93
40) Benzene	6.038	78	1217311	190.535	ug/l	99
42) 1,2-Dichloroethane	6.038	62	10495	4.407	ug/l #	74
43) Isopropyl Acetate	6.348	43	1039	0.278	ug/l #	62
51) 4-Methyl-2-Pentanone	8.549	43	593	0.251	ug/l #	37
52) Toluene	8.720	92	132757	31.606	ug/l	99
53) t-1,3-Dichloropropene	8.720	75	1483	0.720	ug/l #	1
55) 1,1,2-Trichloroethane	9.104	97	436	0.265	ug/l #	16
59) 2-Hexanone	9.445	43	486	0.278	ug/l #	61
67) Ethyl Benzene	10.195	91	4548	0.578	ug/l	97
68) m/p-Xylenes	10.299	106	4365	1.422	ug/l	96
69) o-Xylene	10.640	106	1633	0.537	ug/l	84
74) N-amyl acetate	10.884	43	728	0.348	ug/l #	43
76) 1,2,3-Trichloropropane	11.079	75	49228	36.787	ug/l #	35
81) trans-1,4-Dichloro-2-b...	11.079	75	49228	111.653	ug/l #	7
84) 1,2,4-Trimethylbenzene	11.756	105	863	0.203	ug/l	87
95) Naphthalene	13.780	128	1968	3.477	ug/l #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010623\
Data File : VX033644.D
Acq On : 06 Jan 2023 20:26
Operator : JC/MD
Sample : 01042-07 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MARKETST-SILICA

Quant Time: Jan 07 04:31:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 05 04:43:25 2023
Response via : Initial Calibration




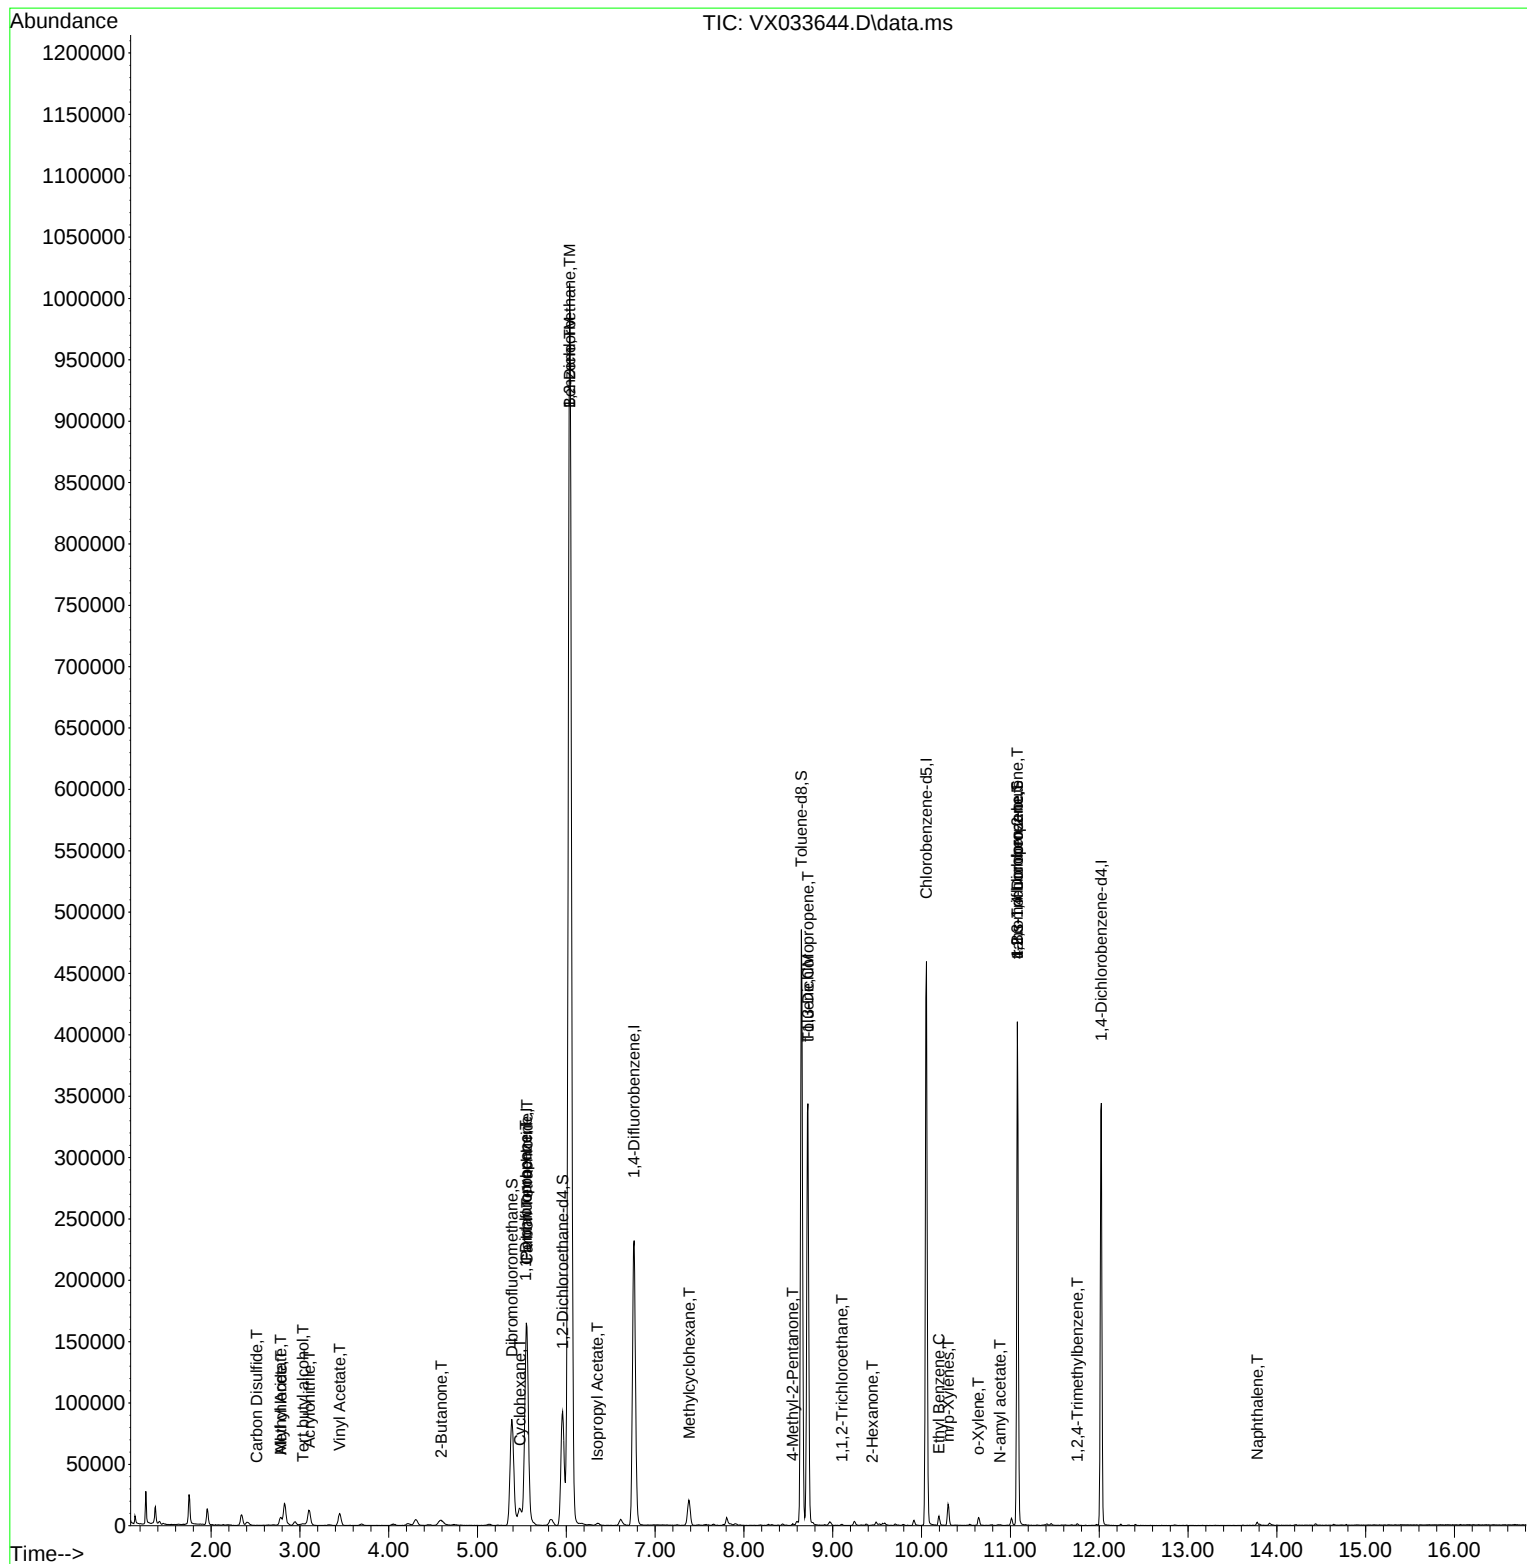




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26




Instrument :
MSVOA_X
ClientSampleId :
MARKETST-SILICA


Tgt Ion:168 Resp: 169289
Ion Ratio Lower Upper
168 100
99 51.7 41.4 62.2

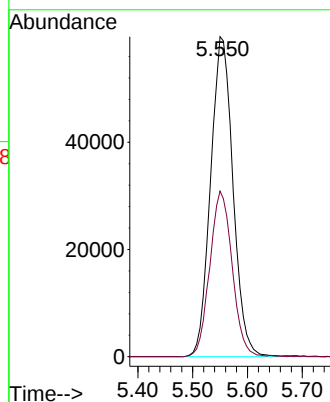

#11
Tert butyl alcohol
Concen: 11.955 ug/l
RT: 3.032 min Scan# 319
Delta R.T. 0.018 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26

Tgt Ion: 59 Resp: 3753
Ion Ratio Lower Upper
59 100
57 0.0 5.5 8.3#

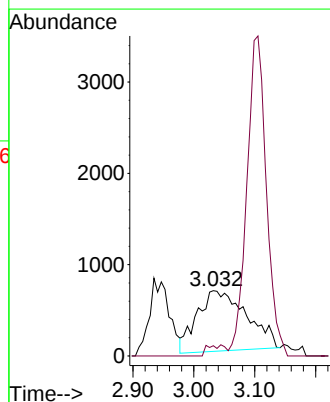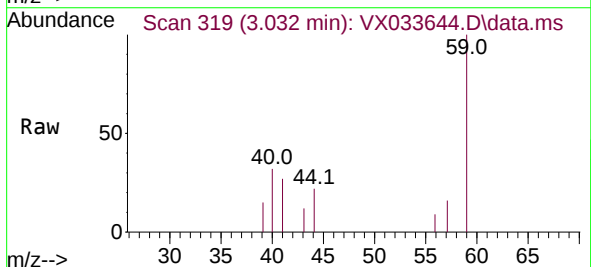



#13

Acrolein

Concen: Below Cal

RT: 2.337 min Scan# 205

Delta R.T. 0.097 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :





MARKETST-SILICA

Tgt Ion: 56 Resp: 1207

Ion Ratio Lower Upper

56 100

55 52.9 56.9 85.3#

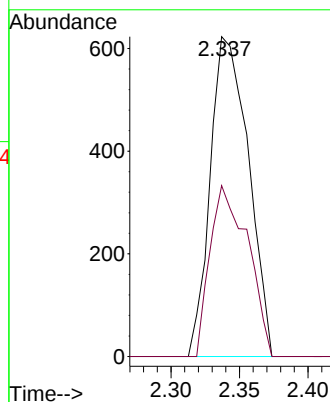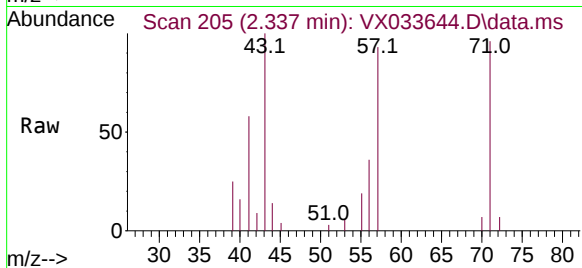

#14

Allyl chloride

Concen: 0.670 ug/l

RT: 2.788 min Scan# 279

Delta R.T. 0.122 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26




Tgt Ion: 41 Resp: 1770


Ion Ratio Lower Upper

41 100

39 46.3 53.3 79.9#

76 0.0 25.0 37.4#

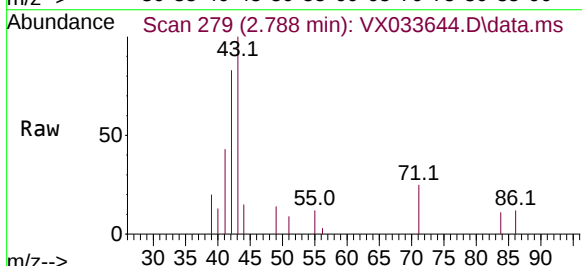



#15

Acrylonitrile

Concen: 0.305 ug/l

RT: 3.105 min Scan# 31

Delta R.T. 0.037 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :

MARKETST-SILICA





Tgt Ion: 53 Resp: 259

Ion Ratio Lower Upper

53 100

52 0.0 66.7 100.1#

51 42.1 29.8 44.8

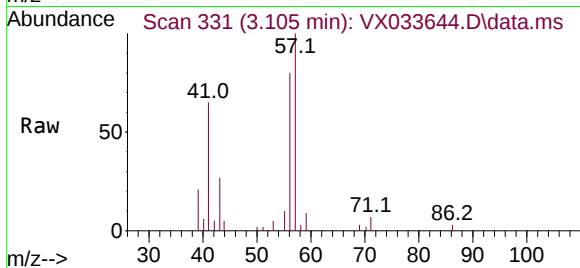

#16

Acetone

Concen: Below Cal

RT: 2.404 min Scan# 216

Delta R.T. 0.006 min

Lab File: VX033644.D




Acq: 06 Jan 2023 20:26


Tgt Ion: 43 Resp: 4593

Ion Ratio Lower Upper

43 100

58 23.2 22.9 34.3

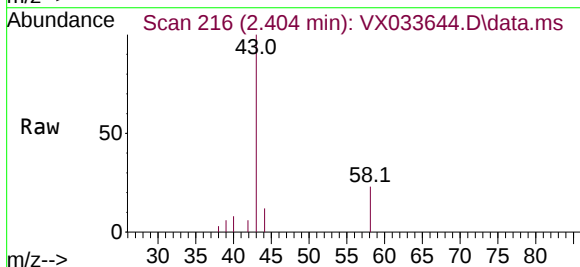

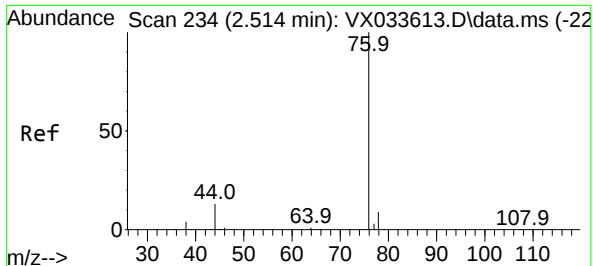

#17

Carbon Disulfide

Concen: 1.665 ug/l

RT: 2.514 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :





MARKETST-SILICA

Tgt Ion: 76 Resp: 161

Ion Ratio Lower Upper

76 100

78 0.0 7.6 11.4#

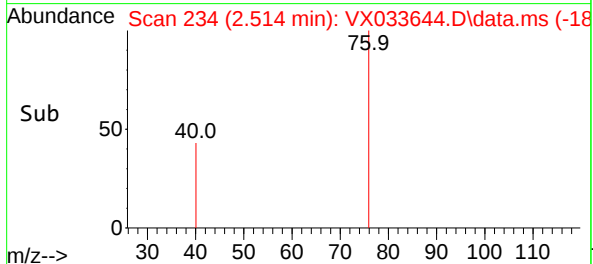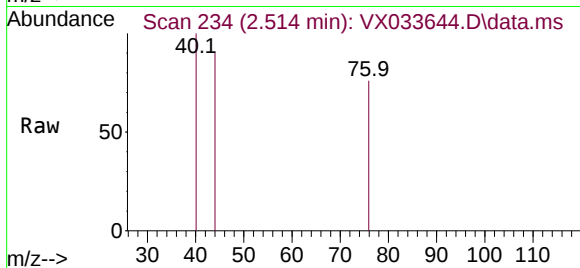

#18

Methyl Acetate

Concen: 1.600 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.079 min

Lab File: VX033644.D




Acq: 06 Jan 2023 20:26


Tgt Ion: 43 Resp: 4238

Ion Ratio Lower Upper

43 100

74 0.0 17.9 26.9#


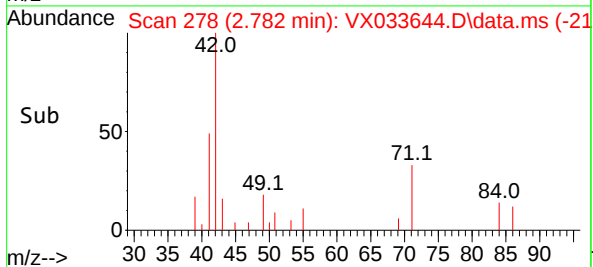

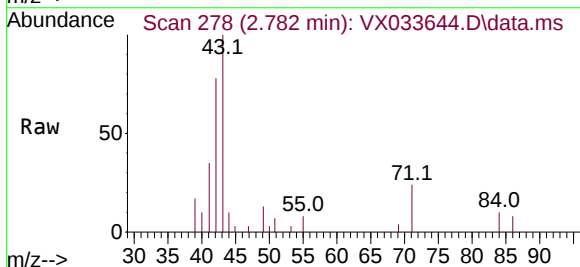




#20
Methylene Chloride
Concen: Below Cal
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26




Instrument :
MSVOA_X
ClientSampleId :
MARKETST-SILICA


Tgt Ion: 84 Resp: 424
Ion Ratio Lower Upper
84 100
49 97.0 97.6 146.4#
51 32.7 30.4 45.6
86 94.7 49.7 74.5#

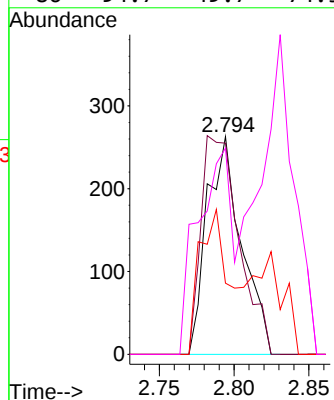

#23
Vinyl Acetate
Concen: 0.687 ug/l
RT: 3.447 min Scan# 387
Delta R.T. -0.274 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26

Tgt Ion: 43 Resp: 2808
Ion Ratio Lower Upper
43 100
86 30.5 8.3 12.5#

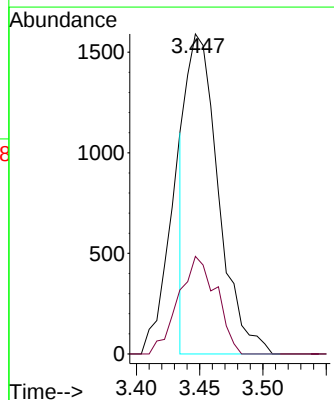



#25

2-Butanone

Concen: 1.582 ug/l

RT: 4.593 min Scan# 51

Delta R.T. 0.030 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :





MARKETST-SILICA

Tgt Ion: 43 Resp: 1974

Ion Ratio Lower Upper

43 100

72 19.0 19.8 29.6#

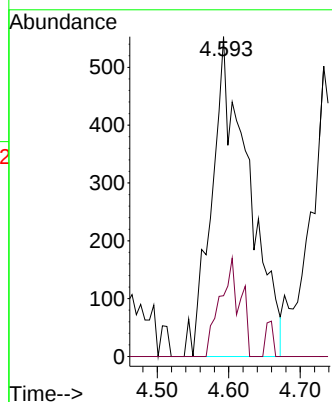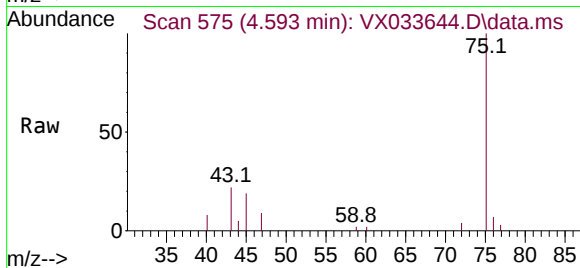

#31

Cyclohexane

Concen: 3.463 ug/l

RT: 5.477 min Scan# 720

Delta R.T. 0.006 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26




Tgt Ion: 56 Resp: 9214


Ion Ratio Lower Upper

56 100

69 32.1 24.6 36.8

84 82.6 72.2 108.2

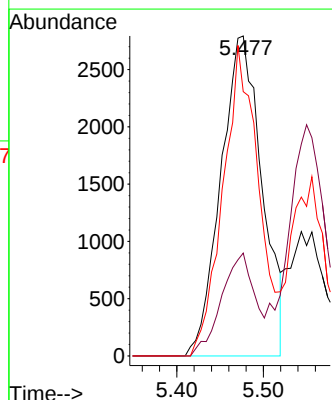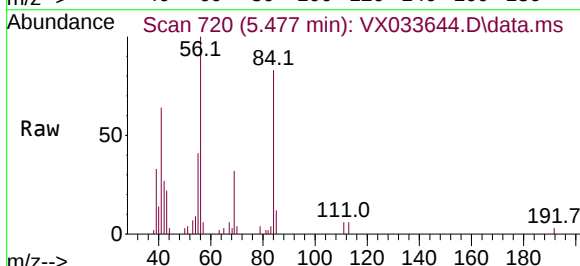



#33

1,2-Dichloroethane-d4

Concen: 48.054 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :





MARKETST-SILICA

Tgt Ion: 65 Resp: 91833

Ion Ratio Lower Upper

65 100

67 51.6 0.0 104.8

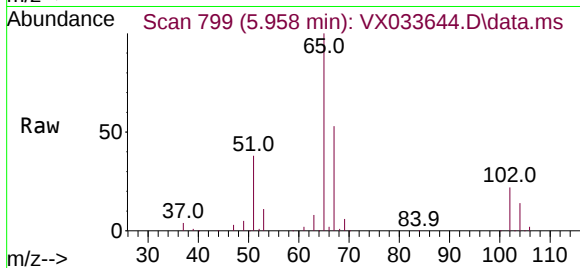

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26




Tgt Ion: 114 Resp: 245514


Ion Ratio Lower Upper

114 100

63 19.4 0.0 40.0

88 14.3 0.0 29.6

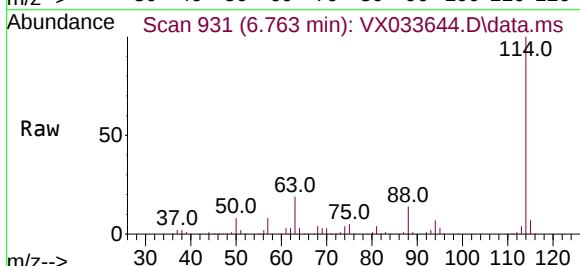

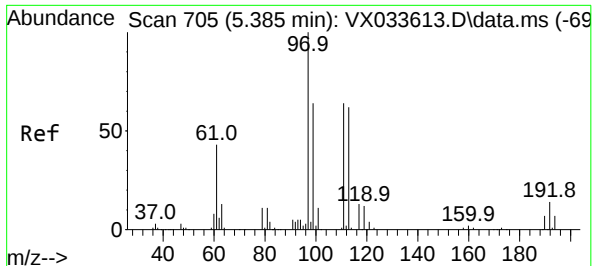

#35

Dibromofluoromethane

Concen: 47.337 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.000 min

Lab File: VX033644.D


Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :

MARKETST-SILICA






Tgt Ion:113 Resp: 76390

Ion Ratio Lower Upper

113 100

111 101.9 81.2 121.8

192 22.5 18.2 27.2

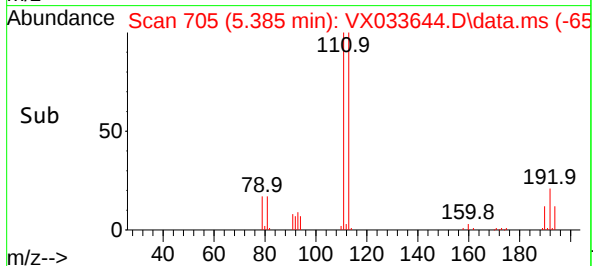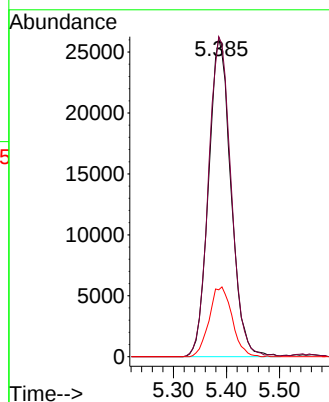

#36

1,1-Dichloropropene

Concen: 5.171 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.146 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26




Tgt Ion: 75 Resp: 11304


Ion Ratio Lower Upper

75 100

110 9.8 18.0 54.0#

77 0.0 24.5 36.7#

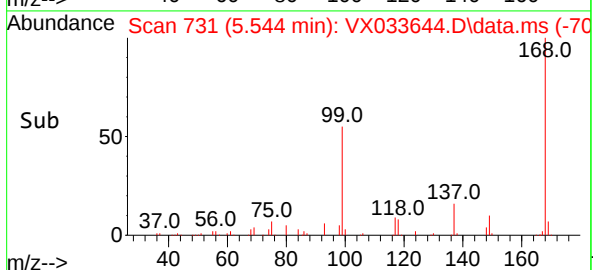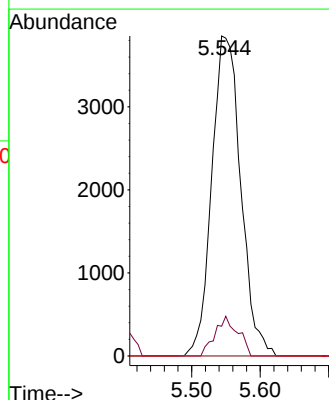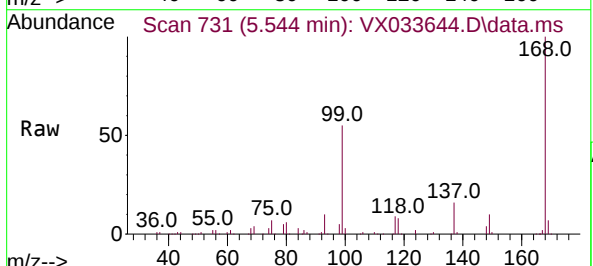



#37

Ethyl Acetate

Concen: Below Cal

RT: 4.733 min Scan# 598

Delta R.T. 0.018 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26





Instrument :

MSVOA_X

ClientSampleId :

MARKETST-SILICA

Tgt Ion: 43	Resp:	1616
Ion	Ratio	Lower Upper
43	100	
61	0.0	10.6 16.0#
70	0.0	8.1 12.1#

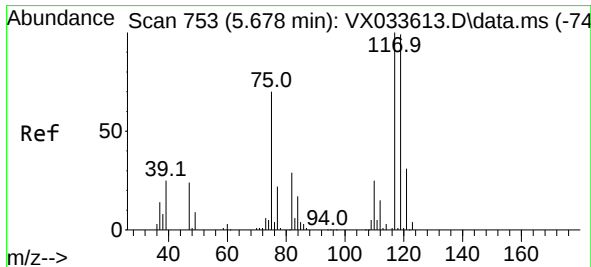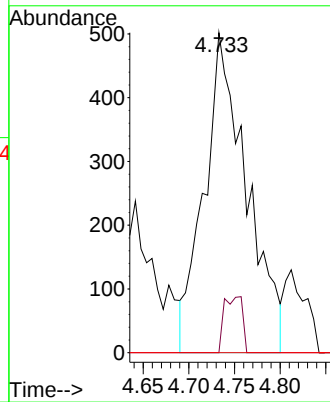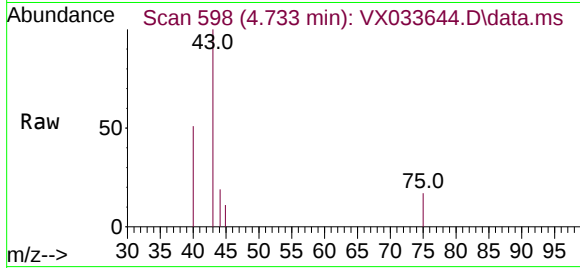

#38

Carbon Tetrachloride

Concen: 6.615 ug/l




RT: 5.556 min Scan# 733


Delta R.T. -0.122 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Tgt Ion: 117	Resp:	15302
Ion	Ratio	Lower Upper
117	100	
119	6.7	78.8 118.2#
121	0.0	24.9 37.3#


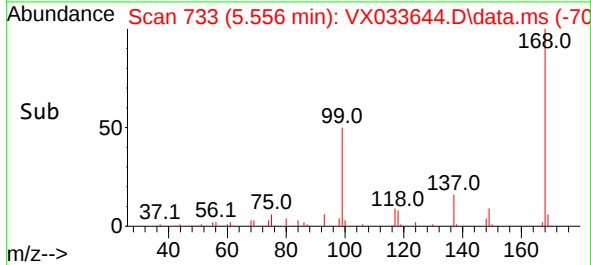

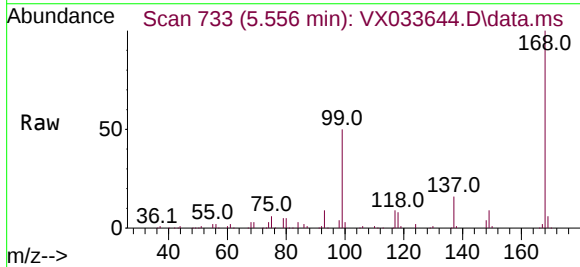




#39
Methylcyclohexane
Concen: 3.390 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. 0.006 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26




Instrument :
MSVOA_X
ClientSampleId :
MARKETST-SILICA


Tgt Ion: 83 Resp: 9251
Ion Ratio Lower Upper
83 100
55 71.8 61.4 92.2
98 44.4 40.2 60.2

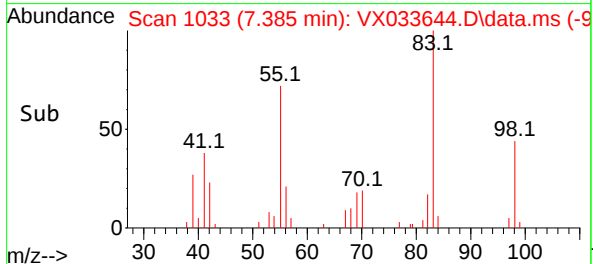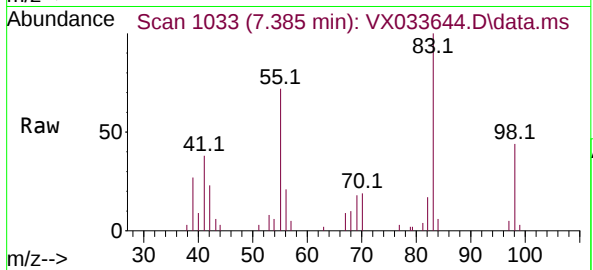

#40
Benzene
Concen: 190.535 ug/l
RT: 6.038 min Scan# 812
Delta R.T. -0.000 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26

Tgt Ion: 78 Resp: 1217311
Ion Ratio Lower Upper
78 100
77 23.5 19.0 28.6

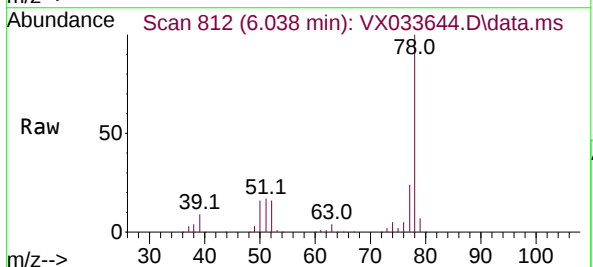

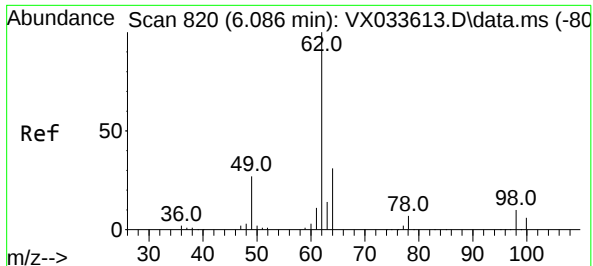

#42

1,2-Dichloroethane

Concen: 4.407 ug/l

RT: 6.038 min Scan# 81

Delta R.T. -0.049 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :





MARKETST-SILICA

Tgt Ion: 62 Resp: 10495

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.0

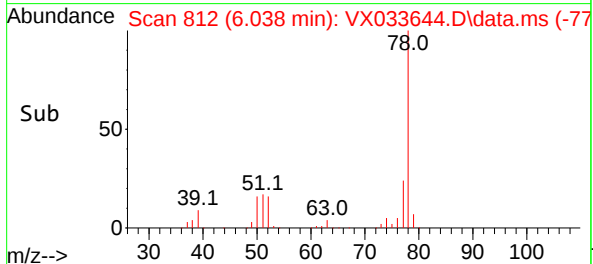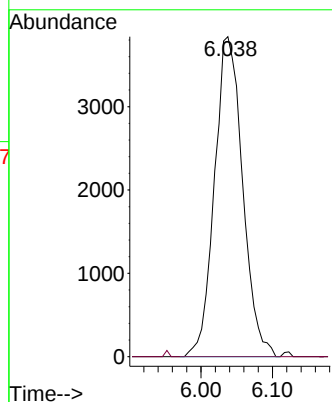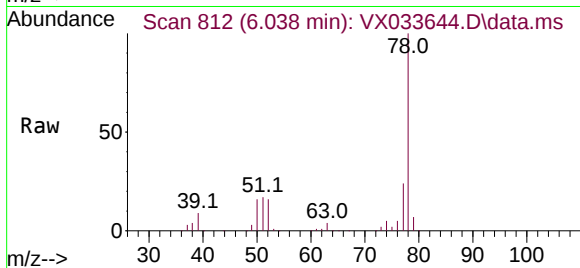

#43

Isopropyl Acetate

Concen: 0.278 ug/l

RT: 6.348 min Scan# 863

Delta R.T. 0.006 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26




Tgt Ion: 43 Resp: 1039


Ion Ratio Lower Upper

43 100

61 0.0 15.2 22.8#

87 0.0 10.6 16.0#



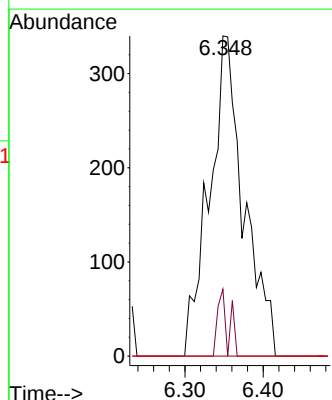
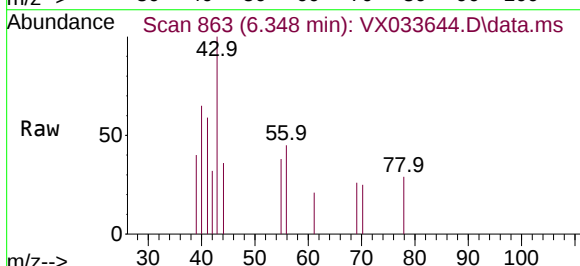


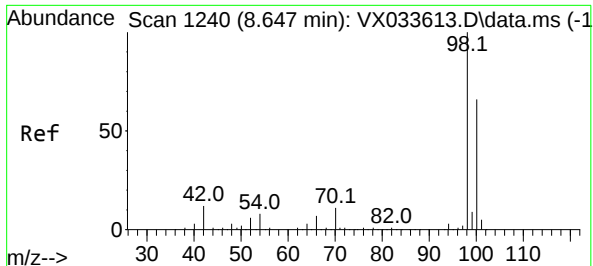

#50
Toluene-d8
Concen: 49.276 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26




Instrument :
MSVOA_X
ClientSampleId :
MARKETST-SILICA


Tgt Ion: 98 Resp: 284222
Ion Ratio Lower Upper
98 100
100 66.0 53.6 80.4

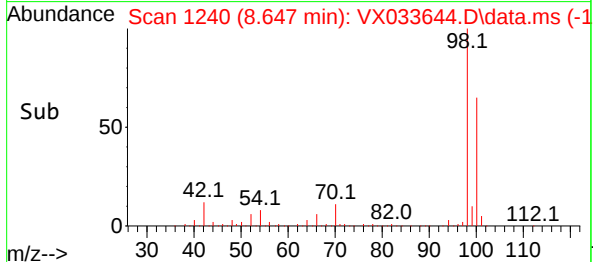

#51
4-Methyl-2-Pentanone
Concen: 0.251 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.024 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26

Tgt Ion: 43 Resp: 593
Ion Ratio Lower Upper
43 100
58 0.0 30.5 45.7#

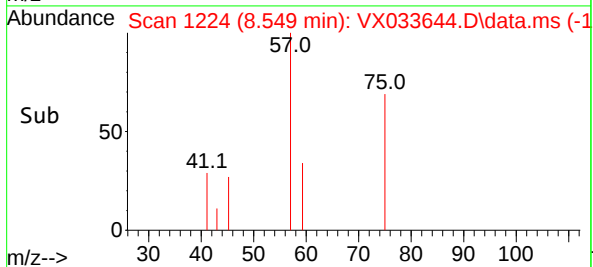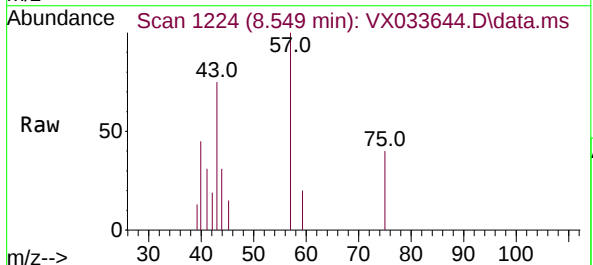



#52

Toluene

Concen: 31.606 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :





MARKETST-SILICA

Tgt Ion: 92 Resp: 132757

Ion Ratio Lower Upper

92 100

91 170.0 135.4 203.2

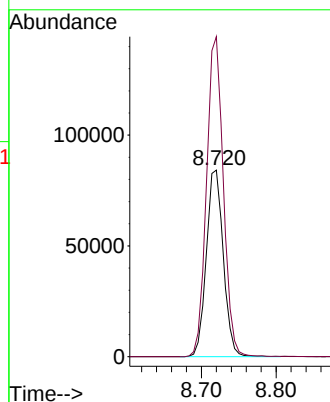

#53

t-1,3-Dichloropropene

Concen: 0.720 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.256 min

Lab File: VX033644.D




Acq: 06 Jan 2023 20:26


Tgt Ion: 75 Resp: 1483

Ion Ratio Lower Upper

75 100

77 178.2 25.3 37.9#



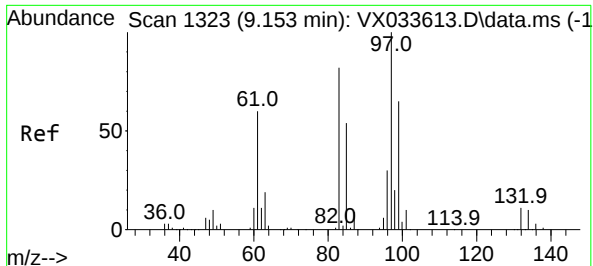

#55

1,1,2-Trichloroethane

Concen: 0.265 ug/l

RT: 9.104 min Scan# 1315

Delta R.T. -0.049 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :

MARKETST-SILICA

Tgt Ion: 97 Resp: 436





Ion Ratio Lower Upper

97 100

83 0.0 65.7 98.5#

85 0.0 43.4 65.0#

99 0.0 51.7 77.5#

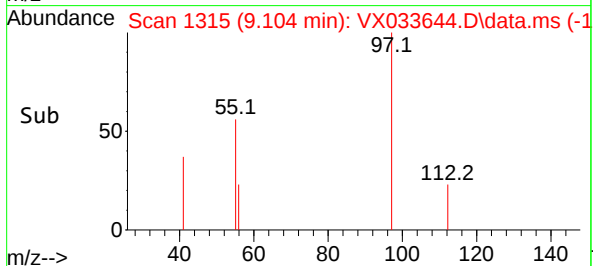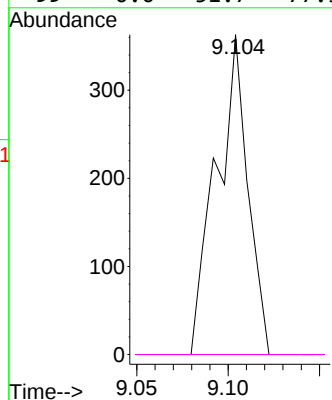

#59

2-Hexanone

Concen: 0.278 ug/l

RT: 9.445 min Scan# 1371

Delta R.T. 0.012 min

Lab File: VX033644.D




Acq: 06 Jan 2023 20:26


Tgt Ion: 43 Resp: 486

Ion Ratio Lower Upper

43 100

58 25.3 26.6 79.8#

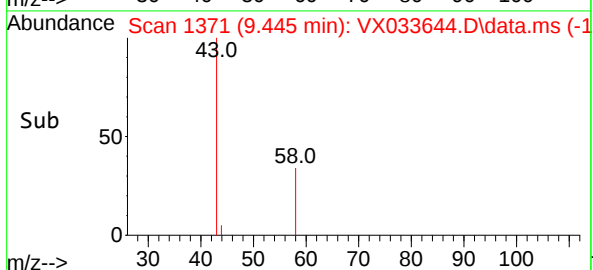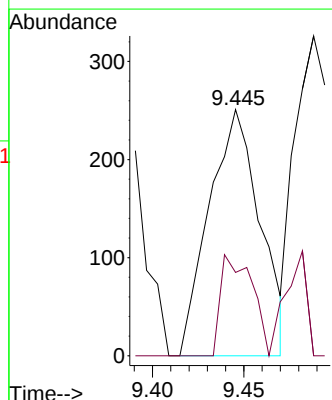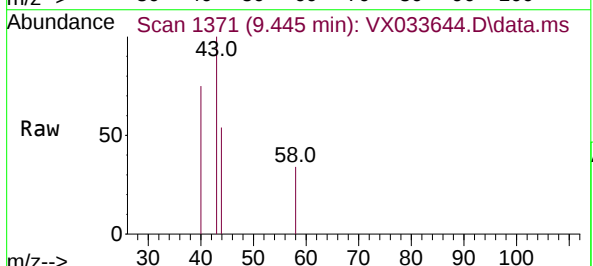



#62

4-Bromofluorobenzene

Concen: 49.591 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :

MARKETST-SILICA





Tgt Ion: 95 Resp: 101388

Ion Ratio Lower Upper

95 100

174 90.8 0.0 180.4

176 87.0 0.0 176.2

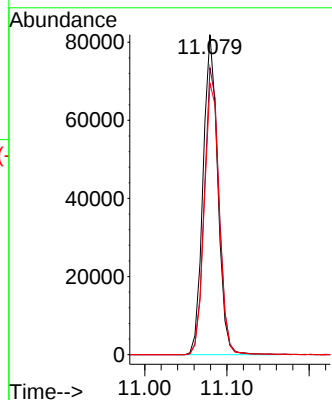

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26




Tgt Ion: 117 Resp: 220140


Ion Ratio Lower Upper

117 100

82 52.0 42.2 63.2

119 32.5 26.2 39.4

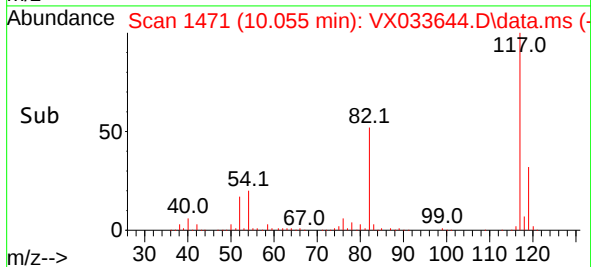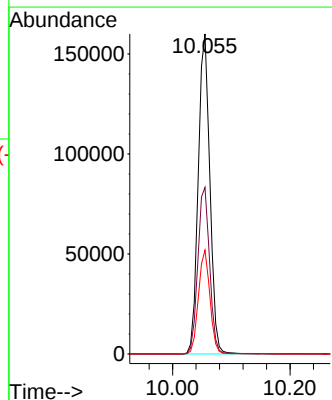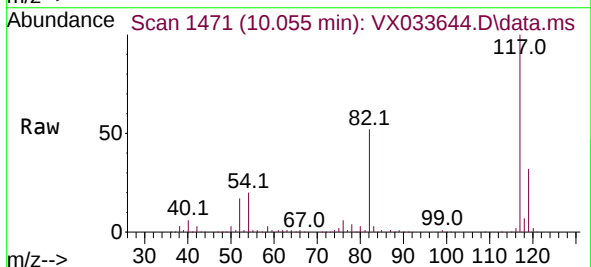



#67

Ethyl Benzene

Concen: 0.578 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. -0.000 min

Lab File: VX033644.D

Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :





MARKETST-SILICA

Tgt Ion: 91 Resp: 4548

Ion Ratio Lower Upper

91 100

106 33.8 25.9 38.9

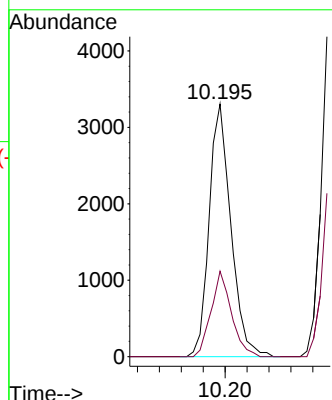

#68

m/p-Xylenes

Concen: 1.422 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX033644.D




Acq: 06 Jan 2023 20:26


Tgt Ion: 106 Resp: 4365

Ion Ratio Lower Upper

106 100

91 194.1 159.6 239.4


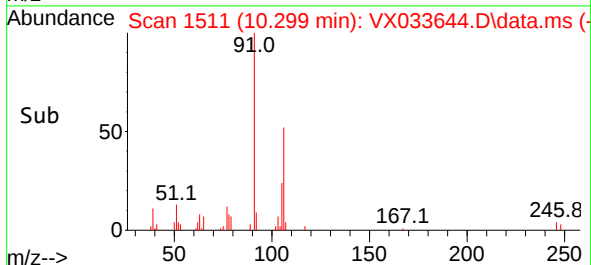
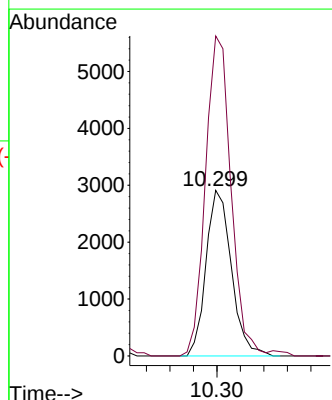
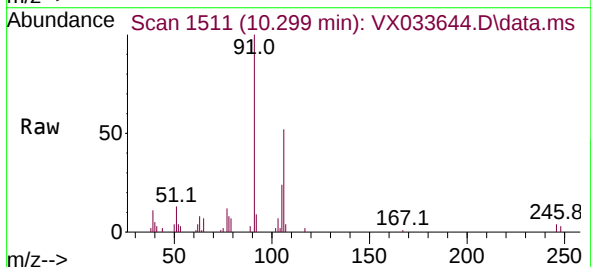




#69
o-Xylene
Concen: 0.537 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26




Instrument :
MSVOA_X
ClientSampleId :
MARKETST-SILICA


Tgt Ion:106 Resp: 1633
Ion Ratio Lower Upper
106 100
91 184.1 104.1 312.3

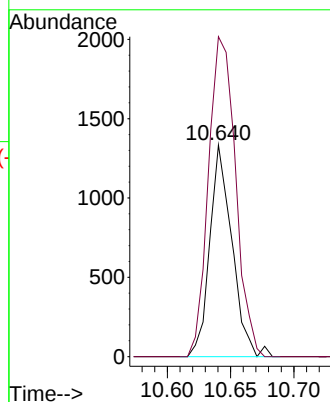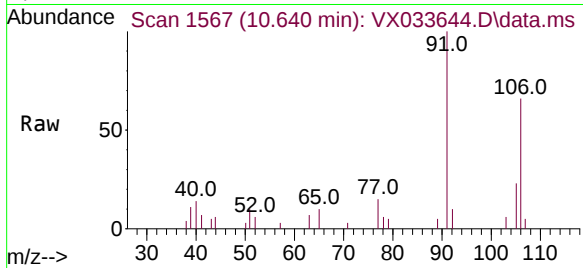

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26

Tgt Ion:152 Resp: 73045
Ion Ratio Lower Upper
152 100
115 55.4 38.5 115.5
150 157.6 0.0 340.4




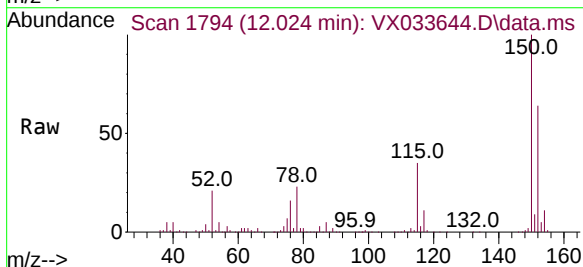




#74
N-amy1 acetate
Concen: 0.348 ug/l
RT: 10.884 min Scan# 1607
Delta R.T. 0.043 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26




Instrument :
MSVOA_X
ClientSampleId :
MARKETST-SILICA


Tgt Ion:	43	Resp:	728
Ion	Ratio	Lower	Upper
43	100		
70	0.0	33.4	50.0#
55	0.0	18.6	27.8#
61	0.0	19.0	28.6#

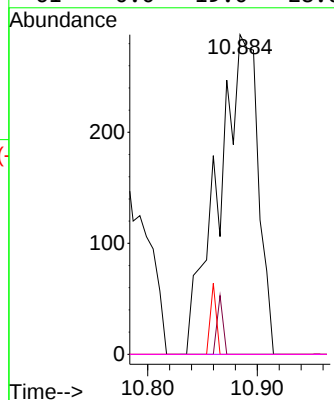

#76
1,2,3-Trichloropropane
Concen: 36.787 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26

Tgt Ion:	75	Resp:	49228
Ion	Ratio	Lower	Upper
75	100		
77	1.3	21.3	63.9#



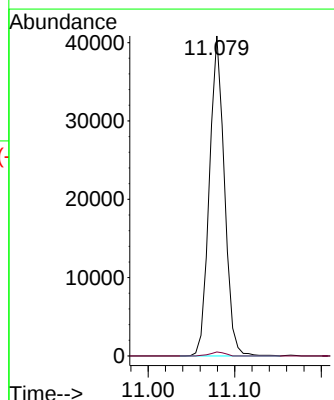
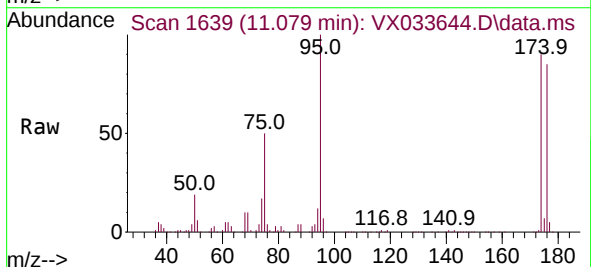




#81
trans-1,4-Dichloro-2-butene
Concen: 111.653 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26




Instrument :
MSVOA_X
ClientSampleId :
MARKETST-SILICA


Tgt Ion: 75 Resp: 49228
Ion Ratio Lower Upper
75 100
53 0.0 86.4 129.6#
89 0.0 37.4 56.2#

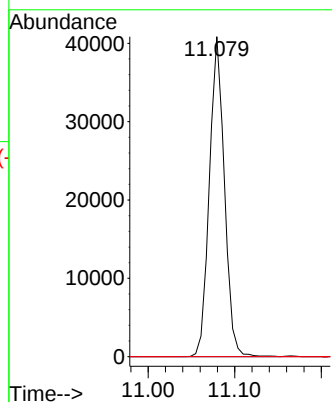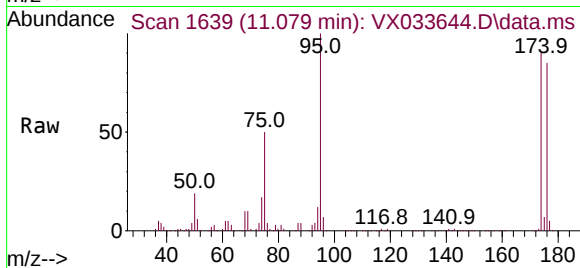

#84
1,2,4-Trimethylbenzene
Concen: 0.203 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX033644.D
Acq: 06 Jan 2023 20:26

Tgt Ion: 105 Resp: 863
Ion Ratio Lower Upper
105 100
120 38.4 23.4 70.0

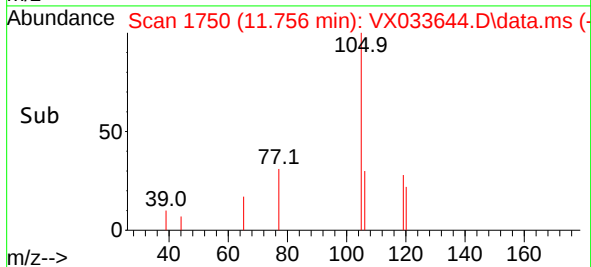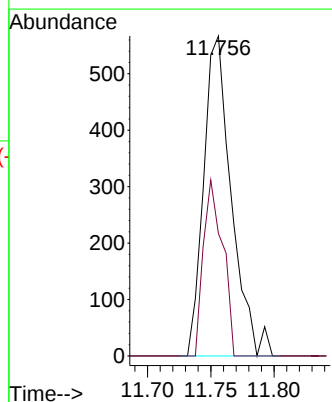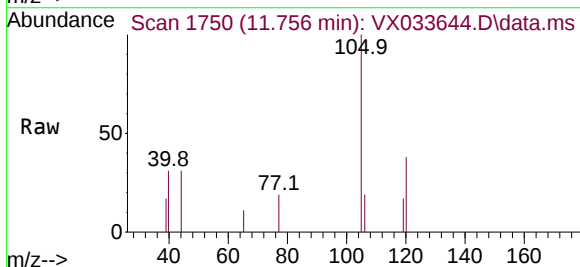



#95

Naphthalene

Concen: 3.477 ug/l

RT: 13.780 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX033644.D


Acq: 06 Jan 2023 20:26

Instrument :

MSVOA_X

ClientSampleId :

MARKETST-SILICA



Tgt Ion:128 Resp: 1968

Ion Ratio Lower Upper

128 100

127 9.6 10.3 15.5#

129 10.9 9.0 13.4

