
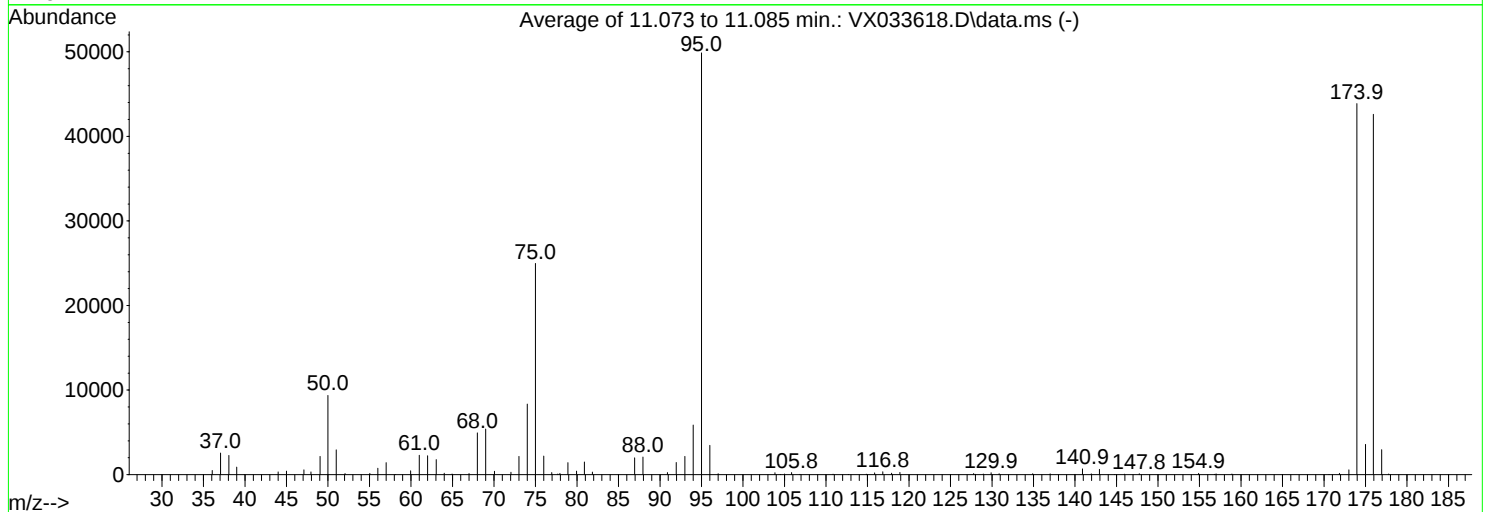


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX010623\  
Data File : VX033618.D  
Acq On : 06 Jan 2023 08:40  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X010423W.M  
Title : SW846 8260  
Last Update : Thu Jan 05 04:43:25 2023

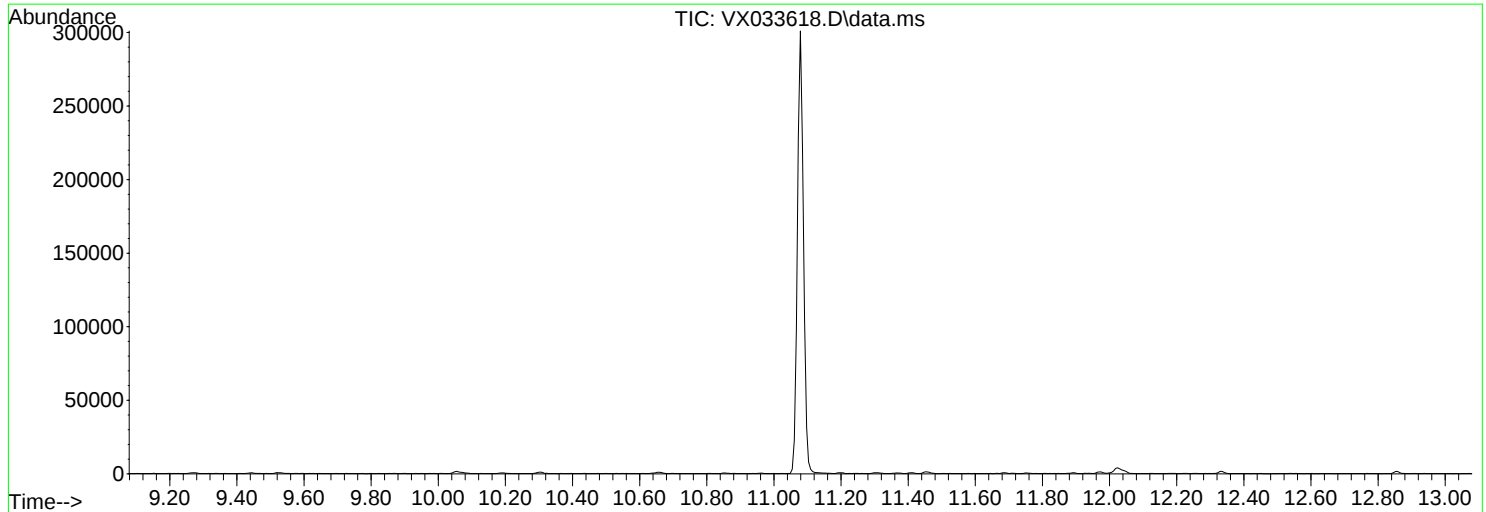

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 18.8  | 9369  | PASS      |
| 75     | 95      | 30     | 60     | 50.1  | 24971 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 49877 | PASS      |
| 96     | 95      | 5      | 9      | 7.0   | 3469  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.3   | 564   | PASS      |
| 174    | 95      | 50     | 100    | 88.0  | 43875 | PASS      |
| 175    | 174     | 5      | 9      | 8.2   | 3576  | PASS      |
| 176    | 174     | 95     | 101    | 97.1  | 42616 | PASS      |
| 177    | 176     | 5      | 9      | 6.9   | 2955  | PASS      |