

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX010719\
 Data File : VX006926.D
 Acq On : 07 Jan 2019 11:02
 Operator : JC/MD
 Sample : VX0107WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0107WBL01

Quant Time: Jan 08 06:45:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 19 15:20:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	669666	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	998038	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	925734	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	456844	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	347526	48.15	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.30%	
35) Dibromofluoromethane	5.50	113	313032	49.60	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.20%	
50) Toluene-d8	8.71	98	1178946	49.55	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.10%	
62) 4-Bromofluorobenzene	11.13	95	429265	49.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.52%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX010719\
Data File : VX006926.D
Acq On : 07 Jan 2019 11:02
Operator : JC/MD
Sample : VX0107WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0107WBL01

Quant Time: Jan 08 06:45:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 19 15:20:58 2018
Response via : Initial Calibration

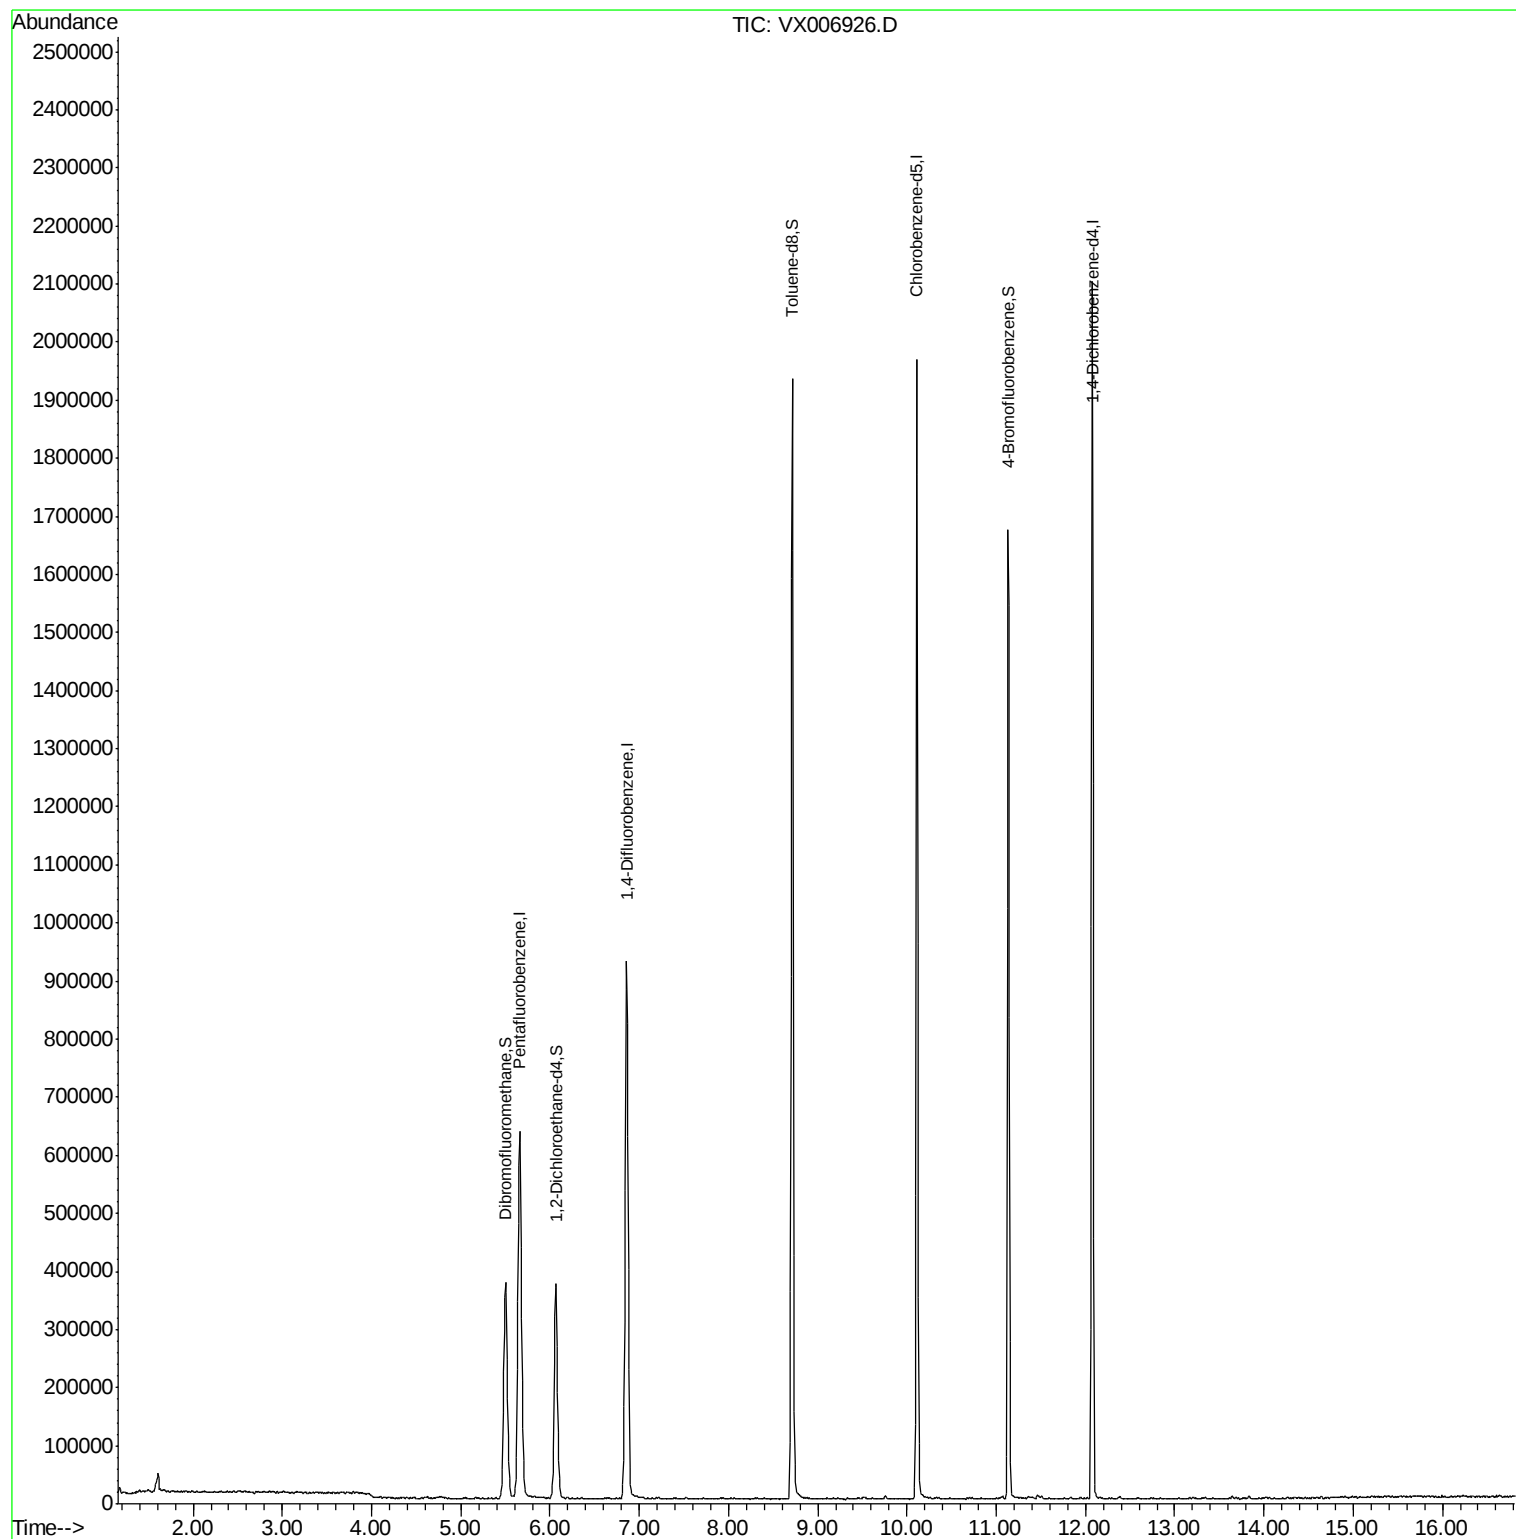

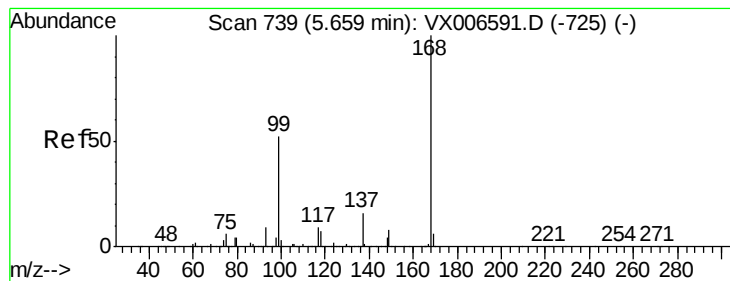

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.00 min

Lab File: VX006926.D

Acq: 07 Jan 2019 11:02

Instrument :

MSVOA_X

ClientSampled :


VX0107WBL01

Tot Ion:168 Resp: 669666

Ion Ratio Lower Upper

168 100

99 49.7 41.8 62.8

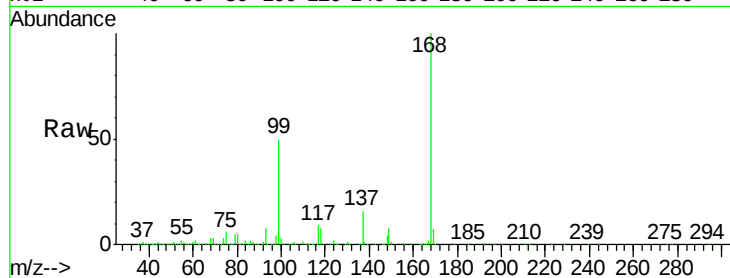

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

250000

200000



150000

100000

50000

0

Time-->

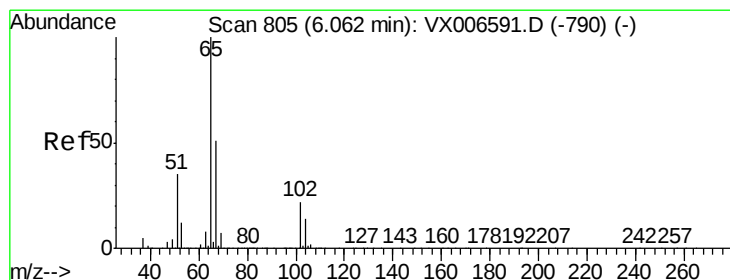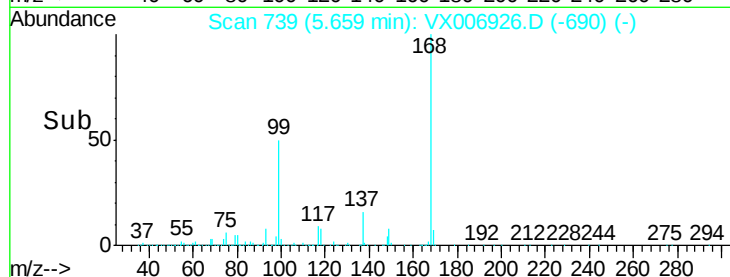

#33

1,2-Dichloroethane-d4

Concen: 48.151 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.01 min

Lab File: VX006926.D


Acq: 07 Jan 2019 11:02

Tgt Ion: 65 Resp: 347526

Ion Ratio Lower Upper

65 100

67 52.5 0.0 105.0

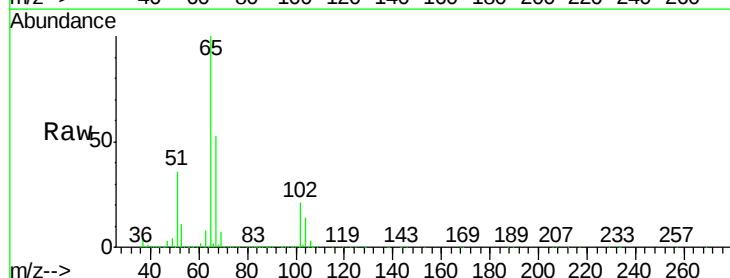

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07


150000


100000

50000

0

Time-->

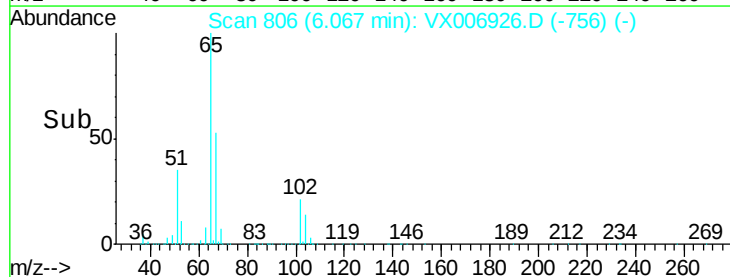

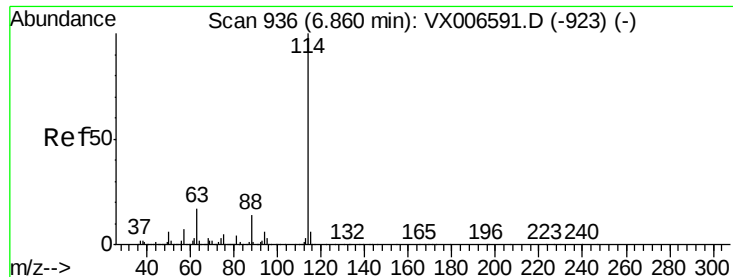

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX006926.D

Acq: 07 Jan 2019 11:02

Instrument :

MSVOA_X

ClientSampleId :

VX0107WBL01


Tot Ion:114 Resp: 998038

Ion Ratio Lower Upper

114 100

63 18.4 0.0 34.8




88 14.7 0.0 28.8

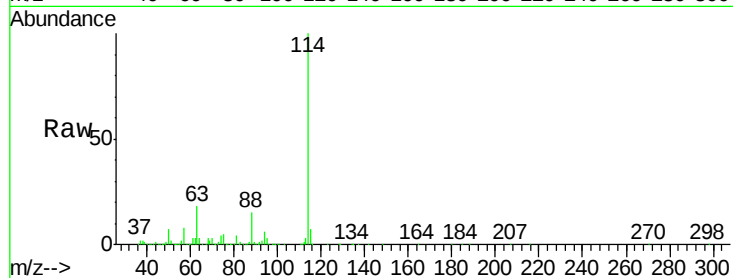

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

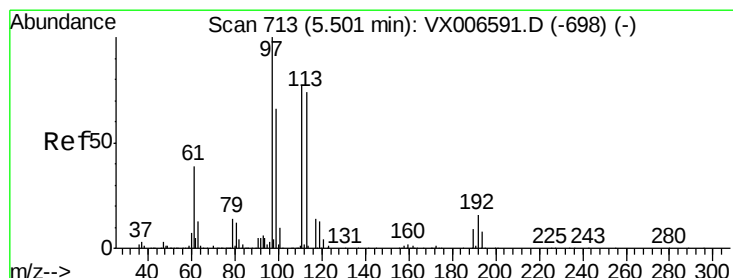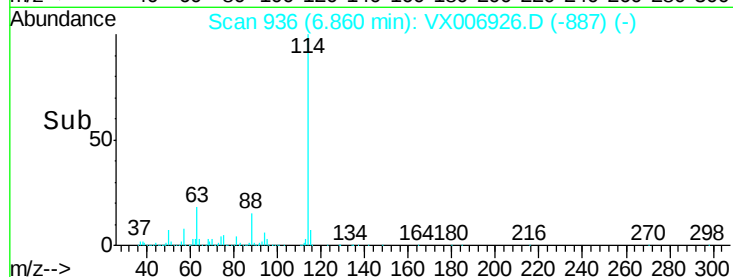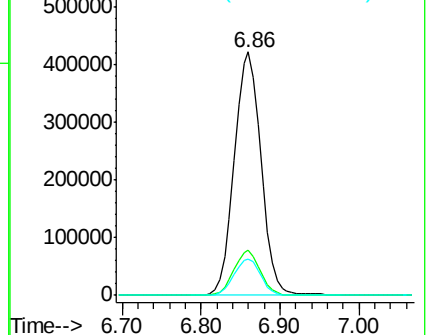

#35

Dibromofluoromethane

Concen: 49.598 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX006926.D

Acq: 07 Jan 2019 11:02


Tgt Ion:113 Resp: 313032

Ion Ratio Lower Upper

113 100

111 102.9 81.6 122.4



192 22.3 16.7 25.1

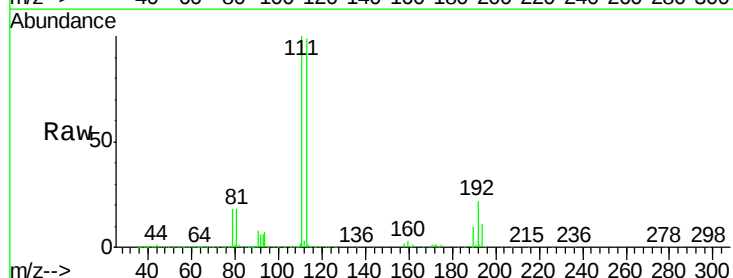


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

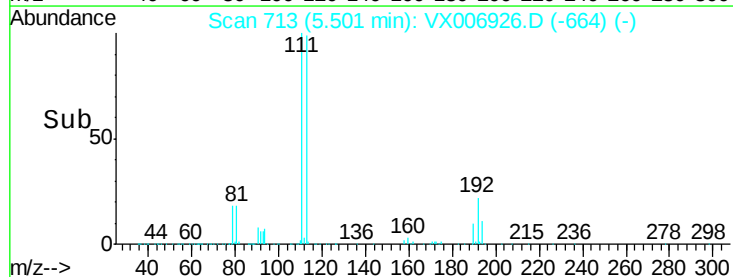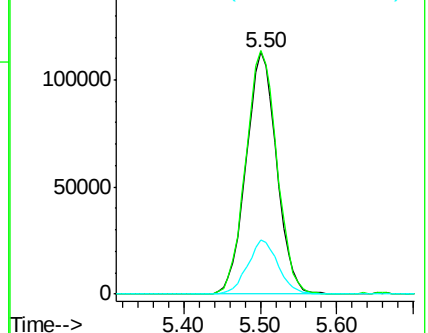

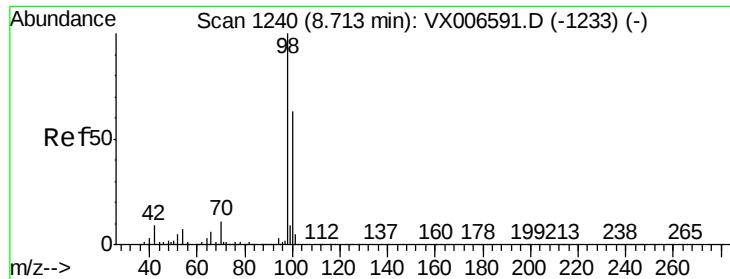

#50

Toluene-d8

Concen: 49.548 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX006926.D

Acq: 07 Jan 2019 11:02

Instrument :

MSVOA_X

ClientSampleId :


VX0107WBL01

Tot Ion: 98 Resp: 1178946

Ion Ratio Lower Upper

98 100

100 64.2 52.0 78.0

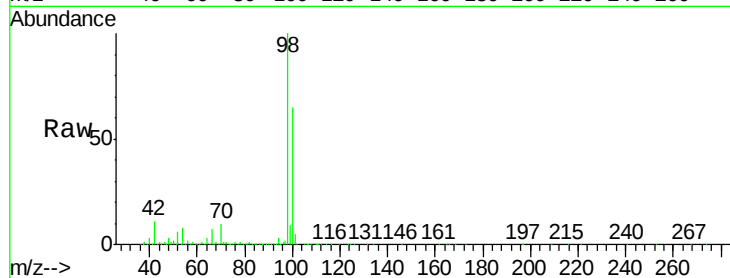

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

8.71

800000

600000



400000

200000

0

8.60 8.70 8.80 8.90

Time-->

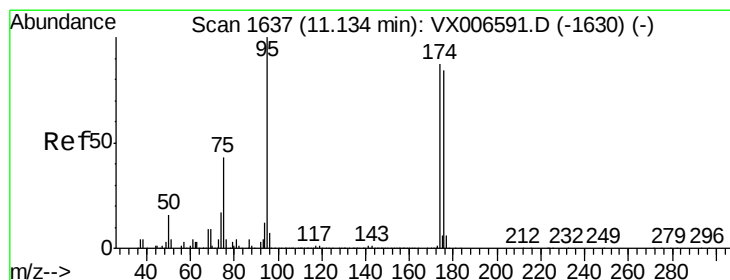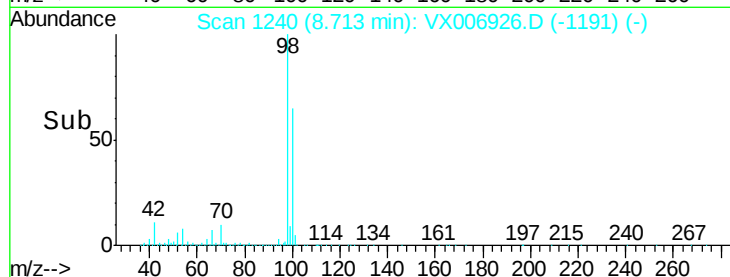

#62

4-Bromofluorobenzene

Concen: 49.259 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX006926.D

Acq: 07 Jan 2019 11:02


Tgt Ion: 95 Resp: 429265

Ion Ratio Lower Upper

95 100

174 92.4 0.0 182.2

176 90.2 0.0 178.8

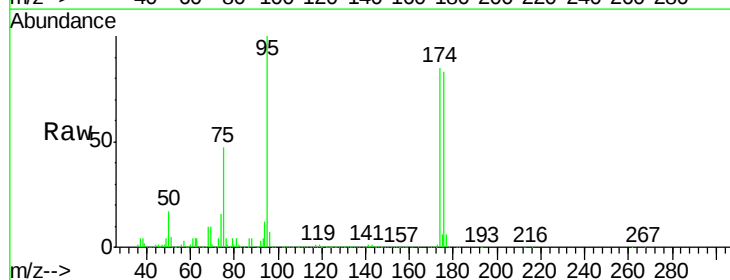

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

11.13

400000

300000


200000


100000

0

11.10 11.20

Time-->

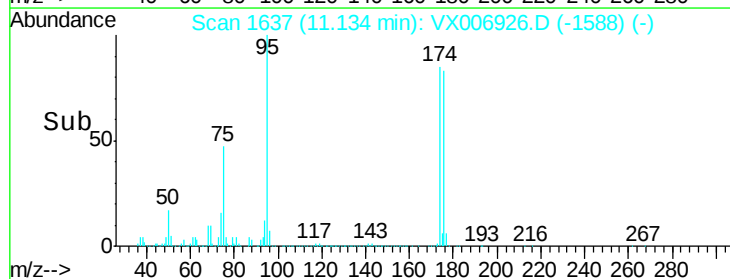

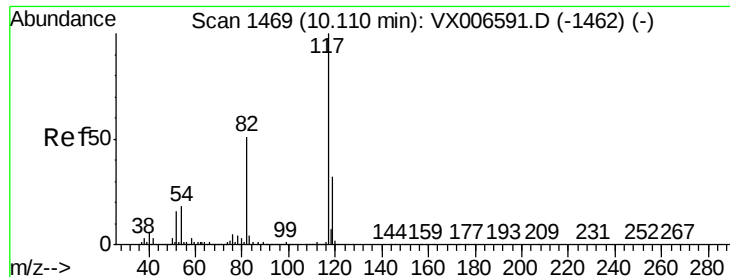

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX006926.D

Acq: 07 Jan 2019 11:02

Instrument :

MSVOA_X

ClientSampleId :

VX0107WBL01


Tot Ion:117 Resp: 925734

Ion Ratio Lower Upper

117 100

82 51.9 41.0 61.6




119 32.0 25.4 38.0

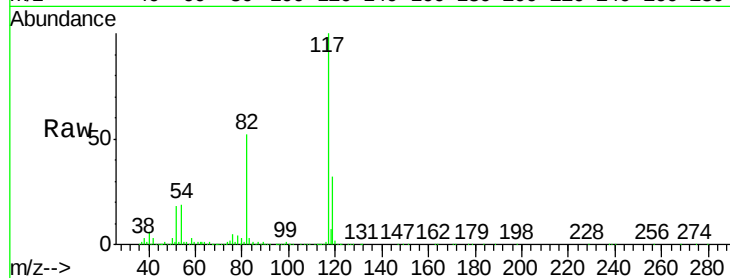

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

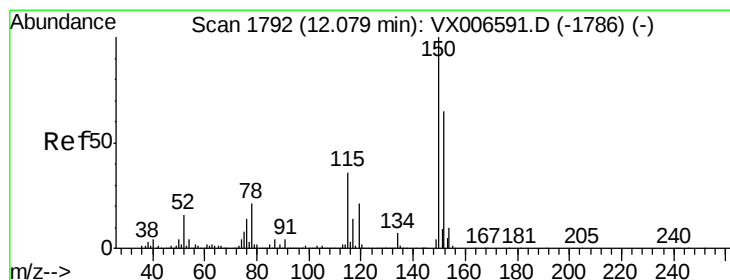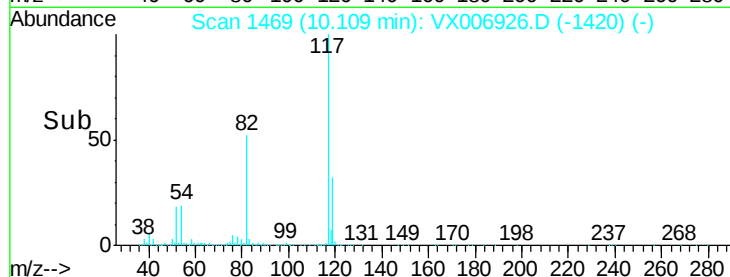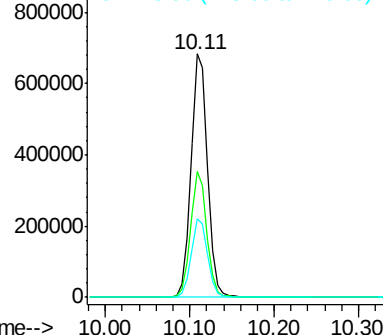

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX006926.D

Acq: 07 Jan 2019 11:02


Tgt Ion:152 Resp: 456844

Ion Ratio Lower Upper

152 100

115 54.1 39.1 117.2

150 157.3 0.0 344.8

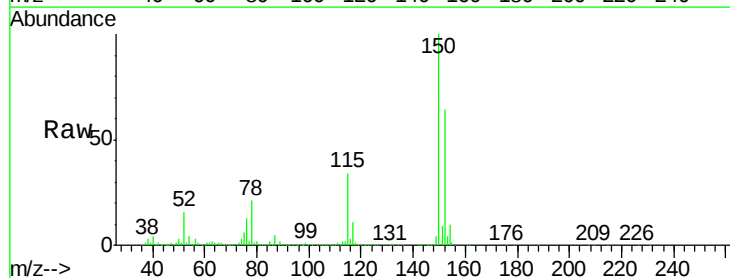

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

