


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010720\
 Data File : VX014443.D
 Acq On : 07 Jan 2020 12:35
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
 Title : SW846 8260
 Last Update : Tue Jan 07 15:54:41 2020

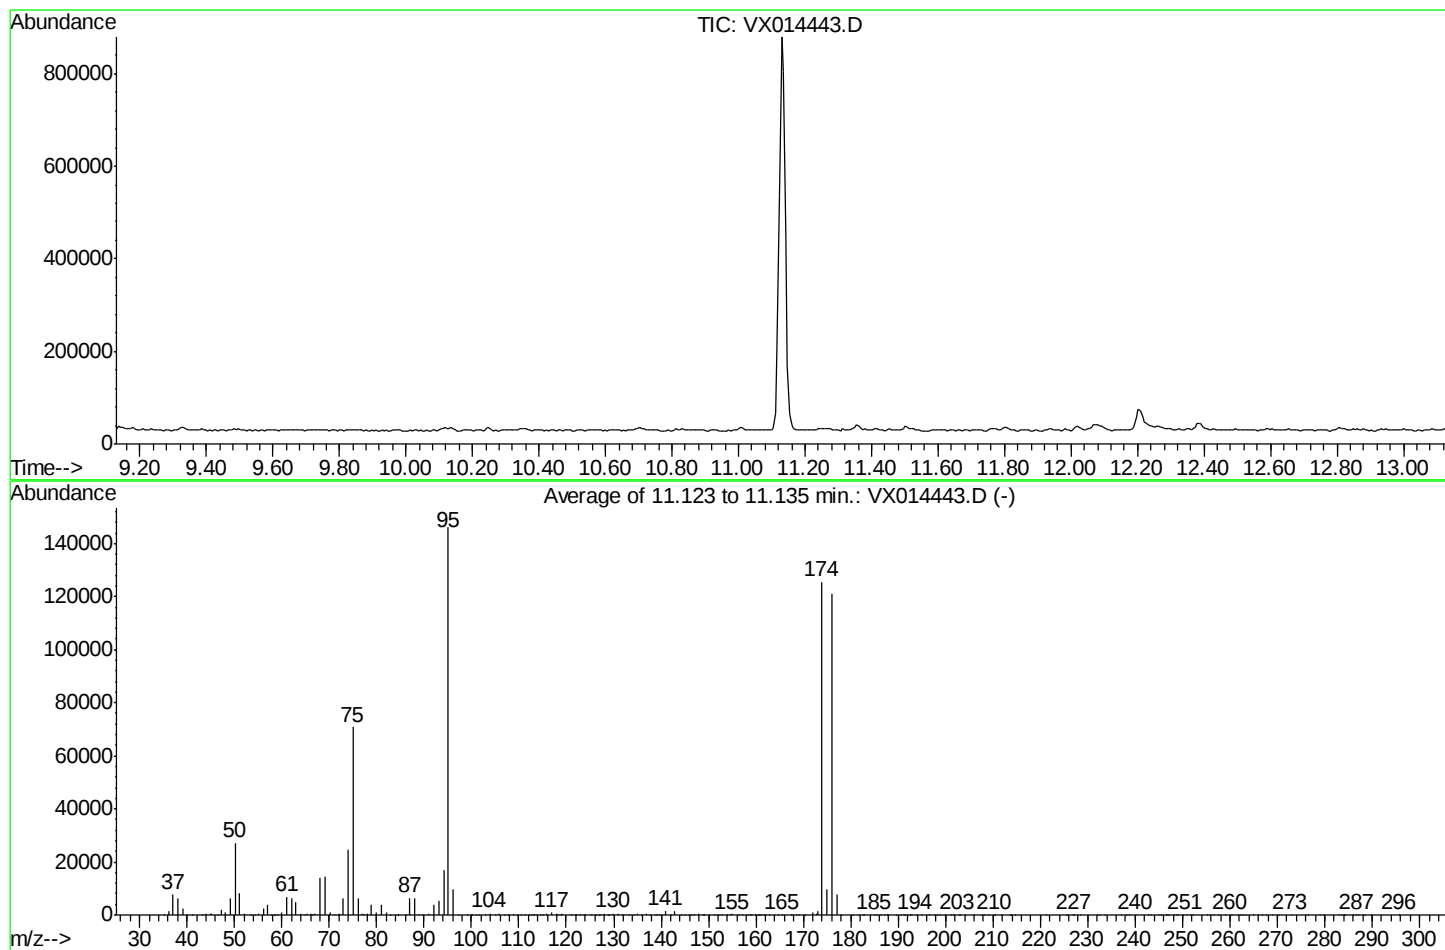

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	27023	PASS
75	95	30	60	48.4	70697	PASS
95	95	100	100	100.0	146098	PASS
96	95	5	9	6.6	9677	PASS
173	174	0.00	2	1.0	1262	PASS
174	95	50	100	85.9	125544	PASS
175	174	5	9	7.5	9469	PASS
176	174	95	101	96.6	121234	PASS
177	176	5	9	6.5	7915	PASS