

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010721\
 Data File : VX020527.D
 Acq On : 07 Jan 2021 12:28
 Operator : JC/MD
 Sample : VX0107MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK401

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M

Title : VOC Analysis

Signal : TIC: VX020527.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.386	46	49	61	rVB	208641	212219	14.07%	1.984%
2	1.697	95	100	111	rVB	166620	207975	13.78%	1.944%
3	2.343	199	206	220	rBV	336601	546091	36.19%	5.106%
4	2.557	238	241	245	rVB4	559	660	0.04%	0.006%
5	2.617	249	251	252	rBV	287	206	0.01%	0.002%
6	2.666	258	259	262	rVB2	497	380	0.03%	0.004%
7	2.703	263	265	268	rVB	304	221	0.01%	0.002%
8	2.739	268	271	273	rBV2	294	354	0.02%	0.003%
9	2.831	282	286	290	rVB4	1701	2372	0.16%	0.022%
10	2.989	303	312	322	rVV	6832	15722	1.04%	0.147%
11	3.380	374	376	381	rVB2	209	233	0.02%	0.002%
12	3.428	381	384	387	rBV2	305	345	0.02%	0.003%
13	3.532	397	401	403	rBV	180	184	0.01%	0.002%
14	3.587	408	410	413	rBV2	200	229	0.02%	0.002%
15	3.684	422	426	432	rVB3	242	484	0.03%	0.005%
16	3.733	432	434	436	rBV2	219	185	0.01%	0.002%
17	3.843	449	452	455	rBV2	141	222	0.01%	0.002%
18	4.178	503	507	512	rBV2	232	520	0.03%	0.005%
19	4.337	532	533	537	rBV2	250	245	0.02%	0.002%
20	4.532	553	565	579	rBV	100784	301259	19.97%	2.817%
21	4.745	599	600	602	rVB2	293	206	0.01%	0.002%
22	4.794	606	608	609	rVB	354	215	0.01%	0.002%
23	5.135	651	664	680	rBV	197175	596109	39.51%	5.573%
24	5.282	686	688	691	rBV4	181	190	0.01%	0.002%
25	5.452	712	716	718	rBV2	336	463	0.03%	0.004%
26	5.471	718	719	722	rVB2	416	362	0.02%	0.003%
27	5.556	729	733	737	rBV3	354	650	0.04%	0.006%
28	5.623	738	744	746	rBV4	357	503	0.03%	0.005%
29	5.897	786	789	792	rVB2	141	196	0.01%	0.002%
30	6.038	799	812	828	rBV2	512035	1508798	100.00%	14.106%
31	6.147	828	830	832	rVV3	943	901	0.06%	0.008%
32	6.166	832	833	836	rVB	615	365	0.02%	0.003%
33	6.257	847	848	852	rBV4	193	219	0.01%	0.002%
34	6.391	867	870	872	rBV	189	207	0.01%	0.002%
35	6.586	900	902	904	rBV	254	266	0.02%	0.002%
36	6.733	924	926	930	rVB2	234	266	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010721\
 Data File : VX020527.D
 Acq On : 07 Jan 2021 12:28
 Operator : JC/MD
 Sample : VX0107MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK401

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
 Title : VOC Analysis

37	6.824	930	941	958	rBV	325312	775833	51.42%	7.253%
38	7.007	969	971	974	rVB2	238	303	0.02%	0.003%
39	7.080	980	983	988	rVB2	172	298	0.02%	0.003%
40	7.165	990	997	1006	rVB3	8083	18408	1.22%	0.172%
41	7.251	1006	1011	1013	rBV2	234	323	0.02%	0.003%
42	7.367	1020	1030	1044	rBV	313469	679954	45.07%	6.357%
43	7.495	1050	1051	1053	rVV	247	215	0.01%	0.002%
44	7.525	1053	1056	1064	rVB2	1026	1848	0.12%	0.017%
45	7.635	1072	1074	1075	rBV2	299	274	0.02%	0.003%
46	7.702	1081	1085	1086	rBV2	214	233	0.02%	0.002%
47	7.726	1086	1089	1092	rBV2	206	240	0.02%	0.002%
48	7.757	1092	1094	1095	rBV	244	236	0.02%	0.002%
49	7.976	1124	1130	1134	rVV4	937	1529	0.10%	0.014%
50	8.373	1187	1195	1204	rBV	198827	331785	21.99%	3.102%
51	8.507	1213	1217	1226	rVB4	888	1969	0.13%	0.018%
52	8.696	1240	1248	1264	rBV	757064	1210841	80.25%	11.320%
53	8.799	1264	1265	1268	rVB3	498	279	0.02%	0.003%
54	8.872	1276	1277	1281	rVB2	289	256	0.02%	0.002%
55	8.909	1281	1283	1285	rBV	200	189	0.01%	0.002%
56	8.946	1287	1289	1290	rBV	308	214	0.01%	0.002%
57	8.988	1290	1296	1307	rBV	150000	229200	15.19%	2.143%
58	9.275	1341	1343	1345	rVB3	250	208	0.01%	0.002%
59	9.324	1348	1351	1353	rBV2	313	349	0.02%	0.003%
60	9.366	1356	1358	1360	rVB2	225	206	0.01%	0.002%
61	9.421	1362	1367	1381	rBV	446664	650764	43.13%	6.084%
62	9.592	1394	1395	1397	rBV2	262	275	0.02%	0.003%
63	9.628	1399	1401	1402	rBV2	193	201	0.01%	0.002%
64	9.738	1412	1419	1424	rBV3	2983	4459	0.30%	0.042%
65	9.830	1433	1434	1437	rVB2	380	327	0.02%	0.003%
66	9.866	1437	1440	1441	rVB	243	219	0.01%	0.002%
67	10.092	1471	1477	1487	rBV	696948	925525	61.34%	8.653%
68	10.232	1497	1500	1502	rVB4	375	429	0.03%	0.004%
69	10.281	1505	1508	1509	rBV	292	377	0.02%	0.004%
70	10.348	1517	1519	1521	rVB2	291	253	0.02%	0.002%
71	10.518	1546	1547	1549	rVV2	261	195	0.01%	0.002%
72	10.878	1604	1606	1610	rVB3	282	324	0.02%	0.003%
73	10.915	1610	1612	1614	rBV2	217	187	0.01%	0.002%
74	10.945	1614	1617	1619	rBV	306	344	0.02%	0.003%
75	11.024	1627	1630	1633	rBV3	144	273	0.02%	0.003%
76	11.232	1658	1664	1671	rBV	545861	693344	45.95%	6.482%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010721\
 Data File : VX020527.D
 Acq On : 07 Jan 2021 12:28
 Operator : JC/MD
 Sample : VX0107MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK401

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
 Title : VOC Analysis

77	11.348	1681	1683	1686	rVB	433	439	0.03%	0.004%
78	11.384	1686	1689	1691	rVB2	223	189	0.01%	0.002%
79	11.402	1691	1692	1696	rVB2	258	205	0.01%	0.002%
80	11.512	1708	1710	1714	rVB3	493	544	0.04%	0.005%
81	11.744	1746	1748	1751	rVB	391	263	0.02%	0.002%
82	11.982	1785	1787	1788	rBV2	210	200	0.01%	0.002%
83	12.061	1794	1800	1808	rBV	654453	803564	53.26%	7.513%
84	12.262	1831	1833	1835	rVB2	416	330	0.02%	0.003%
85	12.280	1835	1836	1838	rBV2	248	236	0.02%	0.002%
86	12.360	1843	1849	1856	rBV	762320	953148	63.17%	8.911%
87	12.512	1873	1874	1877	rVB2	340	224	0.01%	0.002%
88	13.000	1952	1954	1955	rBV2	230	239	0.02%	0.002%
89	13.042	1960	1961	1964	rVB3	361	373	0.02%	0.003%
90	13.225	1990	1991	1995	rVB	363	227	0.02%	0.002%
91	13.487	2032	2034	2035	rBV2	296	224	0.01%	0.002%
92	13.628	2055	2057	2059	rVB2	445	311	0.02%	0.003%
93	13.829	2088	2090	2091	rBV2	256	192	0.01%	0.002%
94	13.969	2111	2113	2115	rBV2	272	227	0.02%	0.002%
95	14.158	2142	2144	2145	rVB	471	327	0.02%	0.003%
96	14.189	2145	2149	2150	rBV2	467	445	0.03%	0.004%
97	14.323	2168	2171	2173	rBV3	315	445	0.03%	0.004%
98	14.506	2199	2201	2202	rVB2	369	253	0.02%	0.002%
99	14.658	2224	2226	2227	rBV	325	180	0.01%	0.002%
100	15.749	2403	2405	2407	rBV3	517	511	0.03%	0.005%

Sum of corrected areas: 10696004




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010721\
Data File : VX020527.D
Acq On : 07 Jan 2021 12:28
Operator : JC/MD
Sample : VX0107MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK401

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L

TIC Integration Parameters: LSCINT.P

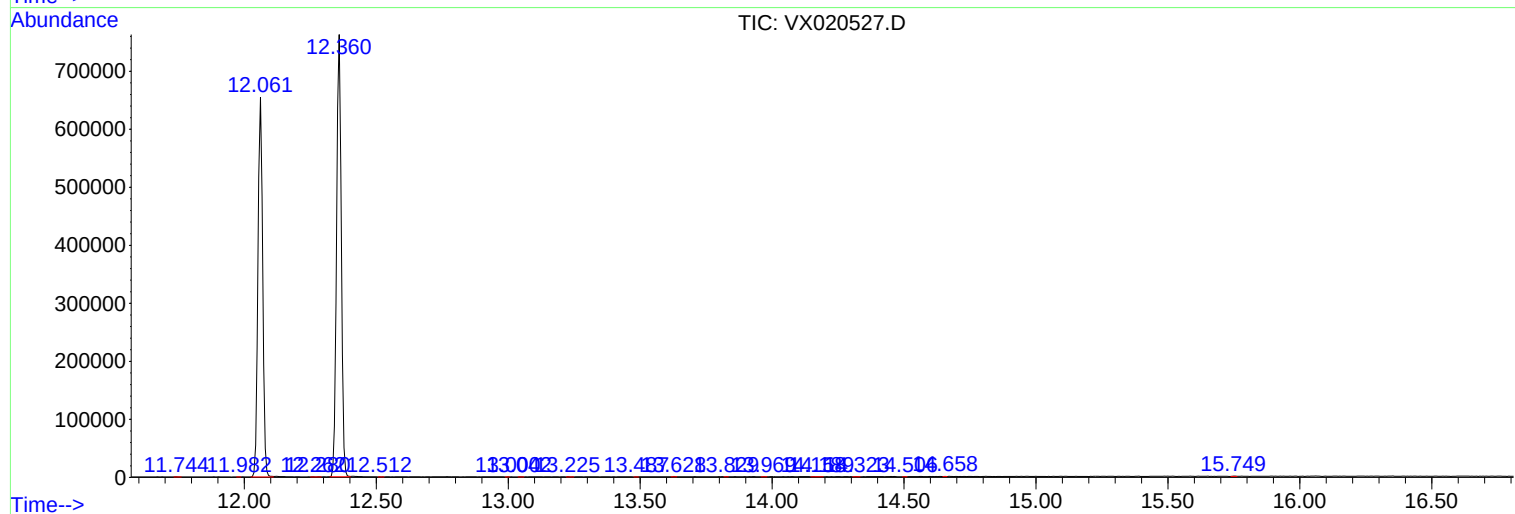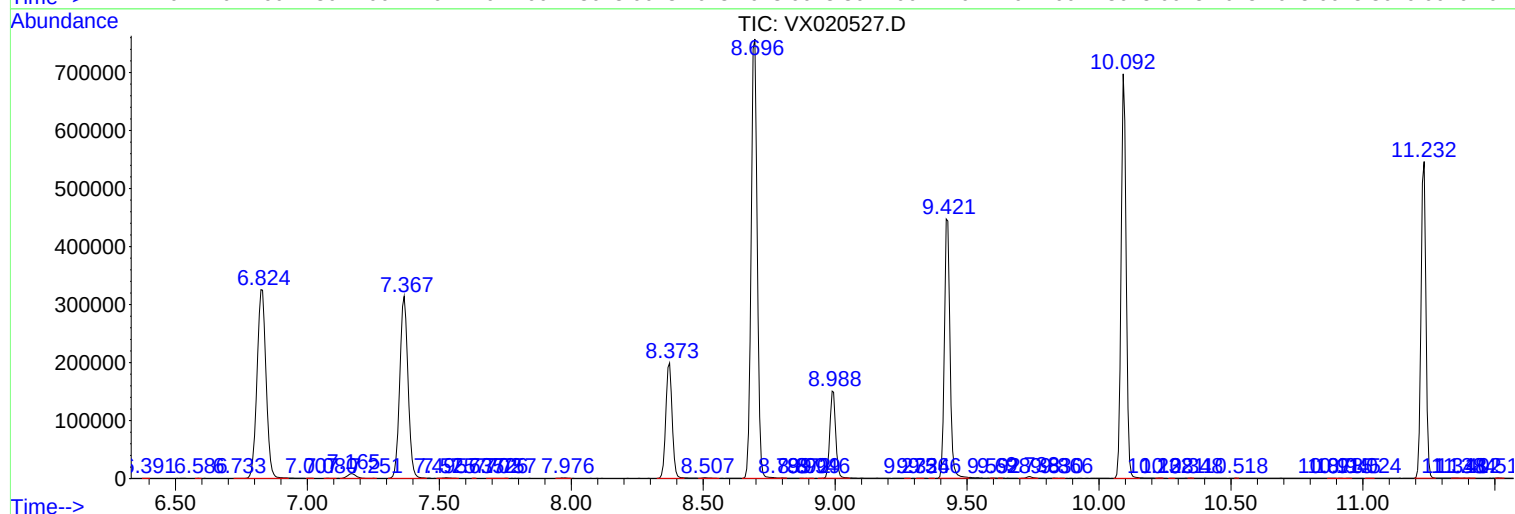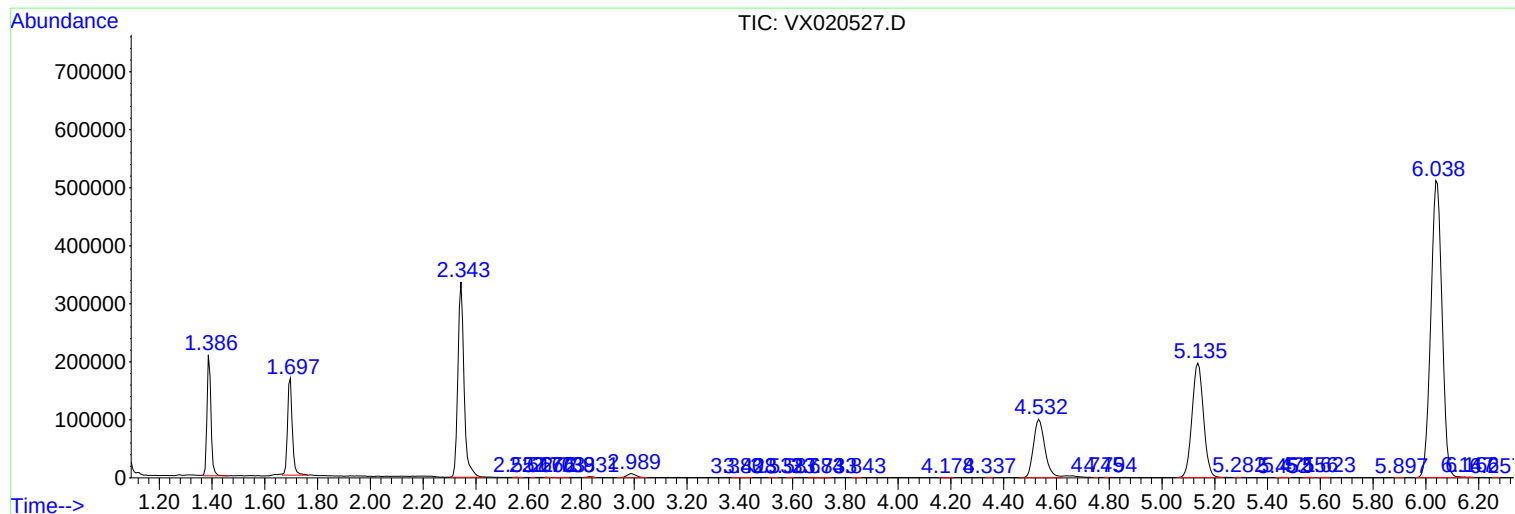

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010721\
Data File : VX020527.D
Acq On : 07 Jan 2021 12:28
Operator : JC/MD
Sample : VX0107MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK401

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXMLM010721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010721\
Data File : VX020527.D
Acq On : 07 Jan 2021 12:28
Operator : JC/MD
Sample : VX0107MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK401

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
