
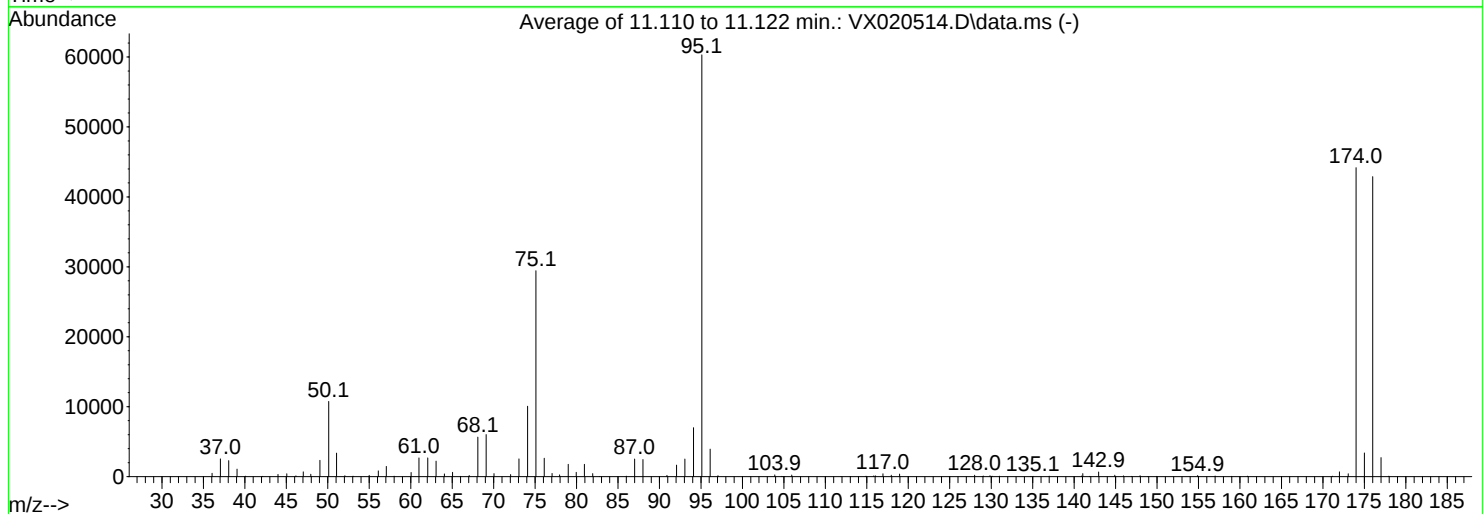


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010721\
 Data File : VX020514.D
 Acq On : 06 Jan 2021 12:37
 Operator : JC/MD
 Sample : BFB63
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB603

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM010721WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 15 16:52:29 2021

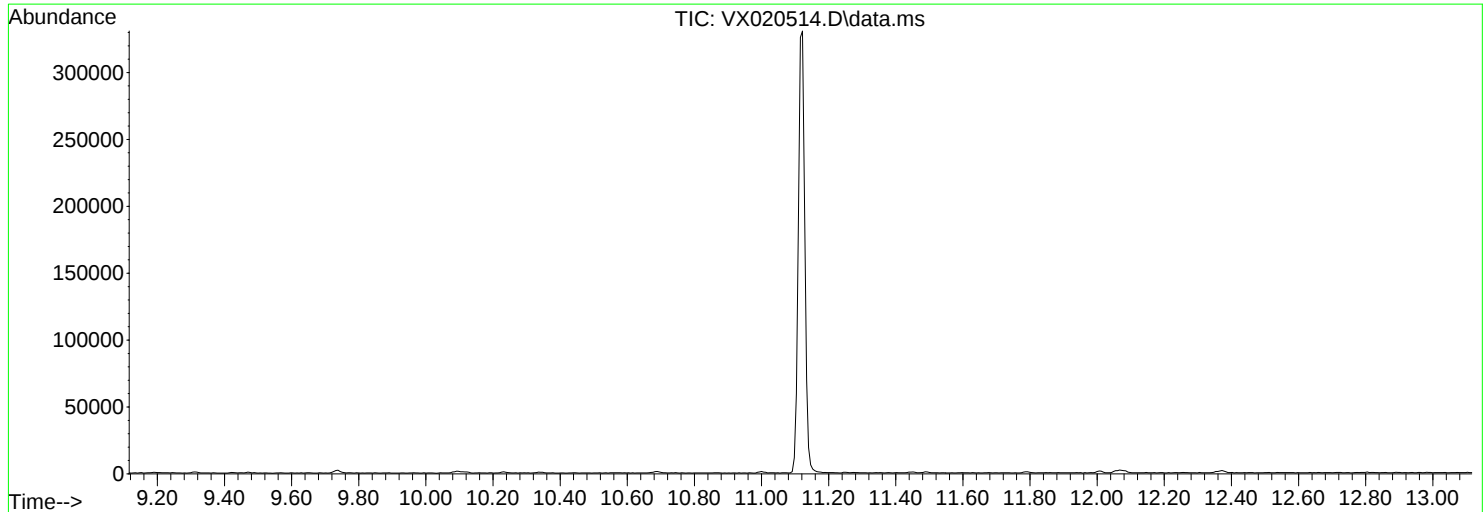

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	10753	PASS
75	95	30	80	48.8	29451	PASS
95	95	100	100	100.0	60309	PASS
96	95	5	9	6.5	3947	PASS
173	174	0.00	2	0.9	416	PASS
174	95	50	120	73.2	44168	PASS
175	174	5	9	7.7	3379	PASS
176	174	95	101	97.1	42896	PASS
177	176	5	9	6.3	2723	PASS

Scan 1639 (11.079 min): VX020514.D\data.ms
BFB63

m/z	Abundance
39.90	186.0
44.00	514.0
207.00	58.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.10	443.0
37.10	1894.0
38.10	1780.0
39.00	812.0
39.90	202.0
42.20	78.0
44.00	800.0
45.10	319.0
46.20	72.0
47.00	600.0
47.90	314.0
49.00	1828.0
50.10	7676.0
51.00	2306.0
52.00	93.0
55.00	118.0
56.10	654.0
57.00	987.0
58.00	66.0
60.00	357.0
61.00	2092.0
62.10	1869.0
63.10	1625.0
64.00	299.0
65.10	453.0
67.10	130.0
68.10	4076.0
69.10	4106.0
70.00	351.0
72.00	205.0
73.00	1516.0
74.10	7101.0
75.10	20904.0
76.10	1885.0
77.10	247.0
77.90	170.0
79.00	1199.0
79.90	448.0
80.90	1301.0
81.90	272.0
82.80	51.0
87.00	1554.0
88.00	1784.0
90.80	119.0
92.10	1058.0
93.10	1708.0
94.10	4809.0
95.10	41016.0
96.10	2738.0
97.00	166.0
104.00	169.0
104.80	58.0
106.00	113.0
114.80	51.0
115.80	89.0
116.10	85.0
116.90	295.0
118.00	177.0
119.00	256.0
128.10	117.0
128.90	59.0
129.90	126.0
135.10	63.0
140.90	303.0
143.00	522.0
144.90	123.0
146.00	62.0
146.90	55.0
148.00	84.0
155.00	94.0
171.20	68.0
172.00	435.0
173.10	250.0
174.00	24864.0
175.00	2167.0
176.00	23952.0
177.00	1653.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.00	481.0
37.00	3002.0
38.00	2766.0
39.00	1204.0
39.90	218.0
42.10	53.0
44.10	903.0
45.00	511.0
46.10	88.0
47.00	748.0
48.00	341.0
49.10	2651.0
50.10	12766.0
51.10	4213.0
52.00	164.0
53.00	71.0
55.00	242.0
56.10	921.0
57.10	1751.0
58.00	62.0
60.00	769.0
61.00	2965.0
62.00	3218.0
63.00	2604.0
64.10	572.0
65.00	774.0
66.00	82.0
67.00	205.0
68.10	6424.0
69.10	6849.0
70.10	496.0
72.10	347.0
73.10	3004.0
74.10	11542.0
75.10	34808.0
76.10	3126.0
77.10	602.0
77.90	264.0
79.00	2014.0
79.90	693.0
81.00	1987.0
82.00	614.0
86.10	130.0
87.00	3071.0
88.00	2779.0
90.90	208.0
92.10	1951.0
93.10	2712.0
94.10	8238.0
95.10	70952.0
96.10	4436.0
97.10	152.0
103.80	300.0
104.70	90.0
105.10	67.0
105.90	304.0
114.90	84.0
115.90	244.0
117.00	486.0
118.00	227.0
118.90	394.0
128.00	207.0
129.10	110.0
130.10	189.0
131.00	109.0
134.80	154.0
137.00	95.0
141.10	591.0
141.90	87.0
143.00	717.0
144.90	225.0
145.90	115.0
147.00	52.0
147.90	168.0
148.90	59.0
150.00	86.0
154.80	171.0
157.00	159.0
159.00	63.0
160.90	68.0
171.10	66.0
172.00	722.0
173.00	489.0
174.00	52152.0
175.00	4028.0
176.00	48032.0
177.00	3345.0
177.90	106.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.10	496.0
37.10	2725.0
38.10	2342.0
39.10	1196.0
40.10	194.0
44.00	838.0
45.00	434.0
46.10	156.0
47.10	715.0
47.90	373.0
49.10	2538.0
50.10	11816.0
51.10	3598.0
52.10	170.0
53.10	103.0
55.00	170.0
56.10	920.0
57.10	1650.0
58.00	75.0
60.10	669.0
61.00	2982.0
62.10	2932.0
63.10	2411.0
64.00	328.0
65.10	637.0
66.00	70.0
67.00	169.0
68.10	6420.0
69.10	7067.0
70.10	467.0
72.00	349.0
73.10	3070.0
74.10	11572.0
75.10	32640.0
76.10	2873.0
77.00	552.0
78.00	352.0
79.00	2069.0
80.00	704.0
81.00	2007.0
81.90	435.0
85.90	102.0
87.00	2909.0
88.00	2778.0
91.00	194.0
92.00	1961.0
93.00	3135.0
94.10	7988.0
95.10	68960.0
96.10	4667.0
97.10	125.0
104.00	297.0
104.90	79.0
106.00	266.0
111.90	57.0
113.00	56.0
115.00	86.0
116.00	255.0
117.00	433.0
117.90	204.0
118.90	441.0
127.90	272.0
129.00	171.0
129.80	262.0
131.00	105.0
135.00	105.0
137.00	131.0
141.00	680.0
141.90	74.0
142.90	740.0
144.90	280.0
145.90	154.0
147.90	136.0
149.90	85.0
155.00	243.0
157.00	139.0
159.00	85.0
160.90	116.0
171.20	84.0
172.00	925.0
173.00	509.0
174.00	55488.0
175.00	3941.0
176.00	56704.0
177.00	3172.0
178.00	120.0
207.10	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603