
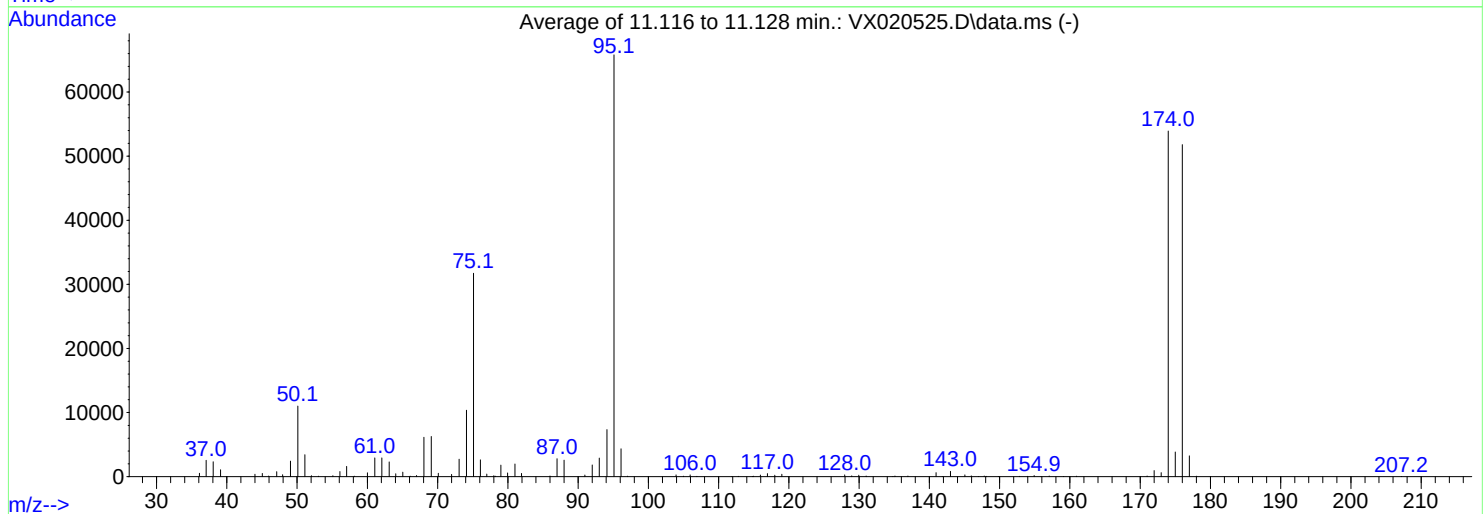


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010721\
Data File : VX020525.D
Acq On : 07 Jan 2021 09:25
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB604

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM010721WMA.M
Title : VOC Analysis
Last Update : Sat Jan 09 04:41:43 2021

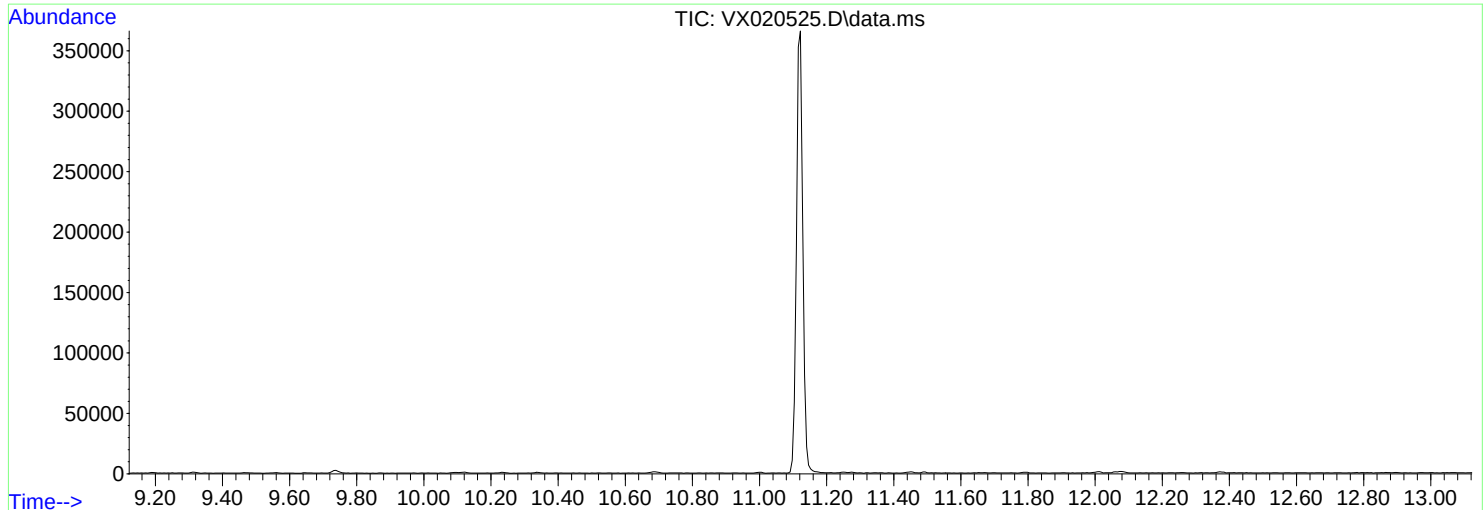

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	11013	PASS
75	95	30	80	48.2	31717	PASS
95	95	100	100	100.0	65805	PASS
96	95	5	9	6.6	4349	PASS
173	174	0.00	2	1.1	619	PASS
174	95	50	120	82.0	53931	PASS
175	174	5	9	7.1	3845	PASS
176	174	95	101	96.1	51803	PASS
177	176	5	9	6.3	3248	PASS

m/z	Abundance
40.10	200.0
44.00	467.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604

m/z	Abundance
36.10	602.0
37.10	3182.0
38.10	2969.0
39.10	1463.0
40.00	233.0
44.00	920.0
45.10	566.0
45.90	95.0
47.10	987.0
47.90	394.0
49.00	2973.0
50.10	13842.0
51.10	4467.0
52.10	195.0
53.10	75.0
55.10	236.0
56.10	925.0
57.10	2018.0
58.20	96.0
60.00	856.0
61.10	3535.0
62.10	3416.0
63.10	2676.0
64.10	522.0
65.10	702.0
66.00	126.0
67.00	237.0
68.10	7491.0
69.10	7637.0
70.10	695.0
72.00	404.0
73.00	3303.0
74.10	12085.0
75.10	38344.0
76.10	3323.0
77.10	502.0
78.00	291.0
79.00	2185.0
79.90	641.0
81.00	2478.0
82.00	532.0
86.00	155.0
87.00	3319.0
88.00	3087.0
91.00	327.0
92.00	2017.0
93.00	3398.0
94.10	8619.0
95.10	75792.0
96.10	5250.0
97.10	120.0
103.90	332.0
105.00	94.0
106.00	274.0
106.90	77.0
114.80	67.0
115.90	261.0
116.90	572.0
118.00	232.0
119.00	485.0
127.90	280.0
129.00	144.0
130.00	252.0
131.00	100.0
135.10	171.0
137.10	128.0
141.00	629.0
143.00	854.0
145.00	318.0
146.00	144.0
148.10	150.0
149.80	71.0
152.80	68.0
154.00	69.0
155.10	141.0
157.10	109.0
161.00	94.0
171.00	118.0
172.00	936.0
173.00	744.0
174.00	54432.0
175.00	3998.0
176.00	52904.0
177.00	3529.0
178.00	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604

m/z	Abundance
36.10	615.0
37.00	2928.0
38.00	2545.0
39.10	1146.0
40.00	251.0
44.00	967.0
45.00	671.0
46.00	167.0
47.10	902.0
48.00	324.0
49.10	2728.0
50.10	12044.0
51.10	3761.0
52.00	152.0
53.00	102.0
55.10	137.0
56.10	903.0
57.00	1942.0
58.10	81.0
60.00	578.0
61.00	3368.0
62.00	3523.0
63.10	2776.0
64.00	504.0
65.00	846.0
66.10	67.0
67.00	207.0
68.00	7224.0
69.10	7411.0
70.10	563.0
72.00	445.0
73.10	3127.0
74.10	12249.0
75.10	36192.0
76.10	3037.0
77.00	445.0
78.20	250.0
79.00	2090.0
80.00	677.0
81.00	2295.0
81.90	551.0
86.00	125.0
87.00	3372.0
88.00	2907.0
90.90	271.0
92.00	2037.0
93.00	3358.0
94.10	8089.0
95.10	76088.0
96.10	4995.0
97.00	94.0
104.00	300.0
105.00	101.0
105.90	353.0
106.90	84.0
111.90	75.0
112.90	65.0
115.00	109.0
116.00	303.0
117.00	561.0
118.00	318.0
119.00	406.0
128.00	343.0
128.90	134.0
130.00	309.0
131.00	114.0
135.10	114.0
136.90	107.0
140.90	752.0
141.80	60.0
143.00	1008.0
145.10	311.0
145.90	157.0
147.00	60.0
147.80	168.0
152.90	59.0
153.90	55.0
154.90	242.0
155.90	59.0
157.00	110.0
159.10	59.0
161.00	93.0
171.00	108.0
172.00	1085.0
173.00	658.0
174.00	65024.0
175.00	4196.0
176.00	62328.0
177.00	3740.0
178.10	92.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604

m/z	Abundance
36.00	331.0
37.10	1508.0
38.00	1432.0
39.00	635.0
40.00	217.0
44.10	628.0
45.10	268.0
46.00	79.0
47.00	455.0
48.00	201.0
49.10	1572.0
50.10	7153.0
51.10	2065.0
52.00	94.0
53.10	74.0
55.10	93.0
56.00	535.0
57.00	873.0
58.10	62.0
60.00	348.0
61.10	1897.0
62.10	1850.0
63.10	1464.0
64.10	324.0
65.00	560.0
66.20	68.0
67.00	118.0
68.10	3686.0
69.10	3719.0
70.00	349.0
71.90	233.0
73.10	1756.0
74.10	6733.0
75.10	20616.0
76.10	1492.0
76.90	279.0
78.00	133.0
78.90	1096.0
80.00	444.0
81.10	1173.0
82.00	421.0
87.00	1743.0
88.00	1696.0
90.90	164.0
92.00	1393.0
93.00	1915.0
94.10	5312.0
95.10	45536.0
96.10	2803.0
97.10	59.0
103.90	189.0
105.00	73.0
105.90	207.0
112.70	62.0
114.90	100.0
116.00	200.0
117.00	303.0
118.00	161.0
119.00	266.0
128.00	172.0
129.00	96.0
129.80	157.0
130.90	62.0
134.80	86.0
136.80	90.0
141.00	485.0
141.90	53.0
143.00	616.0
145.00	189.0
145.90	109.0
147.80	124.0
152.80	51.0
154.80	148.0
157.00	80.0
160.90	64.0
171.00	65.0
172.00	867.0
172.90	455.0
174.00	42336.0
175.00	3342.0
176.00	40176.0
177.00	2475.0
178.10	54.0
207.20	55.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604